

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110419\
 Data File : PS007608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2019 19:51
 Operator : SM\AJ
 Sample : K5615-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 3465

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:48:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.434	5.159	155.4E6	79314496	113.569	112.774
Target Compounds							
1) T	Dalapon	1.993	1.657	50476192	687.8E6	30.166	755.802 #
2) T	3,5-DICHL...	0.000	4.493	0	50650246	N.D.	58.866
5) T	DICAMBA	5.527	0.000	38096972	0	7.754	N.D. #
7) T	MCPA	5.902	5.527	34840804	30668160	6.755	10.549 #
8) T	DICHLORPROP	0.000	5.818	0	6925845	N.D.	10.635
9) T	2,4-D	6.490	6.061	30952600	10799557	25.117	13.537 #
10) T	Pentachlo...	0.000	6.446	0	10502310	N.D.	1.092
11) T	2,4,5-TP ...	0.000	6.755	0	24968279	N.D.	6.564
12) T	2,4,5-T	0.000	7.157	0	15926753	N.D.	4.546
13) T	2,4-DB	0.000	7.679	0	10934845	N.D.	23.330
14) T	DINOSEB	0.000	7.984	0	24868761	N.D.	8.858
15) T	Picloram	0.000	8.913	0	26790957	N.D.	4.363
16) T	DCPA	0.000	8.913	0	26790957	N.D.	5.343



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110419\
Data File : PS007608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2019 19:51
Operator : SM\AJ
Sample : K5615-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
3465

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:48:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

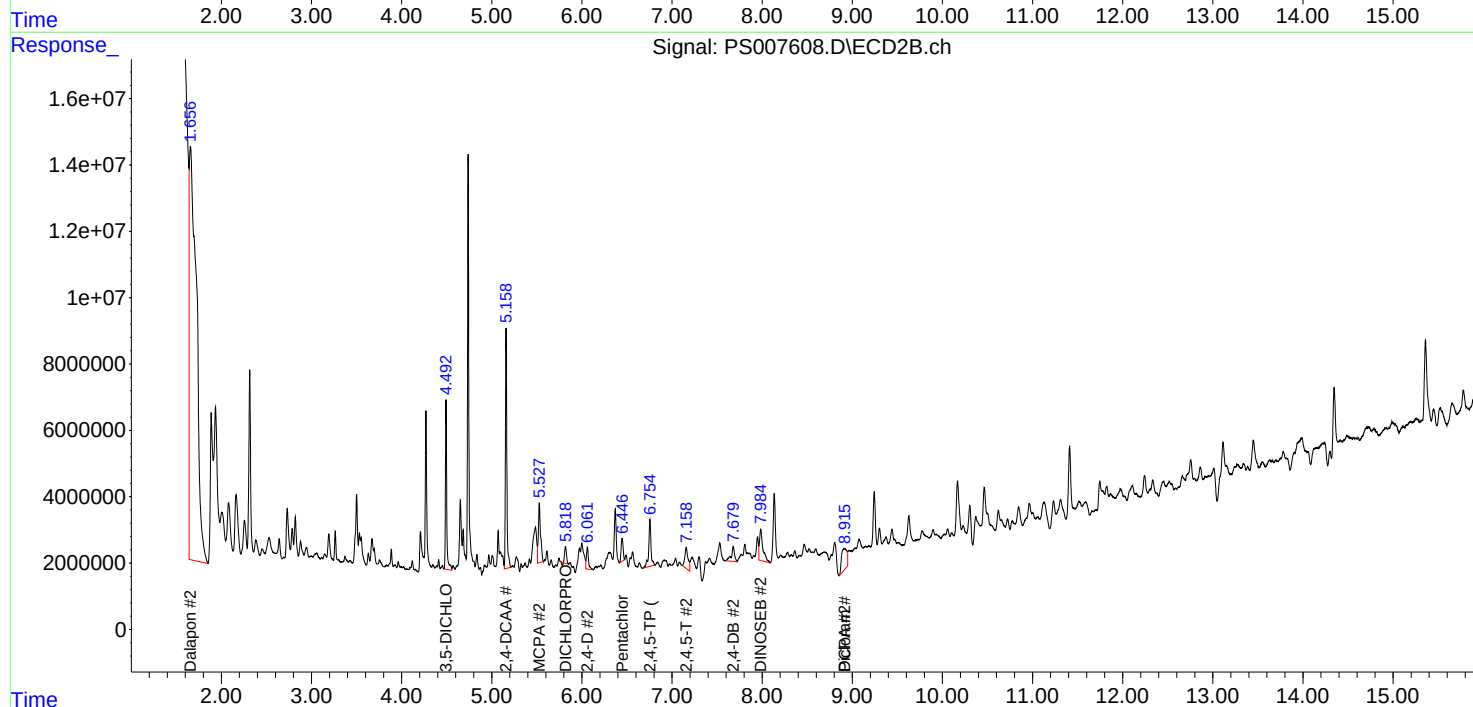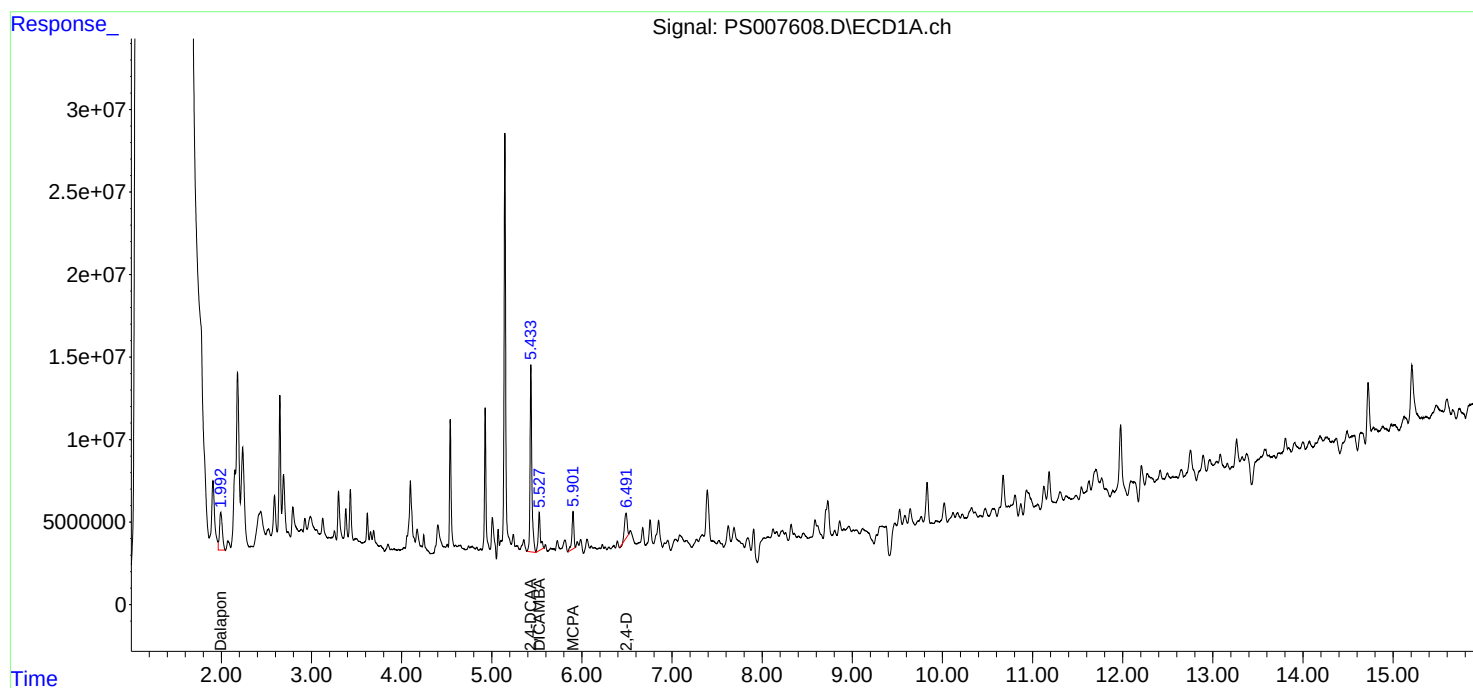


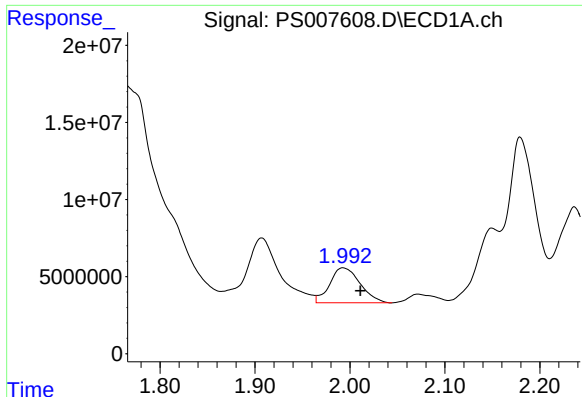

#1 Dalapon


R.T.: 1.993 min
Delta R.T.: -0.018 min
Response: 50476192
Conc: 30.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
3465

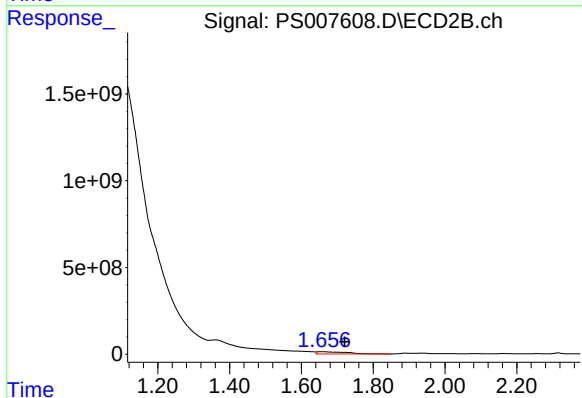


#1 Dalapon

R.T.: 1.657 min
Delta R.T.: -0.063 min
Response: 687782185
Conc: 755.80 ng/ml

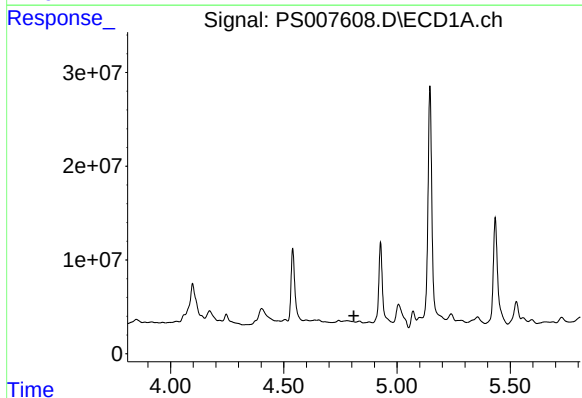


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

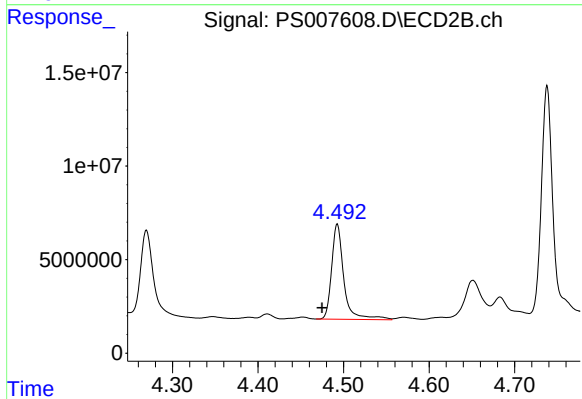

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.493 min
Delta R.T.: 0.018 min
Response: 50650246
Conc: 58.87 ng/ml

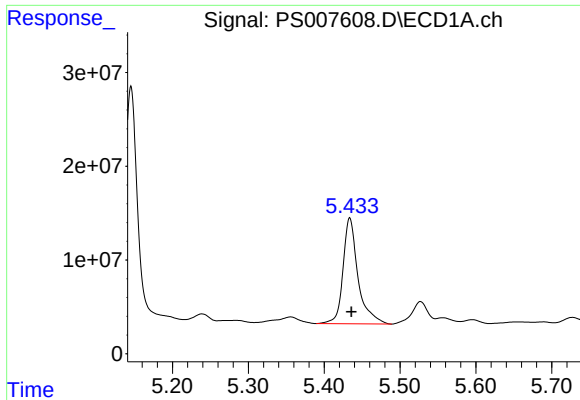

#4 2,4-DCAA


R.T.: 5.434 min
Delta R.T.: -0.002 min
Response: 155438361
Conc: 113.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
3465

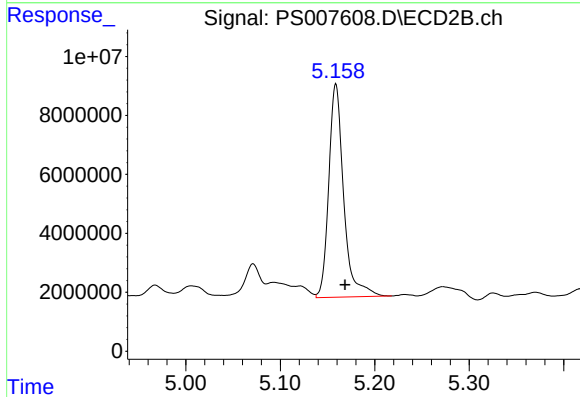


#4 2,4-DCAA

R.T.: 5.159 min
Delta R.T.: -0.010 min
Response: 79314496
Conc: 112.77 ng/ml

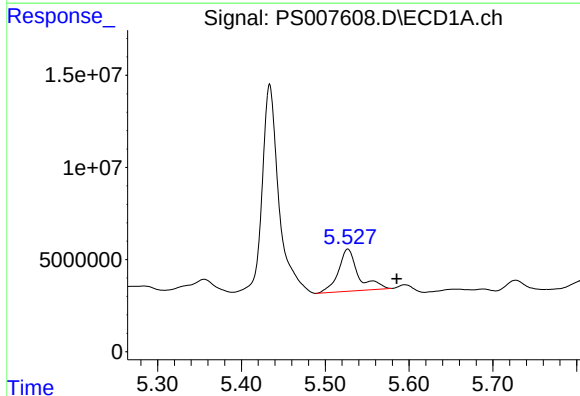


#5 DICAMBA

R.T.: 5.527 min
Delta R.T.: -0.058 min
Response: 38096972
Conc: 7.75 ng/ml

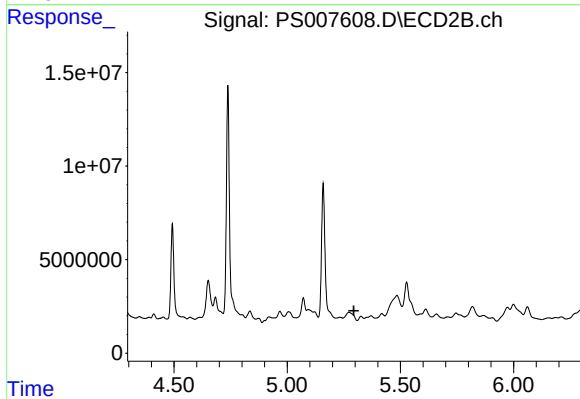

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

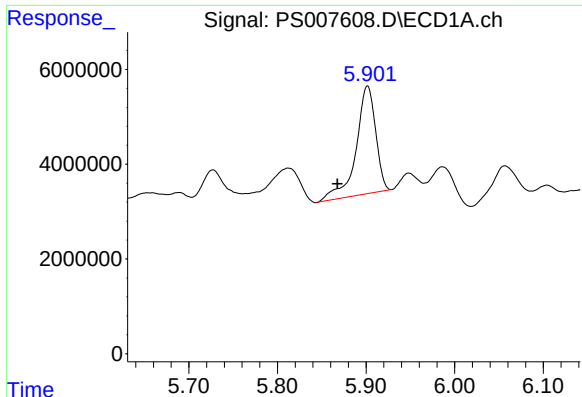

#7 MCPA


R.T.: 5.902 min
Delta R.T.: 0.034 min
Response: 34840804
Conc: 6.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
3465

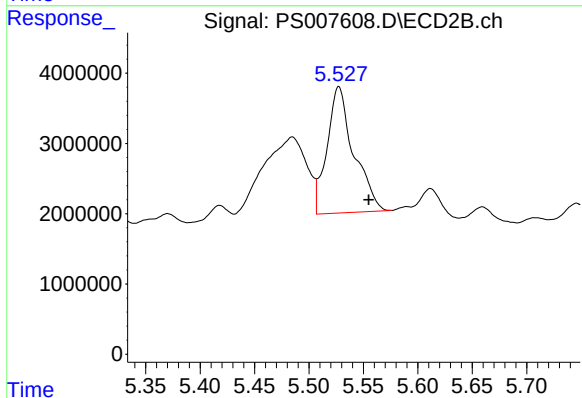


#7 MCPA

R.T.: 5.527 min
Delta R.T.: -0.027 min
Response: 30668160
Conc: 10.55 ug/ml

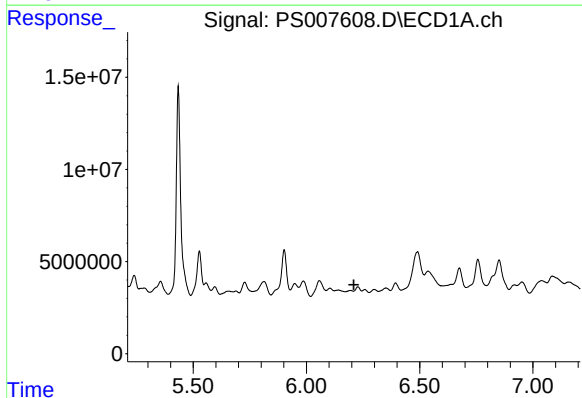


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

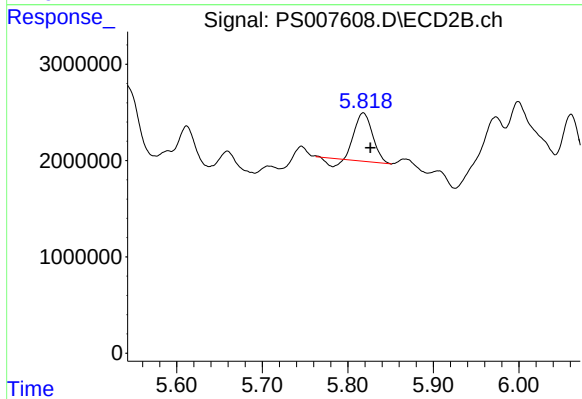

#8 DICHLORPROP


R.T.: 5.818 min
Delta R.T.: -0.008 min
Response: 6925845
Conc: 10.64 ng/ml

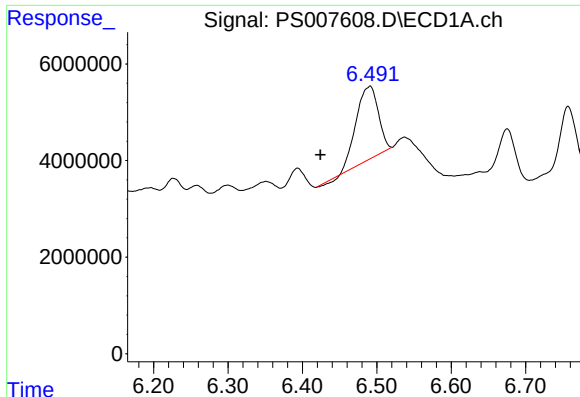

#9 2,4-D


R.T.: 6.490 min
Delta R.T.: 0.066 min
Response: 30952600
Conc: 25.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
3465

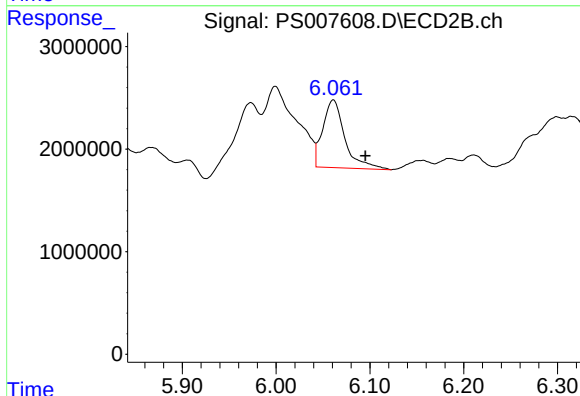


#9 2,4-D

R.T.: 6.061 min
Delta R.T.: -0.034 min
Response: 10799557
Conc: 13.54 ng/ml

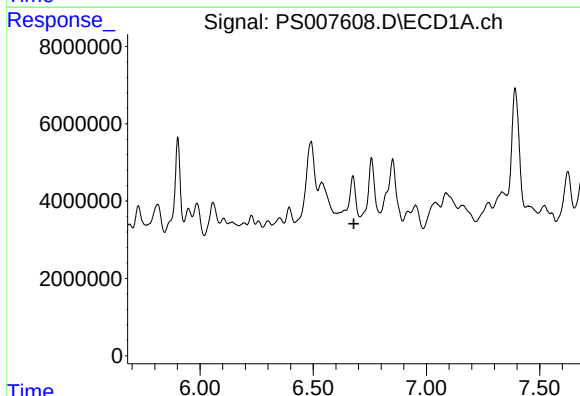


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

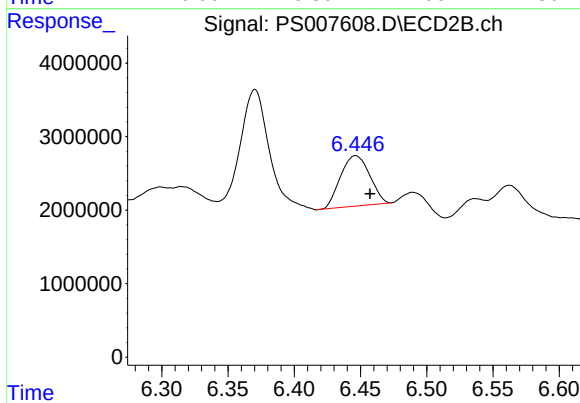

#10 Pentachlorophenol


R.T.: 6.446 min
Delta R.T.: -0.011 min
Response: 10502310
Conc: 1.09 ng/ml

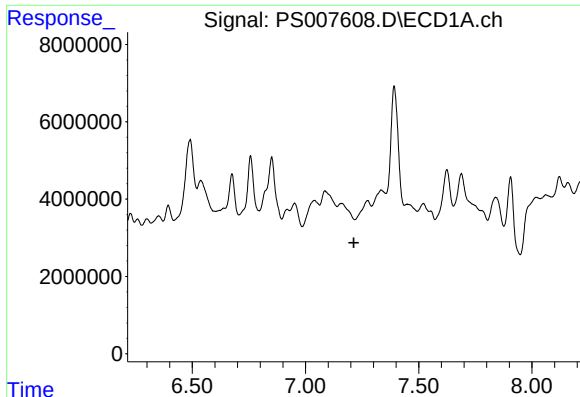

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
3465

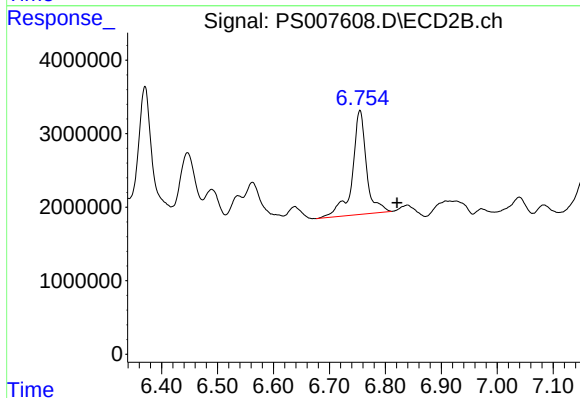


#11 2,4,5-TP (SILVEX)

R.T.: 6.755 min
Delta R.T.: -0.066 min
Response: 24968279
Conc: 6.56 ng/ml

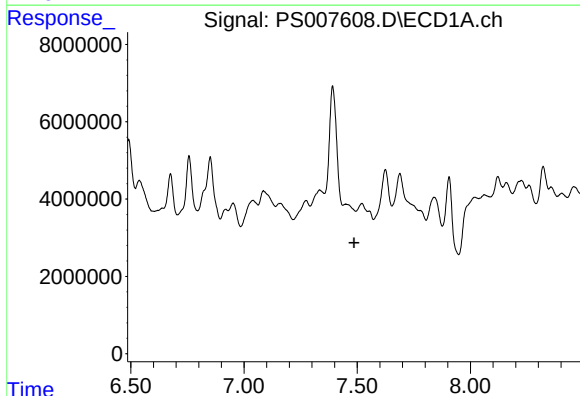


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

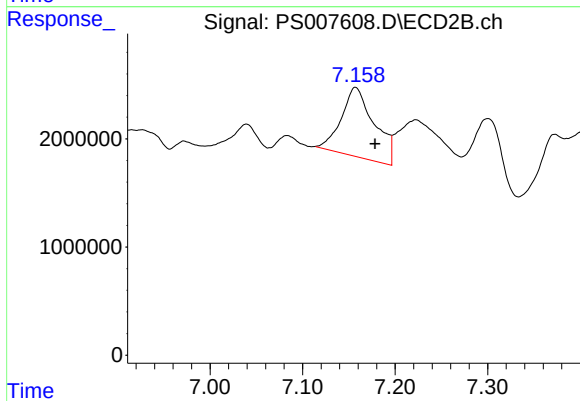

#12 2,4,5-T


R.T.: 7.157 min
Delta R.T.: -0.021 min
Response: 15926753
Conc: 4.55 ng/ml

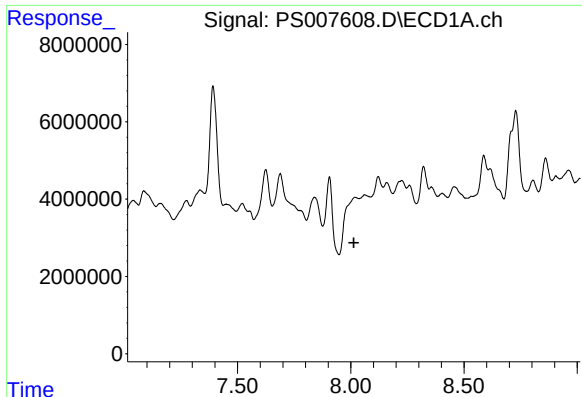

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
3465

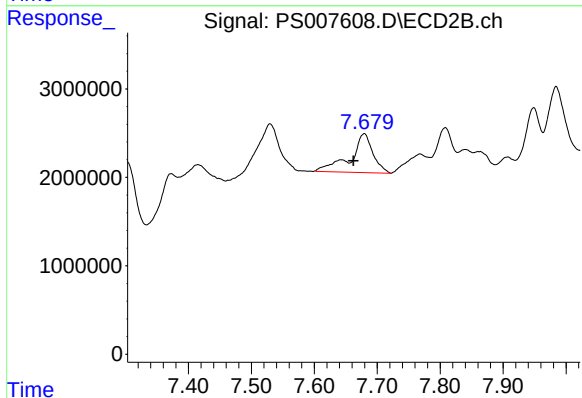


#13 2,4-DB

R.T.: 7.679 min
Delta R.T.: 0.017 min
Response: 10934845
Conc: 23.33 ng/ml

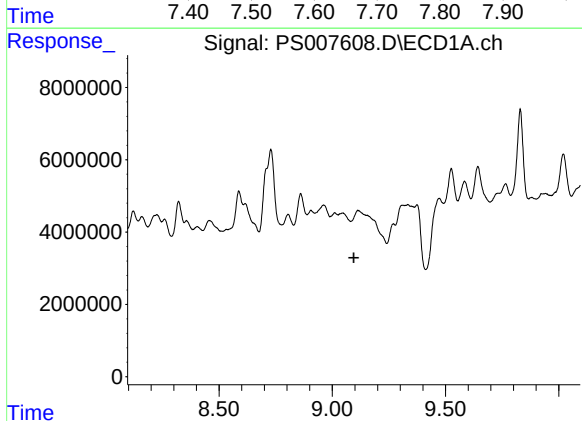


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

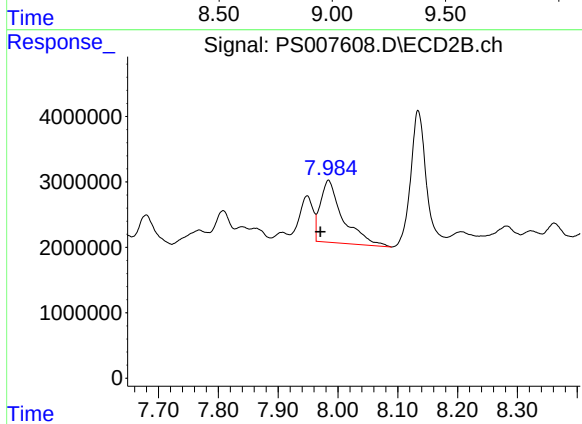

#14 DINOSEB


R.T.: 7.984 min
Delta R.T.: 0.014 min
Response: 24868761
Conc: 8.86 ng/ml

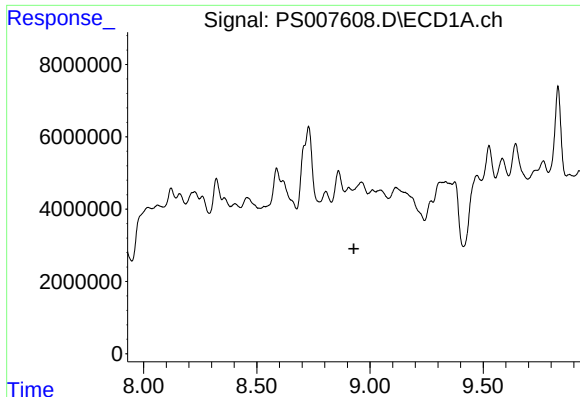

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
3465

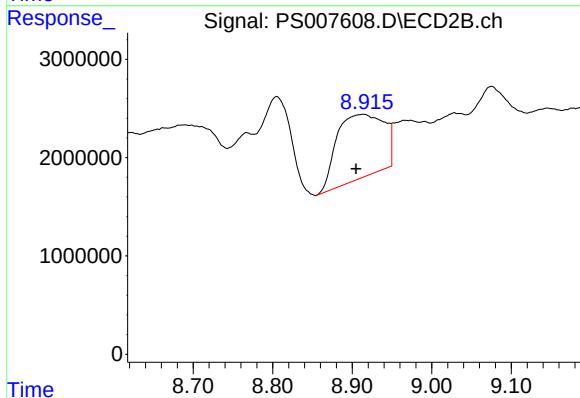


#15 Picloram

R.T.: 8.913 min
Delta R.T.: 0.009 min
Response: 26790957
Conc: 4.36 ng/ml

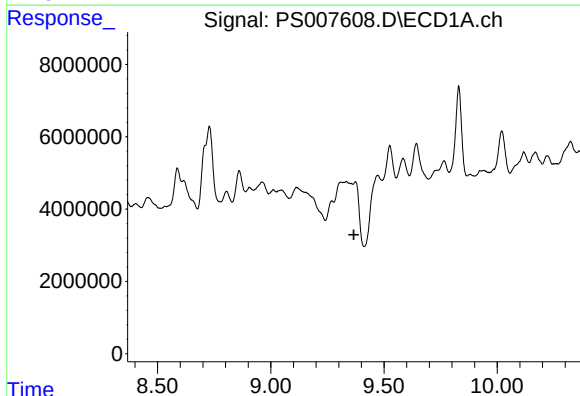

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

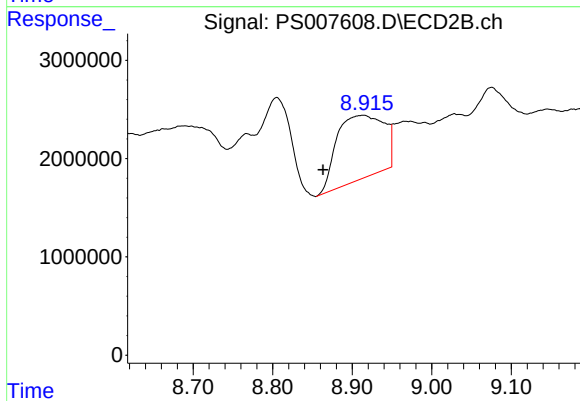

#16 DCPA

R.T.: 8.913 min
Delta R.T.: 0.050 min
Response: 26790957
Conc: 5.34 ng/ml