

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
 Data File : PS013115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 19:12
 Operator : DD\AJ
 Sample : L4600-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:55:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	340.7E6	172.1E6	381.148	442.198
Target Compounds							
1) T	Dalapon	2.994	2.590	72880969	161.6E6	68.885	304.965 #
2) T	3,5-DICHL...	0.000	6.095	0	87016768	N.D.	141.451
3) T	4-Nitroph...	7.098f	6.576f	10686100	2548181	25.056	10.700 #
5) T	DICAMBA	7.387	7.047	11502147	6070136	3.221	3.657
7) T	MCPA	7.710	0.000	71438547	0	18.709	N.D. #
8) T	DICHLORPROP	0.000	7.748f	0	6486387	N.D.	14.512
9) T	2,4-D	0.000	7.951f	0	18176545	N.D.	34.250
10) T	Pentachlo...	8.683f	0.000	8884488	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.740f	0	39535898	N.D.	17.060
15) T	Picloram	10.976	0.000	13434519	0	2.043	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
Data File : PS013115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 19:12
Operator : DD\AJ
Sample : L4600-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:55:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

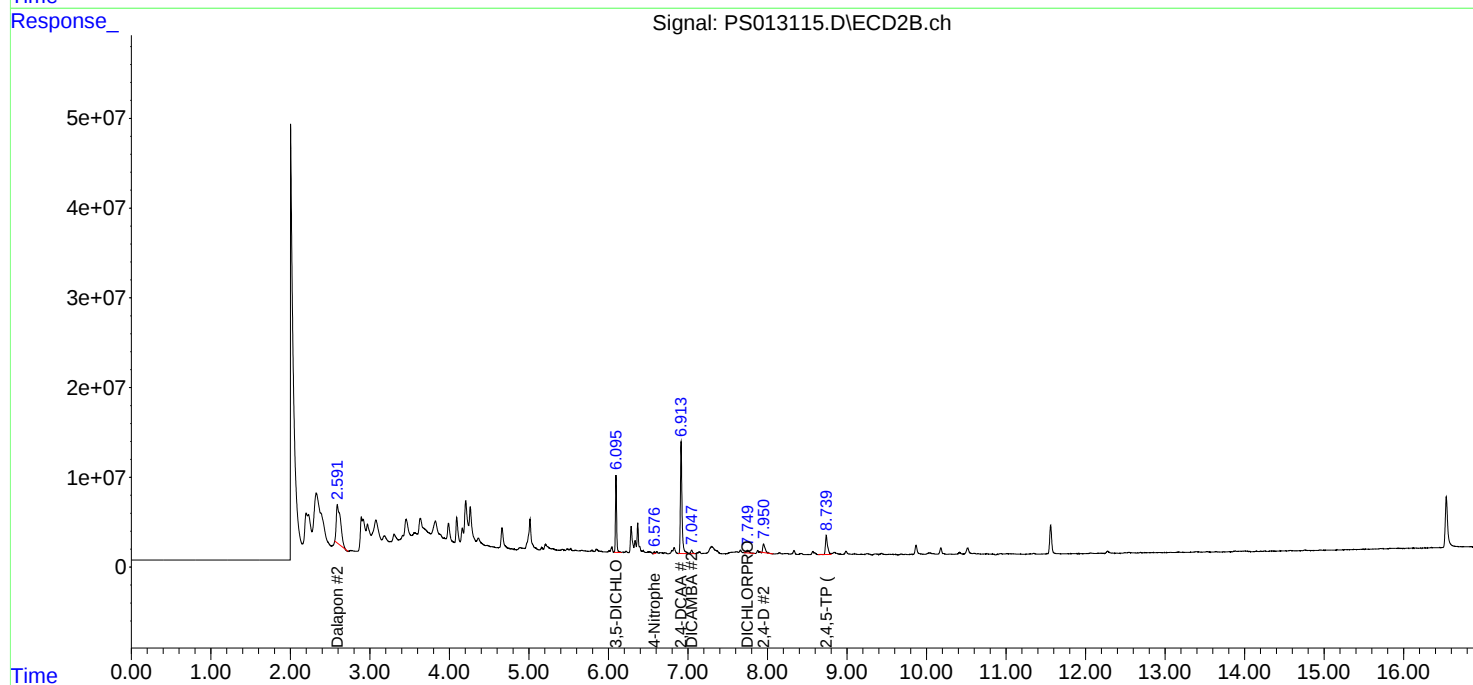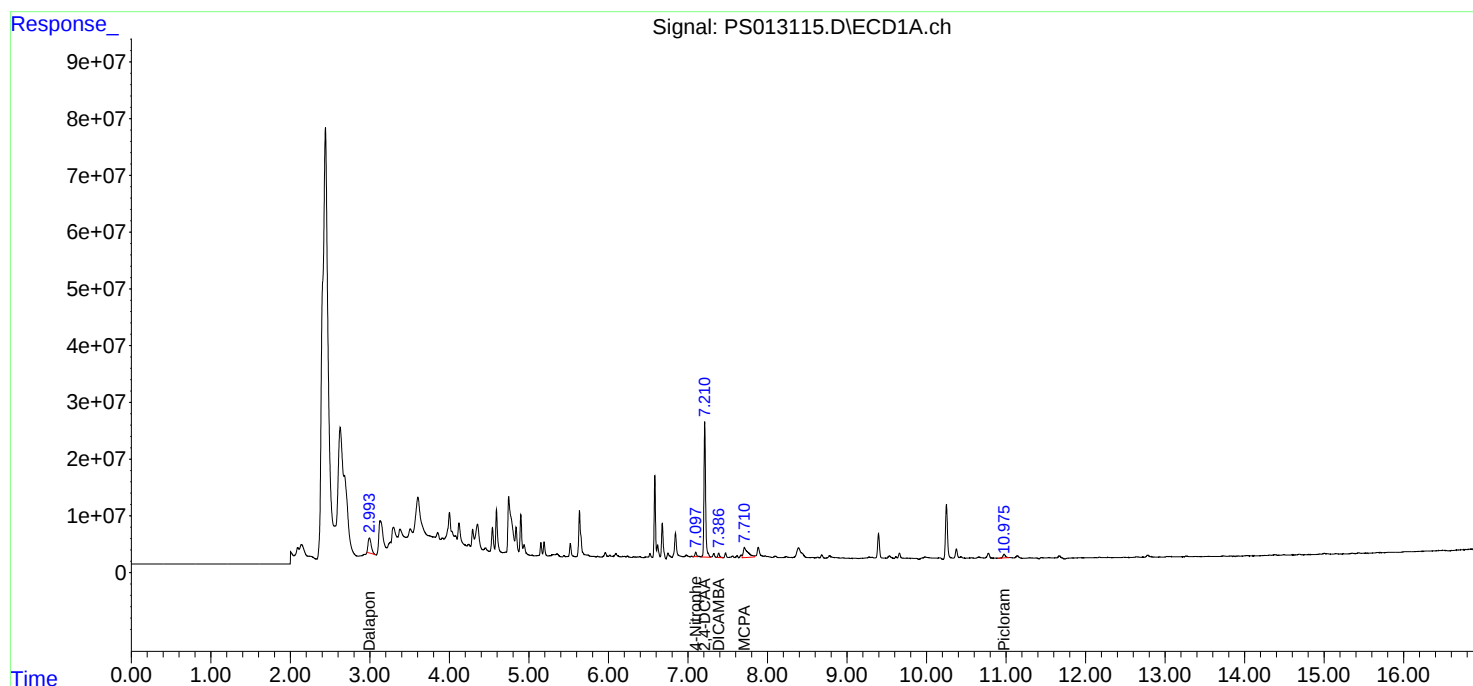


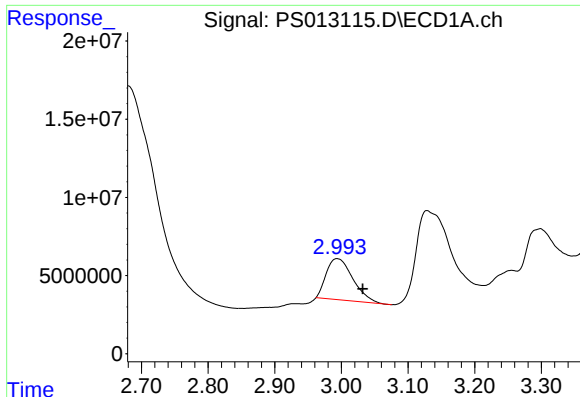

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.038 min
Response: 72880969
Conc: 68.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

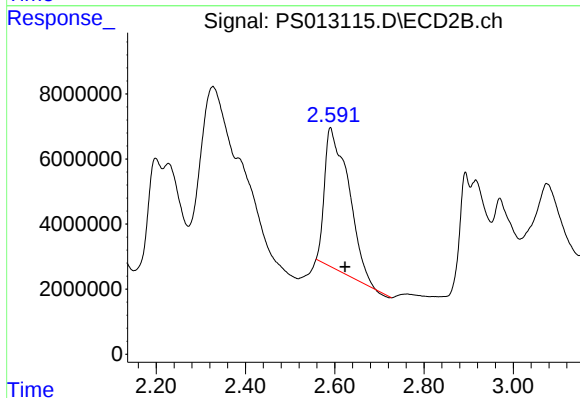


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.033 min
Response: 161623928
Conc: 304.97 ng/ml

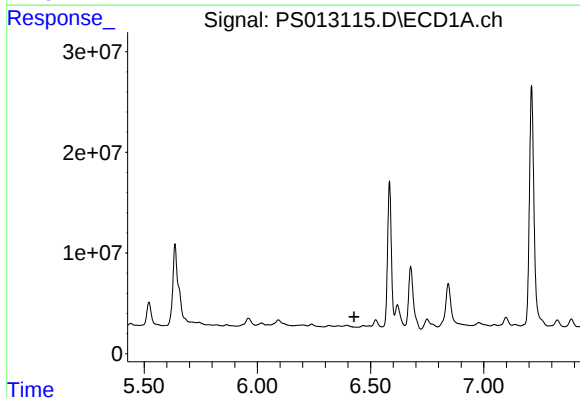


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.427 min
Response: 0
Conc: N.D.

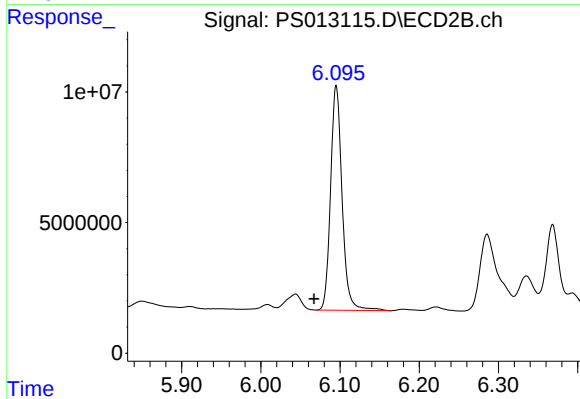

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 87016768
Conc: 141.45 ng/ml

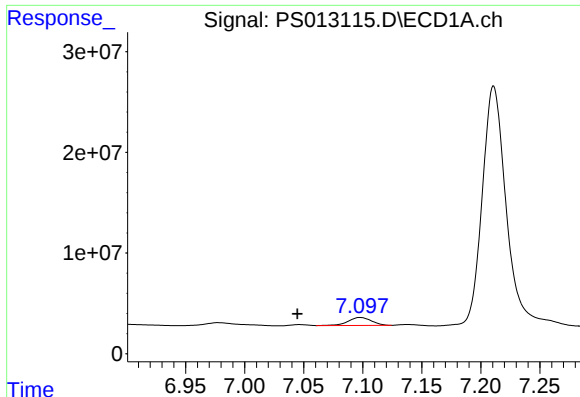

#3 4-Nitrophenol


R.T.: 7.098 min
Delta R.T.: 0.053 min
Response: 10686100
Conc: 25.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

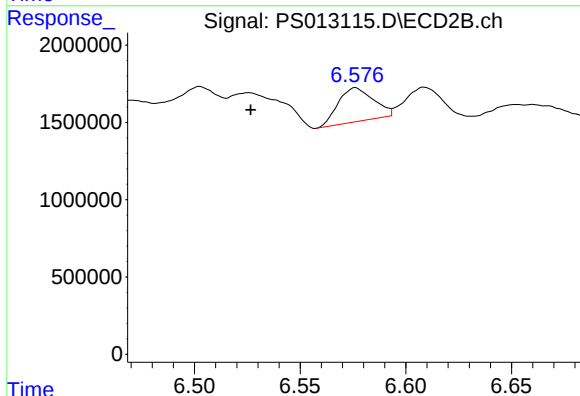


#3 4-Nitrophenol

R.T.: 6.576 min
Delta R.T.: 0.050 min
Response: 2548181
Conc: 10.70 ng/ml

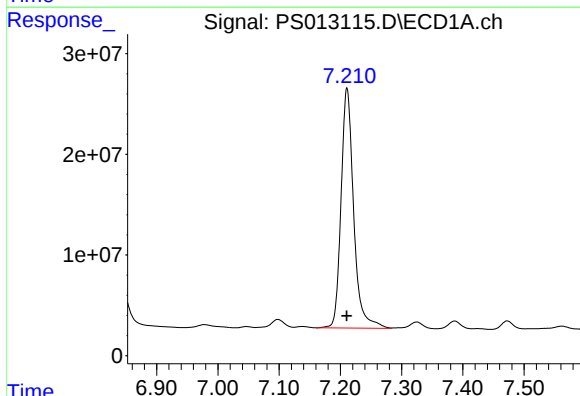


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 340719112
Conc: 381.15 ng/ml

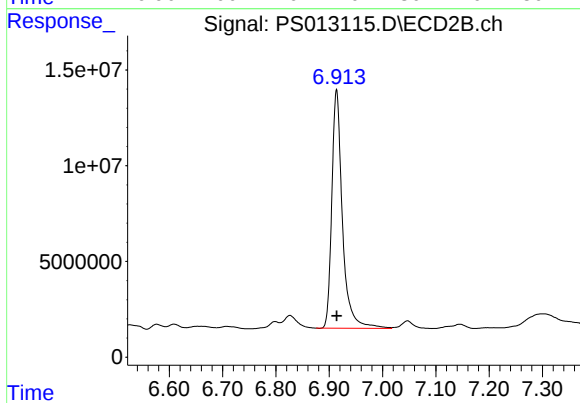

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 172054386
Conc: 442.20 ng/ml

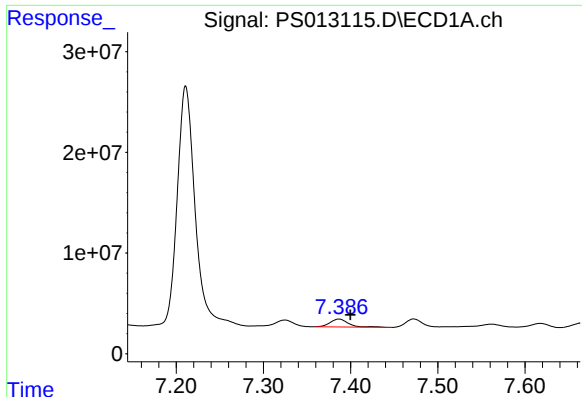

#5 DICAMBA


R.T.: 7.387 min
Delta R.T.: -0.013 min
Response: 11502147
Conc: 3.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

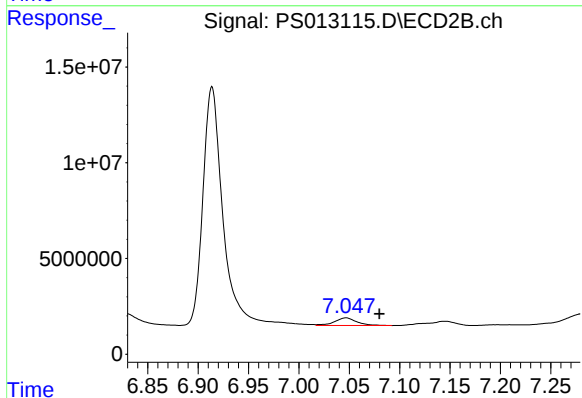


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.033 min
Response: 6070136
Conc: 3.66 ng/ml

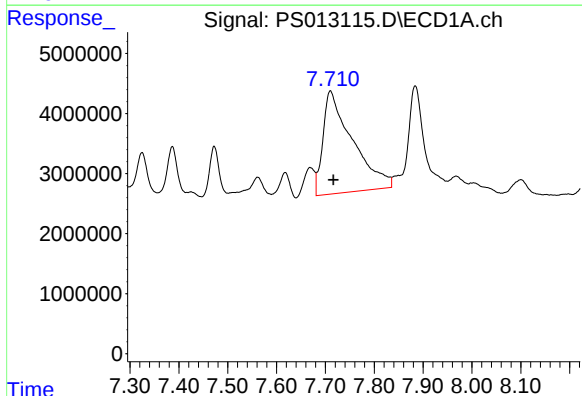


#7 MCPA

R.T.: 7.710 min
Delta R.T.: -0.006 min
Response: 71438547
Conc: 18.71 ug/ml

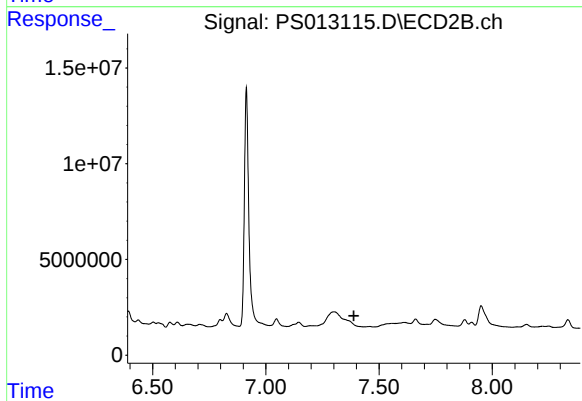

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.389 min
Response: 0
Conc: N.D.

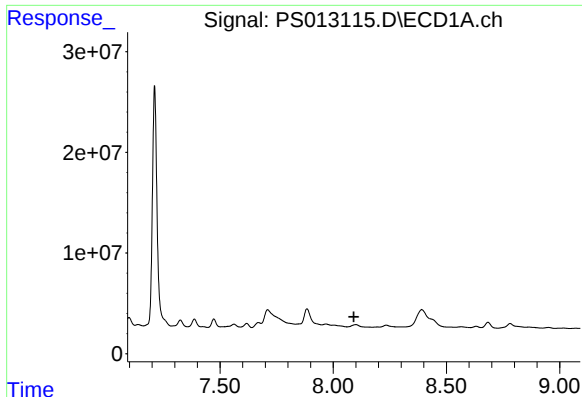

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

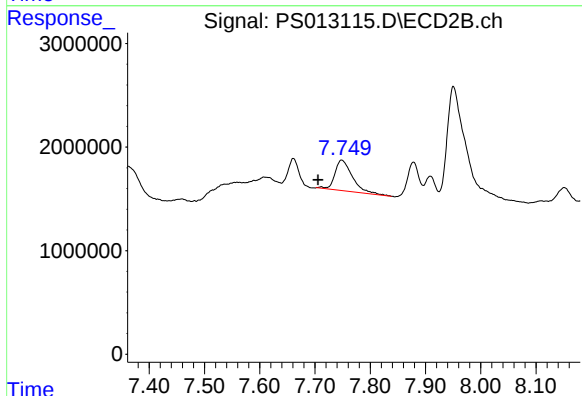


#8 DICHLORPROP

R.T.: 7.748 min
Delta R.T.: 0.043 min
Response: 6486387
Conc: 14.51 ng/ml

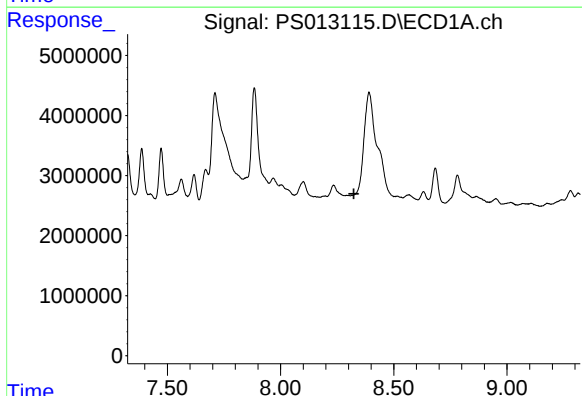


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

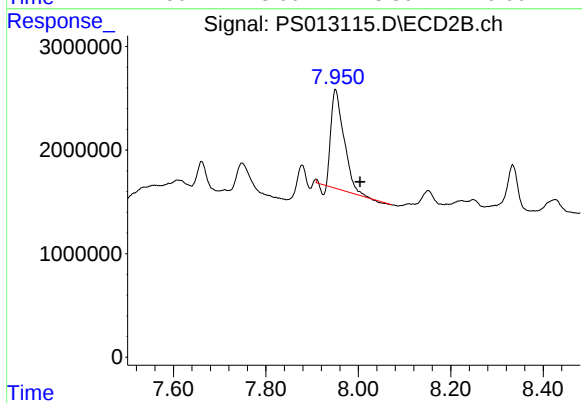

#9 2,4-D


R.T.: 7.951 min
Delta R.T.: -0.053 min
Response: 18176545
Conc: 34.25 ng/ml

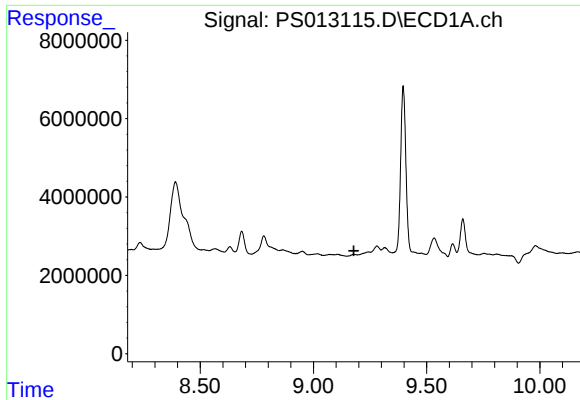

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

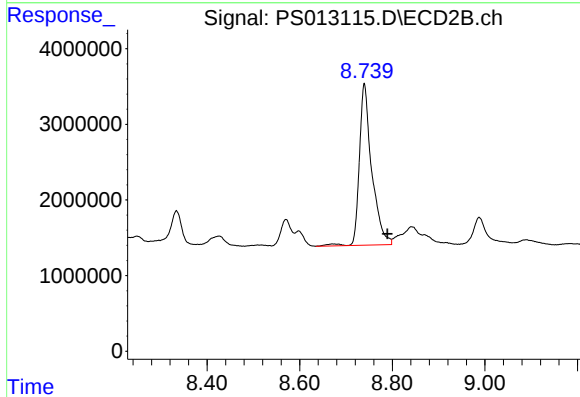


#11 2,4,5-TP (SILVEX)

R.T.: 8.740 min
Delta R.T.: -0.050 min
Response: 39535898
Conc: 17.06 ng/ml

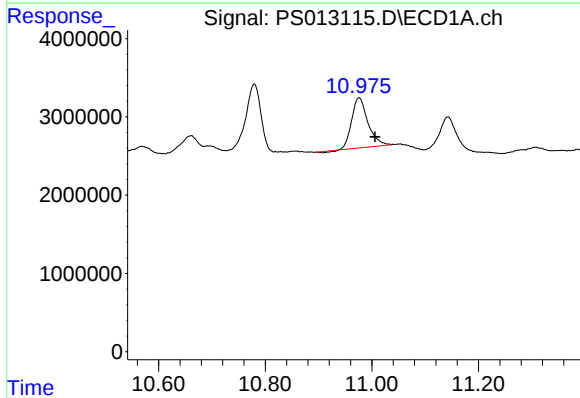

#15 Picloram

R.T.: 10.976 min
Delta R.T.: -0.030 min
Response: 13434519
Conc: 2.04 ng/ml

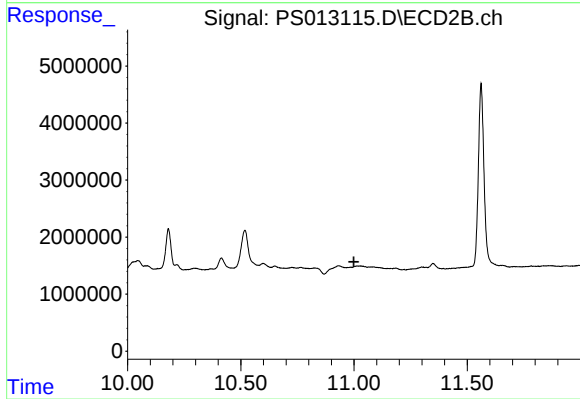

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.999 min
Response: 0
Conc: N.D.