

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
 Data File : PS013116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 19:35
 Operator : DD\AJ
 Sample : L4600-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:55:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	6.913	338.8E6	169.8E6	379.038	436.294
Target Compounds							
1) T	Dalapon	2.994	2.590	73101043	151.0E6	69.093	284.842 #
2) T	3,5-DICHL...	0.000	6.095	0	81482218	N.D.	132.454
3) T	4-Nitroph...	7.097f	6.576f	10632263	2355337	24.930	9.890 #
5) T	DICAMBA	7.385	7.046	10182746	5485114	2.851	3.304
7) T	MCPA	7.709	0.000	76752565	0	20.101	N.D. #
8) T	DICHLORPROP	0.000	7.747f	0	6261078	N.D.	14.008
9) T	2,4-D	0.000	7.950f	0	27593562	N.D.	51.994
10) T	Pentachlo...	8.683f	8.427	8071855	5445725	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.739f	0	39117441	N.D.	16.879
15) T	Picloram	10.974	0.000	13001819	0	1.977	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
Data File : PS013116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 19:35
Operator : DD\AJ
Sample : L4600-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:55:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

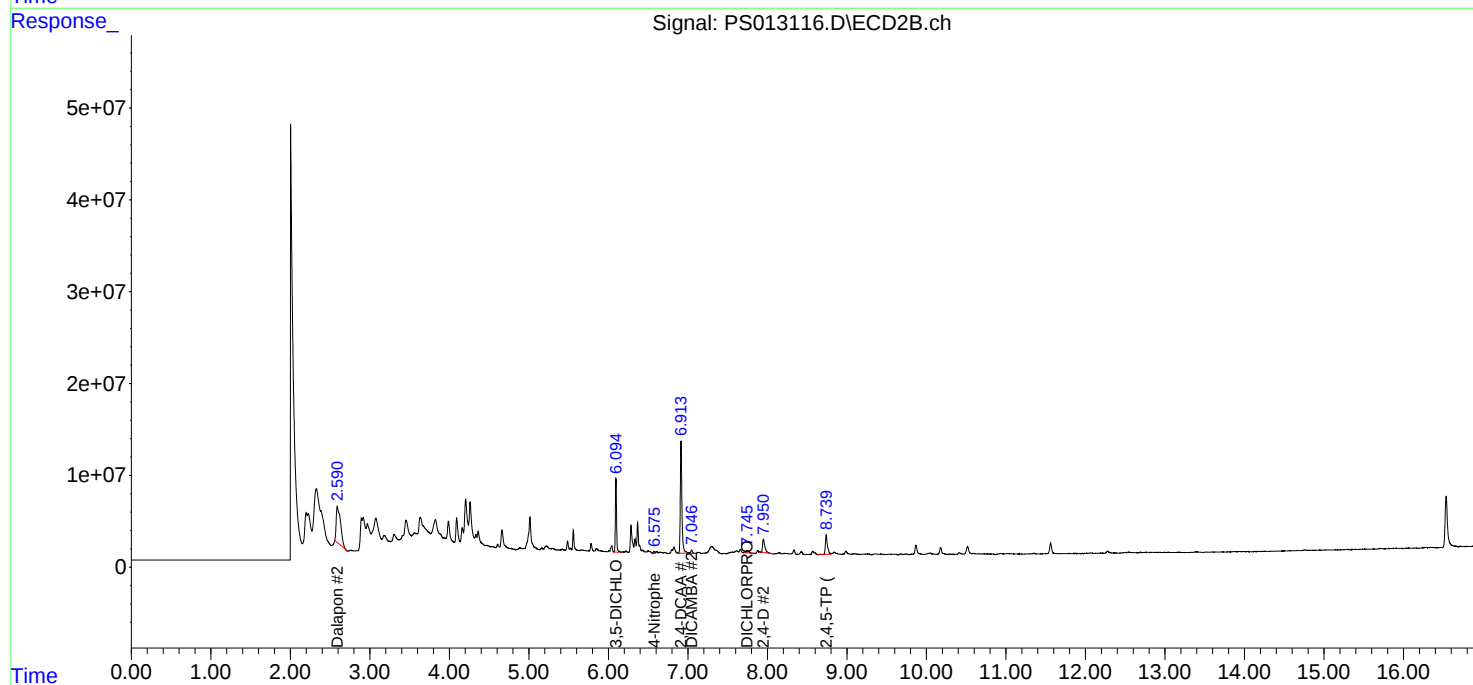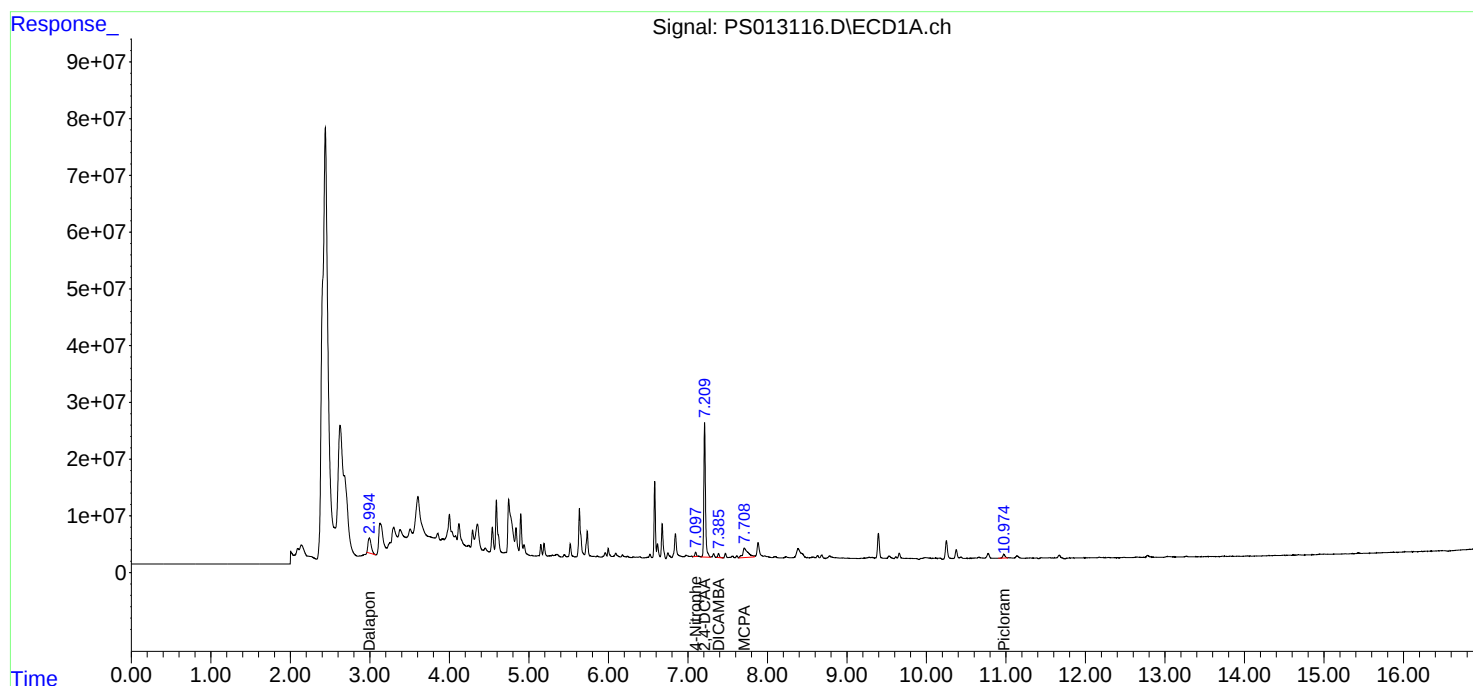


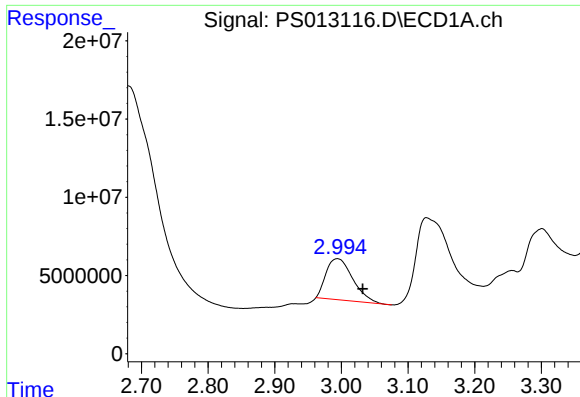

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.038 min
Response: 73101043
Conc: 69.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

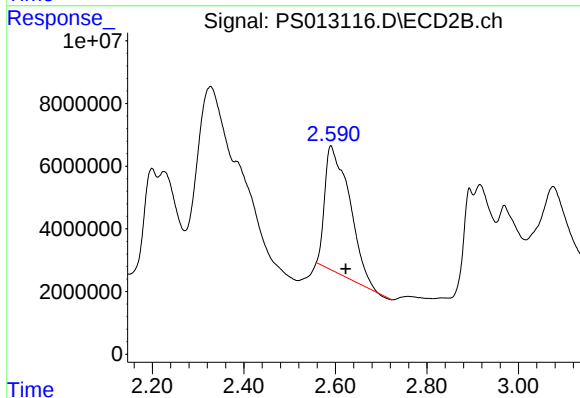


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.033 min
Response: 150959170
Conc: 284.84 ng/ml

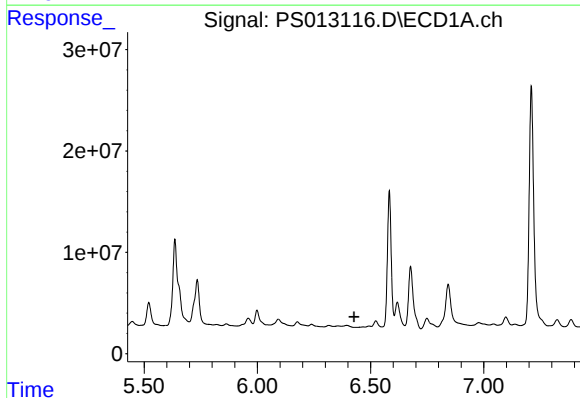


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.427 min
Response: 0
Conc: N.D.

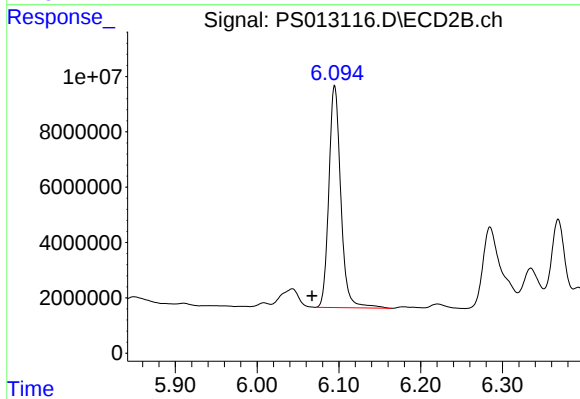

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 81482218
Conc: 132.45 ng/ml

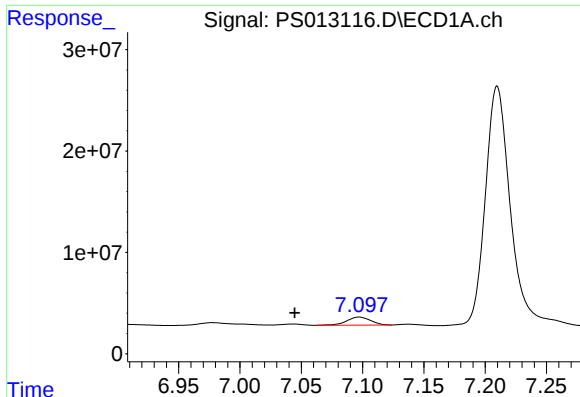

#3 4-Nitrophenol


R.T.: 7.097 min
Delta R.T.: 0.053 min
Response: 10632263
Conc: 24.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

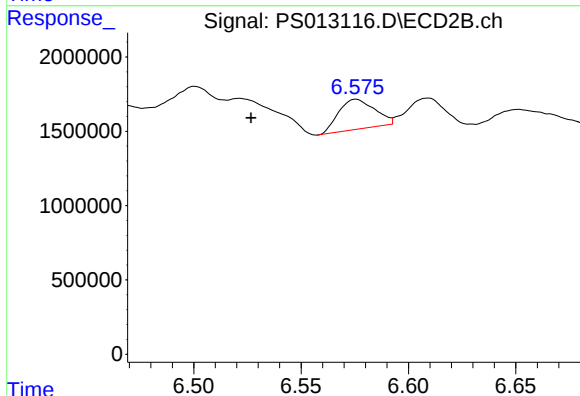


#3 4-Nitrophenol

R.T.: 6.576 min
Delta R.T.: 0.049 min
Response: 2355337
Conc: 9.89 ng/ml

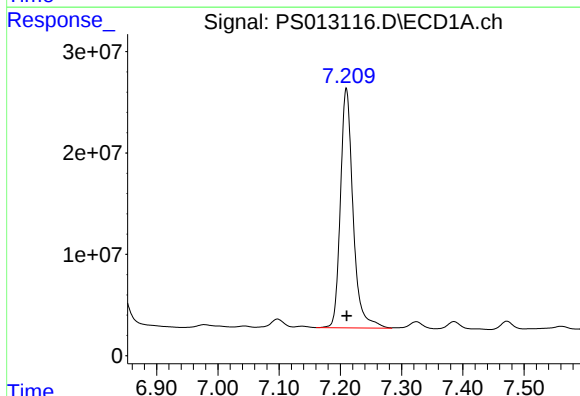


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: 0.000 min
Response: 338832997
Conc: 379.04 ng/ml

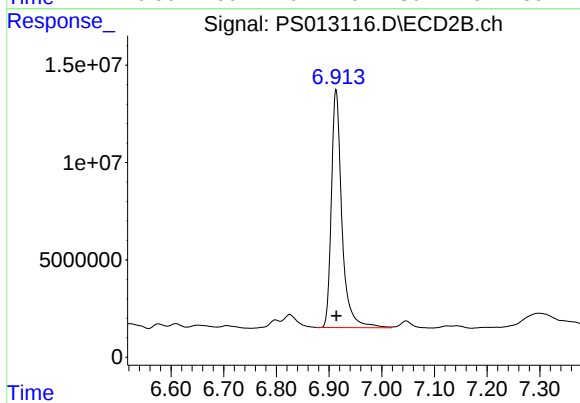

#4 2,4-DCAA


R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 169757276
Conc: 436.29 ng/ml

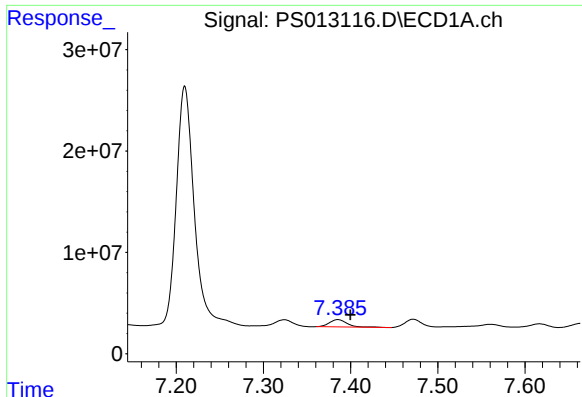

#5 DICAMBA


R.T.: 7.385 min
Delta R.T.: -0.014 min
Response: 10182746
Conc: 2.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

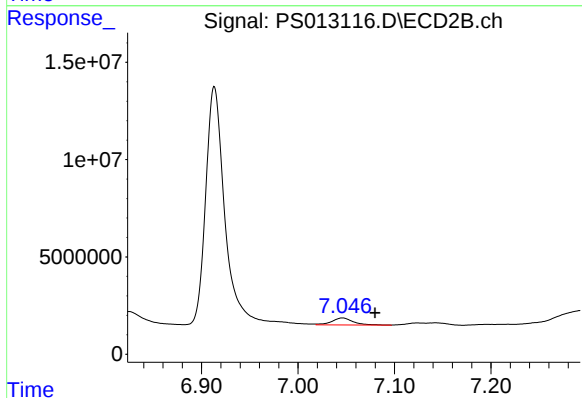


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 5485114
Conc: 3.30 ng/ml

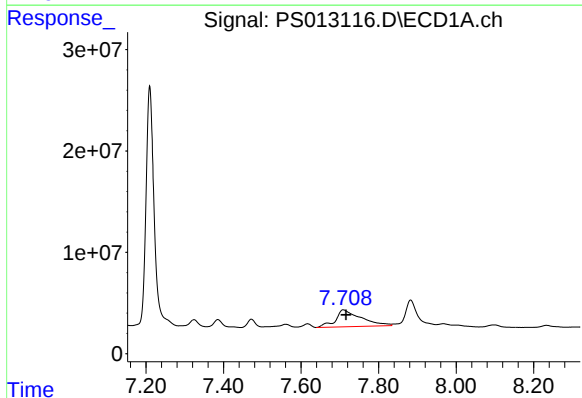


#7 MCPA

R.T.: 7.709 min
Delta R.T.: -0.007 min
Response: 76752565
Conc: 20.10 ug/ml

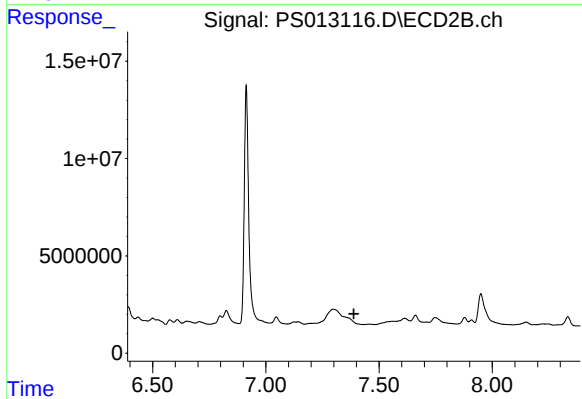

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.389 min
Response: 0
Conc: N.D.

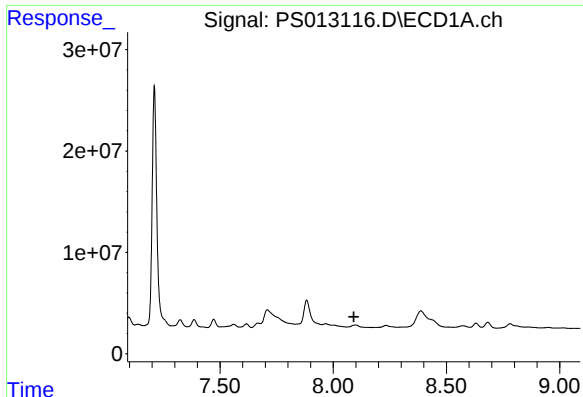

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

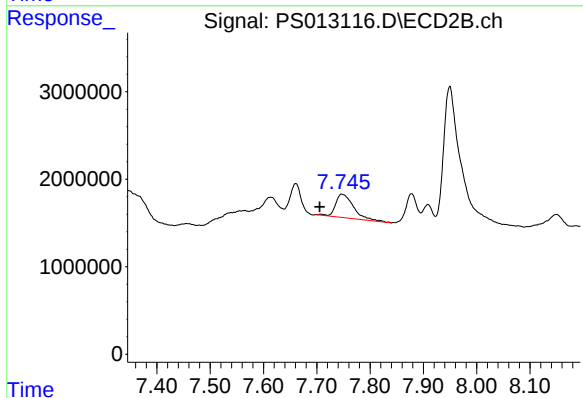


#8 DICHLORPROP

R.T.: 7.747 min
Delta R.T.: 0.041 min
Response: 6261078
Conc: 14.01 ng/ml

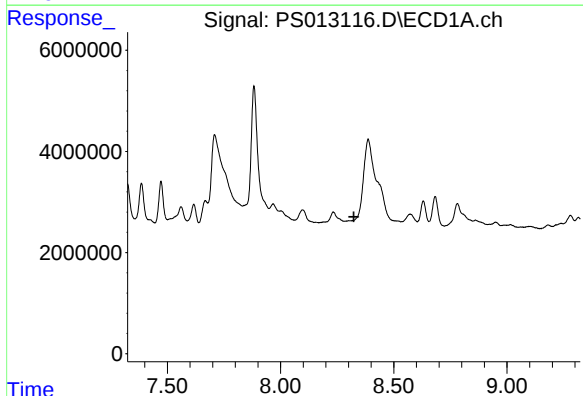


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

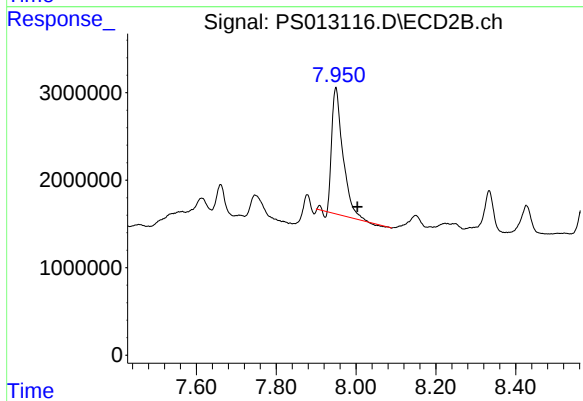

#9 2,4-D


R.T.: 7.950 min
Delta R.T.: -0.054 min
Response: 27593562
Conc: 51.99 ng/ml

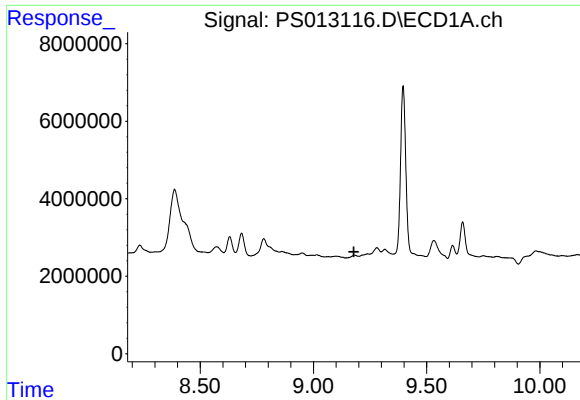

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

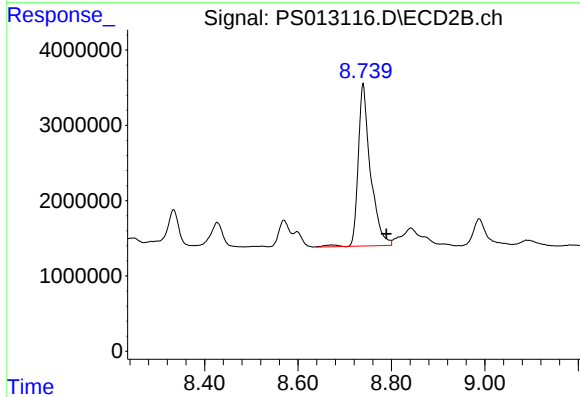


#11 2,4,5-TP (SILVEX)

R.T.: 8.739 min
Delta R.T.: -0.050 min
Response: 39117441
Conc: 16.88 ng/ml

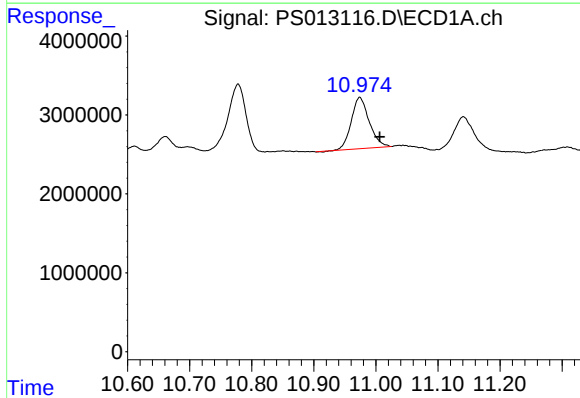

#15 Picloram

R.T.: 10.974 min
Delta R.T.: -0.032 min
Response: 13001819
Conc: 1.98 ng/ml

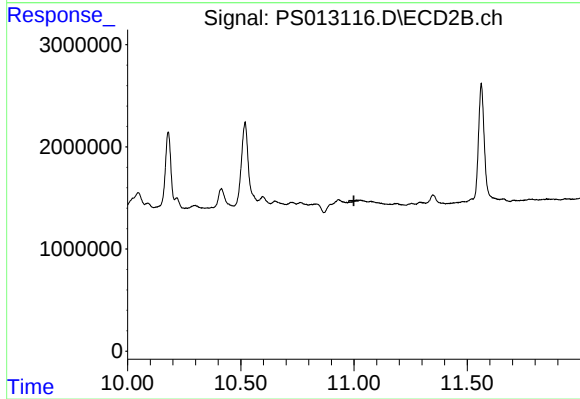

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.999 min
Response: 0
Conc: N.D.