

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
 Data File : PS013119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 20:44
 Operator : DD\AJ
 Sample : L4605-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:56:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	340.1E6	170.4E6	380.492	437.983
Target Compounds							
1) T	Dalapon	2.994	2.591	74881680	146.3E6	70.776	276.073 #
2) T	3,5-DICHL...	0.000	6.044	0	2079574	N.D.	3.380
3) T	4-Nitroph...	7.098f	6.576f	10501239	2293813	24.623	9.632 #
5) T	DICAMBA	7.386	7.046	12697469	6395134	3.555	3.852
7) T	MCPA	7.712	0.000	69310976	0	18.152	N.D. #
8) T	DICHLORPROP	0.000	7.748f	0	6659577	N.D.	14.900
9) T	2,4-D	0.000	7.951f	0	15138673	N.D.	28.526
10) T	Pentachlo...	8.682f	0.000	8784954	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.739f	0	33489890	N.D.	14.451
15) T	Picloram	10.976	11.040f	12290675	15265706	1.869	4.229 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
Data File : PS013119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 20:44
Operator : DD\AJ
Sample : L4605-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:56:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

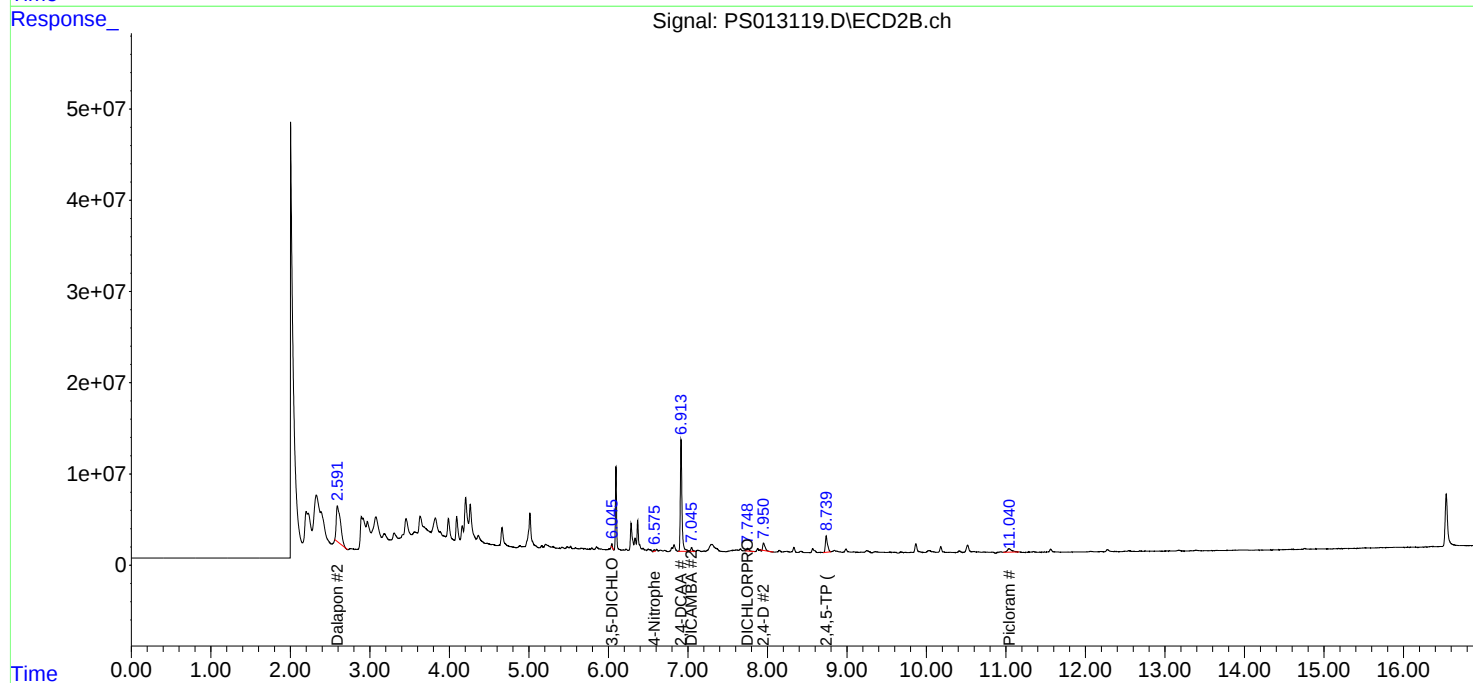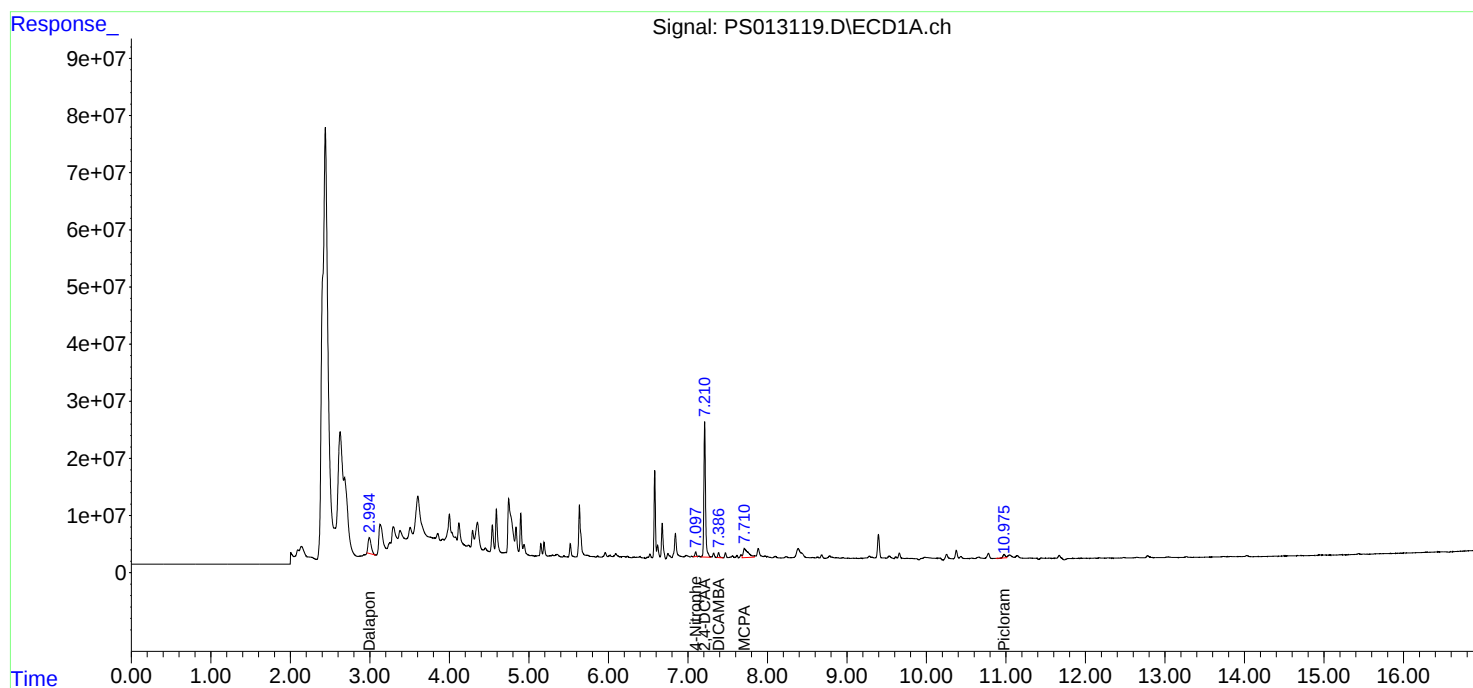


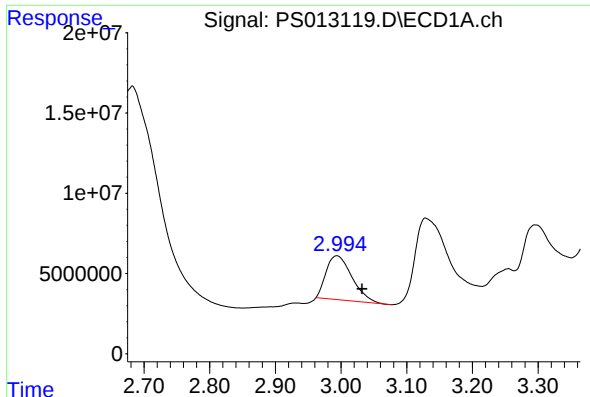

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.038 min
Response: 74881680
Conc: 70.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

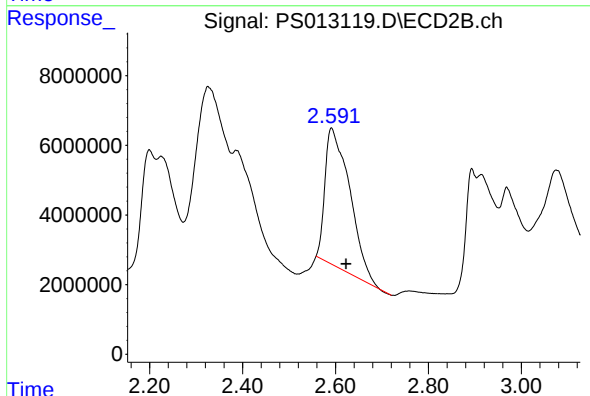


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.032 min
Response: 146311714
Conc: 276.07 ng/ml

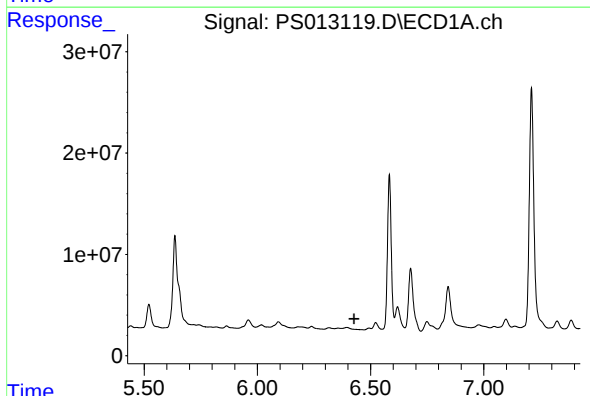


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.427 min
Response: 0
Conc: N.D.

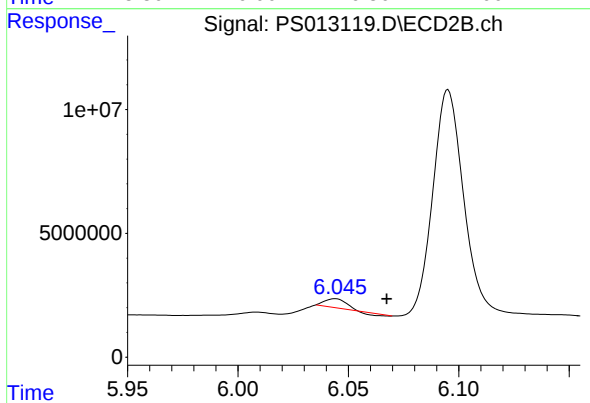

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.044 min
Delta R.T.: -0.023 min
Response: 2079574
Conc: 3.38 ng/ml

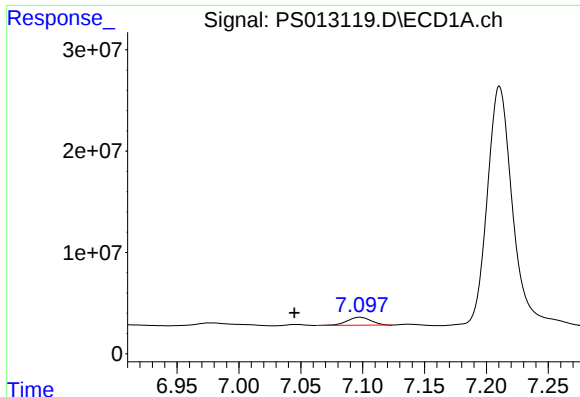

#3 4-Nitrophenol


R.T.: 7.098 min
Delta R.T.: 0.053 min
Response: 10501239
Conc: 24.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

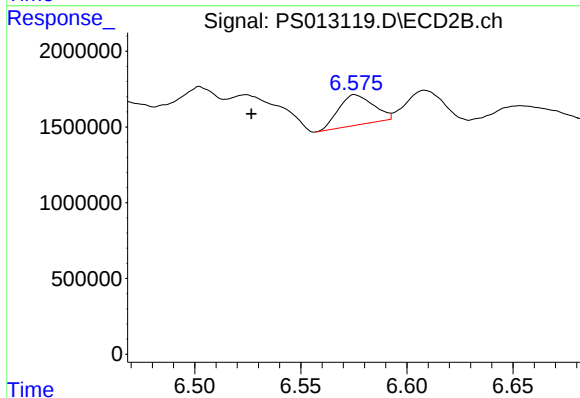


#3 4-Nitrophenol

R.T.: 6.576 min
Delta R.T.: 0.049 min
Response: 2293813
Conc: 9.63 ng/ml

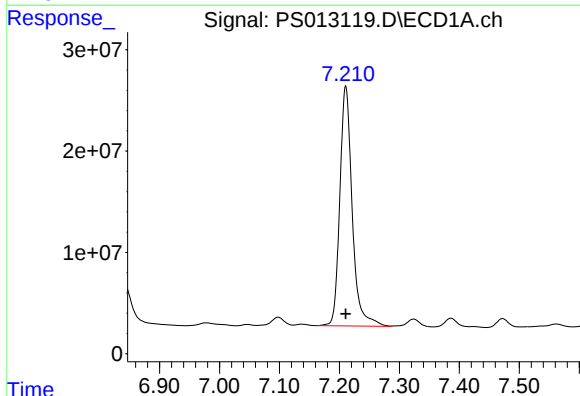


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 340132505
Conc: 380.49 ng/ml

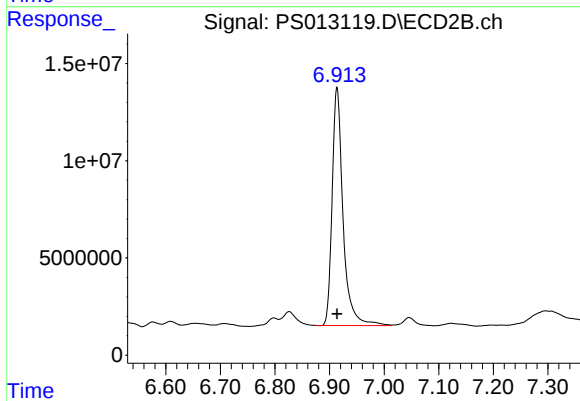

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 170414432
Conc: 437.98 ng/ml

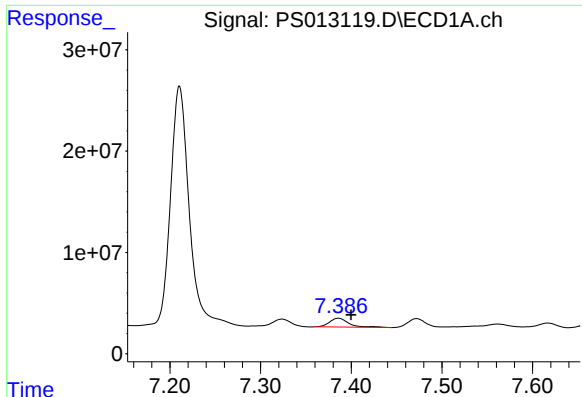

#5 DICAMBA


R.T.: 7.386 min
Delta R.T.: -0.014 min
Response: 12697469
Conc: 3.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

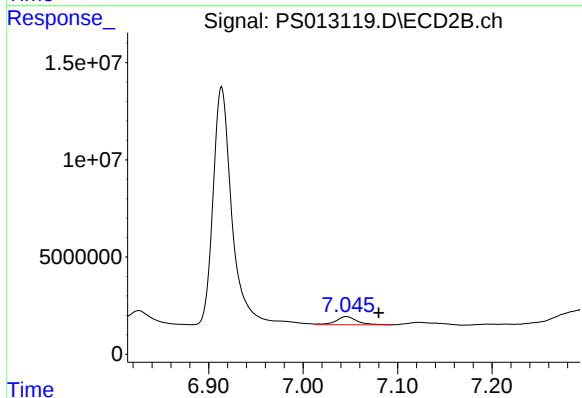


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 6395134
Conc: 3.85 ng/ml

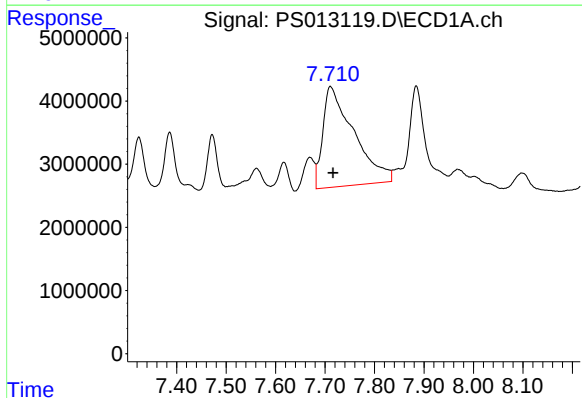


#7 MCPA

R.T.: 7.712 min
Delta R.T.: -0.005 min
Response: 69310976
Conc: 18.15 ug/ml

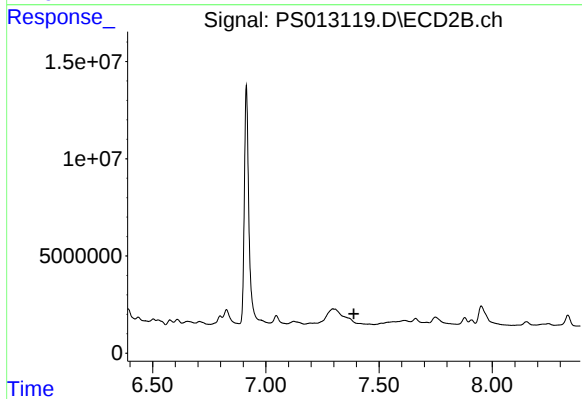

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.389 min
Response: 0
Conc: N.D.

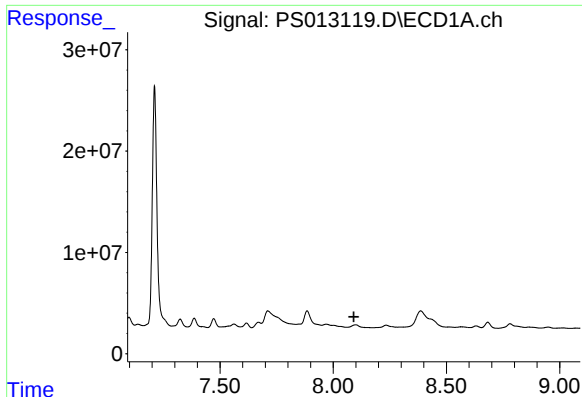

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

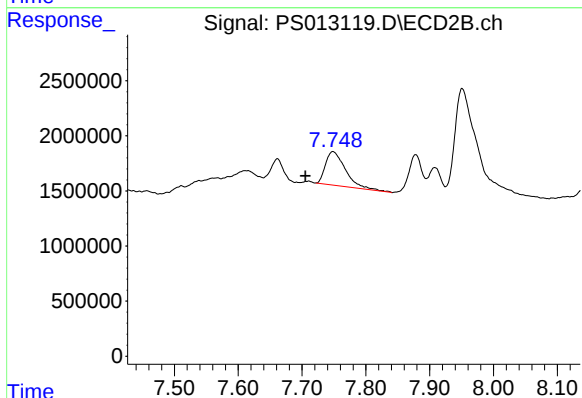


#8 DICHLORPROP

R.T.: 7.748 min
Delta R.T.: 0.043 min
Response: 6659577
Conc: 14.90 ng/ml

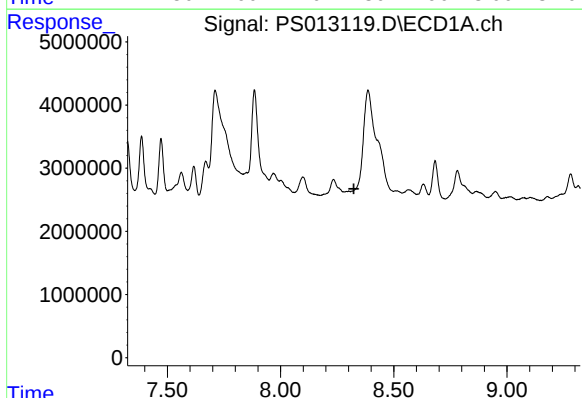


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

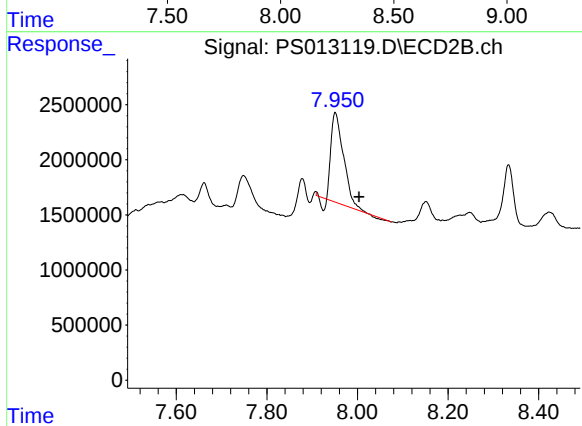

#9 2,4-D


R.T.: 7.951 min
Delta R.T.: -0.053 min
Response: 15138673
Conc: 28.53 ng/ml

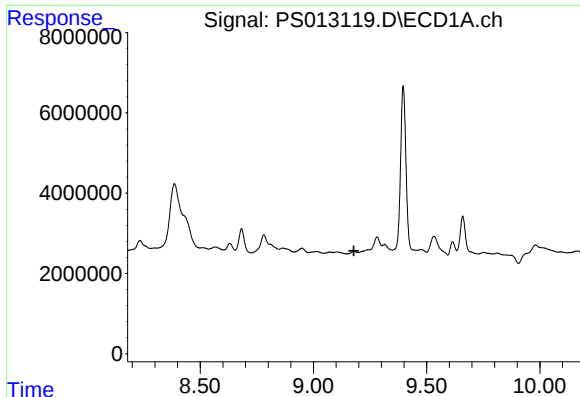

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

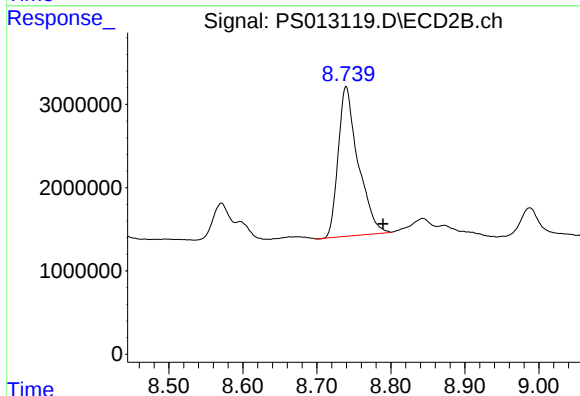


#11 2,4,5-TP (SILVEX)

R.T.: 8.739 min
Delta R.T.: -0.050 min
Response: 33489890
Conc: 14.45 ng/ml

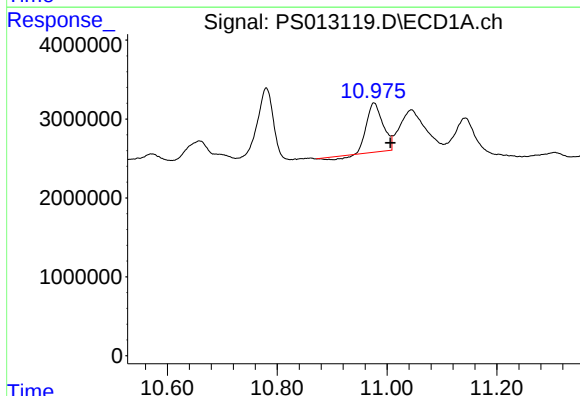

#15 Picloram

R.T.: 10.976 min
Delta R.T.: -0.030 min
Response: 12290675
Conc: 1.87 ng/ml

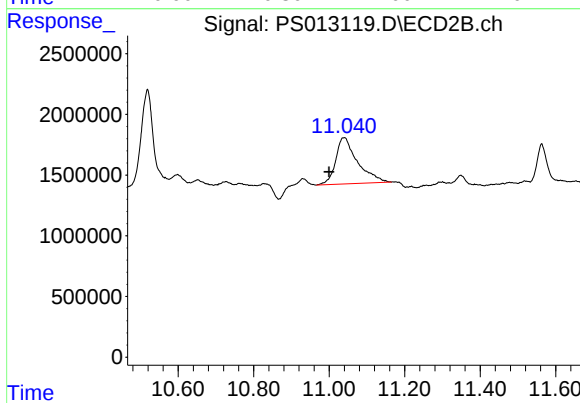

#15 Picloram

R.T.: 11.040 min
Delta R.T.: 0.041 min
Response: 15265706
Conc: 4.23 ng/ml