

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
 Data File : PS013120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 21:07
 Operator : DD\AJ
 Sample : L4621-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:56:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	272.5E6	143.3E6	304.887	368.258
Target Compounds							
1) T	Dalapon	2.994	2.589	42786851	20231682	40.441	38.175
2) T	3,5-DICHL...	0.000	6.045	0	3393483	N.D.	5.516
3) T	4-Nitroph...	6.978f	0.000	3796264	0	8.901	N.D. #
5) T	DICAMBA	7.386	7.046	9374707	5835121	2.625	3.515 #
7) T	MCPA	7.723	0.000	83287746	0	21.812	N.D. #
9) T	2,4-D	0.000	7.959f	0	3429425	N.D.	6.462
11) T	2,4,5-TP ...	0.000	8.759	0	12381161	N.D.	5.343
15) T	Picloram	10.981	0.000	9428530	0	1.434	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110420\
Data File : PS013120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 21:07
Operator : DD\AJ
Sample : L4621-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:56:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

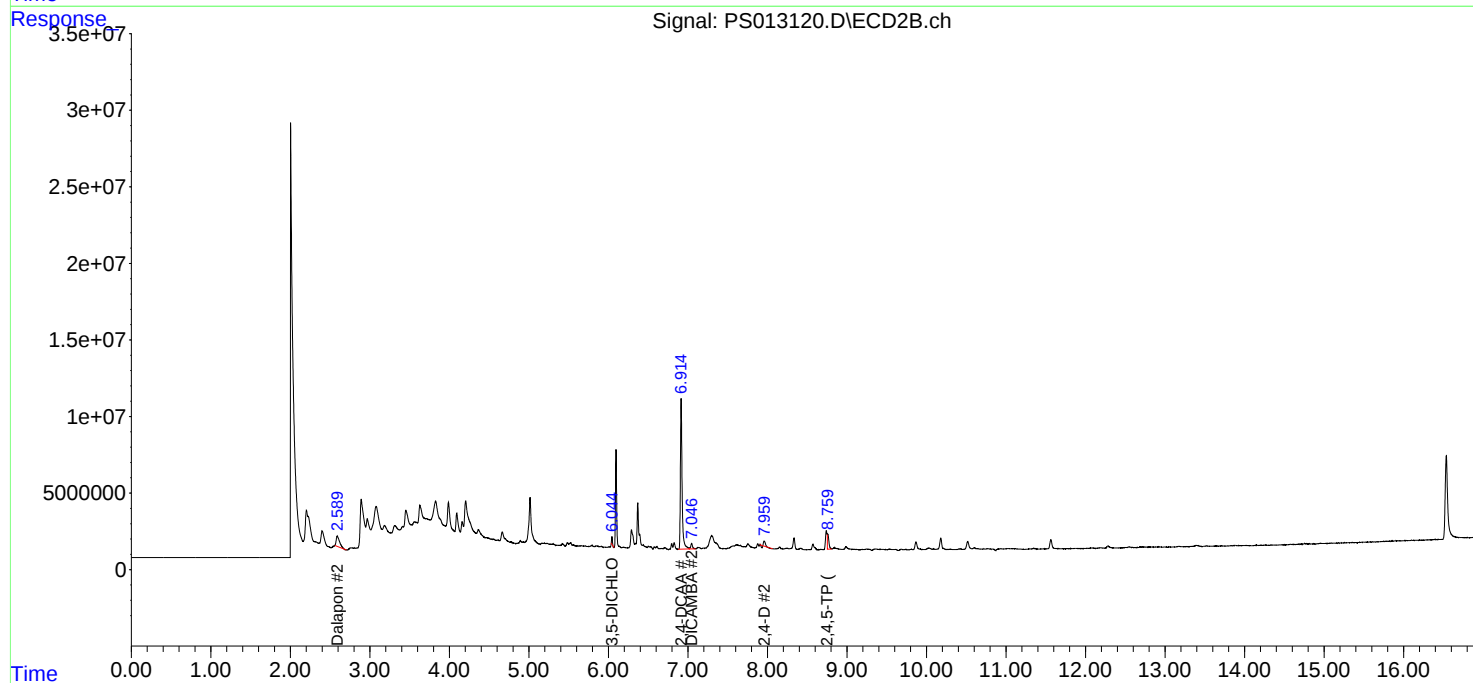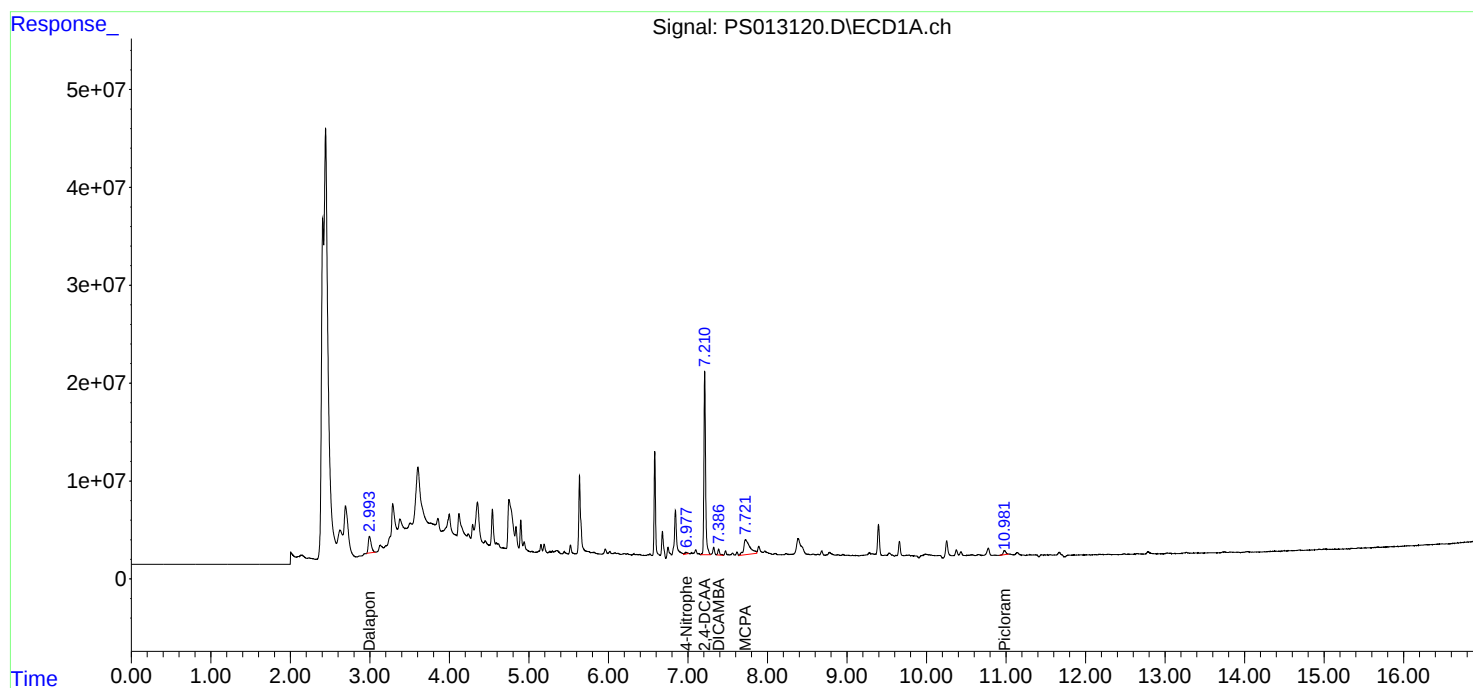


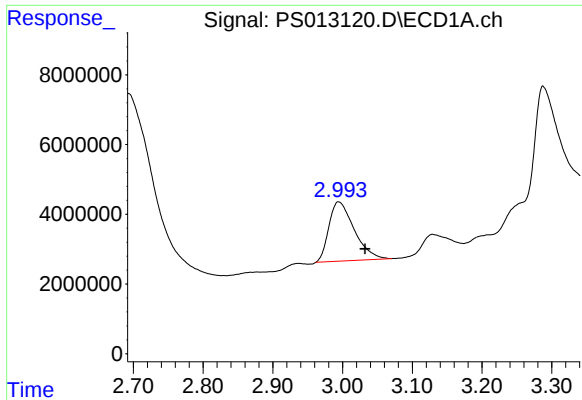

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.038 min
Response: 42786851
Conc: 40.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

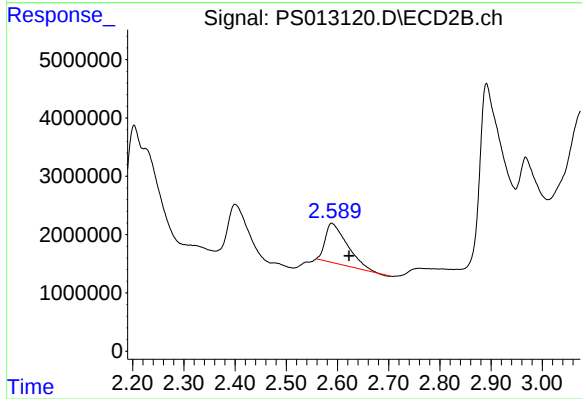


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.034 min
Response: 20231682
Conc: 38.17 ng/ml

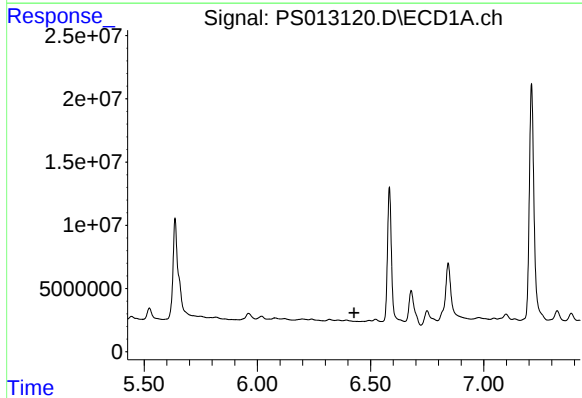


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.427 min
Response: 0
Conc: N.D.

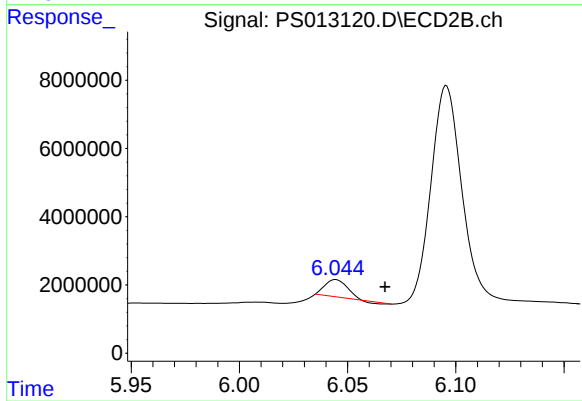

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.045 min
Delta R.T.: -0.023 min
Response: 3393483
Conc: 5.52 ng/ml

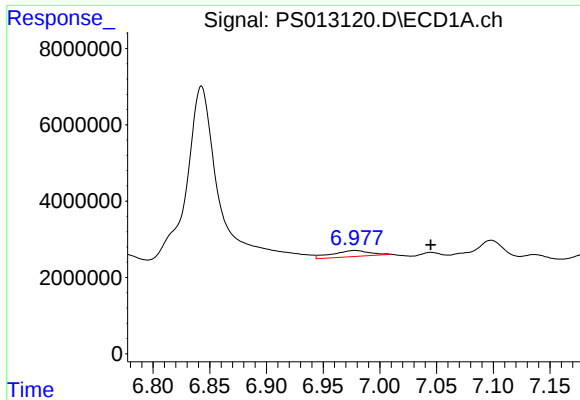

#3 4-Nitrophenol


R.T.: 6.978 min
Delta R.T.: -0.067 min
Response: 3796264
Conc: 8.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

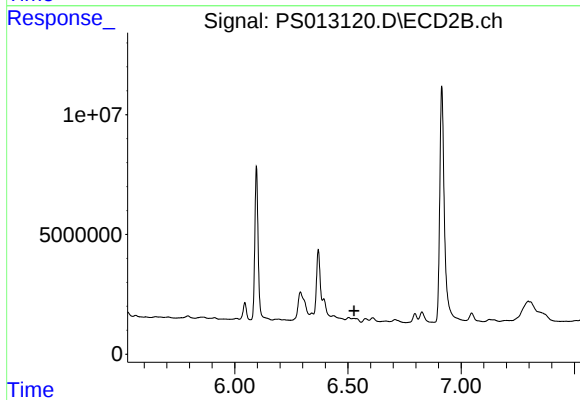


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

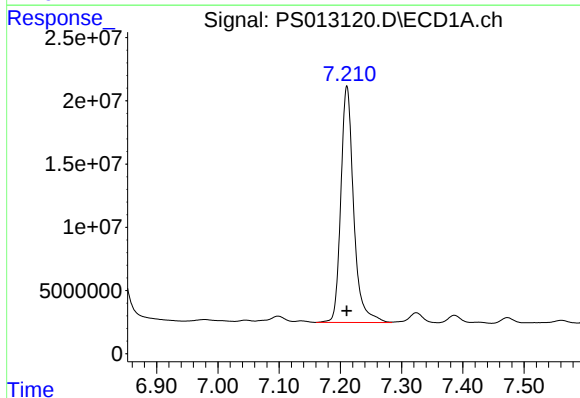


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 272546956
Conc: 304.89 ng/ml

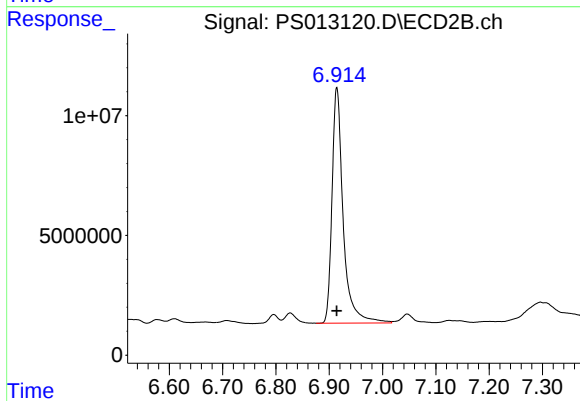

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 143285197
Conc: 368.26 ng/ml

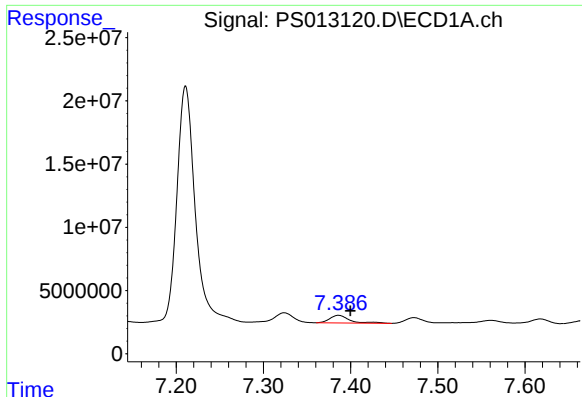

#5 DICAMBA


R.T.: 7.386 min
Delta R.T.: -0.014 min
Response: 9374707
Conc: 2.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

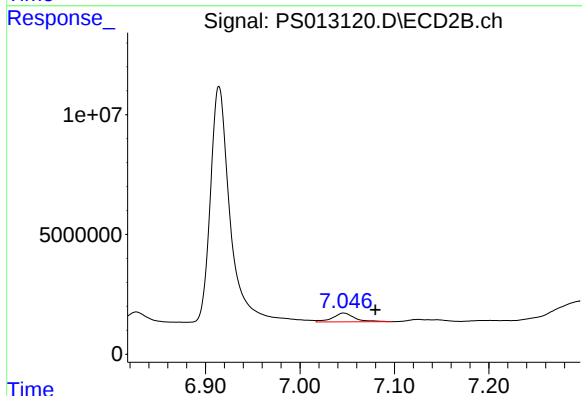


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 5835121
Conc: 3.52 ng/ml

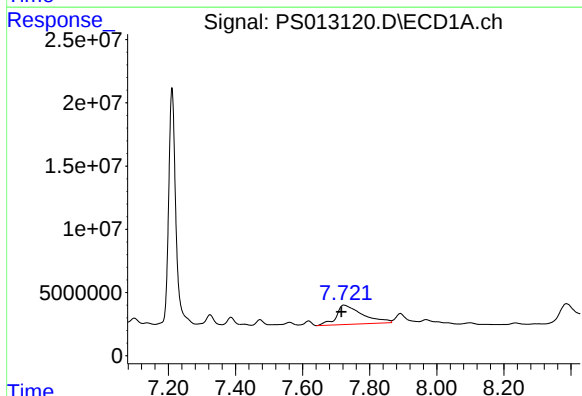


#7 MCPA

R.T.: 7.723 min
Delta R.T.: 0.007 min
Response: 83287746
Conc: 21.81 ug/ml

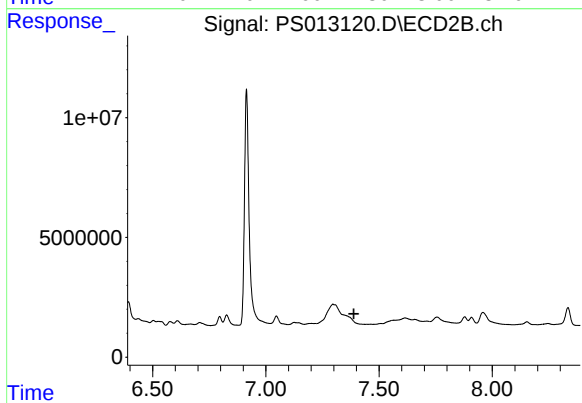

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.389 min
Response: 0
Conc: N.D.

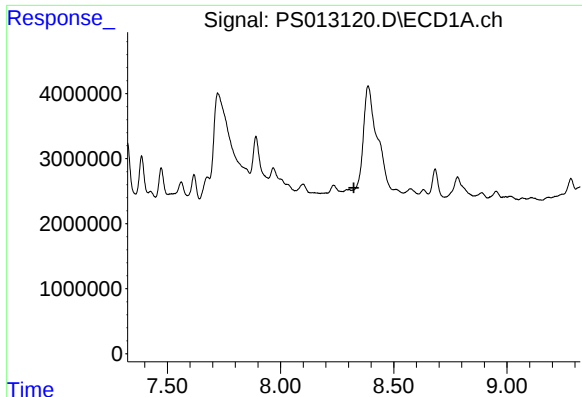

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

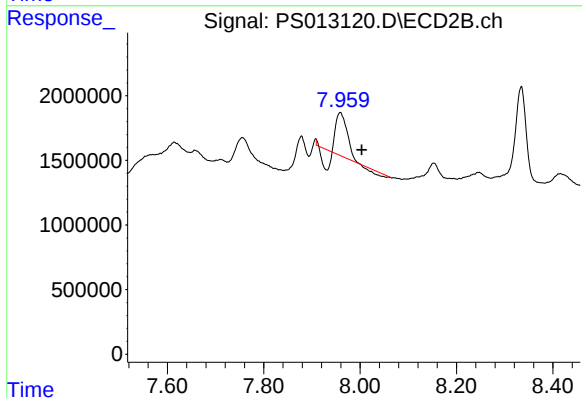


#9 2,4-D

R.T.: 7.959 min
Delta R.T.: -0.045 min
Response: 3429425
Conc: 6.46 ng/ml

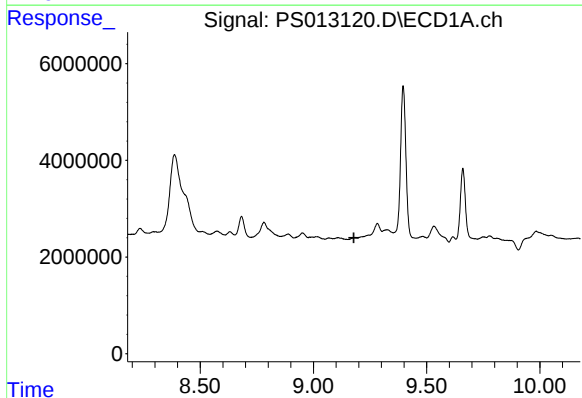


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

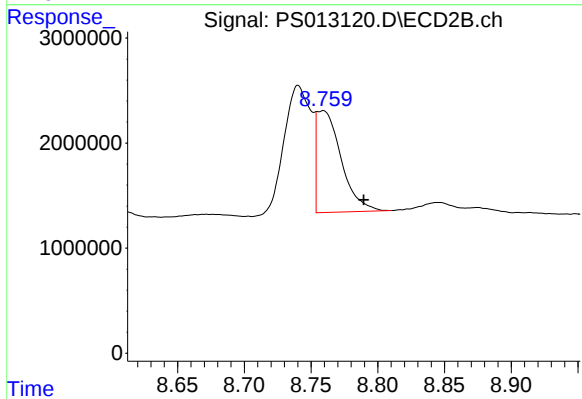

#11 2,4,5-TP (SILVEX)


R.T.: 8.759 min
Delta R.T.: -0.031 min
Response: 12381161
Conc: 5.34 ng/ml

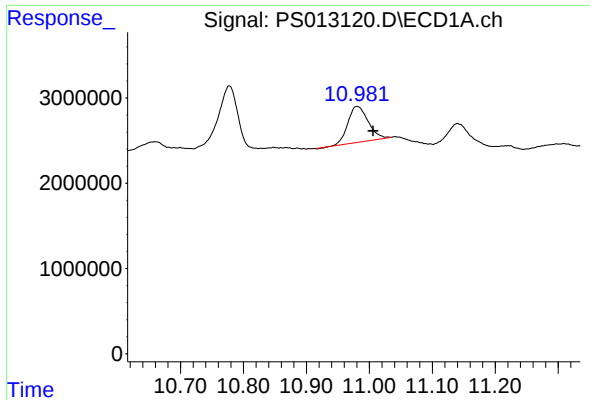

#15 Picloram

R.T.: 10.981 min
Delta R.T.: -0.025 min
Response: 9428530
Conc: 1.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

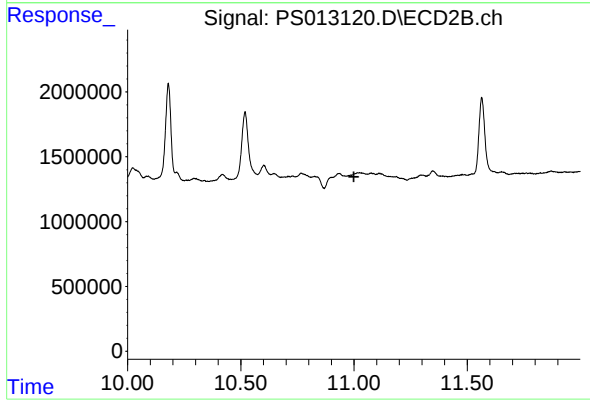

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.