

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110421\
 Data File : PS017330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2021 09:53
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 17:08:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
11)	T	2,4,5-TP ...	9.130	0.000	3758408	0	<MDL	N.D.	#
12)	T	2,4,5-T	9.435	0.000	9249778	0	1.152	N.D.	#
13)	T	2,4-DB	9.883f	0.000	7685007	0	5.109	N.D.	#
14)	T	DINOSEB	11.099	0.000	14174842	0	2.502	N.D.	#
15)	T	Picloram	10.958	10.791	201.0E6	65111039	18.817	17.001	
16)	T	DCPA	11.367	10.791f	5350982	65111039	<MDL	15.258	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110421\
Data File : PS017330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2021 09:53
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 17:08:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

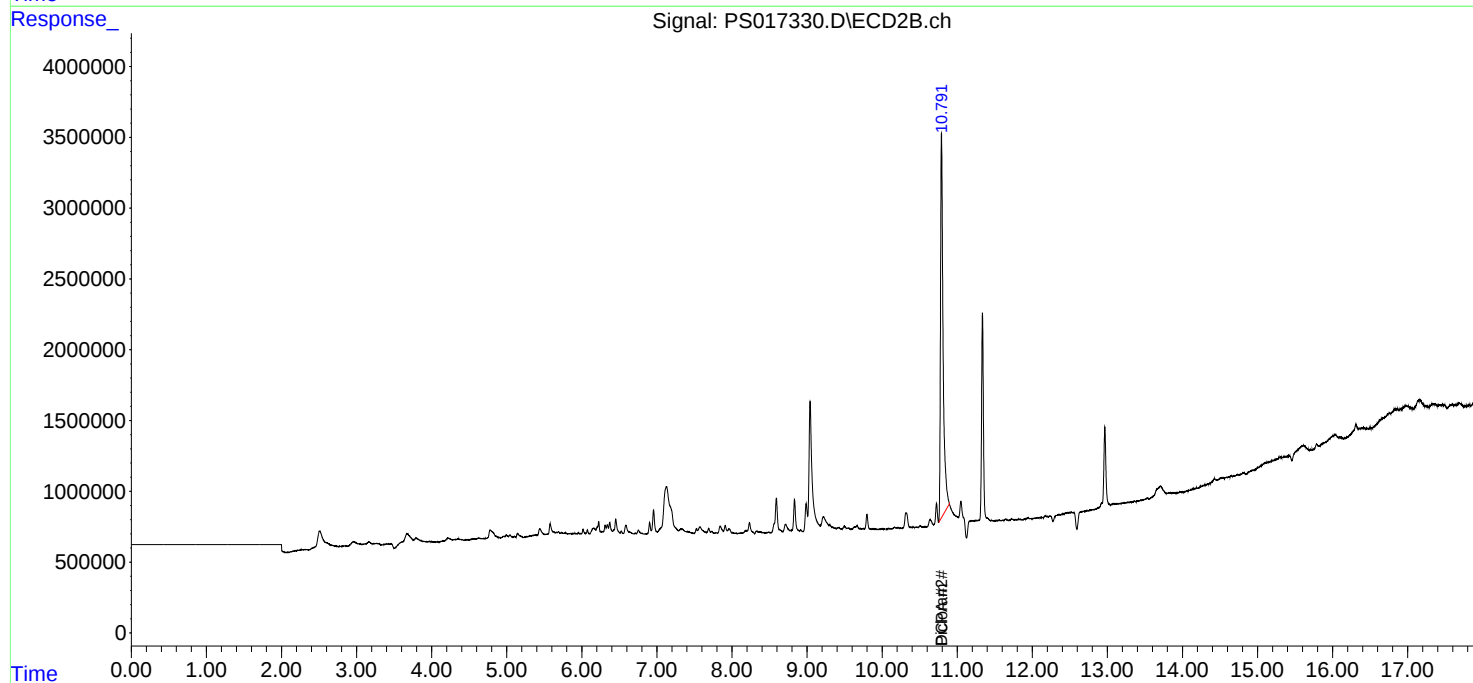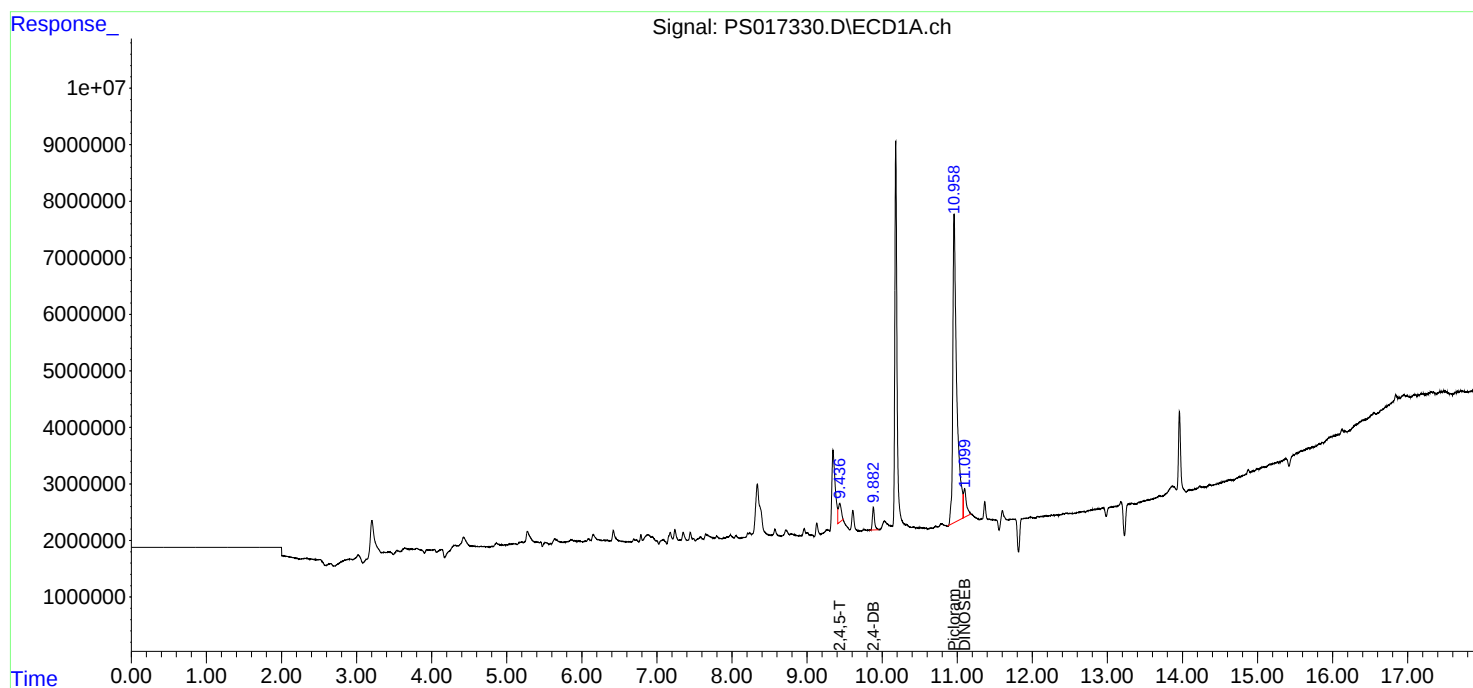


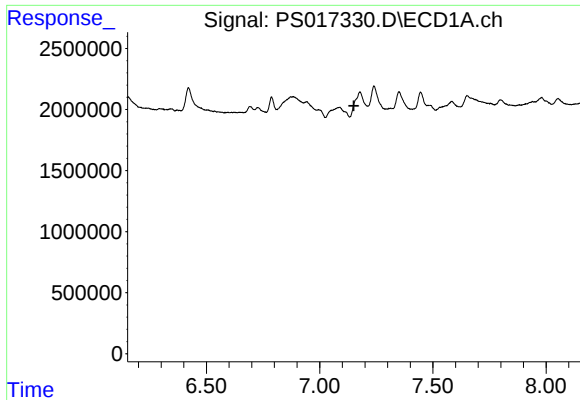

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

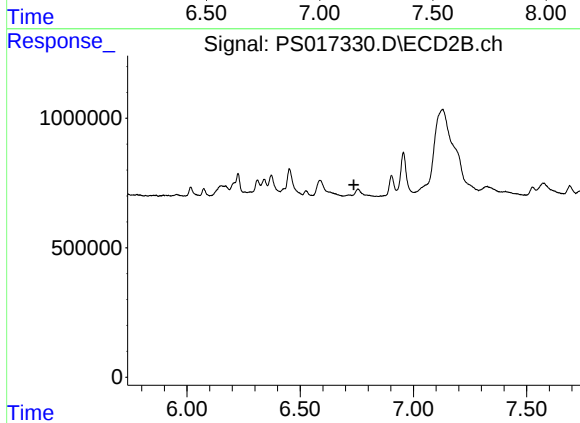


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.737 min
Response: 0
Conc: N.D.

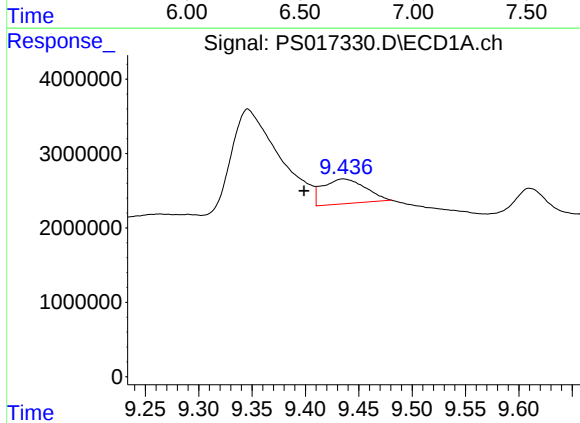


#12 2,4,5-T

R.T.: 9.435 min
Delta R.T.: 0.037 min
Response: 9249778
Conc: 1.15 ng/ml

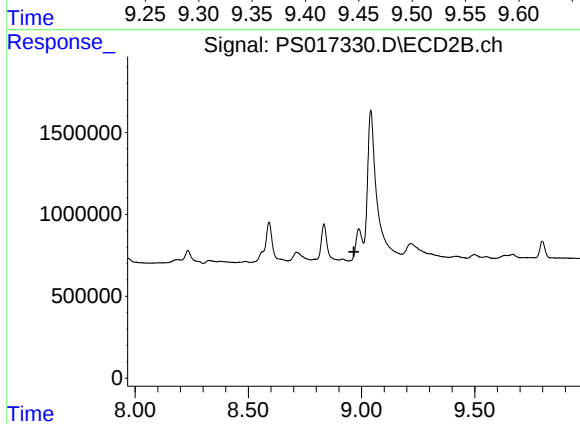

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.966 min
Response: 0
Conc: N.D.

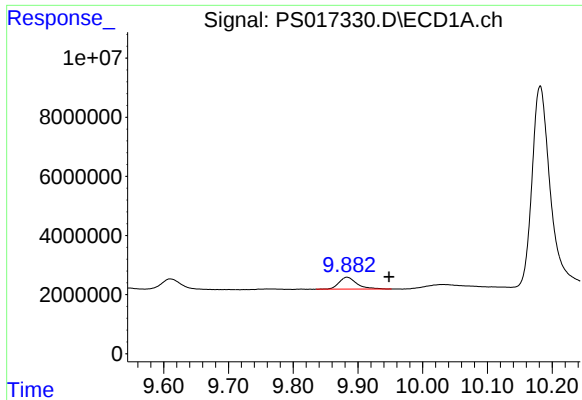

#13 2,4-DB


R.T.: 9.883 min
Delta R.T.: -0.065 min
Response: 7685007
Conc: 5.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

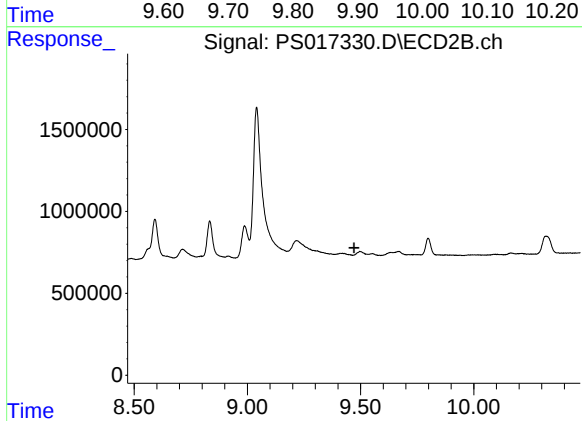


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.471 min
Response: 0
Conc: N.D.

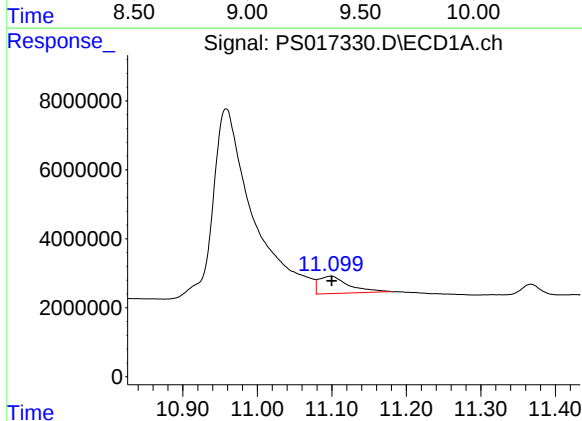


#14 DINOSEB

R.T.: 11.099 min
Delta R.T.: 0.000 min
Response: 14174842
Conc: 2.50 ng/ml

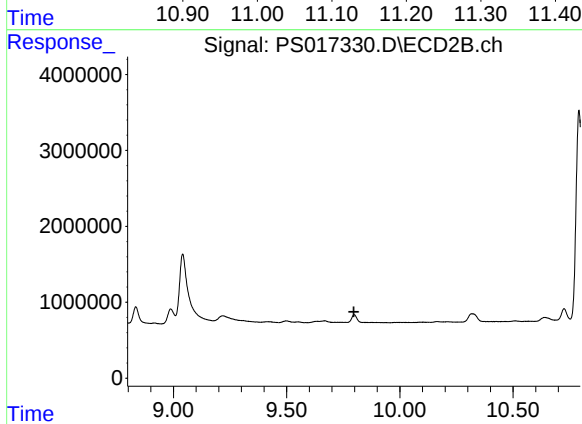

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.797 min
Response: 0
Conc: N.D.

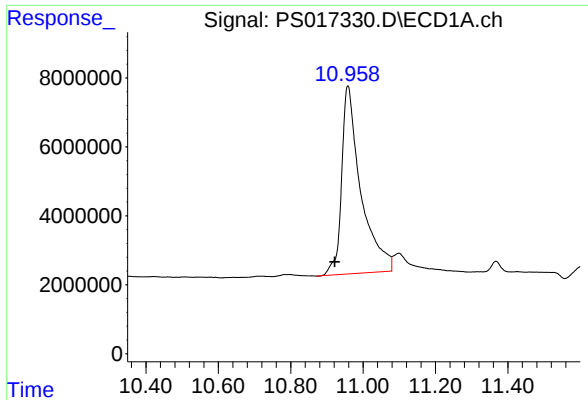

#15 Picloram


R.T.: 10.958 min
Delta R.T.: 0.036 min
Response: 200988625
Conc: 18.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

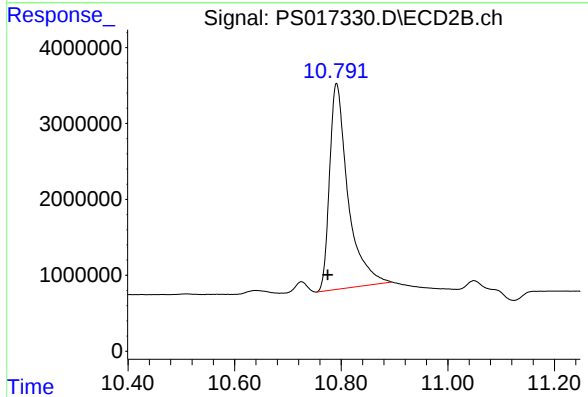


#15 Picloram

R.T.: 10.791 min
Delta R.T.: 0.016 min
Response: 65111039
Conc: 17.00 ng/ml

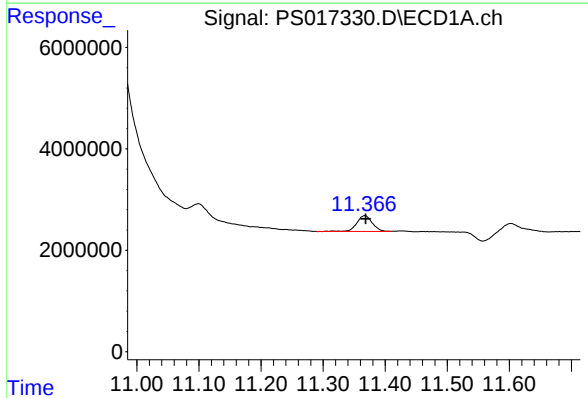

#16 DCPA

R.T.: 11.367 min
Delta R.T.: -0.001 min
Response: 5350982
Conc: N.D.

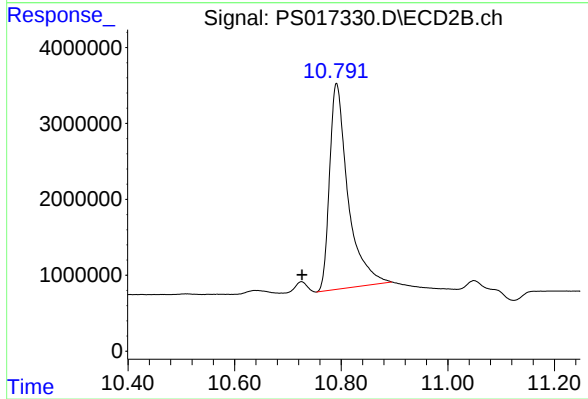

#16 DCPA

R.T.: 10.791 min
Delta R.T.: 0.065 min
Response: 65111039
Conc: 15.26 ng/ml