

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110421\
 Data File : PS017331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2021 10:17
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 17:15:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.154	6.739	679.1E6	282.2E6	444.290	482.850
Target Compounds							
12) T	2,4,5-T	9.366	0.000	23188316	0	2.887	N.D. #
15) T	Picloram	10.974f	10.799	127.5E6	41146388	11.936	10.744



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110421\
Data File : PS017331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2021 10:17
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 17:15:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

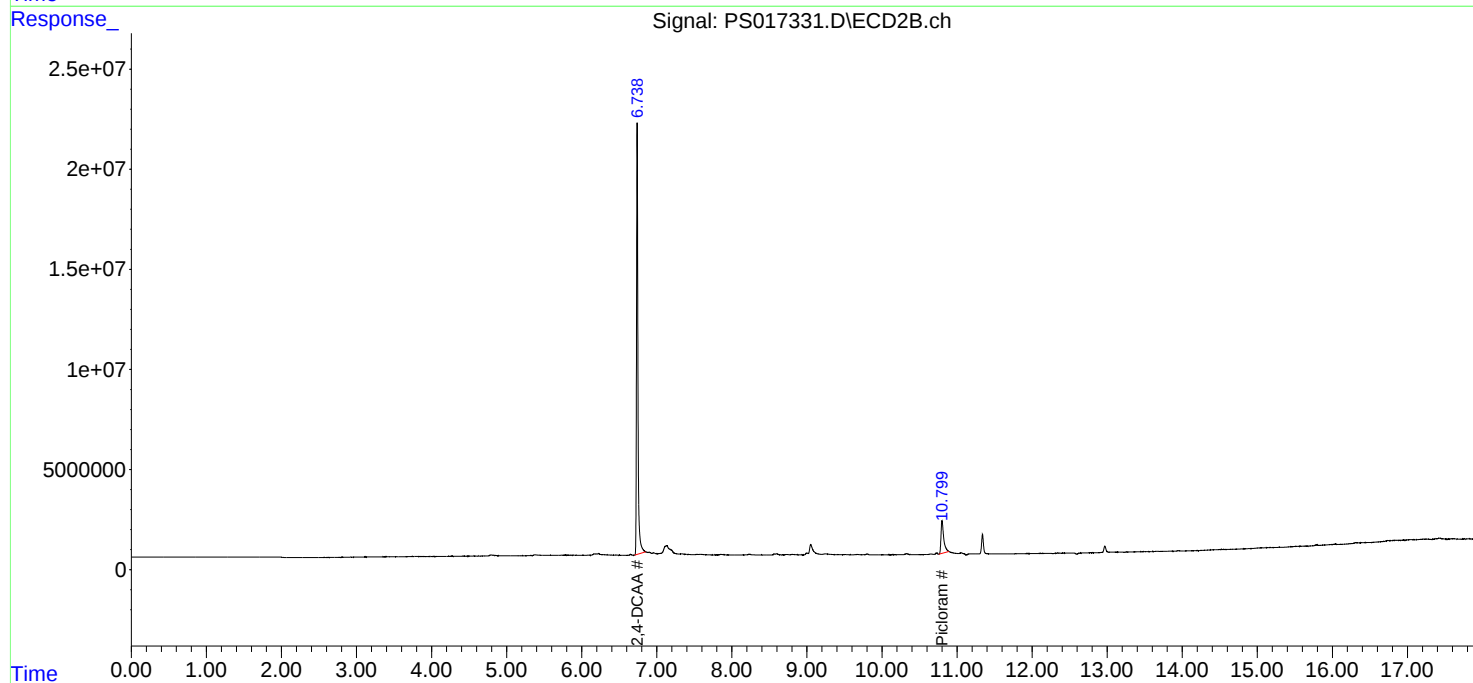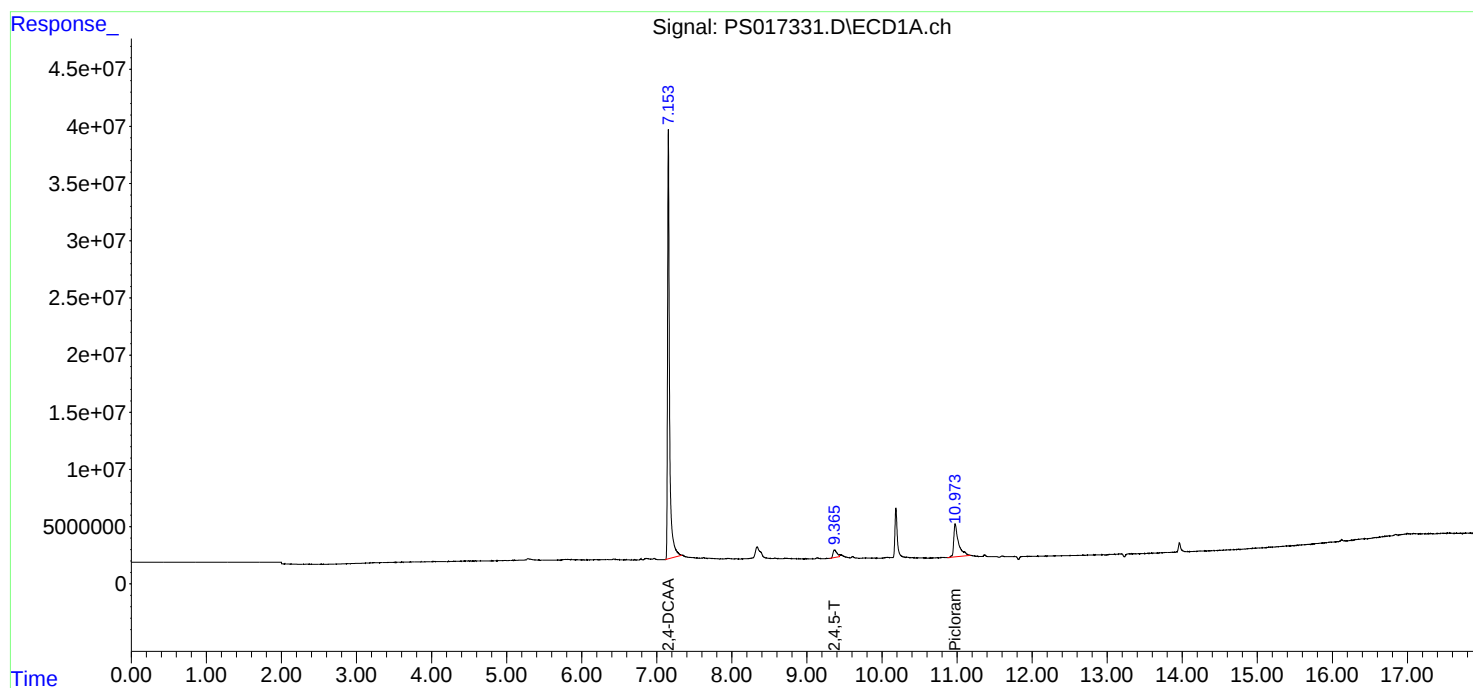


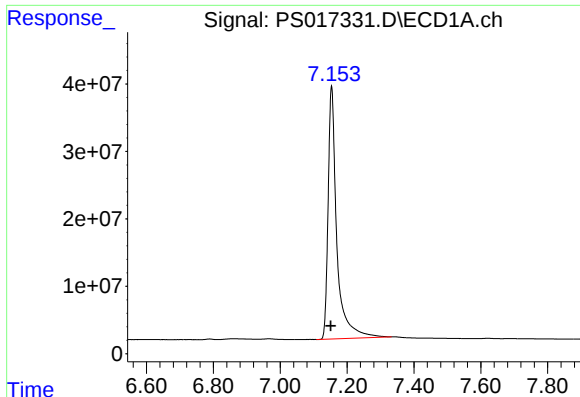

#4 2,4-DCAA


R.T.: 7.154 min
Delta R.T.: 0.002 min
Response: 679078806
Conc: 444.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

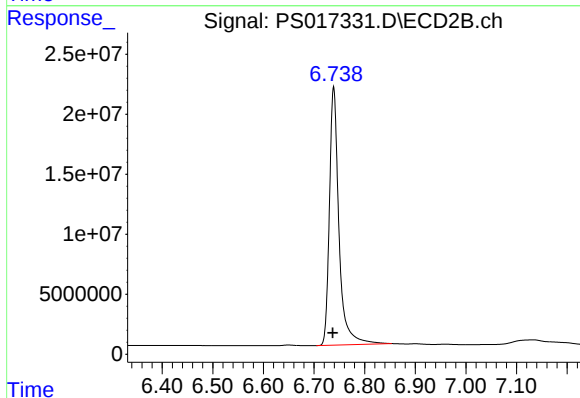


#4 2,4-DCAA

R.T.: 6.739 min
Delta R.T.: 0.002 min
Response: 282197584
Conc: 482.85 ng/ml

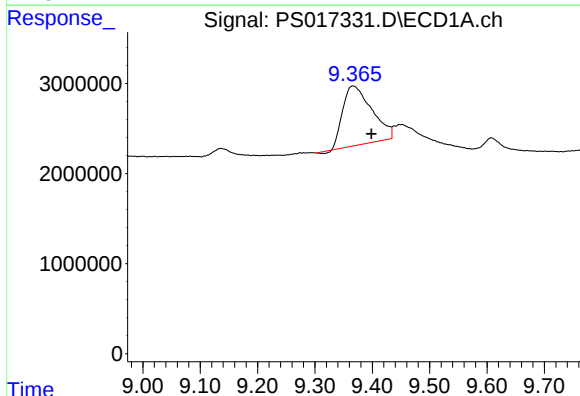


#12 2,4,5-T

R.T.: 9.366 min
Delta R.T.: -0.032 min
Response: 23188316
Conc: 2.89 ng/ml

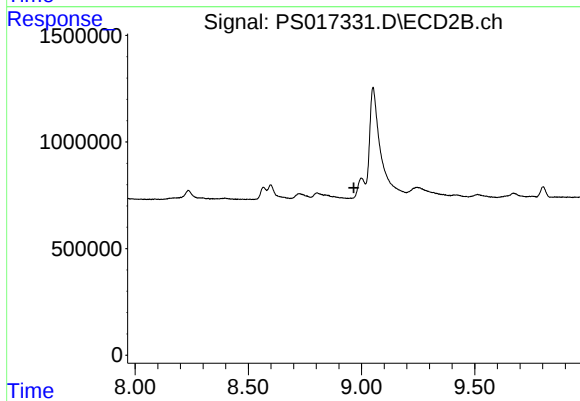

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.966 min
Response: 0
Conc: N.D.

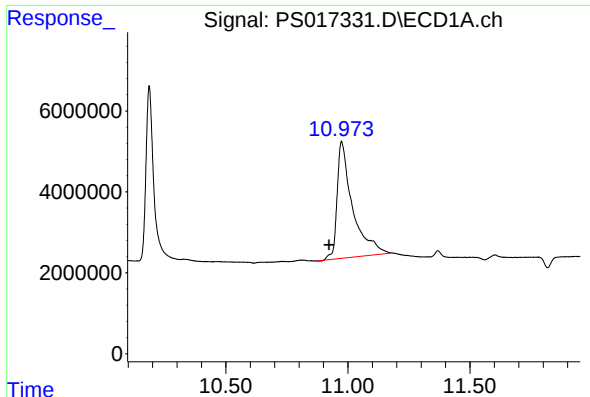

#15 Picloram

R.T.: 10.974 min
Delta R.T.: 0.052 min
Response: 127493239
Conc: 11.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

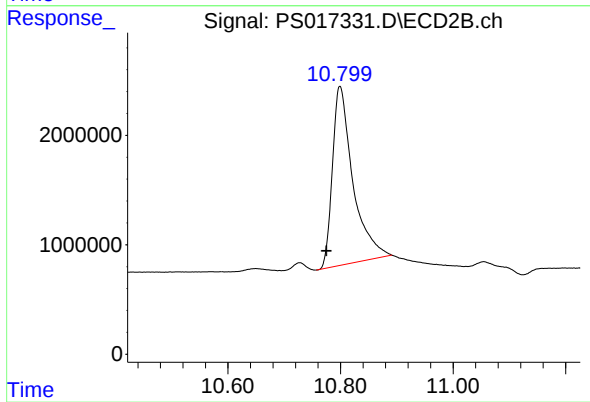

#15 Picloram

R.T.: 10.799 min
Delta R.T.: 0.024 min
Response: 41146388
Conc: 10.74 ng/ml