

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110424\
 Data File : PS028188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2024 22:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 03:57:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110424.M
 Quant Title : 8080.M
 QLast Update : Mon Nov 04 23:43:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.704f	7.902	4738075	813.5E6	1.875	485.674	#
Target Compounds								
1) T	Dalapon	2.997f	0.000	790253	0	<MDL	N.D.	#
5) T	DICAMBA	7.890f	0.000	3149132	0	<MDL	N.D.	#
6) T	MCPD	8.040	0.000	18220902	0	2.998	N.D.	#
7) T	MCPA	8.182	0.000	1629665	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.575	0.000	1917160	0	<MDL	N.D.	#
9) T	2,4-D	8.846f	0.000	69529229	0	26.853	N.D.	#
10) T	Pentachlo...	9.174f	0.000	476258	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.703	10.119f	12578990	4418246	<MDL	<MDL	#
12) T	2,4,5-T	10.013	0.000	1163702	0	<MDL	N.D.	#
13) T	2,4-DB	10.605	0.000	1139031	0	<MDL	N.D.	#
14) T	DINOSEB	11.794	0.000	6331494	0	<MDL	N.D.	#
15) T	Picloram	0.000	12.585	0	12881516	N.D.	<MDL	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110424\
Data File : PS028188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2024 22:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:57:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110424.M
Quant Title : 8080.M
QLast Update : Mon Nov 04 23:43:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

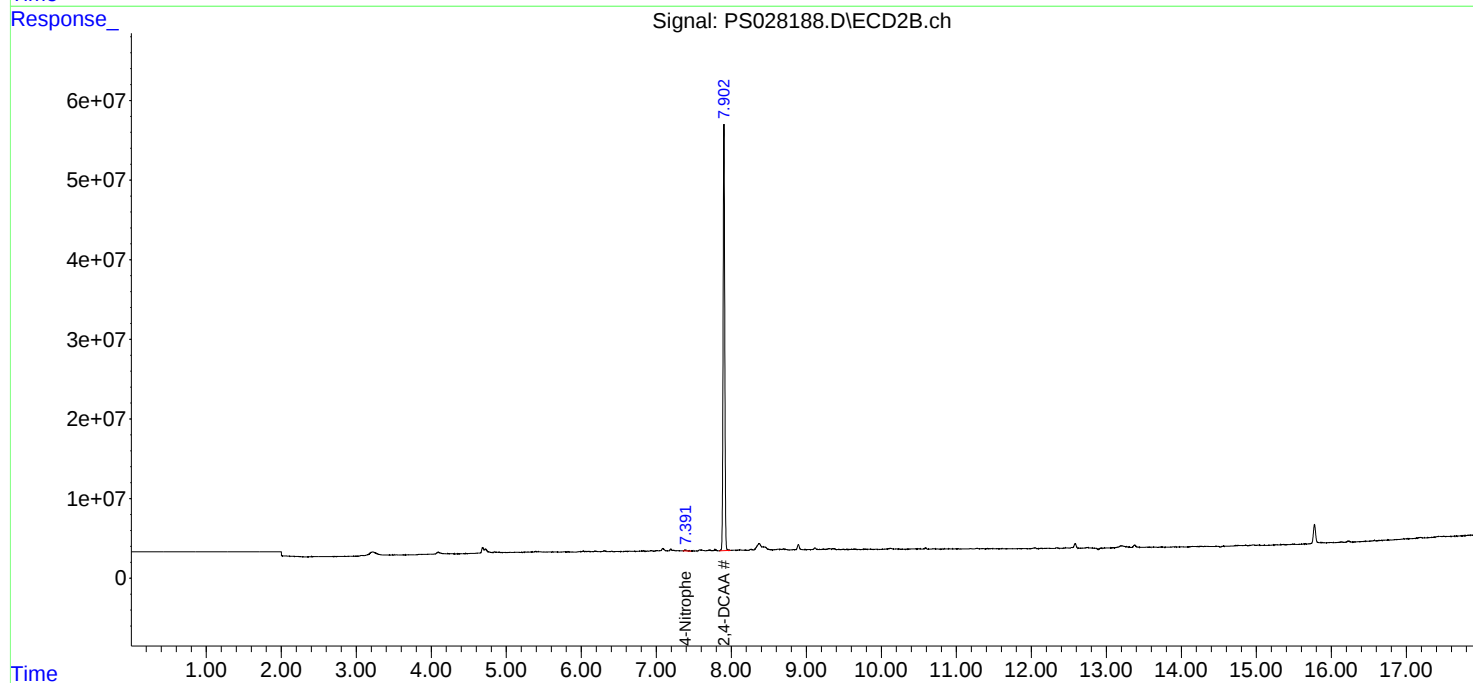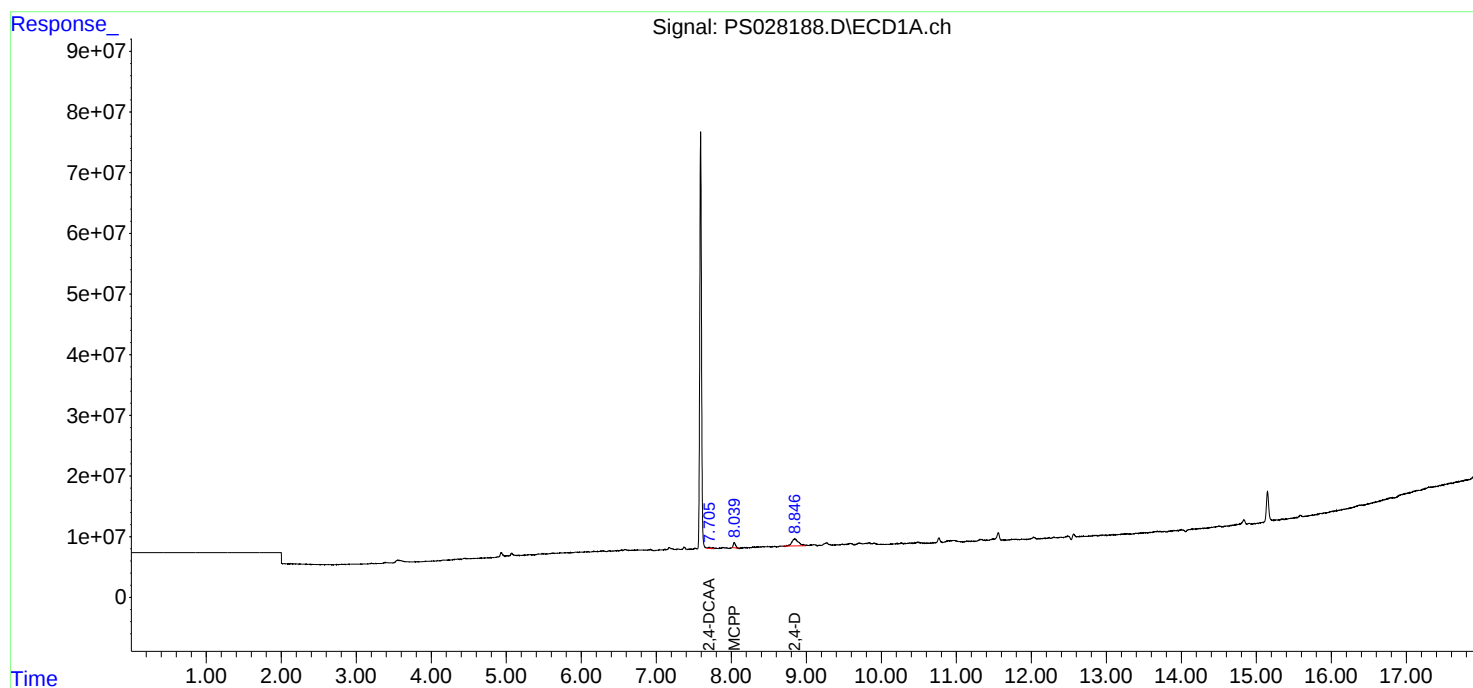


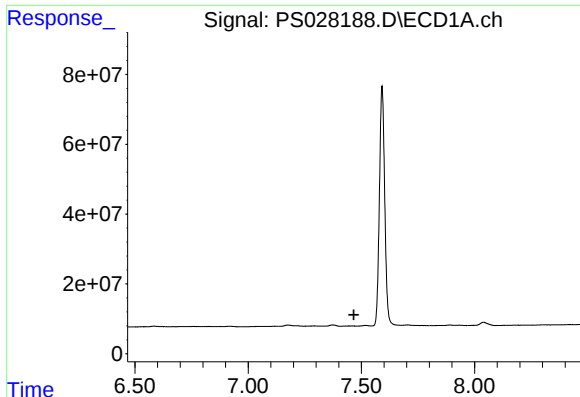

#3 4-Nitrophenol


R.T.: 7.461 min
Delta R.T.: -0.006 min
Response: -4008707
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

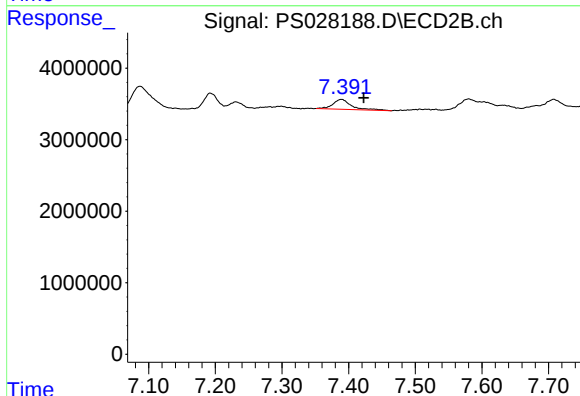


#3 4-Nitrophenol

R.T.: 7.389 min
Delta R.T.: -0.033 min
Response: 2687078
Conc: 2.30 ng/ml

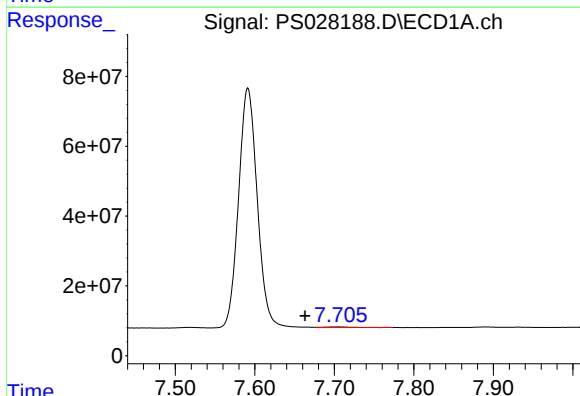


#4 2,4-DCAA

R.T.: 7.704 min
Delta R.T.: 0.041 min
Response: 4738075
Conc: 1.87 ng/ml

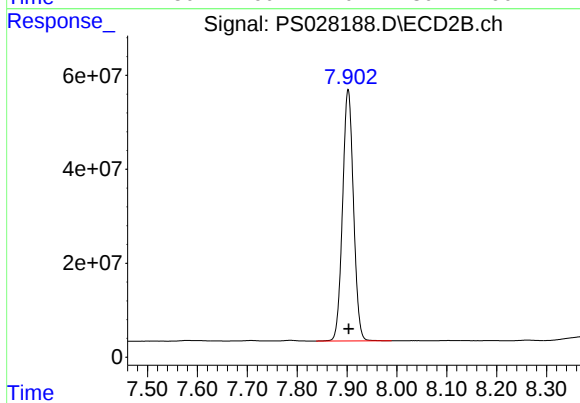

#4 2,4-DCAA


R.T.: 7.902 min
Delta R.T.: -0.001 min
Response: 813536939
Conc: 485.67 ng/ml

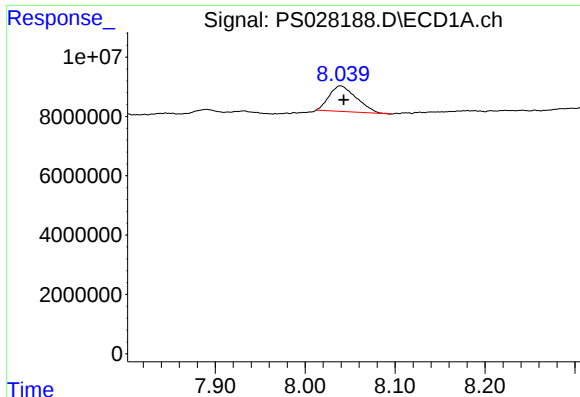

#6 MCPP


R.T.: 8.040 min
Delta R.T.: -0.003 min
Response: 18220902
Conc: 3.00 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

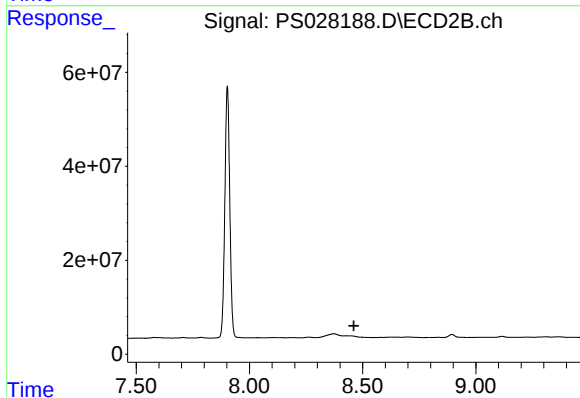


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.461 min
Response: 0
Conc: N.D.

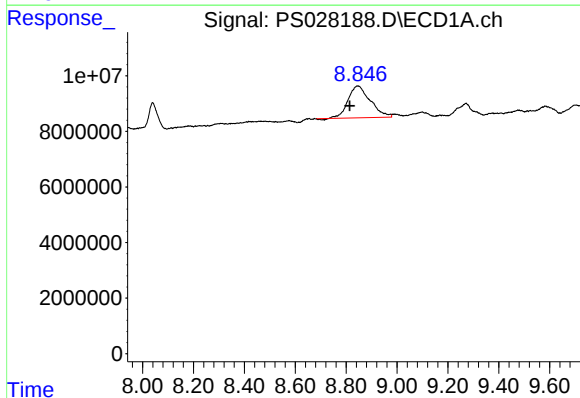

#9 2,4-D

R.T.: 8.846 min
Delta R.T.: 0.031 min
Response: 69529229
Conc: 26.85 ng/ml

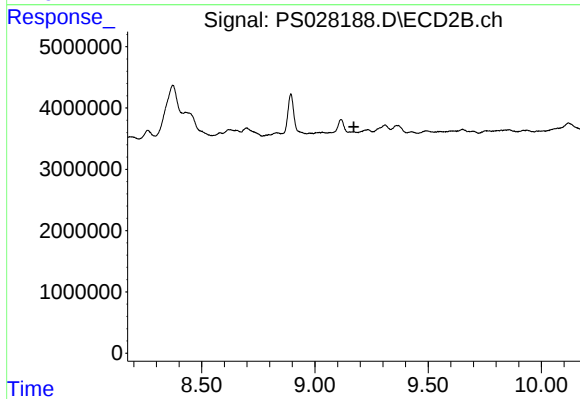

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.