

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110424\
 Data File : PS028189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2024 23:11
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 03:58:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110424.M
 Quant Title : 8080.M
 QLast Update : Mon Nov 04 23:43:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	7.903	0	1193.1E6	N.D.	712.297
Target Compounds							
1) T	Dalapon	0.000	2.783	0	1846.5E6	N.D.	656.740
2) T	3,5-DICHL...	0.000	6.835	0	1691.2E6	N.D.	665.946
3) T	4-Nitroph...	0.000	7.422	0	758.3E6	N.D.	649.560
5) T	DICAMBA	0.000	8.109	0	5191.2E6	N.D.	682.844
6) T	MCPD	8.047	8.461	21840462	475.4E6	3.594	68.392 #
7) T	MCPA	0.000	8.461	0	475.4E6	N.D.	67.664
8) T	DICHLORPROP	0.000	8.836	0	1255.0E6	N.D.	670.945
9) T	2,4-D	8.846f	9.171	59442503	1404.3E6	22.957	672.892 #
10) T	Pentachlo...	0.000	9.714	0	19209.5E6	N.D.	689.808
11) T	2,4,5-TP ...	9.718	10.090	45289865	7678.1E6	3.500	684.842 #
12) T	2,4,5-T	0.000	10.516	0	7601.5E6	N.D.	685.028
13) T	2,4-DB	0.000	11.088	0	925.7E6	N.D.	689.526
14) T	DINOSEB	0.000	11.474	0	5243.9E6	N.D.	669.166
15) T	Picloram	0.000	12.585	0	11033.4E6	N.D.	689.340
16) T	DCPA	0.000	12.530	0	8510.5E6	N.D.	690.636



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110424\
Data File : PS028189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2024 23:11
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:58:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110424.M
Quant Title : 8080.M
QLast Update : Mon Nov 04 23:43:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

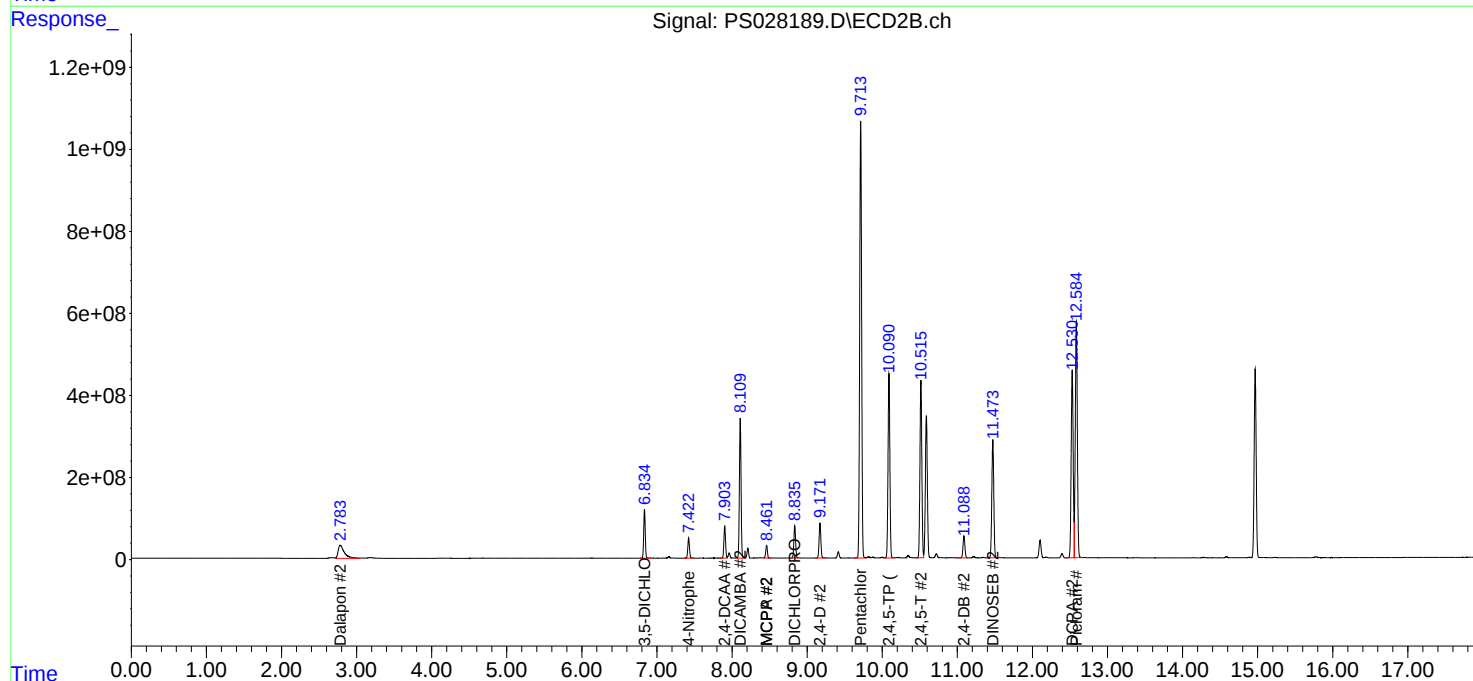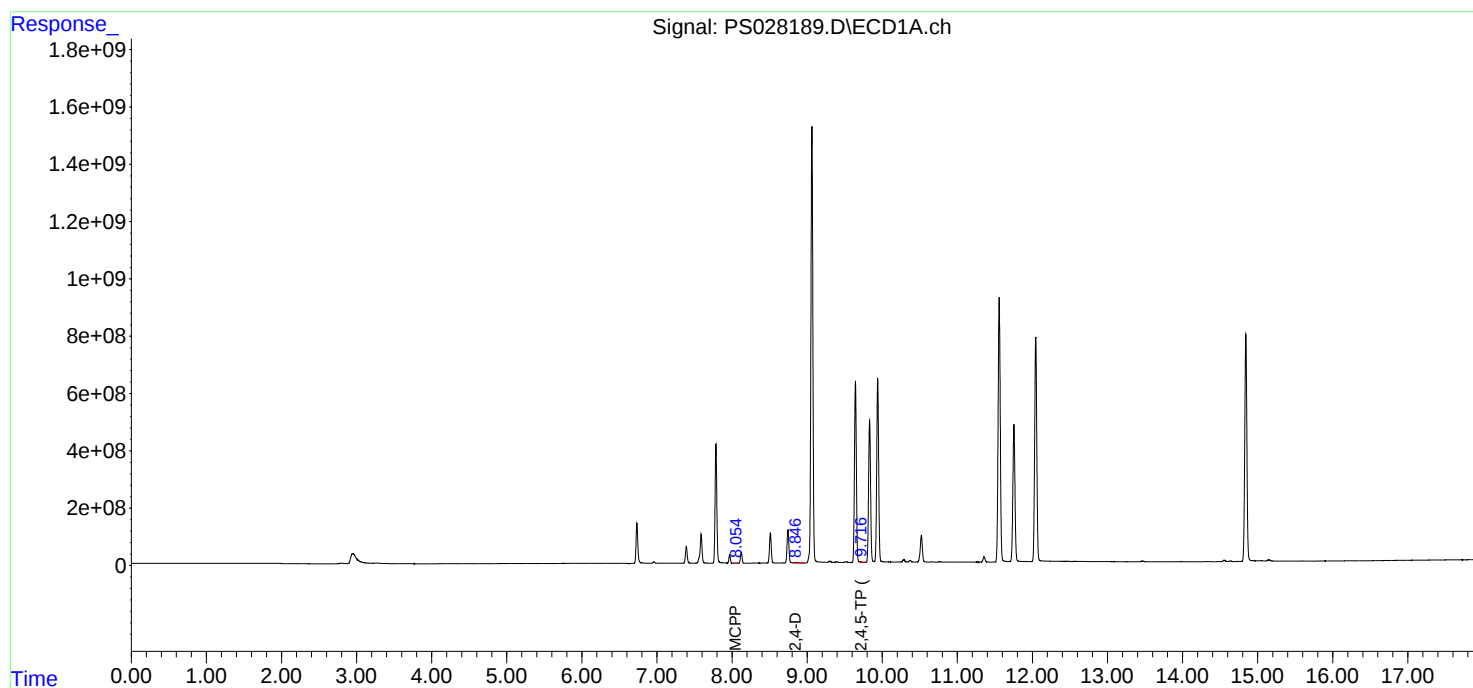


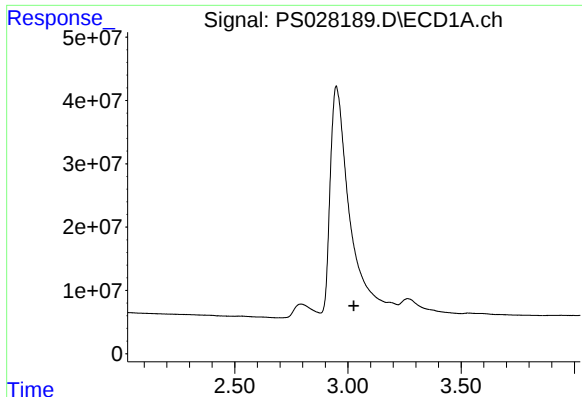

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

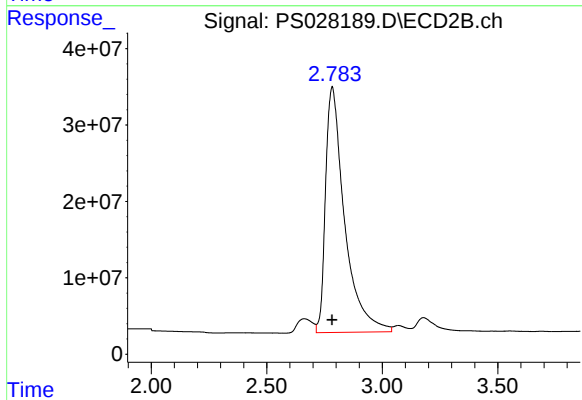


#1 Dalapon

R.T.: 2.783 min
Delta R.T.: 0.001 min
Response: 1846522659
Conc: 656.74 ng/ml

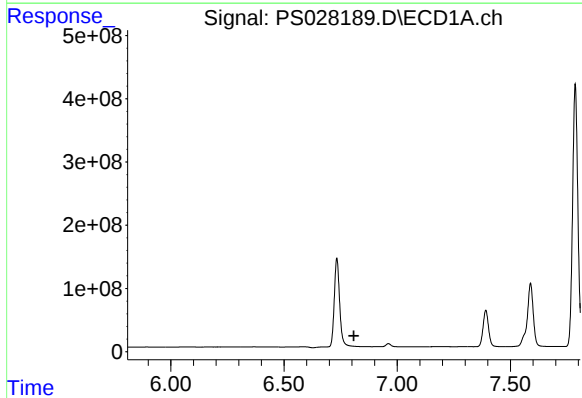


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.809 min
Response: 0
Conc: N.D.

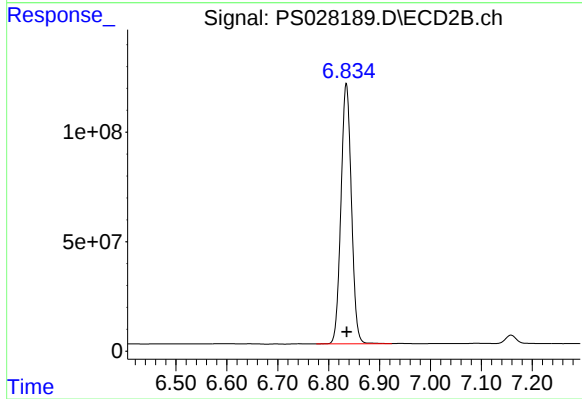

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.835 min
Delta R.T.: 0.000 min
Response: 1691195238
Conc: 665.95 ng/ml

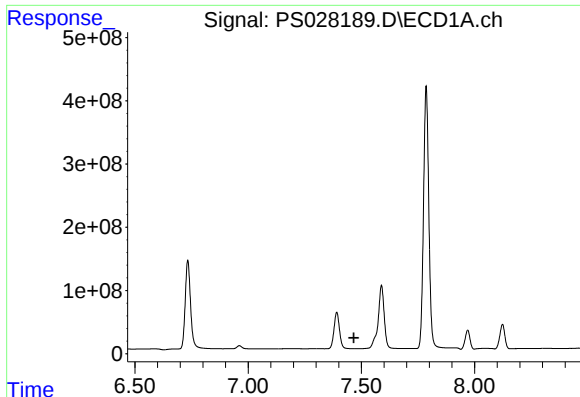

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

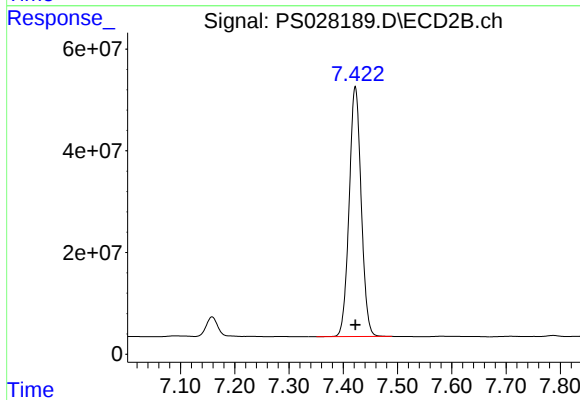


#3 4-Nitrophenol

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 758337949
Conc: 649.56 ng/ml

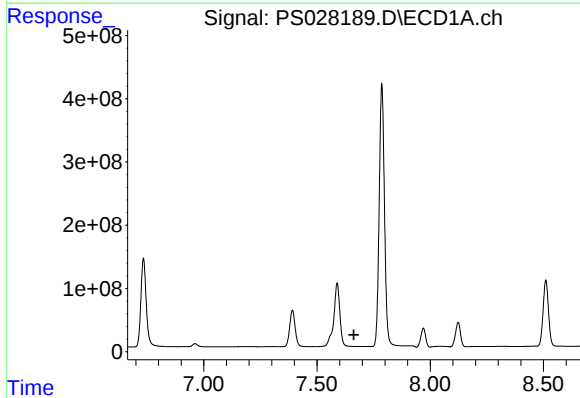


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.663 min
Response: 0
Conc: N.D.

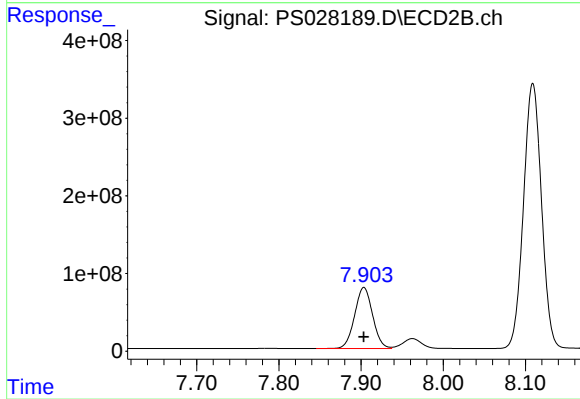

#4 2,4-DCAA


R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 1193146227
Conc: 712.30 ng/ml

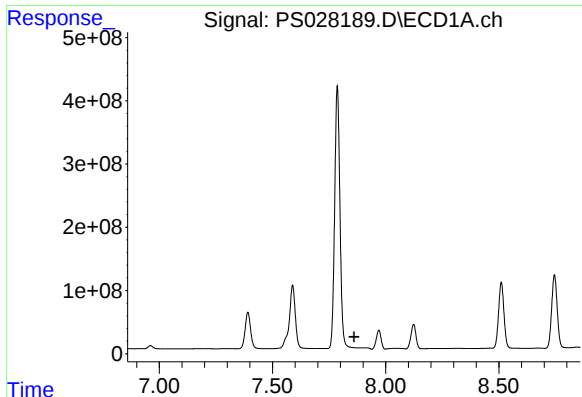

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

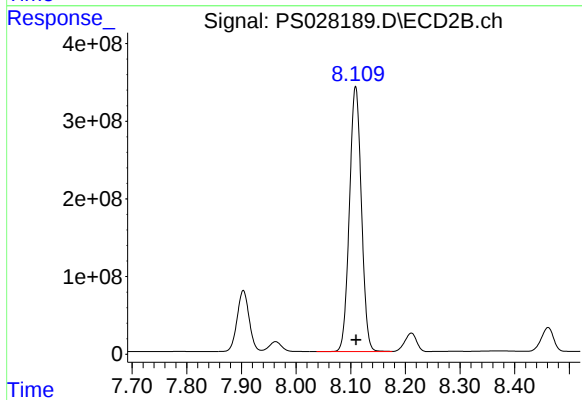


#5 DICAMBA

R.T.: 8.109 min
Delta R.T.: 0.000 min
Response: 5191165930
Conc: 682.84 ng/ml

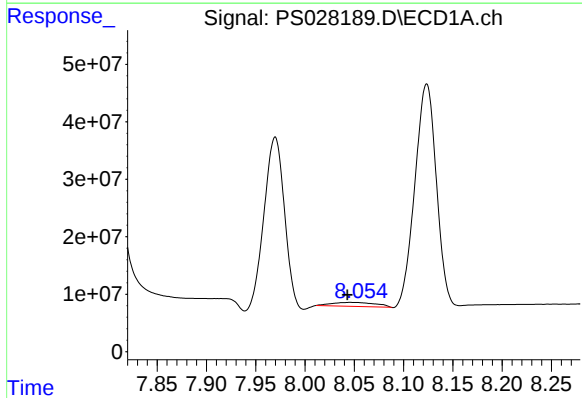


#6 MCP

R.T.: 8.047 min
Delta R.T.: 0.004 min
Response: 21840462
Conc: 3.59 ug/ml

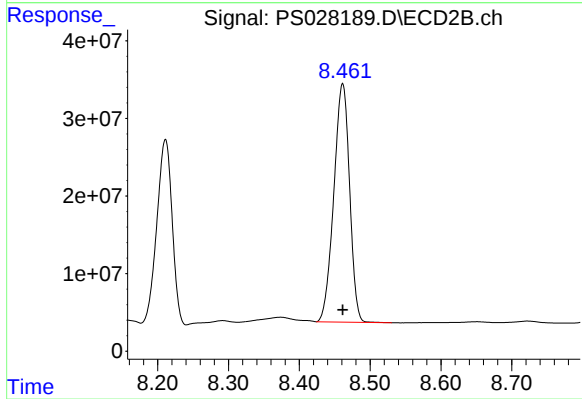

#6 MCP


R.T.: 8.461 min
Delta R.T.: 0.000 min
Response: 475424468
Conc: 68.39 ug/ml

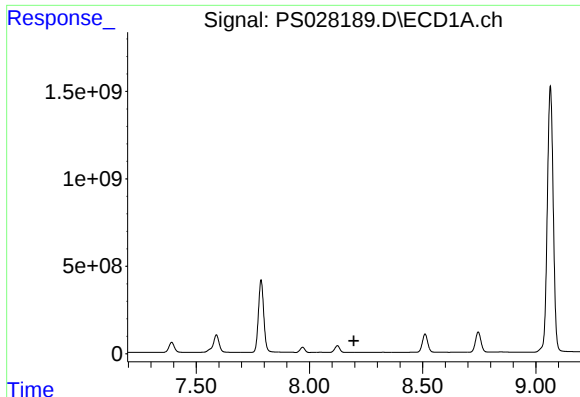

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 8.196 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

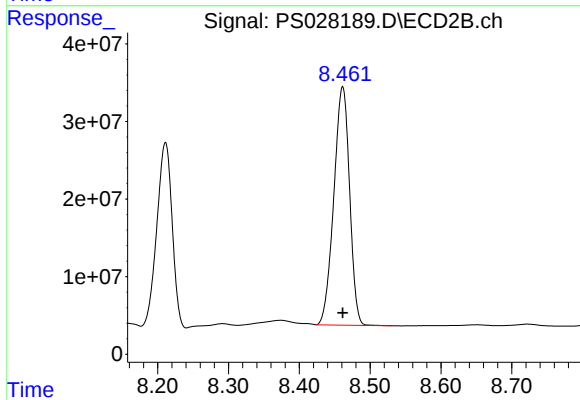


#7 MCPA

R.T.: 8.461 min
Delta R.T.: 0.000 min
Response: 475424468
Conc: 67.66 ug/ml

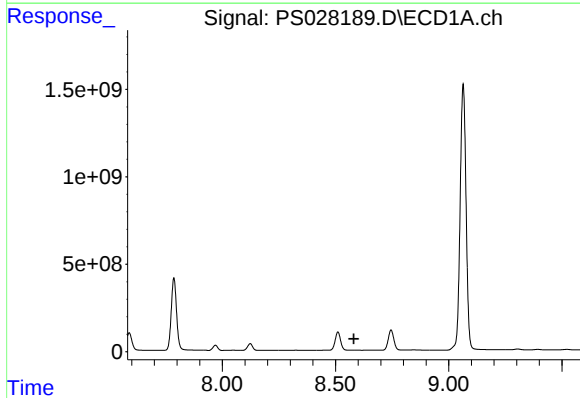


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.581 min
Response: 0
Conc: N.D.

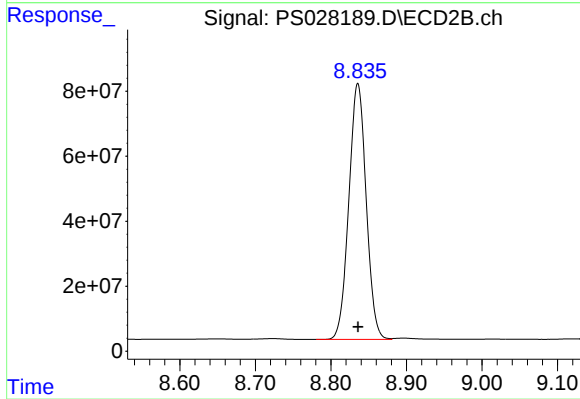

#8 DICHLORPROP


R.T.: 8.836 min
Delta R.T.: 0.000 min
Response: 1254955582
Conc: 670.94 ng/ml

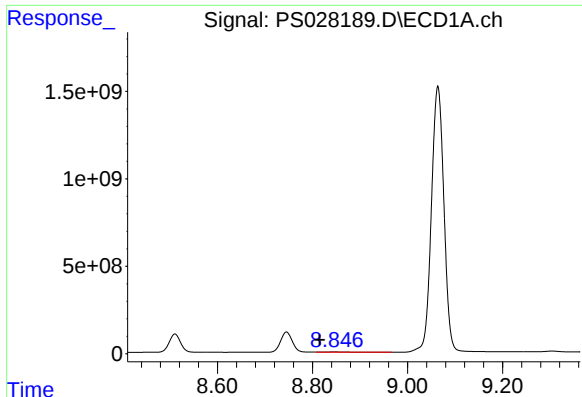

#9 2,4-D


R.T.: 8.846 min
Delta R.T.: 0.031 min
Response: 59442503
Conc: 22.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

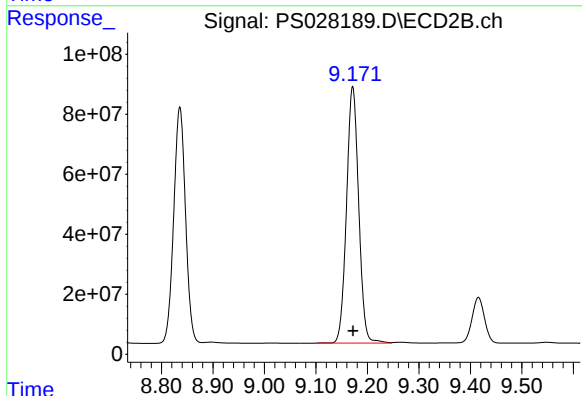


#9 2,4-D

R.T.: 9.171 min
Delta R.T.: 0.000 min
Response: 1404341415
Conc: 672.89 ng/ml

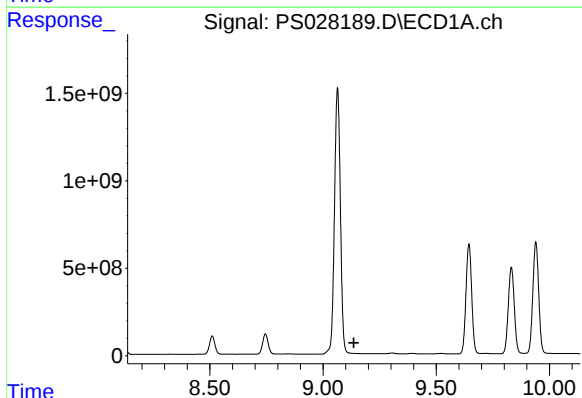


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 9.136 min
Response: 0
Conc: N.D.

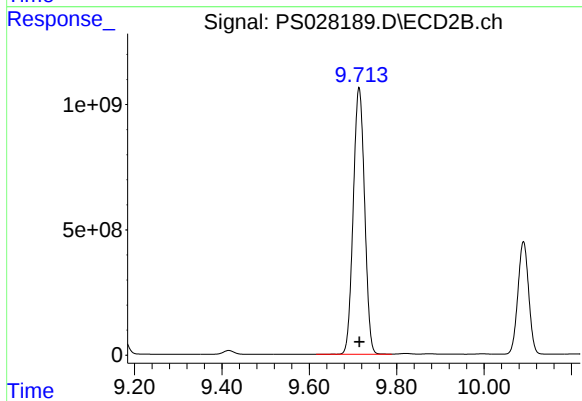

#10 Pentachlorophenol


R.T.: 9.714 min
Delta R.T.: 0.000 min
Response: 19209476705
Conc: 689.81 ng/ml

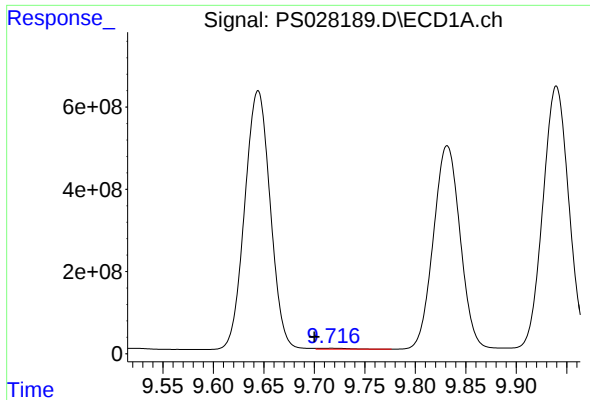

#11 2,4,5-TP (SILVEX)


R.T.: 9.718 min
Delta R.T.: 0.018 min
Response: 45289865
Conc: 3.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

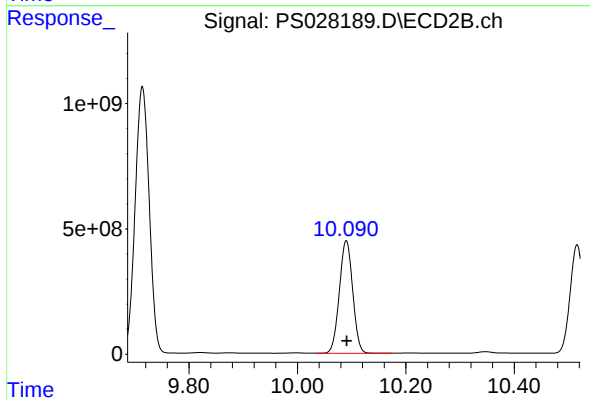


#11 2,4,5-TP (SILVEX)

R.T.: 10.090 min
Delta R.T.: 0.000 min
Response: 7678063380
Conc: 684.84 ng/ml

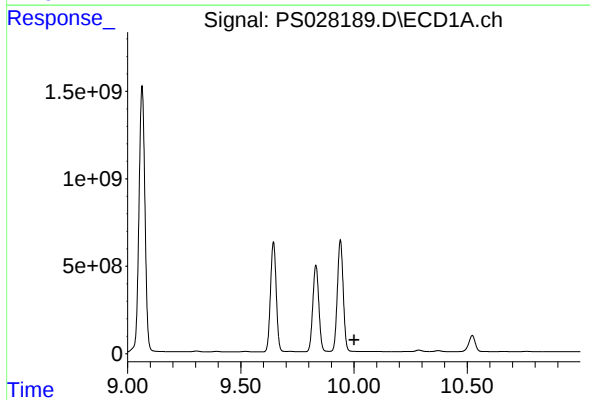


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 10.000 min
Response: 0
Conc: N.D.

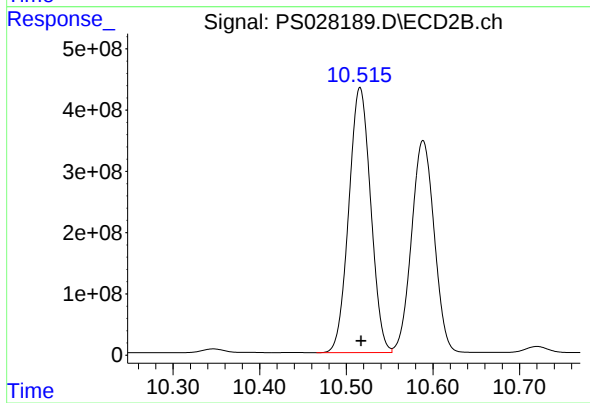

#12 2,4,5-T


R.T.: 10.516 min
Delta R.T.: -0.001 min
Response: 7601470773
Conc: 685.03 ng/ml

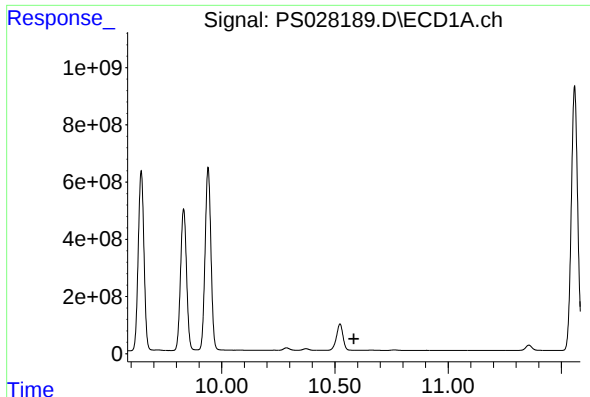

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.584 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

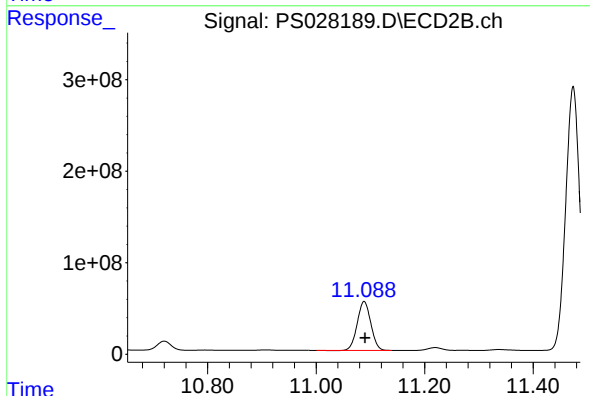


#13 2,4-DB

R.T.: 11.088 min
Delta R.T.: -0.001 min
Response: 925683390
Conc: 689.53 ng/ml

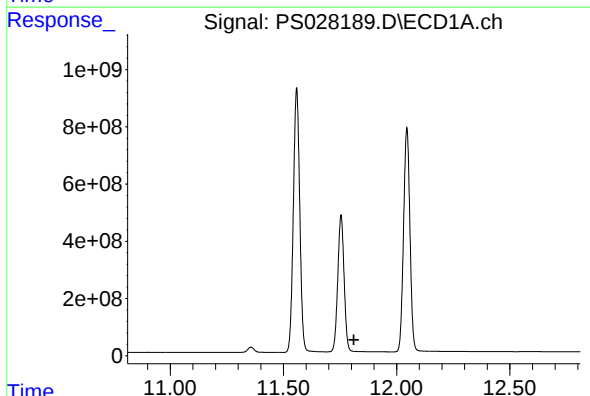


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.811 min
Response: 0
Conc: N.D.

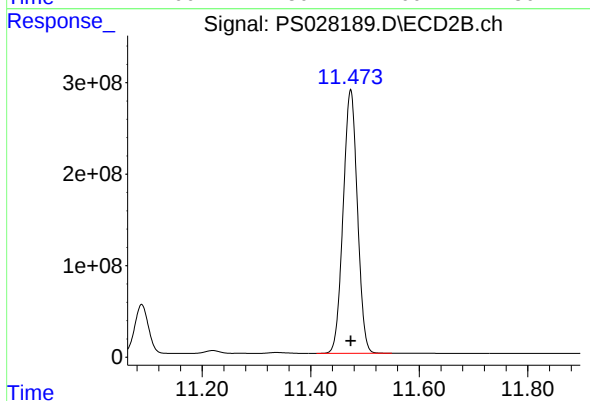

#14 DINOSEB


R.T.: 11.474 min
Delta R.T.: 0.000 min
Response: 5243926097
Conc: 669.17 ng/ml

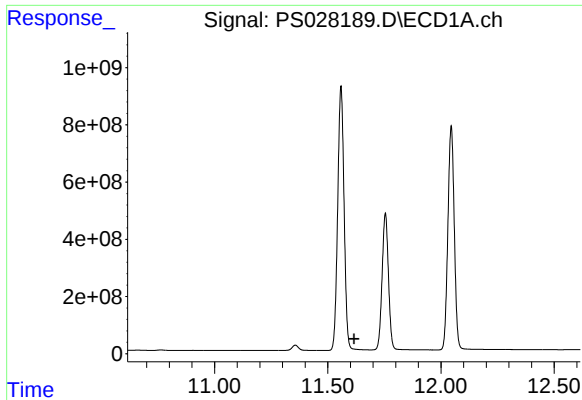

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.616 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

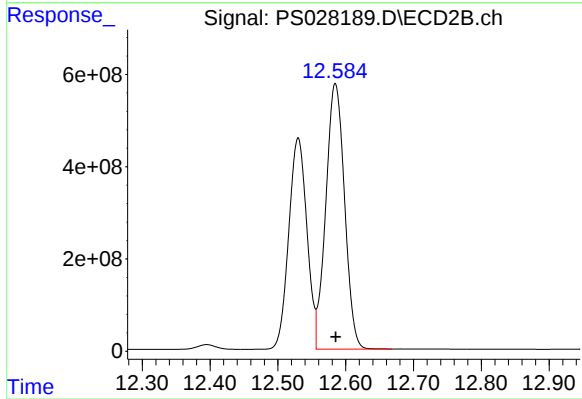


#15 Picloram

R.T.: 12.585 min
Delta R.T.: 0.000 min
Response: 11033444259
Conc: 689.34 ng/ml

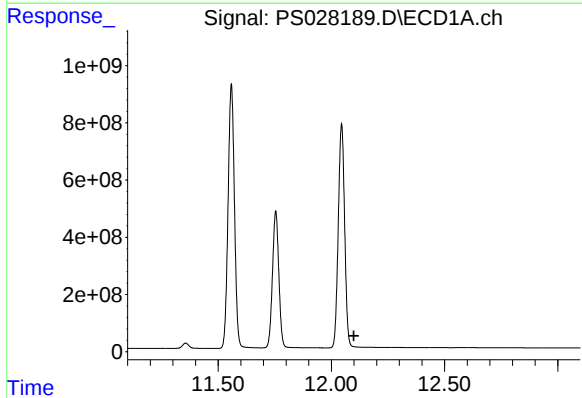

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 12.100 min
Response: 0
Conc: N.D.

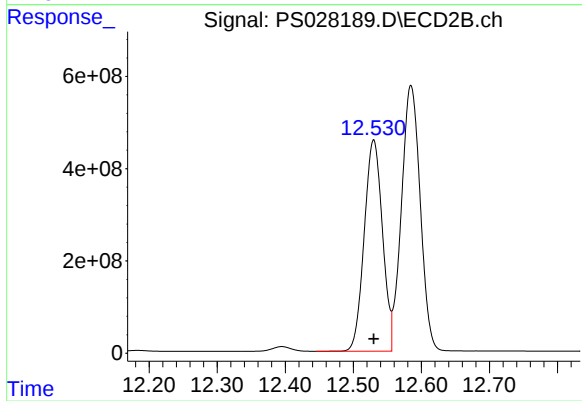

#16 DCPA

R.T.: 12.530 min
Delta R.T.: 0.000 min
Response: 8510465446
Conc: 690.64 ng/ml