

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110424\
 Data File : PS028201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 03:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 07:04:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110424.M
 Quant Title : 8080.M
 QLast Update : Mon Nov 04 23:43:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.669	7.906	-13536856	773.0E6	N.D.	461.455
Target Compounds							
1) T	Dalapon	2.986f	0.000	163879	0	<MDL	N.D. #
3) T	4-Nitroph...	7.486	0.000	2240993	0	1.671	N.D. #
5) T	DICAMBA	7.859	0.000	1377611	0	<MDL	N.D. #
6) T	MCP	0.000	8.434f	0	7446313	N.D.	1.071
7) T	MCPA	0.000	8.434f	0	7446313	N.D.	1.060
8) T	DICHLORPROP	8.570	0.000	8686245	0	3.698	N.D. #
9) T	2,4-D	8.813	0.000	88276786	0	34.093	N.D. #
10) T	Pentachlo...	0.000	9.764f	0	13403313	N.D.	<MDL
11) T	2,4,5-TP ...	9.664f	10.117f	6221459	6955837	<MDL	<MDL #
12) T	2,4,5-T	10.044f	0.000	40982771	0	3.206	N.D. #
14) T	DINOSEB	11.839f	0.000	1139.1E6	0	130.911	N.D. #
15) T	Picloram	11.590f	12.548f	-1025237	4915023	N.D.	<MDL
16) T	DCPA	12.142f	12.548	1342520	4915023	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110424\
Data File : PS028201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 03:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 07:04:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110424.M
Quant Title : 8080.M
QLast Update : Mon Nov 04 23:43:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

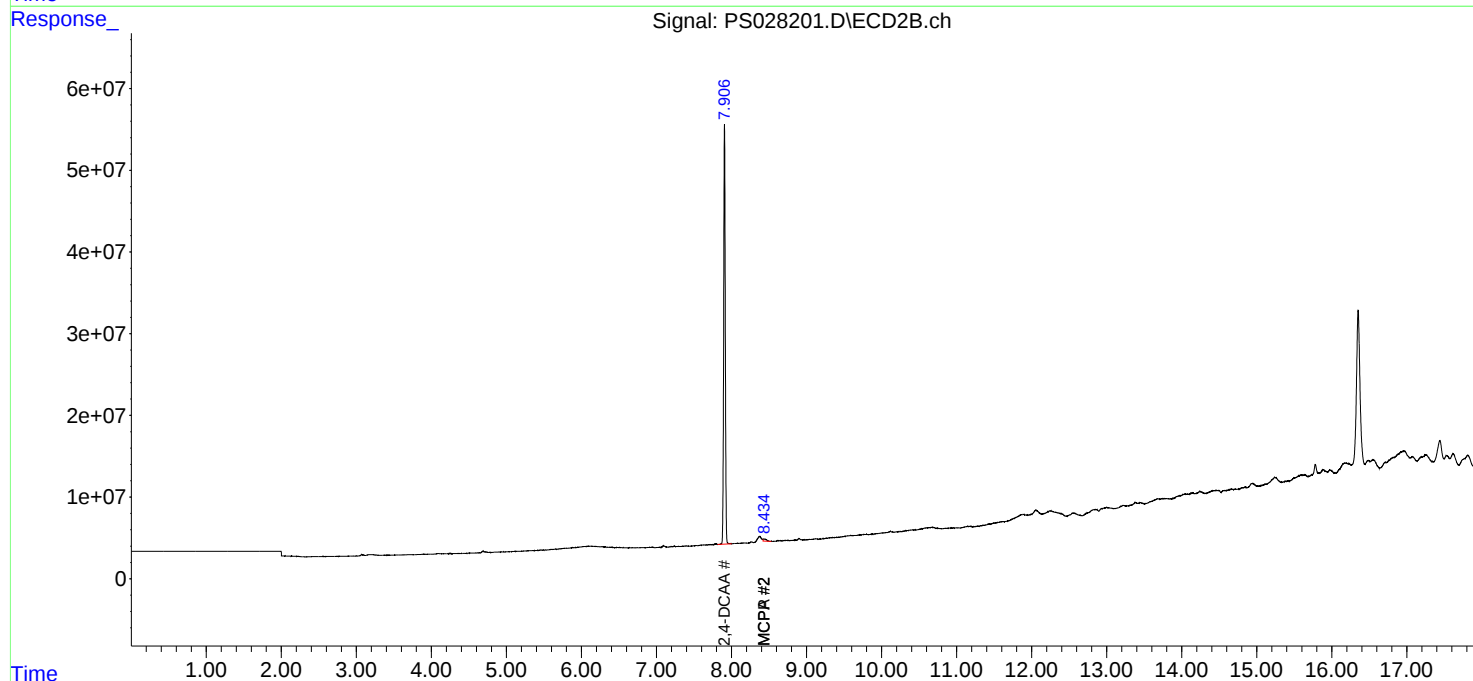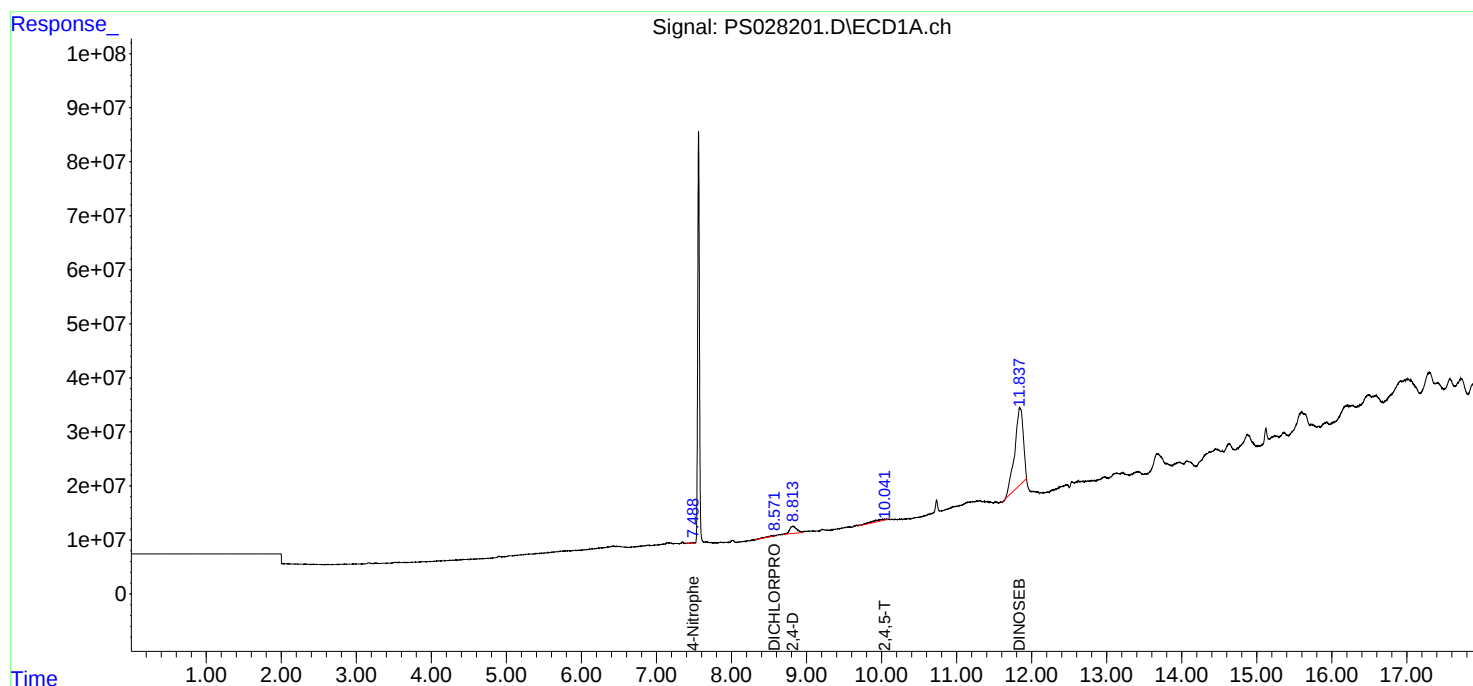


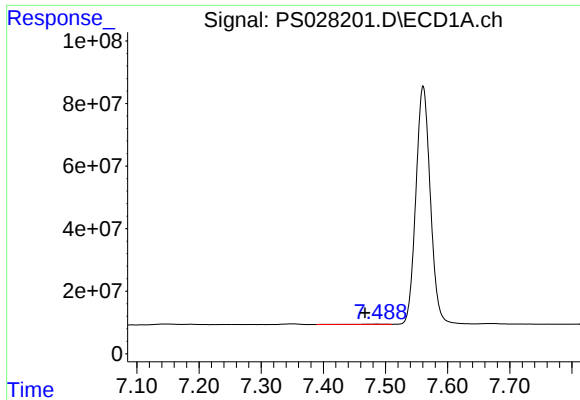

#3 4-Nitrophenol


R.T.: 7.486 min
Delta R.T.: 0.019 min
Response: 2240993
Conc: 1.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

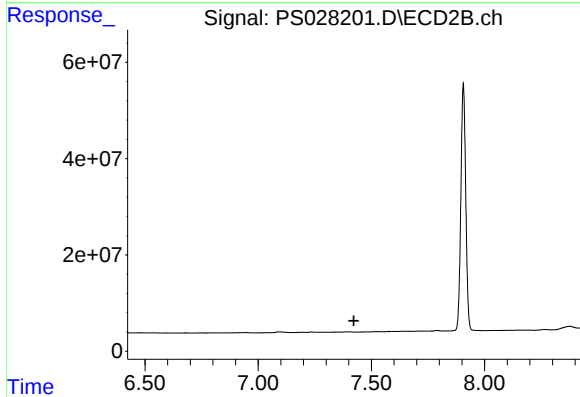


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

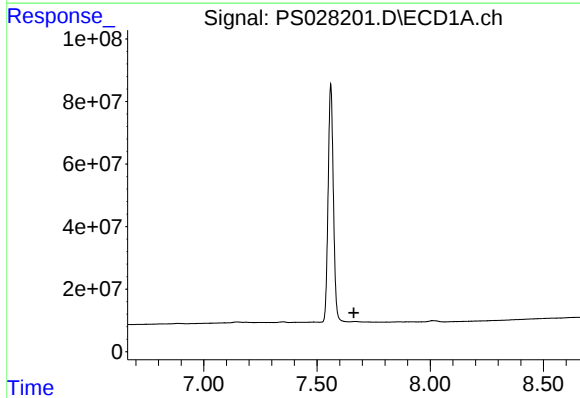


#4 2,4-DCAA

R.T.: 7.669 min
Delta R.T.: 0.006 min
Response: -13536856
Conc: N.D.

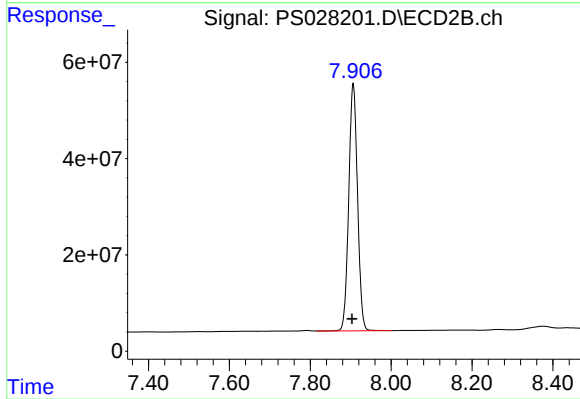

#4 2,4-DCAA


R.T.: 7.906 min
Delta R.T.: 0.003 min
Response: 772968288
Conc: 461.45 ng/ml

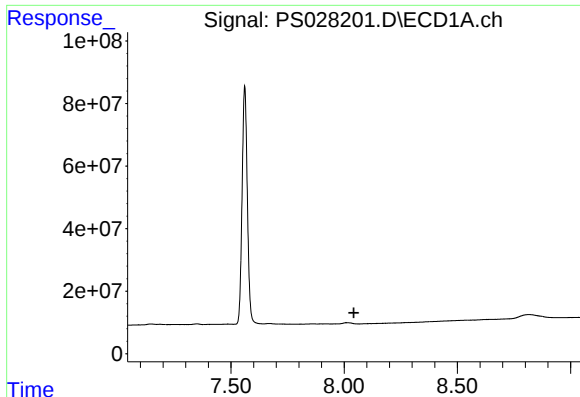

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 8.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

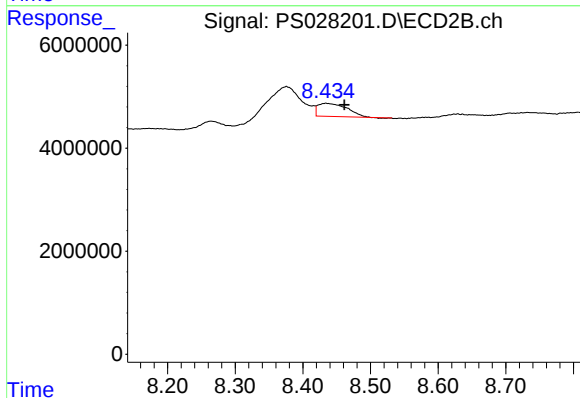


#6 MCPP

R.T.: 8.434 min
Delta R.T.: -0.027 min
Response: 7446313
Conc: 1.07 ug/ml

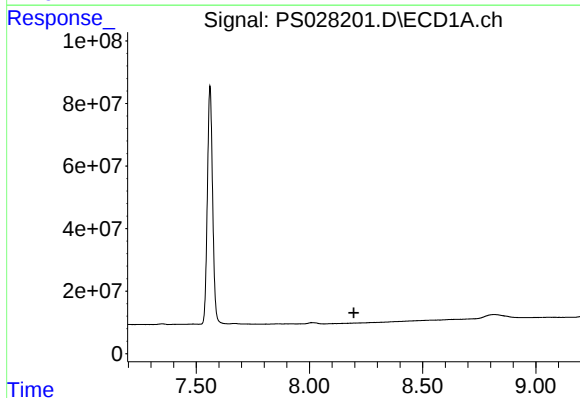


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 8.196 min
Response: 0
Conc: N.D.

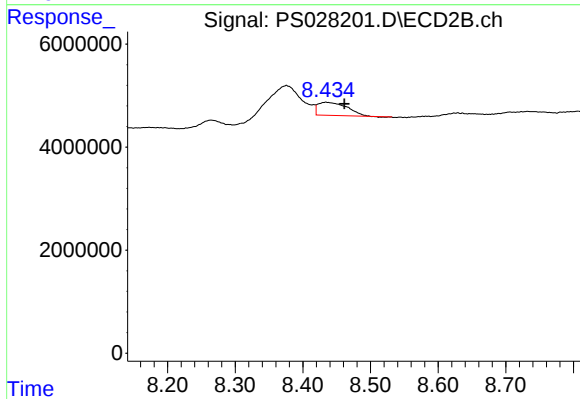

#7 MCPA


R.T.: 8.434 min
Delta R.T.: -0.027 min
Response: 7446313
Conc: 1.06 ug/ml

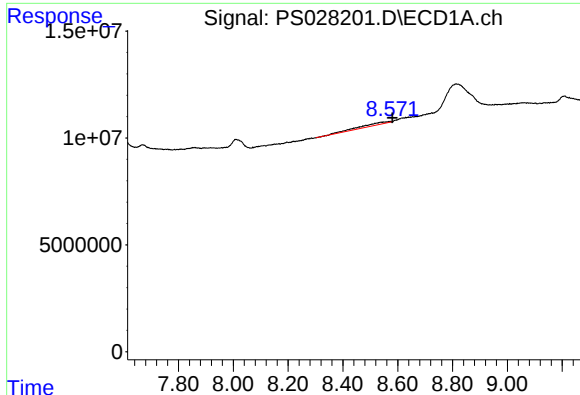

#8 DICHLORPROP


R.T.: 8.570 min
Delta R.T.: -0.011 min
Response: 8686245
Conc: 3.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

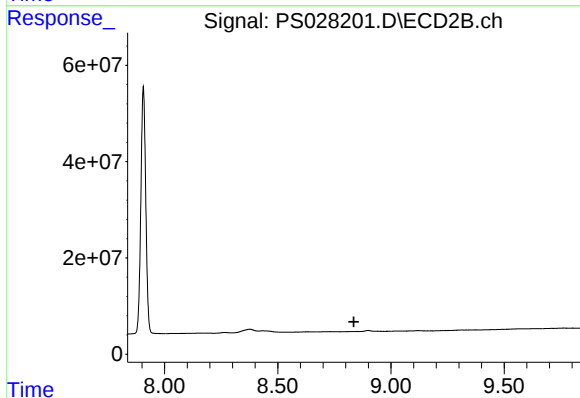


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.836 min
Response: 0
Conc: N.D.

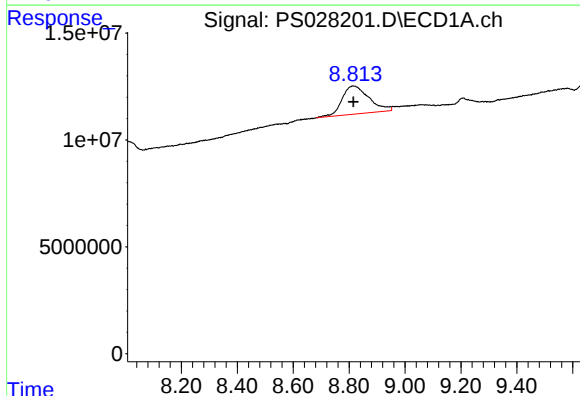


#9 2,4-D

R.T.: 8.813 min
Delta R.T.: -0.002 min
Response: 88276786
Conc: 34.09 ng/ml

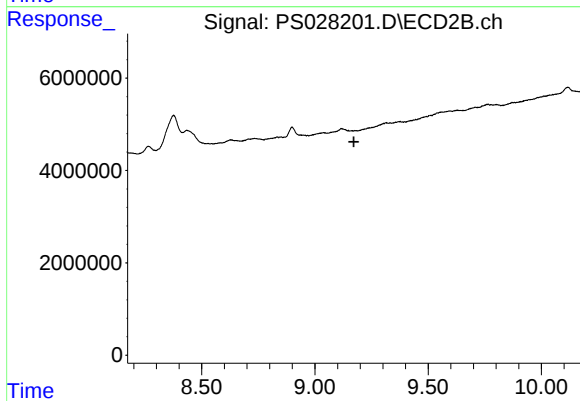

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

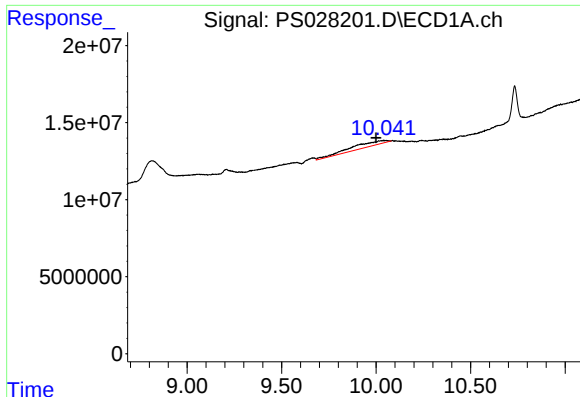

#12 2,4,5-T


R.T.: 10.044 min
Delta R.T.: 0.044 min
Response: 40982771
Conc: 3.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

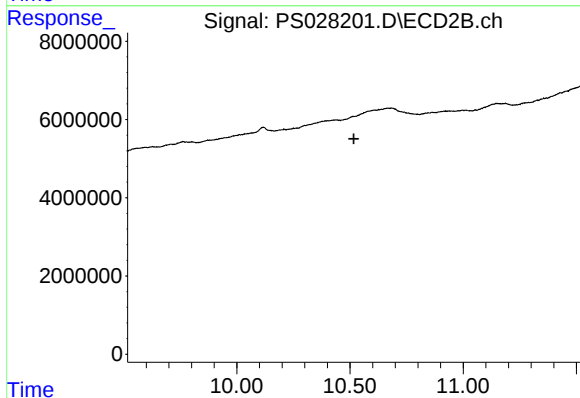


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 10.517 min
Response: 0
Conc: N.D.

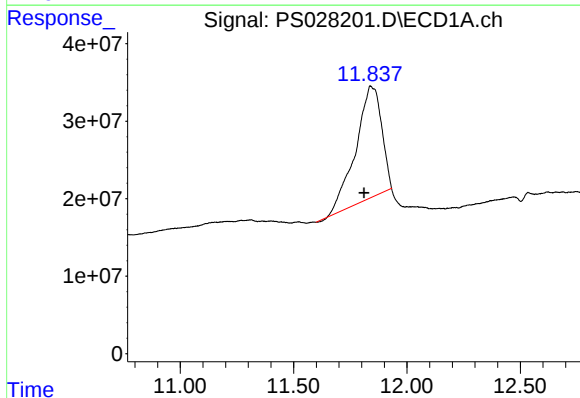

#14 DINOSEB

R.T.: 11.839 min
Delta R.T.: 0.028 min
Response: 1139140490
Conc: 130.91 ng/ml

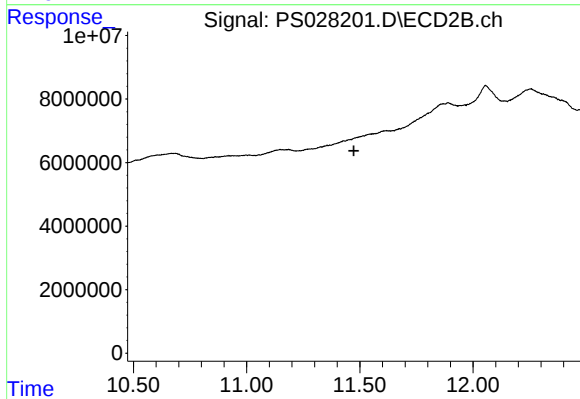

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.474 min
Response: 0
Conc: N.D.