

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
 Data File : PS002306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2018 18:26
 Operator : EI\SJ
 Sample : PB114497BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:00:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.413	10.903	163.0E6	183.3E6	517.889	510.580
Target Compounds							
1) T	Dalapon	2.937	2.375	212.0E6	185.2E6	462.305	410.232
2) T	3,5-DICHL...	0.000	9.059	0	201.9E6	N.D.	455.203 #
3) T	4-Nitroph...	11.005	10.051	86715711	115.7E6	519.788	648.880
5) T	DICAMBA	11.722	11.187	646.5E6	329.4E6	486.837	263.582 #
6) T	MCPD	12.096	11.416	-2353984	41625834	N.D.	48.383
7) T	MCPA	12.374	11.790	-41508335	87930221	N.D.	64.970
8) T	DICHLORPROP	12.908	12.310	169.3E6	-119339160	486.157	N.D. #
9) T	2,4-D	0.000	12.781	0	85079475	N.D.	199.767 #
10) T	Pentachlo...	13.645	13.327	2524.4E6	1866.6E6	524.755	397.373
11) T	2,4,5-TP ...	0.000	13.945	0	1040.1E6	N.D.	568.488 #
12) T	2,4,5-T	14.909	14.509	831.6E6	595.4E6	463.993	397.626
13) T	2,4-DB	0.000	15.159	0	59716112	N.D.	269.528 #
14) T	DINOSEB	17.134	15.587	660.9E6	675.0E6	482.427	533.241
15) T	Picloram	16.902	16.764	1036.0E6	712.6E6	434.326	314.985 #
16) T	DCPA	0.000	16.817	0	1004.5E6	N.D.	424.222 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
Data File : PS002306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2018 18:26
Operator : EI\SJ
Sample : PB114497BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:00:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

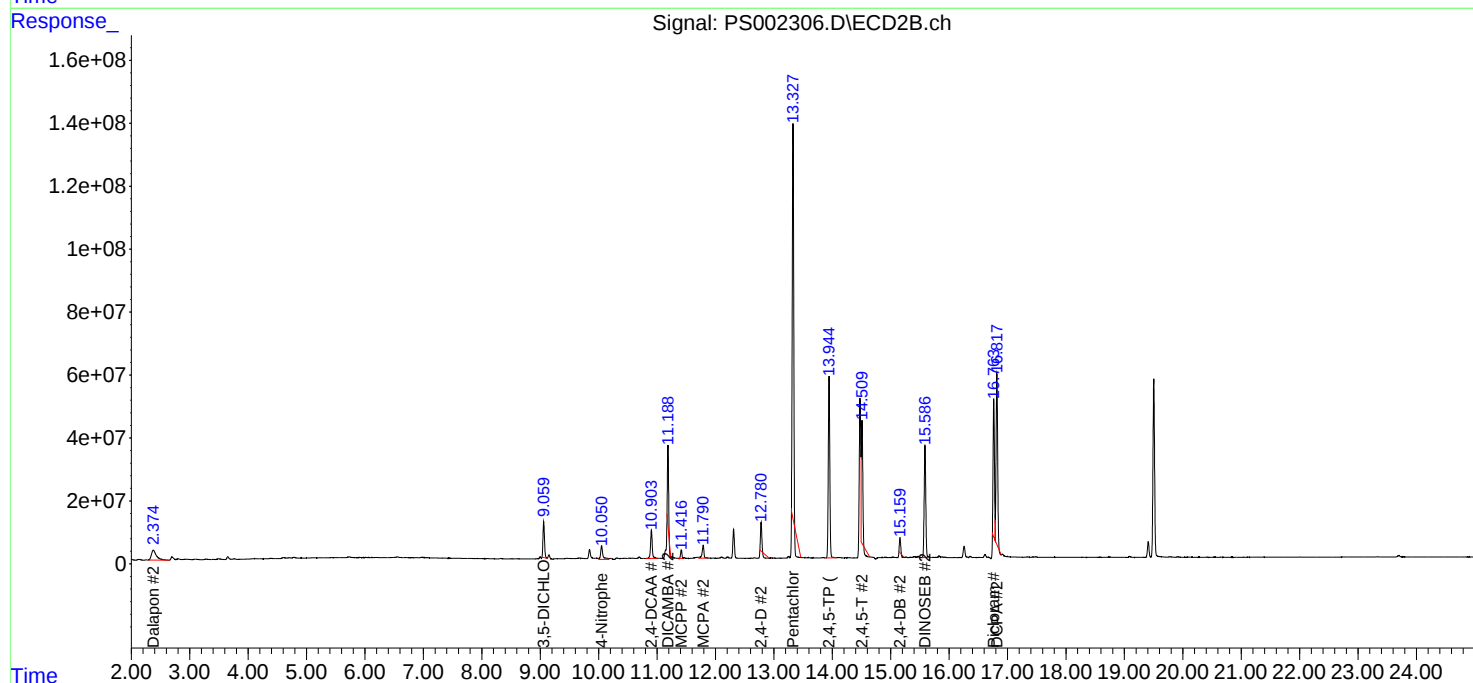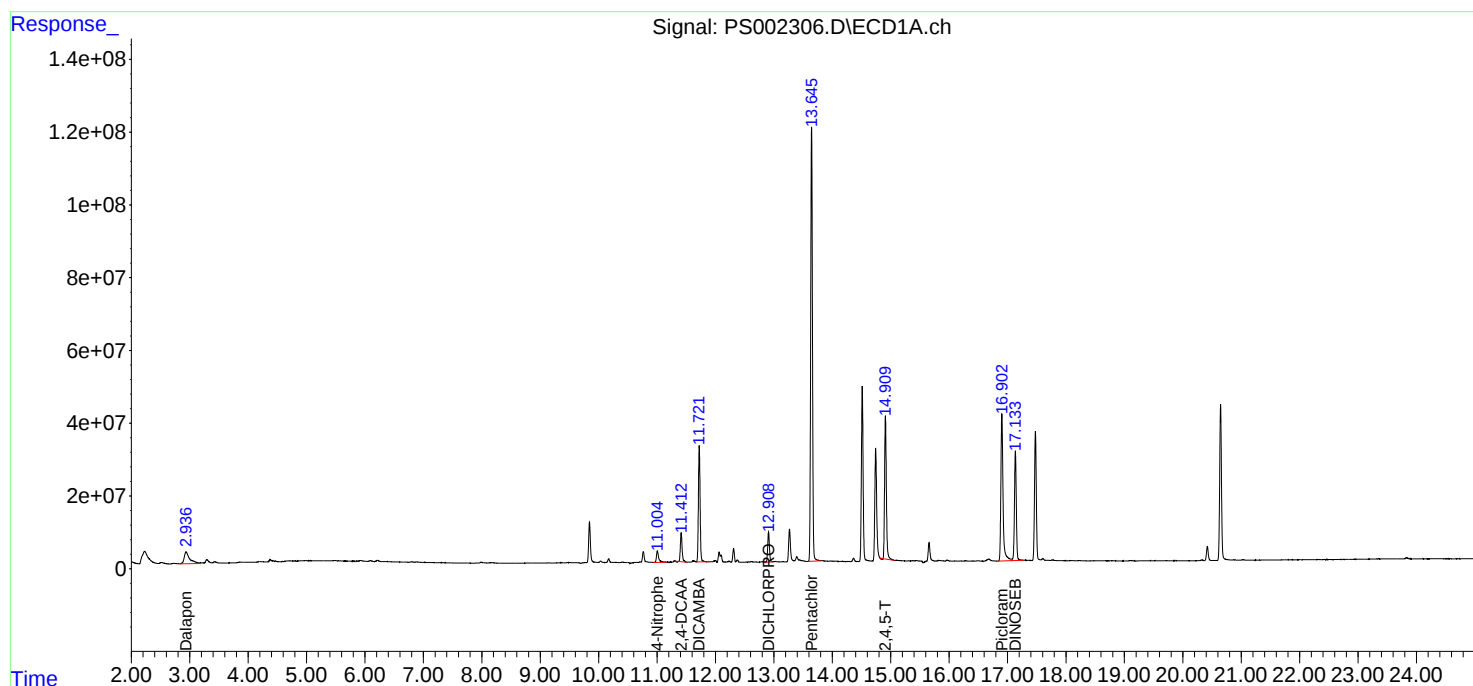


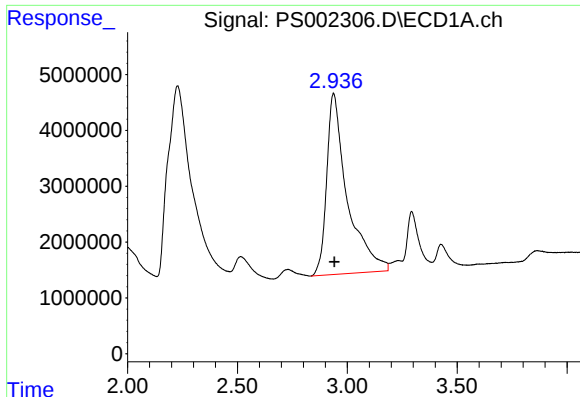

#1 Dalapon


R.T.: 2.937 min
Delta R.T.: -0.005 min
Response: 212044040
Conc: 462.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

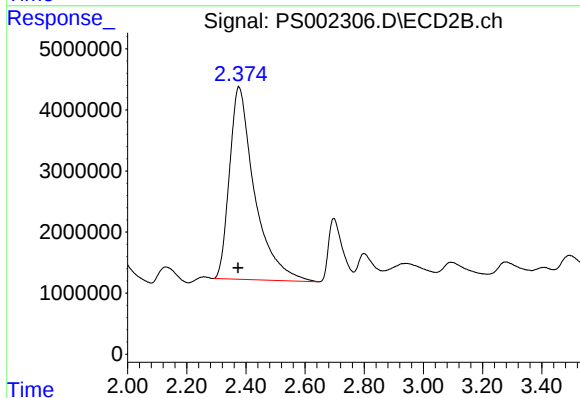


#1 Dalapon

R.T.: 2.375 min
Delta R.T.: 0.002 min
Response: 185222706
Conc: 410.23 ng/ml

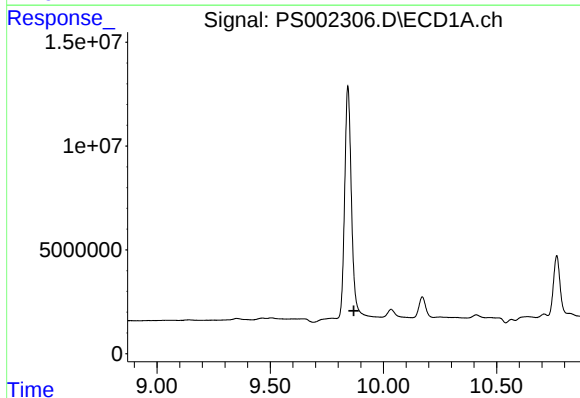


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

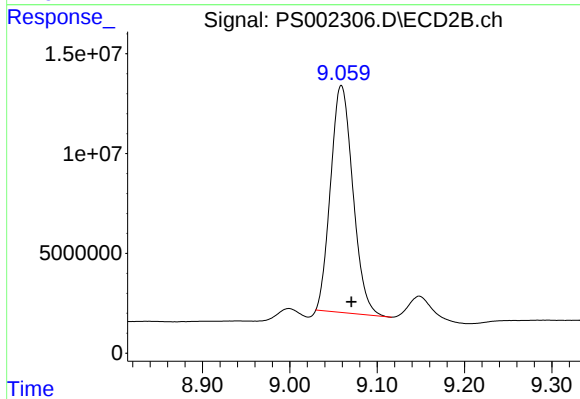

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.059 min
Delta R.T.: -0.011 min
Response: 201907593
Conc: 455.20 ng/ml

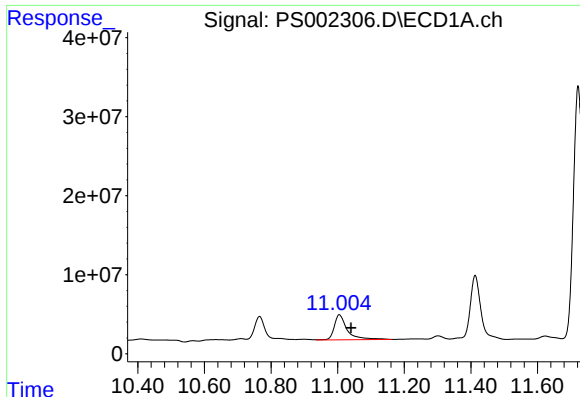

#3 4-Nitrophenol


R.T.: 11.005 min
Delta R.T.: -0.035 min
Response: 86715711
Conc: 519.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

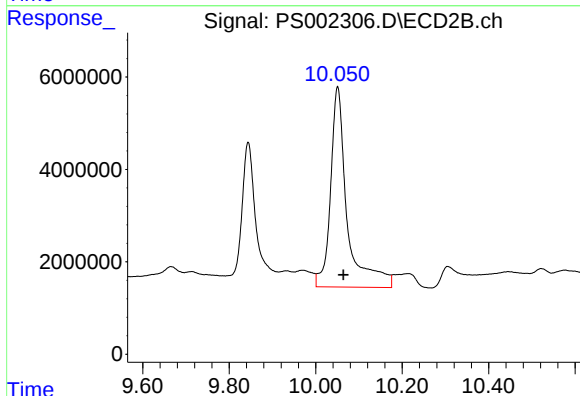


#3 4-Nitrophenol

R.T.: 10.051 min
Delta R.T.: -0.013 min
Response: 115702118
Conc: 648.88 ng/ml

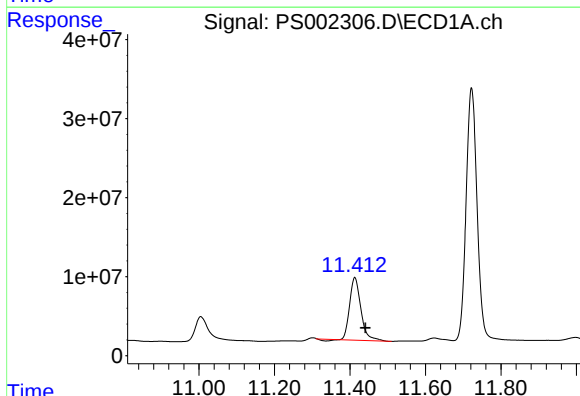


#4 2,4-DCAA

R.T.: 11.413 min
Delta R.T.: -0.028 min
Response: 162972116
Conc: 517.89 ng/ml

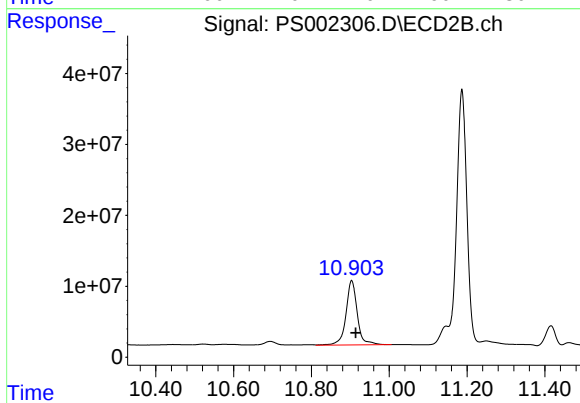

#4 2,4-DCAA


R.T.: 10.903 min
Delta R.T.: -0.011 min
Response: 183348232
Conc: 510.58 ng/ml

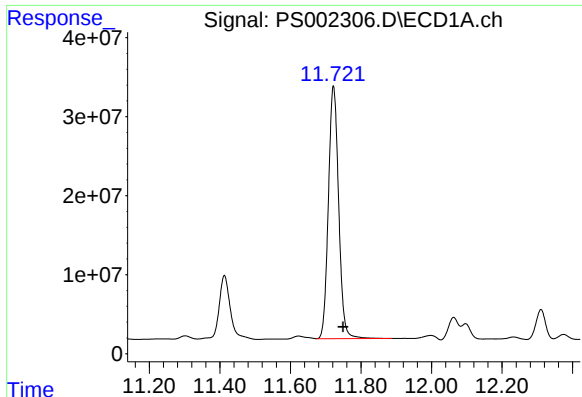

#5 DICAMBA


R.T.: 11.722 min
Delta R.T.: -0.027 min
Response: 646528403
Conc: 486.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

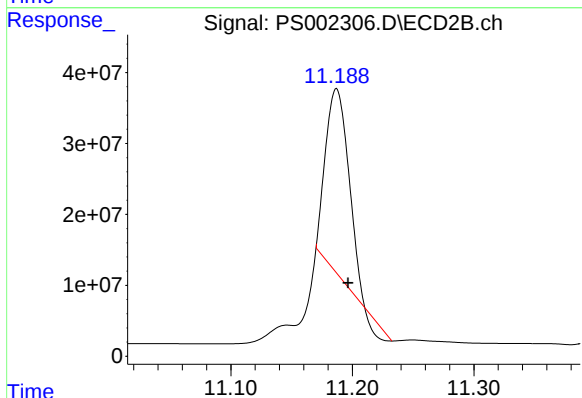


#5 DICAMBA

R.T.: 11.187 min
Delta R.T.: -0.010 min
Response: 329397787
Conc: 263.58 ng/ml

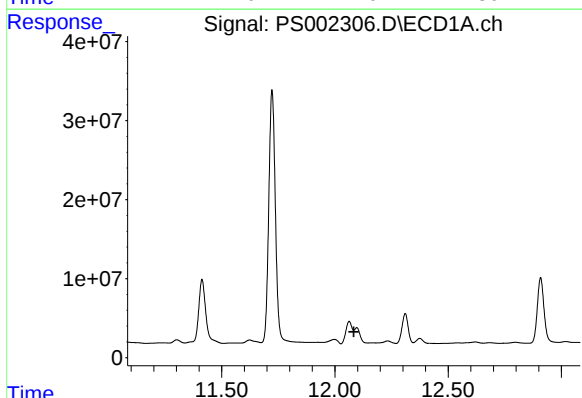


#6 MCPP

R.T.: 12.096 min
Delta R.T.: 0.013 min
Response: -2353984
Conc: N.D.

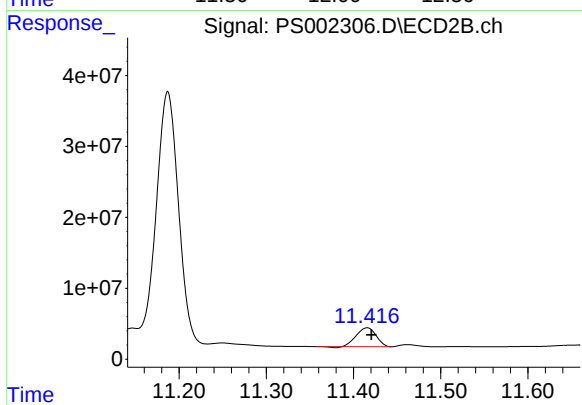

#6 MCPP


R.T.: 11.416 min
Delta R.T.: -0.005 min
Response: 41625834
Conc: 48.38 ug/ml

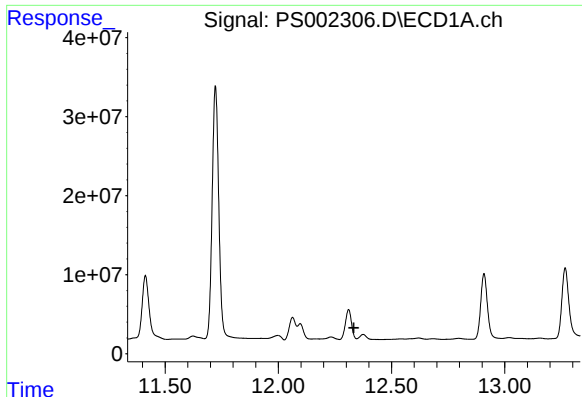

#7 MCPA


R.T.: 12.374 min
Delta R.T.: 0.041 min
Response: -41508335
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

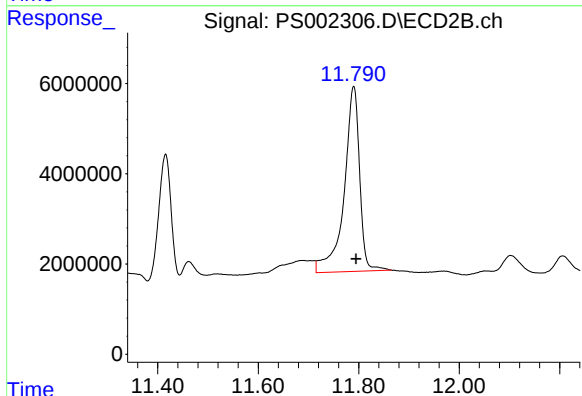


#7 MCPA

R.T.: 11.790 min
Delta R.T.: -0.005 min
Response: 87930221
Conc: 64.97 ug/ml

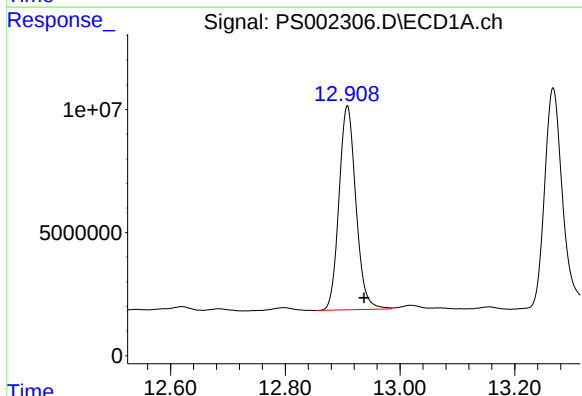


#8 DICHLORPROP

R.T.: 12.908 min
Delta R.T.: -0.029 min
Response: 169305501
Conc: 486.16 ng/ml

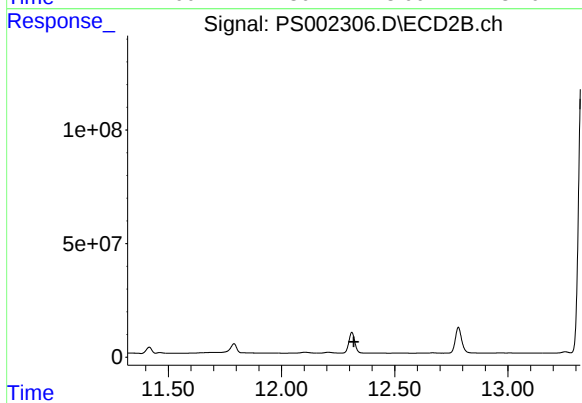

#8 DICHLORPROP


R.T.: 12.310 min
Delta R.T.: -0.009 min
Response: -119339160
Conc: N.D.

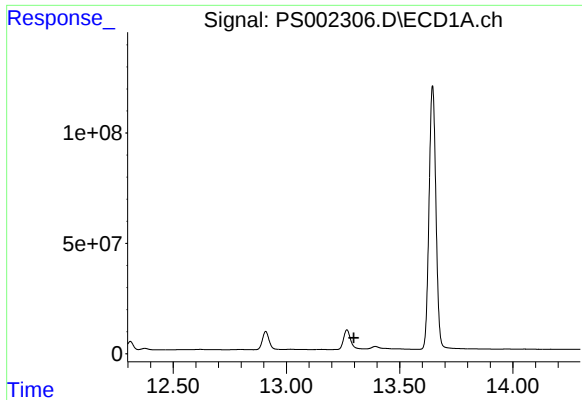

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

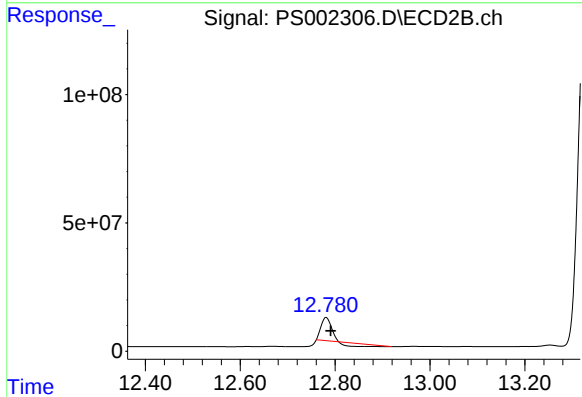


#9 2,4-D

R.T.: 12.781 min
Delta R.T.: -0.010 min
Response: 85079475
Conc: 199.77 ng/ml

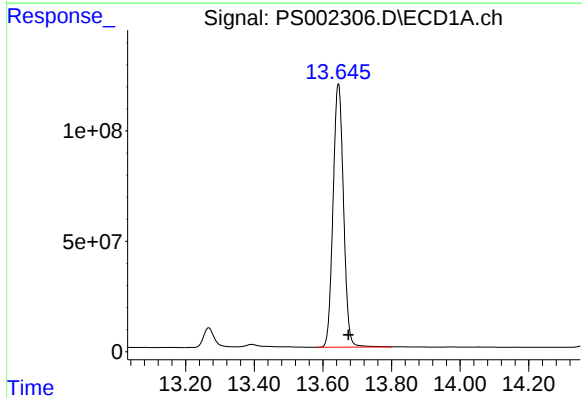


#10 Pentachlorophenol

R.T.: 13.645 min
Delta R.T.: -0.029 min
Response: 2524424732
Conc: 524.75 ng/ml

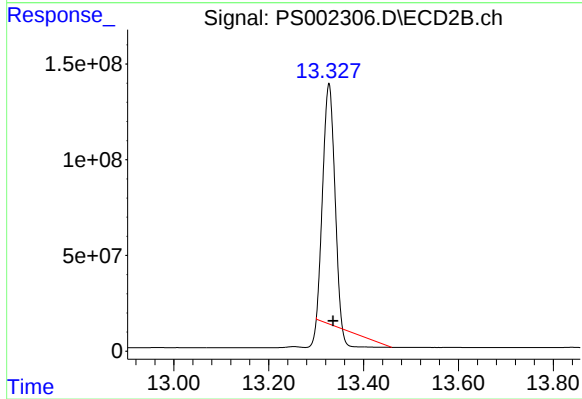

#10 Pentachlorophenol


R.T.: 13.327 min
Delta R.T.: -0.008 min
Response: 1866636903
Conc: 397.37 ng/ml

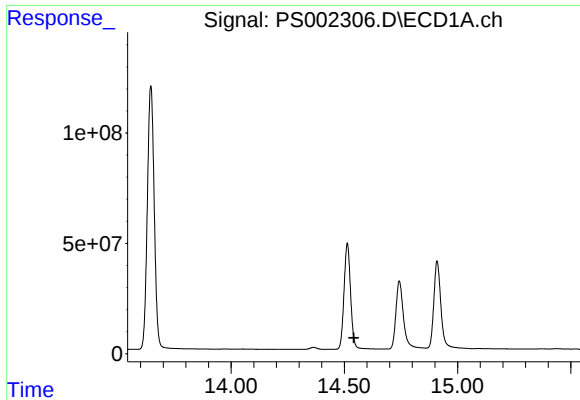

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

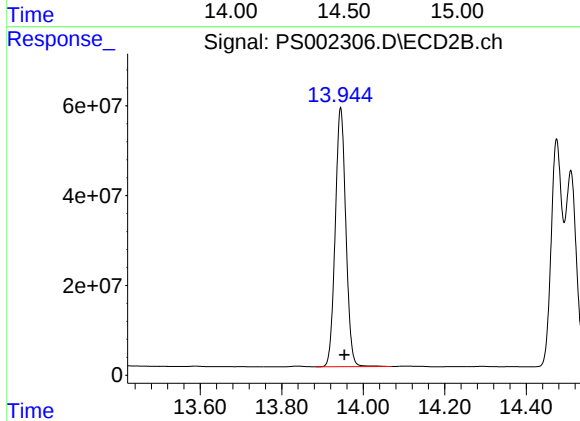


#11 2,4,5-TP (SILVEX)

R.T.: 13.945 min
Delta R.T.: -0.009 min
Response: 1040086393
Conc: 568.49 ng/ml

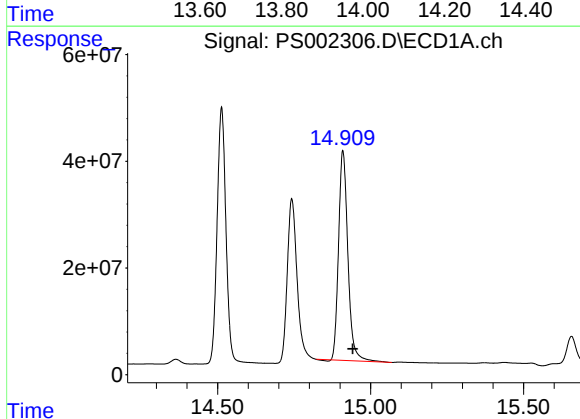


#12 2,4,5-T

R.T.: 14.909 min
Delta R.T.: -0.032 min
Response: 831595825
Conc: 463.99 ng/ml

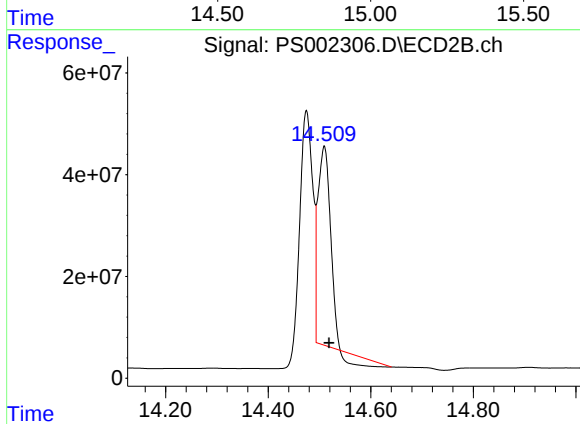

#12 2,4,5-T


R.T.: 14.509 min
Delta R.T.: -0.010 min
Response: 595437079
Conc: 397.63 ng/ml

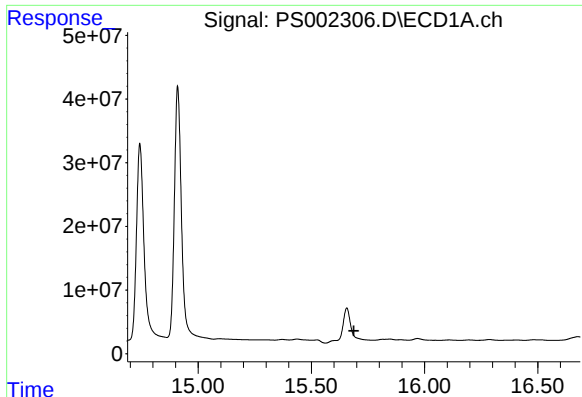

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

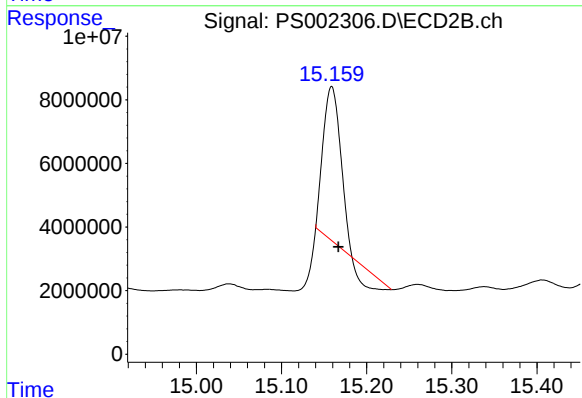


#13 2,4-DB

R.T.: 15.159 min
Delta R.T.: -0.008 min
Response: 59716112
Conc: 269.53 ng/ml

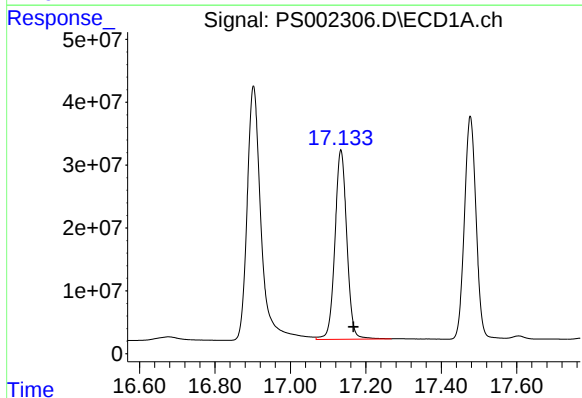


#14 DINOSEB

R.T.: 17.134 min
Delta R.T.: -0.034 min
Response: 660947947
Conc: 482.43 ng/ml

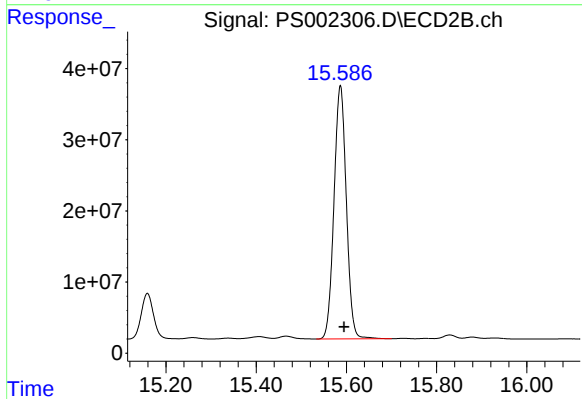

#14 DINOSEB


R.T.: 15.587 min
Delta R.T.: -0.008 min
Response: 675012563
Conc: 533.24 ng/ml

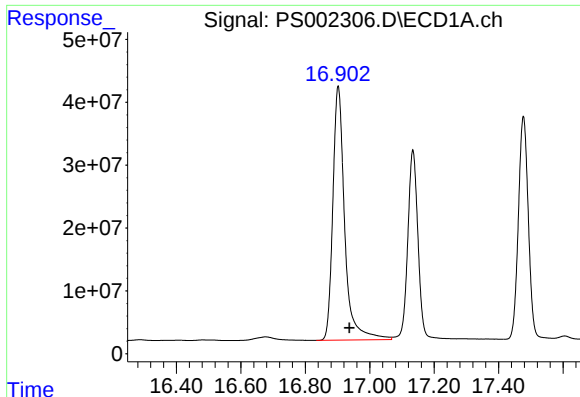

#15 Picloram


R.T.: 16.902 min
Delta R.T.: -0.035 min
Response: 1035994745
Conc: 434.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

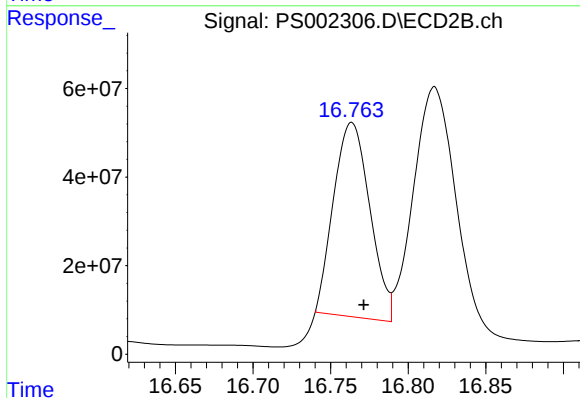


#15 Picloram

R.T.: 16.764 min
Delta R.T.: -0.008 min
Response: 712564356
Conc: 314.98 ng/ml

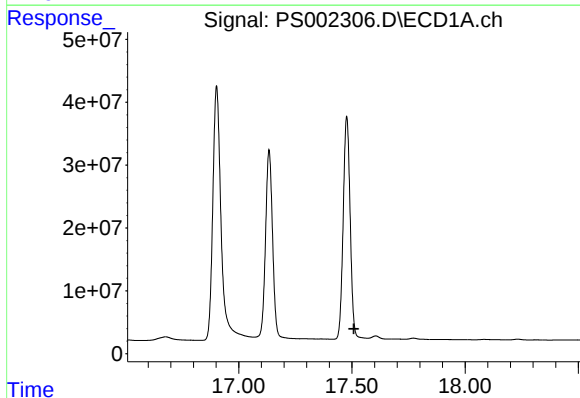

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

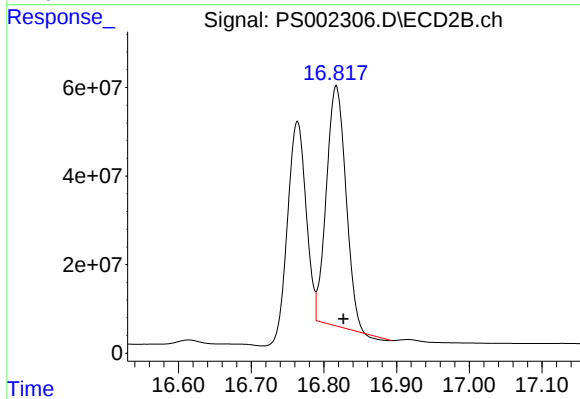

#16 DCPA

R.T.: 16.817 min
Delta R.T.: -0.010 min
Response: 1004499038
Conc: 424.22 ng/ml