

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
 Data File : PS002312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2018 21:32
 Operator : EI\SJ
 Sample : J5764-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:02:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.444	10.936	132.3E6	123.6E6	420.440	344.136
Target Compounds							
1) T	Dalapon	2.914	2.369	10286674	10631279	22.427	23.546
2) T	3,5-DICHL...	9.805	9.096	1789461	-2595	3.942	N.D. #
3) T	4-Nitroph...	0.000	10.097	0	2957568	N.D.	16.587 #
5) T	DICAMBA	11.680	0.000	8598321	0	6.475	N.D. #
6) T	MCPD	12.125	11.445	54965779	931937	55.641	1.083 #
7) T	MCPA	0.000	11.832	0	1604712	N.D.	1.186 #
8) T	DICHLORPROP	0.000	12.286	0	374655	N.D.	1.167 #
10) T	Pentachlo...	13.684	13.359	5709022	-416269	1.187	N.D. #
11) T	2,4,5-TP ...	0.000	13.947	0	138101	N.D.	0.075 #
13) T	2,4-DB	0.000	15.130	0	2827062	N.D.	12.760 #
15) T	Picloram	0.000	16.706	0	7373254	N.D.	3.259 #
16) T	DCPA	0.000	16.860	0	6731810	N.D.	2.843 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
Data File : PS002312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2018 21:32
Operator : EI\SJ
Sample : J5764-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:02:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

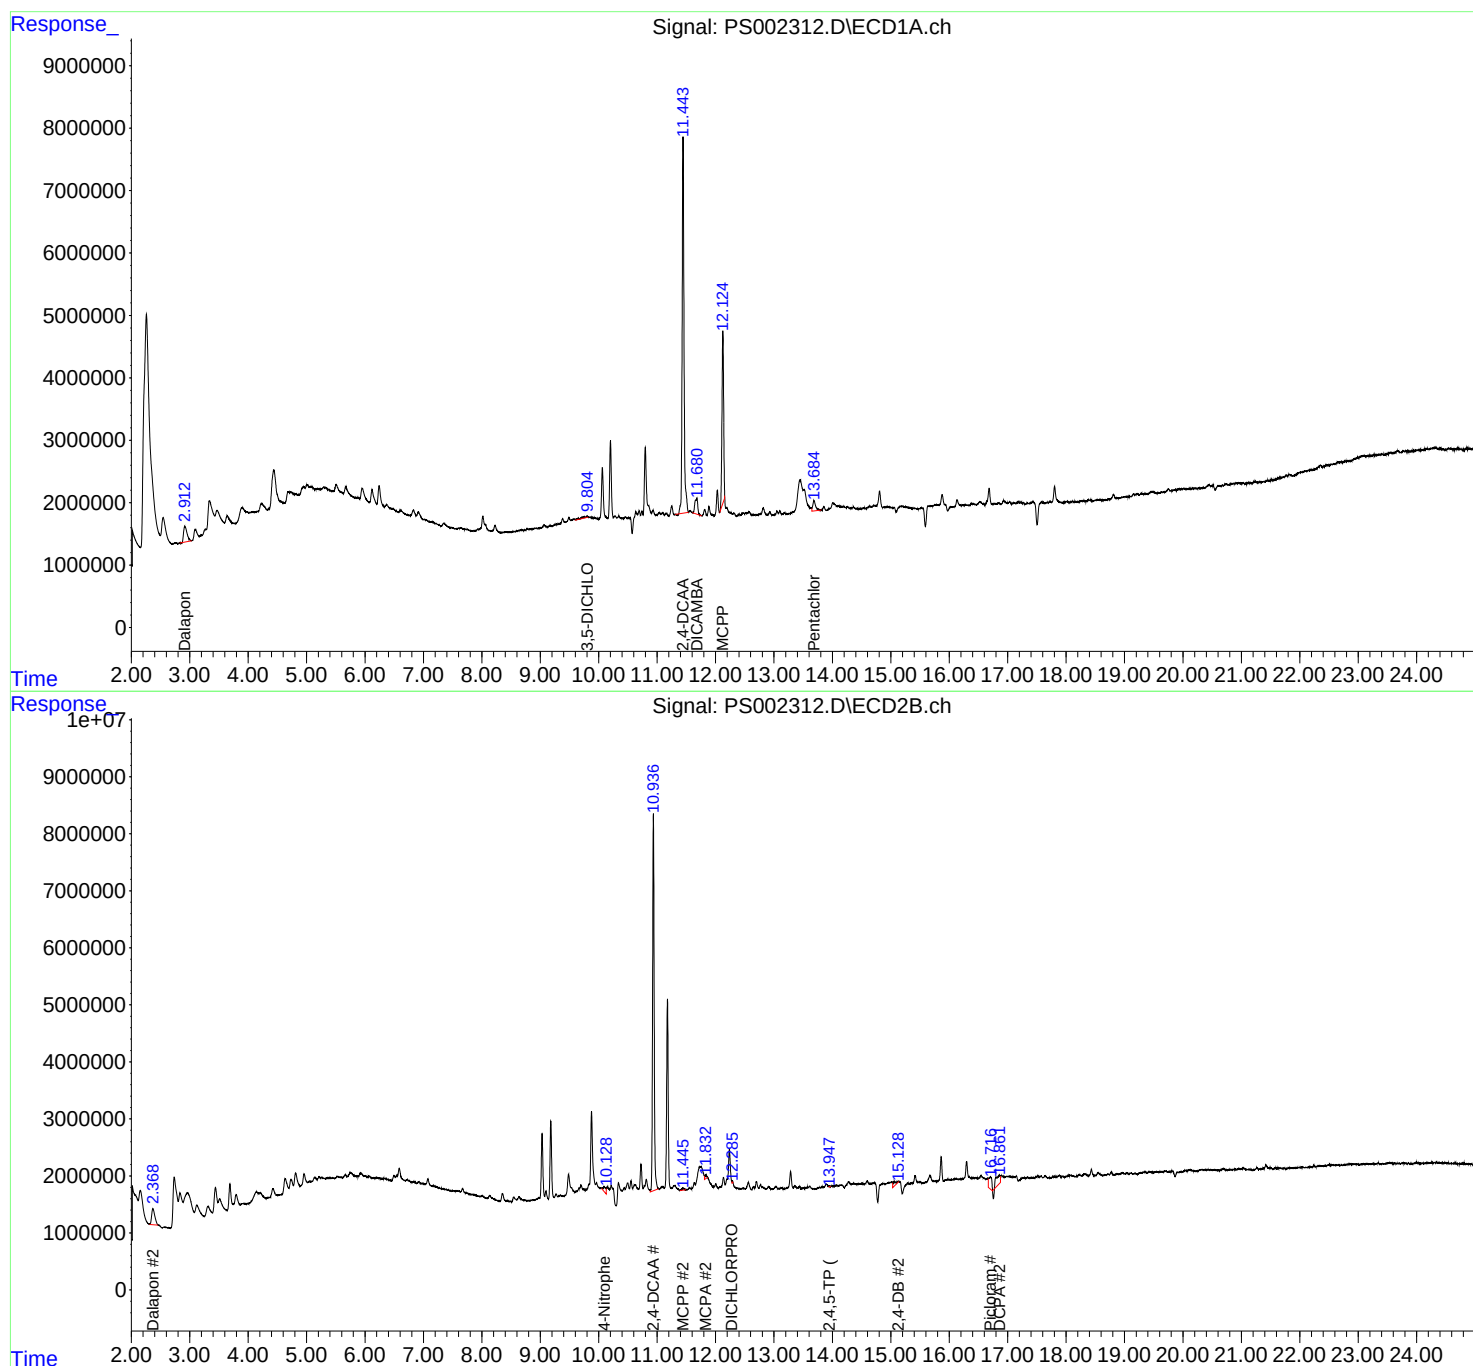


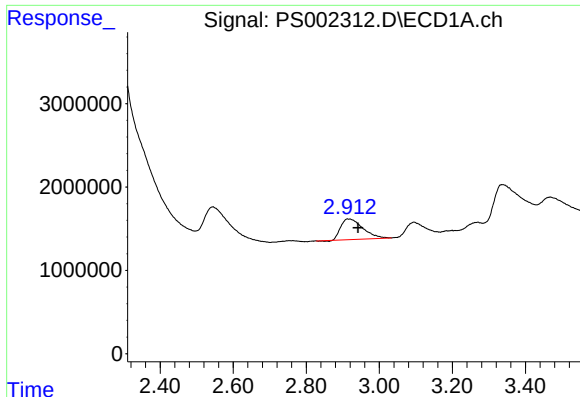

#1 Dalapon


R.T.: 2.914 min
Delta R.T.: -0.028 min
Response: 10286674
Conc: 22.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

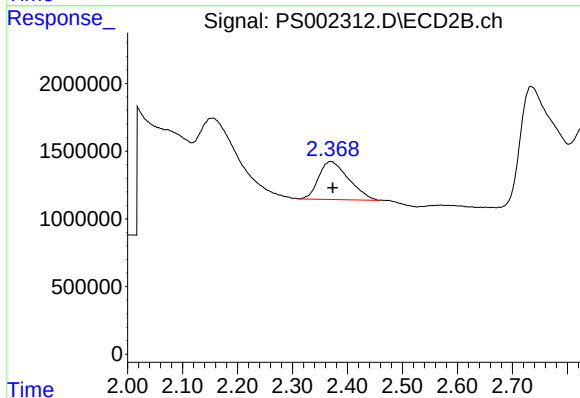


#1 Dalapon

R.T.: 2.369 min
Delta R.T.: -0.005 min
Response: 10631279
Conc: 23.55 ng/ml

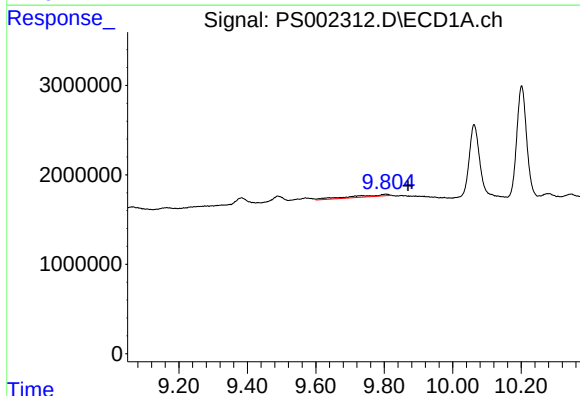


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.805 min
Delta R.T.: -0.065 min
Response: 1789461
Conc: 3.94 ng/ml

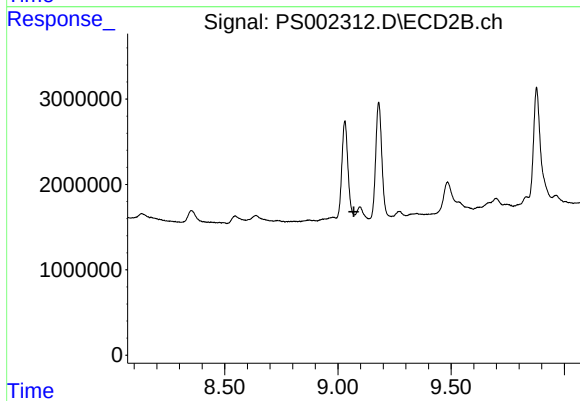

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.096 min
Delta R.T.: 0.026 min
Response: -2595
Conc: N.D.

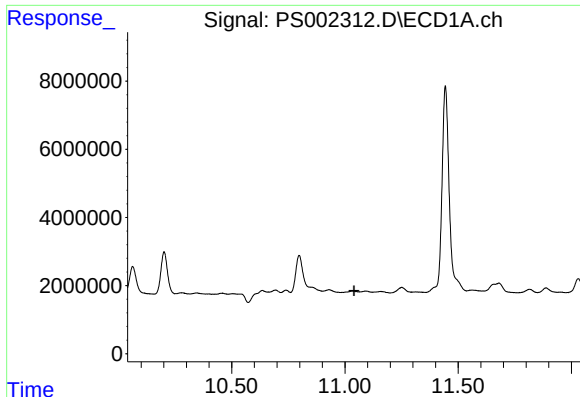

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

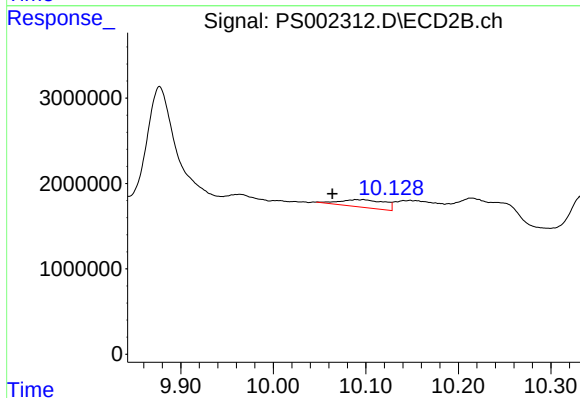


#3 4-Nitrophenol

R.T.: 10.097 min
Delta R.T.: 0.034 min
Response: 2957568
Conc: 16.59 ng/ml

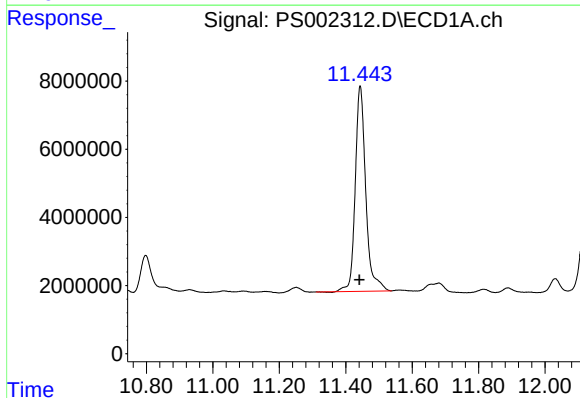


#4 2,4-DCAA

R.T.: 11.444 min
Delta R.T.: 0.002 min
Response: 132306516
Conc: 420.44 ng/ml

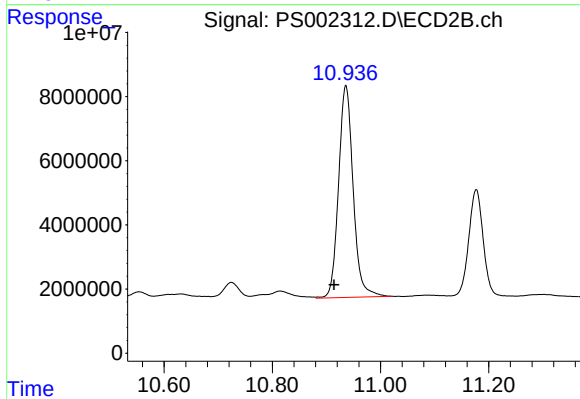

#4 2,4-DCAA


R.T.: 10.936 min
Delta R.T.: 0.022 min
Response: 123578373
Conc: 344.14 ng/ml

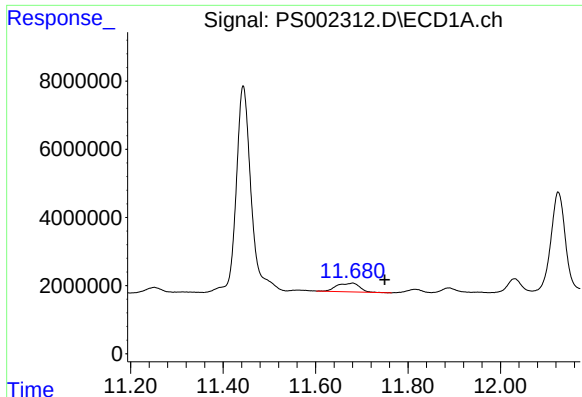

#5 DICAMBA


R.T.: 11.680 min
Delta R.T.: -0.069 min
Response: 8598321
Conc: 6.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

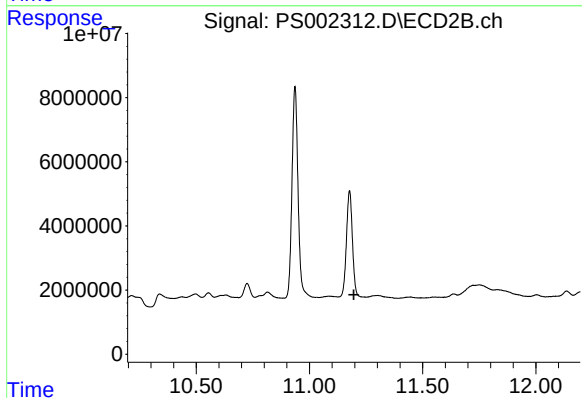


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.197 min
Response: 0
Conc: N.D.

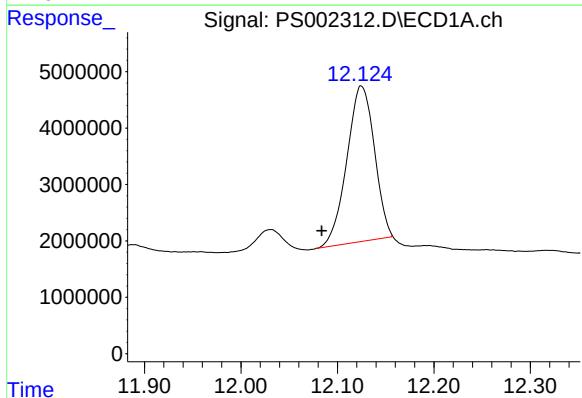


#6 MCP

R.T.: 12.125 min
Delta R.T.: 0.041 min
Response: 54965779
Conc: 55.64 ug/ml

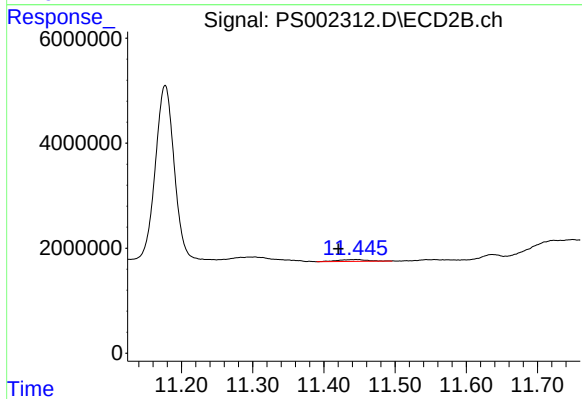

#6 MCP


R.T.: 11.445 min
Delta R.T.: 0.025 min
Response: 931937
Conc: 1.08 ug/ml

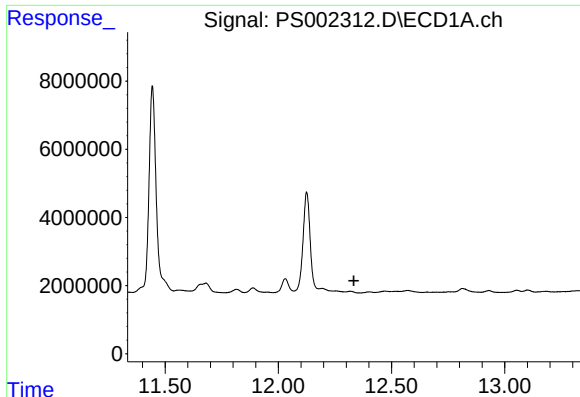

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

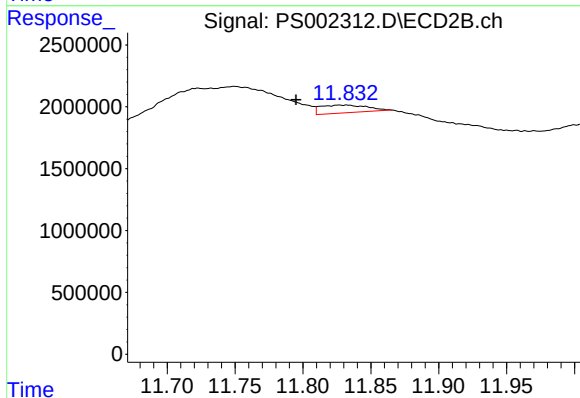


#7 MCPA

R.T.: 11.832 min
Delta R.T.: 0.038 min
Response: 1604712
Conc: 1.19 ug/ml

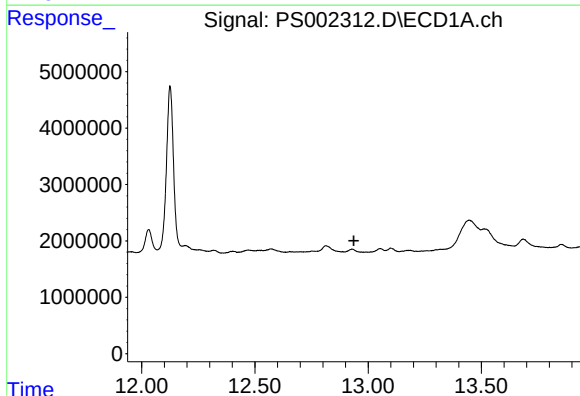


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

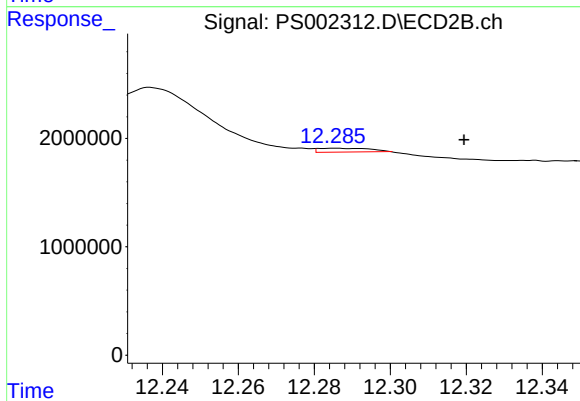

#8 DICHLORPROP


R.T.: 12.286 min
Delta R.T.: -0.034 min
Response: 374655
Conc: 1.17 ng/ml

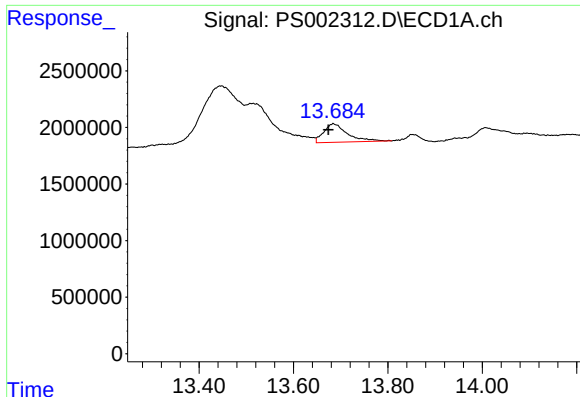

#10 Pentachlorophenol


R.T.: 13.684 min
Delta R.T.: 0.010 min
Response: 5709022
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

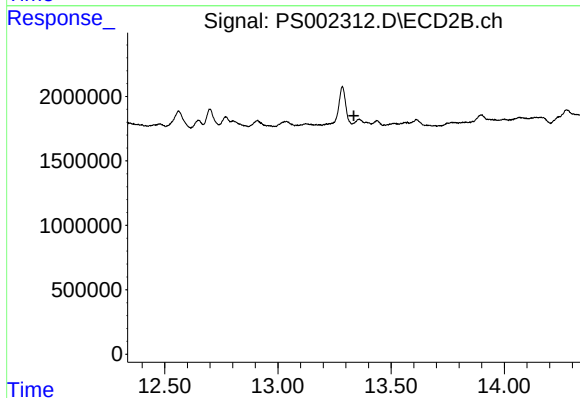


#10 Pentachlorophenol

R.T.: 13.359 min
Delta R.T.: 0.023 min
Response: -416269
Conc: N.D.

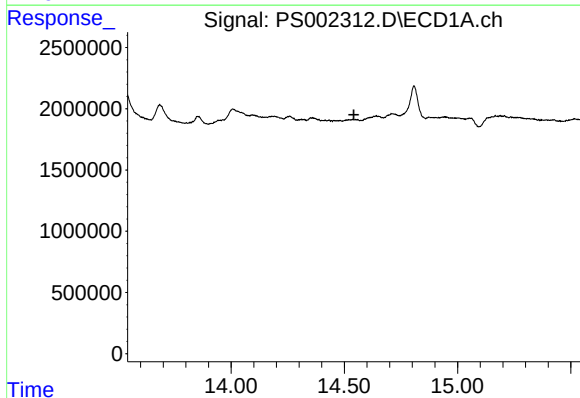


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.542 min
Response: 0
Conc: N.D.

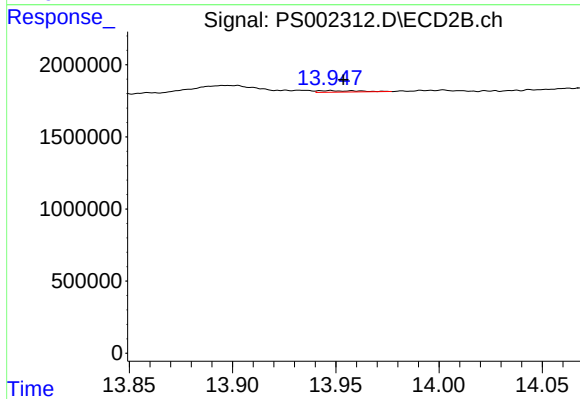

#11 2,4,5-TP (SILVEX)


R.T.: 13.947 min
Delta R.T.: -0.006 min
Response: 138101
Conc: 0.08 ng/ml

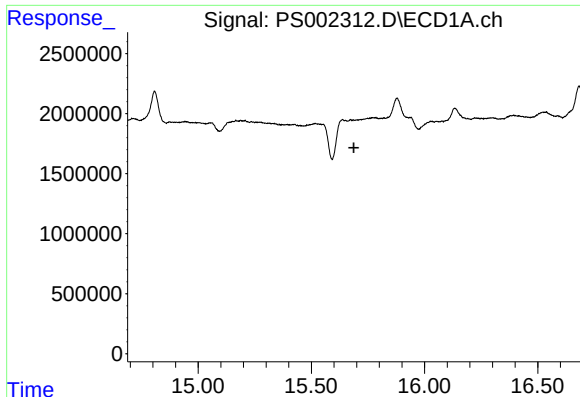

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

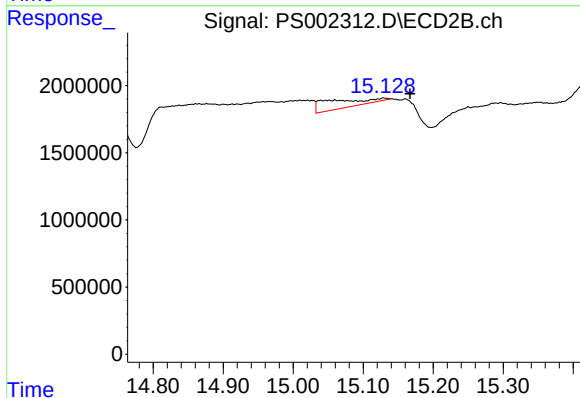


#13 2,4-DB

R.T.: 15.130 min
Delta R.T.: -0.037 min
Response: 2827062
Conc: 12.76 ng/ml

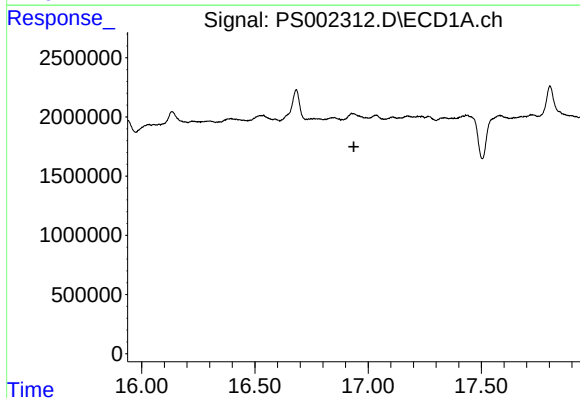


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.937 min
Response: 0
Conc: N.D.

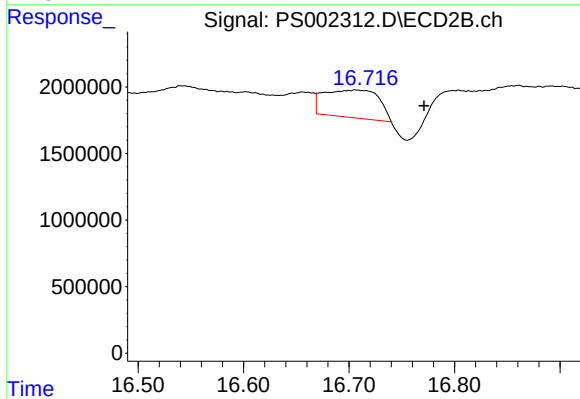

#15 Picloram


R.T.: 16.706 min
Delta R.T.: -0.065 min
Response: 7373254
Conc: 3.26 ng/ml

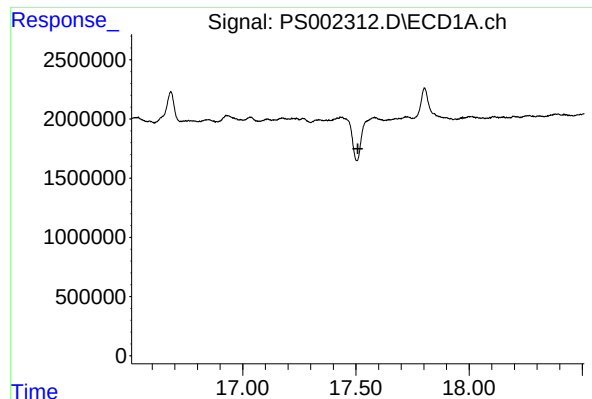

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

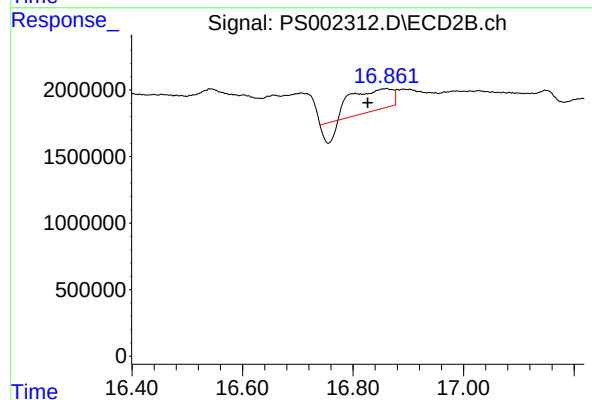

#16 DCPA

R.T.: 16.860 min
Delta R.T.: 0.033 min
Response: 6731810
Conc: 2.84 ng/ml