

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
 Data File : PS002319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 01:10
 Operator : EI\SJ
 Sample : J5764-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 08:00:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.451	10.943	147.8E6	137.0E6	469.751	381.504
Target Compounds							
1) T	Dalapon	2.925	2.378	11658321	15384335	25.418	34.073 #
2) T	3,5-DICHL...	0.000	9.103	0	1547269	N.D.	3.488 #
3) T	4-Nitroph...	11.040	10.099	5969726	2964046	35.783	16.623 #
5) T	DICAMBA	11.687	11.184	9167321	14500591	6.903	11.603 #
6) T	MCPD	12.037	11.447	5874457	-637941	5.947	N.D. #
7) T	MCPA	0.000	11.758	0	9413672	N.D.	6.956 #
9) T	2,4-D	0.000	12.774	0	1108401	N.D.	2.603 #
11) T	2,4,5-TP ...	0.000	13.903	0	854691	N.D.	0.467 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
Data File : PS002319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 01:10
Operator : EI\SJ
Sample : J5764-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 08:00:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

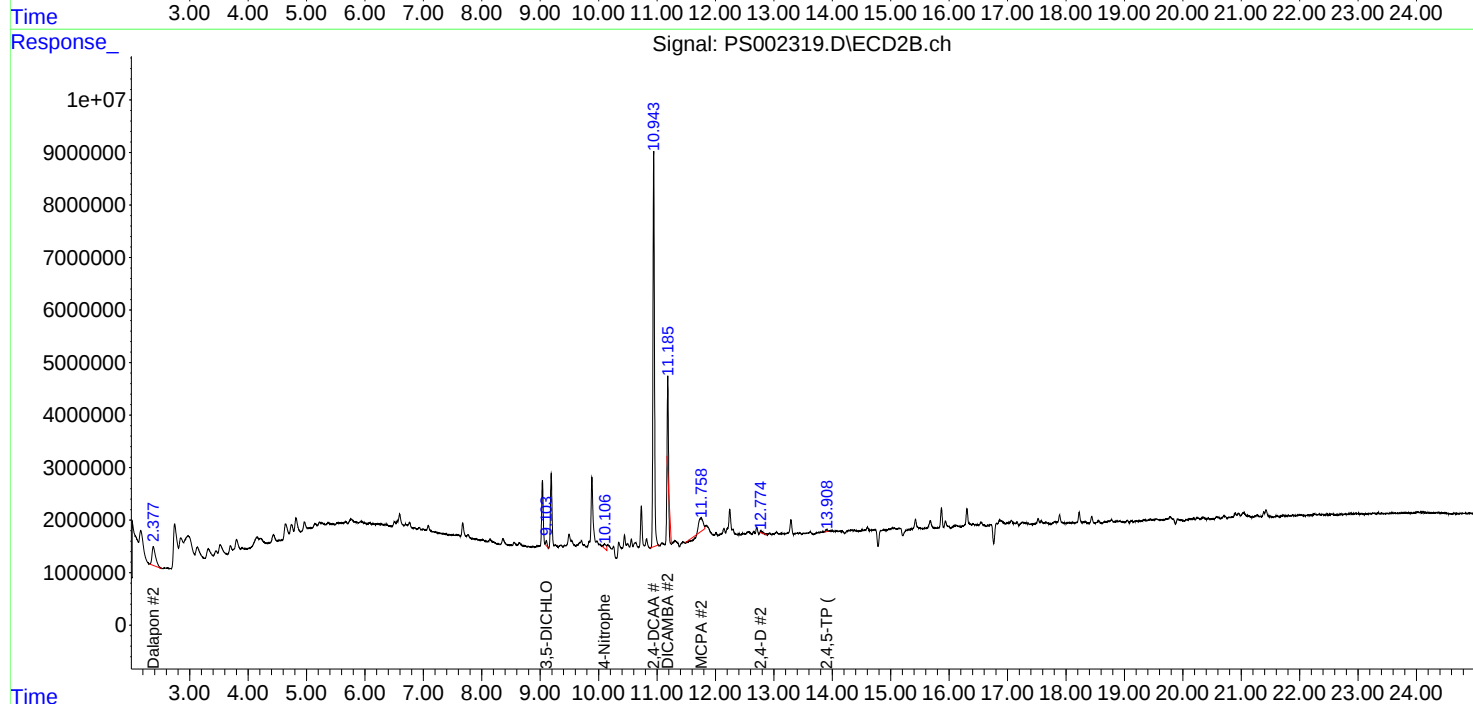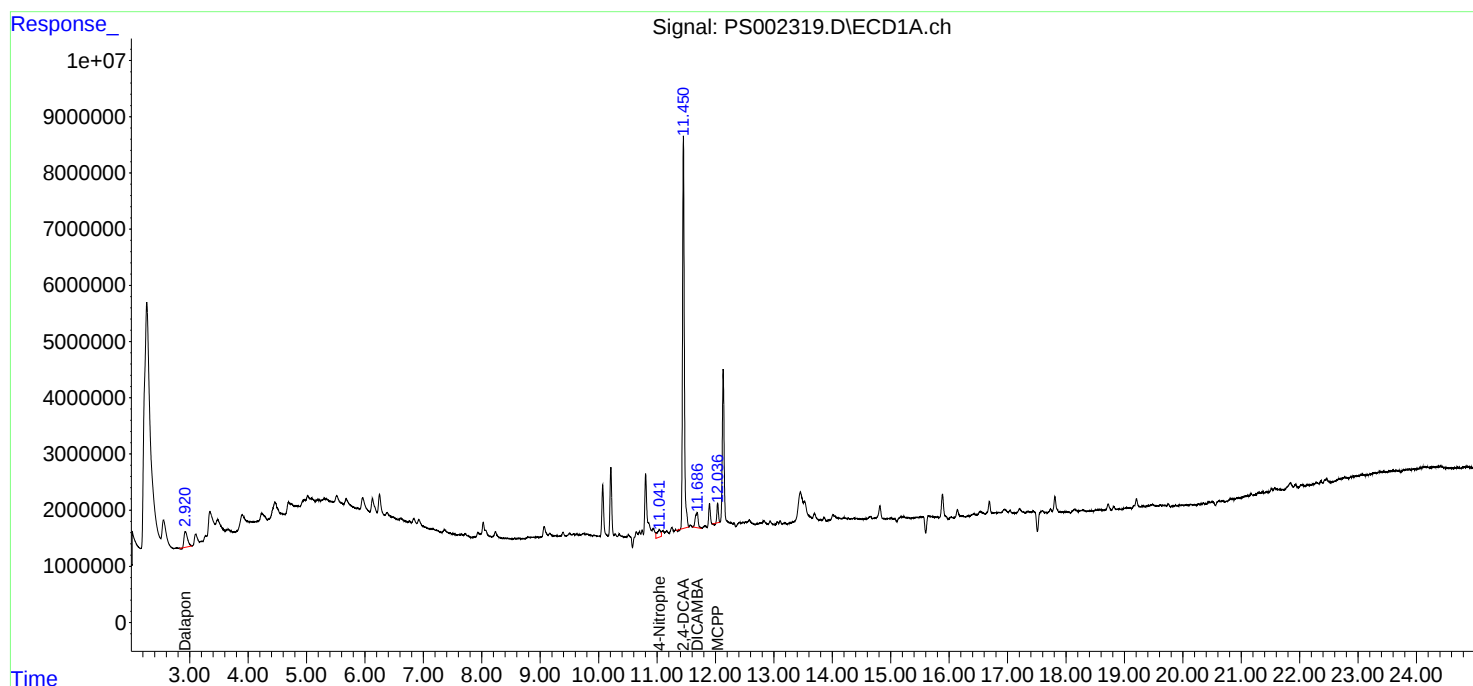


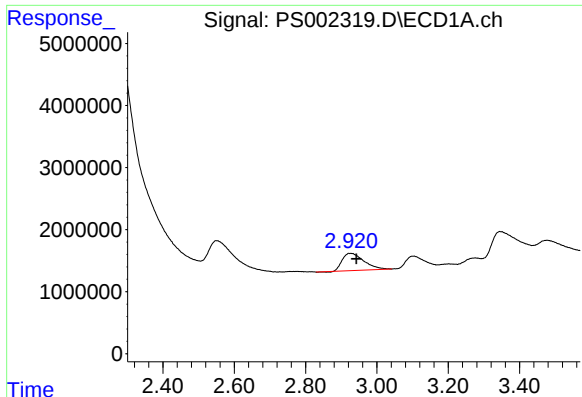

#1 Dalapon


R.T.: 2.925 min
Delta R.T.: -0.017 min
Response: 11658321
Conc: 25.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

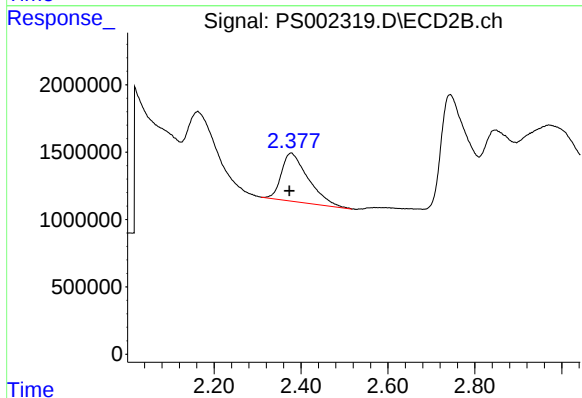


#1 Dalapon

R.T.: 2.378 min
Delta R.T.: 0.004 min
Response: 15384335
Conc: 34.07 ng/ml

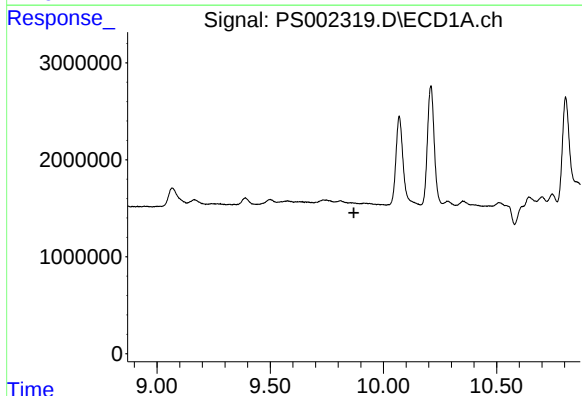


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

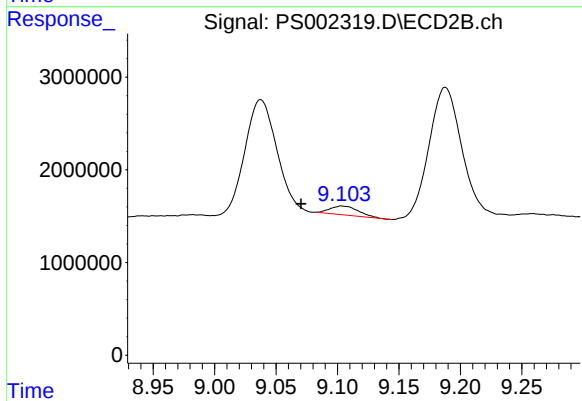

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.103 min
Delta R.T.: 0.033 min
Response: 1547269
Conc: 3.49 ng/ml

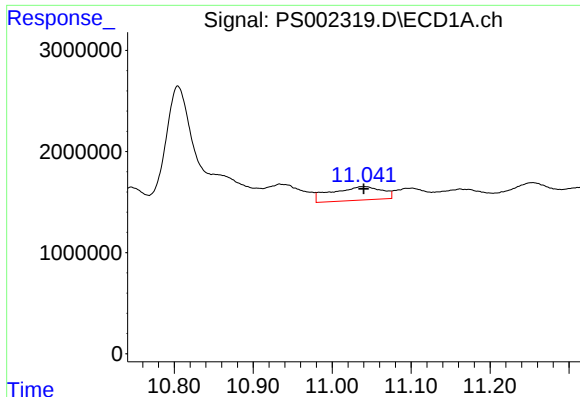

#3 4-Nitrophenol


R.T.: 11.040 min
Delta R.T.: 0.000 min
Response: 5969726
Conc: 35.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

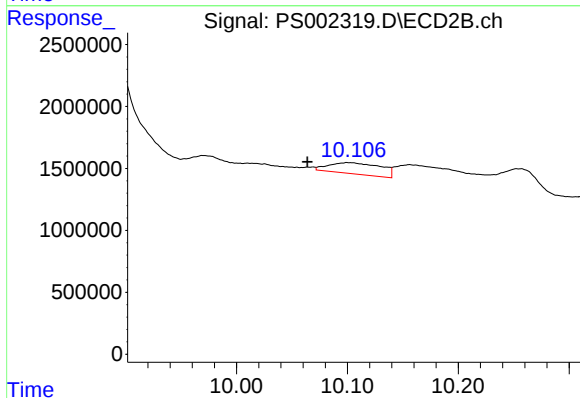


#3 4-Nitrophenol

R.T.: 10.099 min
Delta R.T.: 0.036 min
Response: 2964046
Conc: 16.62 ng/ml

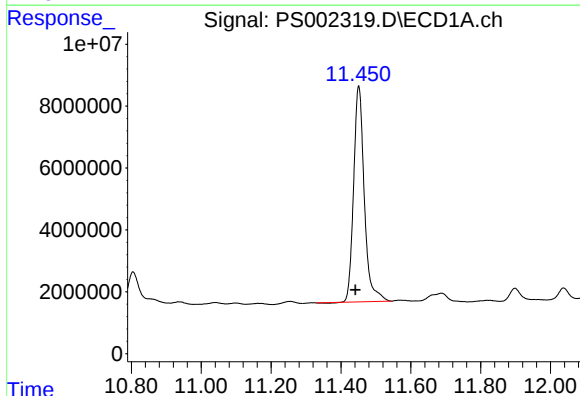


#4 2,4-DCAA

R.T.: 11.451 min
Delta R.T.: 0.010 min
Response: 147824035
Conc: 469.75 ng/ml

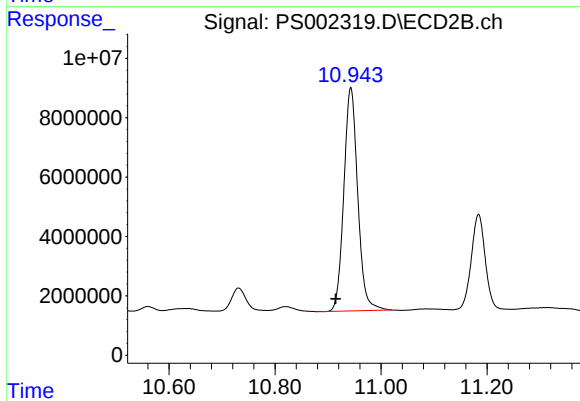

#4 2,4-DCAA


R.T.: 10.943 min
Delta R.T.: 0.029 min
Response: 136997178
Conc: 381.50 ng/ml

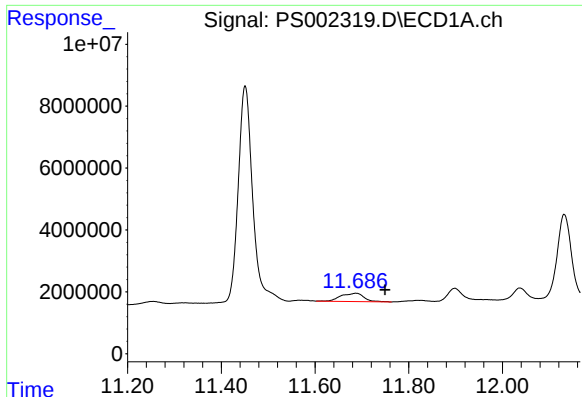

#5 DICAMBA


R.T.: 11.687 min
Delta R.T.: -0.062 min
Response: 9167321
Conc: 6.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

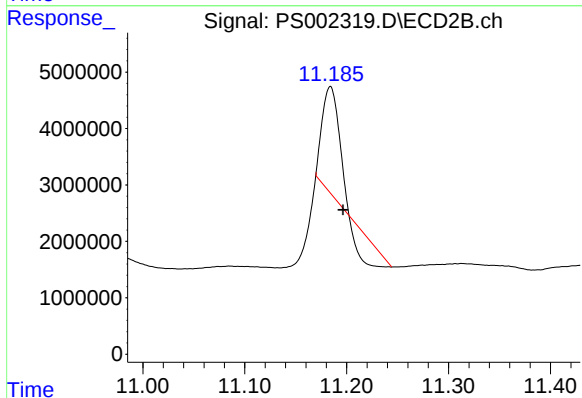


#5 DICAMBA

R.T.: 11.184 min
Delta R.T.: -0.012 min
Response: 14500591
Conc: 11.60 ng/ml

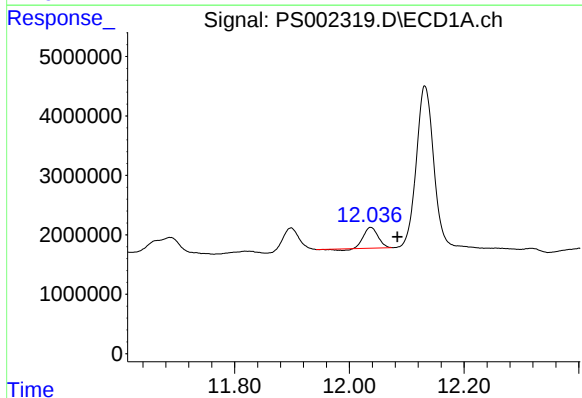


#6 MCP

R.T.: 12.037 min
Delta R.T.: -0.047 min
Response: 5874457
Conc: 5.95 ug/ml

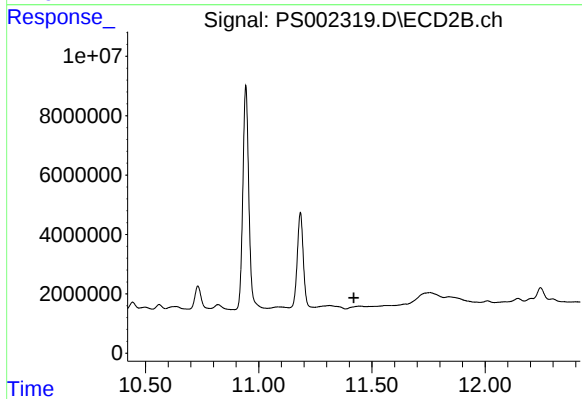

#6 MCP


R.T.: 11.447 min
Delta R.T.: 0.027 min
Response: -637941
Conc: N.D.

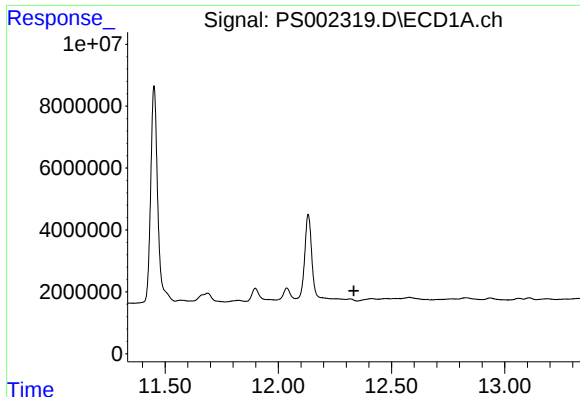

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

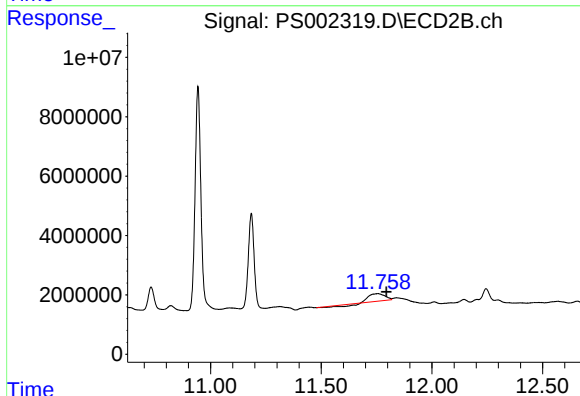


#7 MCPA

R.T.: 11.758 min
Delta R.T.: -0.037 min
Response: 9413672
Conc: 6.96 ug/ml

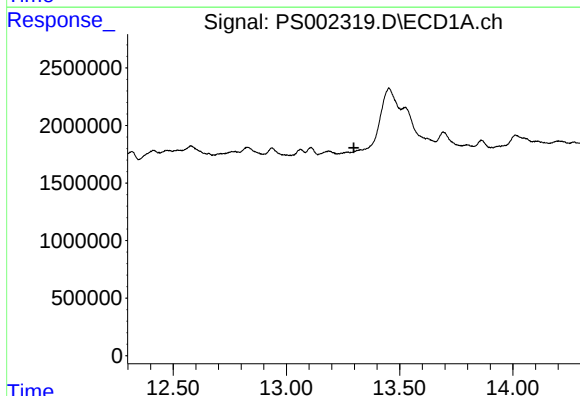


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

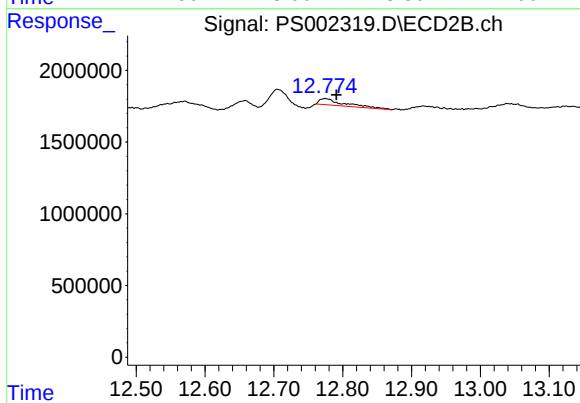

#9 2,4-D


R.T.: 12.774 min
Delta R.T.: -0.017 min
Response: 1108401
Conc: 2.60 ng/ml

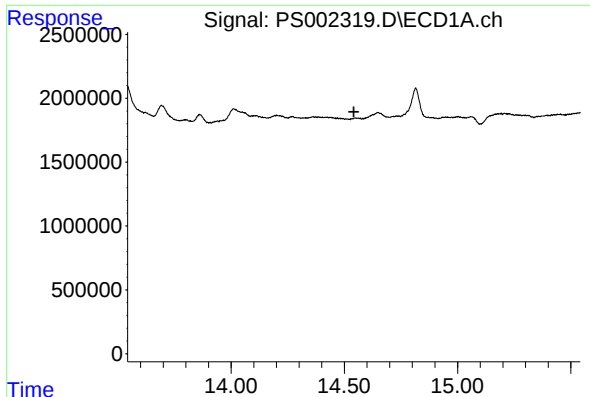

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

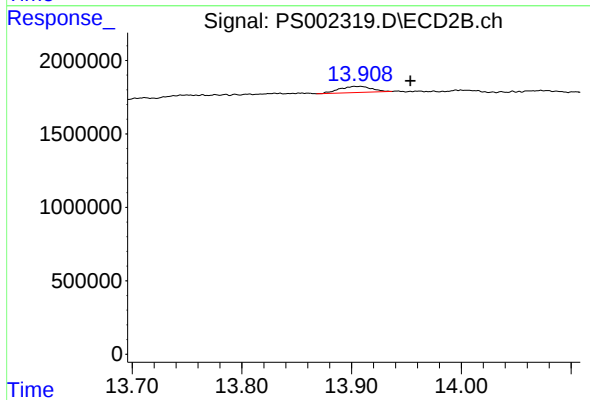

#11 2,4,5-TP (SILVEX)

R.T.: 13.903 min
Delta R.T.: -0.051 min
Response: 854691
Conc: 0.47 ng/ml