

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
 Data File : PS002323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 03:14
 Operator : EI\SJ
 Sample : J5815-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 08:01:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.442	10.937	178.8E6	167.0E6	568.039	465.073
Target Compounds							
1) T	Dalapon	2.920	2.373	19980298	29285500	43.562	64.862 #
3) T	4-Nitroph...	0.000	10.096	0	9280373	N.D.	52.046 #
6) T	MCP	12.124	0.000	69447491	0	70.301	N.D. #
7) T	MCPA	0.000	11.759	0	18397055	N.D.	13.593 #
8) T	DICHLORPROP	0.000	12.292	0	355327	N.D.	1.106 #
10) T	Pentachlo...	0.000	13.286	0	795641	N.D.	0.169 #
11) T	2,4,5-TP ...	0.000	13.972	0	138429	N.D.	0.076 #
15) T	Picloram	0.000	16.804	0	989522	N.D.	0.437 #
16) T	DCPA	0.000	16.804	0	989522	N.D.	0.418 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
Data File : PS002323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 03:14
Operator : EI\SJ
Sample : J5815-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 08:01:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

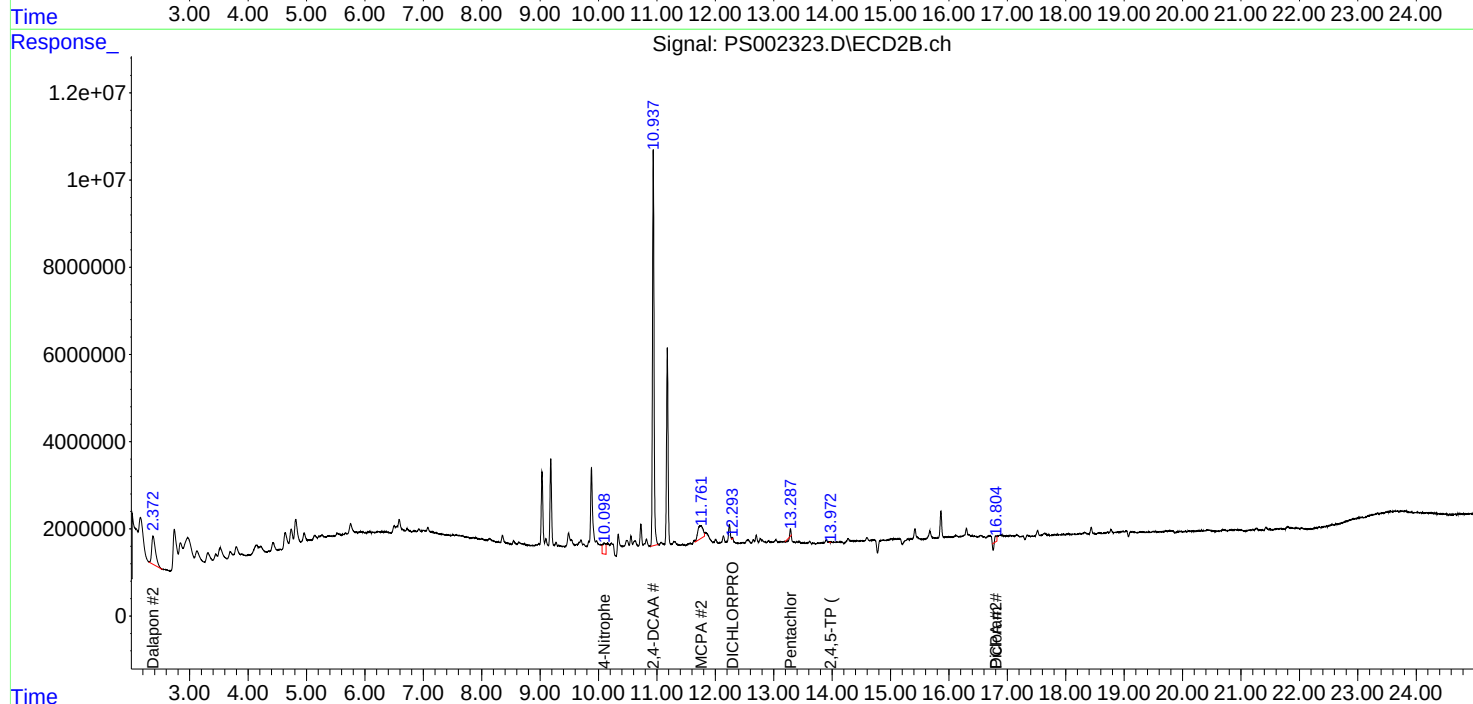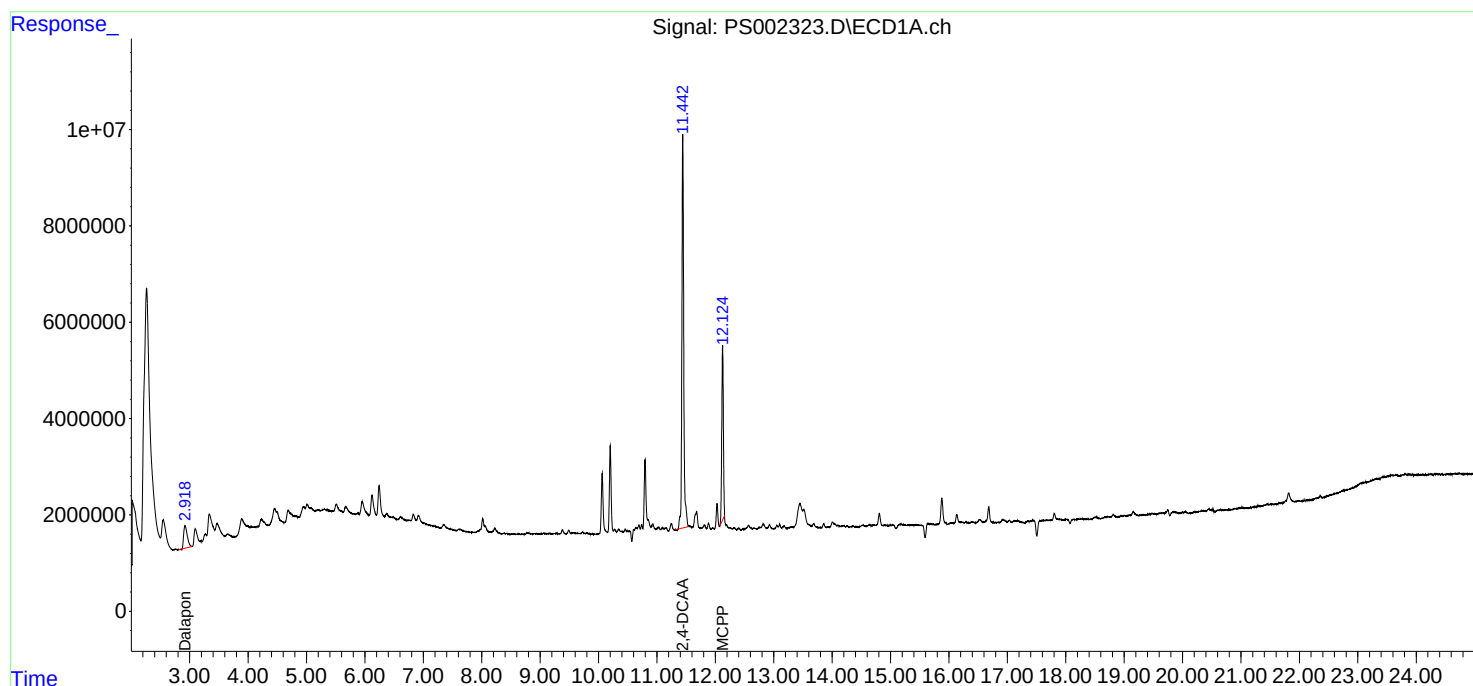


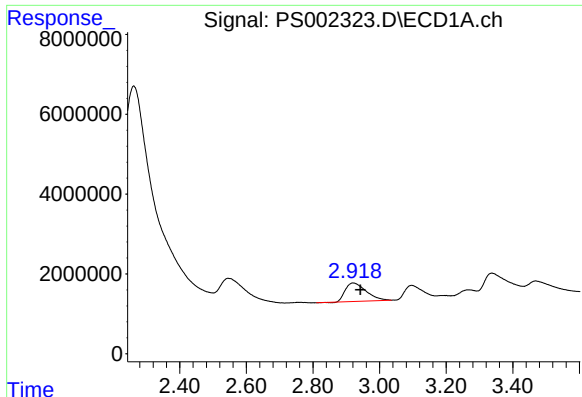

#1 Dalapon


R.T.: 2.920 min
Delta R.T.: -0.022 min
Response: 19980298
Conc: 43.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

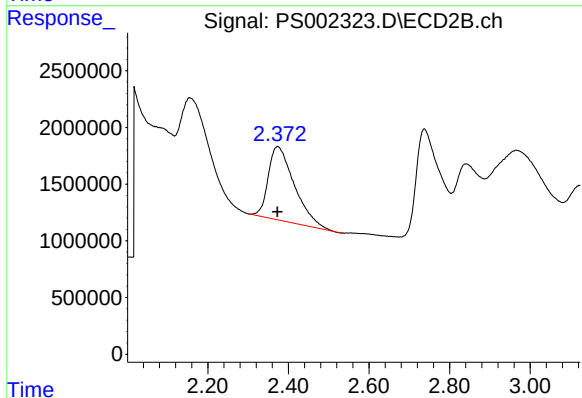


#1 Dalapon

R.T.: 2.373 min
Delta R.T.: 0.000 min
Response: 29285500
Conc: 64.86 ng/ml

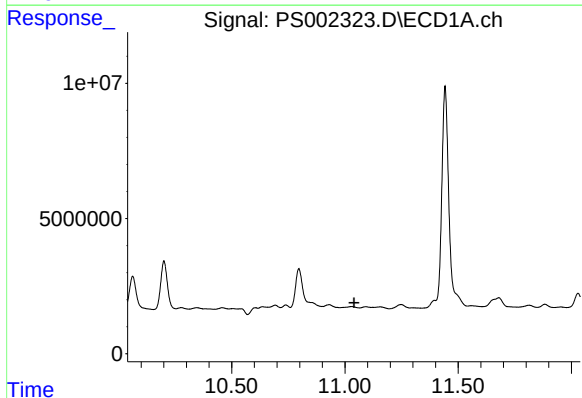


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.040 min
Response: 0
Conc: N.D.

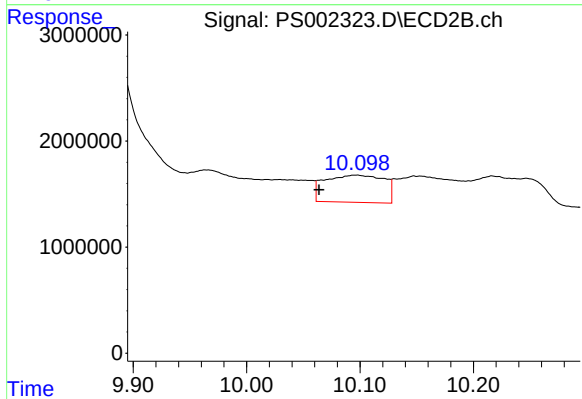

#3 4-Nitrophenol


R.T.: 10.096 min
Delta R.T.: 0.033 min
Response: 9280373
Conc: 52.05 ng/ml

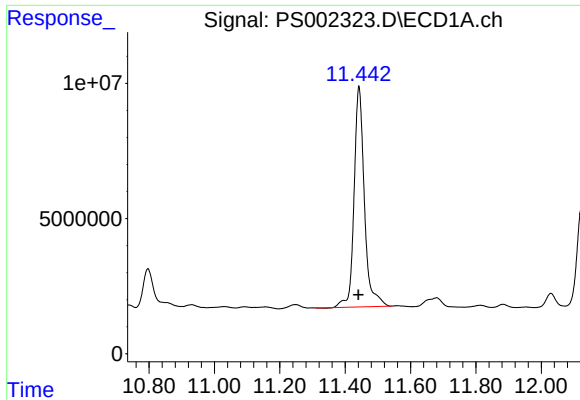

#4 2,4-DCAA


R.T.: 11.442 min
Delta R.T.: 0.001 min
Response: 178753788
Conc: 568.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

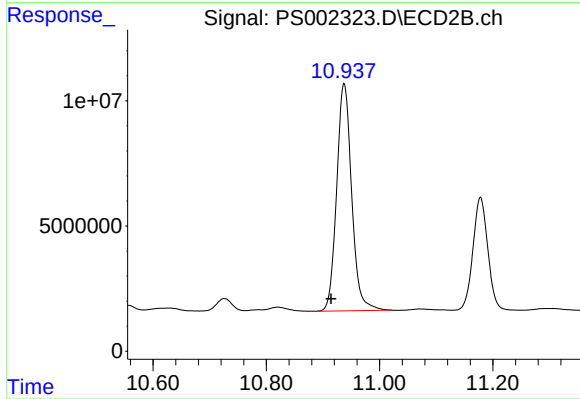


#4 2,4-DCAA

R.T.: 10.937 min
Delta R.T.: 0.023 min
Response: 167006887
Conc: 465.07 ng/ml

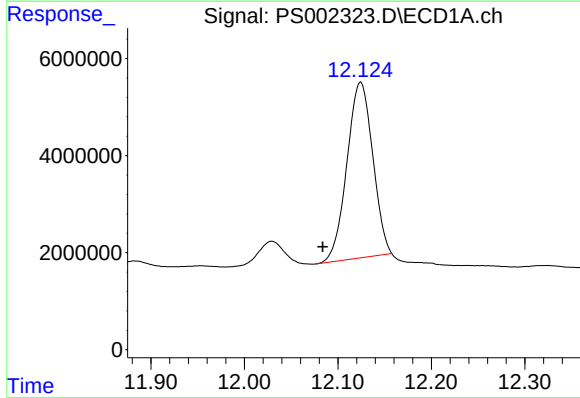


#6 MCPP

R.T.: 12.124 min
Delta R.T.: 0.040 min
Response: 69447491
Conc: 70.30 ug/ml

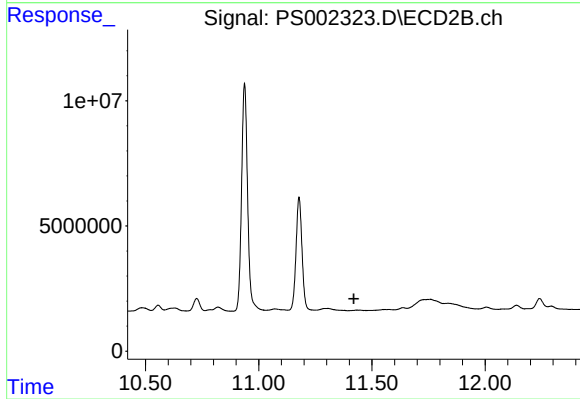

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

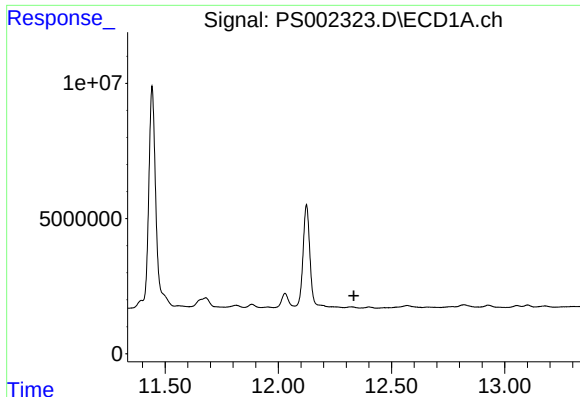

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

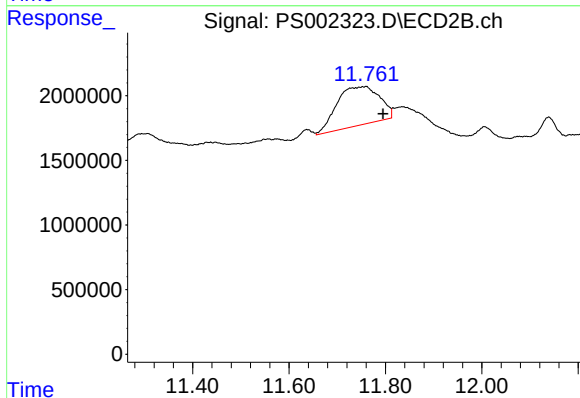


#7 MCPA

R.T.: 11.759 min
Delta R.T.: -0.036 min
Response: 18397055
Conc: 13.59 ug/ml

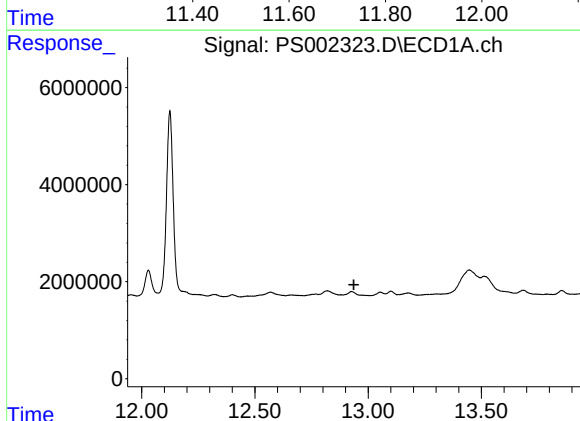


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.937 min
Response: 0
Conc: N.D.

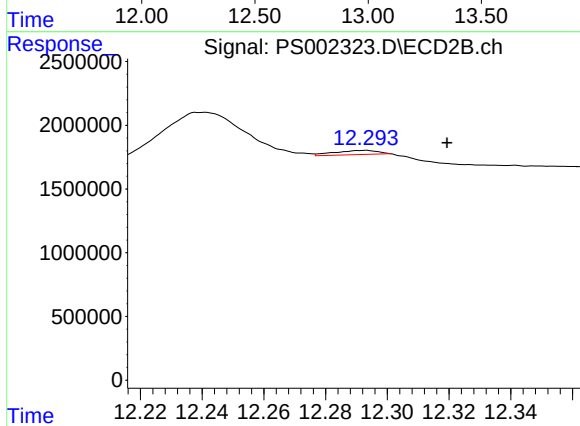

#8 DICHLORPROP


R.T.: 12.292 min
Delta R.T.: -0.027 min
Response: 355327
Conc: 1.11 ng/ml

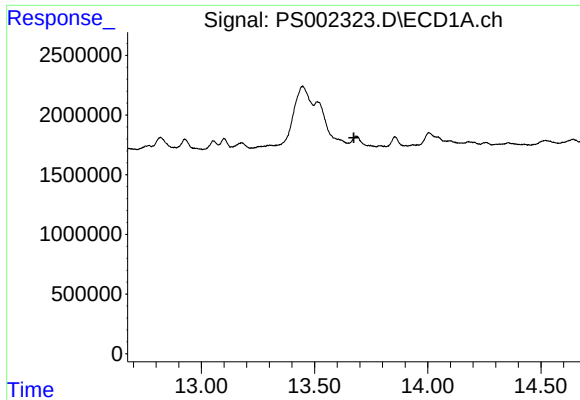

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

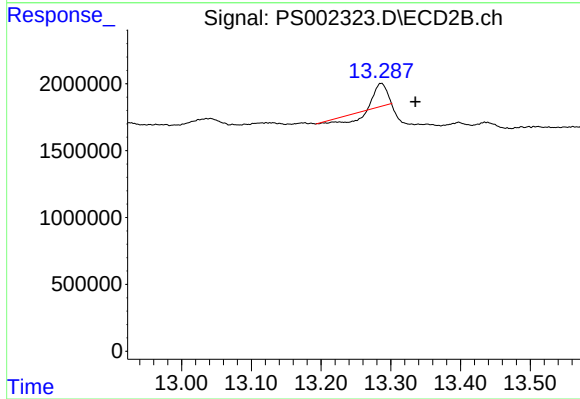


#10 Pentachlorophenol

R.T.: 13.286 min
Delta R.T.: -0.049 min
Response: 795641
Conc: 0.17 ng/ml

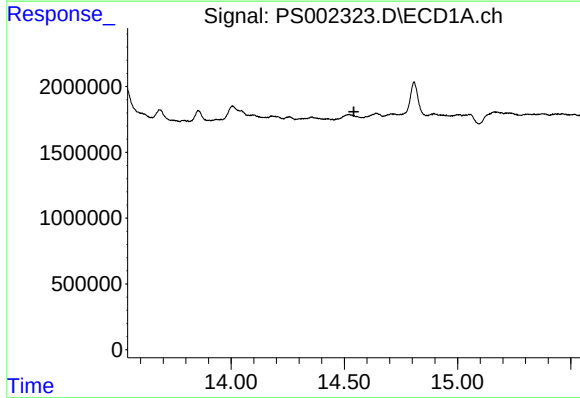


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.542 min
Response: 0
Conc: N.D.

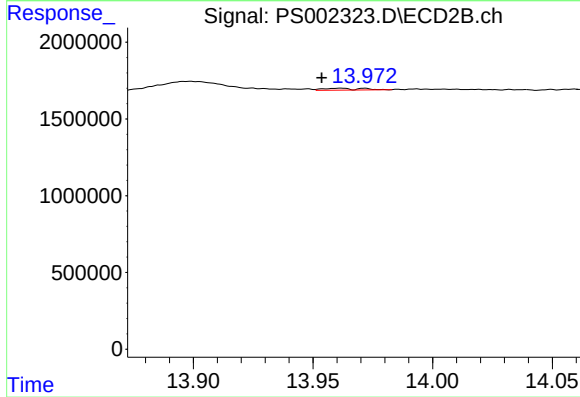

#11 2,4,5-TP (SILVEX)


R.T.: 13.972 min
Delta R.T.: 0.018 min
Response: 138429
Conc: 0.08 ng/ml

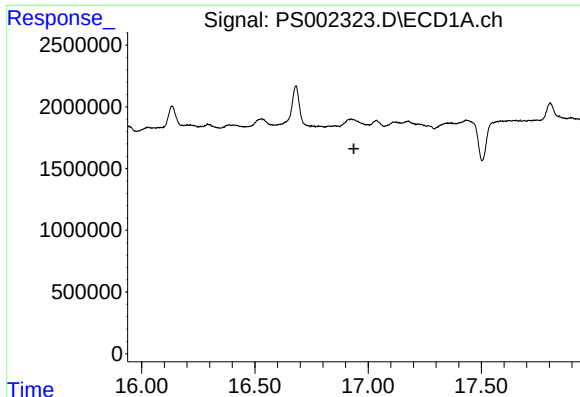

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

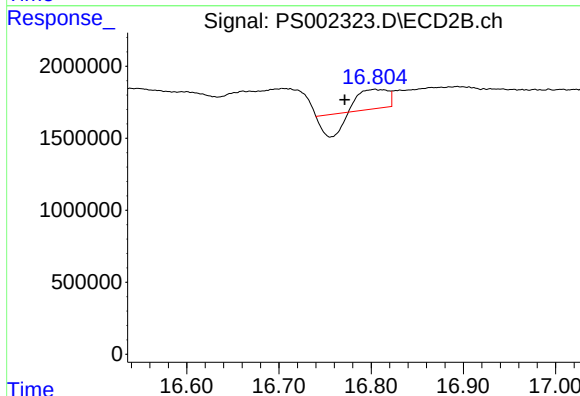


#15 Picloram

R.T.: 16.804 min
Delta R.T.: 0.033 min
Response: 989522
Conc: 0.44 ng/ml

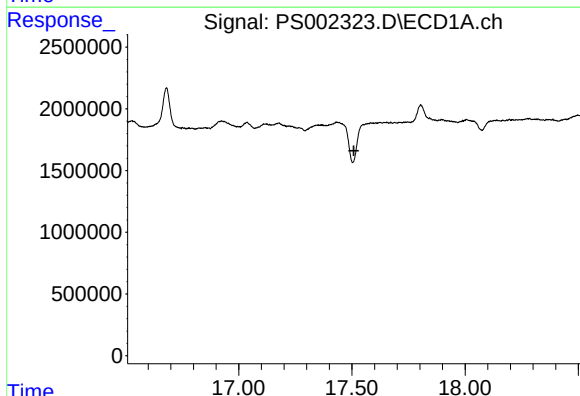

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

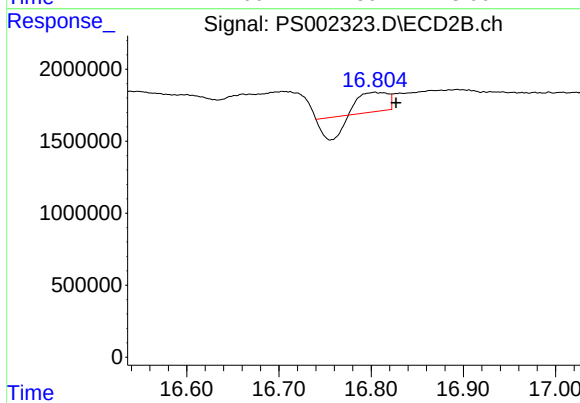

#16 DCPA

R.T.: 16.804 min
Delta R.T.: -0.023 min
Response: 989522
Conc: 0.42 ng/ml