

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
 Data File : PS002325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 04:16
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 08:02:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.448	10.939	151.5E6	149.2E6	481.423	415.508
Target Compounds							
6) T	MCP	0.000	11.481	0	114440	N.D.	0.133 #
7) T	MCPA	0.000	11.829	0	1011516	N.D.	0.747 #
8) T	DICHLORPROP	0.000	12.259	0	16334	N.D.	0.051 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110518\
Data File : PS002325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 04:16
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 08:02:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

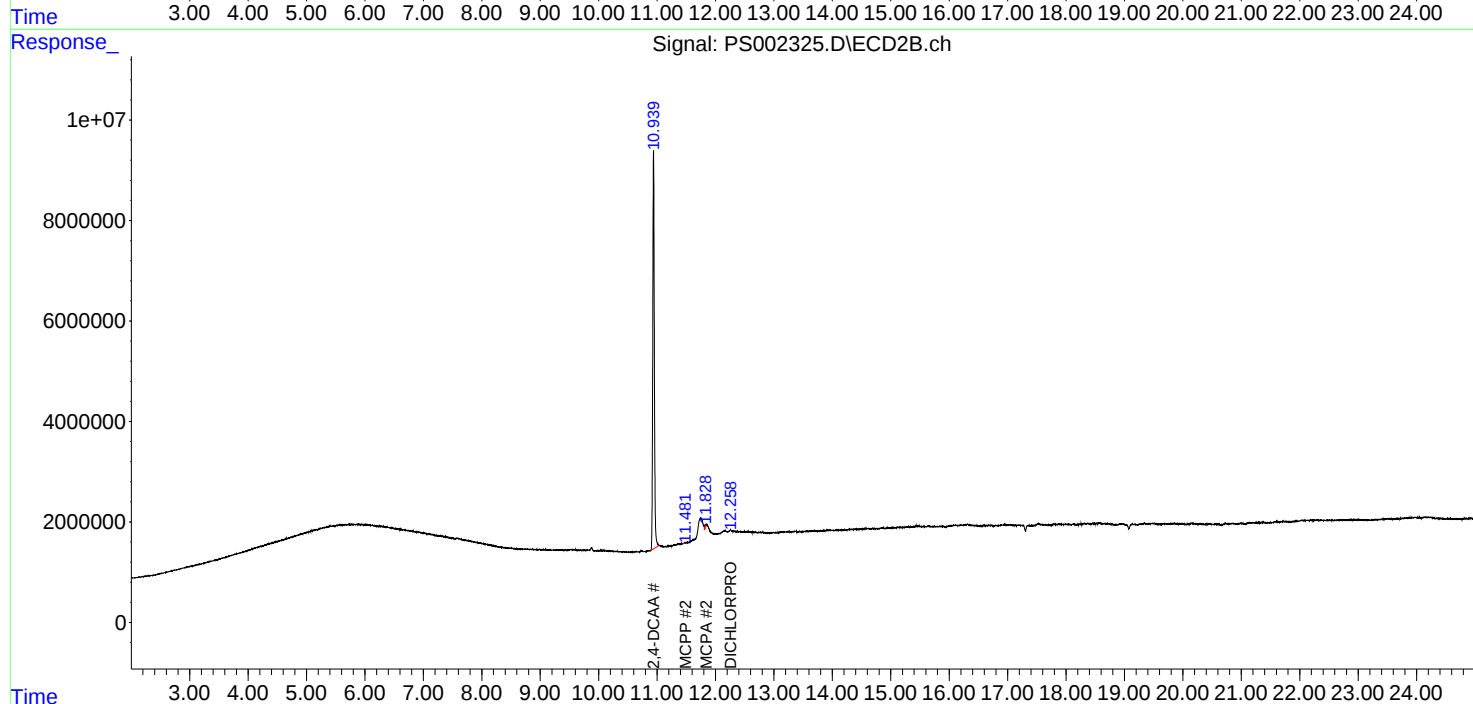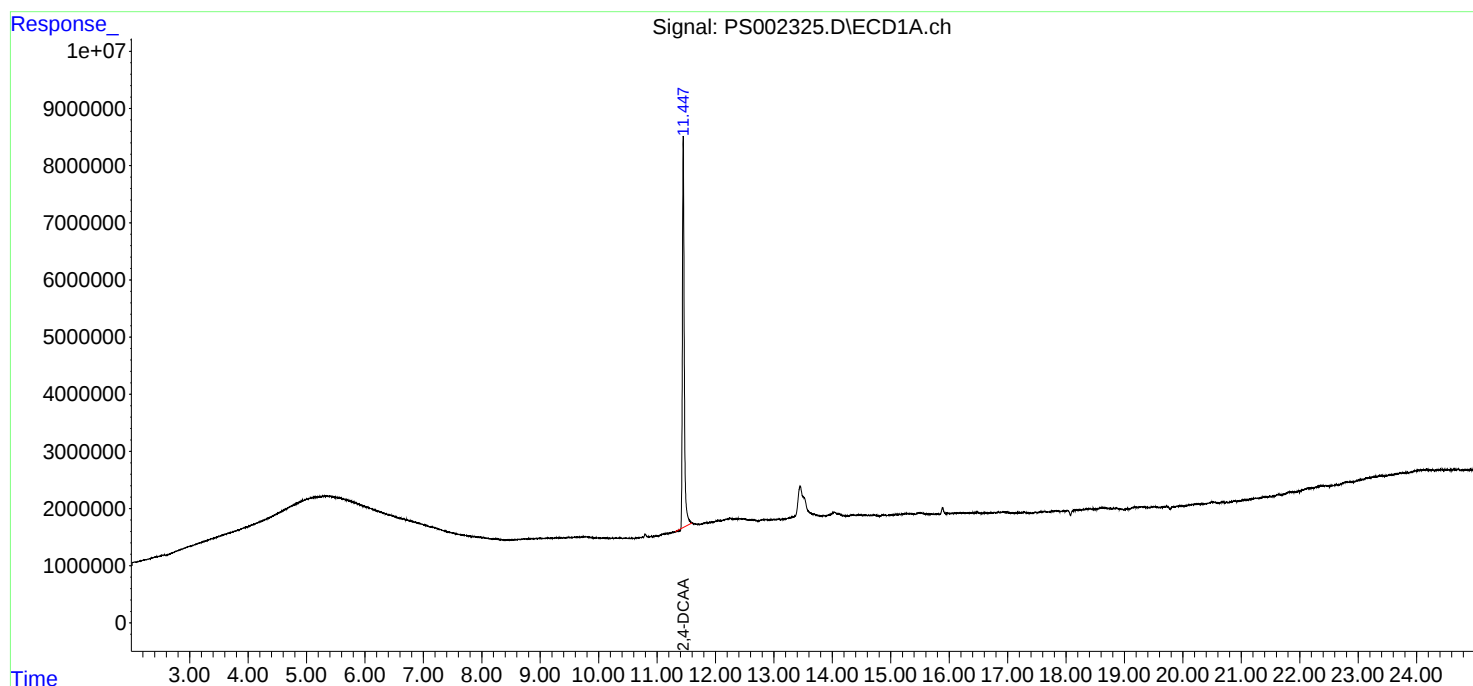


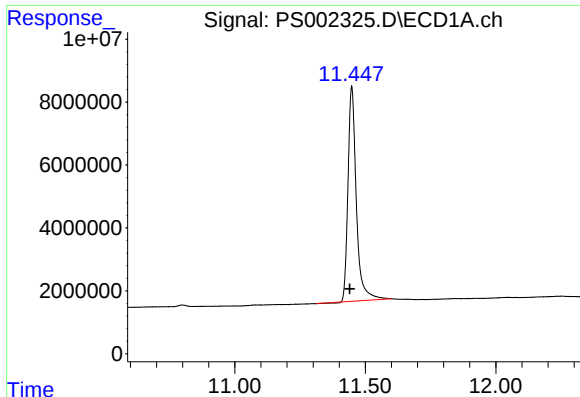

#4 2,4-DCAA


R.T.: 11.448 min
Delta R.T.: 0.007 min
Response: 151496961
Conc: 481.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

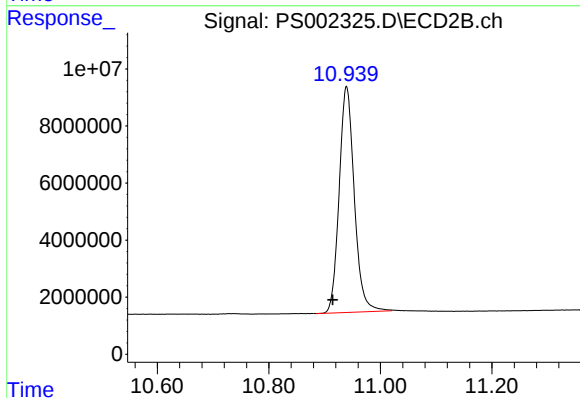


#4 2,4-DCAA

R.T.: 10.939 min
Delta R.T.: 0.025 min
Response: 149208044
Conc: 415.51 ng/ml

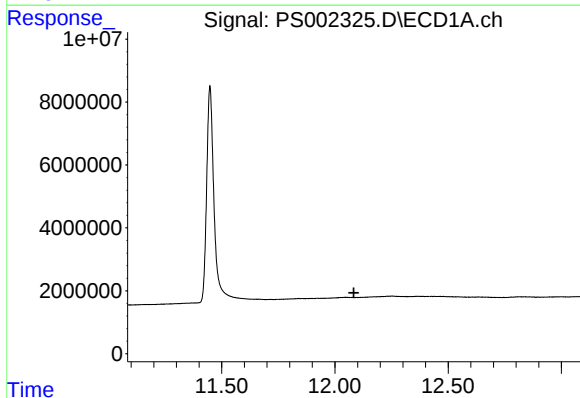


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

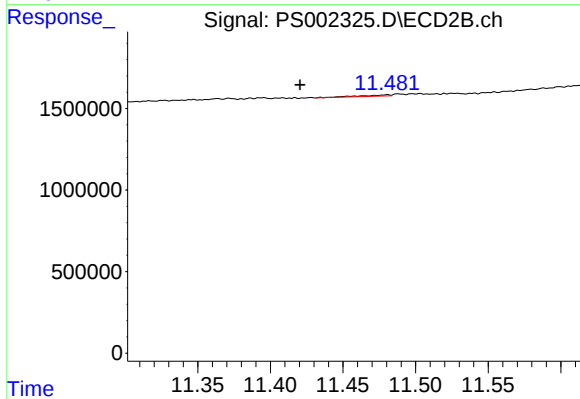

#6 MCP


R.T.: 11.481 min
Delta R.T.: 0.060 min
Response: 114440
Conc: 0.13 ug/ml

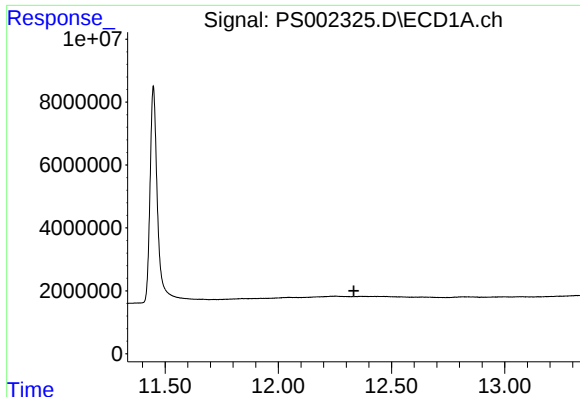

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

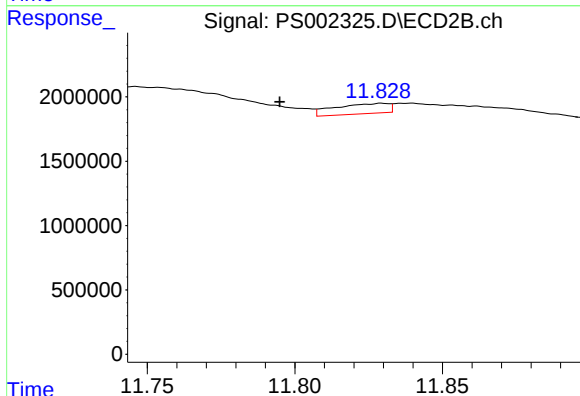


#7 MCPA

R.T.: 11.829 min
Delta R.T.: 0.034 min
Response: 1011516
Conc: 0.75 ug/ml

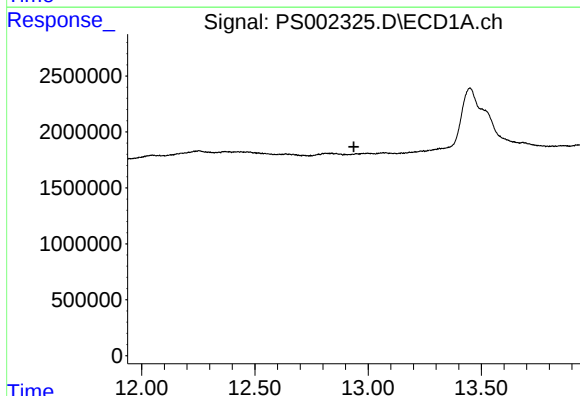

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.937 min
Response: 0
Conc: N.D.

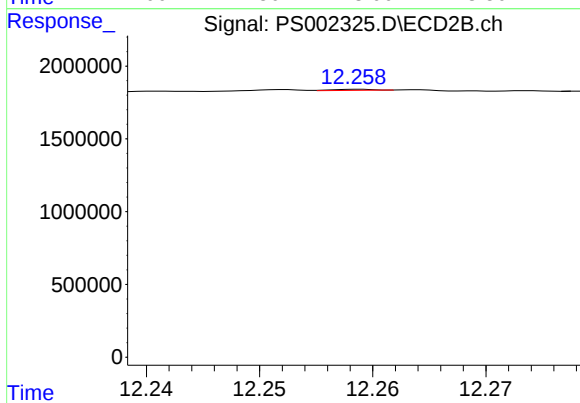

#8 DICHLORPROP

R.T.: 12.259 min
Delta R.T.: -0.061 min
Response: 16334
Conc: 0.05 ng/ml