

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110519\
 Data File : PS007615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2019 11:05
 Operator : SM\AJ
 Sample : PB124542BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 12:00:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.465	5.190	786.0E6	420.2E6	574.248	597.396
Target Compounds							
1) T	Dalapon	2.024	0.000	41501257	0	24.802	N.D. #
2) T	3,5-DICHL...	0.000	4.525	0	64343792	N.D.	74.781
5) T	DICAMBA	5.558	0.000	69091525	0	14.062	N.D. #
7) T	MCPA	0.000	5.559	0	22928435	N.D.	7.887
8) T	DICHLORPROP	0.000	5.856	0	10968112	N.D.	16.843
9) T	2,4-D	0.000	6.093	0	7024644	N.D.	8.805
10) T	Pentachlo...	0.000	6.402	0	37518305	N.D.	3.901
11) T	2,4,5-TP ...	0.000	6.793	0	10848850	N.D.	2.852
12) T	2,4,5-T	7.420	0.000	66069082	0	8.642	N.D. #
15) T	Picloram	0.000	8.946	0	26117524	N.D.	4.254



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110519\
Data File : PS007615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2019 11:05
Operator : SM\AJ
Sample : PB124542BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 12:00:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

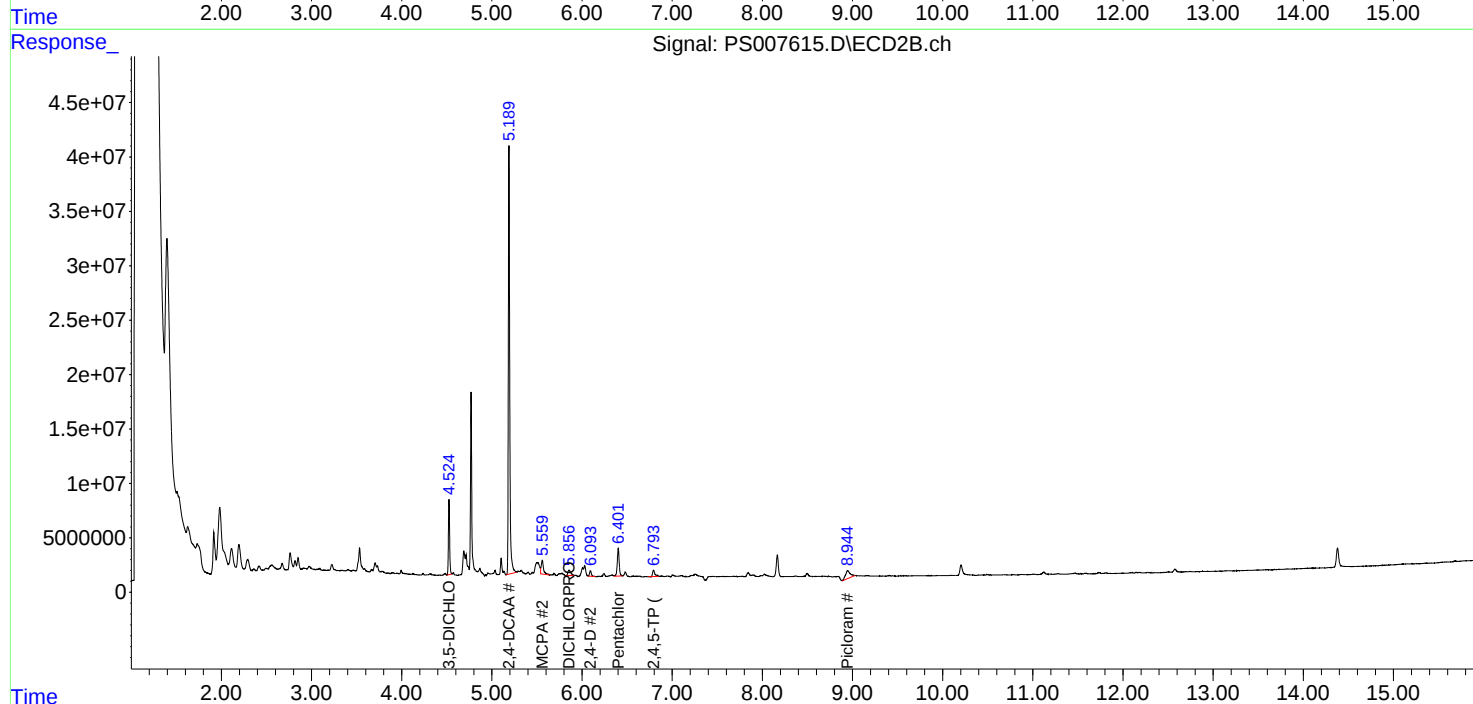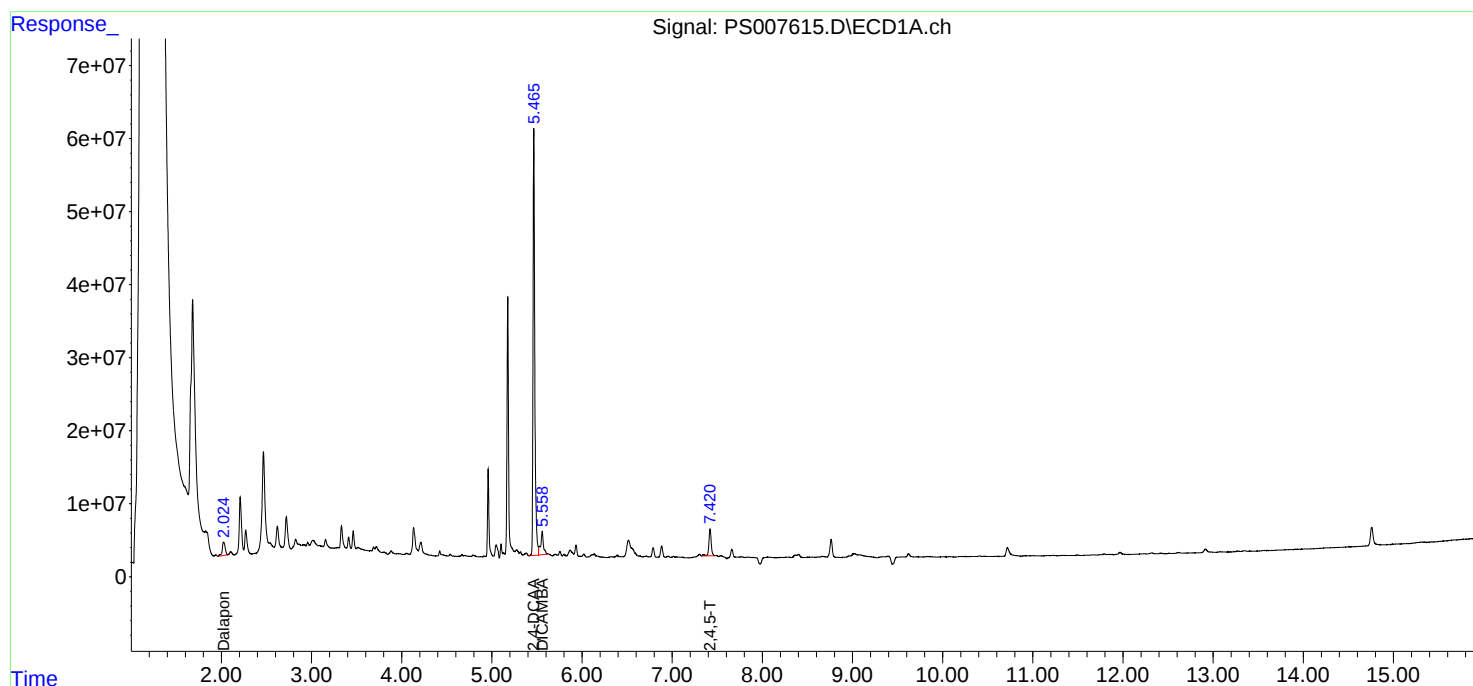


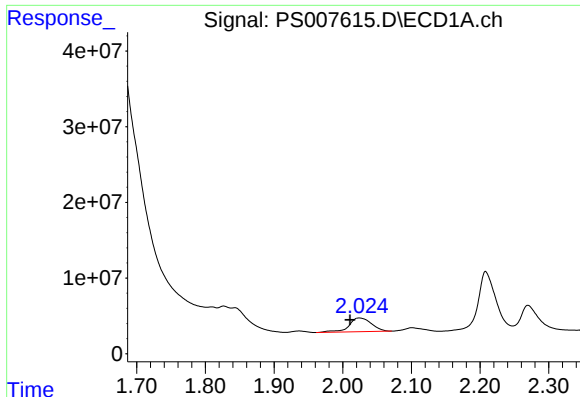

#1 Dalapon


R.T.: 2.024 min
Delta R.T.: 0.013 min
Response: 41501257
Conc: 24.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

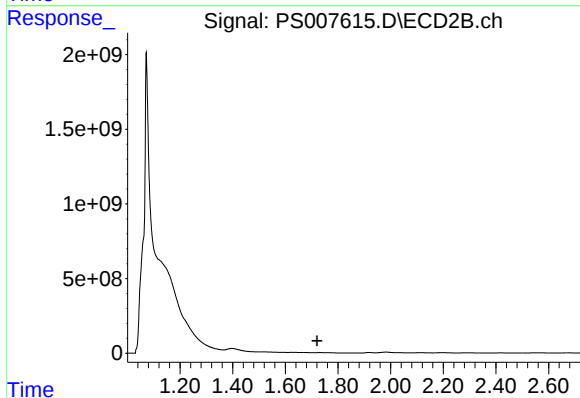


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.721 min
Response: 0
Conc: N.D.

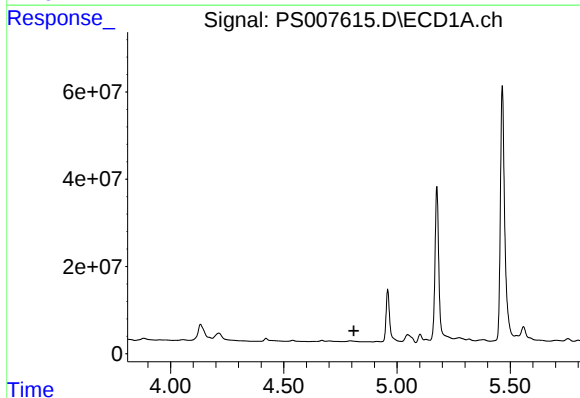


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

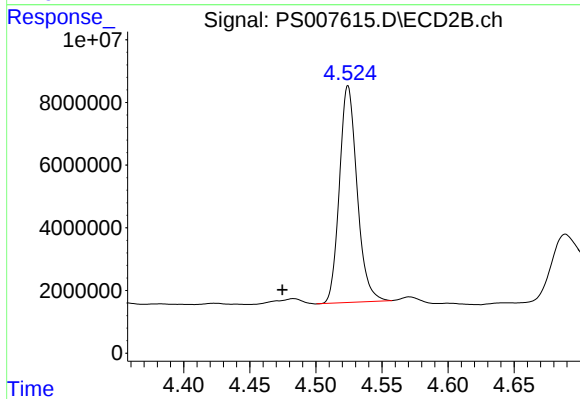

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.525 min
Delta R.T.: 0.050 min
Response: 64343792
Conc: 74.78 ng/ml

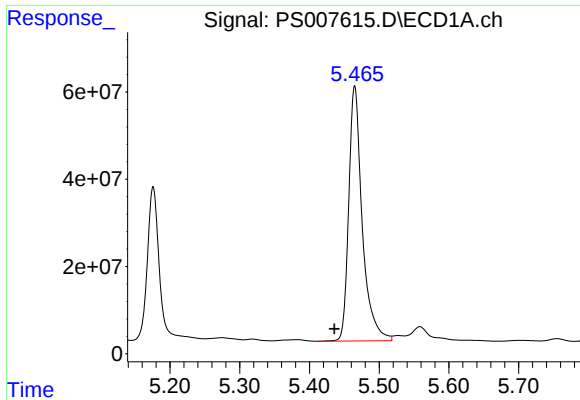

#4 2,4-DCAA


R.T.: 5.465 min
Delta R.T.: 0.029 min
Response: 785954752
Conc: 574.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

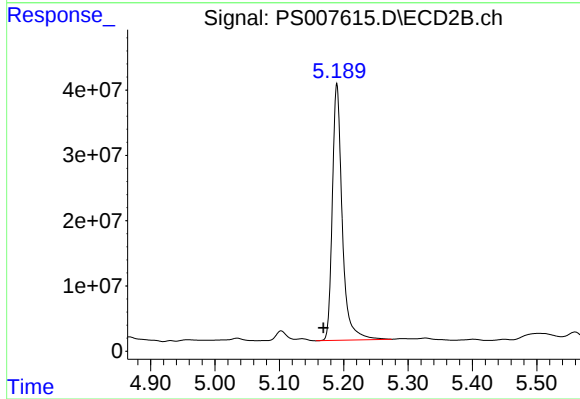


#4 2,4-DCAA

R.T.: 5.190 min
Delta R.T.: 0.021 min
Response: 420152228
Conc: 597.40 ng/ml

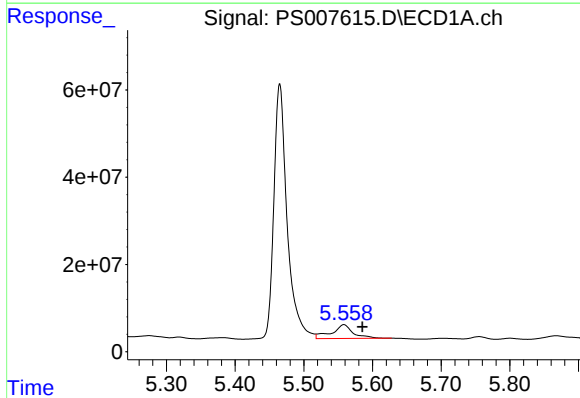


#5 DICAMBA

R.T.: 5.558 min
Delta R.T.: -0.027 min
Response: 69091525
Conc: 14.06 ng/ml

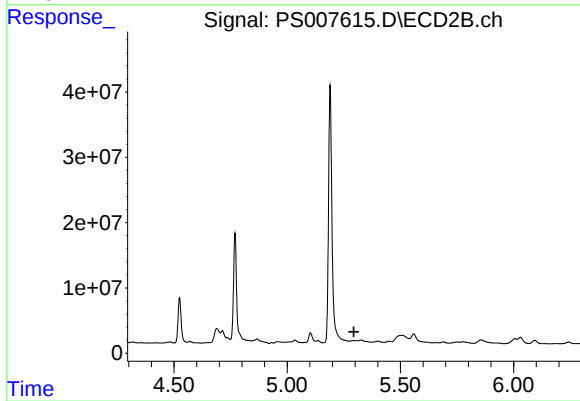

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

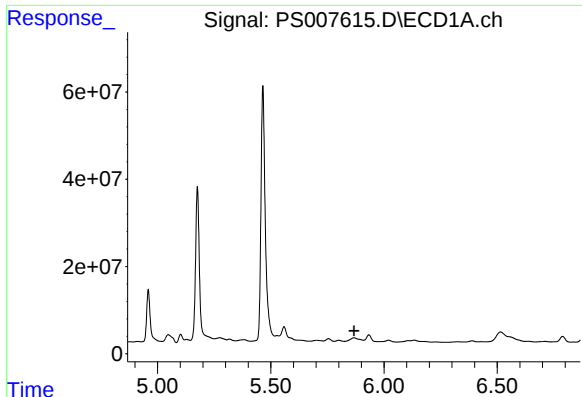

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

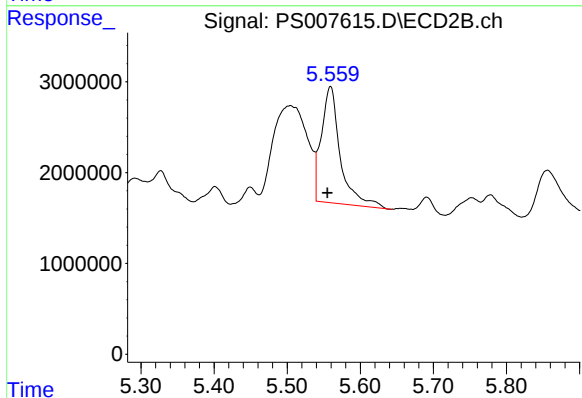


#7 MCPA

R.T.: 5.559 min
Delta R.T.: 0.004 min
Response: 22928435
Conc: 7.89 ug/ml

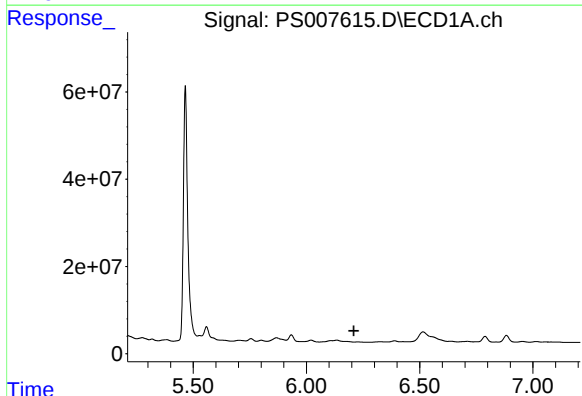


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

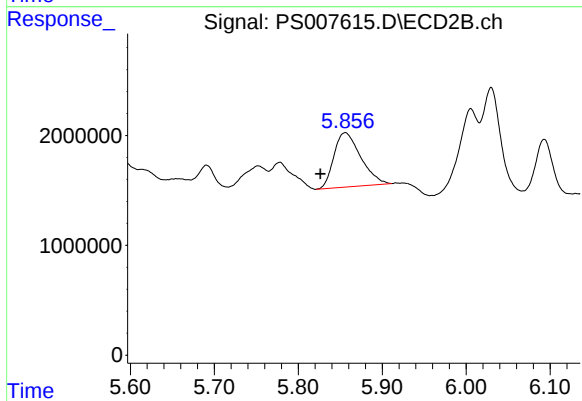

#8 DICHLORPROP


R.T.: 5.856 min
Delta R.T.: 0.030 min
Response: 10968112
Conc: 16.84 ng/ml

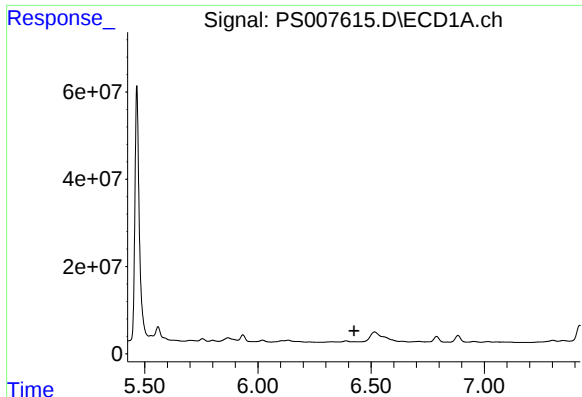

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

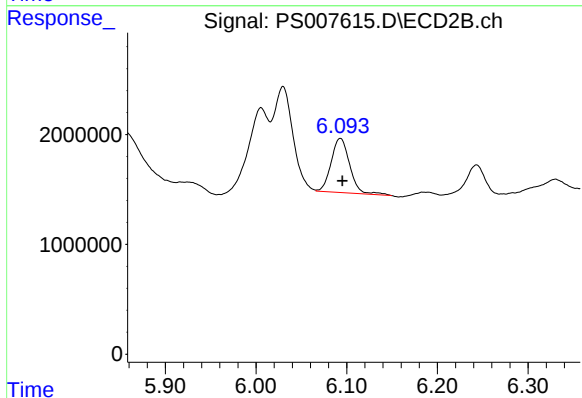


#9 2,4-D

R.T.: 6.093 min
Delta R.T.: -0.002 min
Response: 7024644
Conc: 8.81 ng/ml

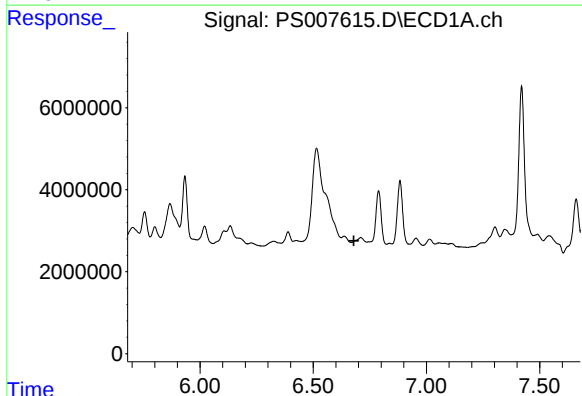


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

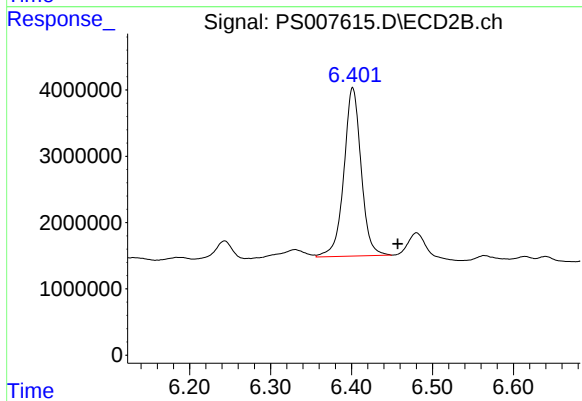

#10 Pentachlorophenol


R.T.: 6.402 min
Delta R.T.: -0.056 min
Response: 37518305
Conc: 3.90 ng/ml

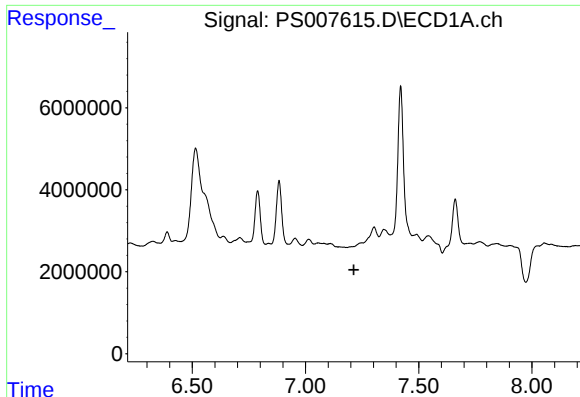

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

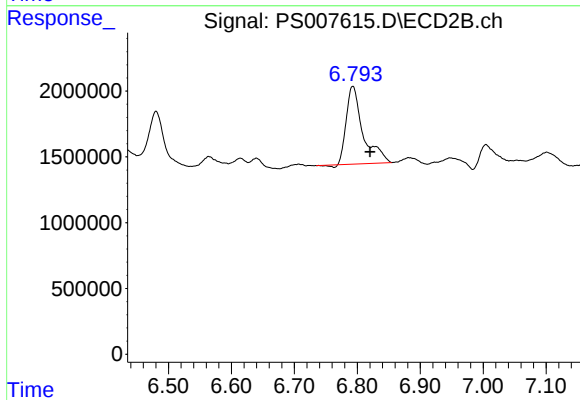


#11 2,4,5-TP (SILVEX)

R.T.: 6.793 min
Delta R.T.: -0.028 min
Response: 10848850
Conc: 2.85 ng/ml

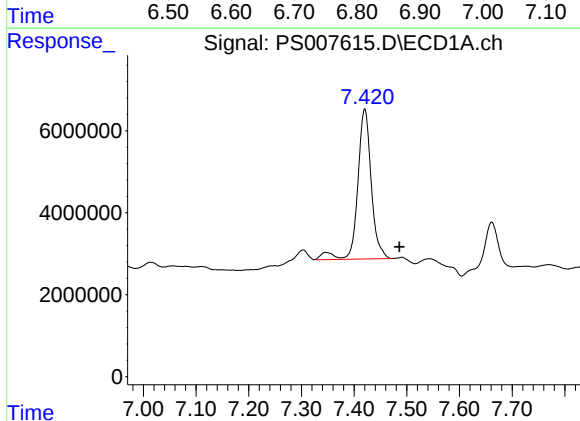


#12 2,4,5-T

R.T.: 7.420 min
Delta R.T.: -0.066 min
Response: 66069082
Conc: 8.64 ng/ml

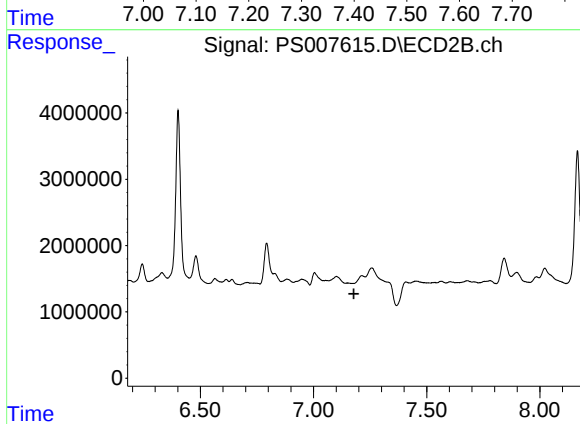

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.

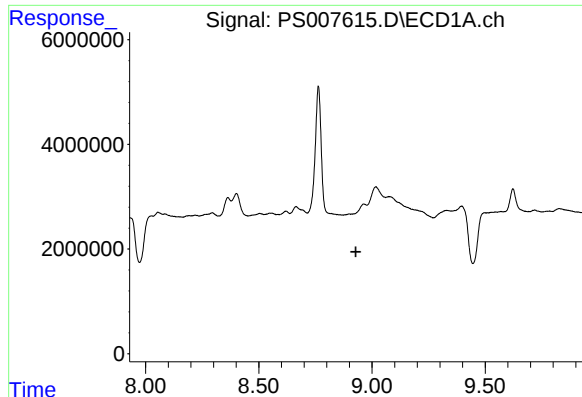

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

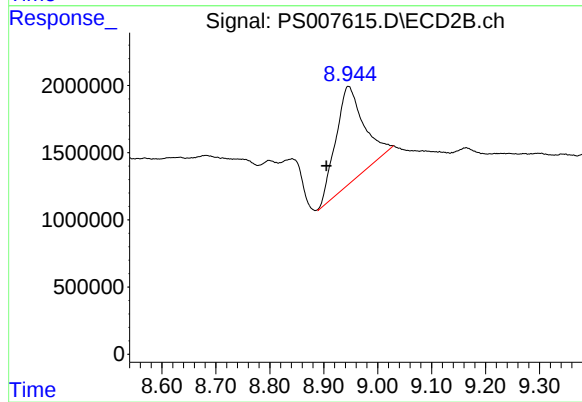

#15 Picloram

R.T.: 8.946 min
Delta R.T.: 0.041 min
Response: 26117524
Conc: 4.25 ng/ml