

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
 Data File : PS028216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 16:59
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:19:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 00:14:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	2.626f	0.000	714099	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.418	0.000	41732010	0	14.890	N.D. #
3) T	4-Nitroph...	7.050	0.000	5597405	0	4.723	N.D. #
6) T	MCP	0.000	8.080	0	18222512	N.D.	3.521
7) T	MCPA	0.000	8.292f	0	8346447	N.D.	1.164
8) T	DICHLORPROP	8.124f	0.000	962047	0	<MDL	N.D. #
9) T	2,4-D	8.417	0.000	109.7E6	0	54.110	N.D. #
10) T	Pentachlo...	8.736f	0.000	1341567	0	<MDL	N.D. #
14) T	DINOSEB	11.359	0.000	122796	0	<MDL	N.D. #
15) T	Picloram	11.147f	12.395	26627142	31574407	1.526	1.923 #
16) T	DCPA	11.655	0.000	721261	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
Data File : PS028216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 16:59
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:19:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 00:14:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

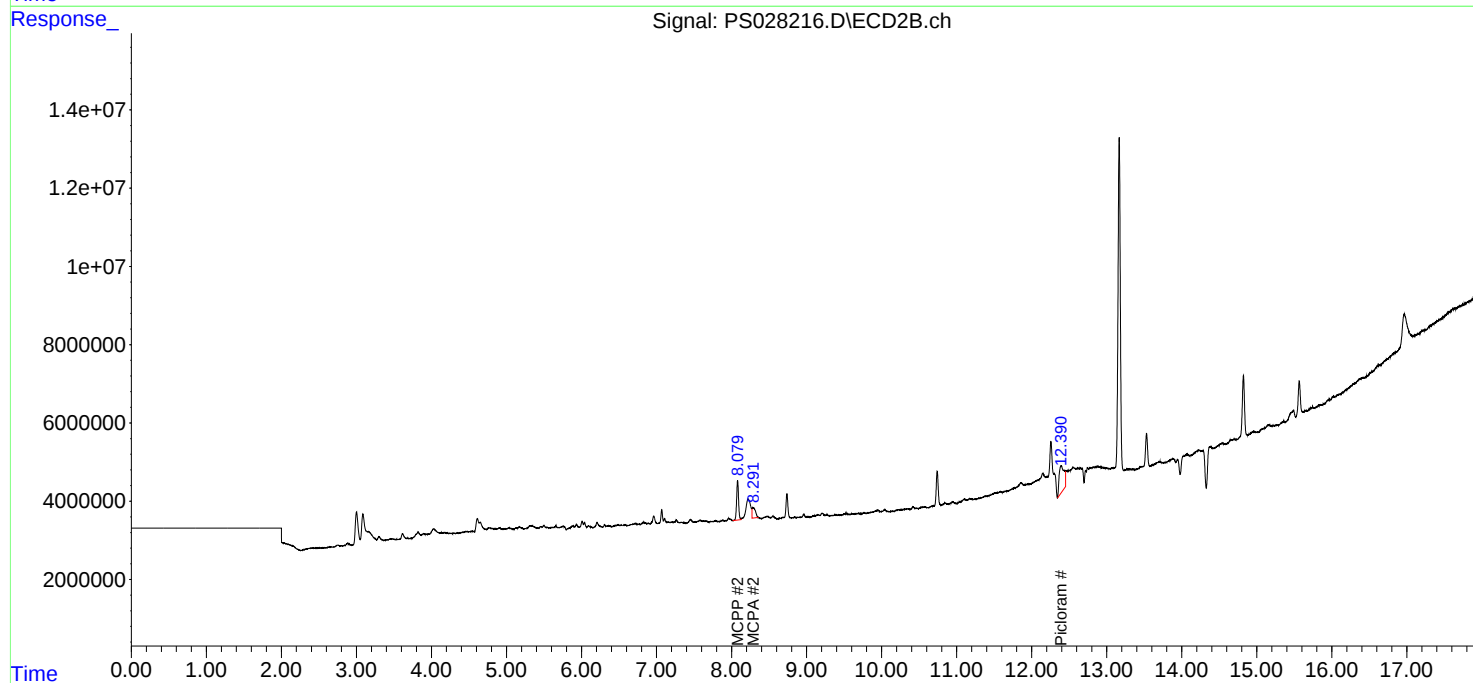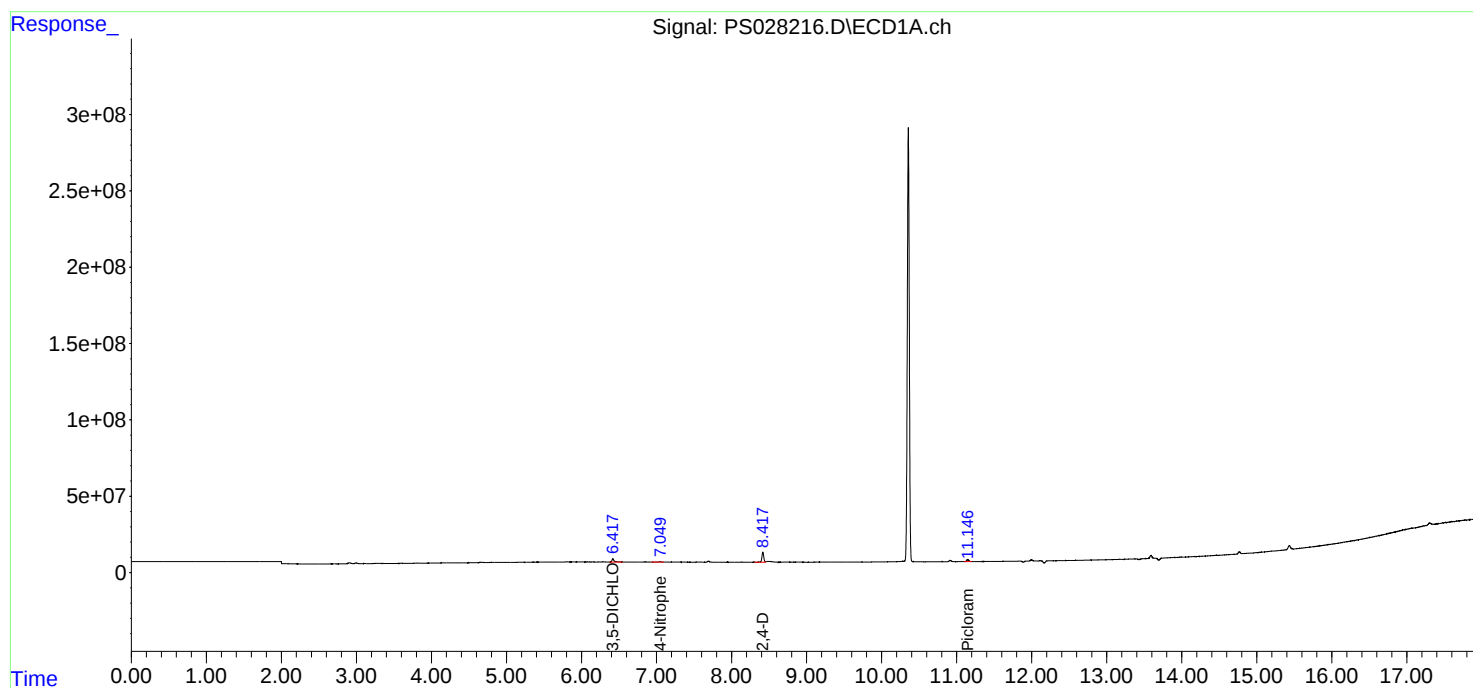


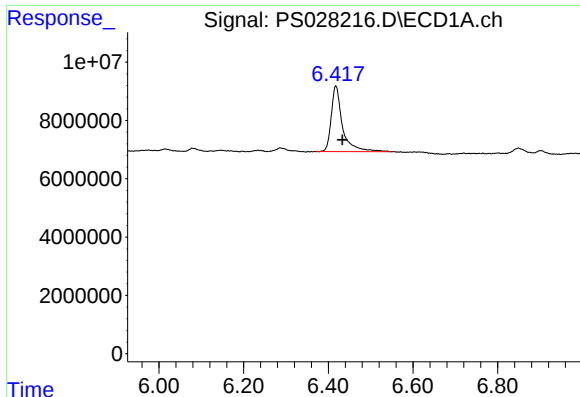

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.418 min
Delta R.T.: -0.015 min
Response: 41732010
Conc: 14.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

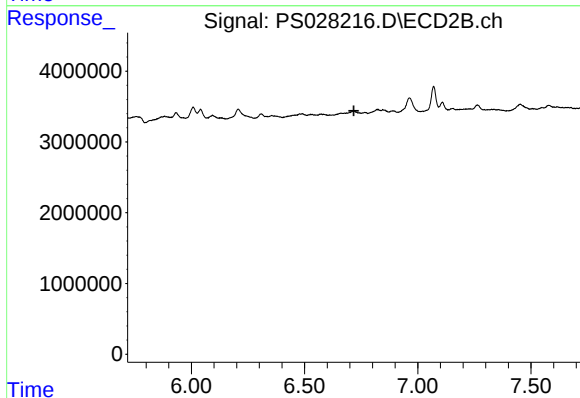


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.718 min
Response: 0
Conc: N.D.

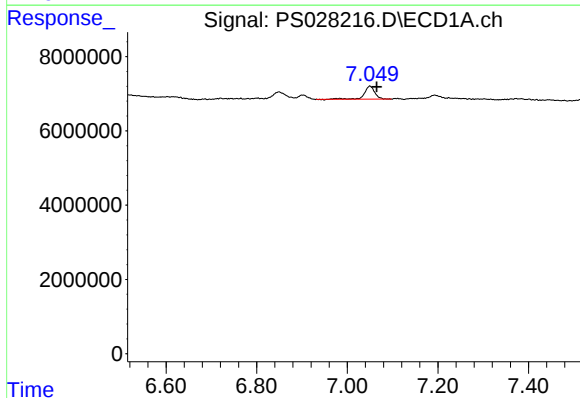


#3 4-Nitrophenol

R.T.: 7.050 min
Delta R.T.: -0.015 min
Response: 5597405
Conc: 4.72 ng/ml

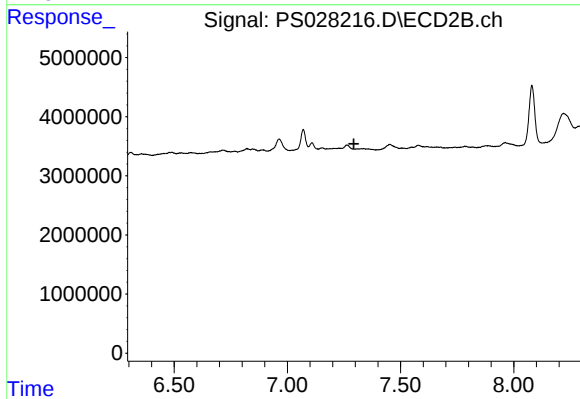

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.293 min
Response: 0
Conc: N.D.

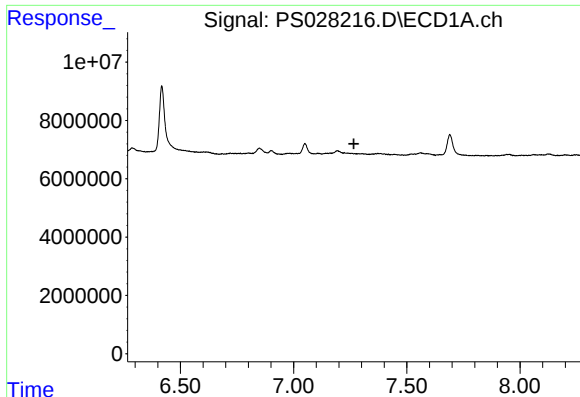

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

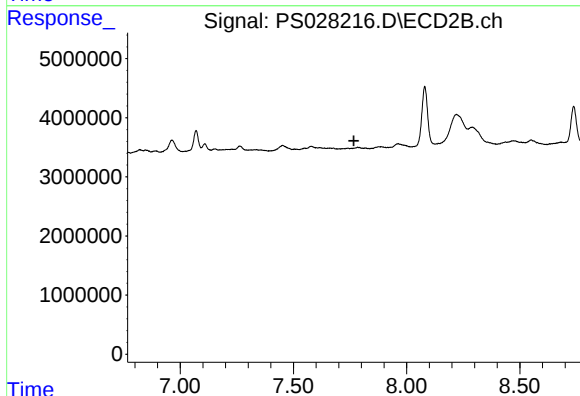


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.767 min
Response: 0
Conc: N.D.

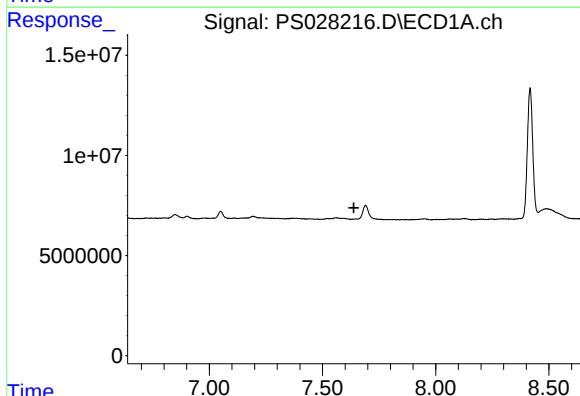


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.639 min
Response: 0
Conc: N.D.

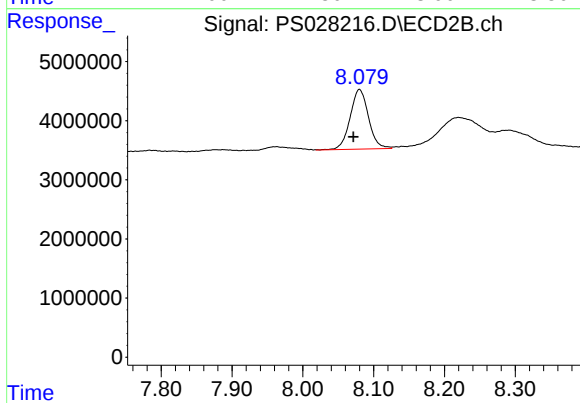

#6 MCPP


R.T.: 8.080 min
Delta R.T.: 0.008 min
Response: 18222512
Conc: 3.52 ug/ml

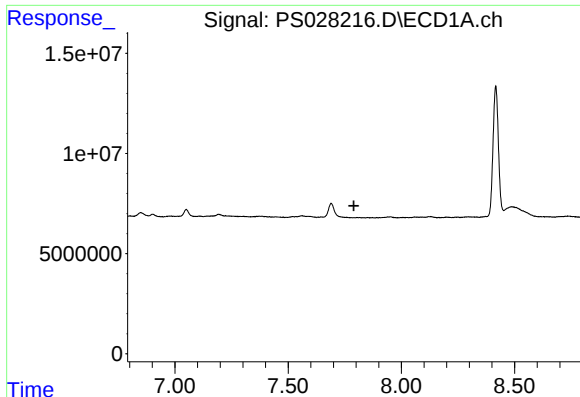

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

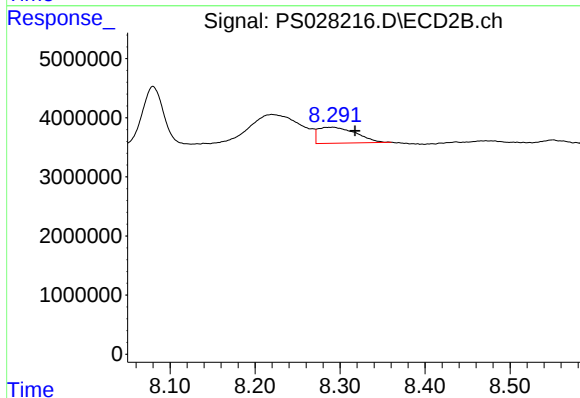


#7 MCPA

R.T.: 8.292 min
Delta R.T.: -0.026 min
Response: 8346447
Conc: 1.16 ug/ml

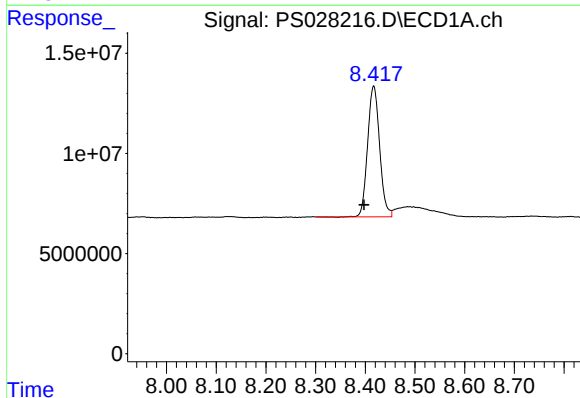


#9 2,4-D

R.T.: 8.417 min
Delta R.T.: 0.019 min
Response: 109703599
Conc: 54.11 ng/ml

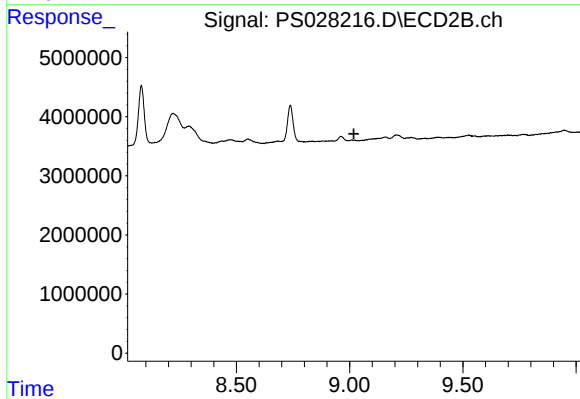

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 9.019 min
Response: 0
Conc: N.D.

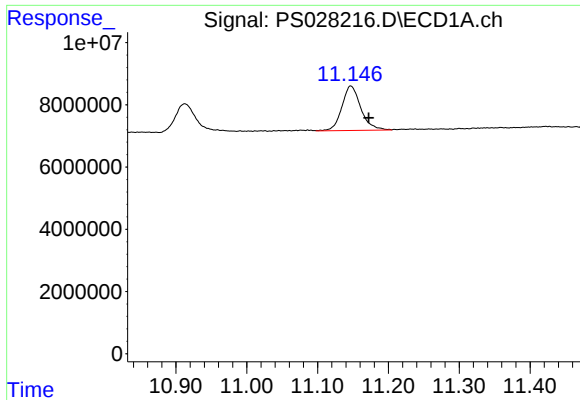

#15 Picloram

R.T.: 11.147 min
Delta R.T.: -0.025 min
Response: 26627142
Conc: 1.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

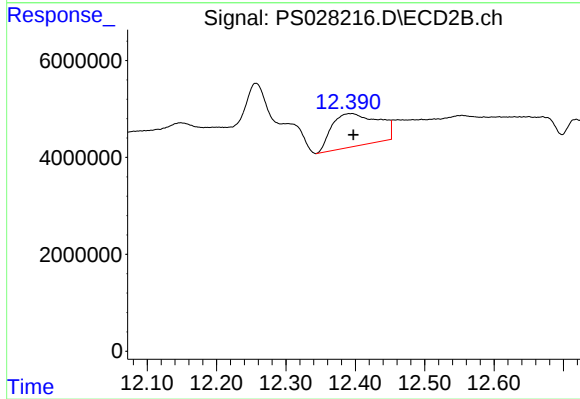

#15 Picloram

R.T.: 12.395 min
Delta R.T.: -0.002 min
Response: 31574407
Conc: 1.92 ng/ml