

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
 Data File : PS028224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 20:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:30:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 00:14:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.265	7.768	875.6E6	874.0E6	485.632	558.891
Target Compounds							
1) T	Dalapon	2.698f	0.000	1252391	0	<MDL	N.D. #
3) T	4-Nitroph...	7.057	0.000	3204066	0	2.703	N.D. #
6) T	MCP	0.000	8.117f	0	31550024	N.D.	6.097
7) T	MCPA	0.000	8.288f	0	14926553	N.D.	2.081
8) T	DICHLORPROP	8.166	0.000	289632	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.947	0	14087174	N.D.	1.310
14) T	DINOSEB	11.342f	0.000	1417910	0	<MDL	N.D. #
15) T	Picloram	11.162	12.394	21211684	22478542	1.216	1.369
16) T	DCPA	11.643	0.000	2300458	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
Data File : PS028224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 20:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:30:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 00:14:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

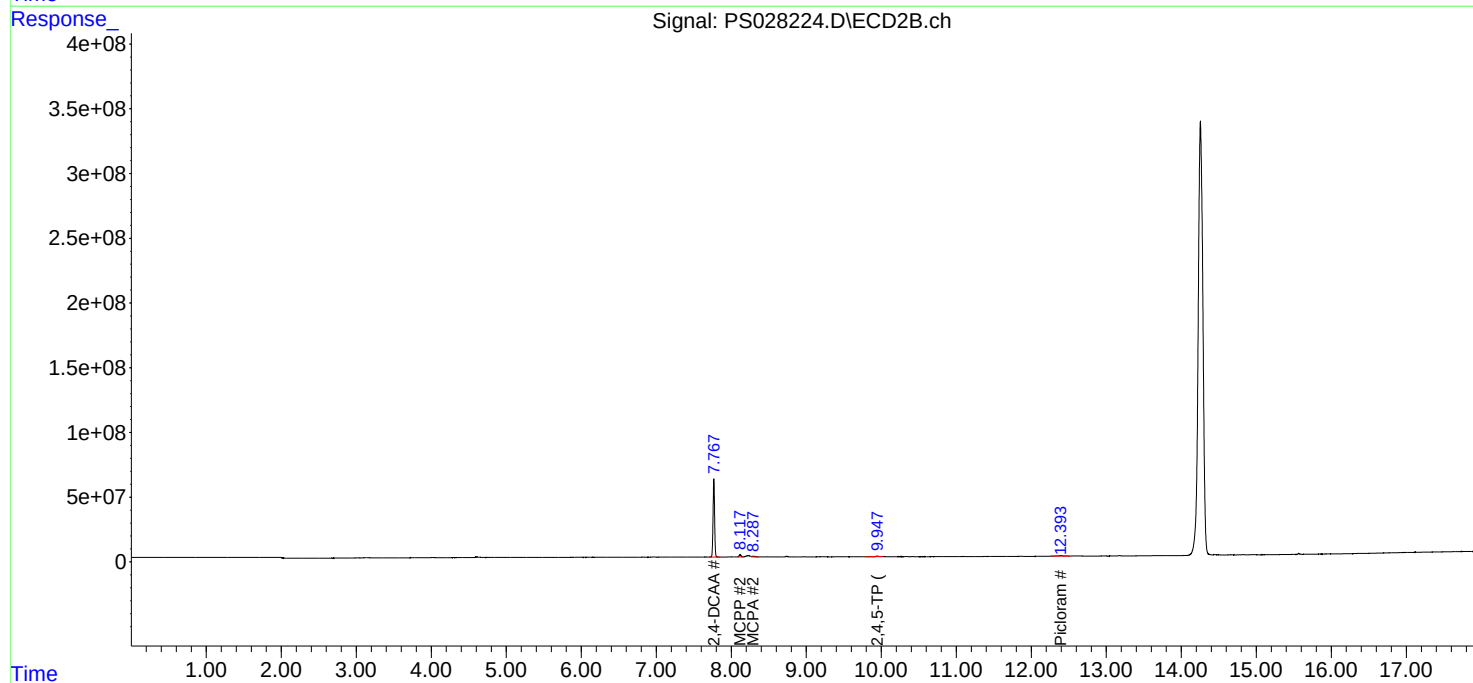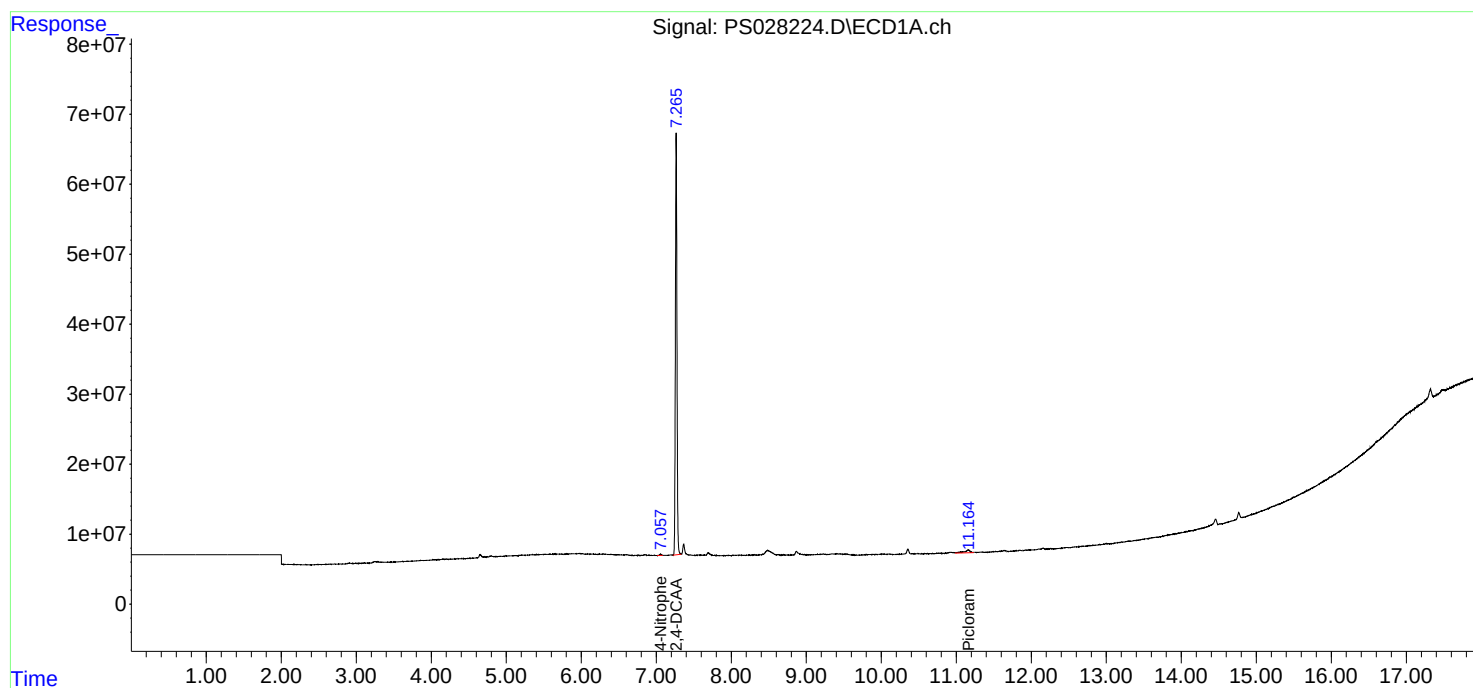


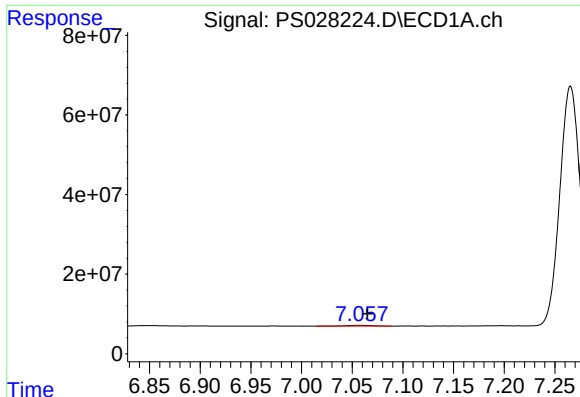

#3 4-Nitrophenol


R.T.: 7.057 min
Delta R.T.: -0.008 min
Response: 3204066
Conc: 2.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

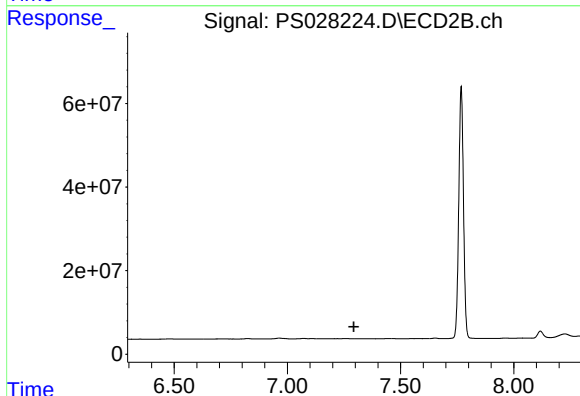


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.293 min
Response: 0
Conc: N.D.

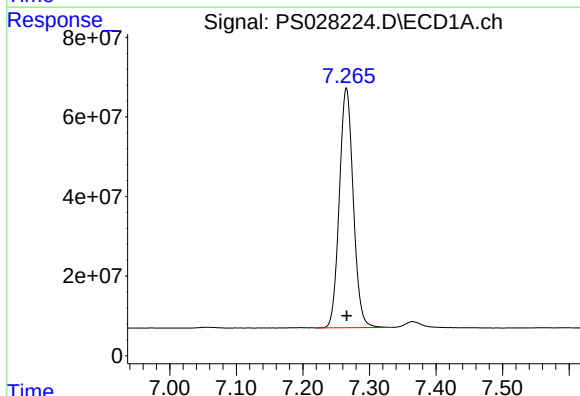


#4 2,4-DCAA

R.T.: 7.265 min
Delta R.T.: 0.000 min
Response: 875609670
Conc: 485.63 ng/ml

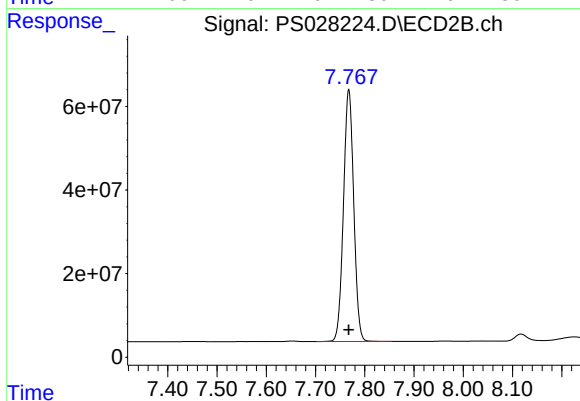

#4 2,4-DCAA


R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 874043936
Conc: 558.89 ng/ml

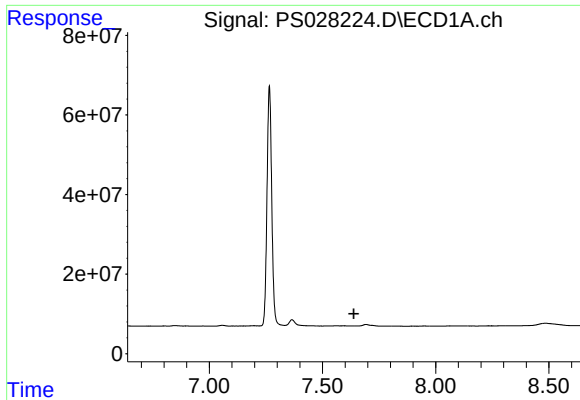

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.639 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

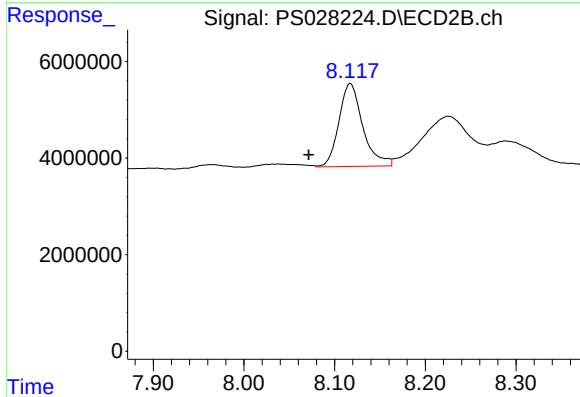


#6 MCPP

R.T.: 8.117 min
Delta R.T.: 0.046 min
Response: 31550024
Conc: 6.10 ug/ml

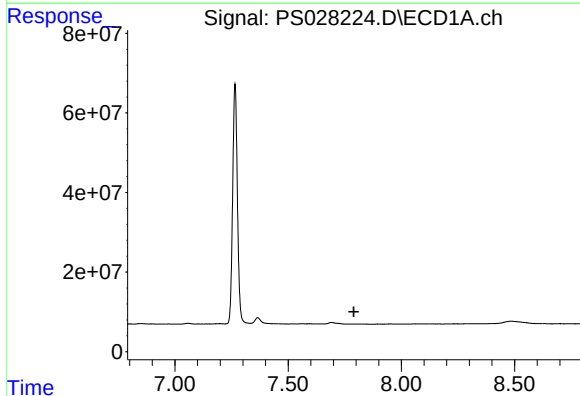


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.790 min
Response: 0
Conc: N.D.

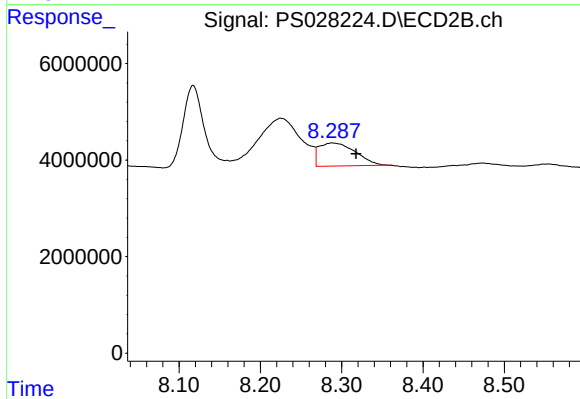

#7 MCPA


R.T.: 8.288 min
Delta R.T.: -0.029 min
Response: 14926553
Conc: 2.08 ug/ml

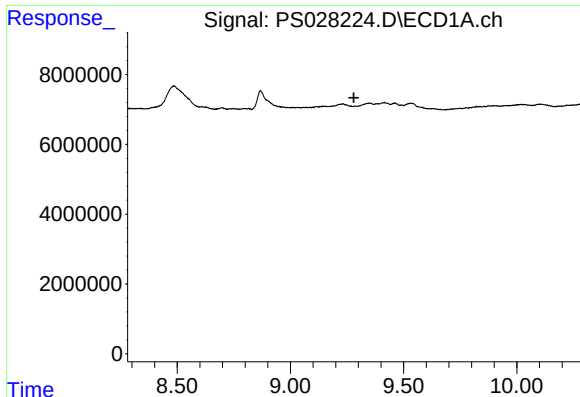

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

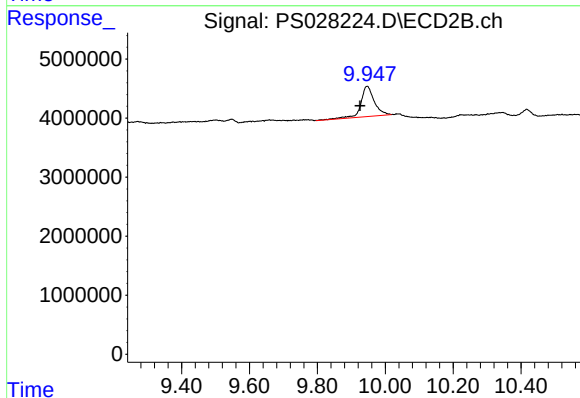


#11 2,4,5-TP (SILVEX)

R.T.: 9.947 min
Delta R.T.: 0.021 min
Response: 14087174
Conc: 1.31 ng/ml

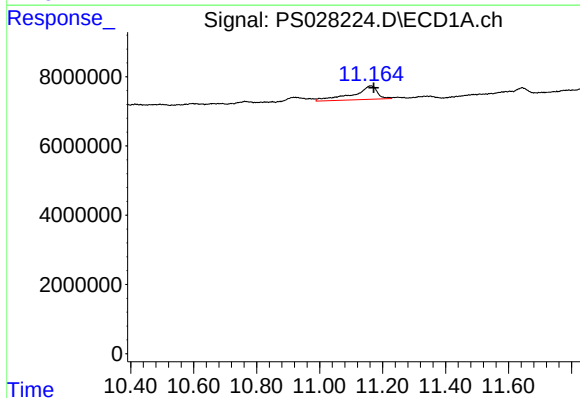

#15 Picloram

R.T.: 11.162 min
Delta R.T.: -0.010 min
Response: 21211684
Conc: 1.22 ng/ml

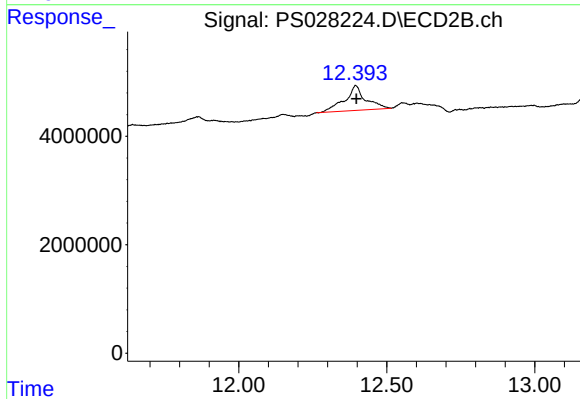

#15 Picloram

R.T.: 12.394 min
Delta R.T.: -0.003 min
Response: 22478542
Conc: 1.37 ng/ml