

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
 Data File : PS028237-2.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 03:48
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 03:40:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 00:14:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.264	7.767	1901.3E6	1203.7E6	1054.507	769.689 #
Target Compounds							
1) T	Dalapon	2.656	2.713	2304.6E6	1993.4E6	723.404	720.260
2) T	3,5-DICHL...	6.432	6.717	2335.7E6	1686.2E6	833.405	719.698
3) T	4-Nitroph...	7.064	7.293	990.3E6	746.5E6	835.538	705.193
5) T	DICAMBA	7.454	7.968	7091.3E6	5287.3E6	897.789	733.038
6) T	MCPD	7.638	8.070	490.6E6	387.4E6	89.093	74.860
7) T	MCPA	7.789	8.316	670.8E6	519.5E6	82.704	72.431
8) T	DICHLORPROP	8.165	8.686	1700.6E6	1265.9E6	941.333	727.230
9) T	2,4-D	8.396	9.018	1925.8E6	1417.3E6	949.862	726.858
10) T	Pentachlo...	8.696	9.549	26537.6E6	19016.9E6	992.208	735.089 #
11) T	2,4,5-TP ...	9.279	9.925	10458.4E6	7868.5E6	1044.870	731.799 #
12) T	2,4,5-T	9.571	10.347	10682.6E6	7810.2E6	1045.568	730.056 #
13) T	2,4-DB	10.149	10.914	1748.6E6	998.0E6	1060.337	720.013 #
14) T	DINOSEB	11.367	11.295	8716.1E6	5501.1E6	1160.054	733.360 #
15) T	Picloram	11.171	12.396	18609.3E6	12023.0E6	1066.472	732.319 #
16) T	DCPA	11.659	12.342	14794.7E6	9021.2E6	1188.342	715.756 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
Data File : PS028237-2.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 03:48
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 03:40:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 00:14:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

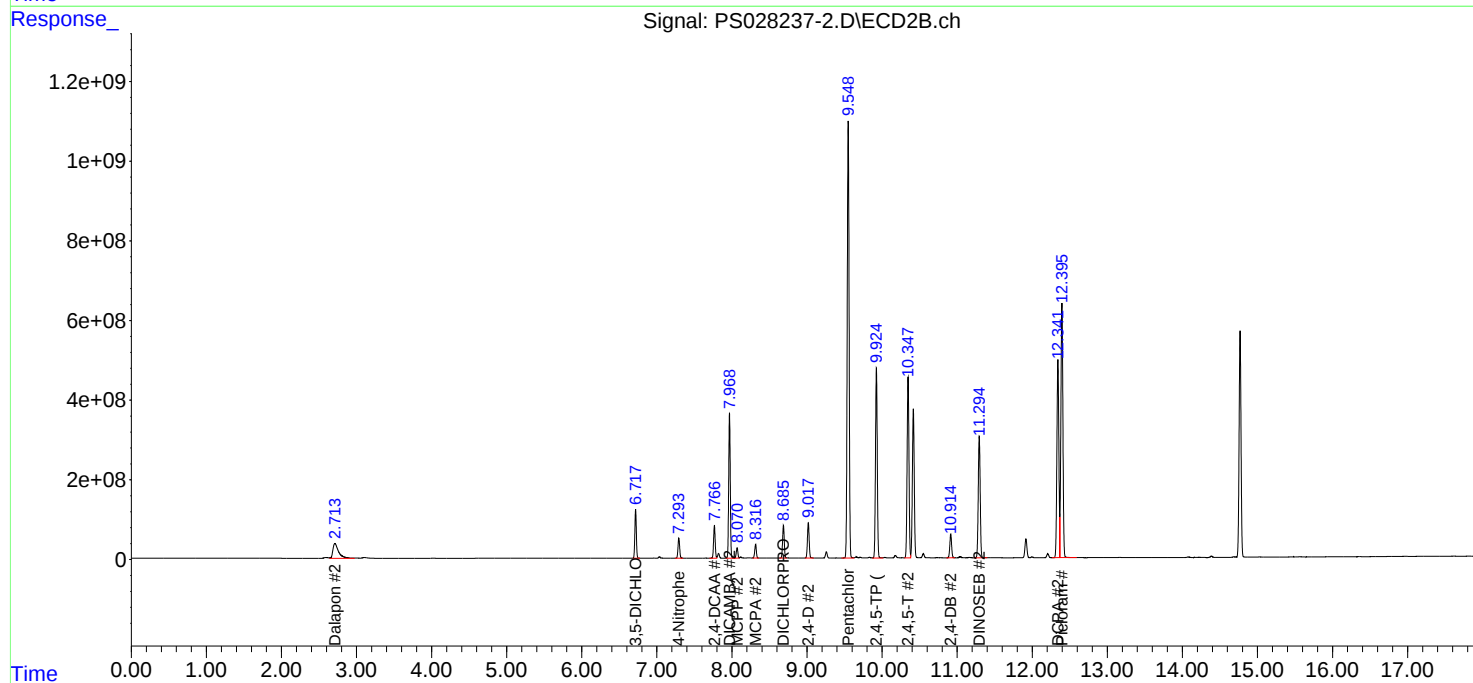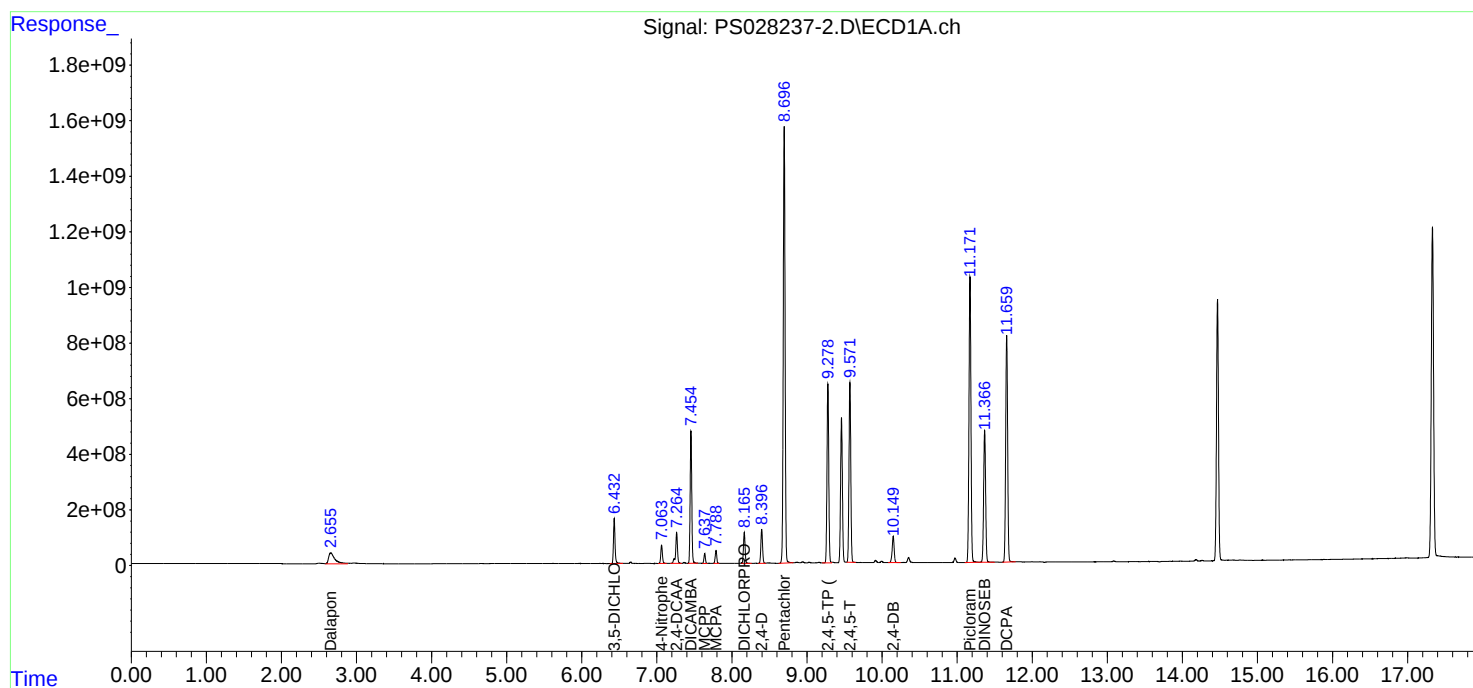


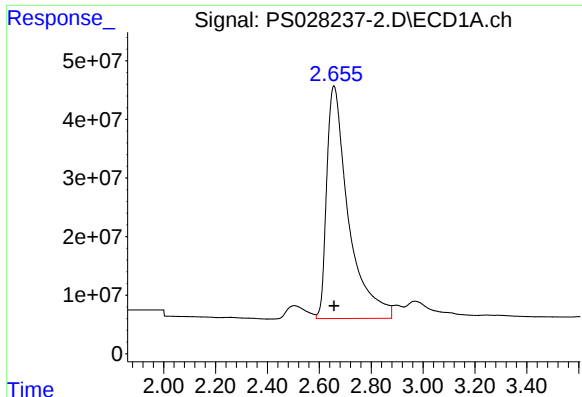

#1 Dalapon


R.T.: 2.656 min
Delta R.T.: 0.000 min
Response: 2304559005
Conc: 723.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

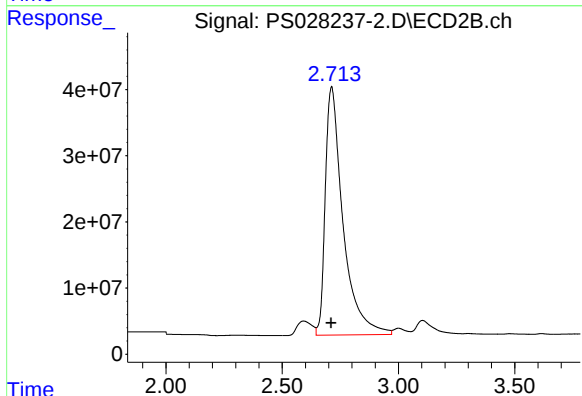


#1 Dalapon

R.T.: 2.713 min
Delta R.T.: 0.002 min
Response: 1993396571
Conc: 720.26 ng/ml

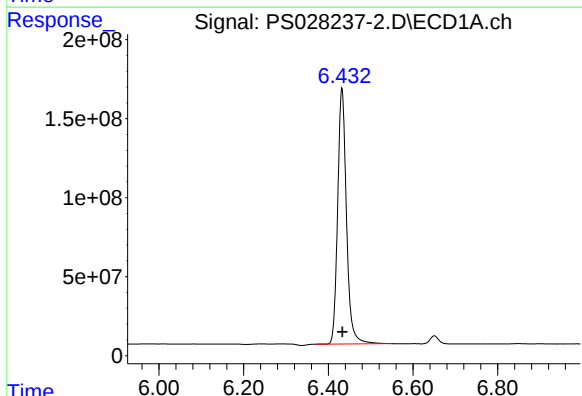


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.432 min
Delta R.T.: 0.000 min
Response: 2335724003
Conc: 833.40 ng/ml

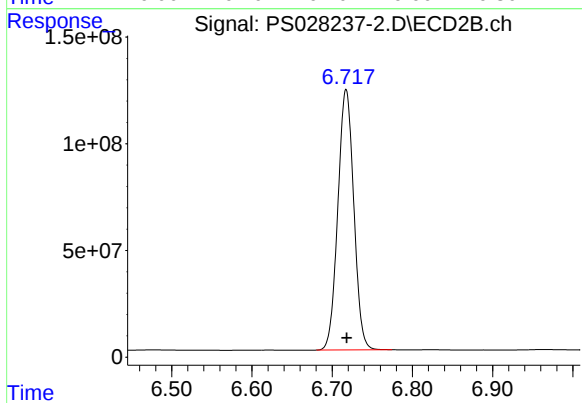

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 1686238221
Conc: 719.70 ng/ml

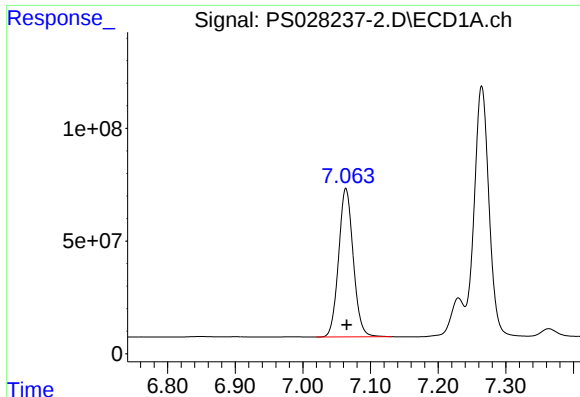

#3 4-Nitrophenol


R.T.: 7.064 min
Delta R.T.: -0.001 min
Response: 990294598
Conc: 835.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

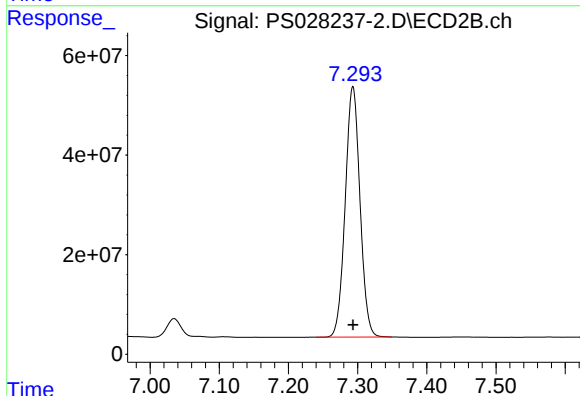


#3 4-Nitrophenol

R.T.: 7.293 min
Delta R.T.: 0.000 min
Response: 746507599
Conc: 705.19 ng/ml

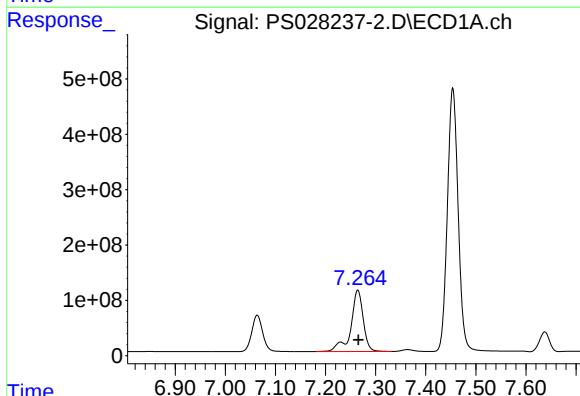


#4 2,4-DCAA

R.T.: 7.264 min
Delta R.T.: -0.002 min
Response: 1901309639
Conc: 1054.51 ng/ml

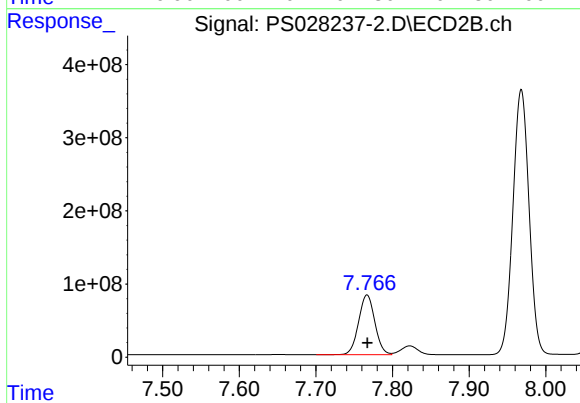

#4 2,4-DCAA


R.T.: 7.767 min
Delta R.T.: 0.000 min
Response: 1203707755
Conc: 769.69 ng/ml

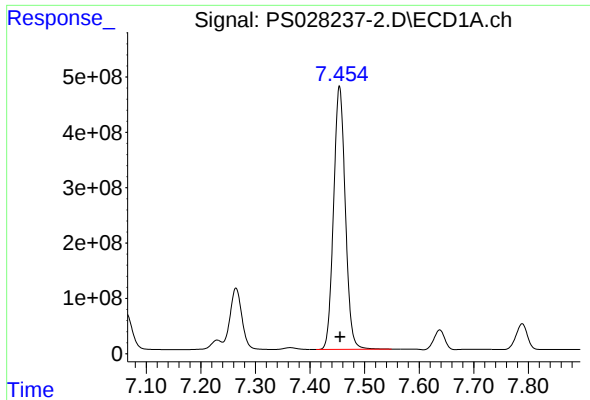

#5 DICAMBA


R.T.: 7.454 min
Delta R.T.: -0.001 min
Response: 7091252824
Conc: 897.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

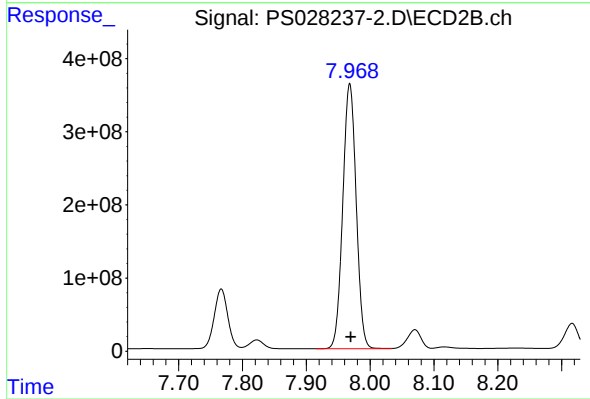


#5 DICAMBA

R.T.: 7.968 min
Delta R.T.: -0.001 min
Response: 5287268206
Conc: 733.04 ng/ml

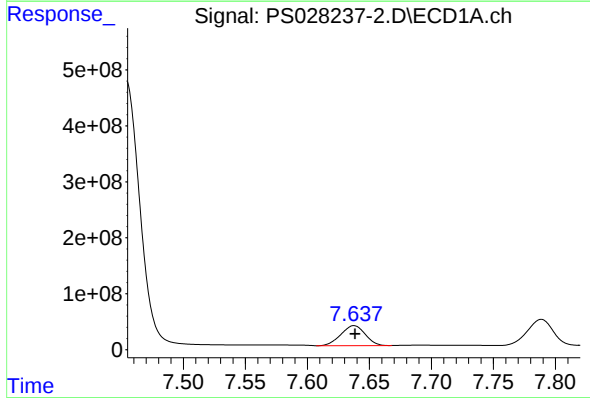


#6 MCP

R.T.: 7.638 min
Delta R.T.: 0.000 min
Response: 490633781
Conc: 89.09 ug/ml

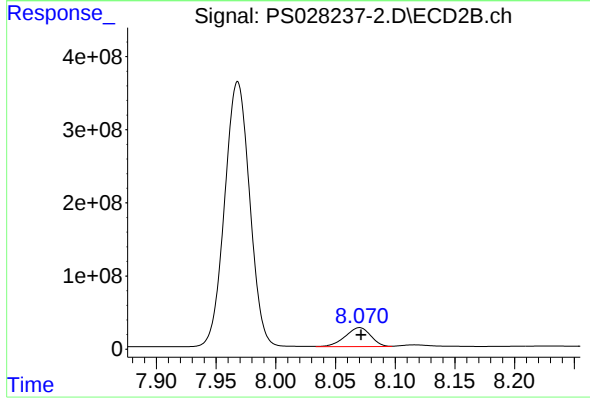

#6 MCP


R.T.: 8.070 min
Delta R.T.: -0.001 min
Response: 387378057
Conc: 74.86 ug/ml

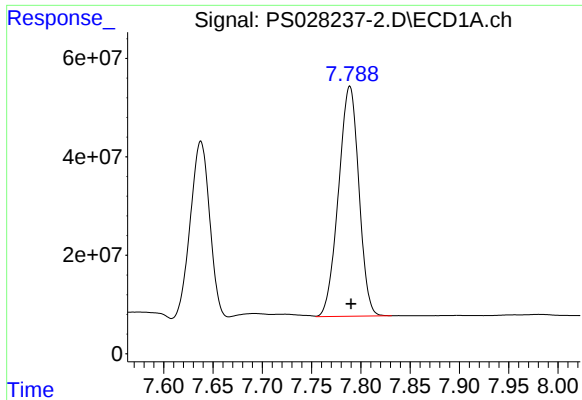

#7 MCPA


R.T.: 7.789 min
Delta R.T.: -0.001 min
Response: 670822753
Conc: 82.70 ug/ml

Instrument :
ECD_S
ClientSampleId :

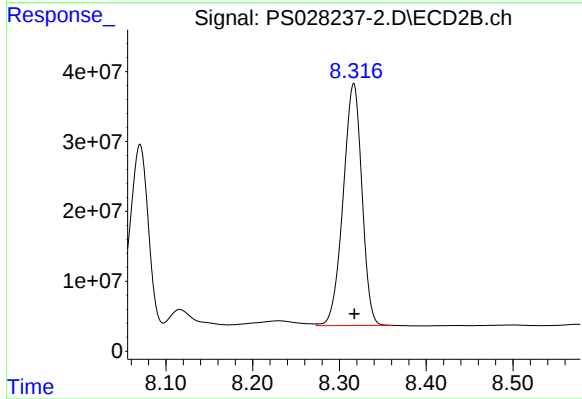


#7 MCPA

R.T.: 8.316 min
Delta R.T.: -0.001 min
Response: 519534122
Conc: 72.43 ug/ml

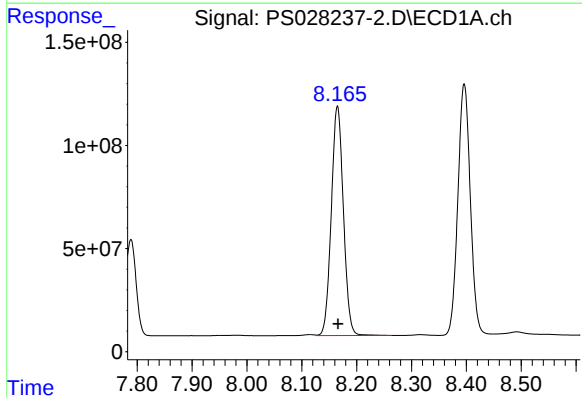


#8 DICHLORPROP

R.T.: 8.165 min
Delta R.T.: -0.001 min
Response: 1700588346
Conc: 941.33 ng/ml

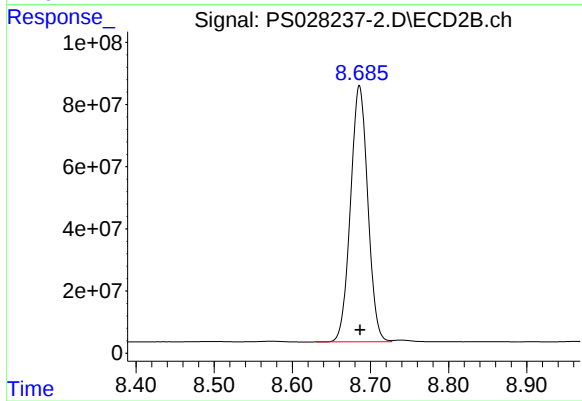

#8 DICHLORPROP


R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 1265854591
Conc: 727.23 ng/ml

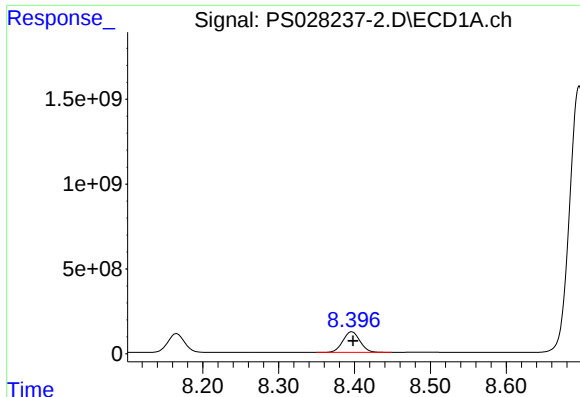

#9 2,4-D


R.T.: 8.396 min
Delta R.T.: -0.002 min
Response: 1925768925
Conc: 949.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

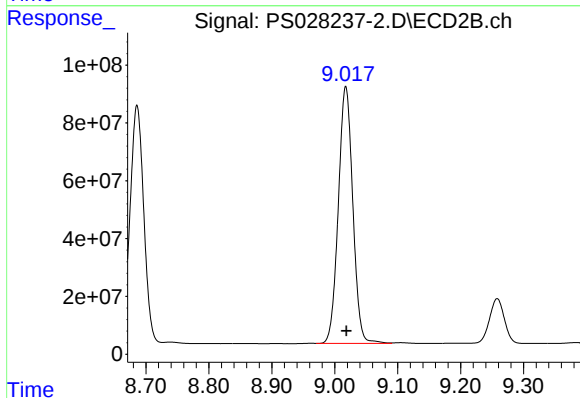


#9 2,4-D

R.T.: 9.018 min
Delta R.T.: -0.001 min
Response: 1417334611
Conc: 726.86 ng/ml

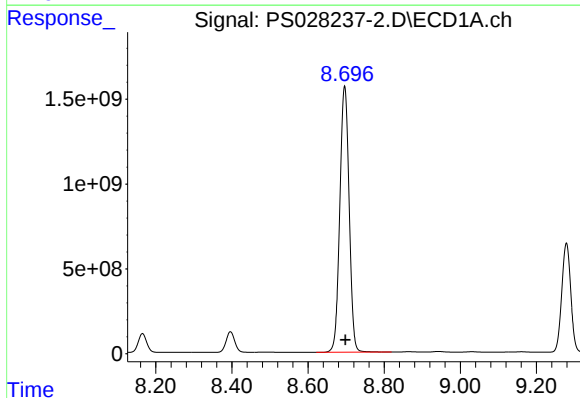


#10 Pentachlorophenol

R.T.: 8.696 min
Delta R.T.: -0.002 min
Response: 26537589039
Conc: 992.21 ng/ml

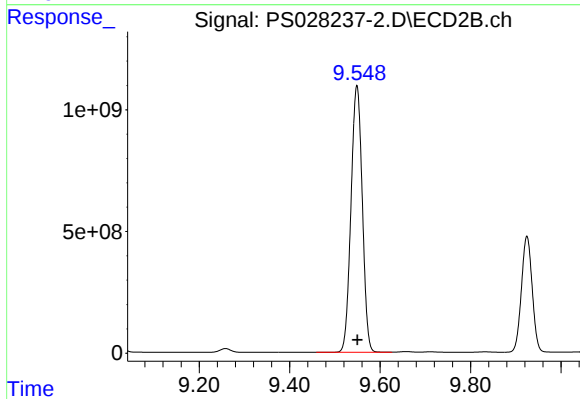

#10 Pentachlorophenol


R.T.: 9.549 min
Delta R.T.: -0.001 min
Response: 19016878261
Conc: 735.09 ng/ml

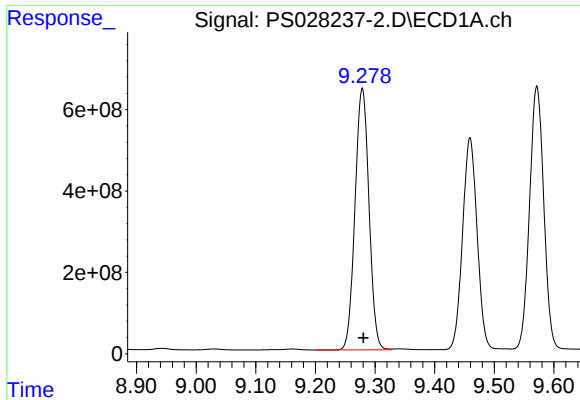

#11 2,4,5-TP (SILVEX)


R.T.: 9.279 min
Delta R.T.: -0.002 min
Response: 10458375777
Conc: 1044.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

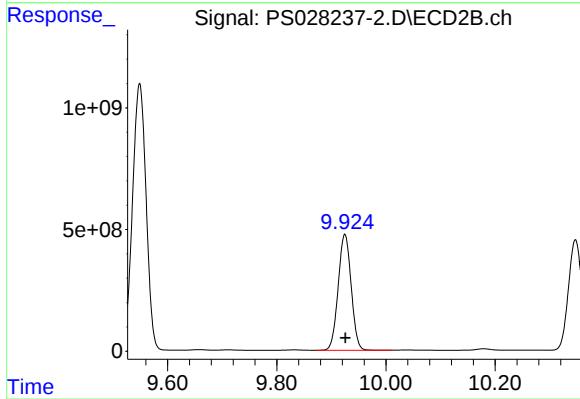


#11 2,4,5-TP (SILVEX)

R.T.: 9.925 min
Delta R.T.: -0.001 min
Response: 7868529318
Conc: 731.80 ng/ml

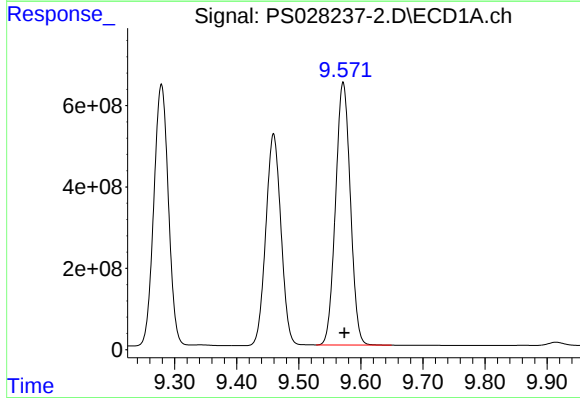


#12 2,4,5-T

R.T.: 9.571 min
Delta R.T.: -0.002 min
Response: 10682582757
Conc: 1045.57 ng/ml

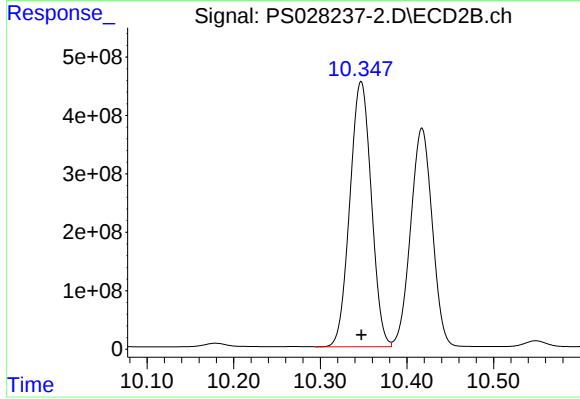

#12 2,4,5-T


R.T.: 10.347 min
Delta R.T.: 0.000 min
Response: 7810231495
Conc: 730.06 ng/ml

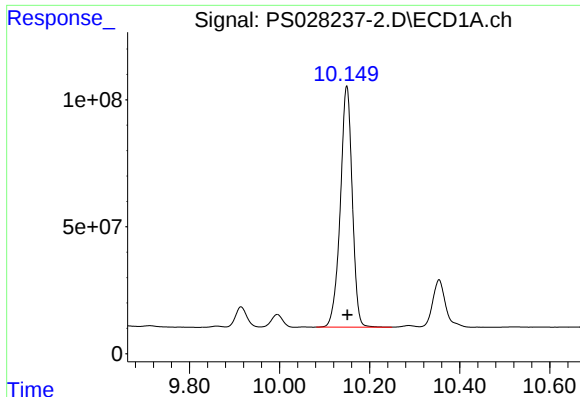

#13 2,4-DB


R.T.: 10.149 min
Delta R.T.: -0.001 min
Response: 1748580084
Conc: 1060.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

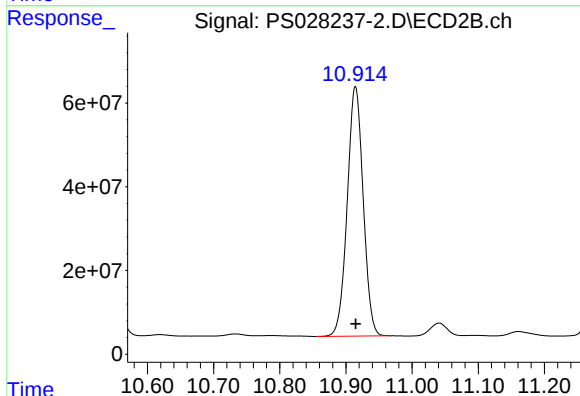


#13 2,4-DB

R.T.: 10.914 min
Delta R.T.: 0.000 min
Response: 998002832
Conc: 720.01 ng/ml

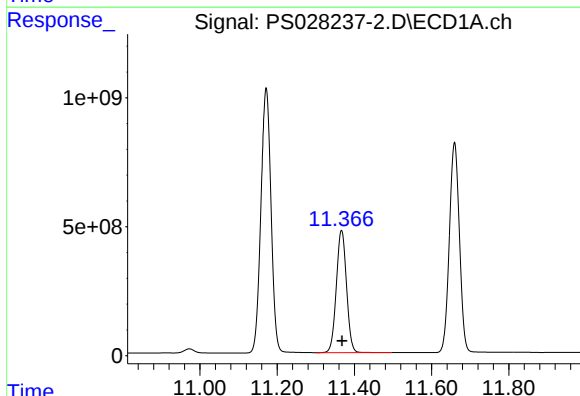


#14 DINOSEB

R.T.: 11.367 min
Delta R.T.: -0.001 min
Response: 8716127530
Conc: 1160.05 ng/ml

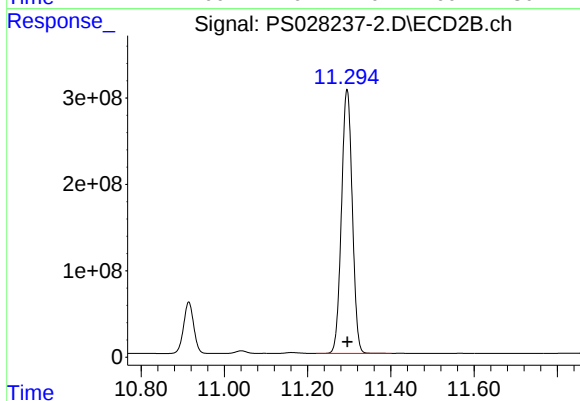

#14 DINOSEB


R.T.: 11.295 min
Delta R.T.: -0.001 min
Response: 5501141384
Conc: 733.36 ng/ml

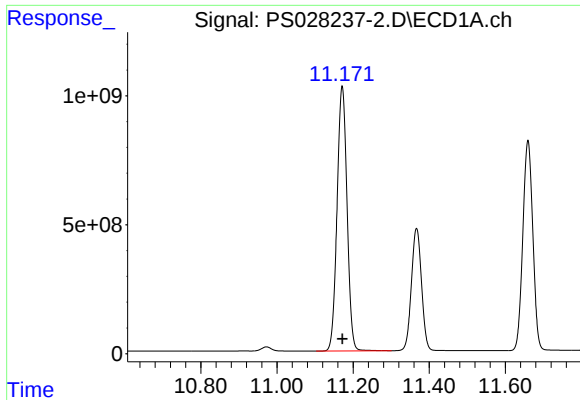

#15 Picloram


R.T.: 11.171 min
Delta R.T.: 0.000 min
Response: 18609334102
Conc: 1066.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

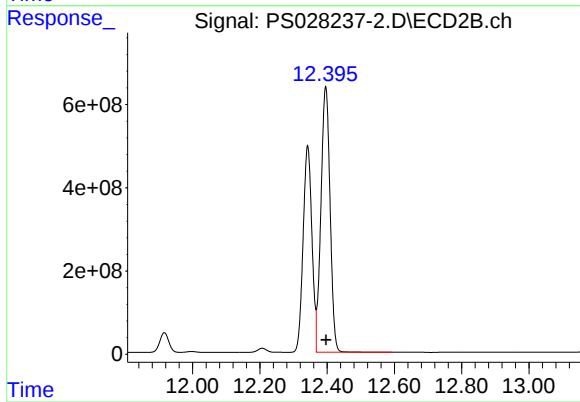


#15 Picloram

R.T.: 12.396 min
Delta R.T.: -0.001 min
Response: 12022995255
Conc: 732.32 ng/ml

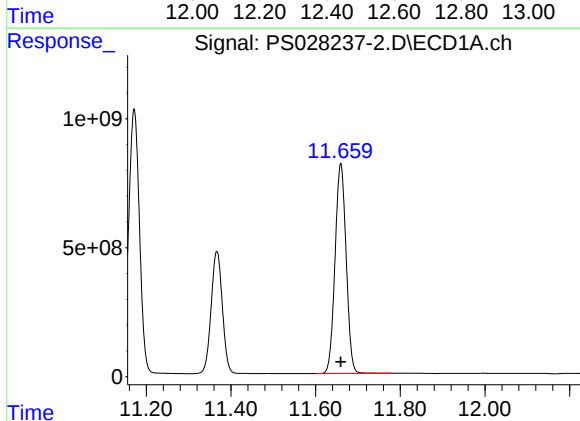

#16 DCPA

R.T.: 11.659 min
Delta R.T.: 0.000 min
Response: 14794666284
Conc: 1188.34 ng/ml

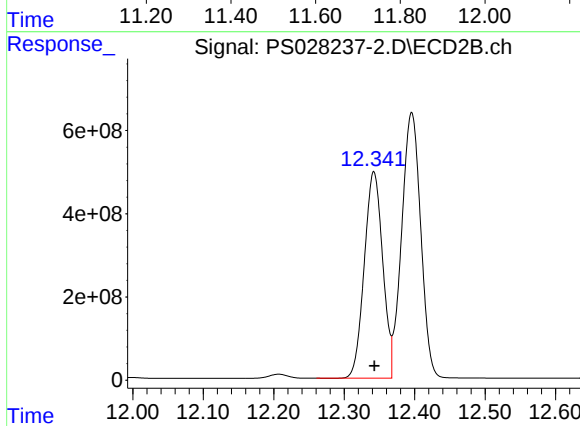

#16 DCPA

R.T.: 12.342 min
Delta R.T.: 0.000 min
Response: 9021249859
Conc: 715.76 ng/ml