

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
 Data File : PS002327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 09:55
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:31:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.349	0	266503	N.D.	0.590 #
6) T	MCPD	0.000	11.419	0	263670	N.D.	0.306 #
7) T	MCPA	0.000	11.819	0	91111	N.D.	0.067 #
12) T	2,4,5-T	0.000	14.510	0	7047202	N.D.	4.706 #
15) T	Picloram	16.924	16.757	21747280	243086	9.117	0.107 #
16) T	DCPA	0.000	16.817	0	21720942	N.D.	9.173 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
Data File : PS002327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 09:55
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:31:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

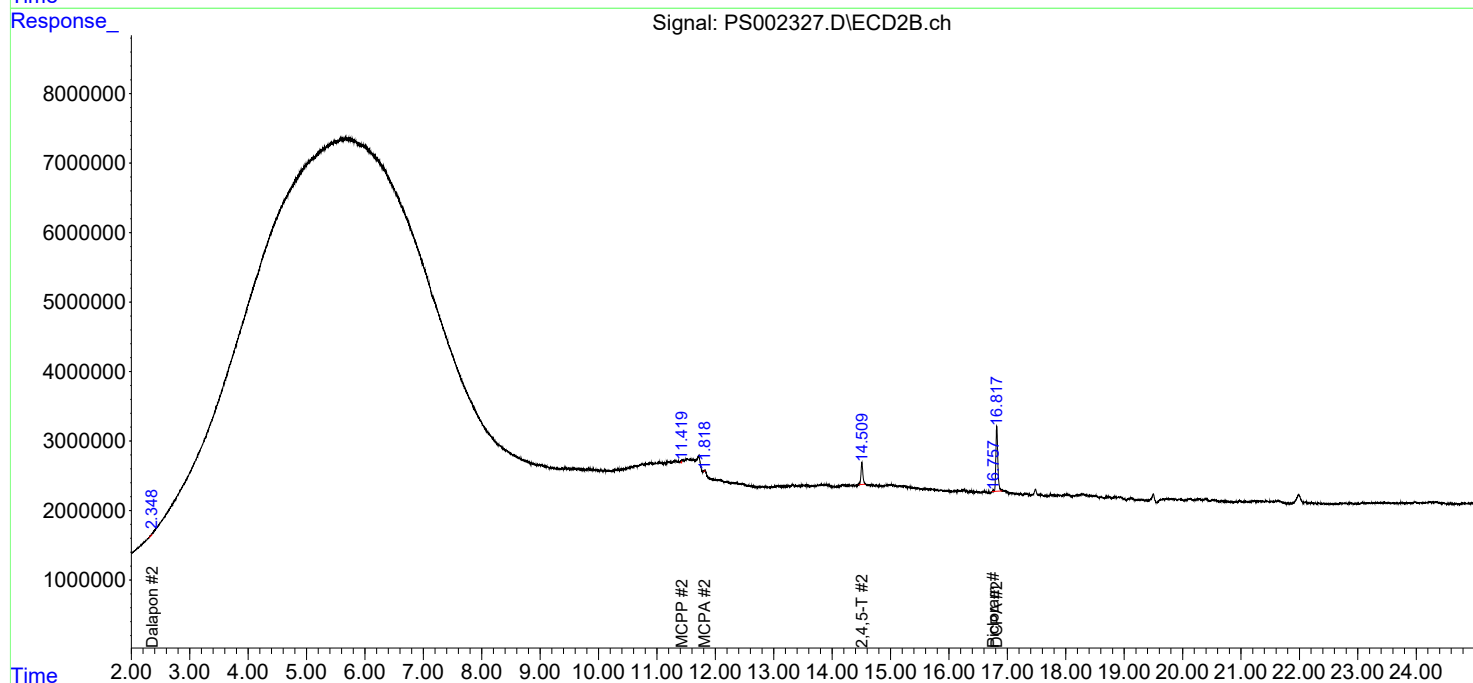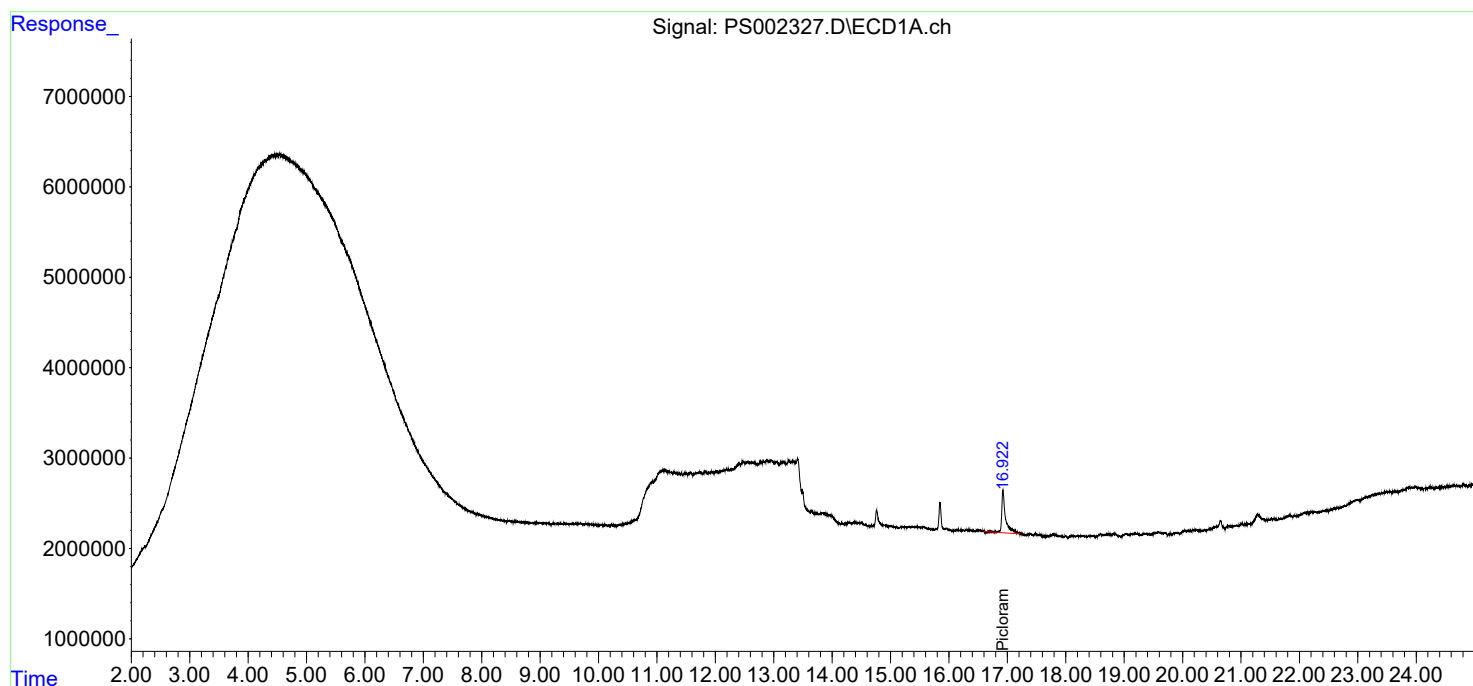


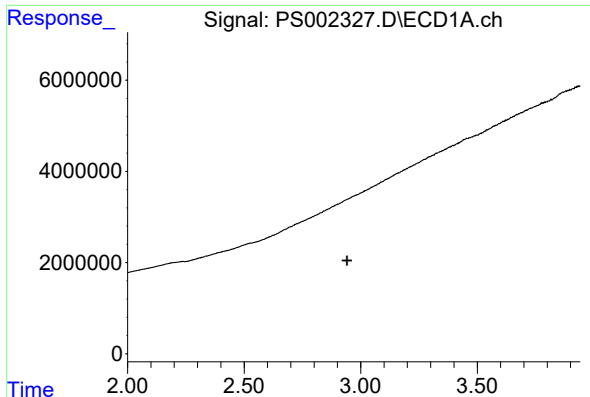

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

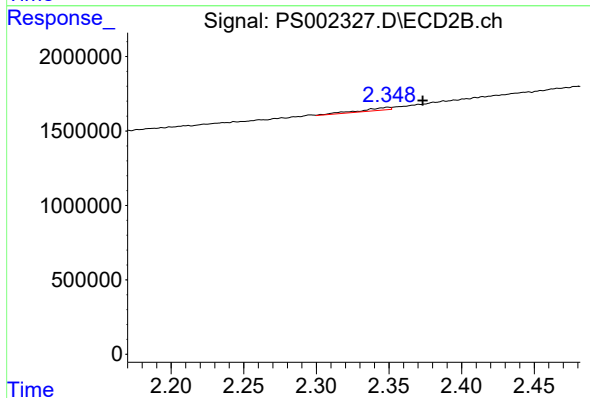


#1 Dalapon

R.T.: 2.349 min
Delta R.T.: -0.024 min
Response: 266503
Conc: 0.59 ng/ml

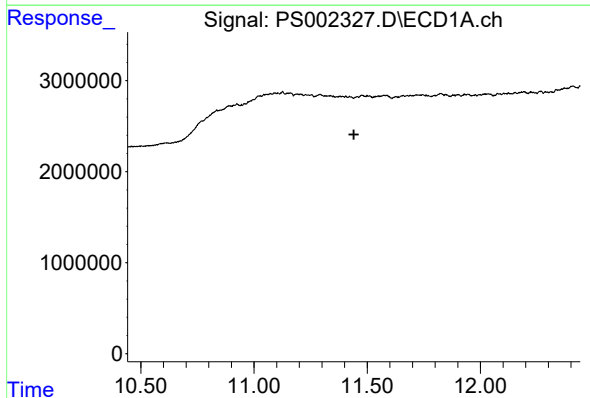


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.441 min
Response: 0
Conc: N.D.

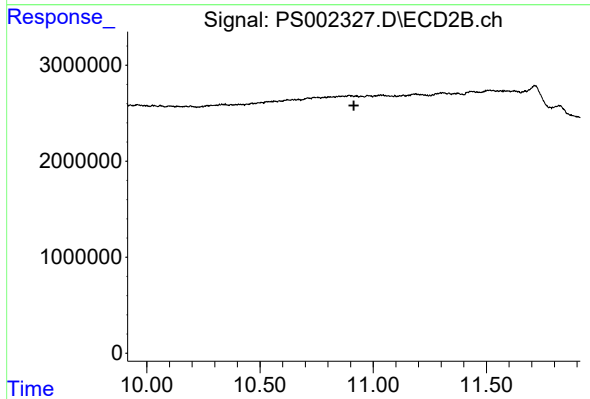

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.914 min
Response: 0
Conc: N.D.

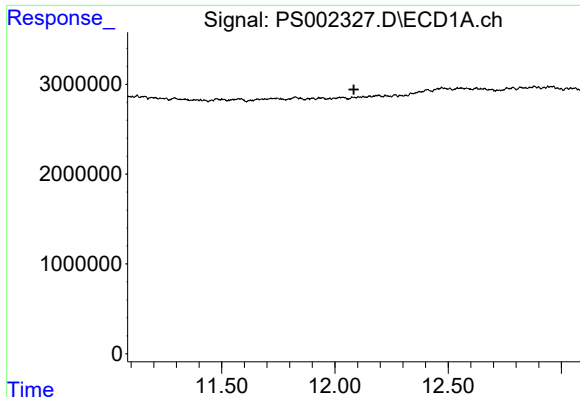

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

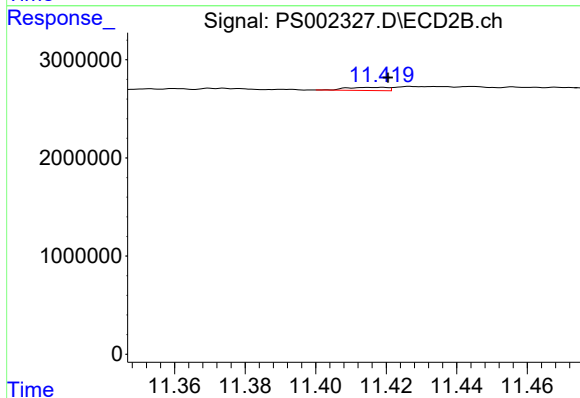


#6 MCPP

R.T.: 11.419 min
Delta R.T.: -0.001 min
Response: 263670
Conc: 0.31 ug/ml

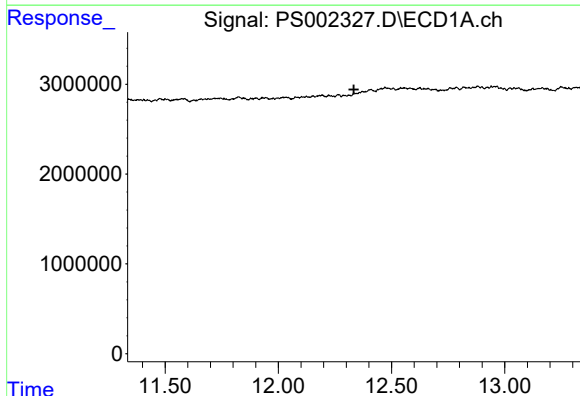


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

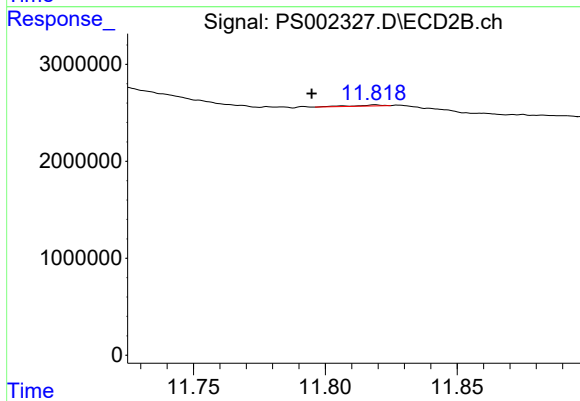

#7 MCPA


R.T.: 11.819 min
Delta R.T.: 0.024 min
Response: 91111
Conc: 0.07 ug/ml

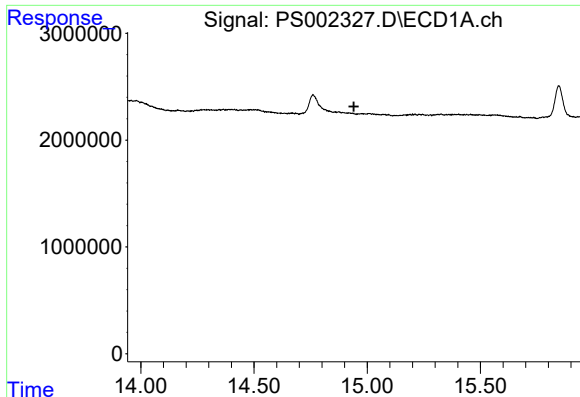

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

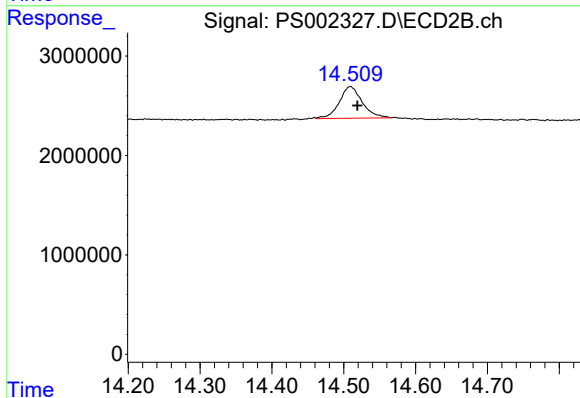


#12 2,4,5-T

R.T.: 14.510 min
Delta R.T.: -0.009 min
Response: 7047202
Conc: 4.71 ng/ml

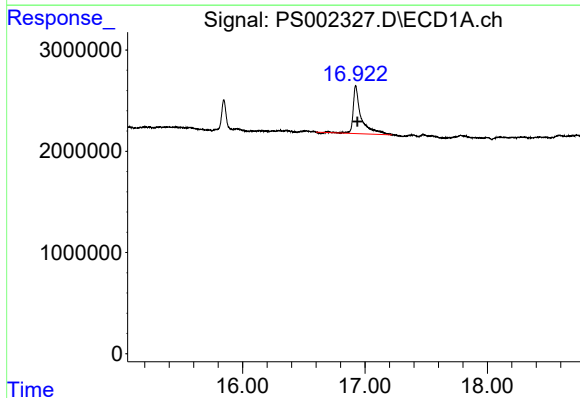


#15 Picloram

R.T.: 16.924 min
Delta R.T.: -0.013 min
Response: 21747280
Conc: 9.12 ng/ml

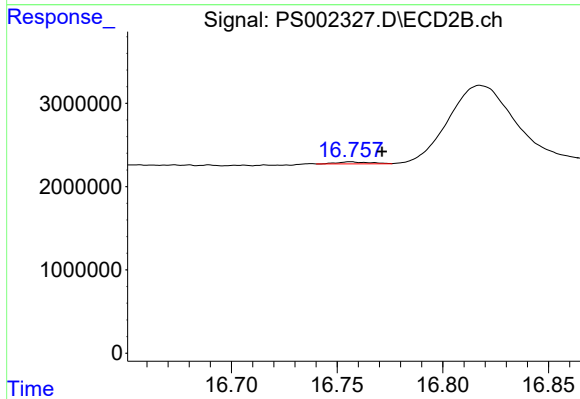

#15 Picloram


R.T.: 16.757 min
Delta R.T.: -0.015 min
Response: 243086
Conc: 0.11 ng/ml

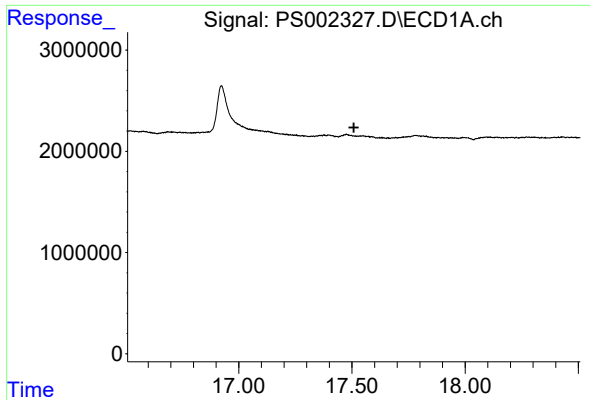

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

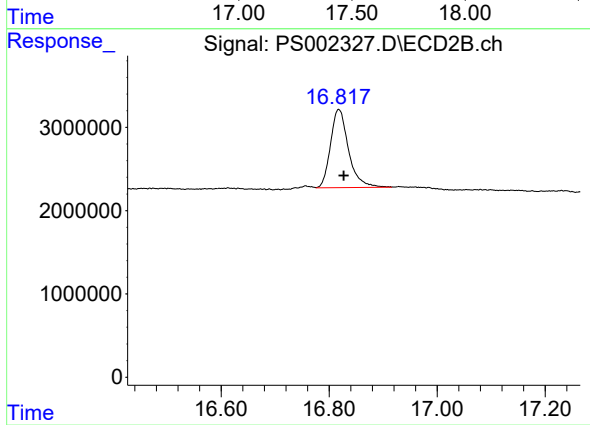

#16 DCPA

R.T.: 16.817 min
Delta R.T.: -0.009 min
Response: 21720942
Conc: 9.17 ng/ml