

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
 Data File : PS002332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 14:14
 Operator : EI\SJ
 Sample : PB114526TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:32:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.445	10.936	132.0E6	121.2E6	419.496	337.532
Target Compounds							
1) T	Dalapon	2.921	2.370	10213789	13883110	22.268	30.748 #
2) T	3,5-DICHL...	0.000	9.097	0	523805	N.D.	1.181 #
3) T	4-Nitroph...	0.000	10.098	0	1210991	N.D.	6.791 #
6) T	MCP	12.127	0.000	45884540	0	46.448	N.D. #
7) T	MCPA	0.000	11.751	0	3822129	N.D.	2.824 #
8) T	DICHLORPROP	0.000	12.284	0	278486	N.D.	0.867 #
10) T	Pentachlo...	0.000	13.285	0	3278257	N.D.	0.698 #
11) T	2,4,5-TP ...	0.000	13.901	0	597669	N.D.	0.327 #
12) T	2,4,5-T	0.000	14.512	0	289239	N.D.	0.193 #
15) T	Picloram	16.959	16.805	2610202	3147401	1.094	1.391 #
16) T	DCPA	0.000	16.805	0	3147401	N.D.	1.329 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
Data File : PS002332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 14:14
Operator : EI\SJ
Sample : PB114526TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:32:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

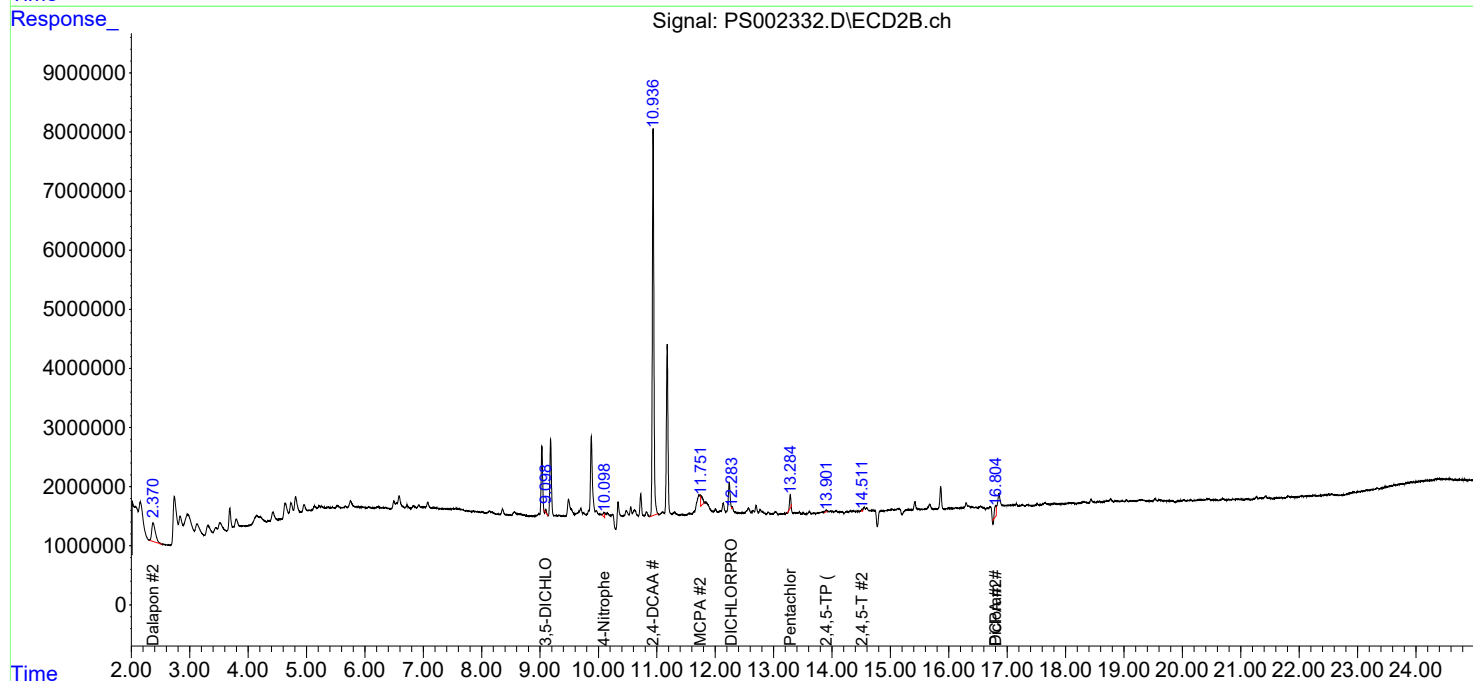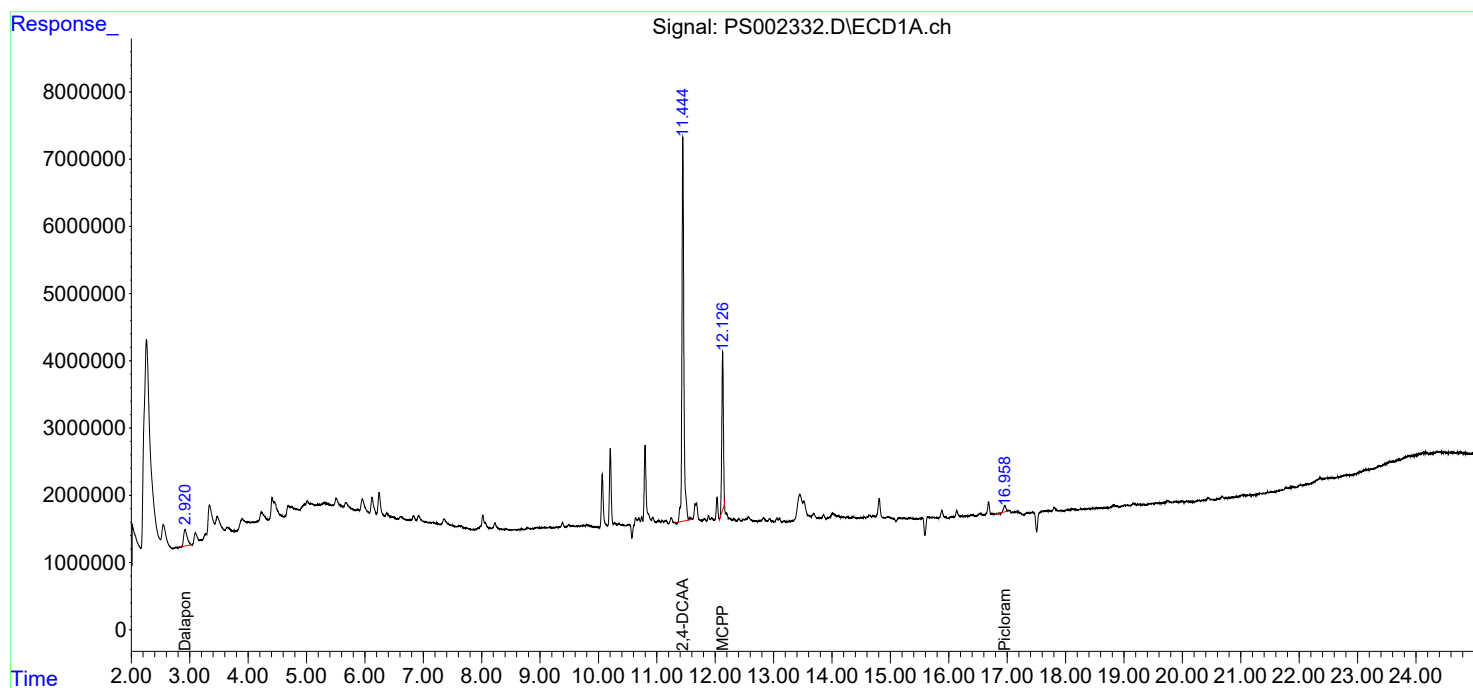


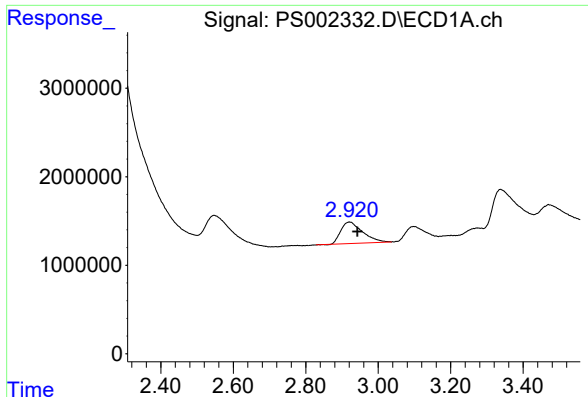

#1 Dalapon


R.T.: 2.921 min
Delta R.T.: -0.021 min
Response: 10213789
Conc: 22.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

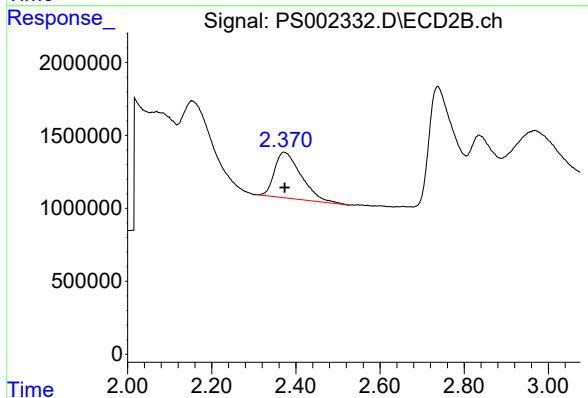


#1 Dalapon

R.T.: 2.370 min
Delta R.T.: -0.003 min
Response: 13883110
Conc: 30.75 ng/ml

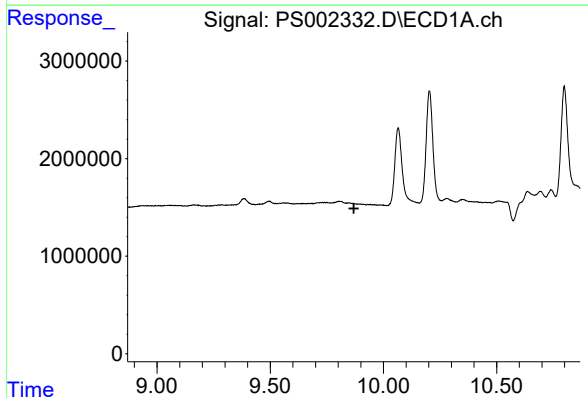


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

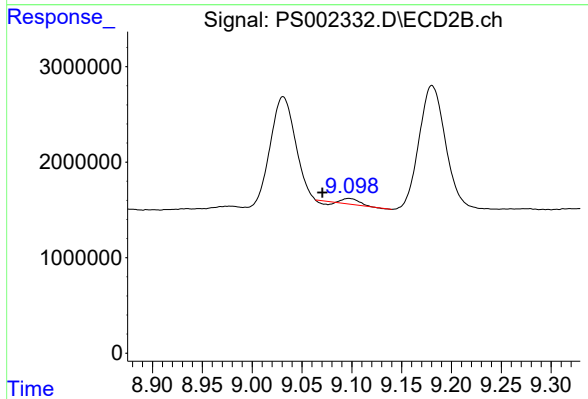

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.097 min
Delta R.T.: 0.026 min
Response: 523805
Conc: 1.18 ng/ml

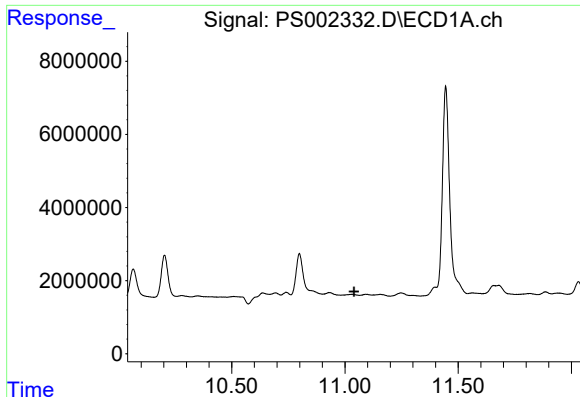

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

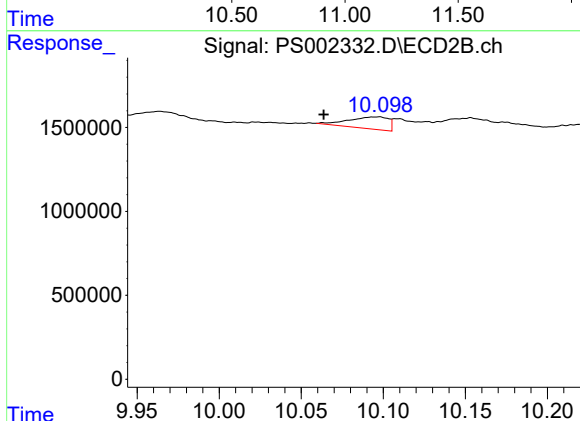


#3 4-Nitrophenol

R.T.: 10.098 min
Delta R.T.: 0.034 min
Response: 1210991
Conc: 6.79 ng/ml

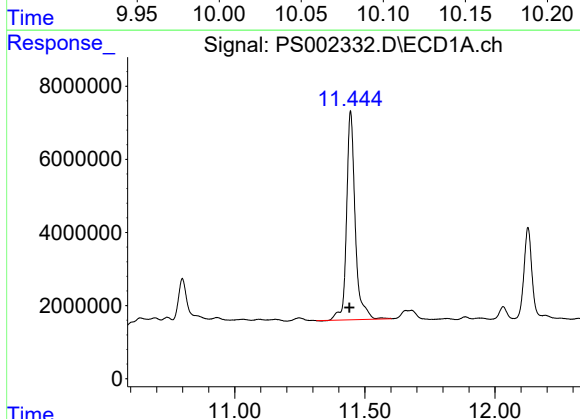


#4 2,4-DCAA

R.T.: 11.445 min
Delta R.T.: 0.004 min
Response: 132009508
Conc: 419.50 ng/ml

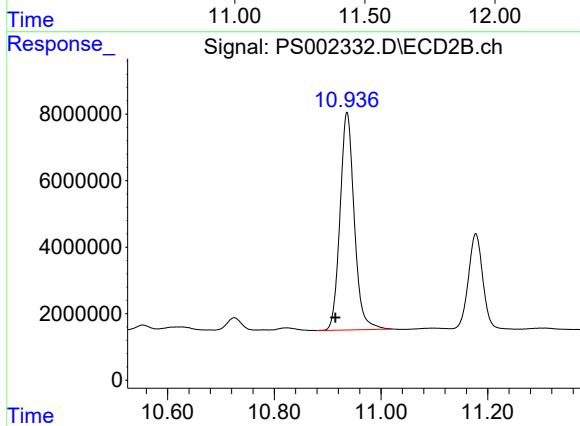

#4 2,4-DCAA


R.T.: 10.936 min
Delta R.T.: 0.022 min
Response: 121207058
Conc: 337.53 ng/ml

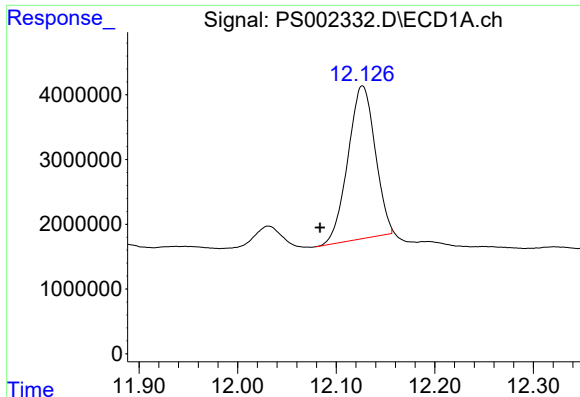

#6 MCPP


R.T.: 12.127 min
Delta R.T.: 0.043 min
Response: 45884540
Conc: 46.45 ug/ml

Instrument :
ECD_S
ClientSampleId :

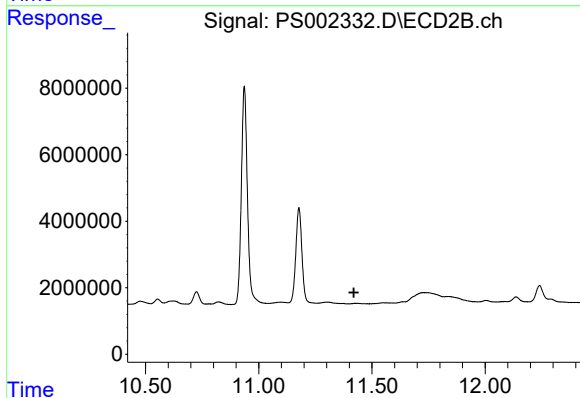


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

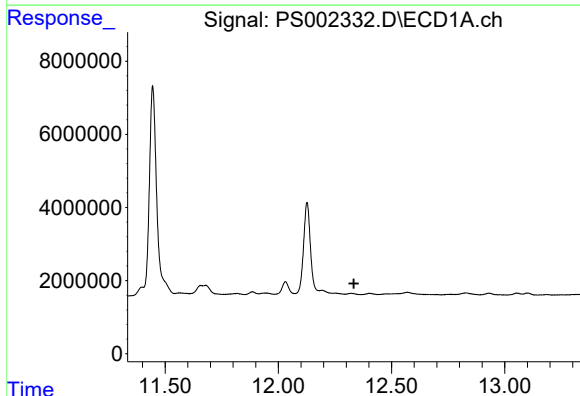


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

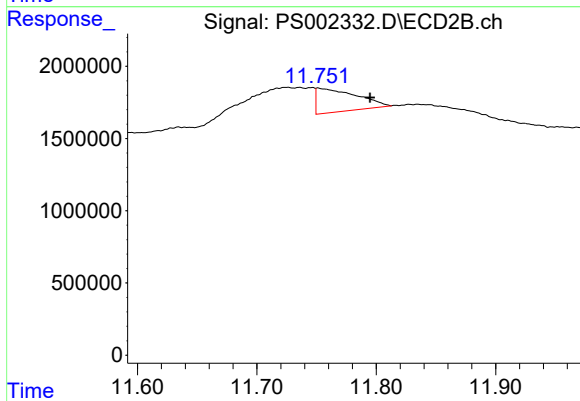

#7 MCPA


R.T.: 11.751 min
Delta R.T.: -0.044 min
Response: 3822129
Conc: 2.82 ug/ml

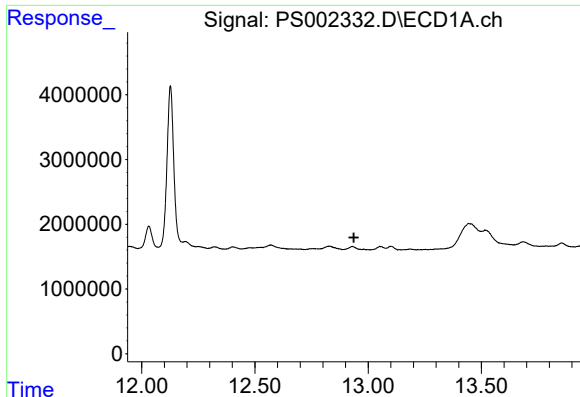

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

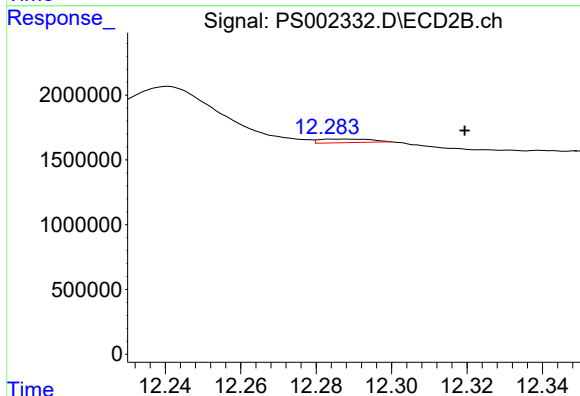


#8 DICHLORPROP

R.T.: 12.284 min
Delta R.T.: -0.036 min
Response: 278486
Conc: 0.87 ng/ml

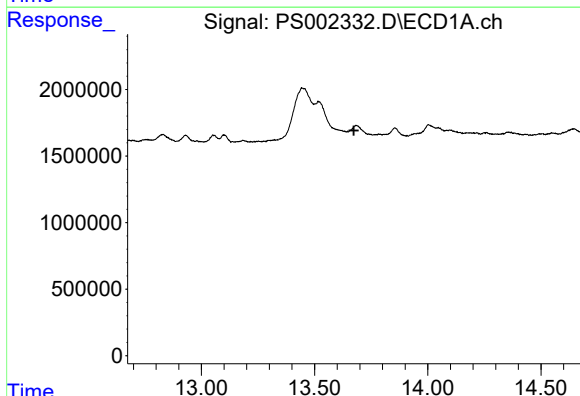


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.674 min
Response: 0
Conc: N.D.

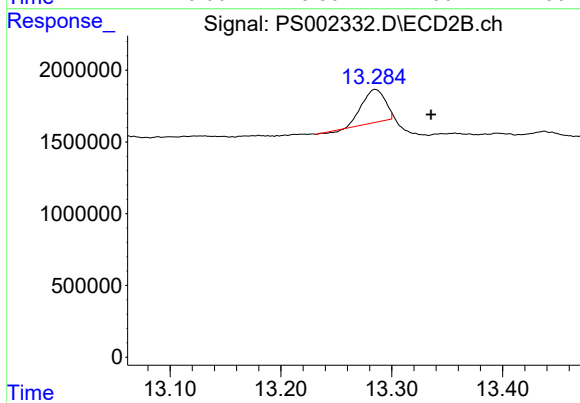

#10 Pentachlorophenol


R.T.: 13.285 min
Delta R.T.: -0.050 min
Response: 3278257
Conc: 0.70 ng/ml

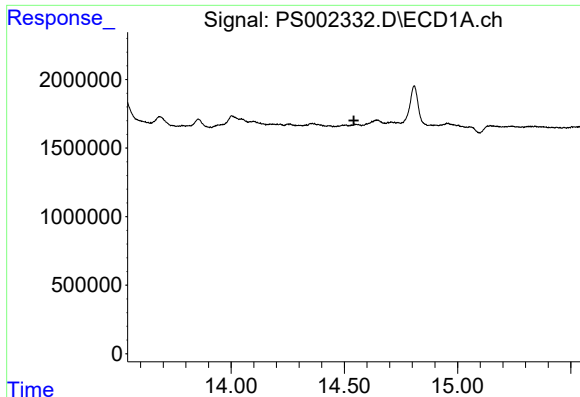

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

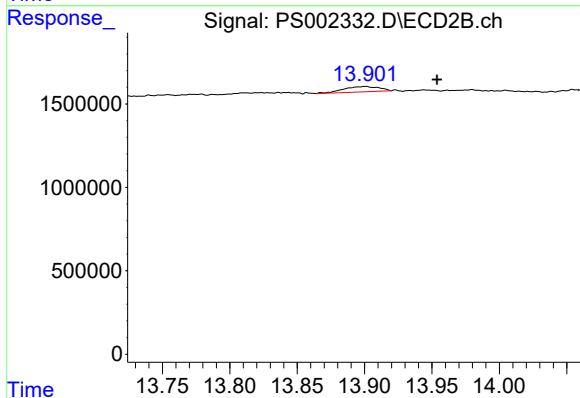


#11 2,4,5-TP (SILVEX)

R.T.: 13.901 min
Delta R.T.: -0.053 min
Response: 597669
Conc: 0.33 ng/ml

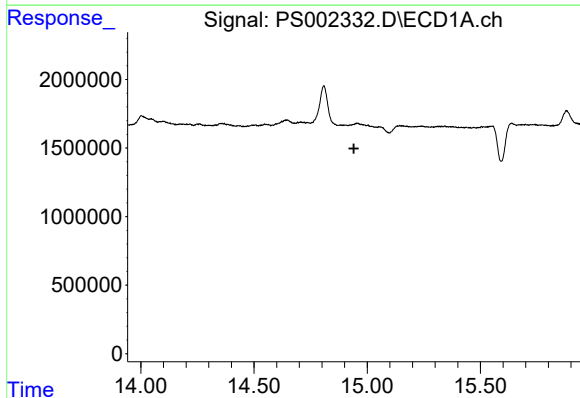


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

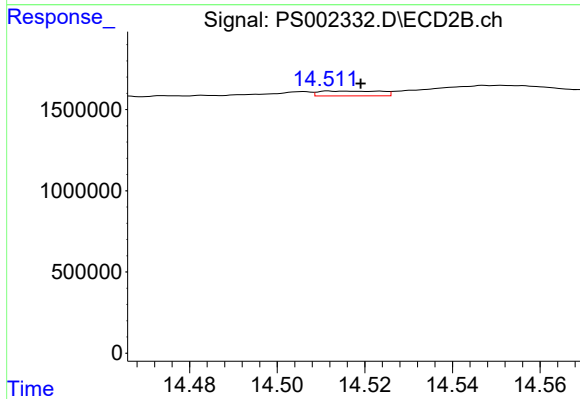

#12 2,4,5-T


R.T.: 14.512 min
Delta R.T.: -0.007 min
Response: 289239
Conc: 0.19 ng/ml

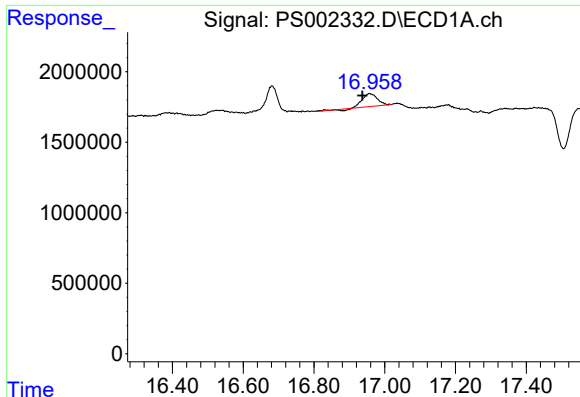

#15 Picloram


R.T.: 16.959 min
Delta R.T.: 0.021 min
Response: 2610202
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

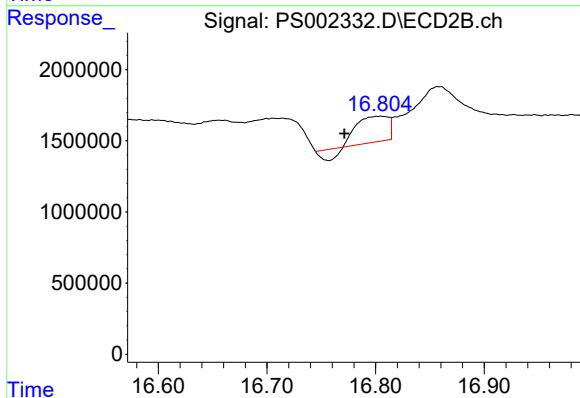


#15 Picloram

R.T.: 16.805 min
Delta R.T.: 0.034 min
Response: 3147401
Conc: 1.39 ng/ml

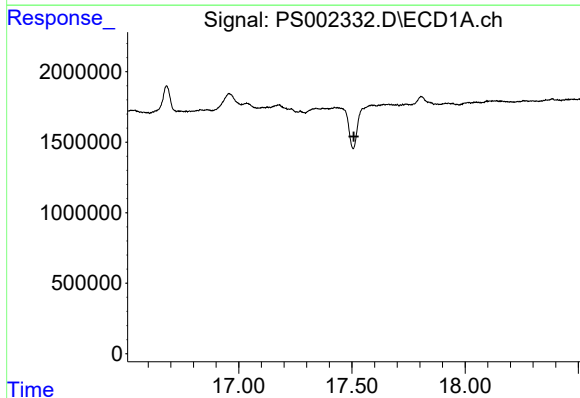

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

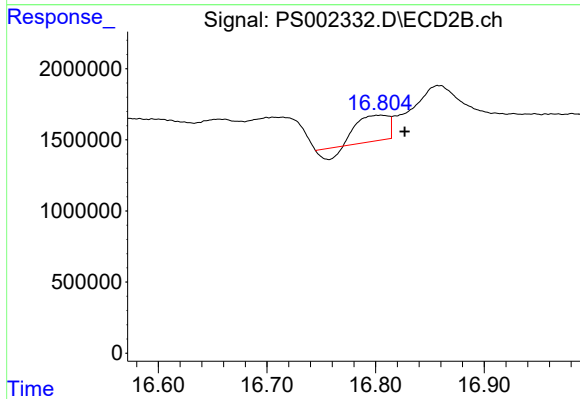

#16 DCPA

R.T.: 16.805 min
Delta R.T.: -0.022 min
Response: 3147401
Conc: 1.33 ng/ml