

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
 Data File : PS002339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 17:51
 Operator : EI\SJ
 Sample : J5805-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:34:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.406	10.900	102.5E6	92653905	325.829	258.018
Target Compounds							
1) T	Dalapon	2.881	2.332	4702007	2766814	10.251	6.128 #
2) T	3,5-DICHL...	0.000	9.059	0	358985	N.D.	0.809 #
3) T	4-Nitroph...	0.000	10.060	0	1778182	N.D.	9.972 #
5) T	DICAMBA	0.000	11.141	0	42090981	N.D.	33.681 #
6) T	MCP	0.000	11.408	0	570888	N.D.	0.664 #
7) T	MCPA	0.000	11.797	0	4857731	N.D.	3.589 #
8) T	DICHLORPROP	0.000	12.252	0	1388221	N.D.	4.323 #
9) T	2,4-D	0.000	12.732	0	781505	N.D.	1.835 #
12) T	2,4,5-T	0.000	14.557	0	1738939	N.D.	1.161 #
14) T	DINOSEB	0.000	15.639	0	3100039	N.D.	2.449 #
15) T	Picloram	0.000	16.767	0	1335414	N.D.	0.590 #
16) T	DCPA	0.000	16.822	0	2963530	N.D.	1.252 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
Data File : PS002339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 17:51
Operator : EI\SJ
Sample : J5805-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:34:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

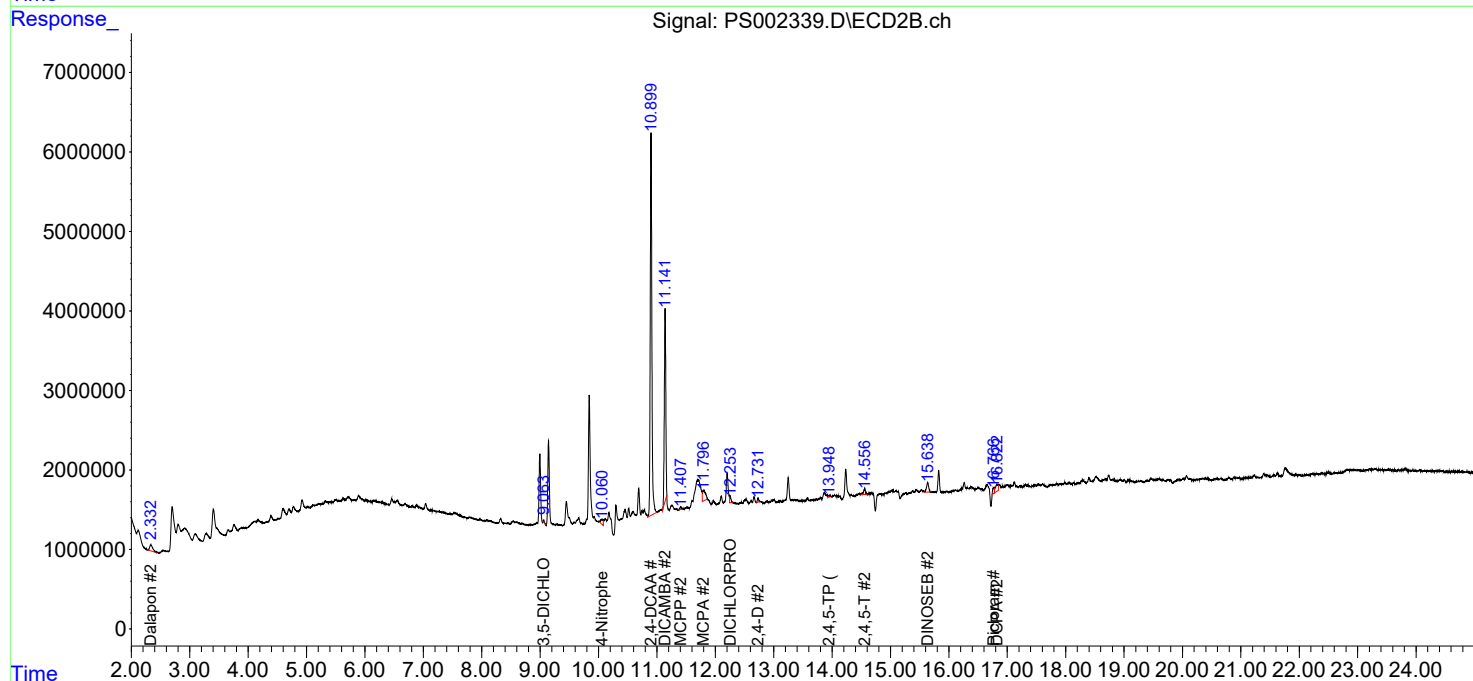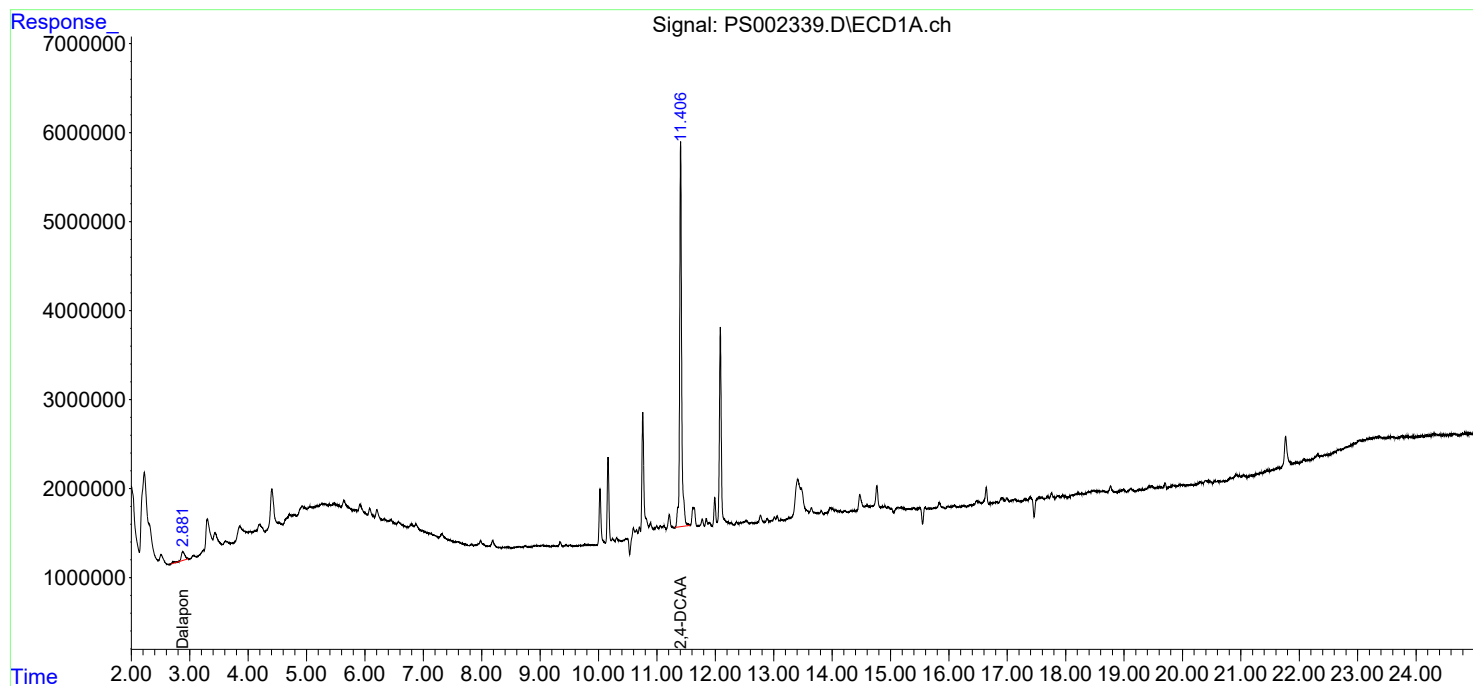


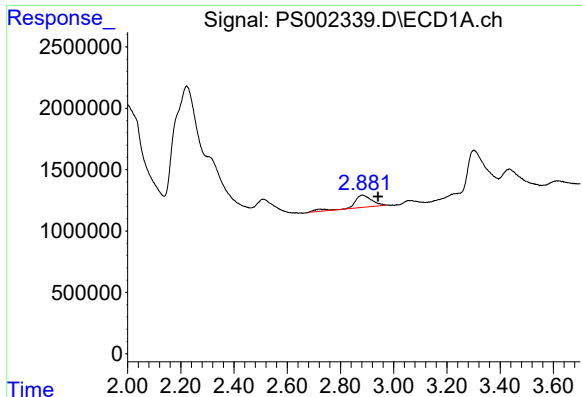

#1 Dalapon


R.T.: 2.881 min
Delta R.T.: -0.061 min
Response: 4702007
Conc: 10.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

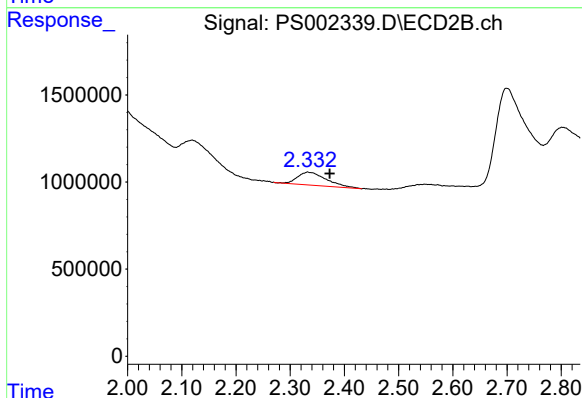


#1 Dalapon

R.T.: 2.332 min
Delta R.T.: -0.041 min
Response: 2766814
Conc: 6.13 ng/ml

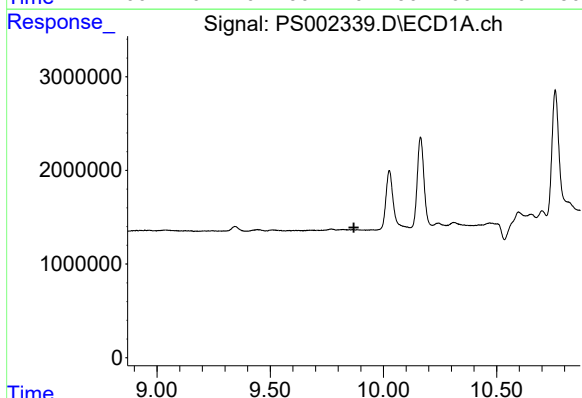


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

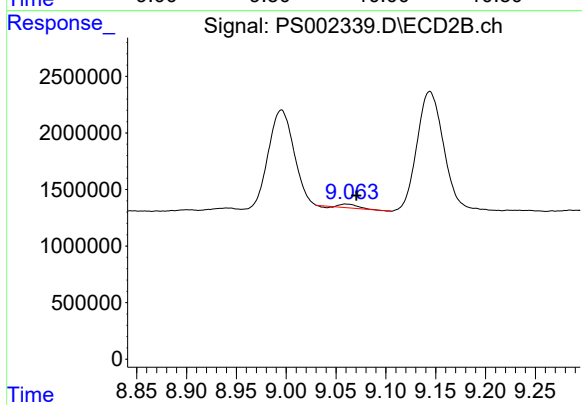

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.059 min
Delta R.T.: -0.012 min
Response: 358985
Conc: 0.81 ng/ml

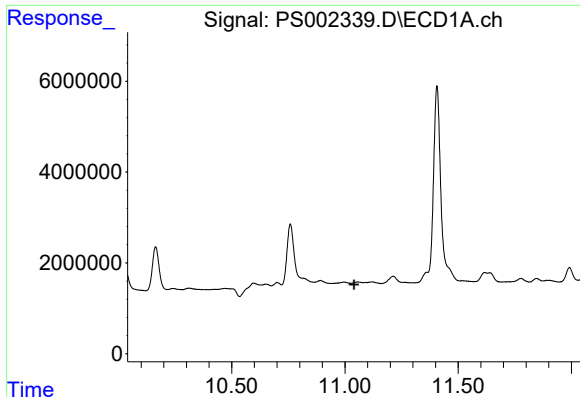

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

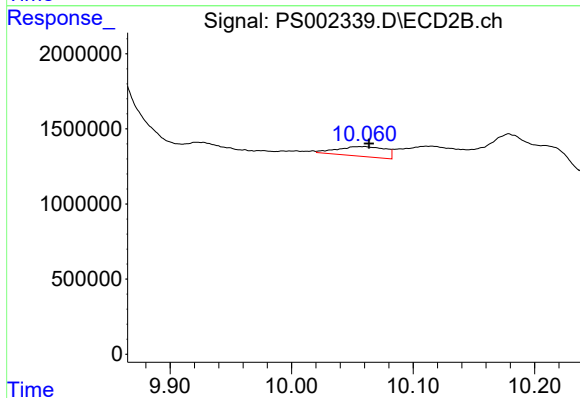


#3 4-Nitrophenol

R.T.: 10.060 min
Delta R.T.: -0.004 min
Response: 1778182
Conc: 9.97 ng/ml

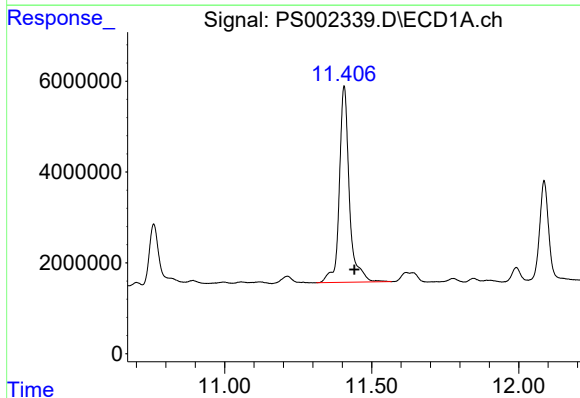


#4 2,4-DCAA

R.T.: 11.406 min
Delta R.T.: -0.035 min
Response: 102533665
Conc: 325.83 ng/ml

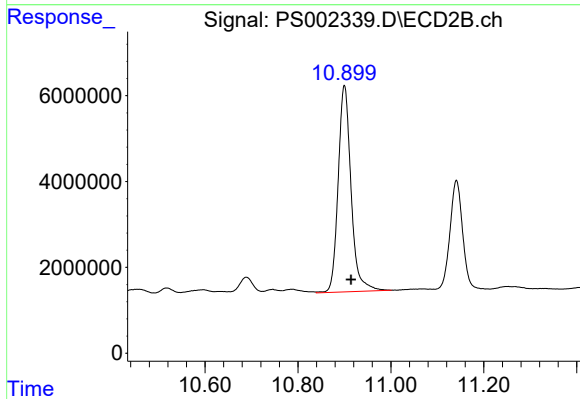

#4 2,4-DCAA


R.T.: 10.900 min
Delta R.T.: -0.014 min
Response: 92653905
Conc: 258.02 ng/ml

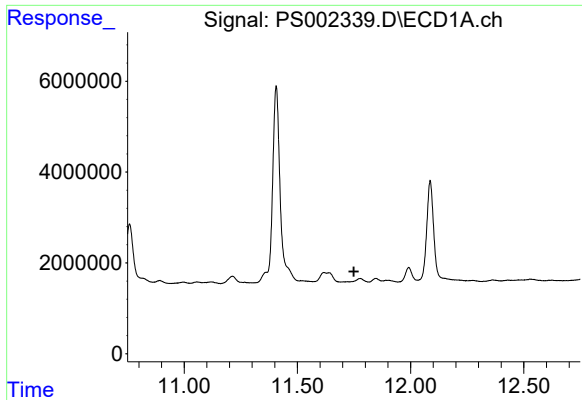

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

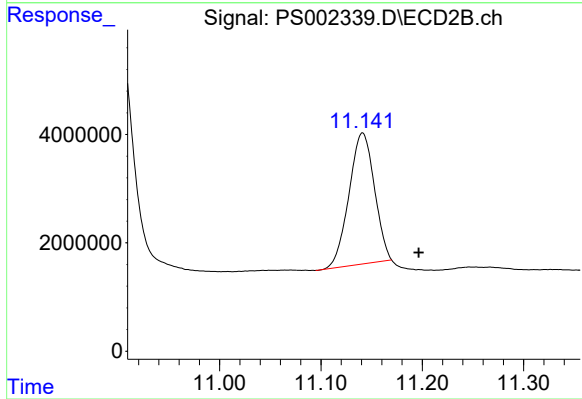


#5 DICAMBA

R.T.: 11.141 min
Delta R.T.: -0.055 min
Response: 42090981
Conc: 33.68 ng/ml

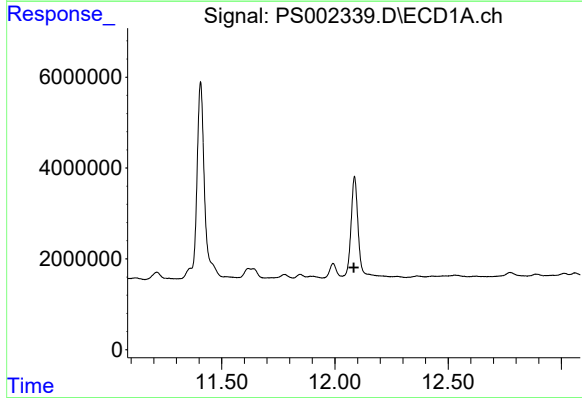


#6 MCP

R.T.: 0.000 min
Exp R.T.: 12.084 min
Response: 0
Conc: N.D.

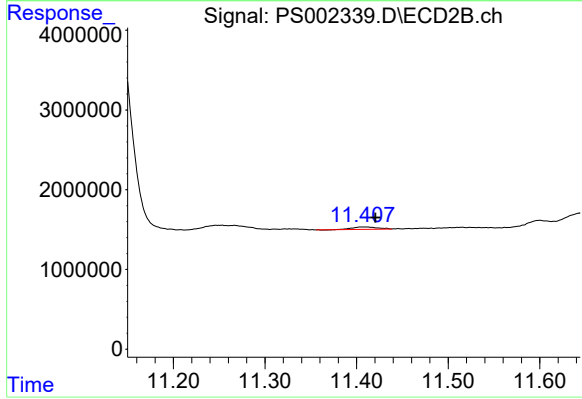

#6 MCP


R.T.: 11.408 min
Delta R.T.: -0.012 min
Response: 570888
Conc: 0.66 ug/ml

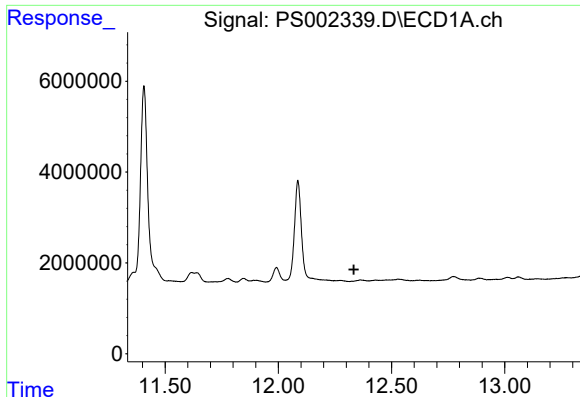

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

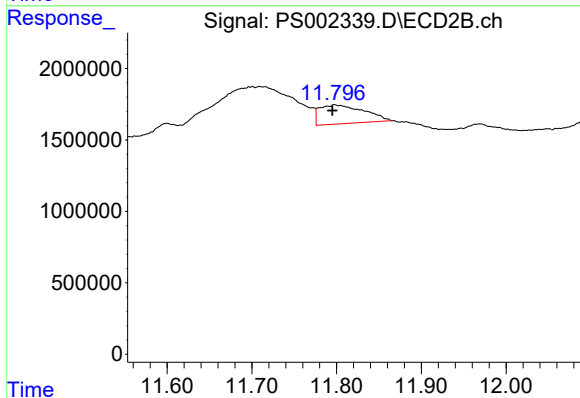


#7 MCPA

R.T.: 11.797 min
Delta R.T.: 0.003 min
Response: 4857731
Conc: 3.59 ug/ml

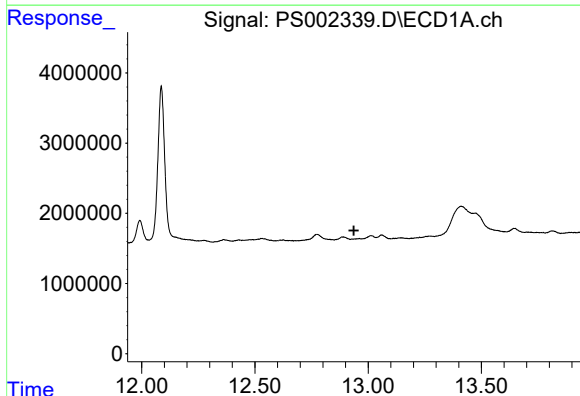


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

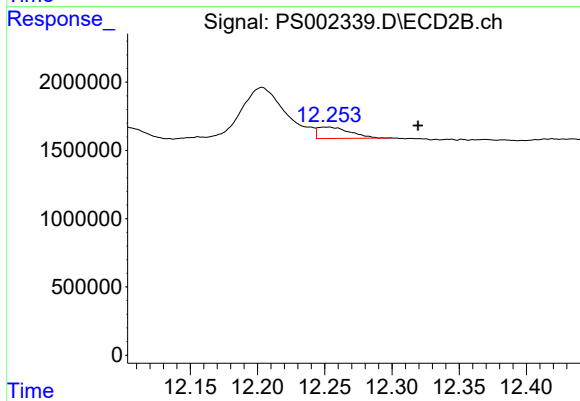

#8 DICHLORPROP


R.T.: 12.252 min
Delta R.T.: -0.067 min
Response: 1388221
Conc: 4.32 ng/ml

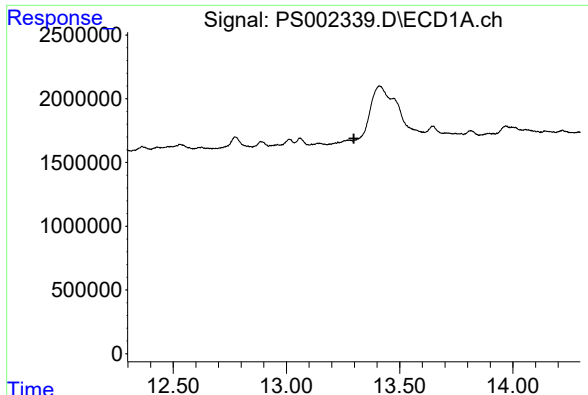

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

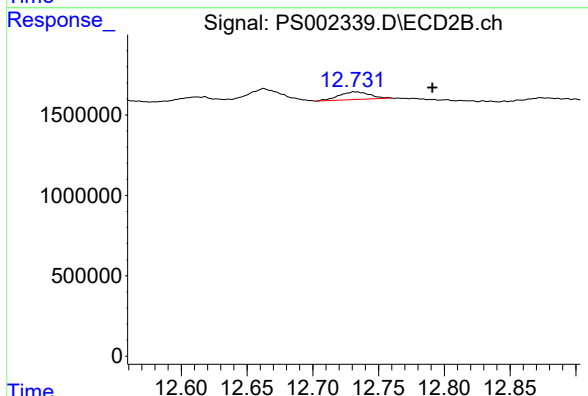


#9 2,4-D

R.T.: 12.732 min
Delta R.T.: -0.059 min
Response: 781505
Conc: 1.83 ng/ml

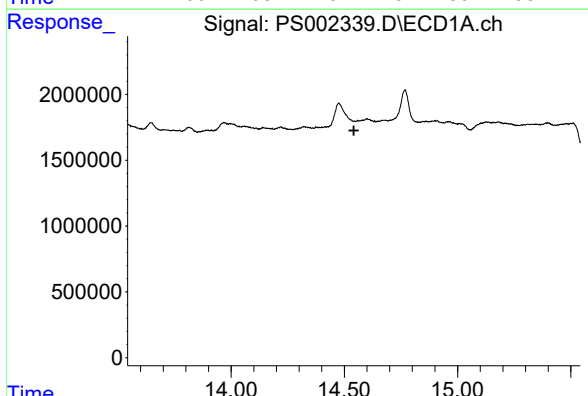


#11 2,4,5-TP (SILVEX)

R.T.: 14.475 min
Delta R.T.: -0.067 min
Response: -654396
Conc: N.D.

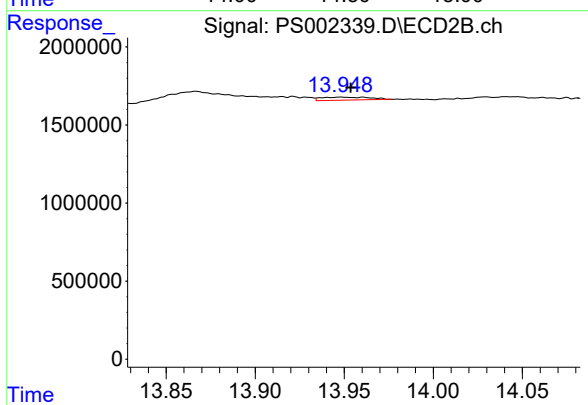

#11 2,4,5-TP (SILVEX)


R.T.: 13.948 min
Delta R.T.: -0.005 min
Response: 363458
Conc: 0.20 ng/ml

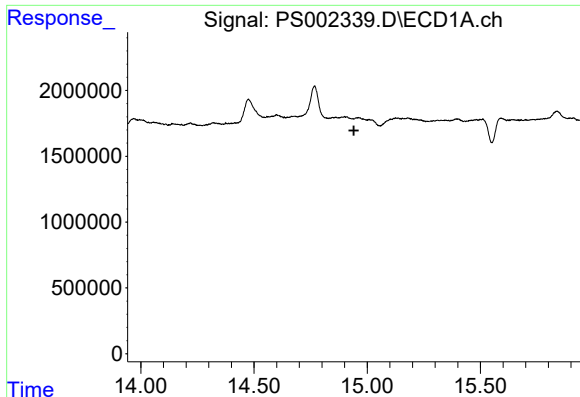

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

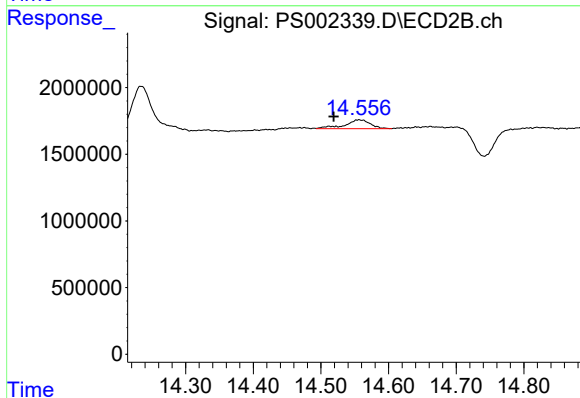


#12 2,4,5-T

R.T.: 14.557 min
Delta R.T.: 0.037 min
Response: 1738939
Conc: 1.16 ng/ml

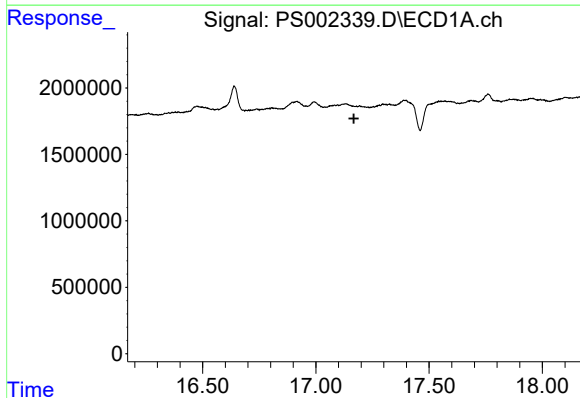


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.168 min
Response: 0
Conc: N.D.

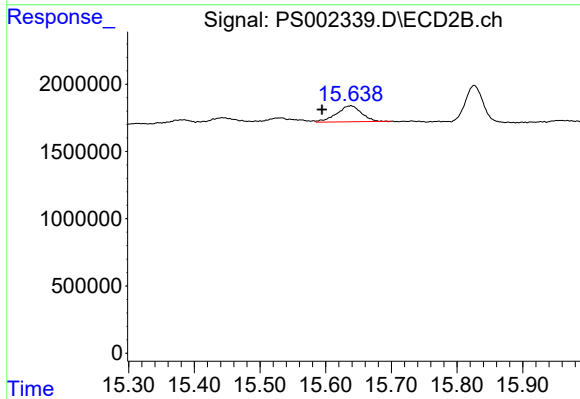

#14 DINOSEB


R.T.: 15.639 min
Delta R.T.: 0.044 min
Response: 3100039
Conc: 2.45 ng/ml

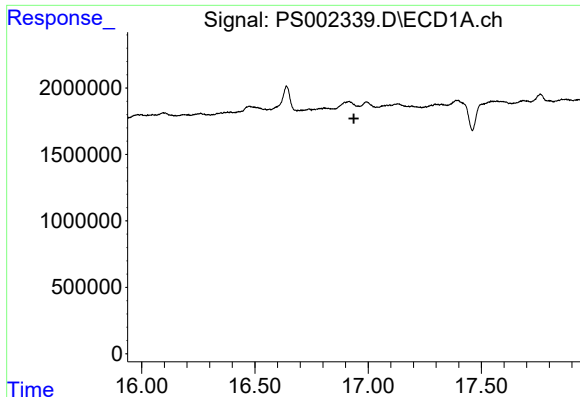

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

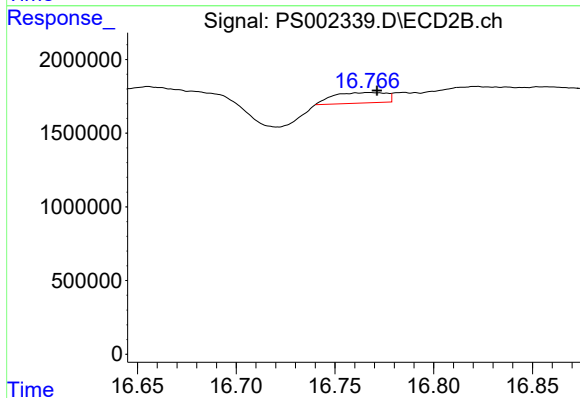


#15 Picloram

R.T.: 16.767 min
Delta R.T.: -0.004 min
Response: 1335414
Conc: 0.59 ng/ml

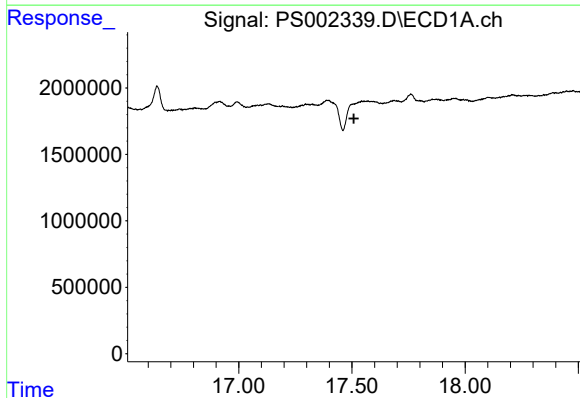

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

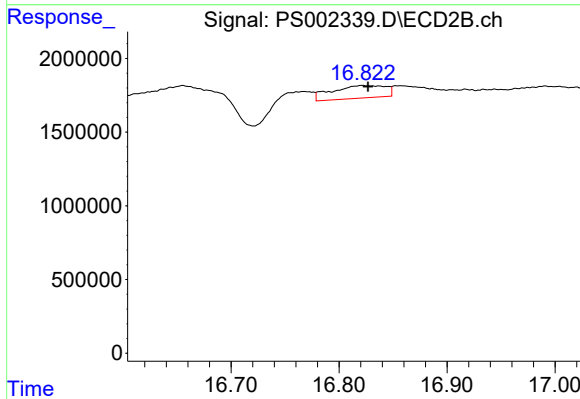

#16 DCPA

R.T.: 16.822 min
Delta R.T.: -0.005 min
Response: 2963530
Conc: 1.25 ng/ml