

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
 Data File : PS002346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 21:28
 Operator : EI\SJ
 Sample : J5812-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:35:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.443	10.935	129.9E6	121.3E6	412.700	337.663
Target Compounds							
1) T	Dalapon	2.920	2.371	10005223	12792032	21.814	28.332 #
2) T	3,5-DICHL...	0.000	9.096	0	1217711	N.D.	2.745 #
3) T	4-Nitroph...	0.000	10.092	0	1705131	N.D.	9.563 #
6) T	MCP	12.124	0.000	41737121	0	42.250	N.D. #
7) T	MCPA	0.000	11.832	0	998819	N.D.	0.738 #
8) T	DICHLORPROP	0.000	12.289	0	345856	N.D.	1.077 #
11) T	2,4,5-TP ...	0.000	14.003	0	289595	N.D.	0.158 #
13) T	2,4-DB	15.632	15.131	6327690	52266379	26.948	235.904 #
15) T	Picloram	0.000	16.807	0	2001535	N.D.	0.885 #
16) T	DCPA	17.565	16.807	-380535	2001535	N.D.	0.845



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
Data File : PS002346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 21:28
Operator : EI\SJ
Sample : J5812-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:35:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

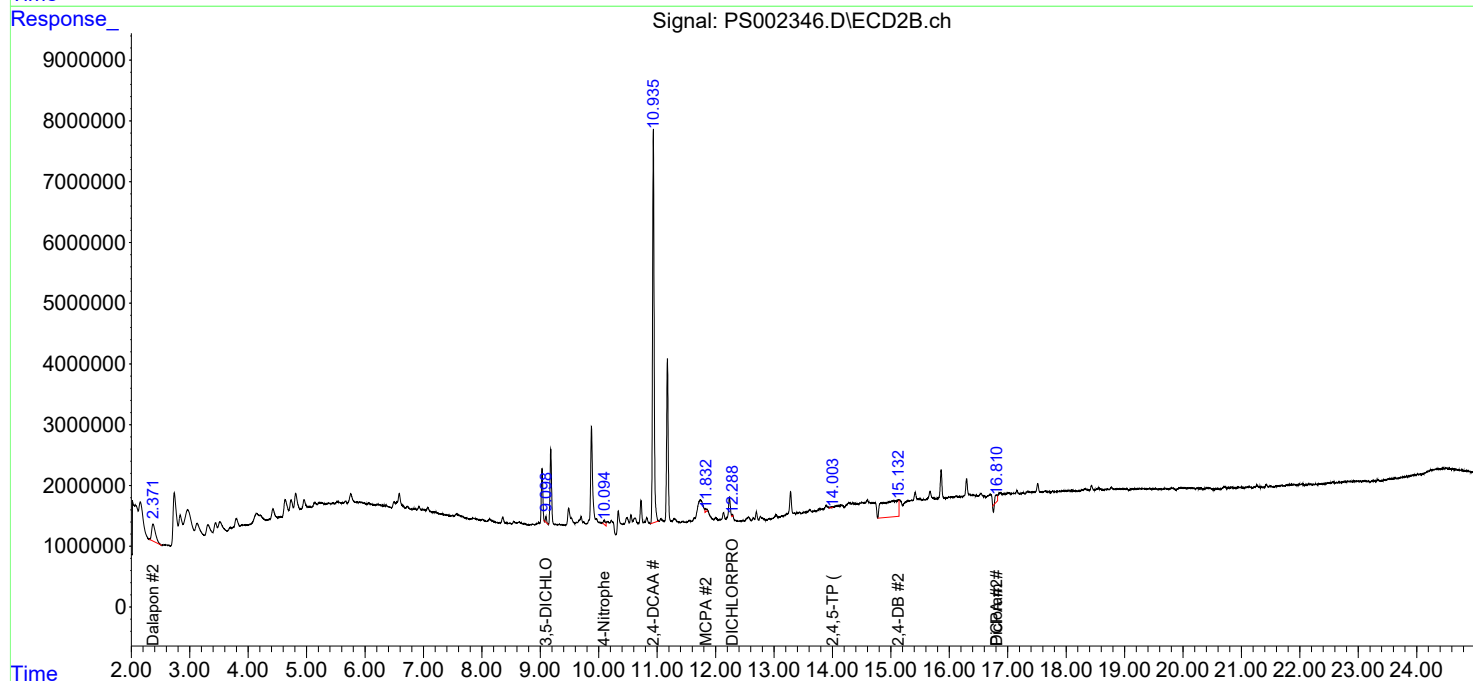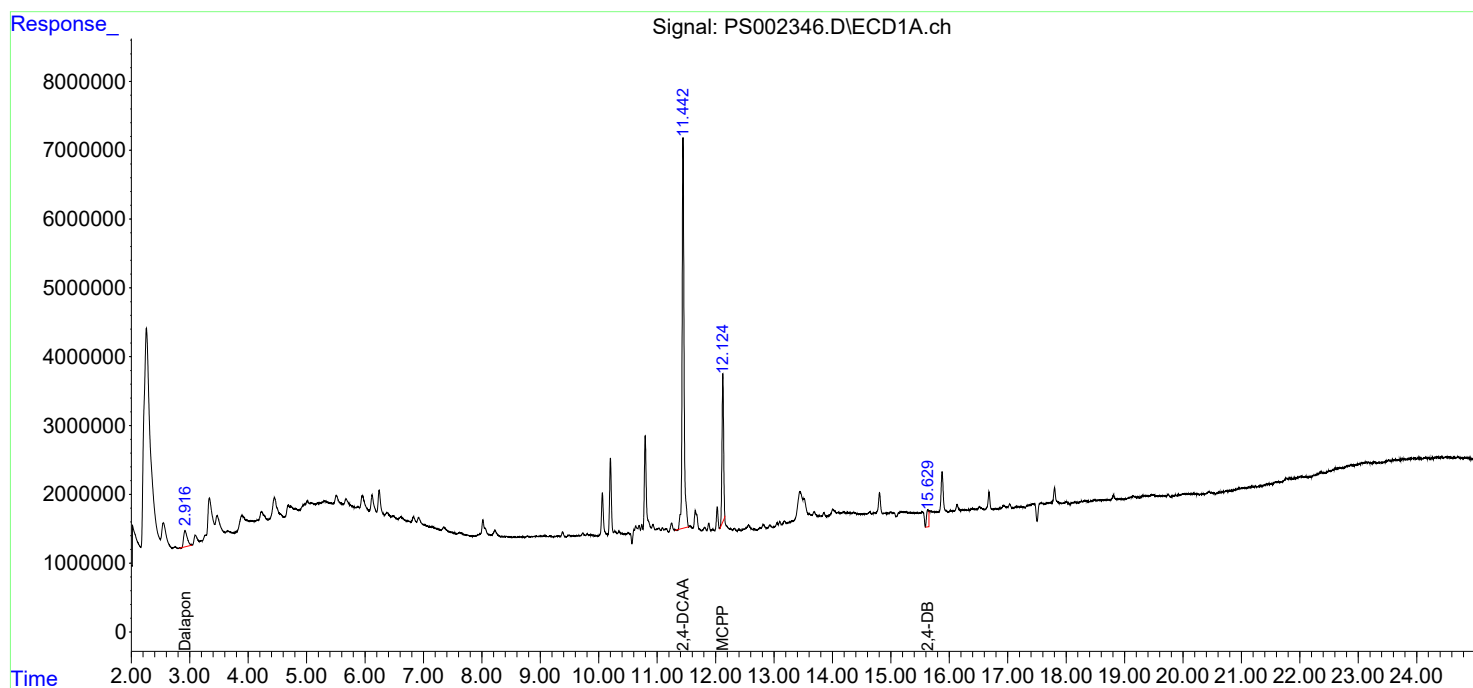


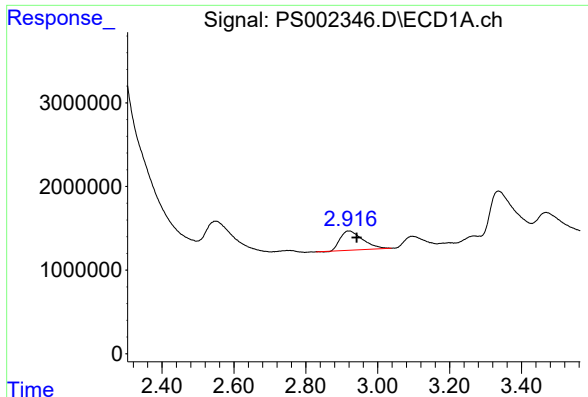

#1 Dalapon


R.T.: 2.920 min
Delta R.T.: -0.022 min
Response: 10005223
Conc: 21.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

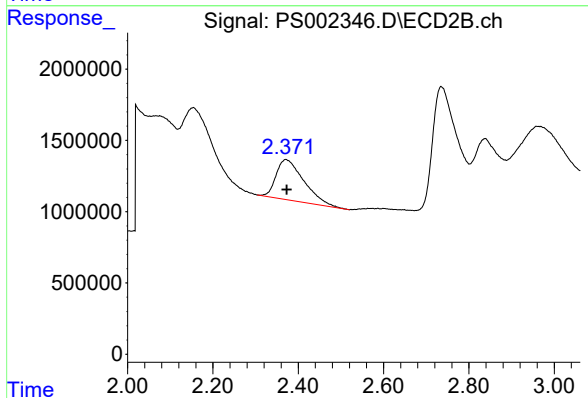


#1 Dalapon

R.T.: 2.371 min
Delta R.T.: -0.002 min
Response: 12792032
Conc: 28.33 ng/ml

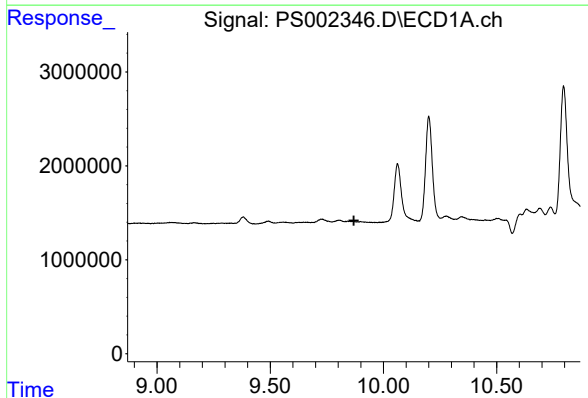


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

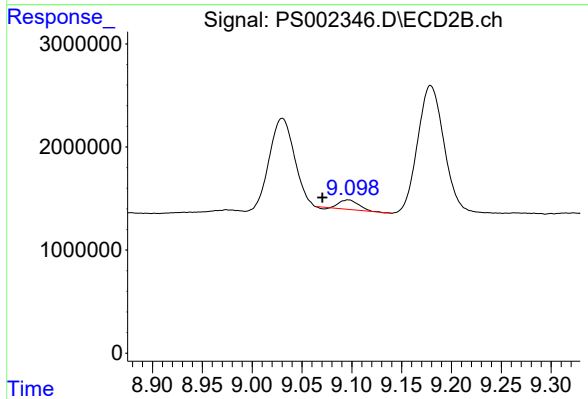

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.096 min
Delta R.T.: 0.026 min
Response: 1217711
Conc: 2.75 ng/ml

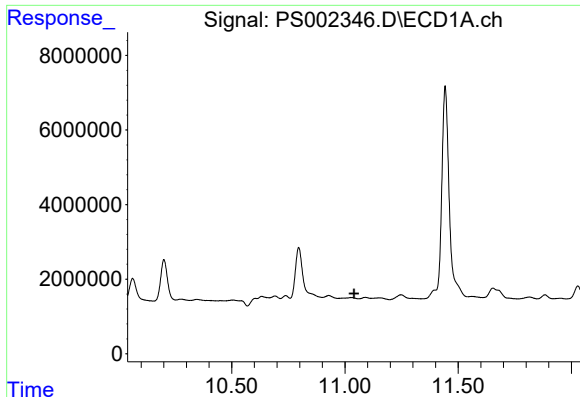

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

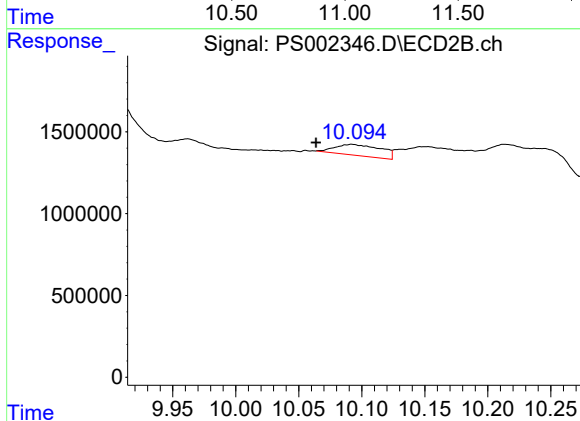


#3 4-Nitrophenol

R.T.: 10.092 min
Delta R.T.: 0.028 min
Response: 1705131
Conc: 9.56 ng/ml

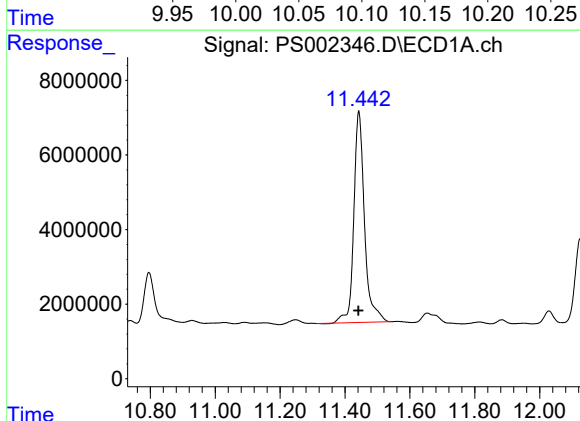


#4 2,4-DCAA

R.T.: 11.443 min
Delta R.T.: 0.002 min
Response: 129870765
Conc: 412.70 ng/ml

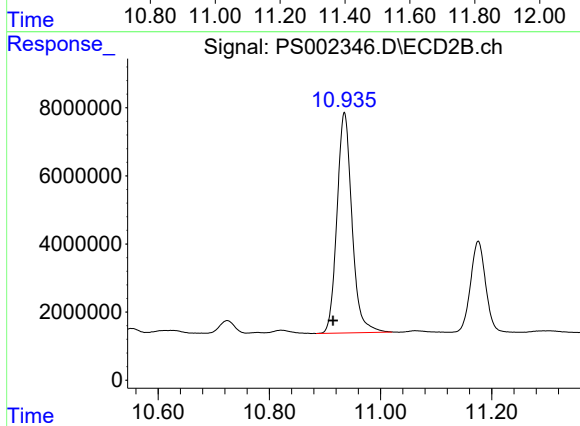

#4 2,4-DCAA


R.T.: 10.935 min
Delta R.T.: 0.021 min
Response: 121253920
Conc: 337.66 ng/ml

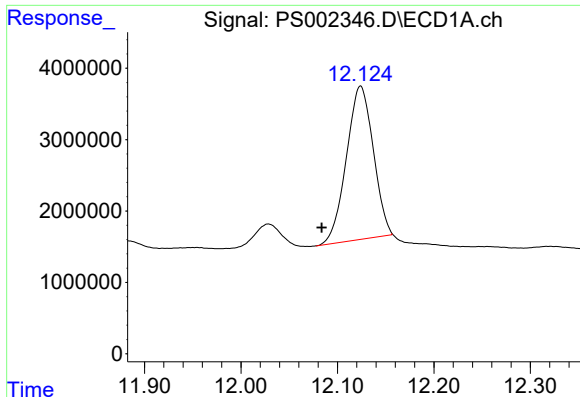

#6 MCPP


R.T.: 12.124 min
Delta R.T.: 0.040 min
Response: 41737121
Conc: 42.25 ug/ml

Instrument :
ECD_S
ClientSampleId :

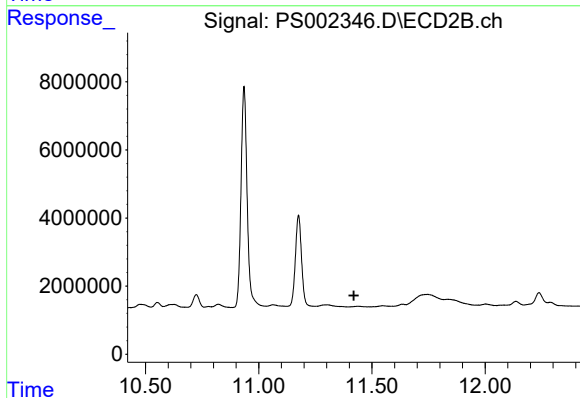


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

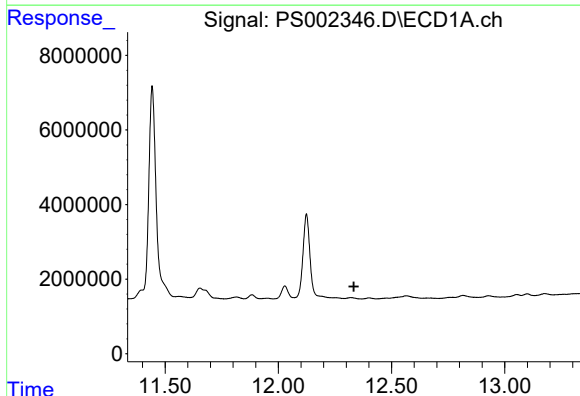


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

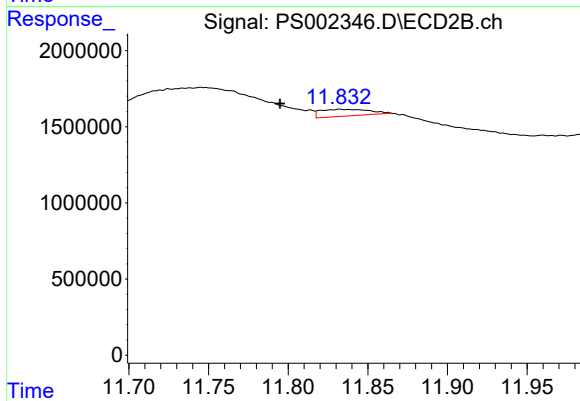

#7 MCPA


R.T.: 11.832 min
Delta R.T.: 0.038 min
Response: 998819
Conc: 0.74 ug/ml

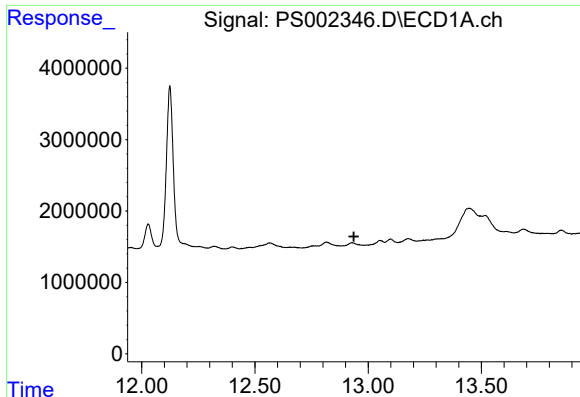

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

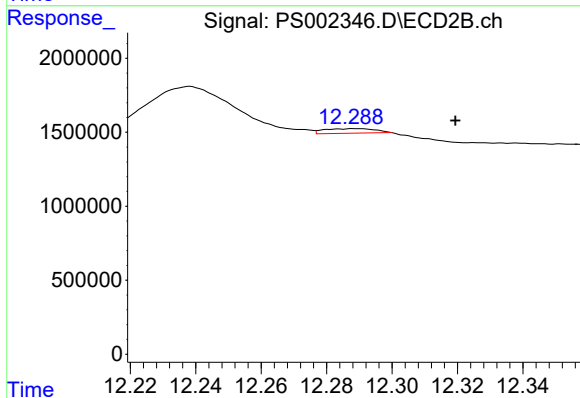


#8 DICHLORPROP

R.T.: 12.289 min
Delta R.T.: -0.030 min
Response: 345856
Conc: 1.08 ng/ml

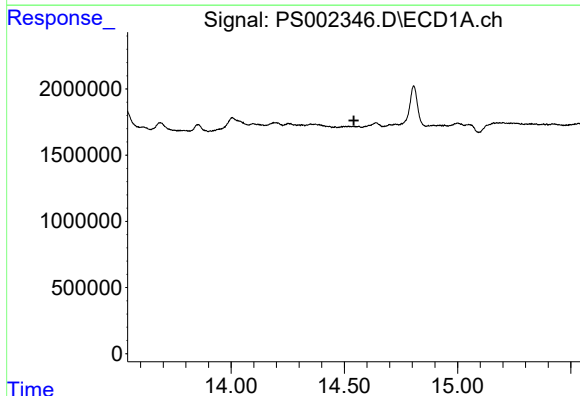


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.542 min
Response: 0
Conc: N.D.

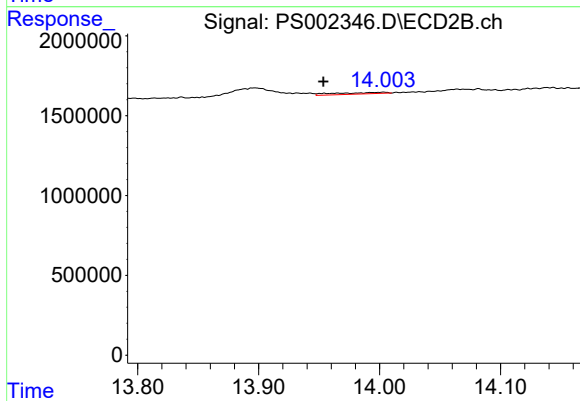

#11 2,4,5-TP (SILVEX)


R.T.: 14.003 min
Delta R.T.: 0.050 min
Response: 289595
Conc: 0.16 ng/ml

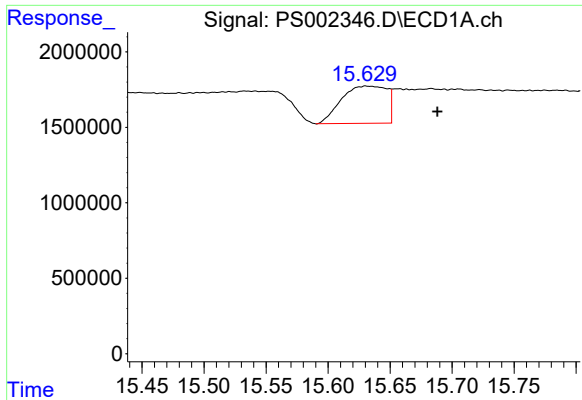

#13 2,4-DB


R.T.: 15.632 min
Delta R.T.: -0.056 min
Response: 6327690
Conc: 26.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

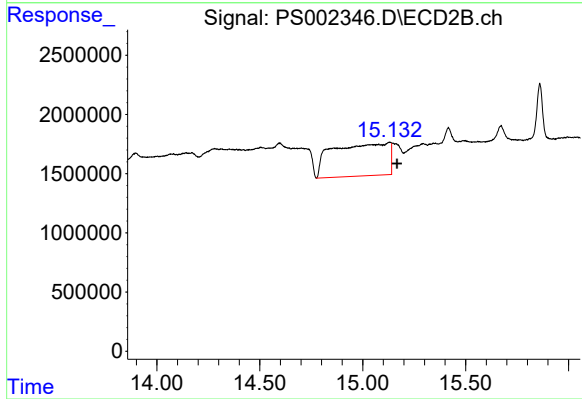


#13 2,4-DB

R.T.: 15.131 min
Delta R.T.: -0.036 min
Response: 52266379
Conc: 235.90 ng/ml

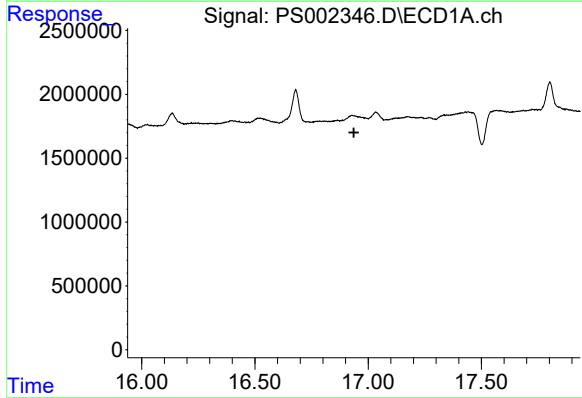


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

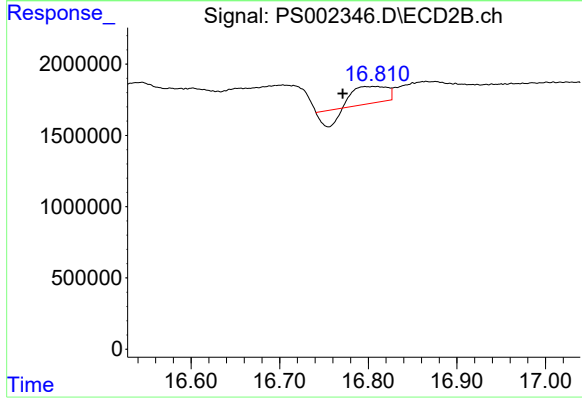

#15 Picloram


R.T.: 16.807 min
Delta R.T.: 0.036 min
Response: 2001535
Conc: 0.88 ng/ml

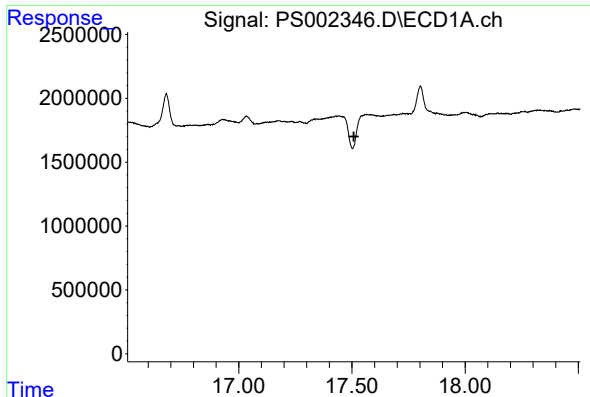

#16 DCPA

R.T.: 17.565 min
Delta R.T.: 0.056 min
Response: -380535
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

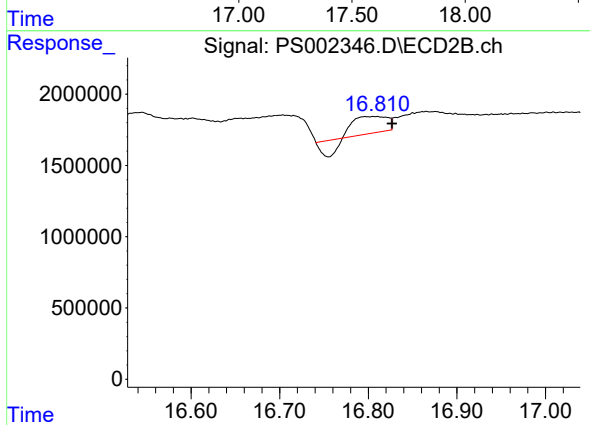

#16 DCPA

R.T.: 16.807 min
Delta R.T.: -0.019 min
Response: 2001535
Conc: 0.85 ng/ml