

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
 Data File : PS002348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 22:30
 Operator : EI\SJ
 Sample : J5812-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:36:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.458	10.951	142.4E6	131.5E6	452.366	366.092
Target Compounds							
1) T	Dalapon	2.934	2.387	11971559	16741028	26.101	37.078 #
2) T	3,5-DICHL...	0.000	9.045	0	10569474	N.D.	23.829 #
3) T	4-Nitroph...	0.000	10.108	0	1682726	N.D.	9.437 #
5) T	DICAMBA	0.000	11.191	0	32970557	N.D.	26.383 #
6) T	MCPD	12.043	0.000	6600704	0	6.682	N.D. #
7) T	MCPA	0.000	11.747	0	13568519	N.D.	10.025 #
8) T	DICHLORPROP	0.000	12.254	0	4177889	N.D.	13.010 #
9) T	2,4-D	0.000	12.784	0	646911	N.D.	1.519 #
11) T	2,4,5-TP ...	0.000	13.911	0	899056	N.D.	0.491 #
16) T	DCPA	0.000	16.823	0	649926	N.D.	0.274 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
Data File : PS002348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 22:30
Operator : EI\SJ
Sample : J5812-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:36:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

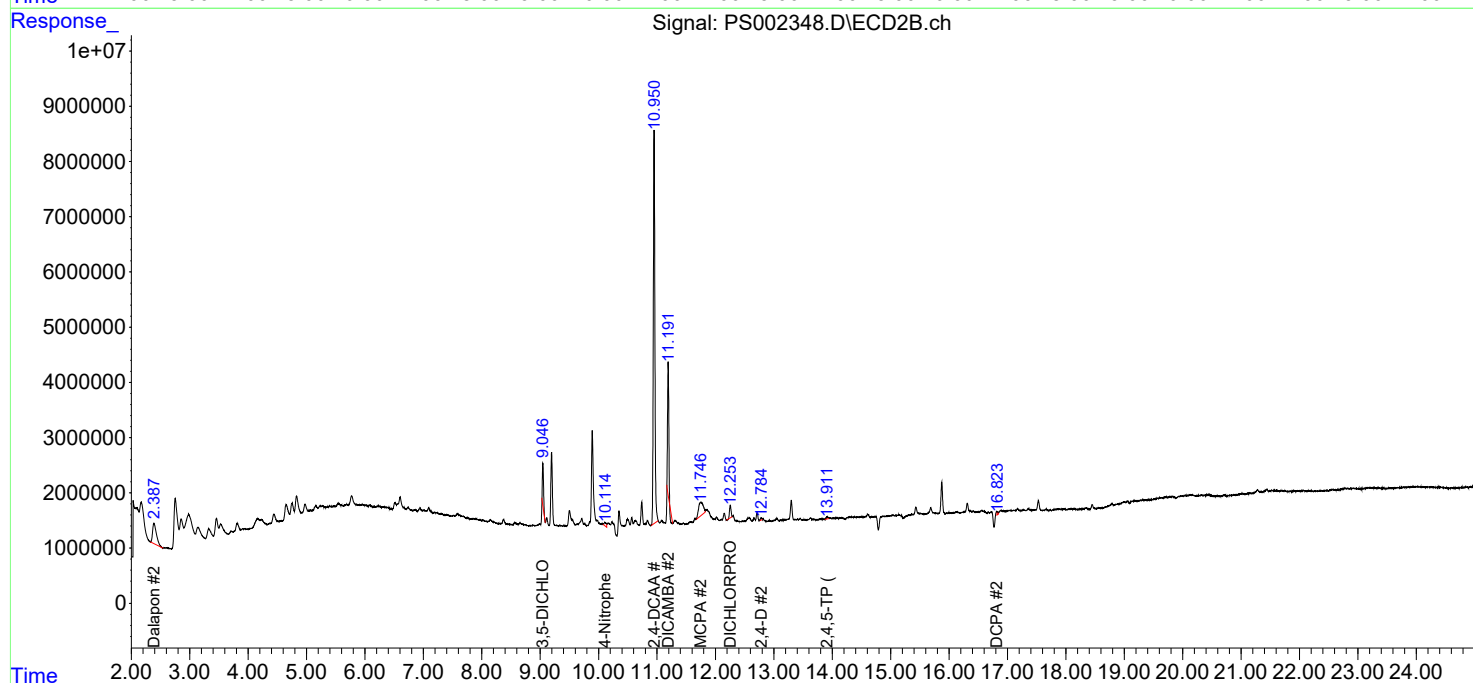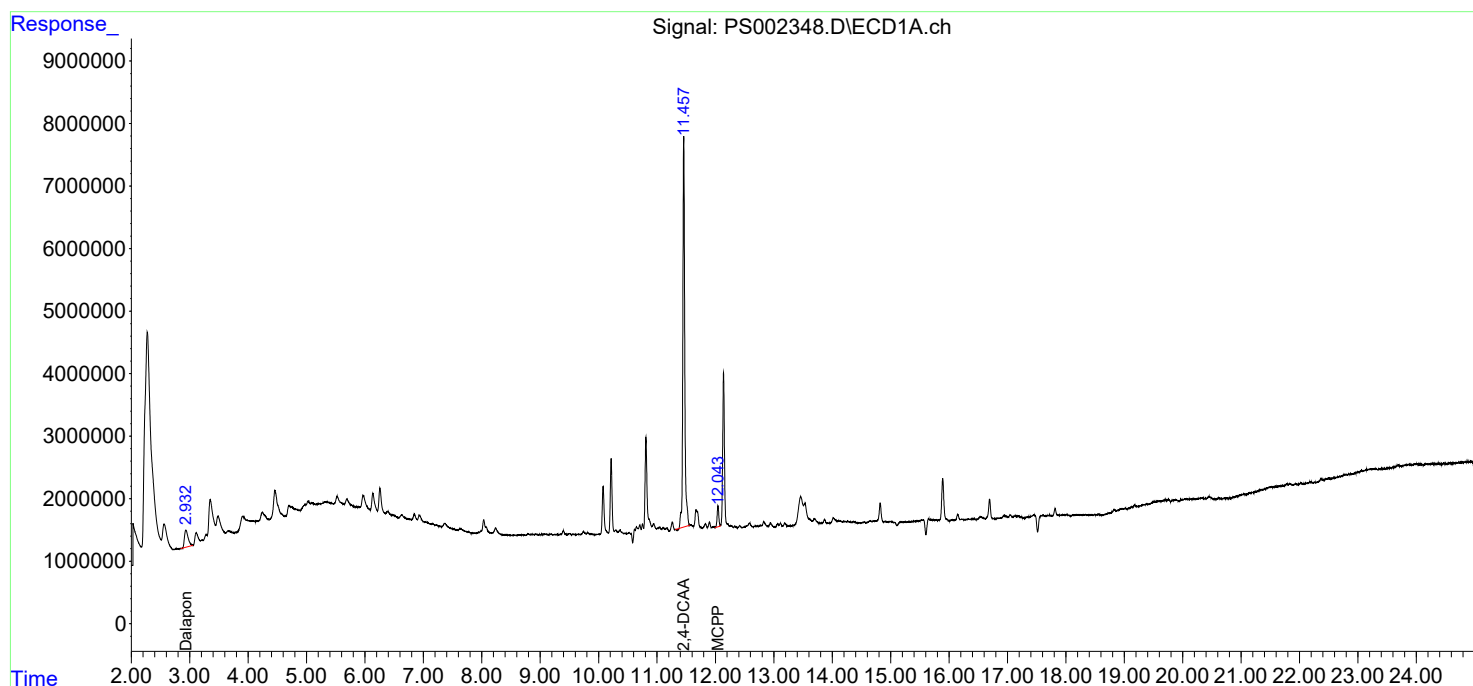


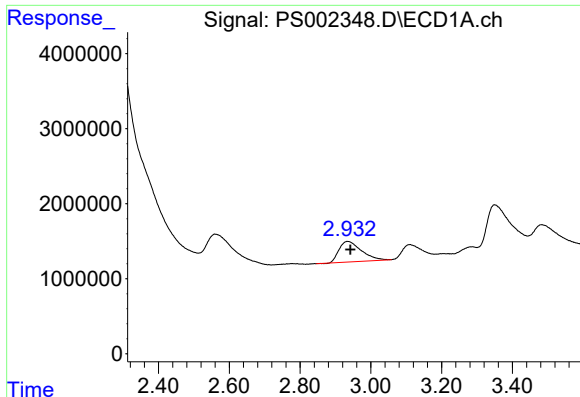

#1 Dalapon


R.T.: 2.934 min
Delta R.T.: -0.008 min
Response: 11971559
Conc: 26.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

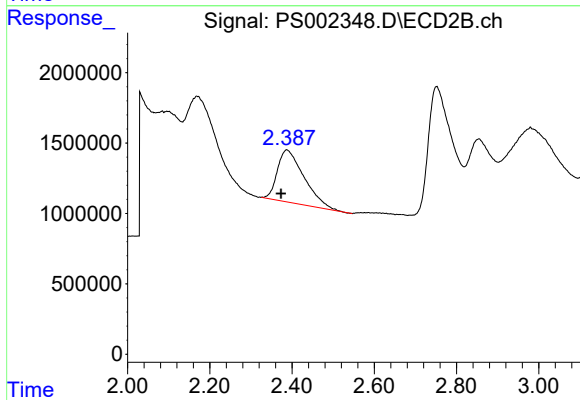


#1 Dalapon

R.T.: 2.387 min
Delta R.T.: 0.014 min
Response: 16741028
Conc: 37.08 ng/ml

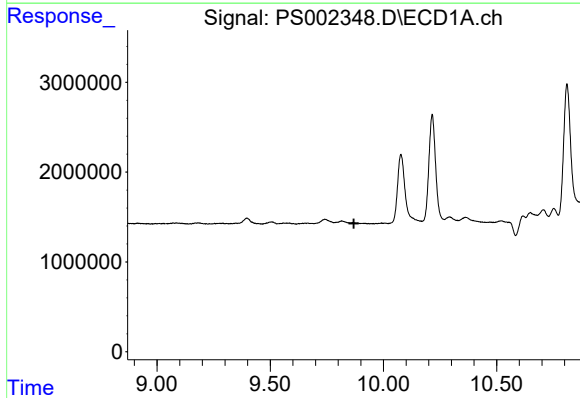


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

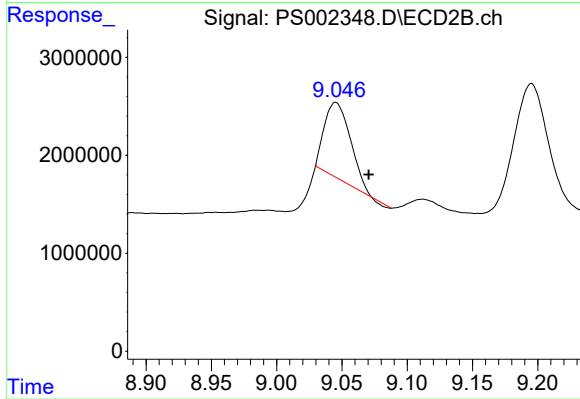

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.045 min
Delta R.T.: -0.025 min
Response: 10569474
Conc: 23.83 ng/ml

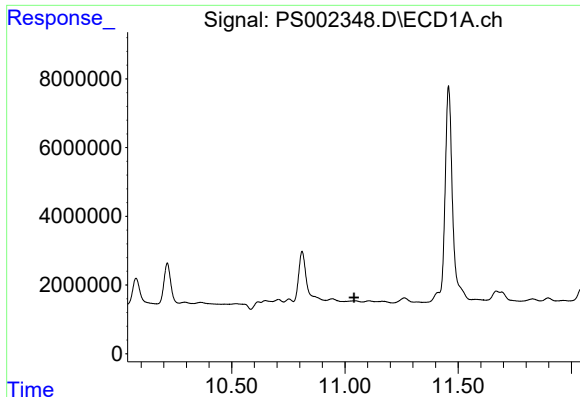

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

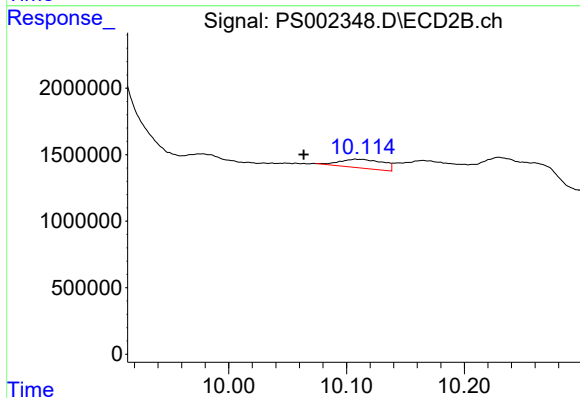


#3 4-Nitrophenol

R.T.: 10.108 min
Delta R.T.: 0.044 min
Response: 1682726
Conc: 9.44 ng/ml

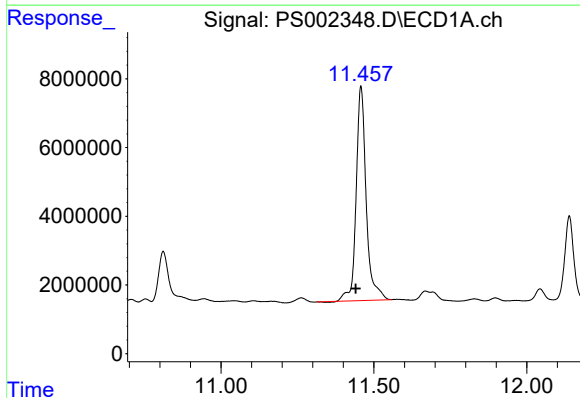


#4 2,4-DCAA

R.T.: 11.458 min
Delta R.T.: 0.017 min
Response: 142353012
Conc: 452.37 ng/ml

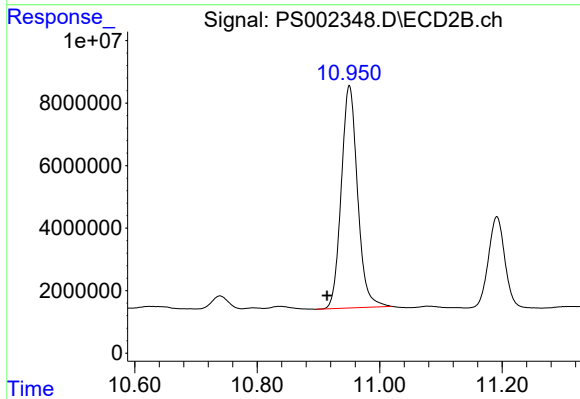

#4 2,4-DCAA


R.T.: 10.951 min
Delta R.T.: 0.036 min
Response: 131462775
Conc: 366.09 ng/ml

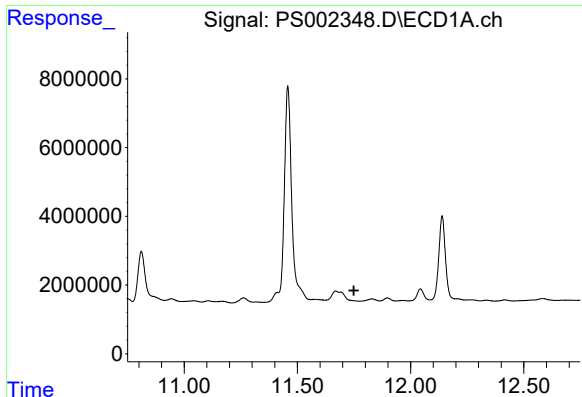

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

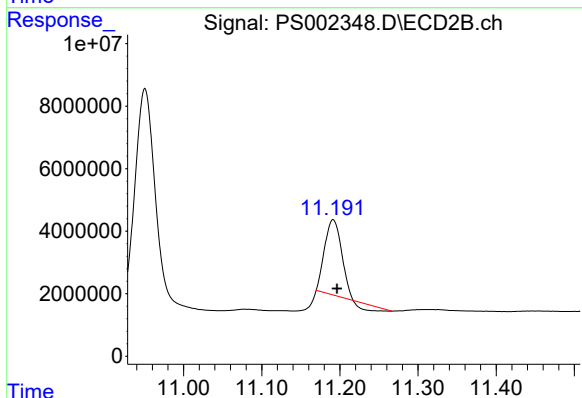


#5 DICAMBA

R.T.: 11.191 min
Delta R.T.: -0.005 min
Response: 32970557
Conc: 26.38 ng/ml

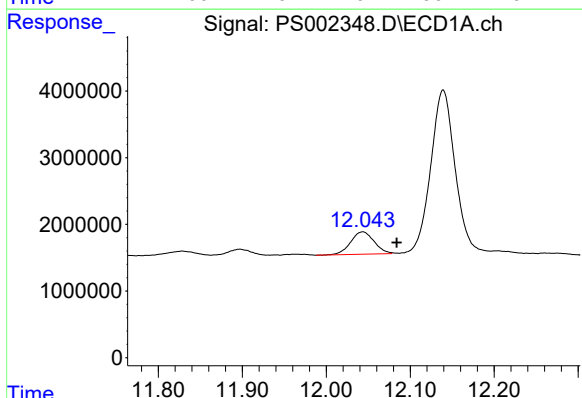


#6 MCPP

R.T.: 12.043 min
Delta R.T.: -0.040 min
Response: 6600704
Conc: 6.68 ug/ml

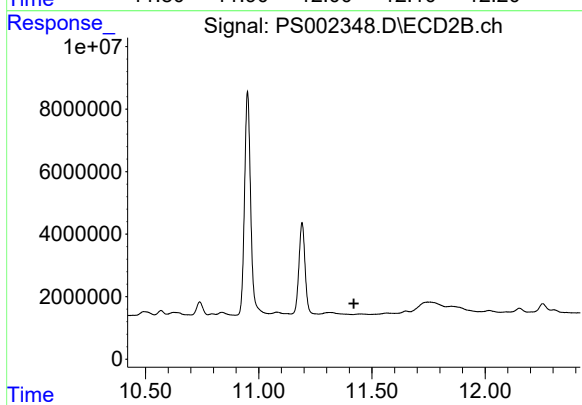

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.420 min
Response: 0
Conc: N.D.

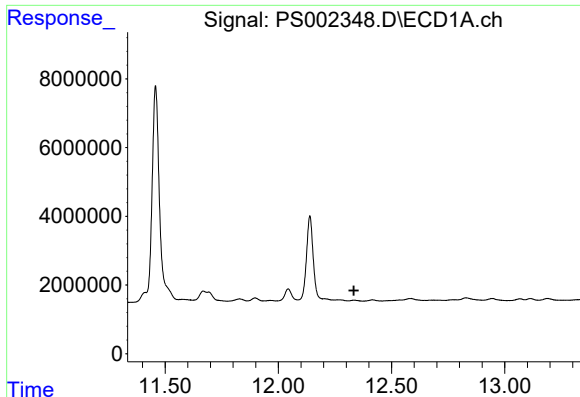

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

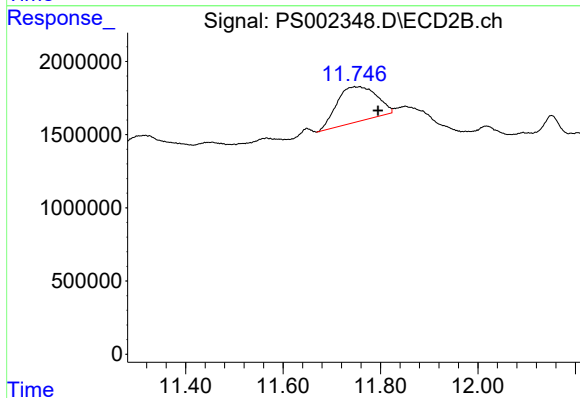


#7 MCPA

R.T.: 11.747 min
Delta R.T.: -0.048 min
Response: 13568519
Conc: 10.03 ug/ml

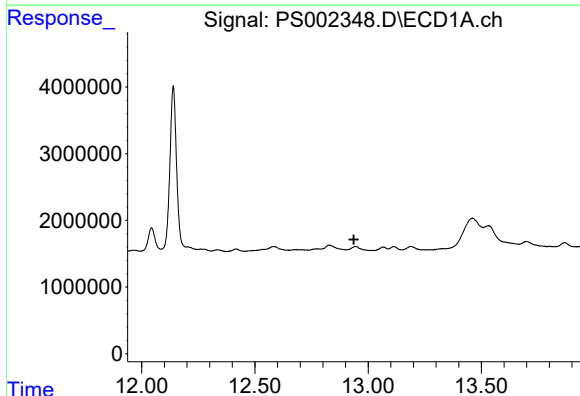


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

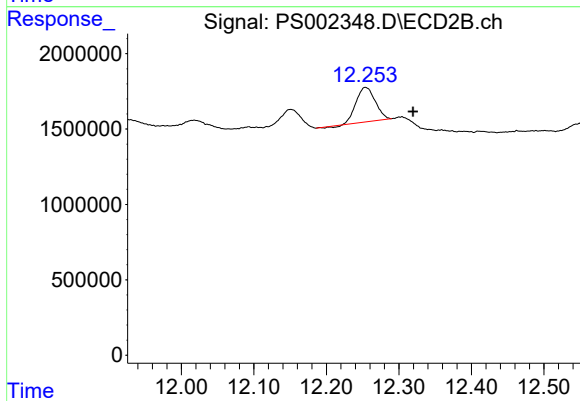

#8 DICHLORPROP


R.T.: 12.254 min
Delta R.T.: -0.066 min
Response: 4177889
Conc: 13.01 ng/ml

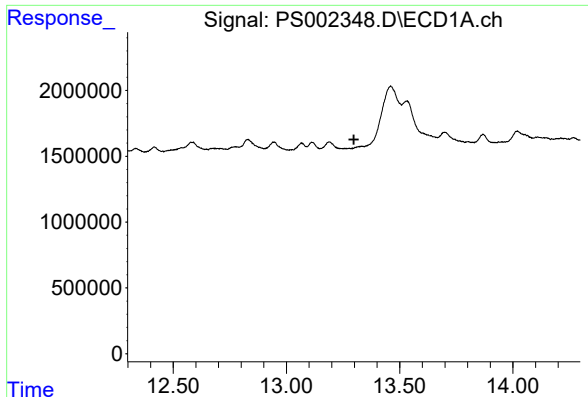

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

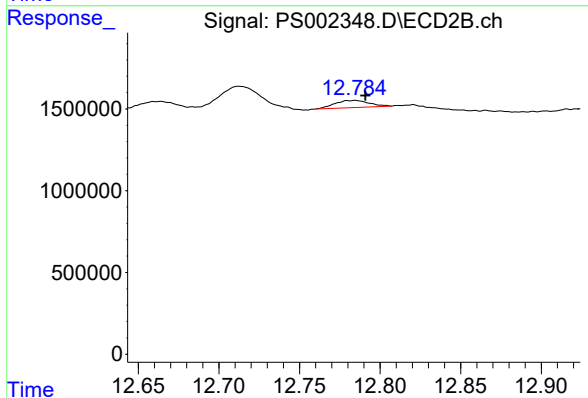


#9 2,4-D

R.T.: 12.784 min
Delta R.T.: -0.007 min
Response: 646911
Conc: 1.52 ng/ml

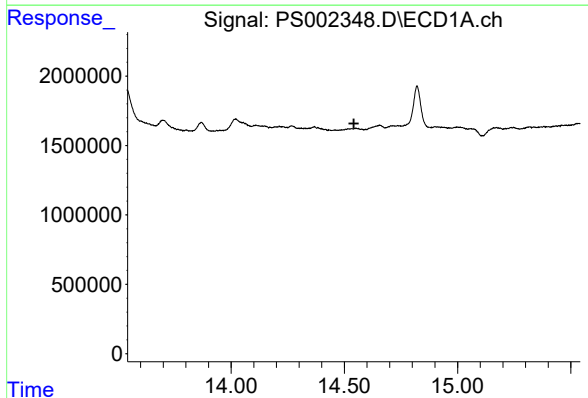


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

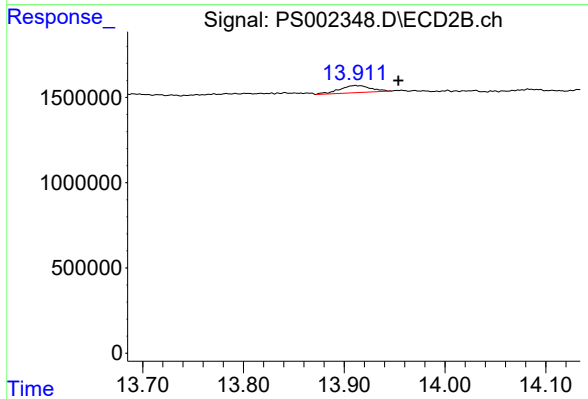

#11 2,4,5-TP (SILVEX)


R.T.: 13.911 min
Delta R.T.: -0.043 min
Response: 899056
Conc: 0.49 ng/ml

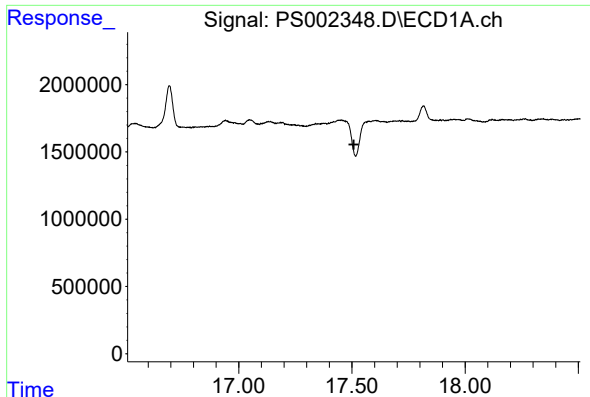

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

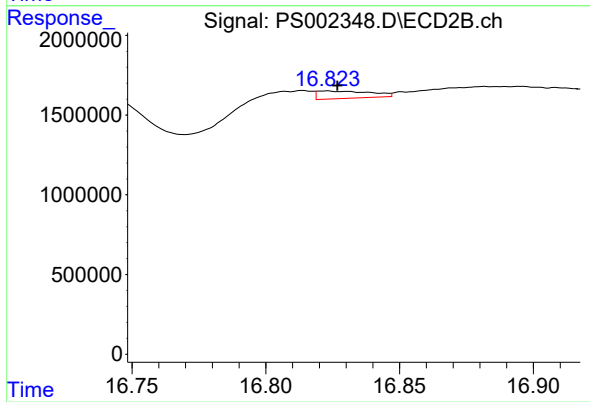

#16 DCPA

R.T.: 16.823 min
Delta R.T.: -0.004 min
Response: 649926
Conc: 0.27 ng/ml