

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
 Data File : PS002350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2018 23:32
 Operator : EI\SJ
 Sample : J5812-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 08:36:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.447	10.939	125.7E6	119.5E6	399.559	332.641
Target Compounds							
1) T	Dalapon	2.924	2.373	6246331	8475941	13.618	18.773 #
2) T	3,5-DICHL...	0.000	9.100	0	210574	N.D.	0.475 #
3) T	4-Nitroph...	0.000	10.096	0	2062758	N.D.	11.568 #
6) T	MCP	12.129	11.450	38347756	629964	38.819	0.732 #
7) T	MCPA	0.000	11.840	0	1206265	N.D.	0.891 #
8) T	DICHLORPROP	0.000	12.292	0	159286	N.D.	0.496 #
11) T	2,4,5-TP ...	0.000	14.004	0	414165	N.D.	0.226 #
15) T	Picloram	0.000	16.809	0	682415	N.D.	0.302 #
16) T	DCPA	0.000	16.809	0	682415	N.D.	0.288 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110618\
Data File : PS002350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2018 23:32
Operator : EI\SJ
Sample : J5812-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:36:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

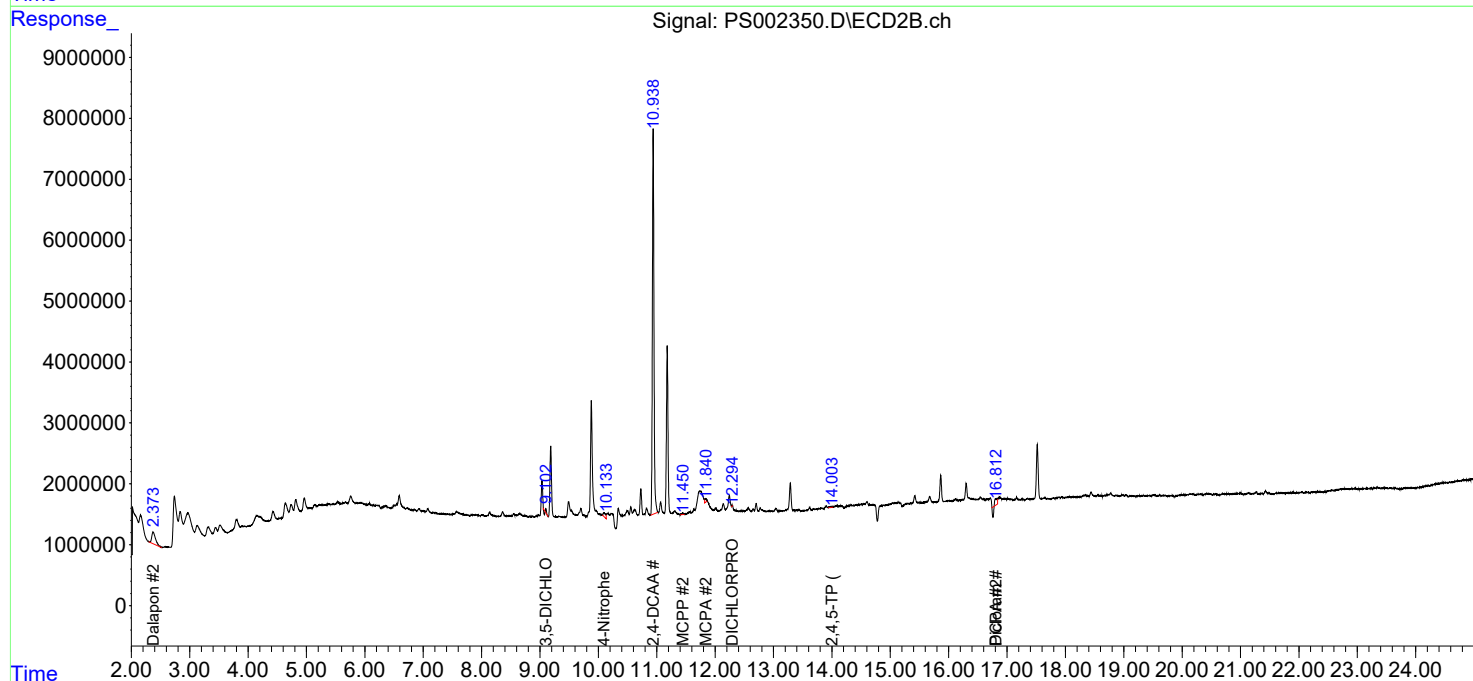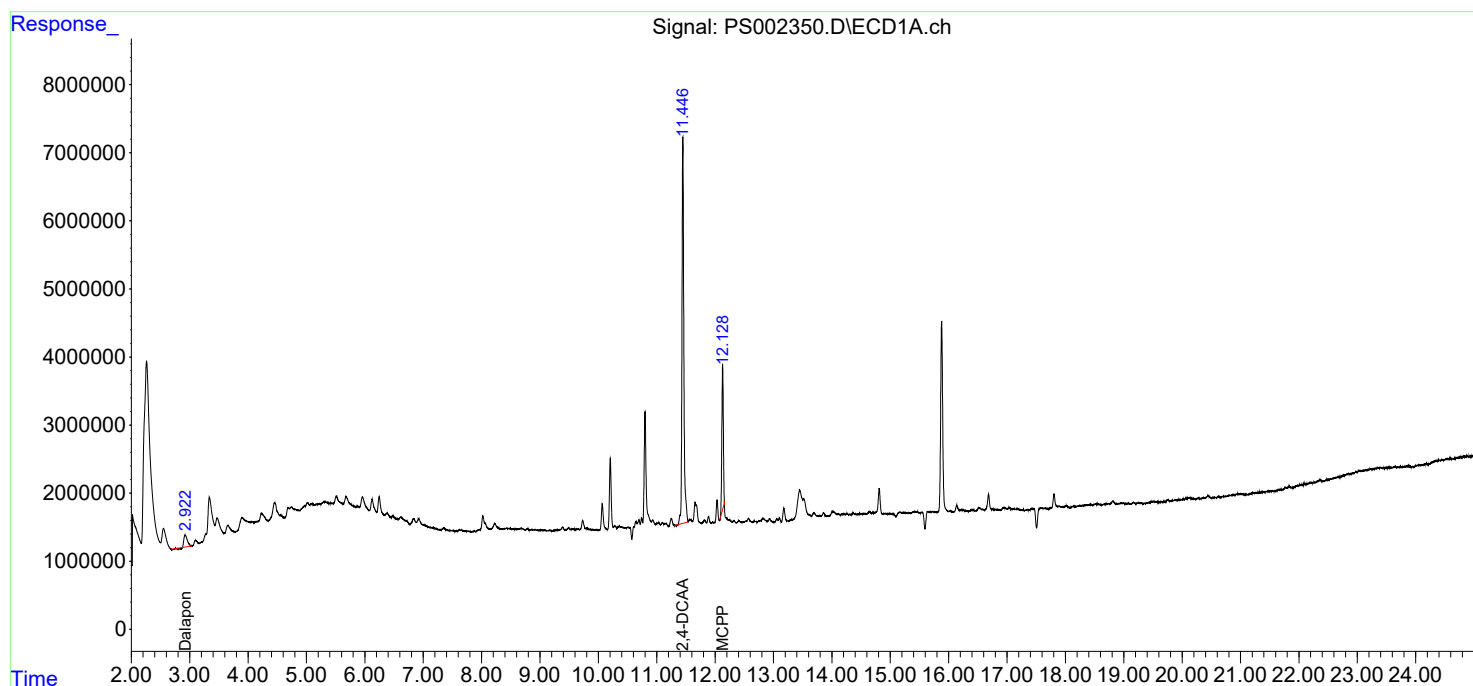


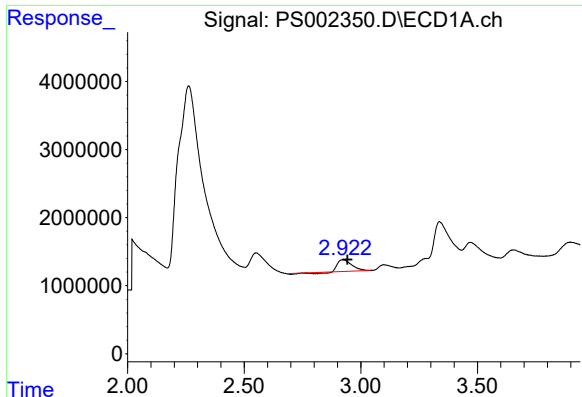

#1 Dalapon


R.T.: 2.924 min
Delta R.T.: -0.018 min
Response: 6246331
Conc: 13.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

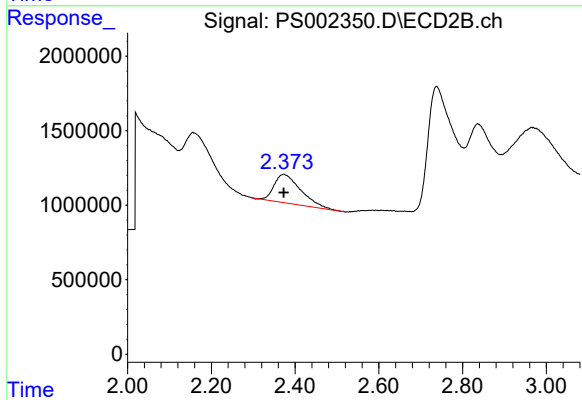


#1 Dalapon

R.T.: 2.373 min
Delta R.T.: 0.000 min
Response: 8475941
Conc: 18.77 ng/ml

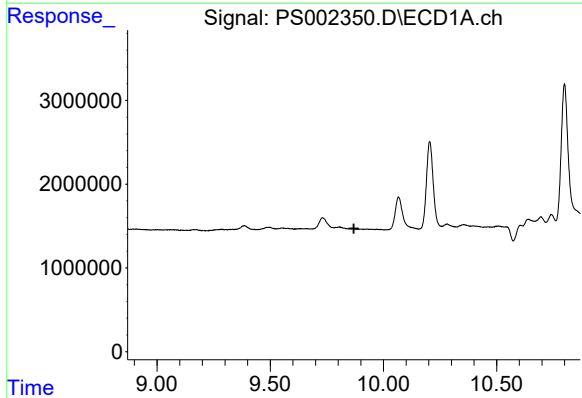


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

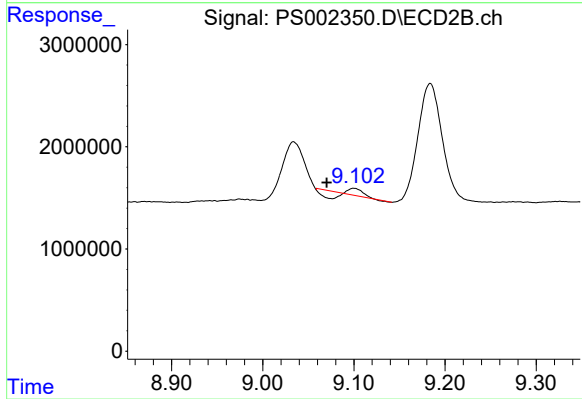

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.100 min
Delta R.T.: 0.030 min
Response: 210574
Conc: 0.47 ng/ml

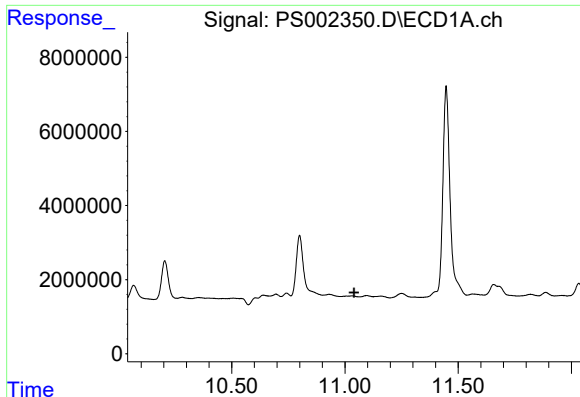

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

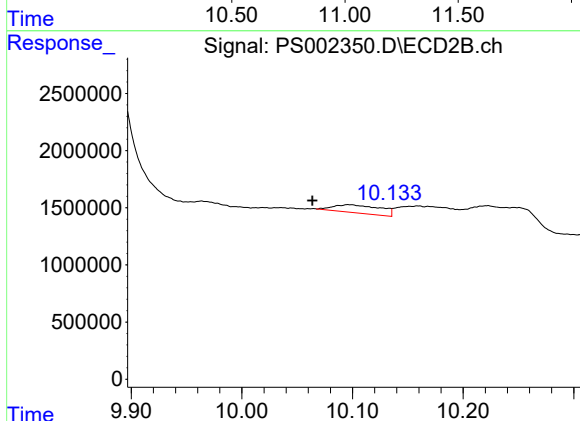


#3 4-Nitrophenol

R.T.: 10.096 min
Delta R.T.: 0.032 min
Response: 2062758
Conc: 11.57 ng/ml

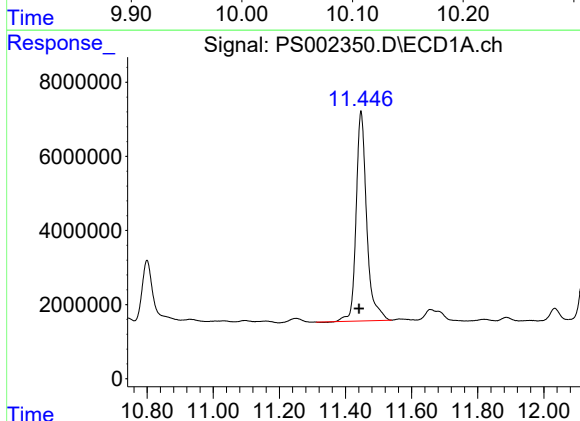


#4 2,4-DCAA

R.T.: 11.447 min
Delta R.T.: 0.006 min
Response: 125735408
Conc: 399.56 ng/ml

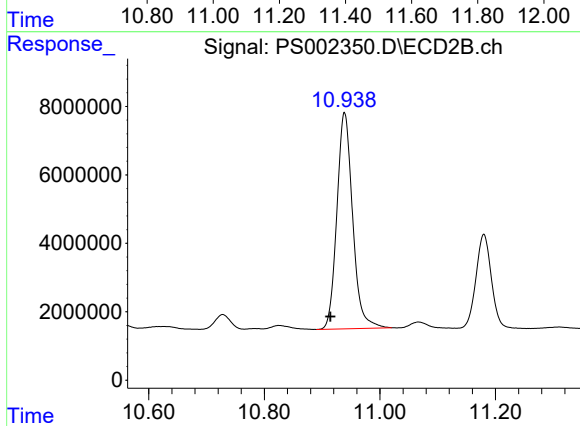

#4 2,4-DCAA


R.T.: 10.939 min
Delta R.T.: 0.025 min
Response: 119450524
Conc: 332.64 ng/ml

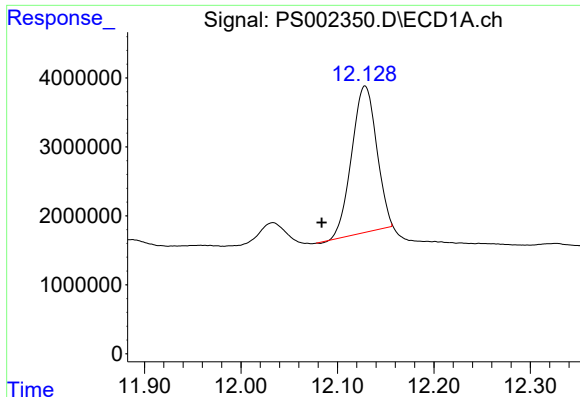

#6 MCPP


R.T.: 12.129 min
Delta R.T.: 0.045 min
Response: 38347756
Conc: 38.82 ug/ml

Instrument :
ECD_S
ClientSampleId :

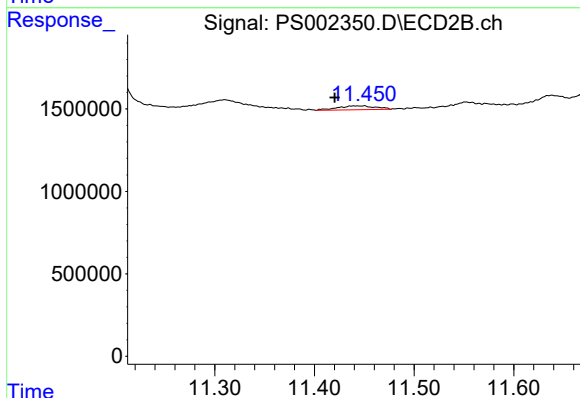


#6 MCPP

R.T.: 11.450 min
Delta R.T.: 0.029 min
Response: 629964
Conc: 0.73 ug/ml

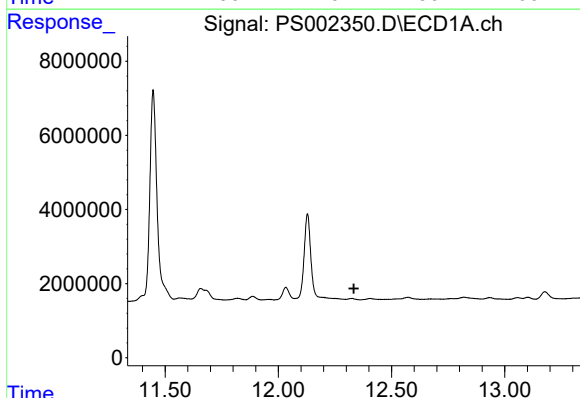


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

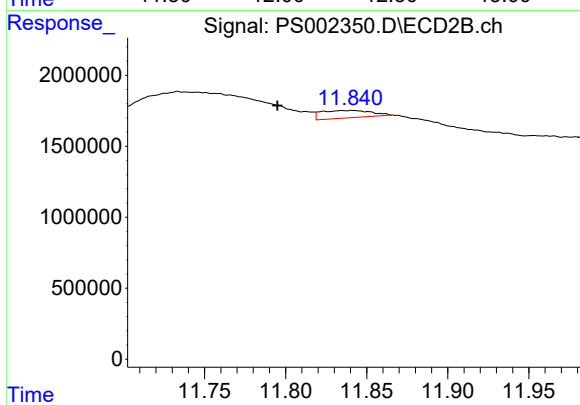

#7 MCPA


R.T.: 11.840 min
Delta R.T.: 0.046 min
Response: 1206265
Conc: 0.89 ug/ml

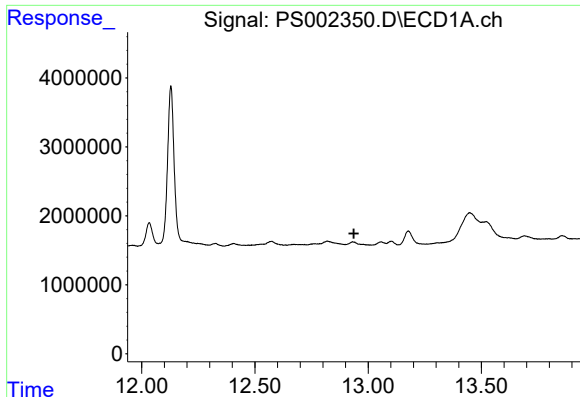

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

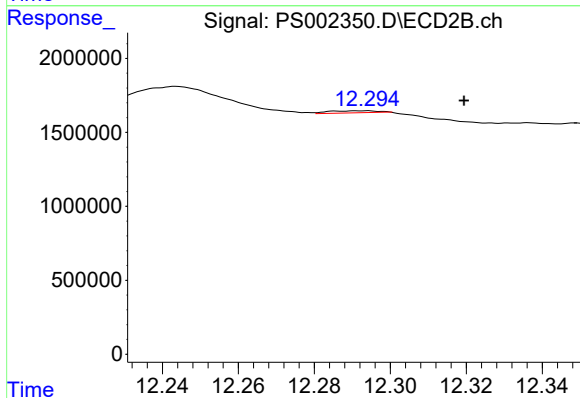


#8 DICHLORPROP

R.T.: 12.292 min
Delta R.T.: -0.028 min
Response: 159286
Conc: 0.50 ng/ml

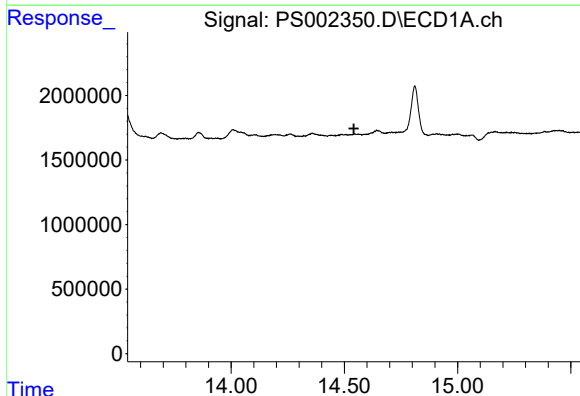


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

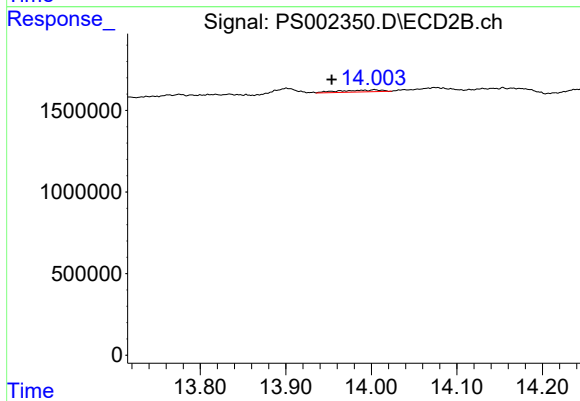

#11 2,4,5-TP (SILVEX)


R.T.: 14.004 min
Delta R.T.: 0.050 min
Response: 414165
Conc: 0.23 ng/ml

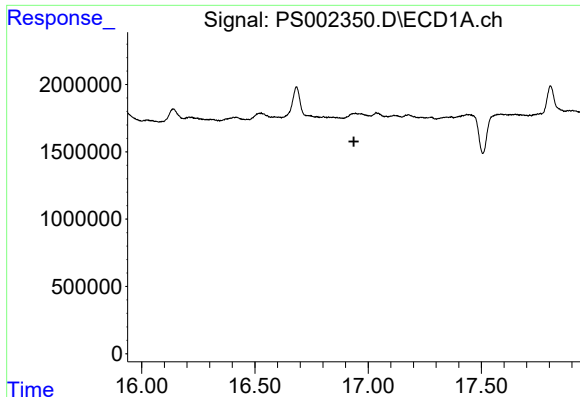

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

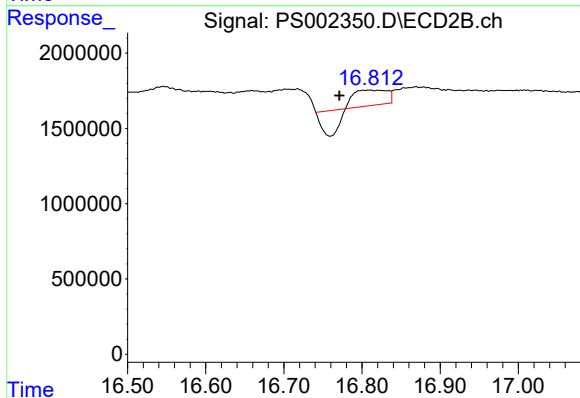


#15 Picloram

R.T.: 16.809 min
Delta R.T.: 0.038 min
Response: 682415
Conc: 0.30 ng/ml

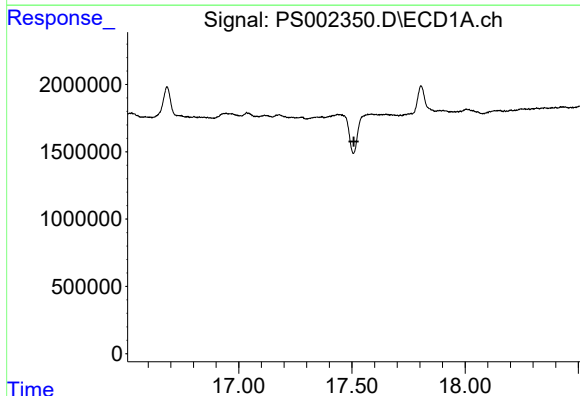

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

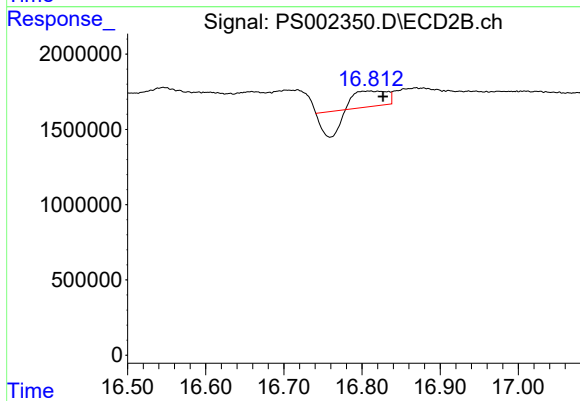

#16 DCPA

R.T.: 16.809 min
Delta R.T.: -0.018 min
Response: 682415
Conc: 0.29 ng/ml