

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110619\
 Data File : PS007626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2019 18:14
 Operator : SM\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 02:31:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:24:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.428	5.153	1023.7E6	519.4E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.012	1.723	1227.0E6	729.5E6	682.500	682.500
2) T	3,5-DICHL...	4.804	4.462	1246.6E6	626.3E6	697.500	697.500
3) T	4-Nitroph...	5.283	4.843	424.1E6	267.7E6	682.500	682.500
5) T	DICAMBA	5.577	5.277	3589.5E6	1864.6E6	705.000	705.000
6) T	MCPD	5.729	5.361	273.2E6	137.0E6	70.500	70.500
7) T	MCPA	5.860	5.536	384.7E6	206.9E6	69.750	69.750
8) T	DICHLORPROP	6.200	5.804	883.9E6	459.4E6	705.000	705.000
9) T	2,4-D	6.414	6.072	977.6E6	565.9E6	705.000	705.000
10) T	Pentachlo...	6.671	6.435	13478.2E6	6963.7E6	712.500	712.500
11) T	2,4,5-TP ...	7.203	6.797	5330.0E6	2792.5E6	712.500	712.500
12) T	2,4,5-T	7.475	7.156	5825.3E6	2663.7E6	712.500	712.500
13) T	2,4-DB	8.002	7.640	794.1E6	352.4E6	712.500	712.500
14) T	DINOSEB	9.083	7.948	4184.6E6	2035.6E6	705.000	705.000
15) T	Picloram	8.918	8.882	8165.4E6	4289.2E6	712.500	712.500
16) T	DCPA	9.357	8.840	6921.4E6	3710.9E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110619\
Data File : PS007626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2019 18:14
Operator : SM\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 02:31:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:24:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

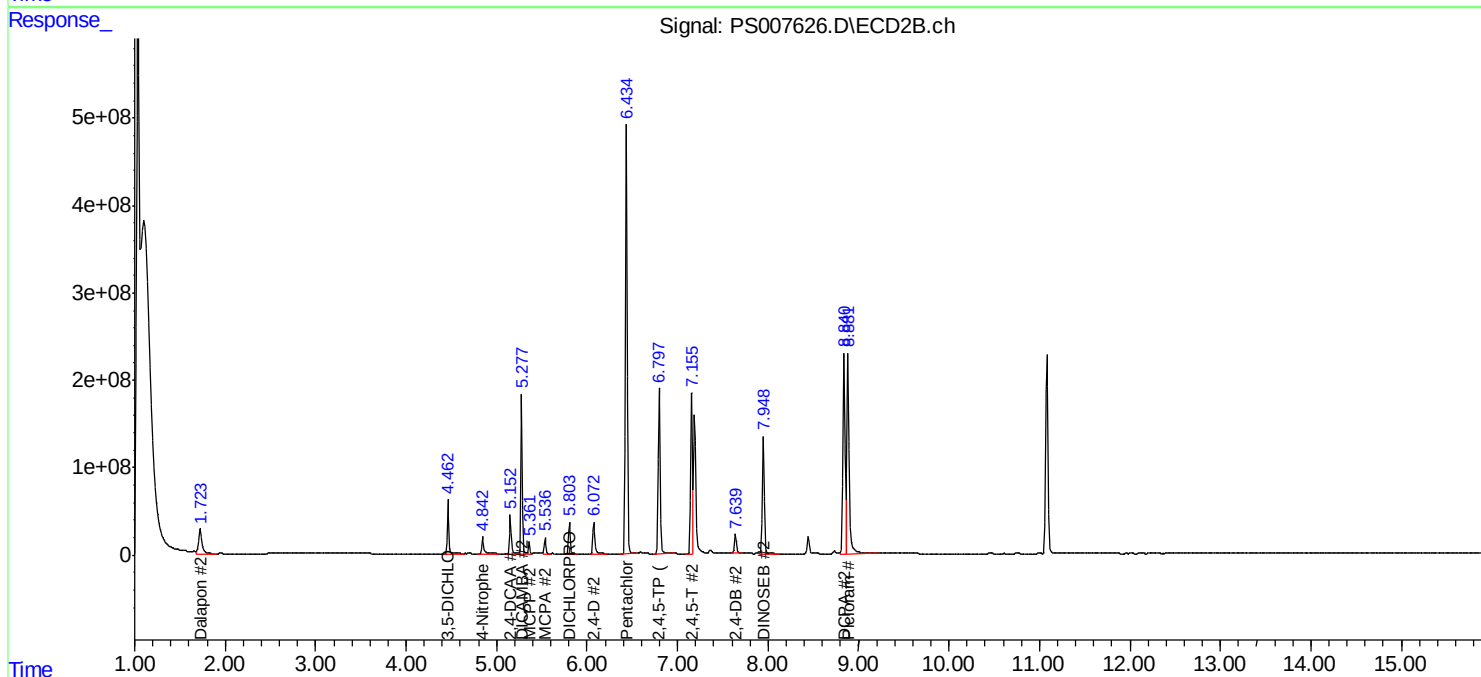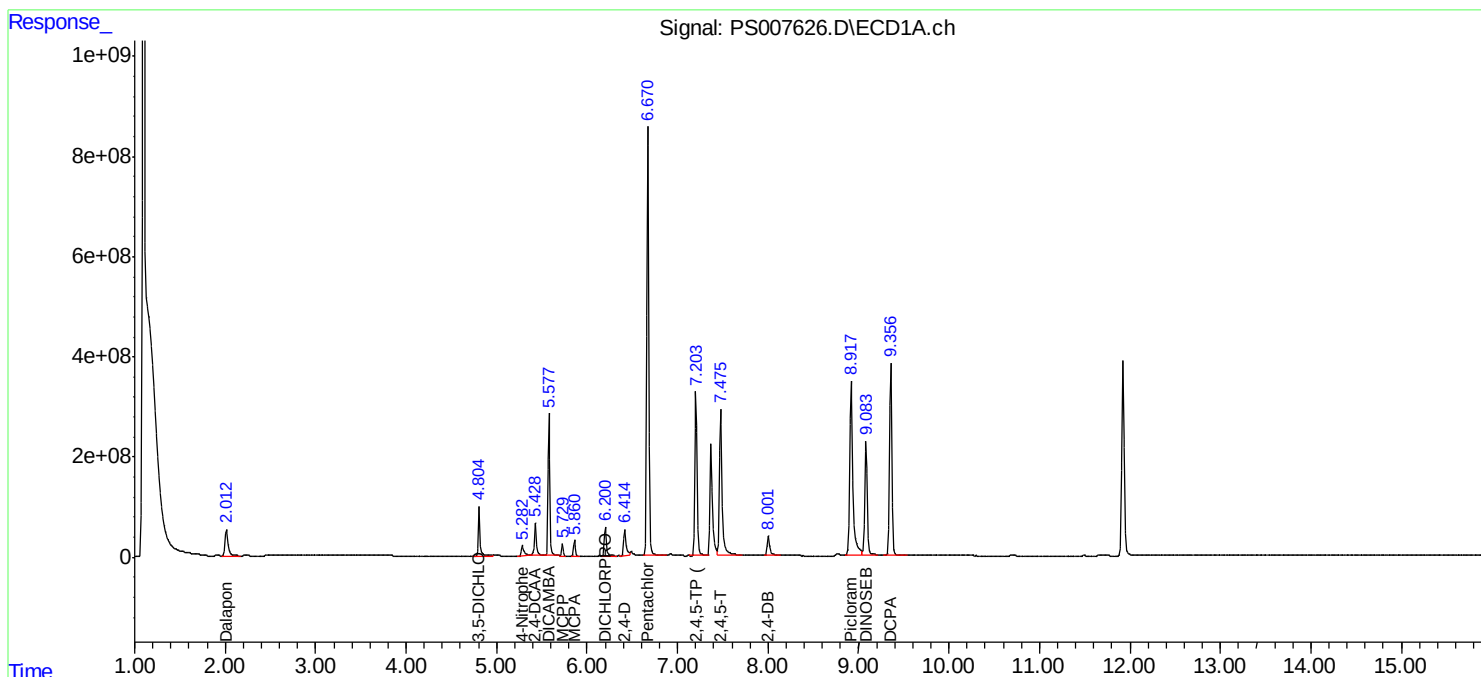


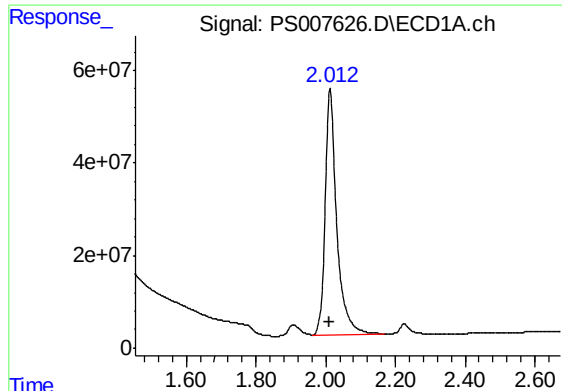

#1 Dalapon


R.T.: 2.012 min
Delta R.T.: 0.000 min
Response: 1226952545
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

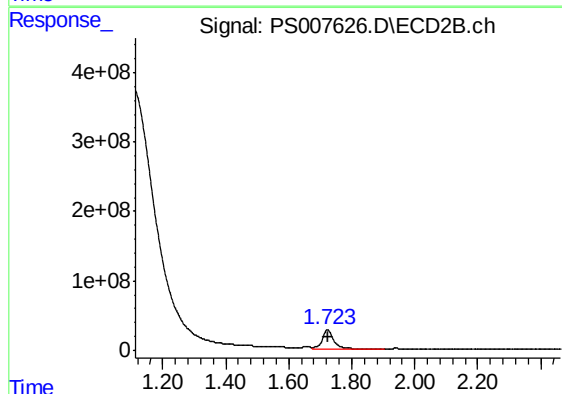


#1 Dalapon

R.T.: 1.723 min
Delta R.T.: 0.000 min
Response: 729465521
Conc: 682.50 ng/ml

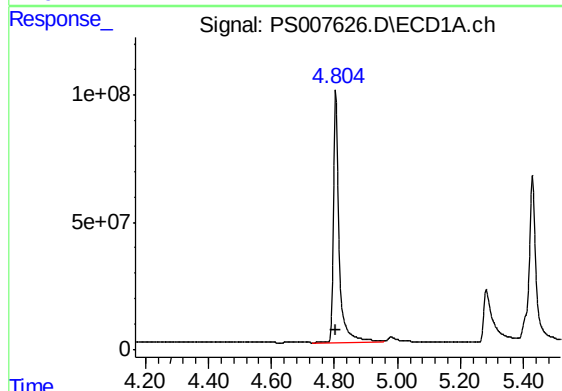


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 1246639531
Conc: 697.50 ng/ml

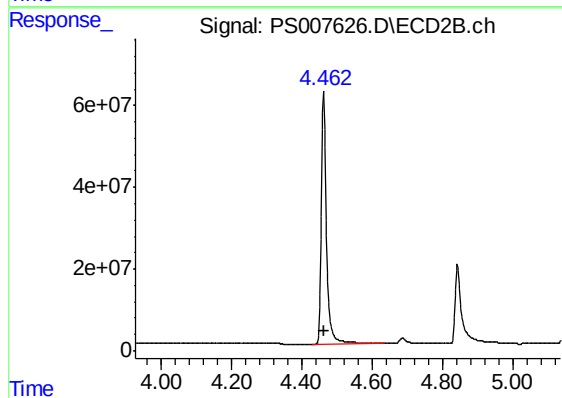

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 626283947
Conc: 697.50 ng/ml

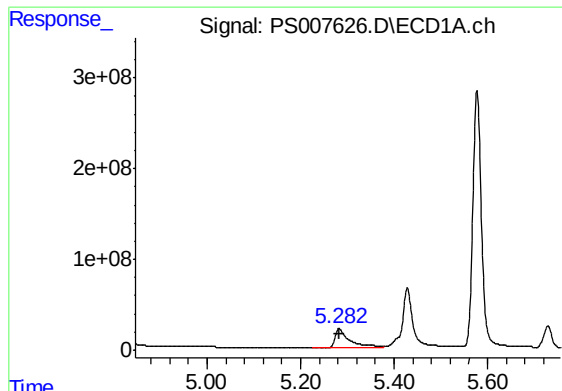

#3 4-Nitrophenol


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 424105237
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

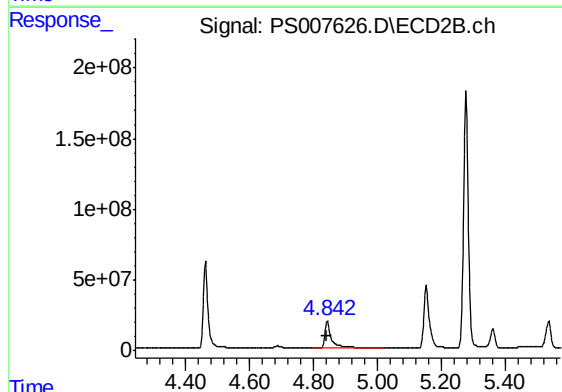


#3 4-Nitrophenol

R.T.: 4.843 min
Delta R.T.: 0.000 min
Response: 267675693
Conc: 682.50 ng/ml

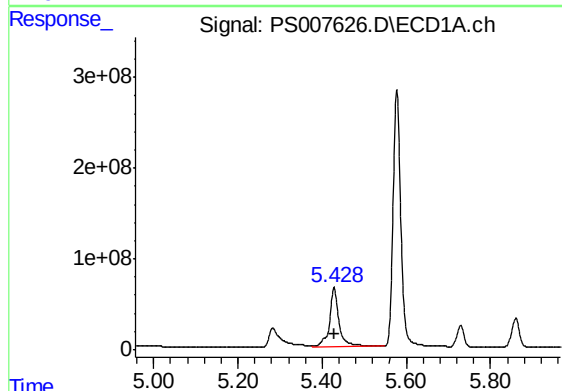


#4 2,4-DCAA

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 1023723773
Conc: 750.00 ng/ml

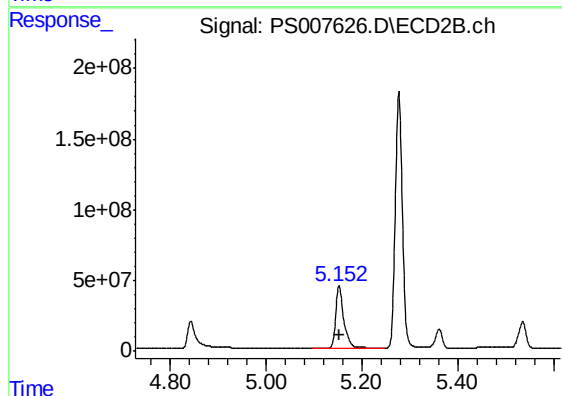

#4 2,4-DCAA


R.T.: 5.153 min
Delta R.T.: 0.000 min
Response: 519378864
Conc: 750.00 ng/ml

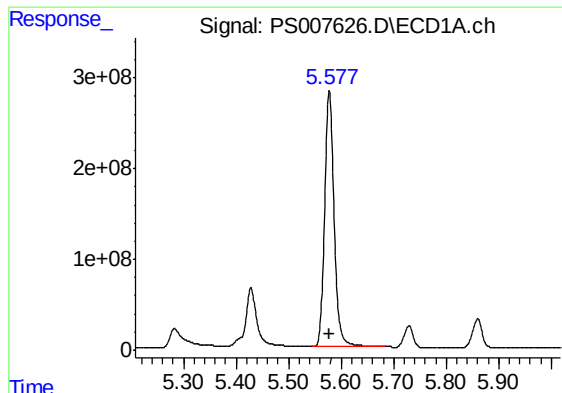

#5 DICAMBA


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 3589458519
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

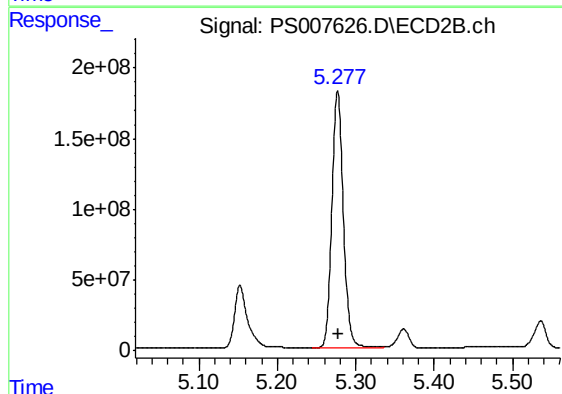


#5 DICAMBA

R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 1864602962
Conc: 705.00 ng/ml

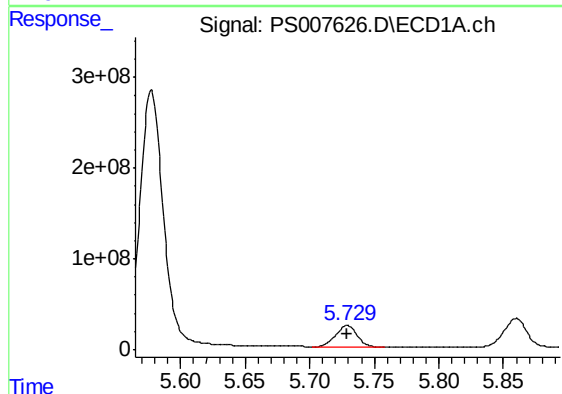


#6 MCPP

R.T.: 5.729 min
Delta R.T.: 0.000 min
Response: 273224067
Conc: 70.50 ug/ml

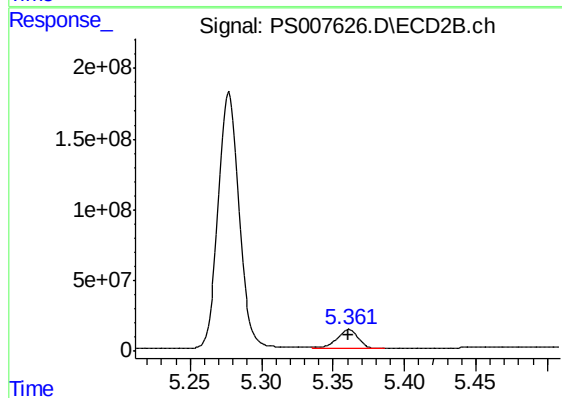

#6 MCPP


R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 137047204
Conc: 70.50 ug/ml

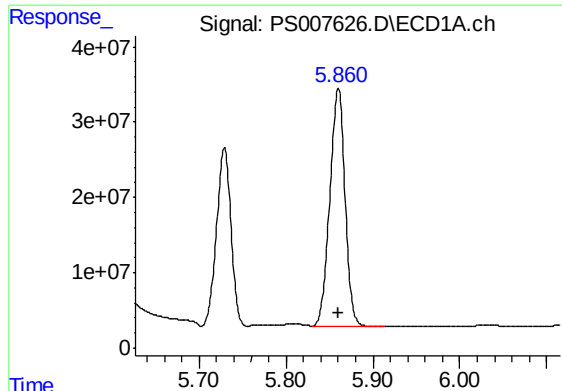

#7 MCPA


R.T.: 5.860 min
Delta R.T.: 0.000 min
Response: 384664360
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

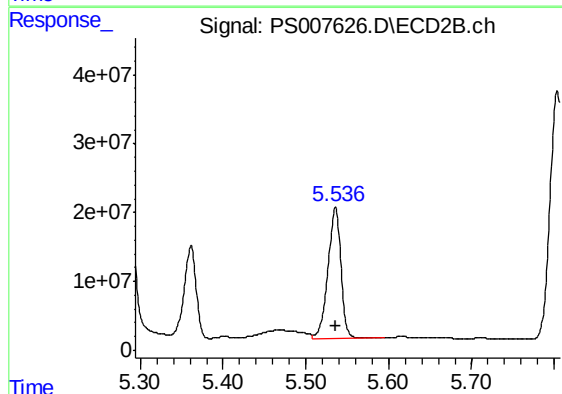


#7 MCPA

R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 206907421
Conc: 69.75 ug/ml

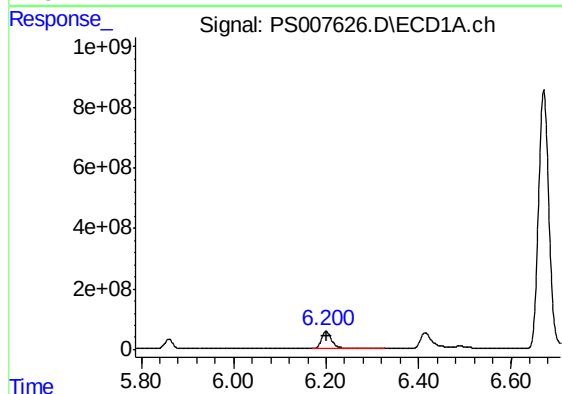


#8 DICHLORPROP

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 883864744
Conc: 705.00 ng/ml

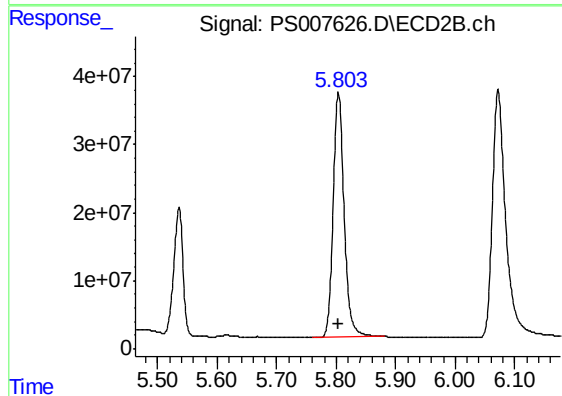

#8 DICHLORPROP


R.T.: 5.804 min
Delta R.T.: 0.000 min
Response: 459439697
Conc: 705.00 ng/ml

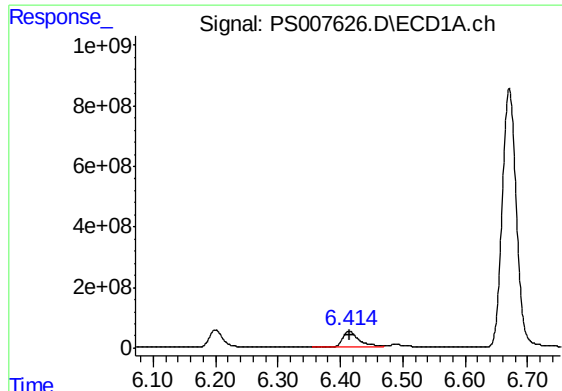

#9 2,4-D


R.T.: 6.414 min
Delta R.T.: 0.000 min
Response: 977589501
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

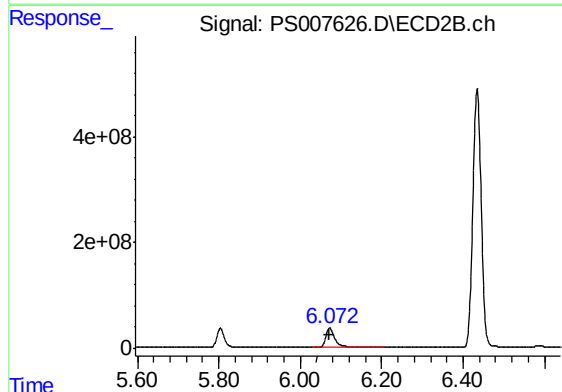


#9 2,4-D

R.T.: 6.072 min
Delta R.T.: 0.000 min
Response: 565853475
Conc: 705.00 ng/ml

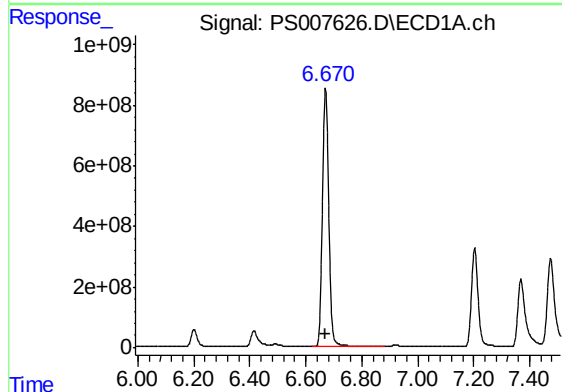


#10 Pentachlorophenol

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 13478153789
Conc: 712.50 ng/ml

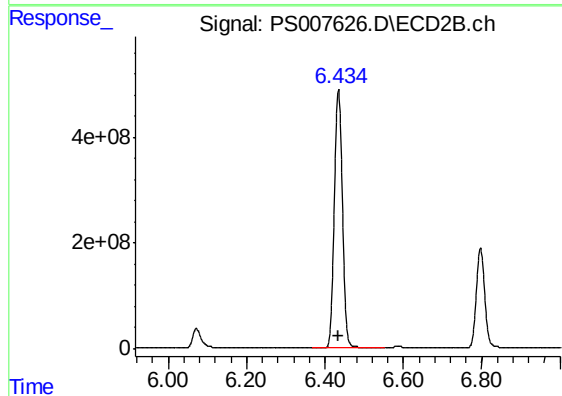

#10 Pentachlorophenol


R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 6963654696
Conc: 712.50 ng/ml

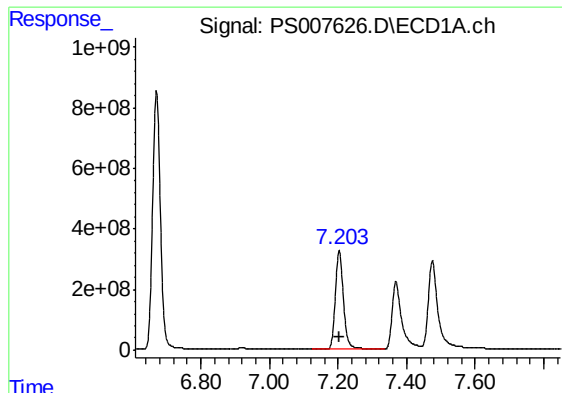

#11 2,4,5-TP (SILVEX)


R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 5329970292
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

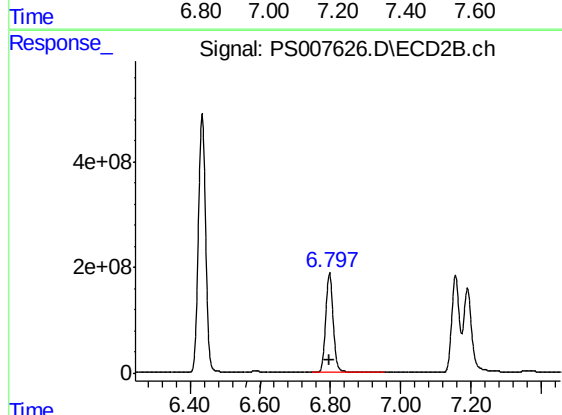


#11 2,4,5-TP (SILVEX)

R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 2792472908
Conc: 712.50 ng/ml

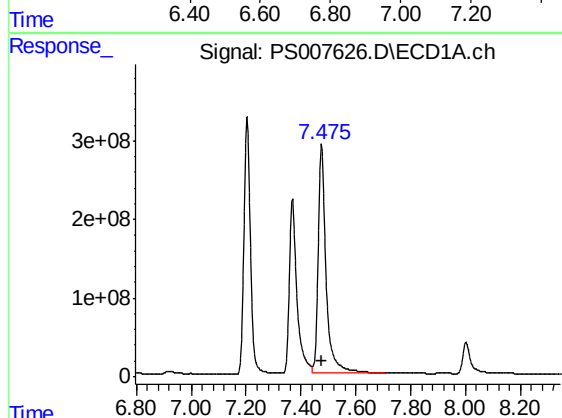


#12 2,4,5-T

R.T.: 7.475 min
Delta R.T.: 0.000 min
Response: 5825306131
Conc: 712.50 ng/ml

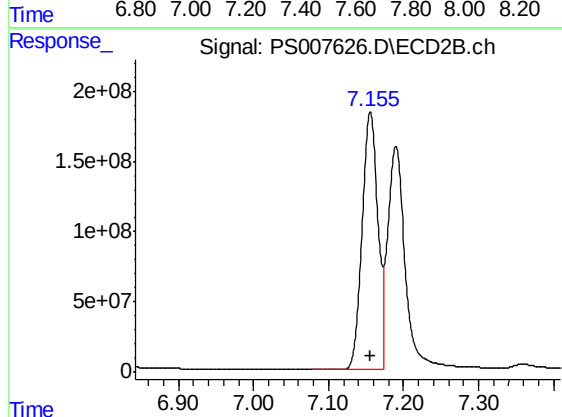

#12 2,4,5-T


R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 2663730565
Conc: 712.50 ng/ml

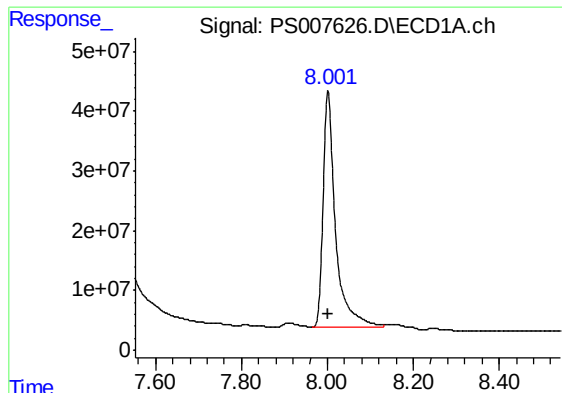

#13 2,4-DB


R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 794145267
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

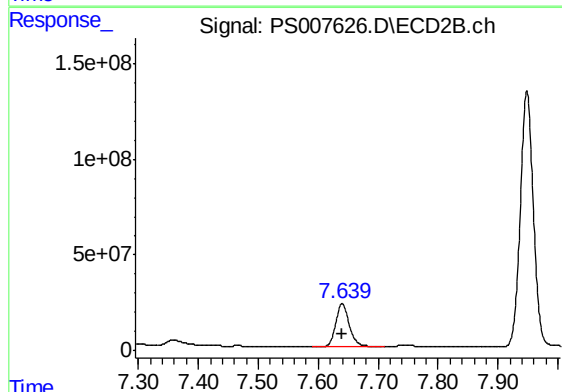


#13 2,4-DB

R.T.: 7.640 min
Delta R.T.: 0.000 min
Response: 352358972
Conc: 712.50 ng/ml

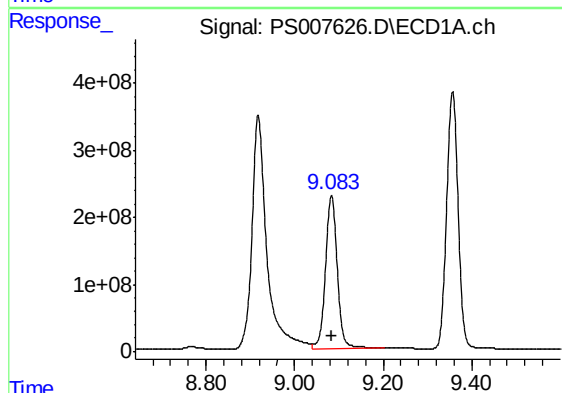


#14 DINOSEB

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 4184643268
Conc: 705.00 ng/ml

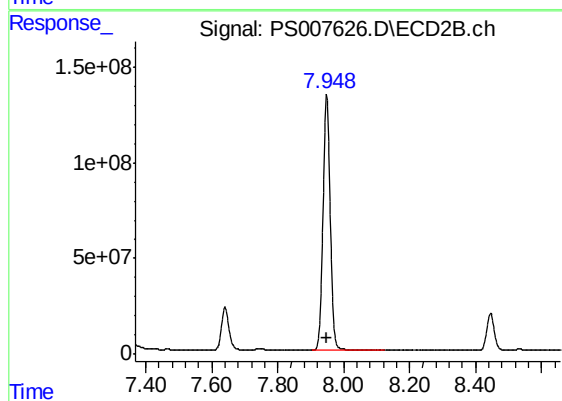

#14 DINOSEB


R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 2035633648
Conc: 705.00 ng/ml

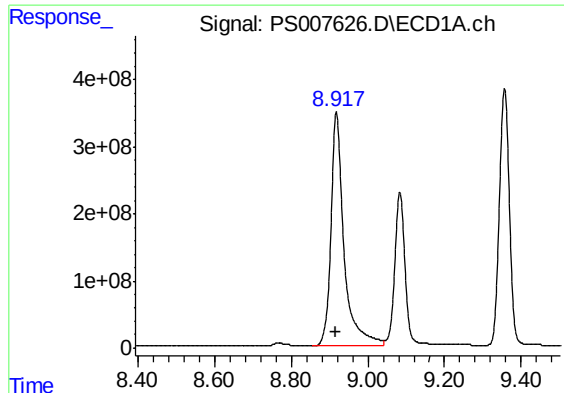

#15 Picloram


R.T.: 8.918 min
Delta R.T.: 0.000 min
Response: 8165447728
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

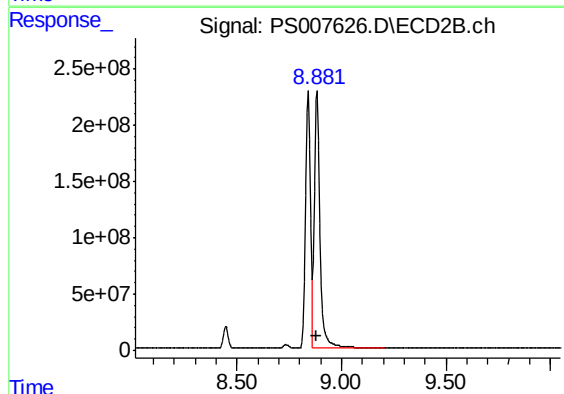


#15 Picloram

R.T.: 8.882 min
Delta R.T.: 0.000 min
Response: 4289222317
Conc: 712.50 ng/ml

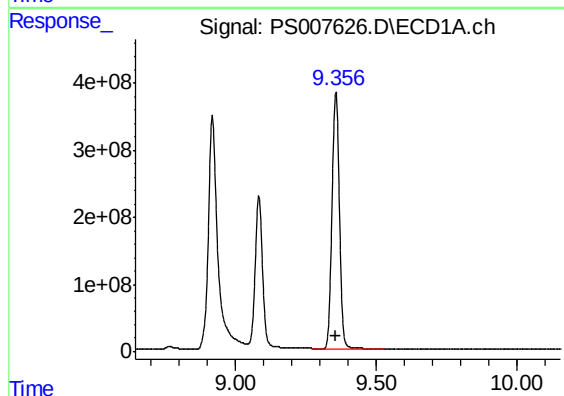

#16 DCPA

R.T.: 9.357 min
Delta R.T.: 0.000 min
Response: 6921438405
Conc: 720.00 ng/ml

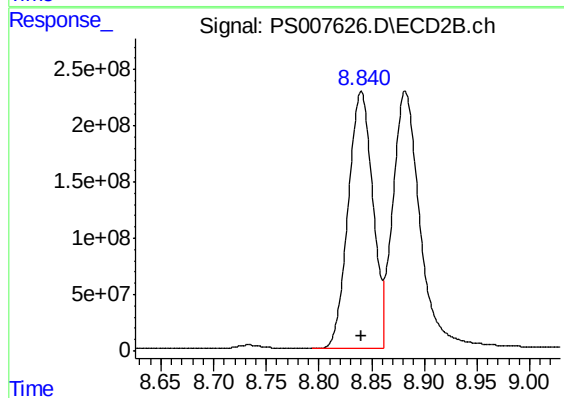

#16 DCPA

R.T.: 8.840 min
Delta R.T.: 0.000 min
Response: 3710897065
Conc: 720.00 ng/ml