

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110620\
 Data File : PS013144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 18:10
 Operator : DD\AJ
 Sample : L4625-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CONTAINER-001-A-B-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:47:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	263.3E6	139.6E6	294.492	358.724
Target Compounds							
1) T	Dalapon	2.993	2.589	73798846	117.5E6	69.752	221.798 #
2) T	3,5-DICHL...	0.000	6.095	0	71548104	N.D.	116.306
3) T	4-Nitroph...	7.098f	0.000	7132854	0	16.725	N.D. #
5) T	DICAMBA	7.386	7.046	11321718	5669896	3.170	3.416
7) T	MCPA	7.707	0.000	153.5E6	0	40.196	N.D. #
8) T	DICHLORPROP	0.000	7.749f	0	6076381	N.D.	13.595
10) T	Pentachlo...	8.683f	0.000	9157697	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.740f	0	37085152	N.D.	16.002
12) T	2,4,5-T	9.397f	0.000	61028022	0	11.532	N.D. #
15) T	Picloram	10.976	0.000	14644015	0	2.227	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110620\
Data File : PS013144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 18:10
Operator : DD\AJ
Sample : L4625-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CONTAINER-001-A-B-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:47:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

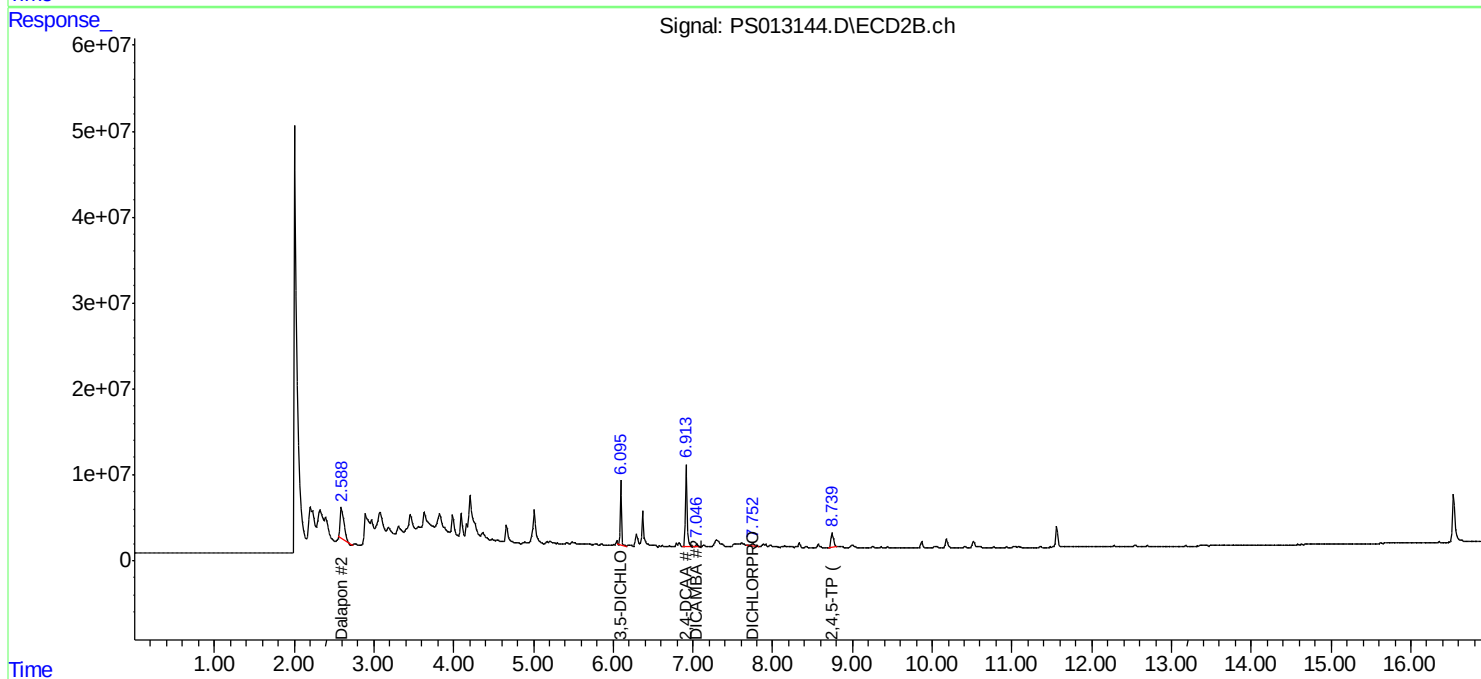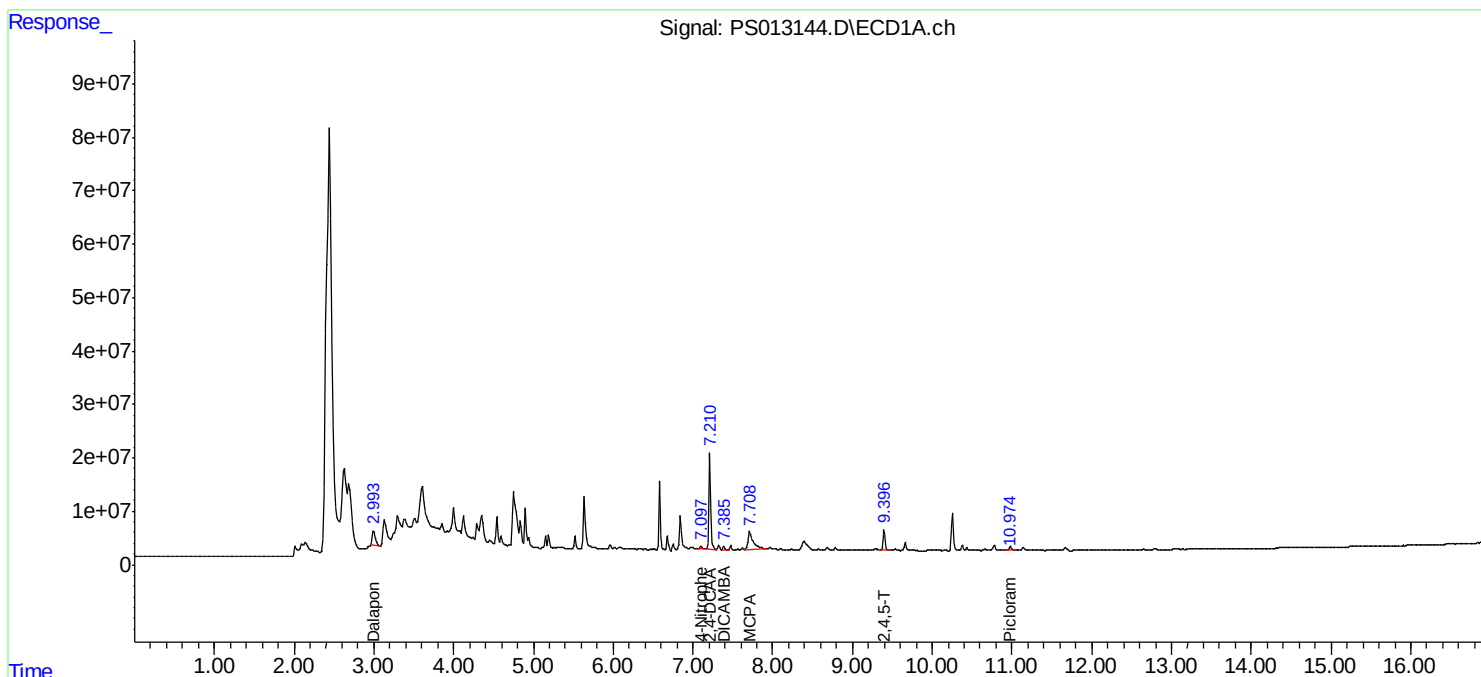


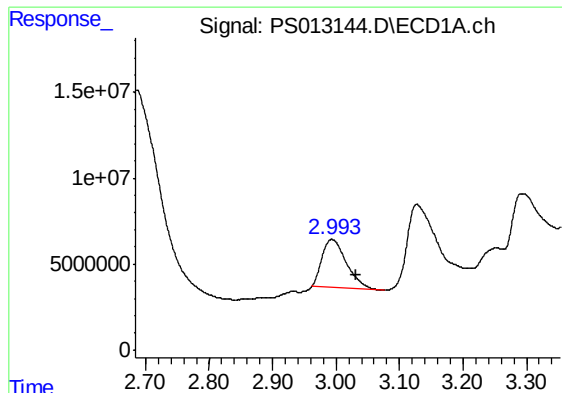

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.039 min
Response: 73798846
Conc: 69.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
CONTAINER-001-A-B-COMP

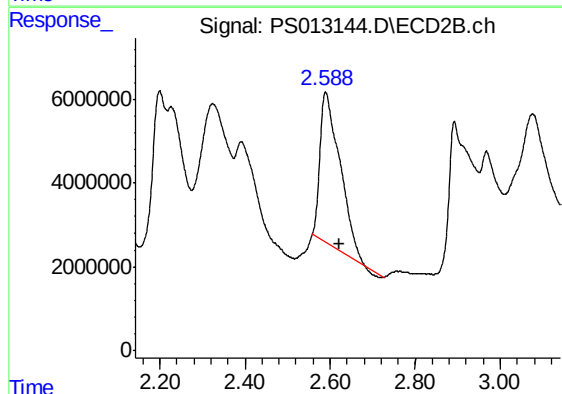


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.034 min
Response: 117547214
Conc: 221.80 ng/ml

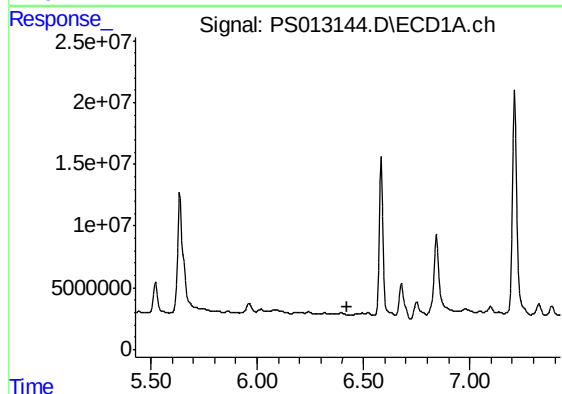


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.427 min
Response: 0
Conc: N.D.

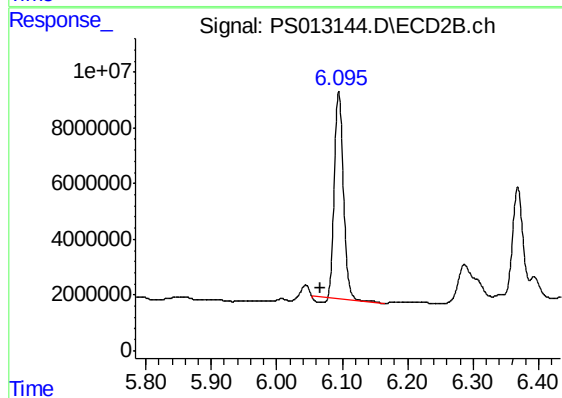

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 71548104
Conc: 116.31 ng/ml

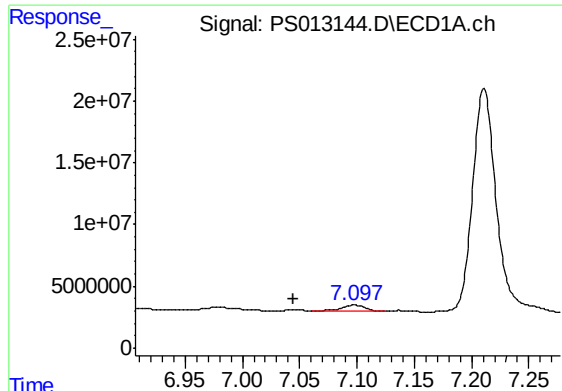

#3 4-Nitrophenol


R.T.: 7.098 min
Delta R.T.: 0.053 min
Response: 7132854
Conc: 16.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
CONTAINER-001-A-B-COMP

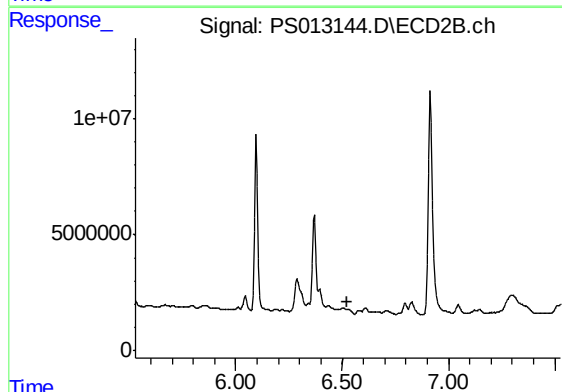


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

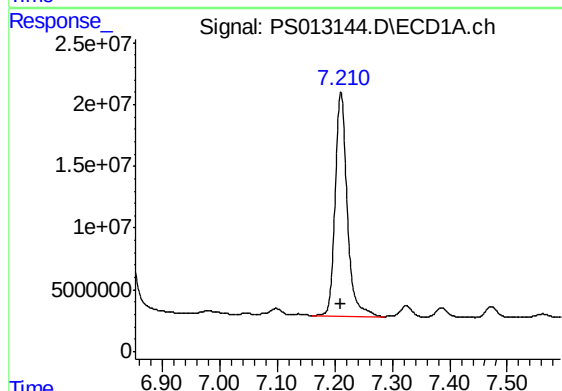


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 263255103
Conc: 294.49 ng/ml

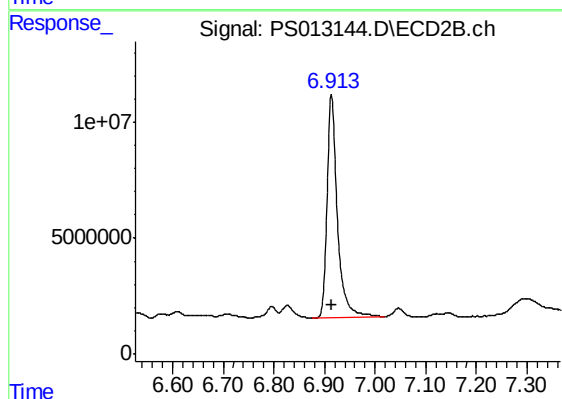

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 139575626
Conc: 358.72 ng/ml

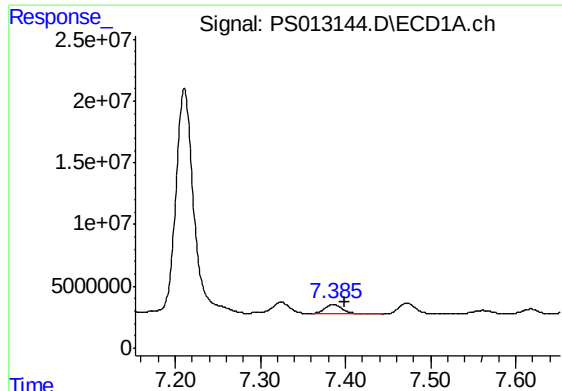

#5 DICAMBA


R.T.: 7.386 min
Delta R.T.: -0.014 min
Response: 11321718
Conc: 3.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
CONTAINER-001-A-B-COMP

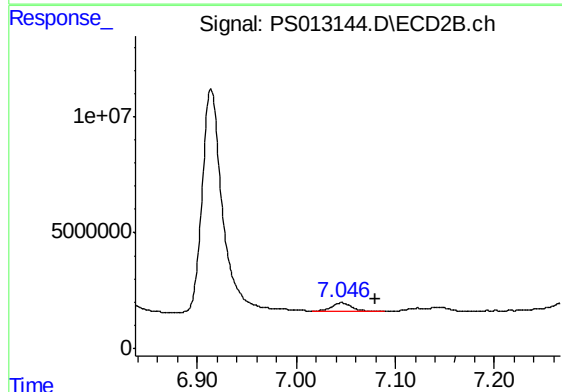


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 5669896
Conc: 3.42 ng/ml

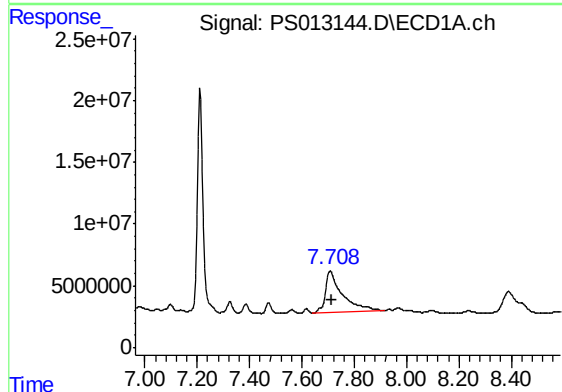


#7 MCPA

R.T.: 7.707 min
Delta R.T.: -0.009 min
Response: 153484216
Conc: 40.20 ug/ml

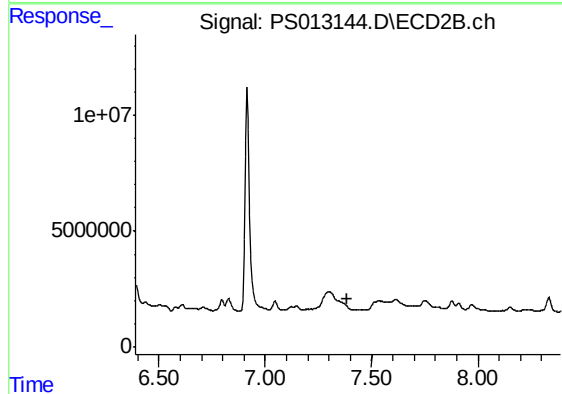

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

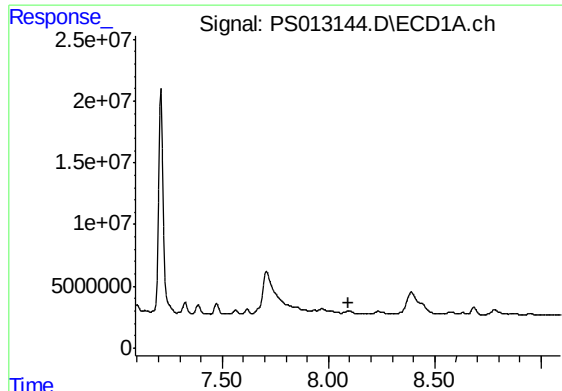

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CONTAINER-001-A-B-COMP

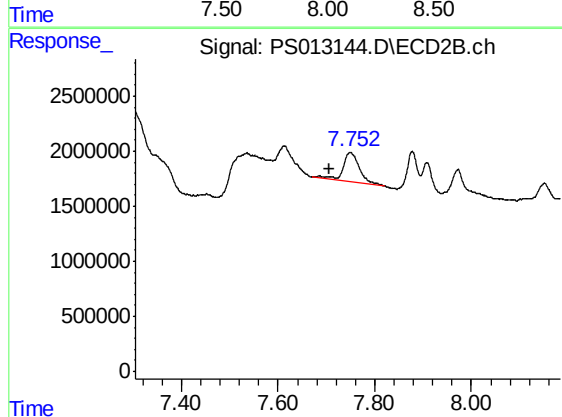


#8 DICHLORPROP

R.T.: 7.749 min
Delta R.T.: 0.044 min
Response: 6076381
Conc: 13.59 ng/ml

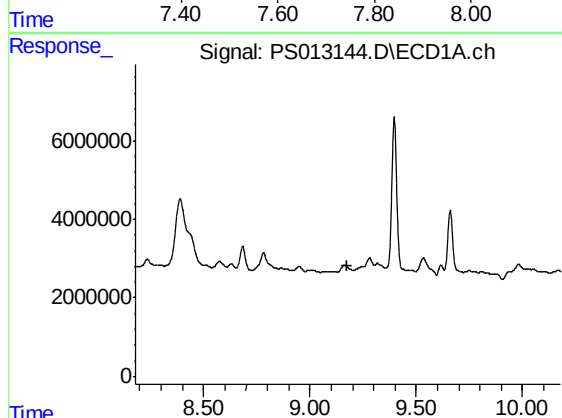


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

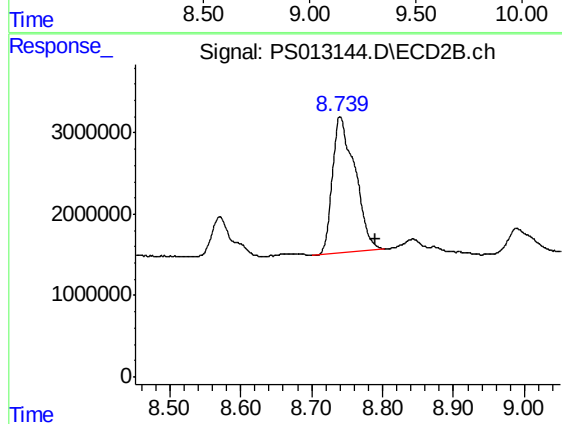

#11 2,4,5-TP (SILVEX)


R.T.: 8.740 min
Delta R.T.: -0.049 min
Response: 37085152
Conc: 16.00 ng/ml

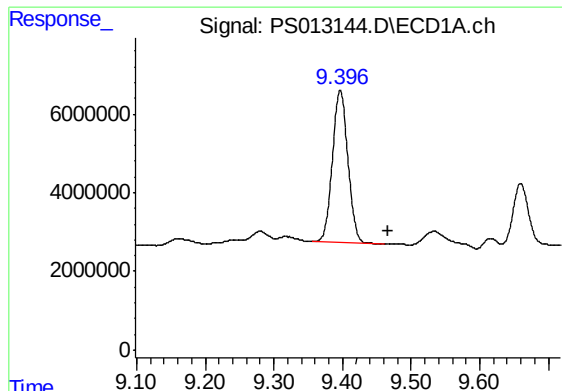

#12 2,4,5-T


R.T.: 9.397 min
Delta R.T.: -0.070 min
Response: 61028022
Conc: 11.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
CONTAINER-001-A-B-COMP

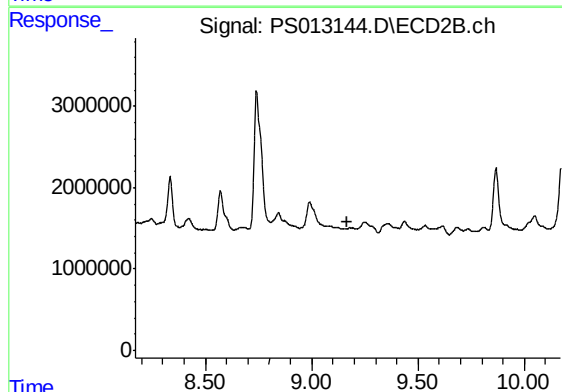


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

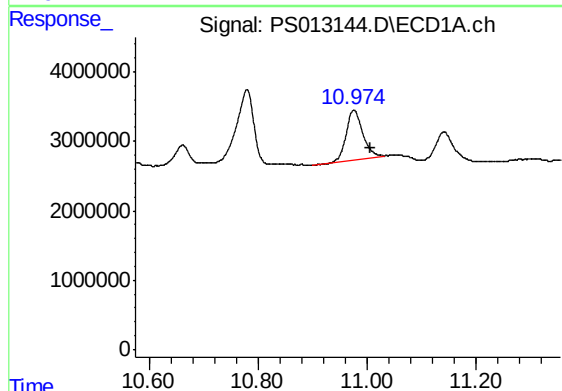

#15 Picloram

R.T.: 10.976 min
Delta R.T.: -0.030 min
Response: 14644015
Conc: 2.23 ng/ml

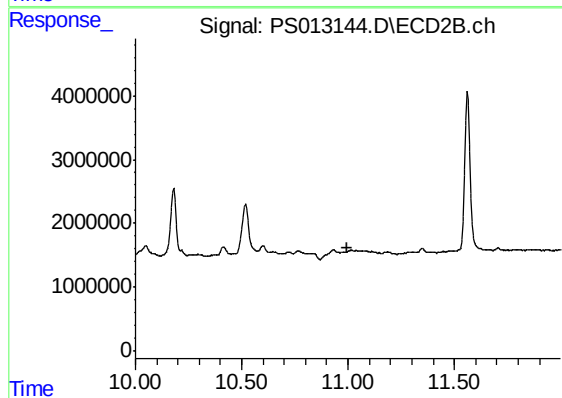

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.