

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110620\
 Data File : PS013149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 20:05
 Operator : DD\AJ
 Sample : L4656-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SR-L14-L13-NORTH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:49:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	319.0E6	167.3E6	356.817	429.908
Target Compounds							
1) T	Dalapon	2.994	2.591	86107630	153.8E6	81.386	290.188 #
2) T	3,5-DICHL...	6.469f	6.096	13875746	58857587	11.267	95.677 #
3) T	4-Nitroph...	6.979f	0.000	4452151	0	10.439	N.D. #
5) T	DICAMBA	7.386	7.047	11177261	5209384	3.130	3.138
7) T	MCPA	7.713	0.000	115.4E6	0	30.229	N.D. #
10) T	Pentachlo...	8.682f	0.000	9417930	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.160	8.740f	7811582	41242262	1.521	17.796 #
14) T	DINOSEB	11.142	0.000	9675927	0	2.347	N.D. #
15) T	Picloram	10.978	0.000	16334191	0	2.484	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110620\
Data File : PS013149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 20:05
Operator : DD\AJ
Sample : L4656-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SR-L14-L13-NORTH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:49:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

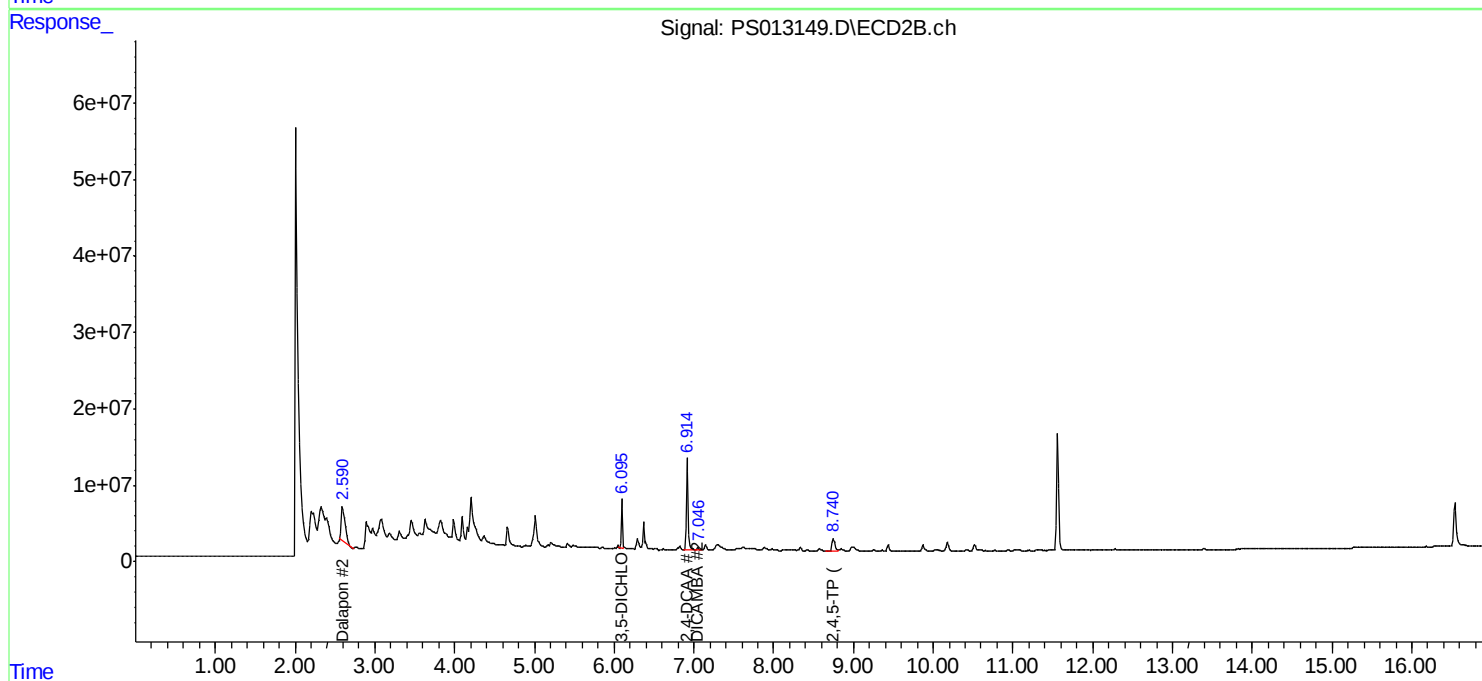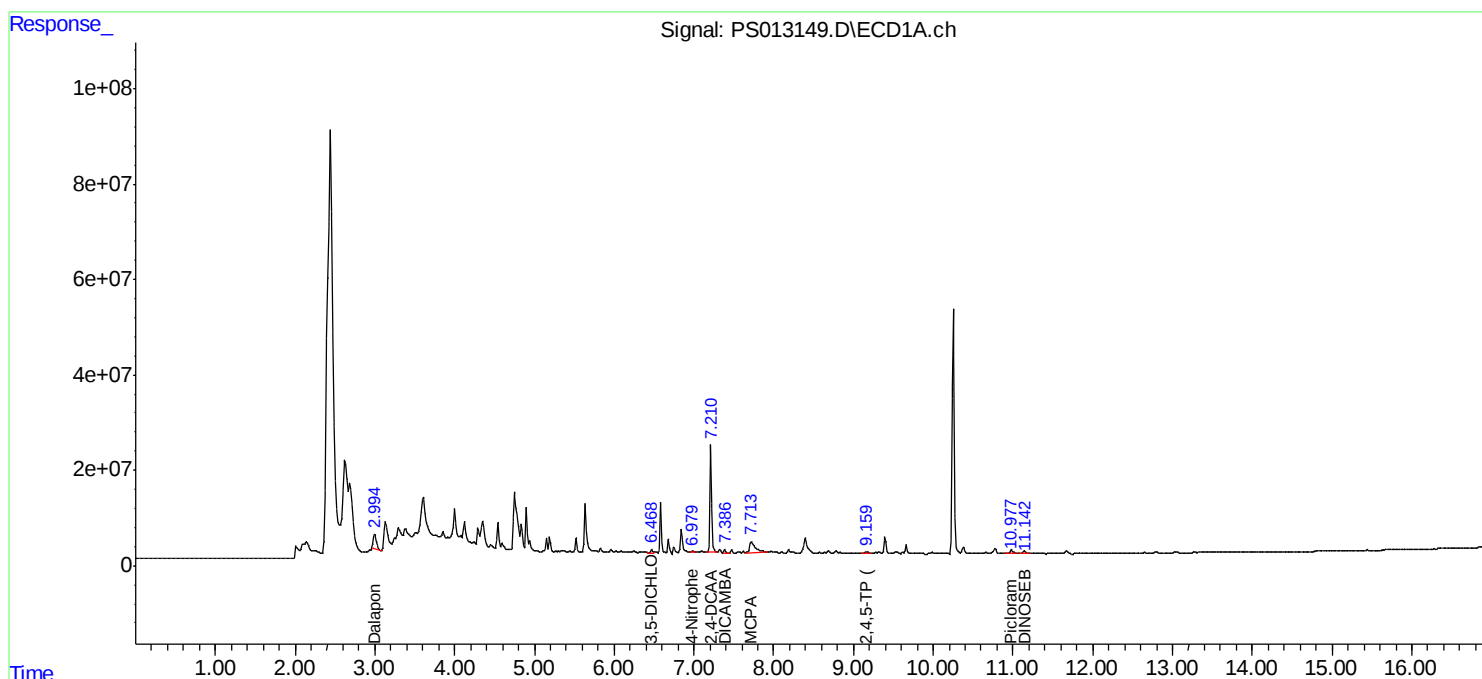


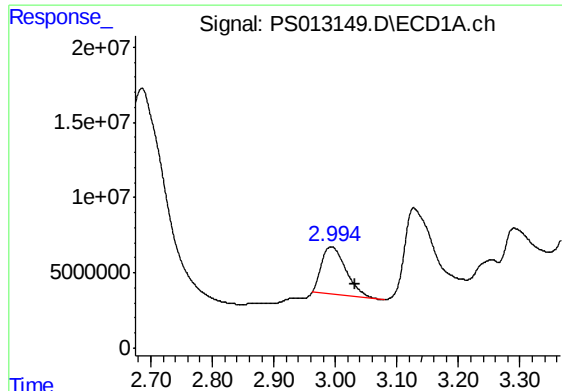

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.038 min
Response: 86107630
Conc: 81.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
SR-L14-L13-NORTH

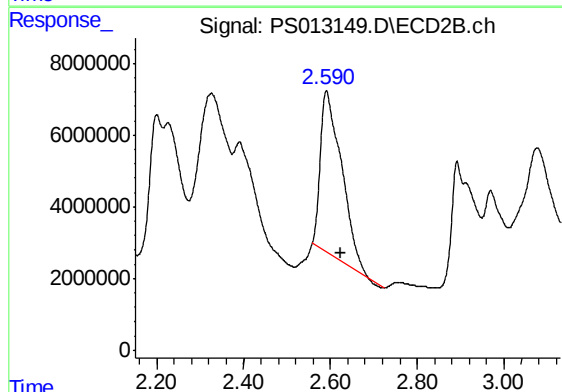


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.032 min
Response: 153792714
Conc: 290.19 ng/ml

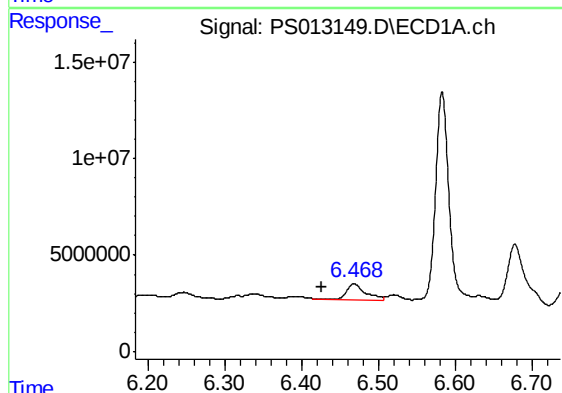


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.469 min
Delta R.T.: 0.042 min
Response: 13875746
Conc: 11.27 ng/ml

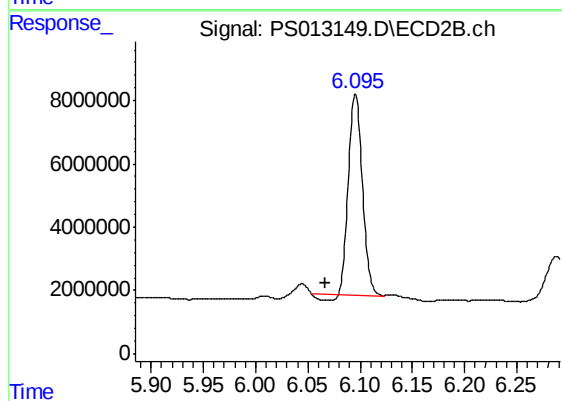

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.028 min
Response: 58857587
Conc: 95.68 ng/ml

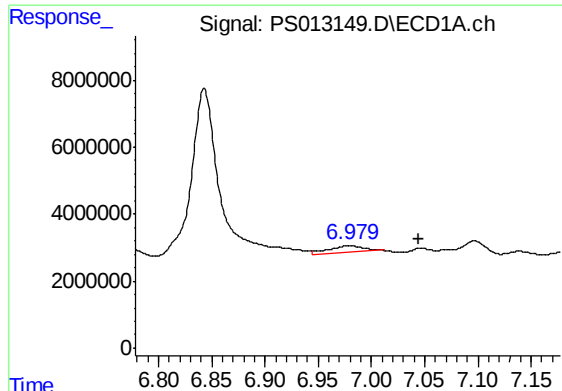

#3 4-Nitrophenol


R.T.: 6.979 min
Delta R.T.: -0.065 min
Response: 4452151
Conc: 10.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
SR-L14-L13-NORTH

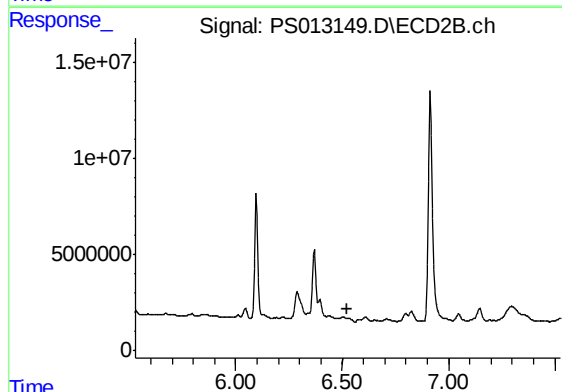


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

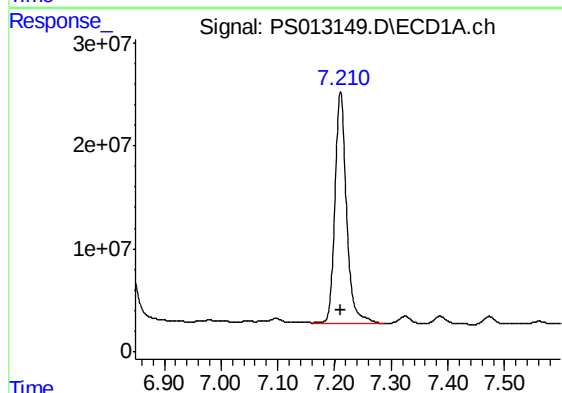


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 318969459
Conc: 356.82 ng/ml

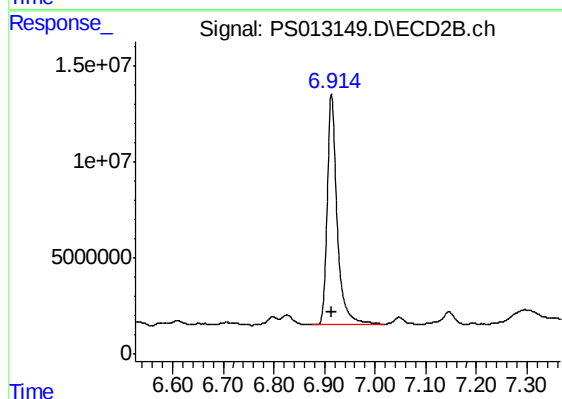

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 167272503
Conc: 429.91 ng/ml

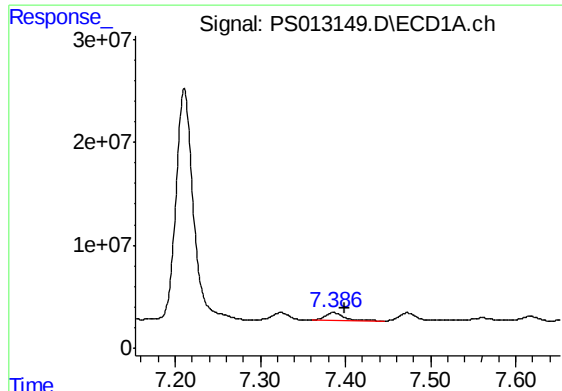

#5 DICAMBA


R.T.: 7.386 min
Delta R.T.: -0.014 min
Response: 11177261
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
SR-L14-L13-NORTH

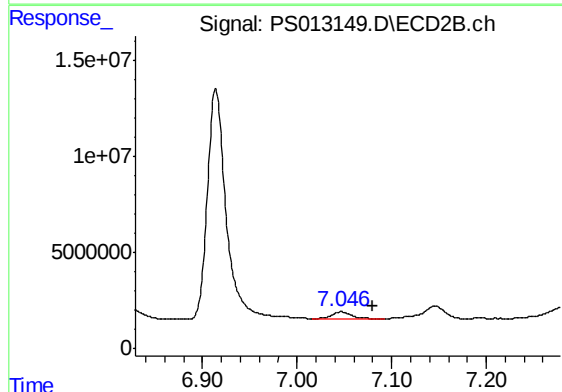


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.033 min
Response: 5209384
Conc: 3.14 ng/ml

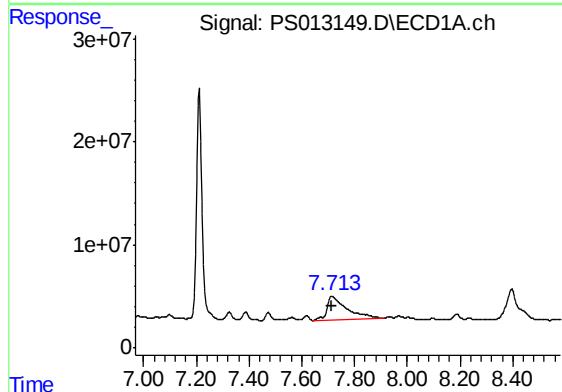


#7 MCPA

R.T.: 7.713 min
Delta R.T.: -0.003 min
Response: 115427054
Conc: 30.23 ug/ml

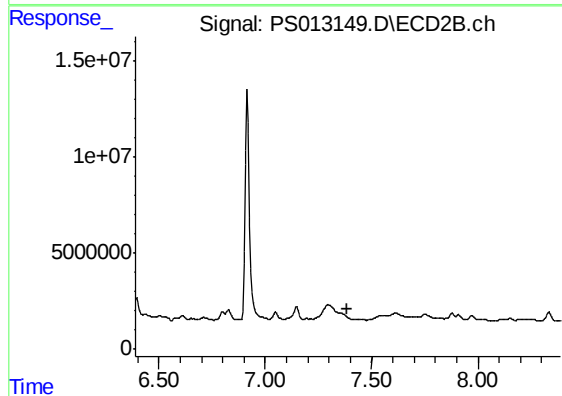

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

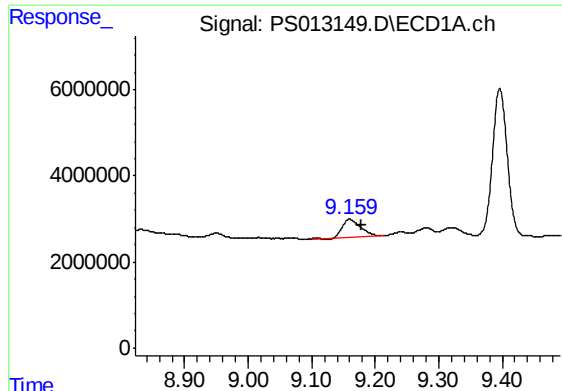

#11 2,4,5-TP (SILVEX)


R.T.: 9.160 min
Delta R.T.: -0.019 min
Response: 7811582
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
SR-L14-L13-NORTH

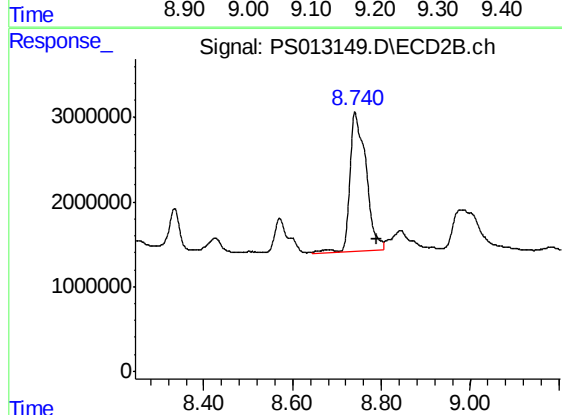


#11 2,4,5-TP (SILVEX)

R.T.: 8.740 min
Delta R.T.: -0.049 min
Response: 41242262
Conc: 17.80 ng/ml

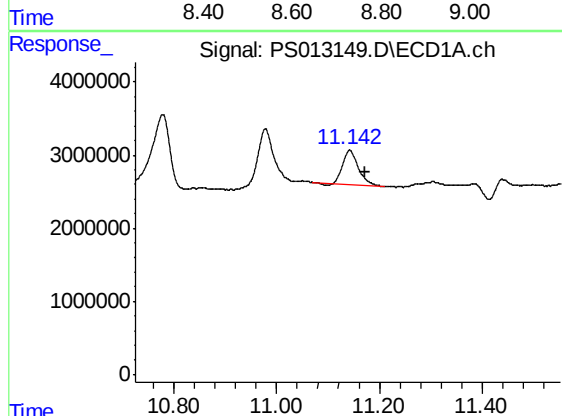


#14 DINOSEB

R.T.: 11.142 min
Delta R.T.: -0.030 min
Response: 9675927
Conc: 2.35 ng/ml

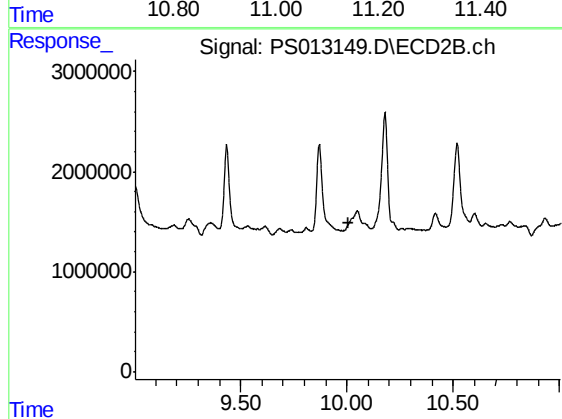

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 10.005 min
Response: 0
Conc: N.D.

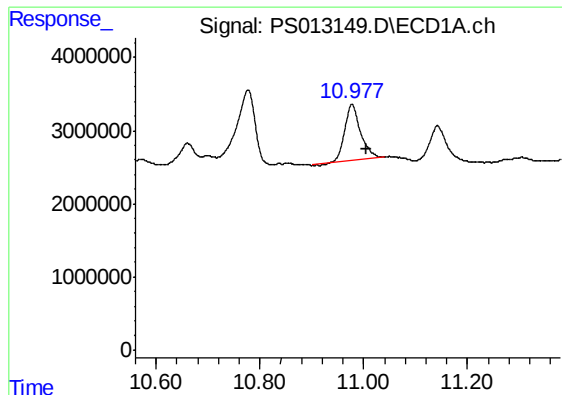

#15 Picloram

R.T.: 10.978 min
Delta R.T.: -0.028 min
Response: 16334191
Conc: 2.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
SR-L14-L13-NORTH

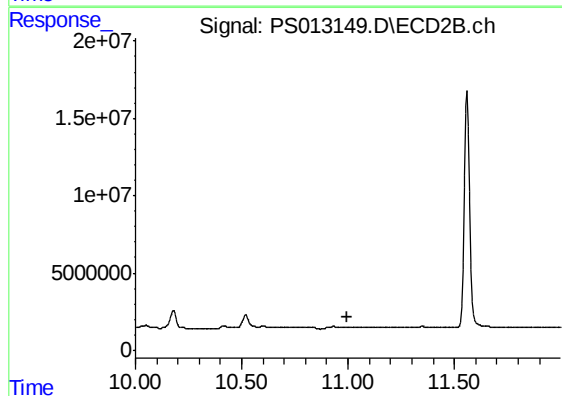

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.