

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110620\
 Data File : PS013152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2020 21:14
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:50:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.912	712.9E6	315.1E6	797.546	809.714
Target Compounds							
1) T	Dalapon	3.032	2.624	719.1E6	364.3E6	679.684	687.351
2) T	3,5-DICHL...	6.426	6.066	906.9E6	458.8E6	736.400	745.758
3) T	4-Nitroph...	7.043	6.524	318.4E6	183.4E6	746.454	769.898
5) T	DICAMBA	7.398	7.078	2689.7E6	1259.8E6	753.147	758.916
6) T	MCPD	7.565	7.173	203.4E6	100.7E6	76.414	76.083
7) T	MCPA	7.715	7.388	287.1E6	155.7E6	75.176	73.184
8) T	DICHLORPROP	8.089	7.704	669.4E6	334.8E6	747.548	749.068
9) T	2,4-D	8.321	8.001	743.6E6	406.1E6	787.077	765.283
10) T	Pentachlo...	8.628	8.425	9779.0E6	4207.1E6	759.812	761.300
11) T	2,4,5-TP ...	9.176	8.787	3888.0E6	1774.3E6	757.076	765.637
12) T	2,4,5-T	9.464	9.167	3967.9E6	1723.8E6	749.783	778.241
13) T	2,4-DB	10.017	9.674	665.0E6	234.6E6	789.391	723.013
14) T	DINOSEB	11.169	10.003	2996.7E6	1252.2E6	726.739	742.760
15) T	Picloram	11.003	10.996	4906.9E6	2632.2E6	746.212	729.235
16) T	DCPA	11.435	10.929	4953.1E6	2333.4E6	762.703	777.211



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110620\
Data File : PS013152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2020 21:14
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:50:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

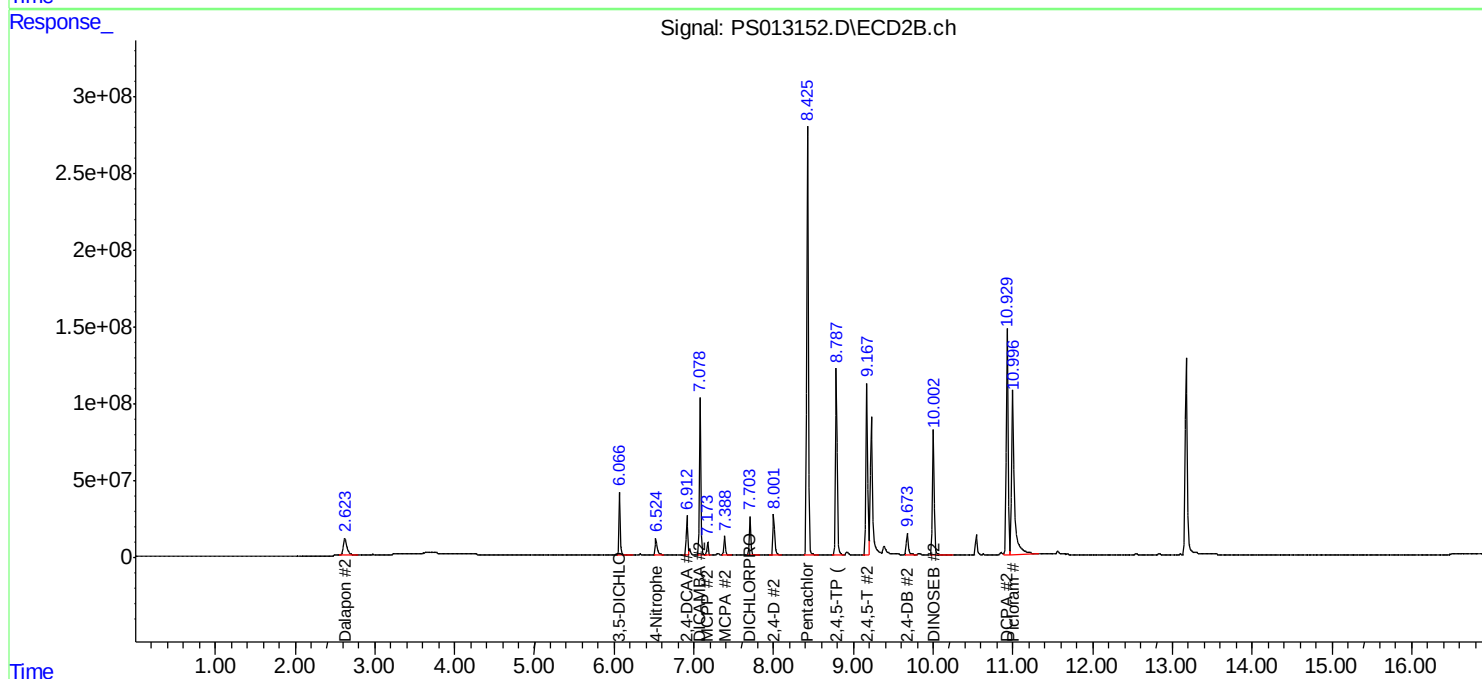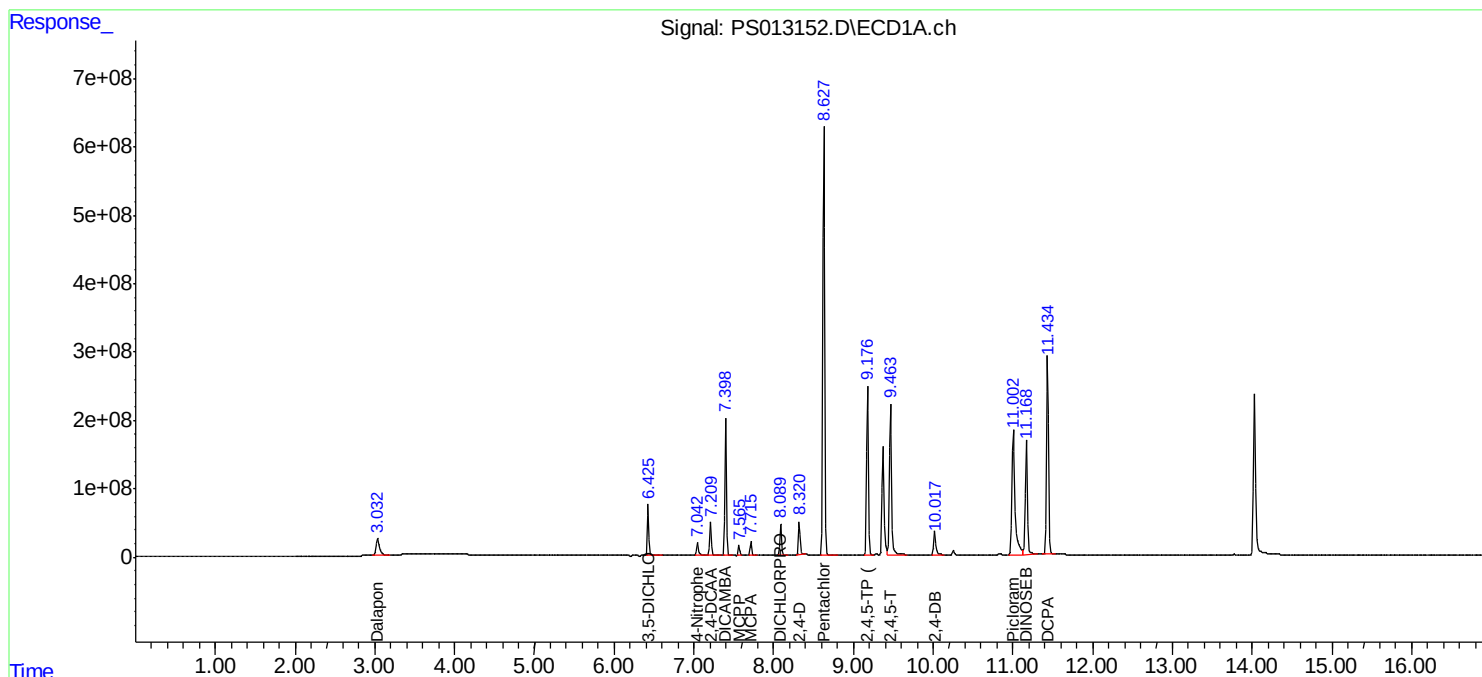


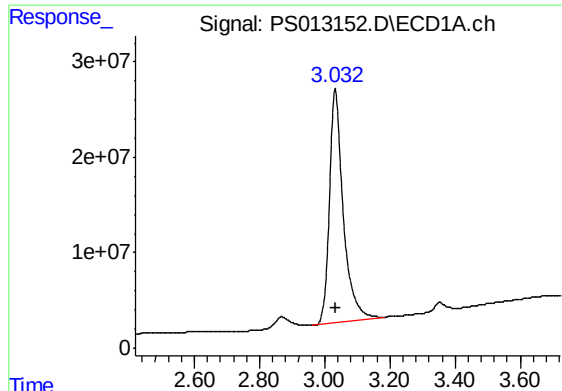

#1 Dalapon


R.T.: 3.032 min
Delta R.T.: 0.000 min
Response: 719113308
Conc: 679.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

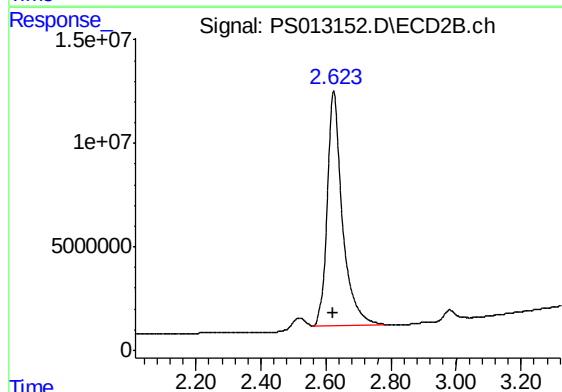


#1 Dalapon

R.T.: 2.624 min
Delta R.T.: 0.000 min
Response: 364279198
Conc: 687.35 ng/ml

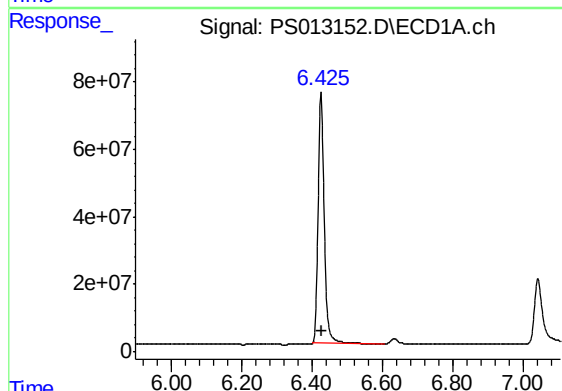


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.426 min
Delta R.T.: -0.001 min
Response: 906932953
Conc: 736.40 ng/ml

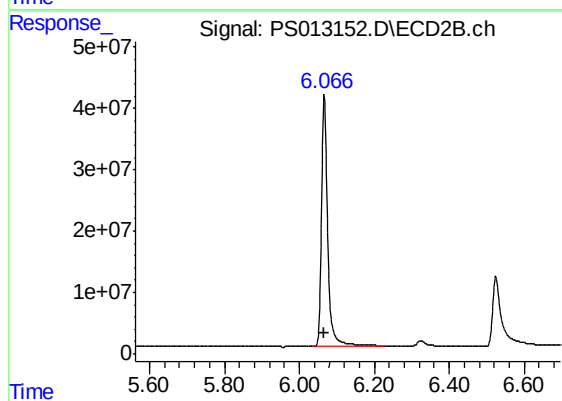

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.066 min
Delta R.T.: -0.001 min
Response: 458769563
Conc: 745.76 ng/ml

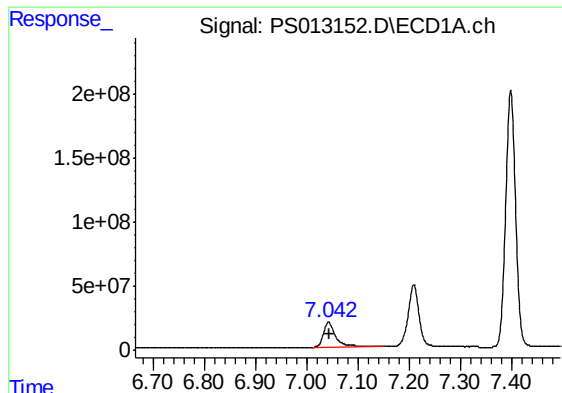

#3 4-Nitrophenol


R.T.: 7.043 min
Delta R.T.: -0.002 min
Response: 318352478
Conc: 746.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

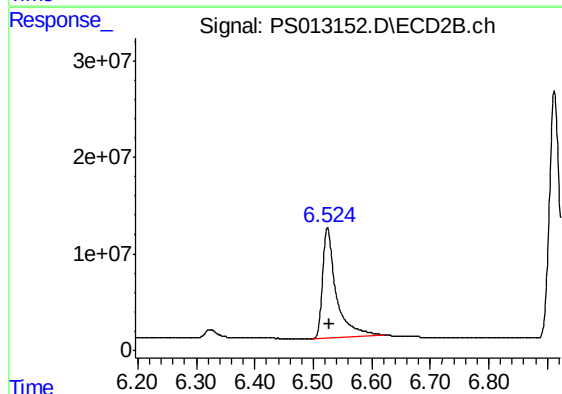


#3 4-Nitrophenol

R.T.: 6.524 min
Delta R.T.: -0.003 min
Response: 183350282
Conc: 769.90 ng/ml

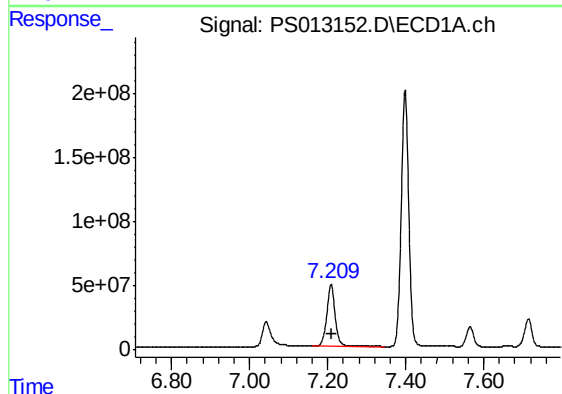


#4 2,4-DCAA

R.T.: 7.209 min
Delta R.T.: -0.001 min
Response: 712949369
Conc: 797.55 ng/ml

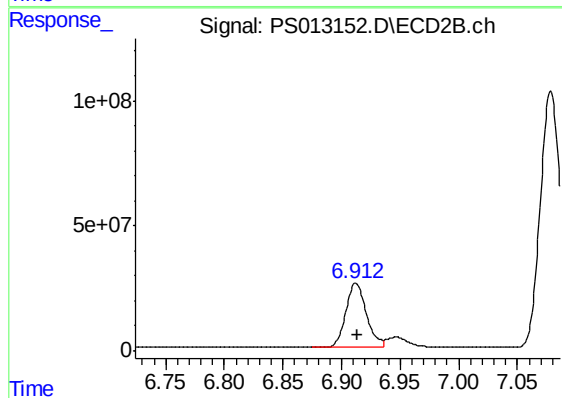

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: -0.002 min
Response: 315051243
Conc: 809.71 ng/ml

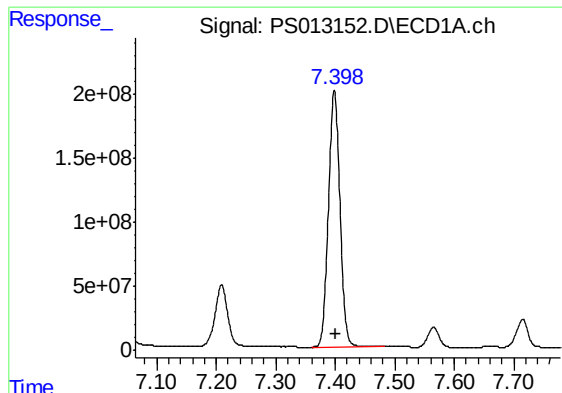

#5 DICAMBA


R.T.: 7.398 min
Delta R.T.: -0.001 min
Response: 2689666863
Conc: 753.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

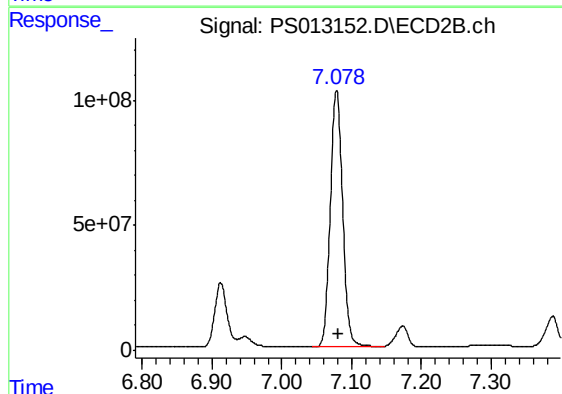


#5 DICAMBA

R.T.: 7.078 min
Delta R.T.: -0.002 min
Response: 1259818316
Conc: 758.92 ng/ml

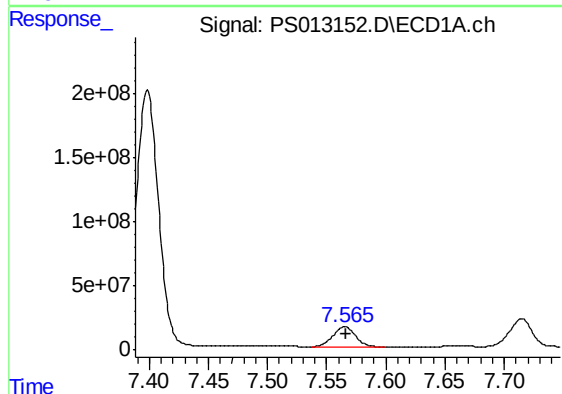


#6 MCPP

R.T.: 7.565 min
Delta R.T.: -0.001 min
Response: 203422341
Conc: 76.41 ug/ml

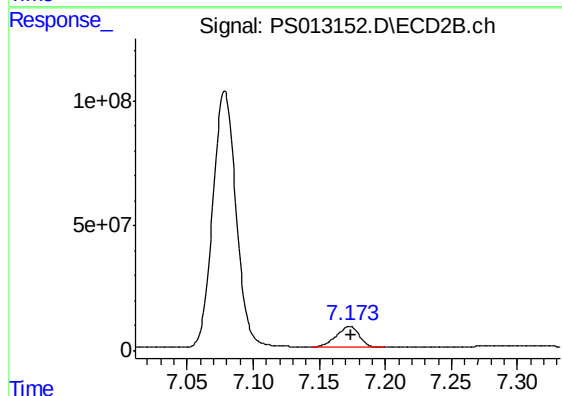

#6 MCPP


R.T.: 7.173 min
Delta R.T.: 0.000 min
Response: 100702971
Conc: 76.08 ug/ml

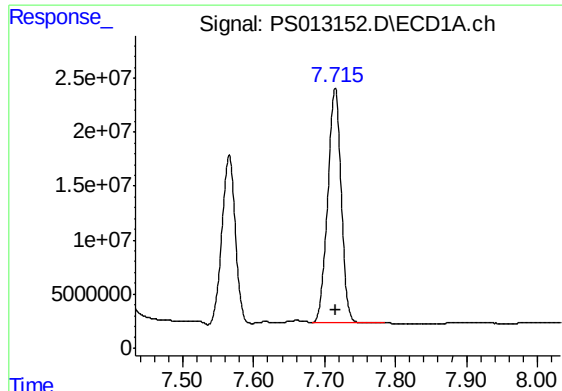

#7 MCPA


R.T.: 7.715 min
Delta R.T.: -0.001 min
Response: 287055482
Conc: 75.18 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

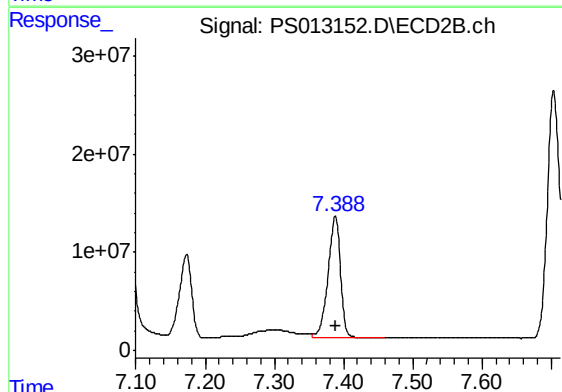


#7 MCPA

R.T.: 7.388 min
Delta R.T.: 0.000 min
Response: 155709989
Conc: 73.18 ug/ml

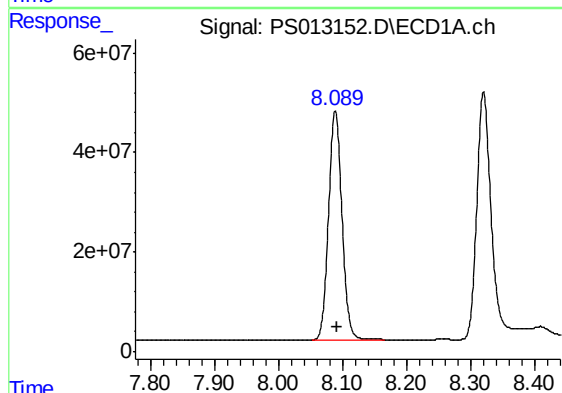


#8 DICHLORPROP

R.T.: 8.089 min
Delta R.T.: -0.002 min
Response: 669425539
Conc: 747.55 ng/ml

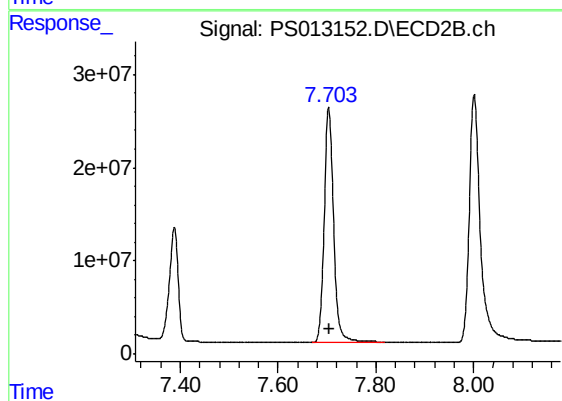

#8 DICHLORPROP


R.T.: 7.704 min
Delta R.T.: -0.002 min
Response: 334802705
Conc: 749.07 ng/ml

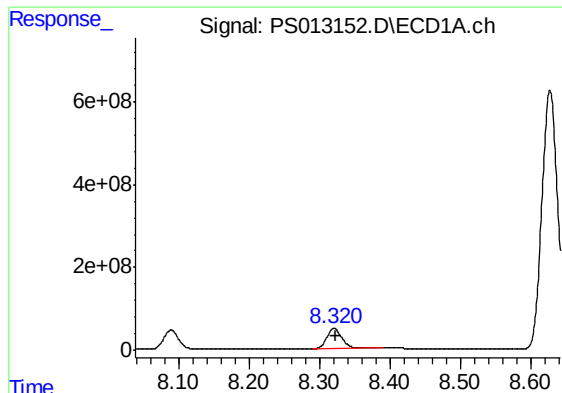

#9 2,4-D


R.T.: 8.321 min
Delta R.T.: -0.003 min
Response: 743585598
Conc: 787.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

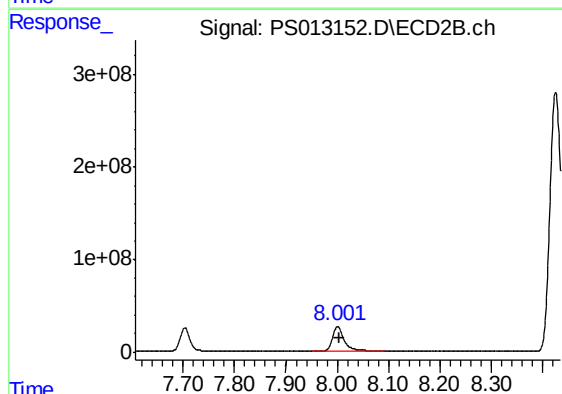


#9 2,4-D

R.T.: 8.001 min
Delta R.T.: -0.003 min
Response: 406139697
Conc: 765.28 ng/ml

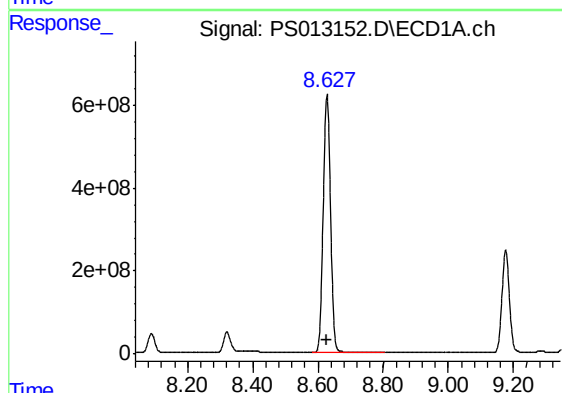


#10 Pentachlorophenol

R.T.: 8.628 min
Delta R.T.: -0.001 min
Response: 9778953468
Conc: 759.81 ng/ml

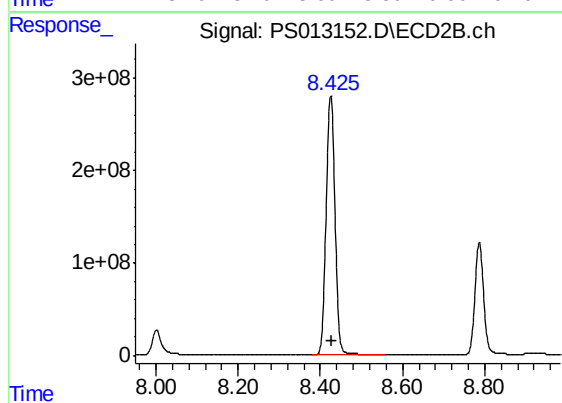

#10 Pentachlorophenol


R.T.: 8.425 min
Delta R.T.: -0.002 min
Response: 4207128895
Conc: 761.30 ng/ml

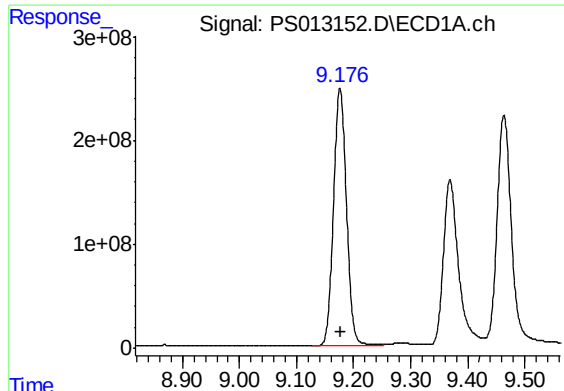

#11 2,4,5-TP (SILVEX)


R.T.: 9.176 min
Delta R.T.: -0.002 min
Response: 3887995682
Conc: 757.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

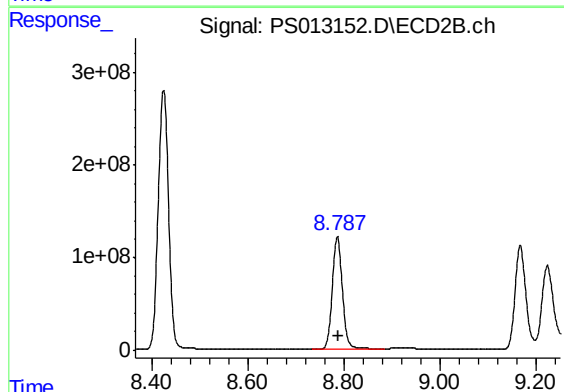


#11 2,4,5-TP (SILVEX)

R.T.: 8.787 min
Delta R.T.: -0.002 min
Response: 1774343025
Conc: 765.64 ng/ml

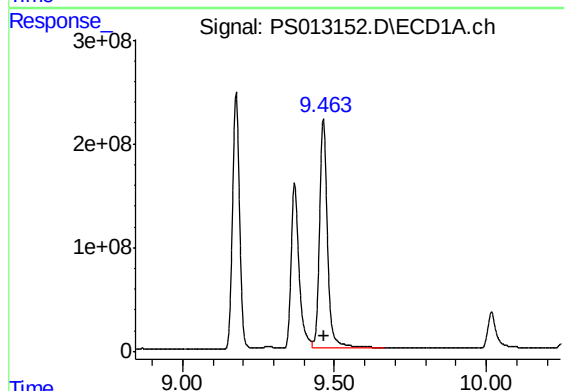


#12 2,4,5-T

R.T.: 9.464 min
Delta R.T.: -0.003 min
Response: 3967937669
Conc: 749.78 ng/ml

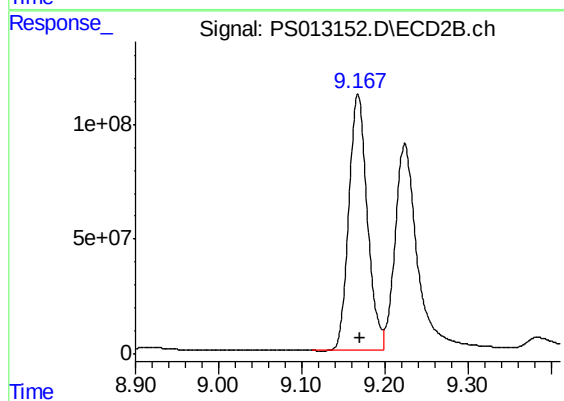

#12 2,4,5-T


R.T.: 9.167 min
Delta R.T.: -0.003 min
Response: 1723797297
Conc: 778.24 ng/ml

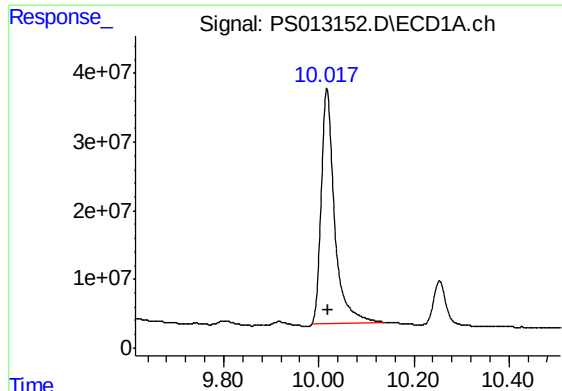

#13 2,4-DB


R.T.: 10.017 min
Delta R.T.: -0.003 min
Response: 665020657
Conc: 789.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

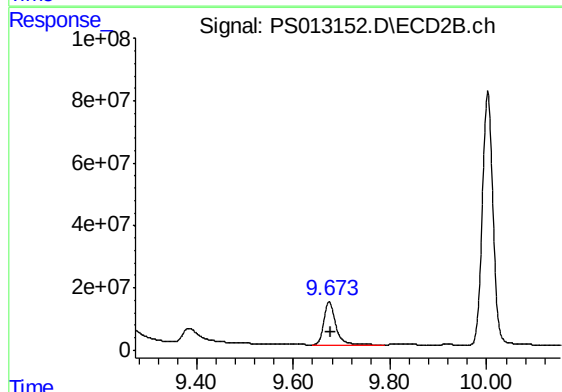


#13 2,4-DB

R.T.: 9.674 min
Delta R.T.: -0.003 min
Response: 234649351
Conc: 723.01 ng/ml

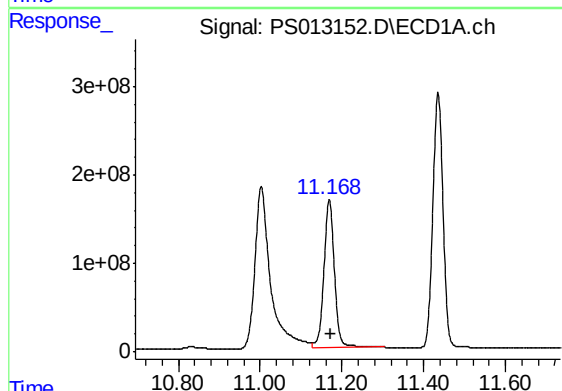


#14 DINOSEB

R.T.: 11.169 min
Delta R.T.: -0.003 min
Response: 2996723961
Conc: 726.74 ng/ml

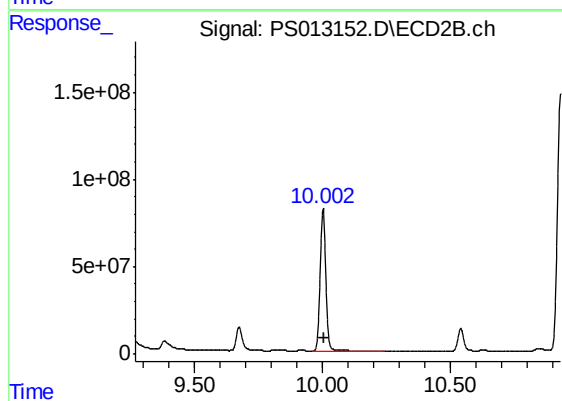

#14 DINOSEB


R.T.: 10.003 min
Delta R.T.: -0.002 min
Response: 1252215531
Conc: 742.76 ng/ml

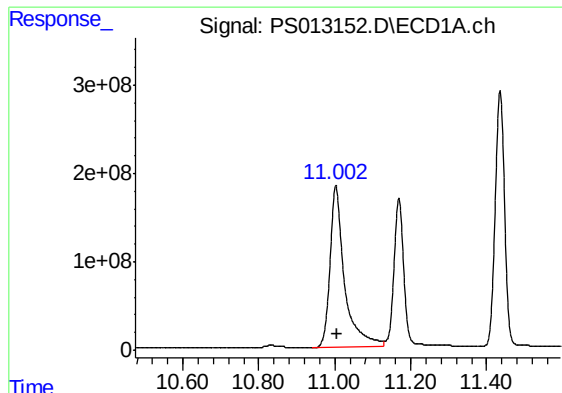

#15 Picloram


R.T.: 11.003 min
Delta R.T.: -0.003 min
Response: 4906875944
Conc: 746.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

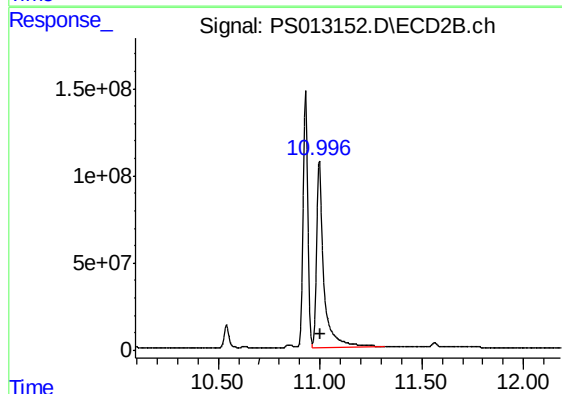


#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.003 min
Response: 2632151387
Conc: 729.23 ng/ml

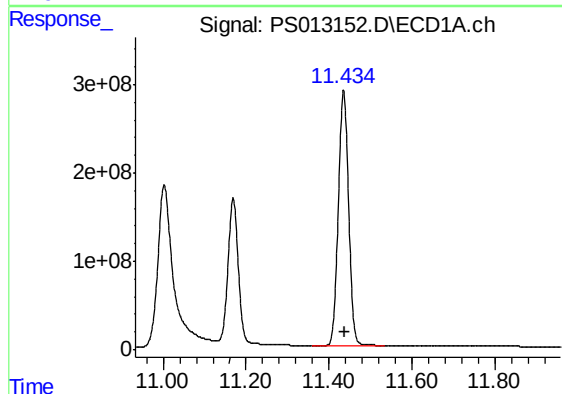

#16 DCPA

R.T.: 11.435 min
Delta R.T.: -0.003 min
Response: 4953092039
Conc: 762.70 ng/ml

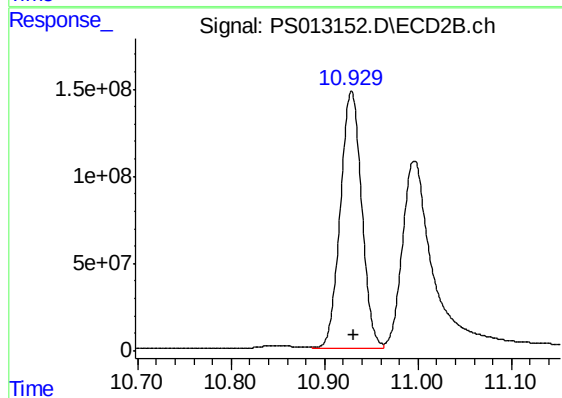

#16 DCPA

R.T.: 10.929 min
Delta R.T.: -0.003 min
Response: 2333388692
Conc: 777.21 ng/ml