

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110623\
 Data File : PS024761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 09:09
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 23:05:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.514	2.564	10434845	8041577	4.332 7.633 #
6) T	MCP	0.000	7.076f	0	658816	N.D. <MDL
7) T	MCPA	0.000	7.260	0	4811711	N.D. 1.561
8) T	DICHLORPROP	0.000	7.594f	0	218667	N.D. <MDL
9) T	2,4-D	7.346f	7.796	51485767	80287	18.730 <MDL #
10) T	Pentachlo...	0.000	8.286	0	268935	N.D. <MDL
11) T	2,4,5-TP ...	0.000	8.620	0	237966	N.D. <MDL
12) T	2,4,5-T	0.000	8.989	0	290914	N.D. <MDL
13) T	2,4-DB	0.000	9.455	0	1833658	N.D. 3.761
14) T	DINOSEB	0.000	9.830	0	363017	N.D. <MDL
15) T	Picloram	9.683	10.767	12025544	7008633	<MDL 1.153 #
16) T	DCPA	0.000	10.767	0	7008633	N.D. 1.395



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110623\
Data File : PS024761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 09:09
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 23:05:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

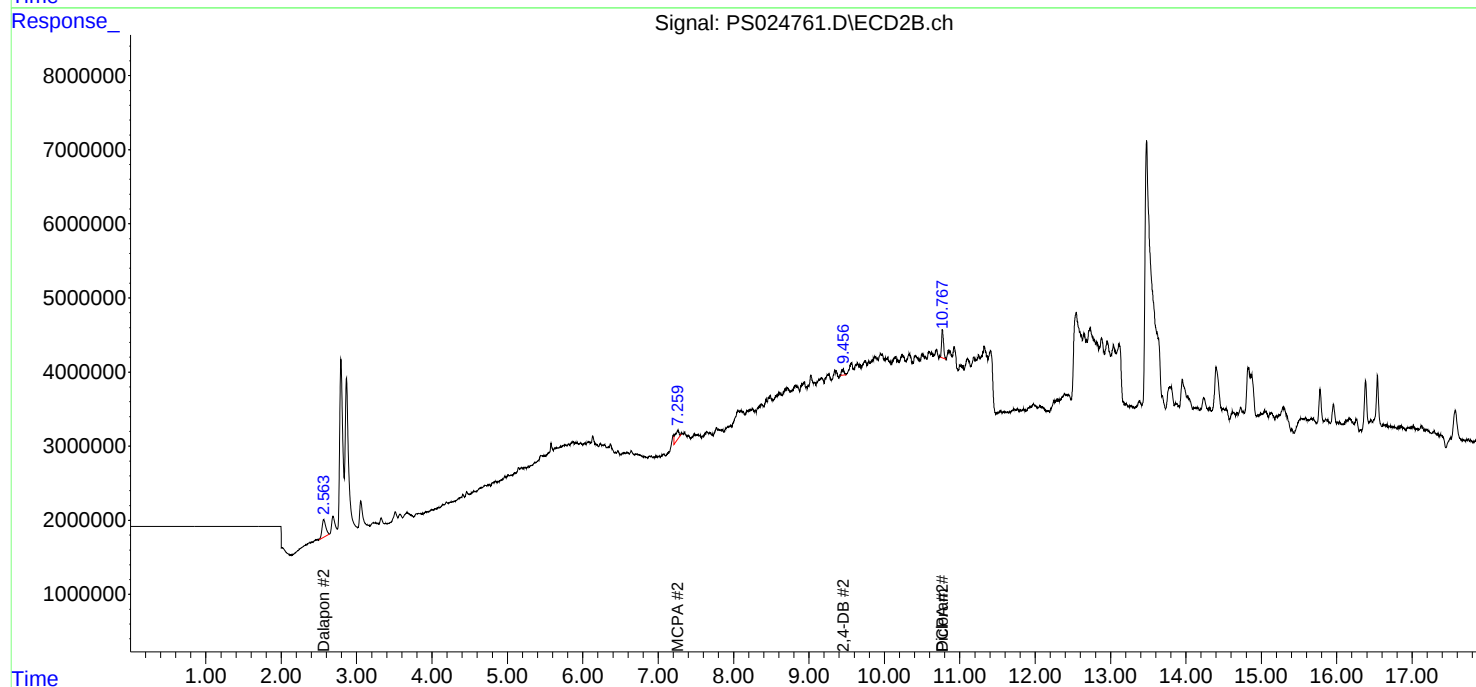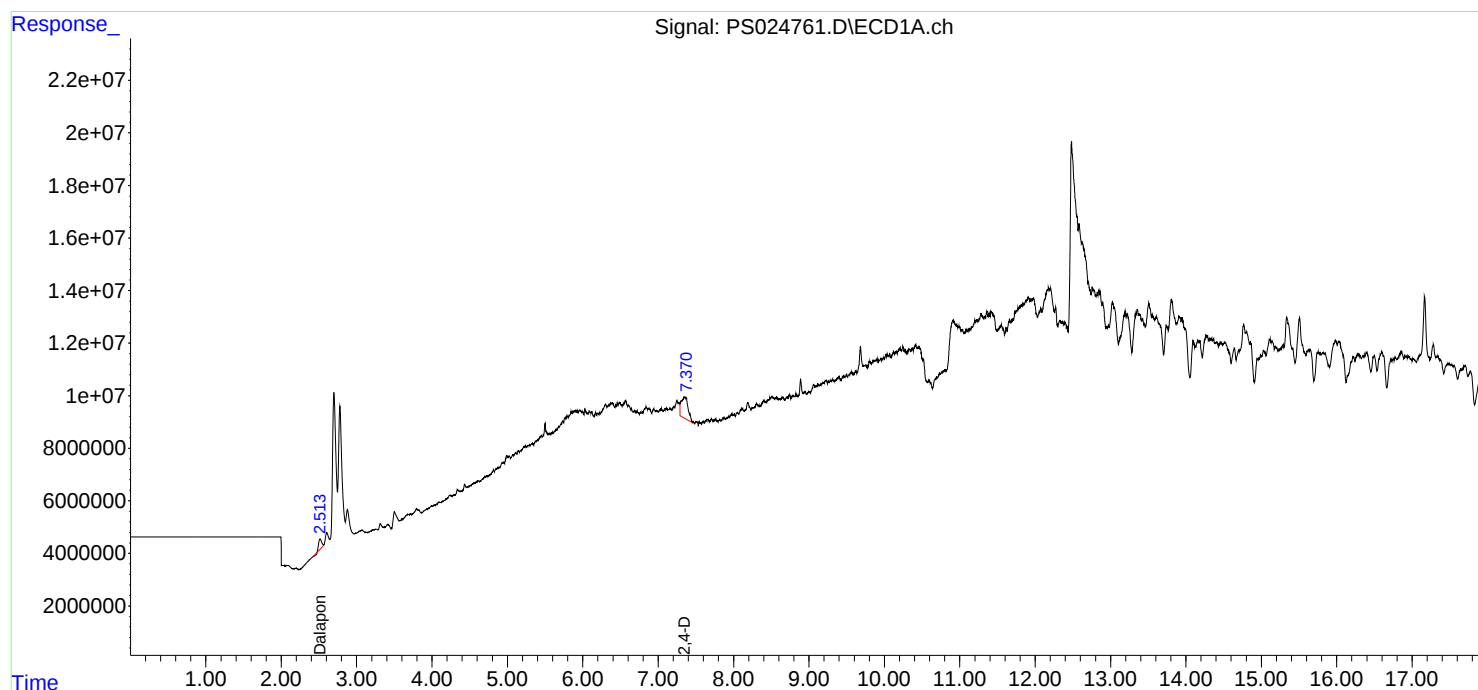


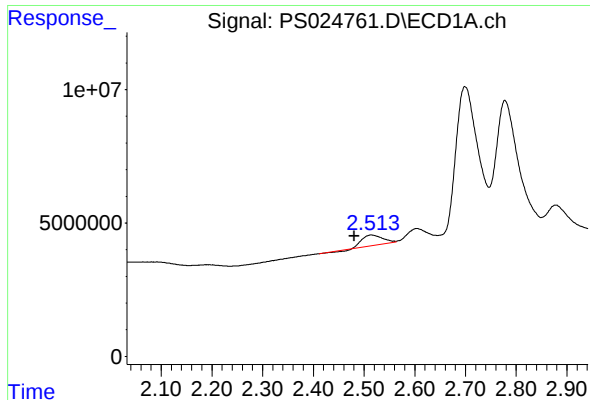

#1 Dalapon


R.T.: 2.514 min
Delta R.T.: 0.033 min
Response: 10434845
Conc: 4.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

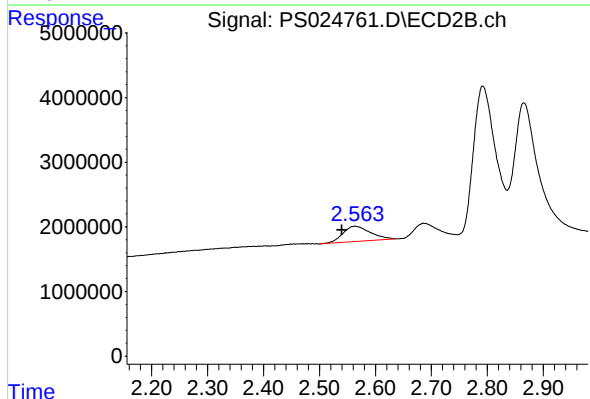


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.023 min
Response: 8041577
Conc: 7.63 ng/ml

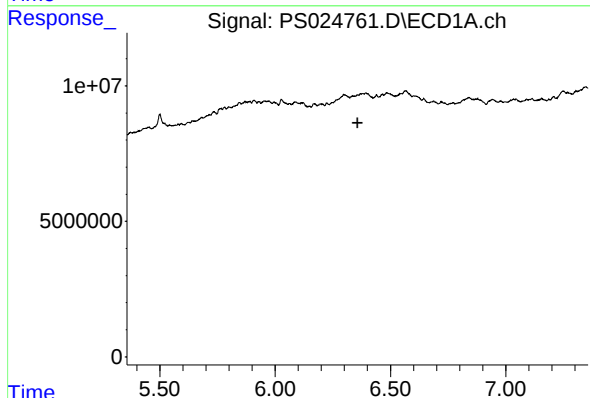


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.357 min
Response: 0
Conc: N.D.

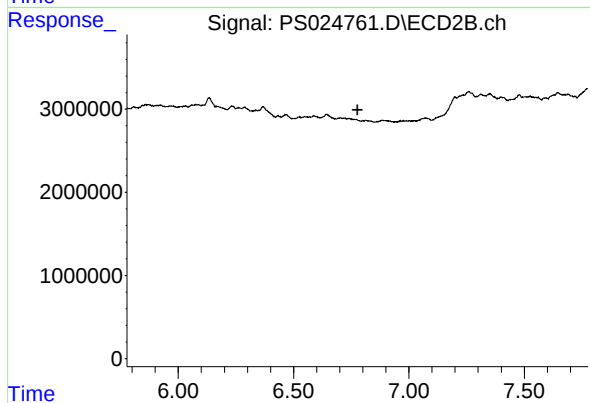

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.777 min
Response: 0
Conc: N.D.

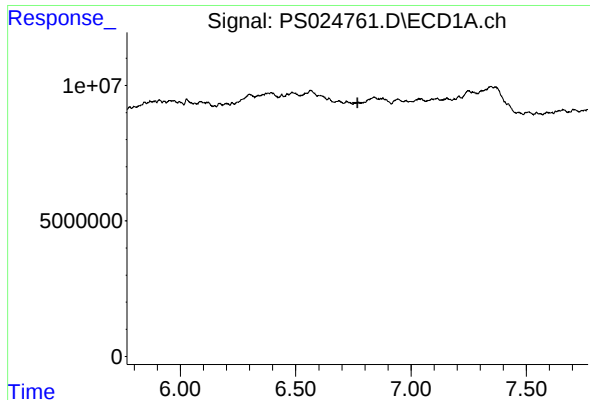

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

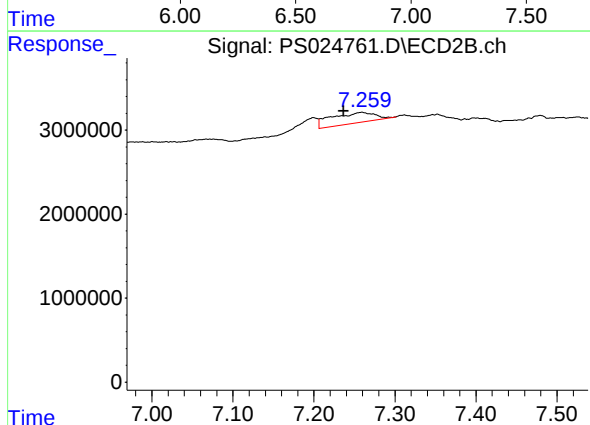


#7 MCPA

R.T.: 7.260 min
Delta R.T.: 0.023 min
Response: 4811711
Conc: 1.56 ug/ml

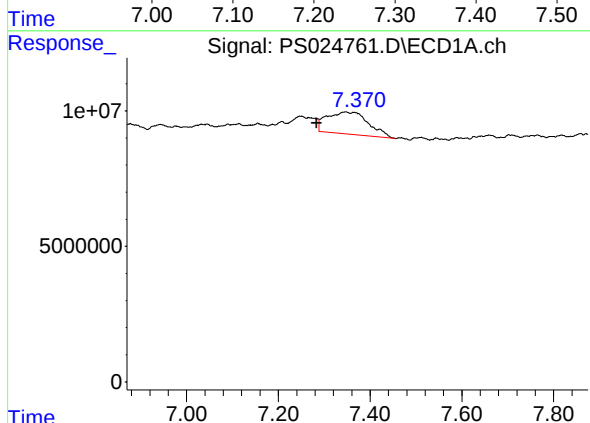


#9 2,4-D

R.T.: 7.346 min
Delta R.T.: 0.063 min
Response: 51485767
Conc: 18.73 ng/ml

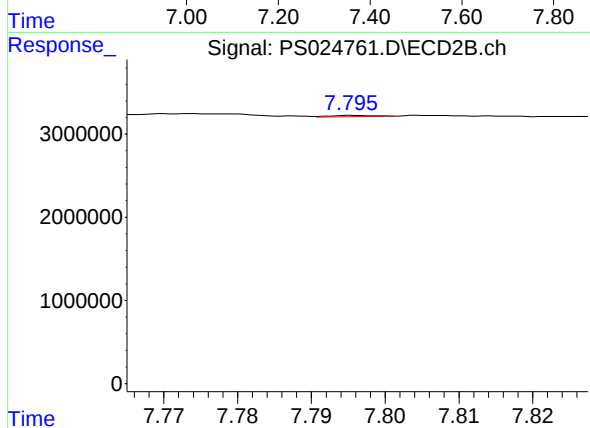

#9 2,4-D


R.T.: 7.796 min
Delta R.T.: -0.039 min
Response: 80287
Conc: N.D.

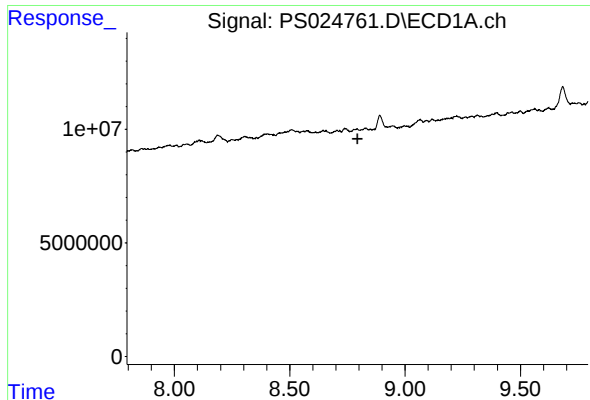

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

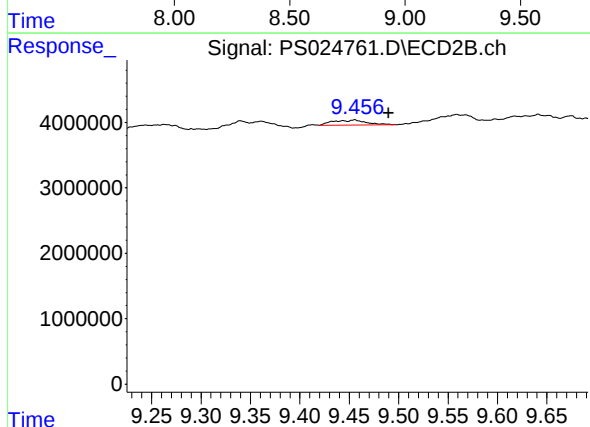


#13 2,4-DB

R.T.: 9.455 min
Delta R.T.: -0.035 min
Response: 1833658
Conc: 3.76 ng/ml

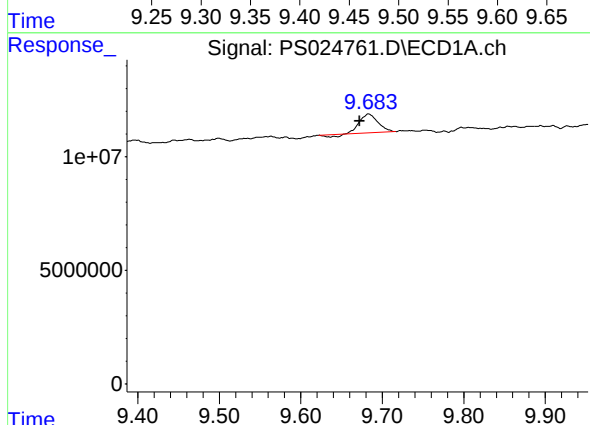


#15 Picloram

R.T.: 9.683 min
Delta R.T.: 0.011 min
Response: 12025544
Conc: N.D.

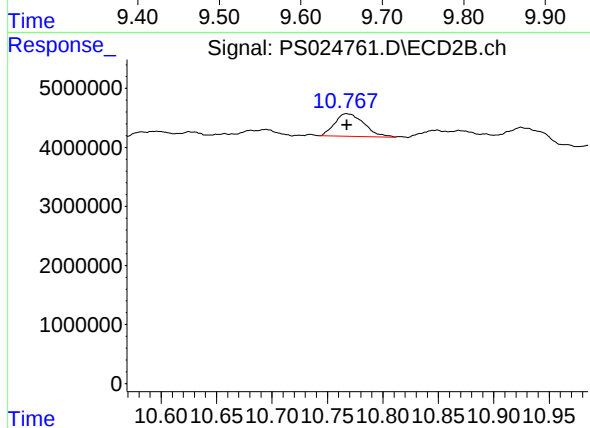

#15 Picloram


R.T.: 10.767 min
Delta R.T.: 0.000 min
Response: 7008633
Conc: 1.15 ng/ml

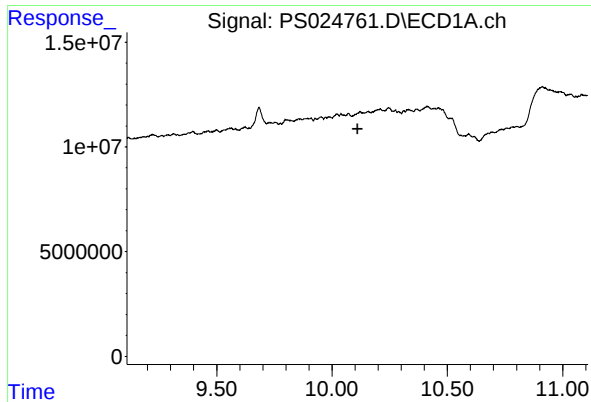

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

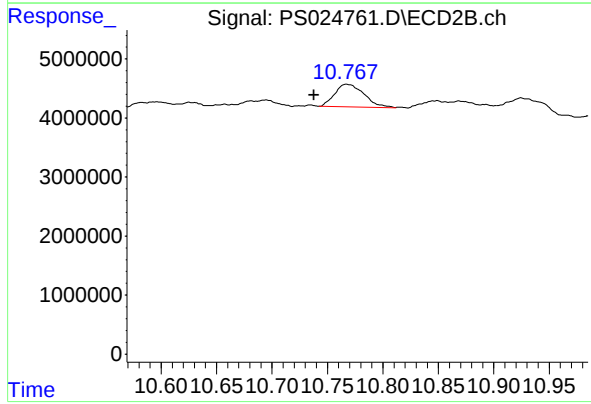

#16 DCPA

R.T.: 10.767 min
Delta R.T.: 0.029 min
Response: 7008633
Conc: 1.39 ng/ml