

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110623\
 Data File : PS024762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 09:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 23:06:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.357	6.776	1102.4E6	362.9E6	540.004	537.892
Target Compounds							
1) T	Dalapon	2.514	2.567	7134676	1688892	2.962	1.603 #
3) T	4-Nitroph...	6.196	6.376	10873136	1265238	8.388	2.881 #
6) T	MCPP	6.682	0.000	5292324	0	<MDL	N.D. #
7) T	MCPA	0.000	7.170f	0	14252166	N.D.	4.623
8) T	DICHLORPROP	0.000	7.565	0	4094330	N.D.	5.605
9) T	2,4-D	0.000	7.778f	0	1594817	N.D.	1.782
11) T	2,4,5-TP ...	0.000	8.617	0	492784	N.D.	<MDL
12) T	2,4,5-T	0.000	9.030f	0	2152859	N.D.	<MDL
13) T	2,4-DB	0.000	9.483	0	942004	N.D.	1.932
15) T	Picloram	9.684	10.773	31104346	9162527	1.749	1.508
16) T	DCPA	0.000	10.773	0	9162527	N.D.	1.823



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110623\
Data File : PS024762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 09:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 23:06:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

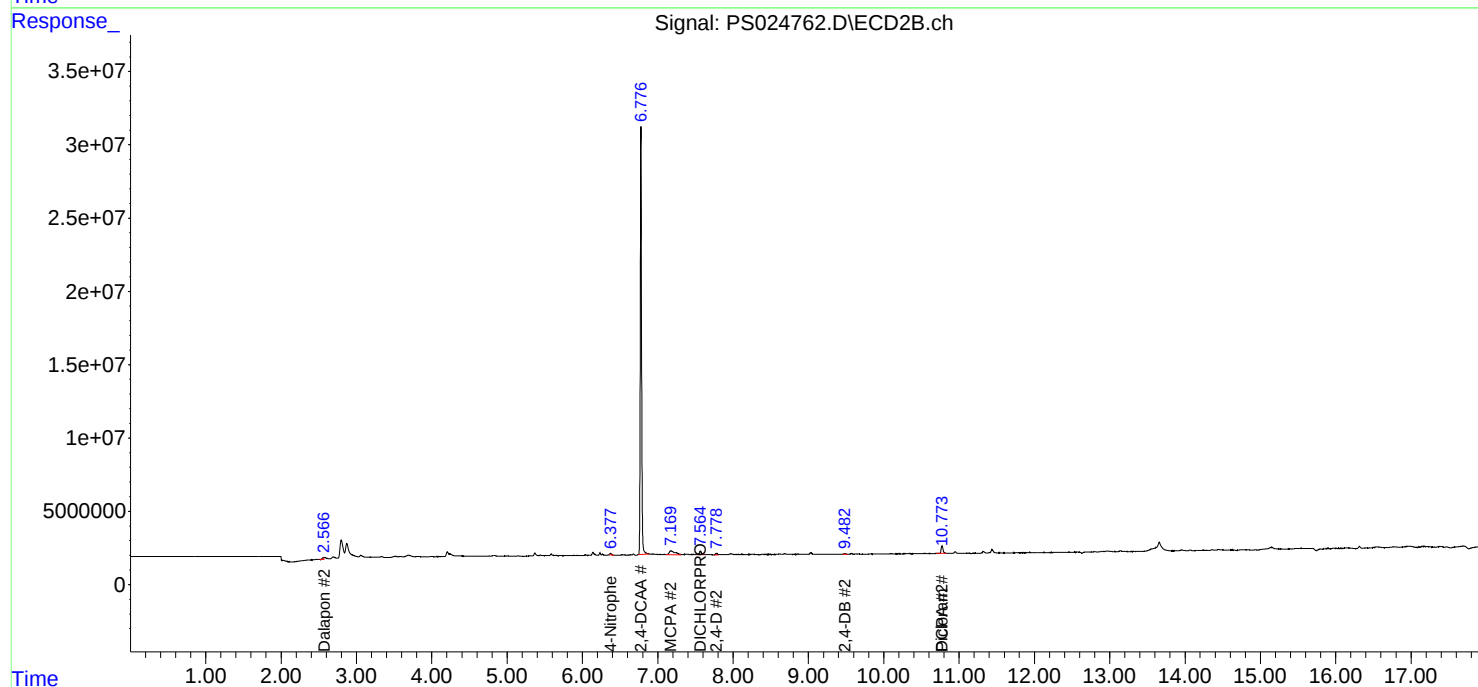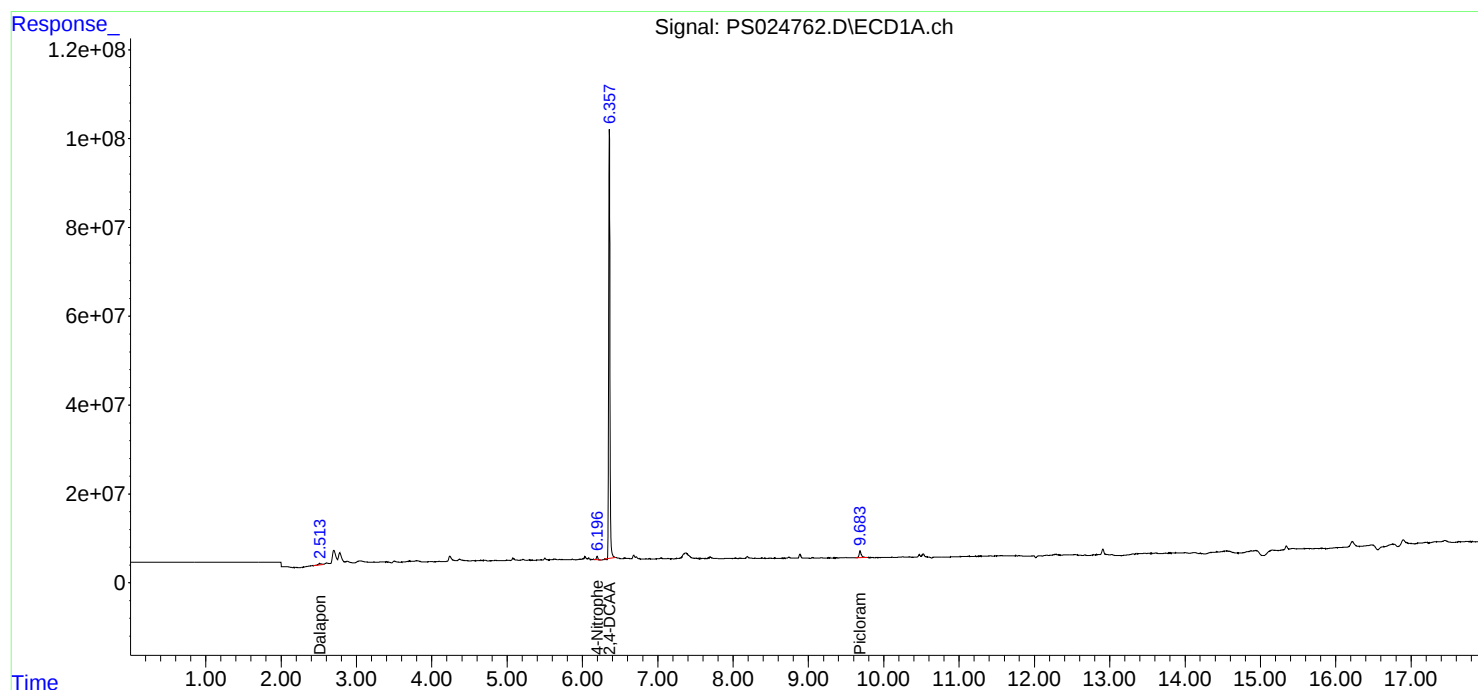


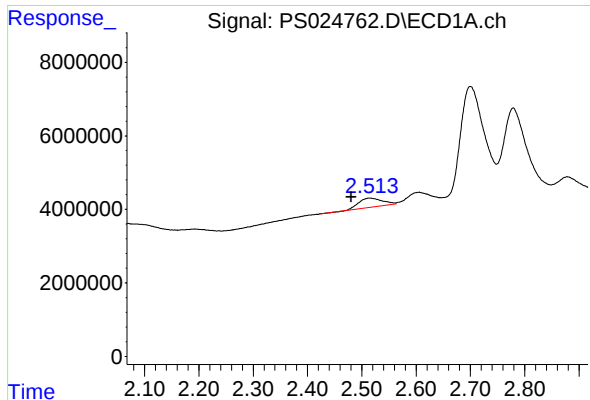

#1 Dalapon


R.T.: 2.514 min
Delta R.T.: 0.033 min
Response: 7134676
Conc: 2.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

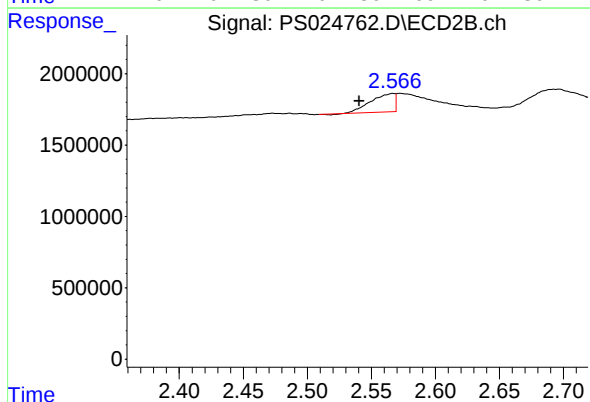


#1 Dalapon

R.T.: 2.567 min
Delta R.T.: 0.026 min
Response: 1688892
Conc: 1.60 ng/ml

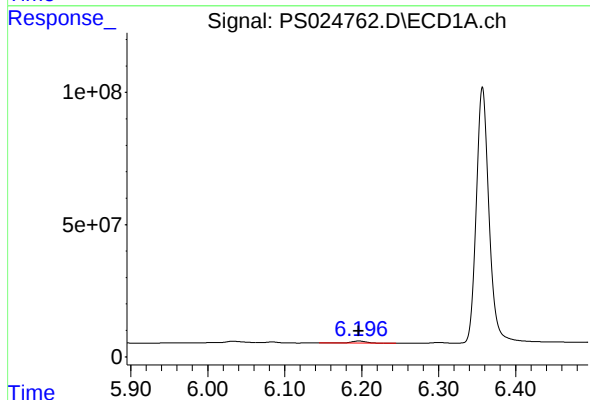


#3 4-Nitrophenol

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 10873136
Conc: 8.39 ng/ml

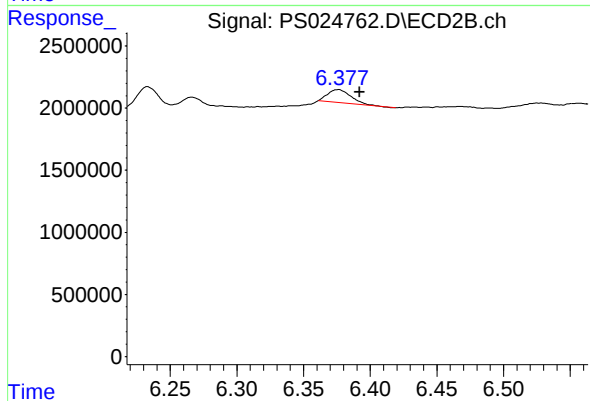

#3 4-Nitrophenol


R.T.: 6.376 min
Delta R.T.: -0.016 min
Response: 1265238
Conc: 2.88 ng/ml

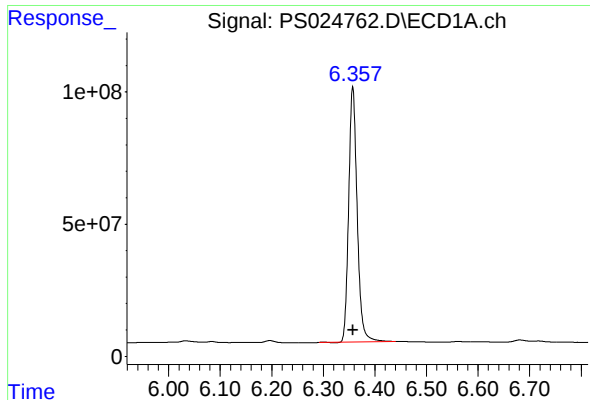

#4 2,4-DCAA


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1102419957
Conc: 540.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

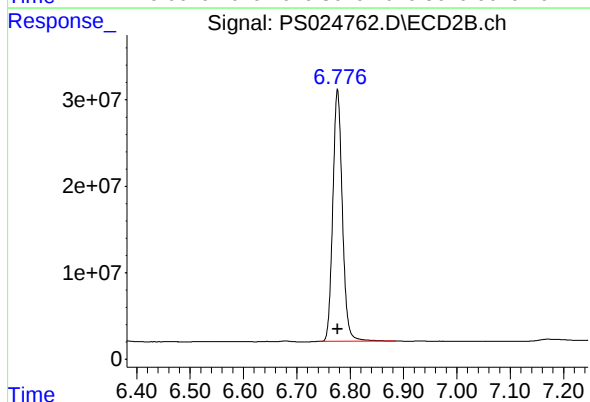


#4 2,4-DCAA

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 362861611
Conc: 537.89 ng/ml

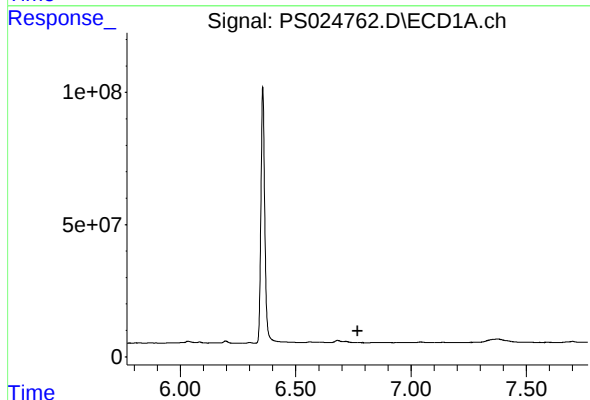


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

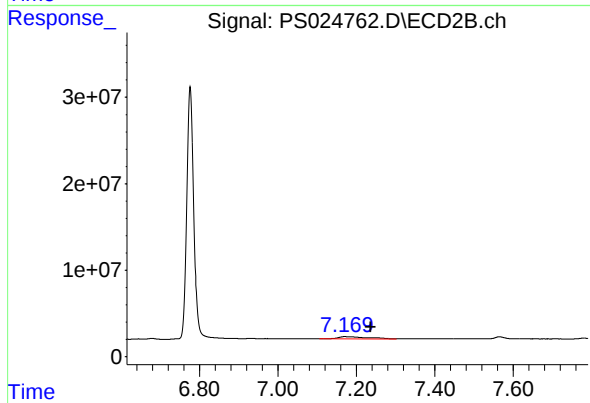

#7 MCPA


R.T.: 7.170 min
Delta R.T.: -0.067 min
Response: 14252166
Conc: 4.62 ug/ml

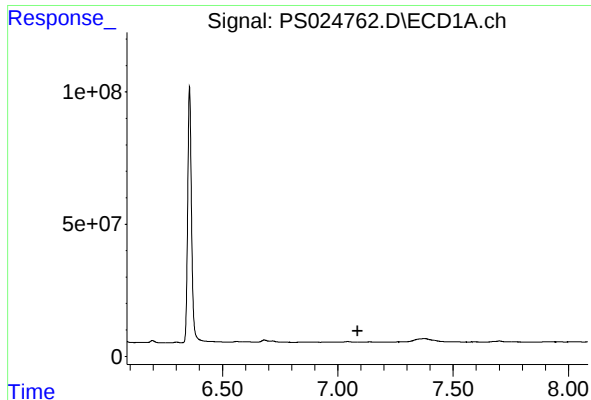

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

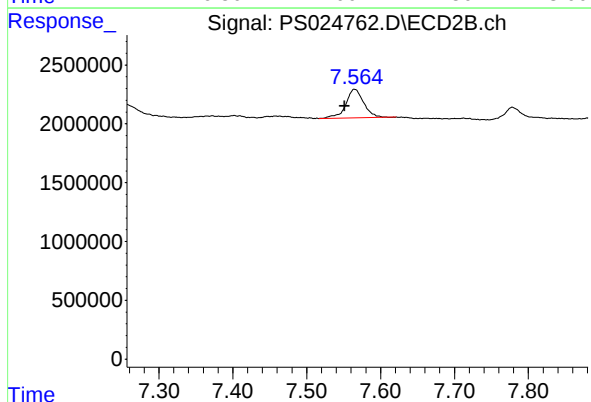


#8 DICHLORPROP

R.T.: 7.565 min
Delta R.T.: 0.014 min
Response: 4094330
Conc: 5.60 ng/ml

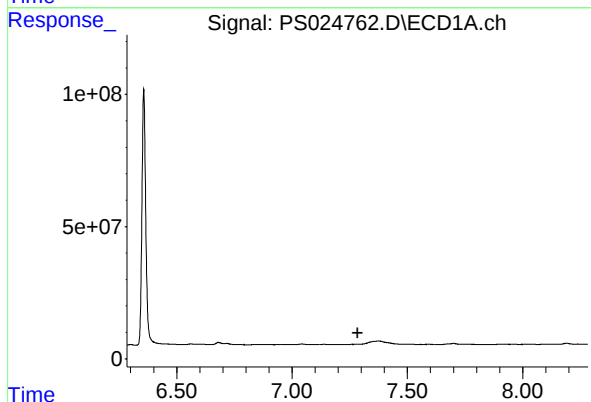


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

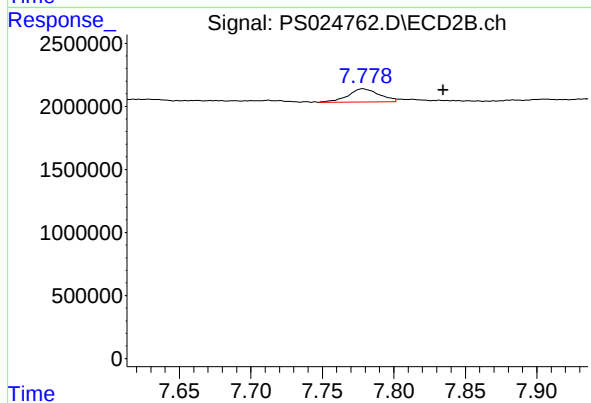

#9 2,4-D


R.T.: 7.778 min
Delta R.T.: -0.056 min
Response: 1594817
Conc: 1.78 ng/ml

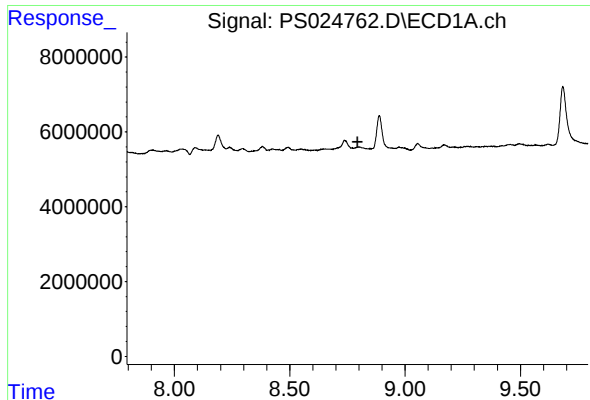

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

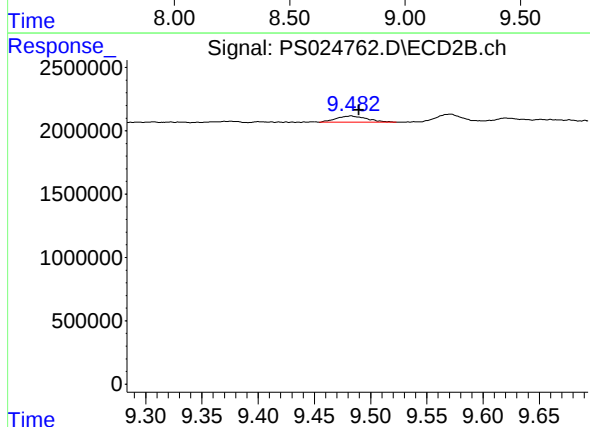


#13 2,4-DB

R.T.: 9.483 min
Delta R.T.: -0.007 min
Response: 942004
Conc: 1.93 ng/ml

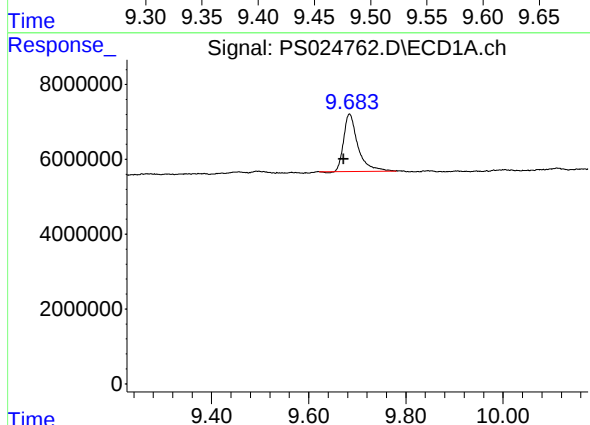


#15 Picloram

R.T.: 9.684 min
Delta R.T.: 0.012 min
Response: 31104346
Conc: 1.75 ng/ml

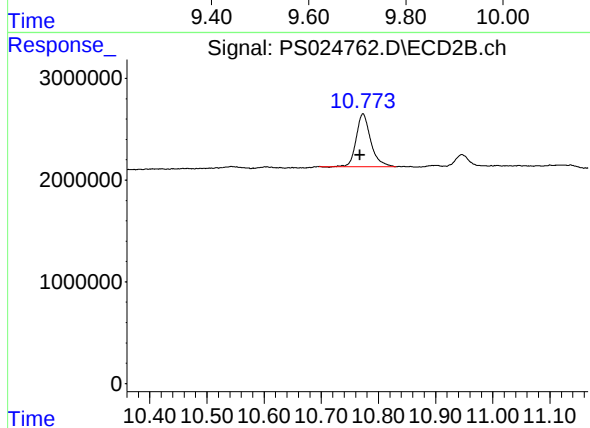

#15 Picloram


R.T.: 10.773 min
Delta R.T.: 0.005 min
Response: 9162527
Conc: 1.51 ng/ml

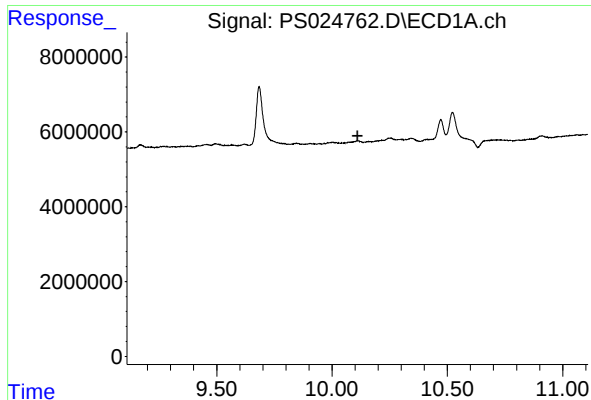

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

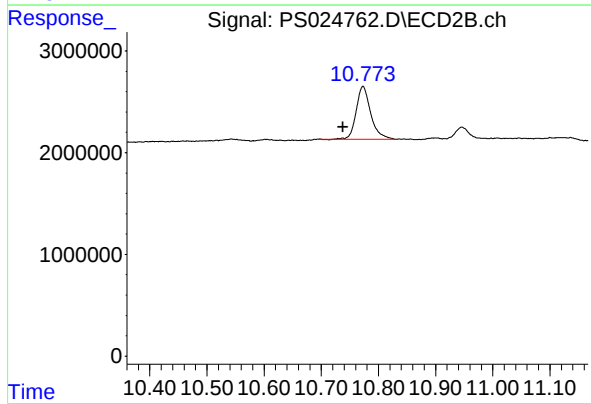

#16 DCPA

R.T.: 10.773 min
Delta R.T.: 0.035 min
Response: 9162527
Conc: 1.82 ng/ml