

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 09:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 11:48:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.262	7.764	1253.5E6	855.9E6	489.362	491.394
Target Compounds							
3) T	4-Nitroph...	7.055	0.000	4405376	0	2.674	N.D. #
6) T	MCPD	7.688f	8.116f	13582644	1602491	1.791	<MDL #
7) T	MCPA	0.000	8.286f	0	12266528	N.D.	1.471
8) T	DICHLORPROP	8.159	0.000	359873	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.946	0	12909934	N.D.	1.038
15) T	Picloram	11.169	12.393	12468607	10163959	<MDL	<MDL #
16) T	DCPA	11.641	0.000	1769706	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 09:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 11:48:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

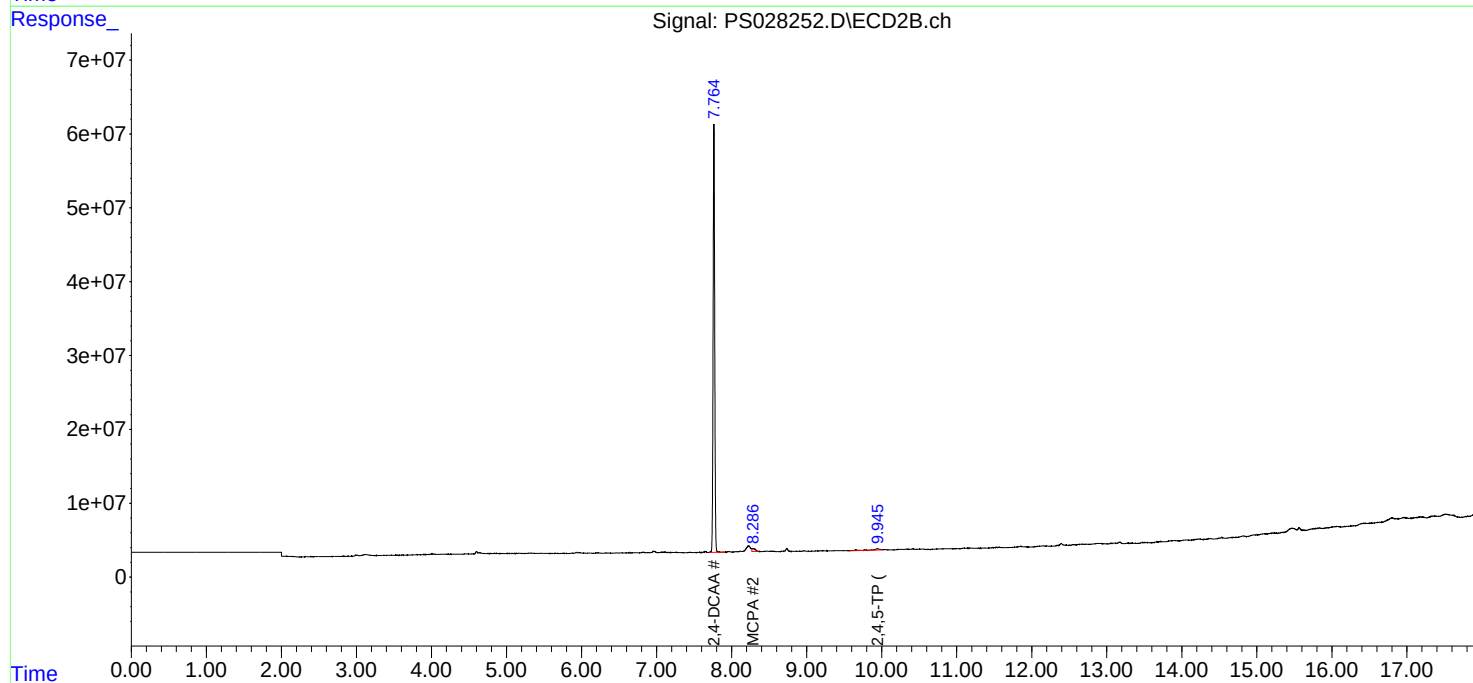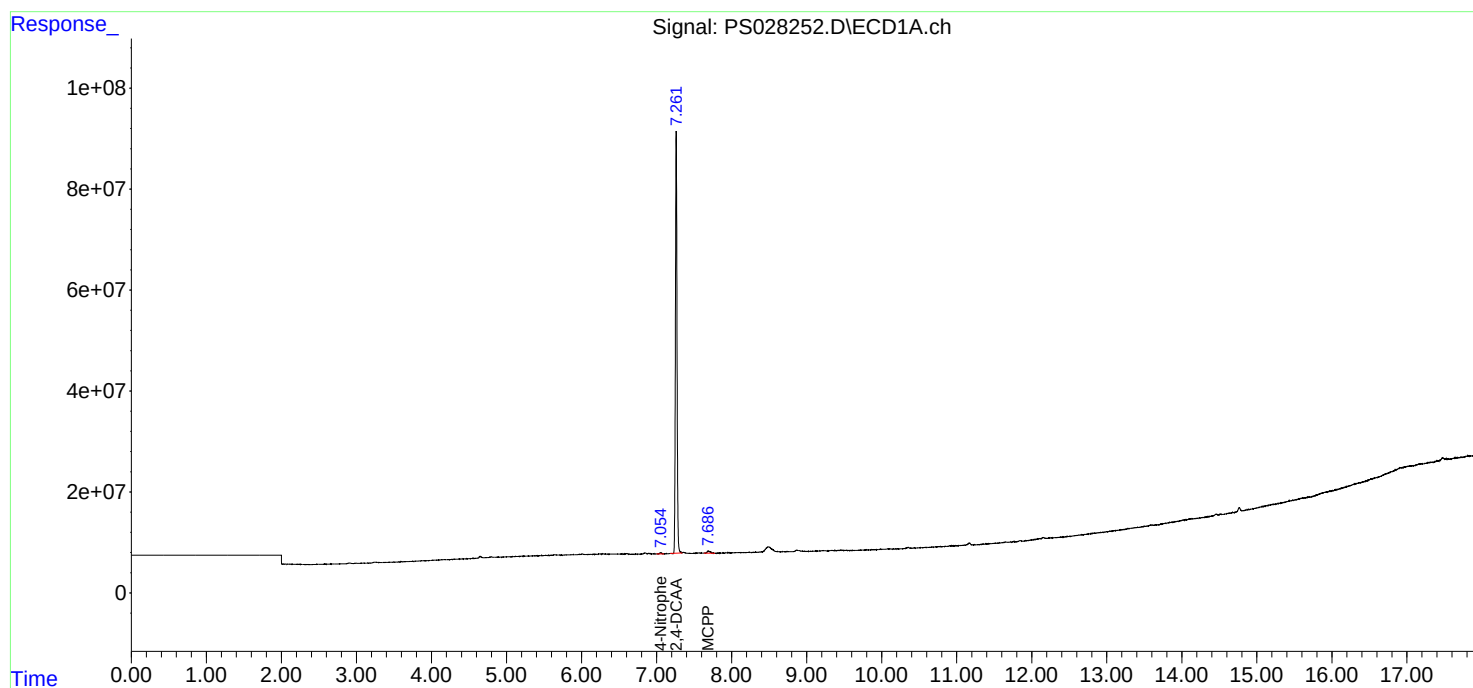


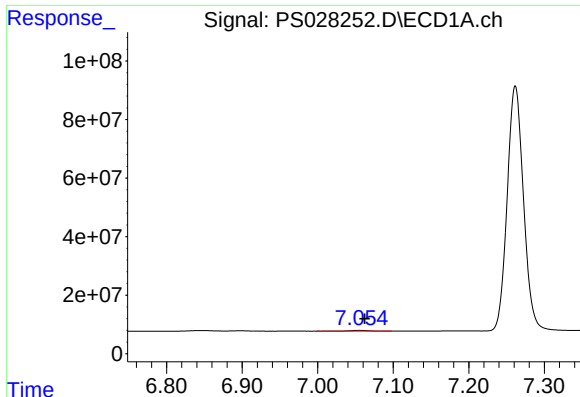

#3 4-Nitrophenol


R.T.: 7.055 min
Delta R.T.: -0.007 min
Response: 4405376
Conc: 2.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

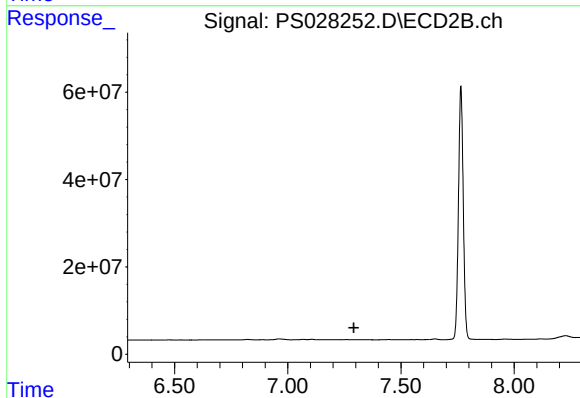


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

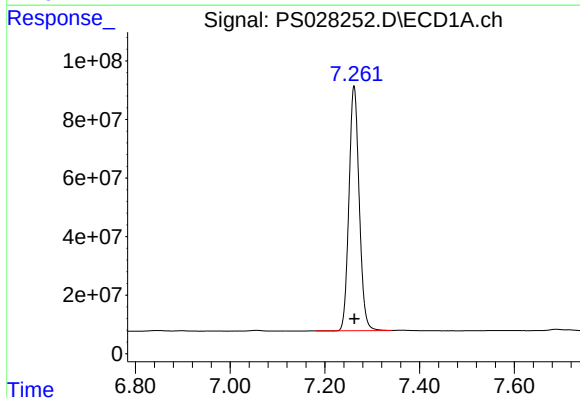


#4 2,4-DCAA

R.T.: 7.262 min
Delta R.T.: 0.000 min
Response: 1253458597
Conc: 489.36 ng/ml

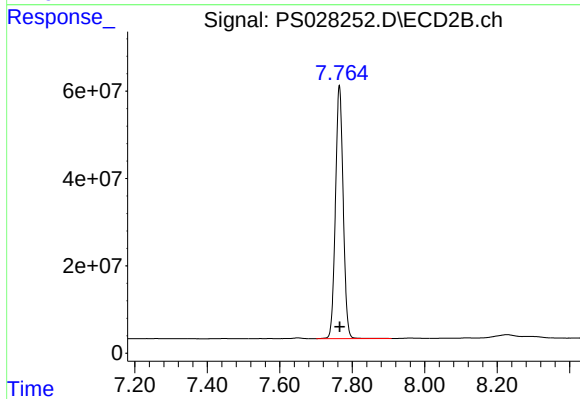

#4 2,4-DCAA


R.T.: 7.764 min
Delta R.T.: 0.000 min
Response: 855899732
Conc: 491.39 ng/ml

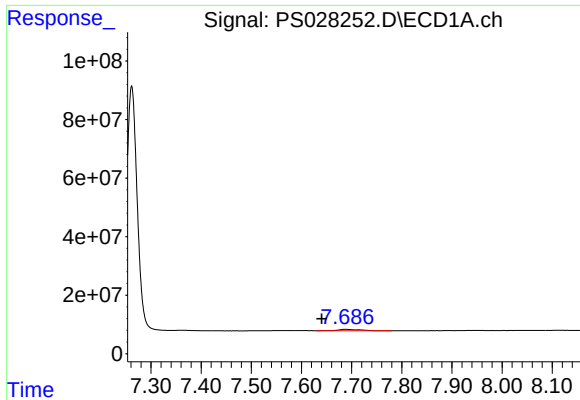

#6 MCPP


R.T.: 7.688 min
Delta R.T.: 0.047 min
Response: 13582644
Conc: 1.79 ug/ml

Instrument :
ECD_S
ClientSampleId :

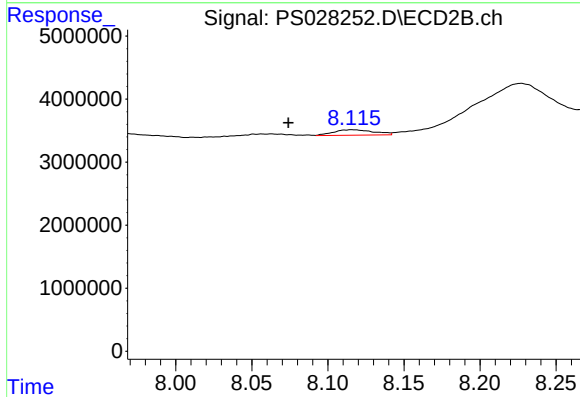


#6 MCPP

R.T.: 8.116 min
Delta R.T.: 0.042 min
Response: 1602491
Conc: N.D.

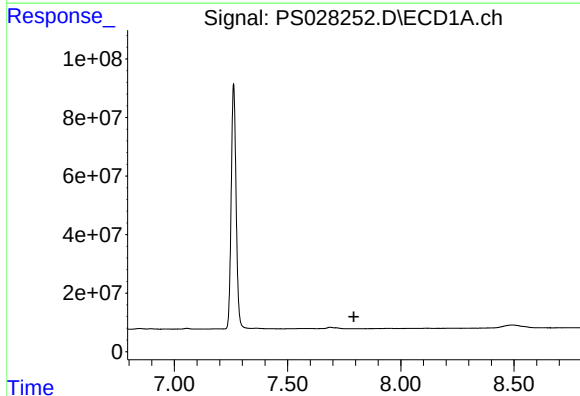


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

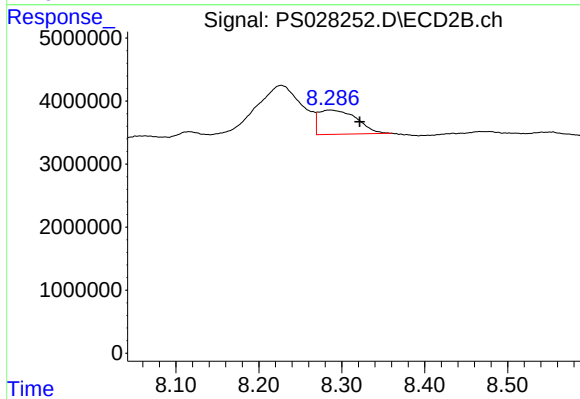

#7 MCPA


R.T.: 8.286 min
Delta R.T.: -0.036 min
Response: 12266528
Conc: 1.47 ug/ml

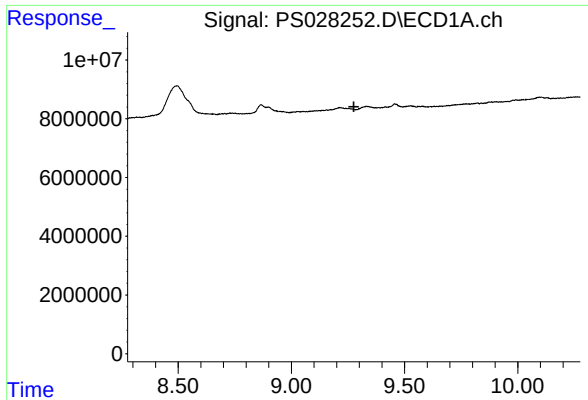

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

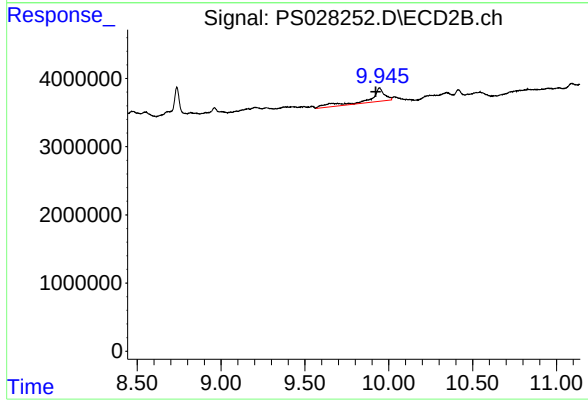

#11 2,4,5-TP (SILVEX)

R.T.: 9.946 min
Delta R.T.: 0.024 min
Response: 12909934
Conc: 1.04 ng/ml