

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 09:48
 Operator : AR\AJ
 Sample : HSTDICC200
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 11:36:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:36:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.262	7.765	582.3E6	371.2E6	223.512	211.533
Target Compounds							
1) T	Dalapon	2.653	2.711	642.4E6	562.1E6	181.633	189.953
2) T	3,5-DICHL...	6.429	6.716	776.6E6	497.7E6	203.432	195.199
3) T	4-Nitroph...	7.062	7.291	321.8E6	224.2E6	193.828	194.321
5) T	DICAMBA	7.451	7.966	2215.0E6	1497.1E6	195.228	186.177
6) T	MCPD	7.631	8.064	125.9E6	109.8E6	16.918	18.245
7) T	MCPA	7.780	8.309	187.1E6	163.1E6	18.066	19.509
8) T	DICHLORPROP	8.162	8.684	591.9E6	395.3E6	206.431	195.806
9) T	2,4-D	8.394	9.015	657.9E6	441.5E6	205.017	196.565
10) T	Pentachlo...	8.693	9.547	8878.0E6	5945.0E6	203.188	199.509
11) T	2,4,5-TP ...	9.276	9.923	3492.5E6	2460.7E6	201.633	195.549
12) T	2,4,5-T	9.569	10.345	3534.9E6	2429.8E6	200.660	195.776
13) T	2,4-DB	10.147	10.912	561.2E6	303.0E6	197.443	191.585
14) T	DINOSEB	11.364	11.292	2842.8E6	1680.5E6	194.787	191.515
15) T	Picloram	11.169	12.392	5567.6E6	3307.4E6	190.816	182.953
16) T	DCPA	11.656	12.339	4826.0E6	2771.8E6	200.001	195.462



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 09:48
Operator : AR\AJ
Sample : HSTDICC200
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 11:36:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:36:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

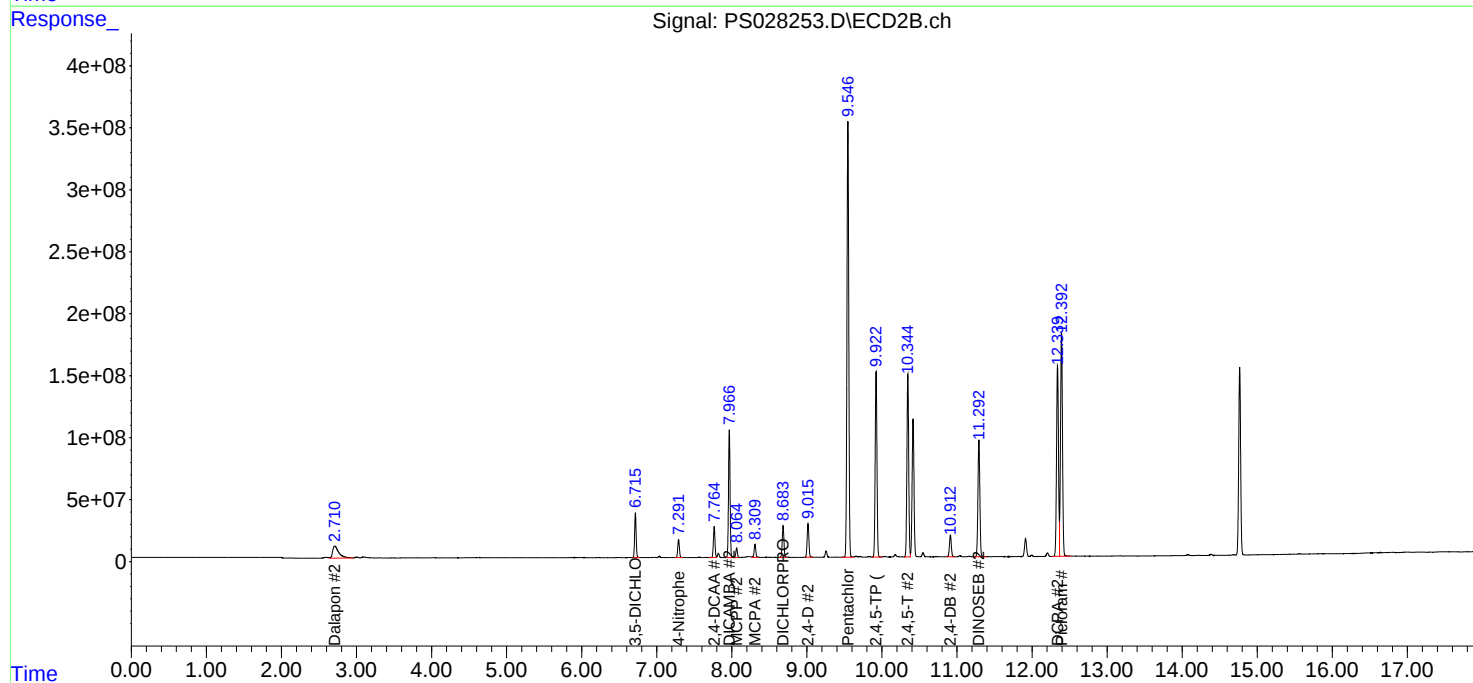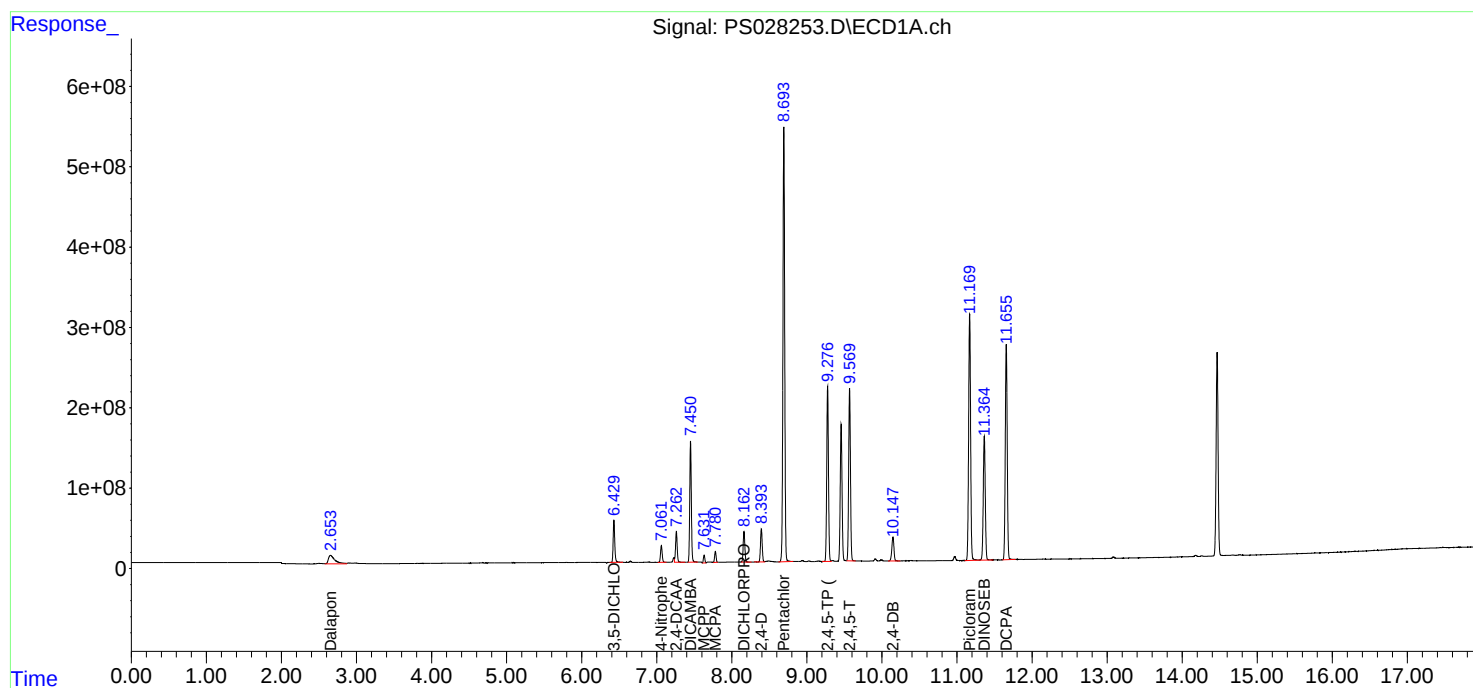


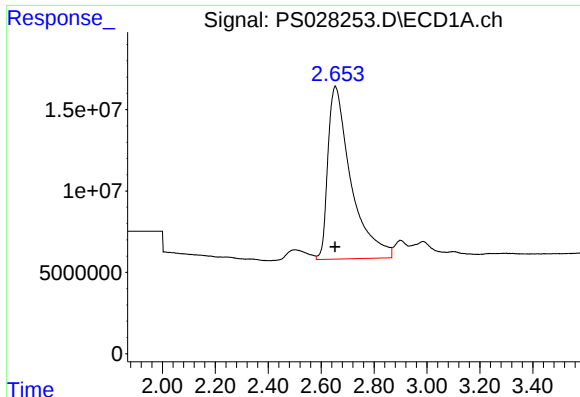

#1 Dalapon


R.T.: 2.653 min
Delta R.T.: 0.000 min
Response: 642355079
Conc: 181.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

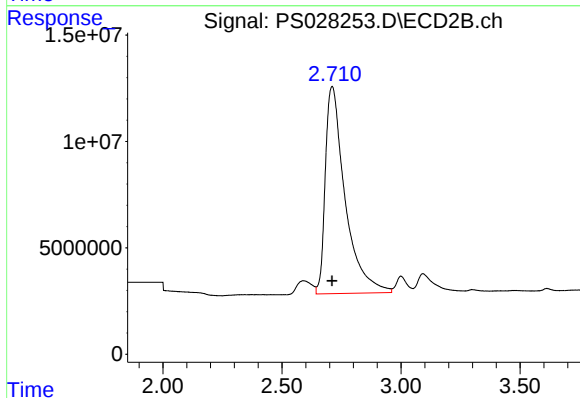


#1 Dalapon

R.T.: 2.711 min
Delta R.T.: 0.000 min
Response: 562114992
Conc: 189.95 ng/ml

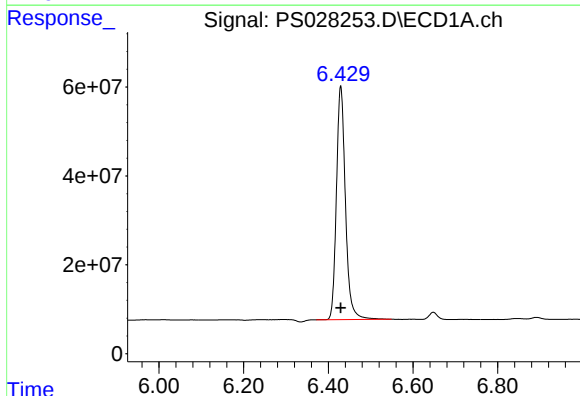


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.429 min
Delta R.T.: 0.000 min
Response: 776591468
Conc: 203.43 ng/ml

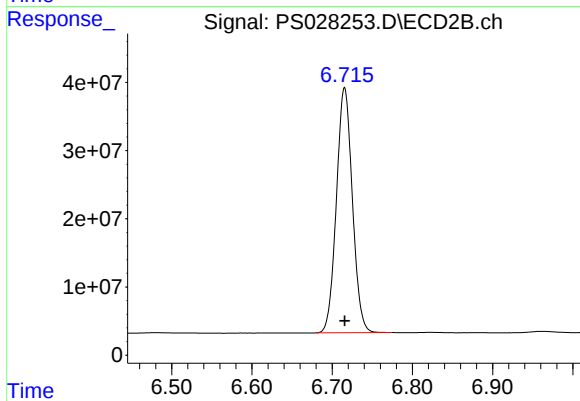

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 497741373
Conc: 195.20 ng/ml

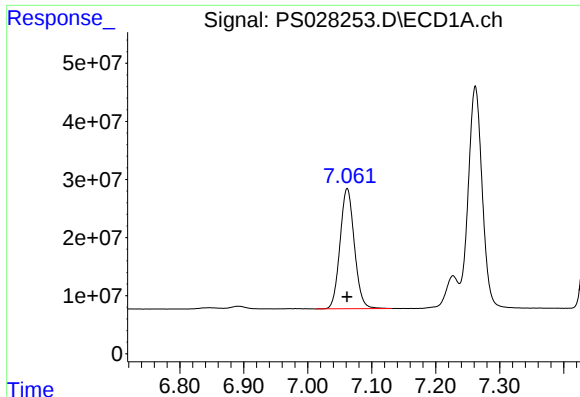

#3 4-Nitrophenol


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 321799911
Conc: 193.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

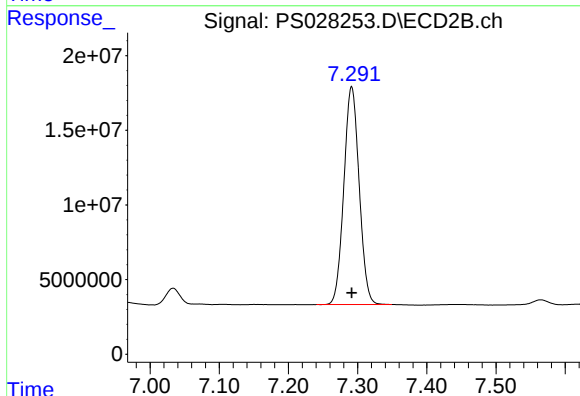


#3 4-Nitrophenol

R.T.: 7.291 min
Delta R.T.: 0.000 min
Response: 224189111
Conc: 194.32 ng/ml

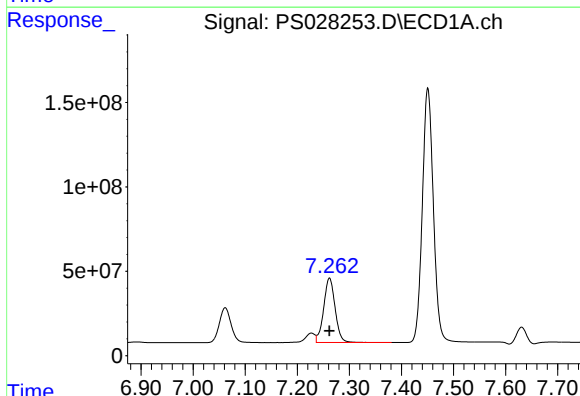


#4 2,4-DCAA

R.T.: 7.262 min
Delta R.T.: 0.000 min
Response: 582320101
Conc: 223.51 ng/ml

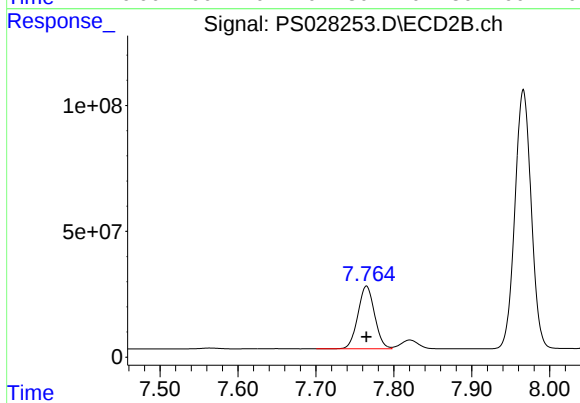

#4 2,4-DCAA


R.T.: 7.765 min
Delta R.T.: 0.000 min
Response: 371191822
Conc: 211.53 ng/ml

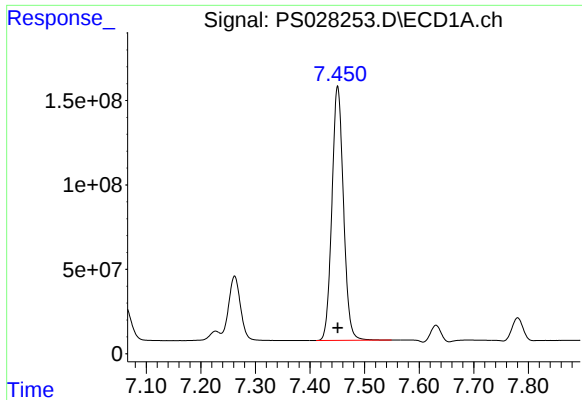

#5 DICAMBA


R.T.: 7.451 min
Delta R.T.: 0.000 min
Response: 2214982590
Conc: 195.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

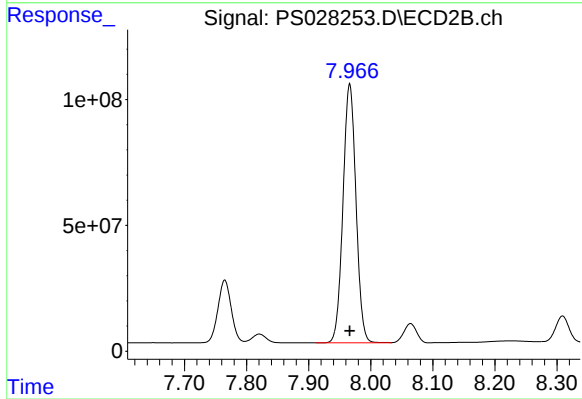


#5 DICAMBA

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 1497117095
Conc: 186.18 ng/ml

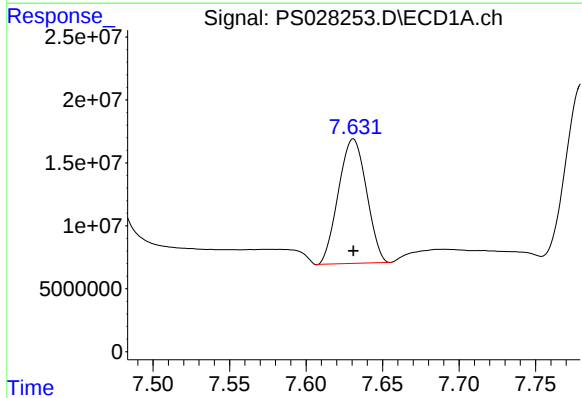


#6 MCP

R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 125946998
Conc: 16.92 ug/ml

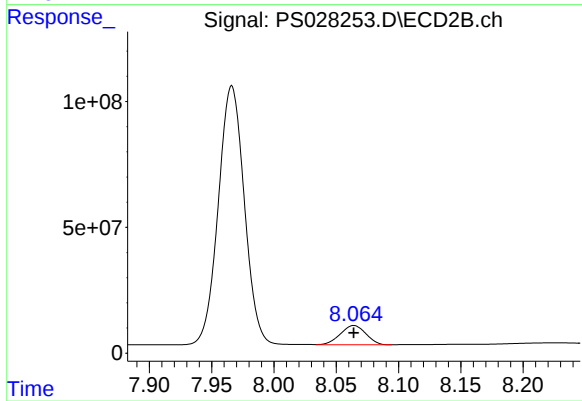

#6 MCP


R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 109825902
Conc: 18.24 ug/ml

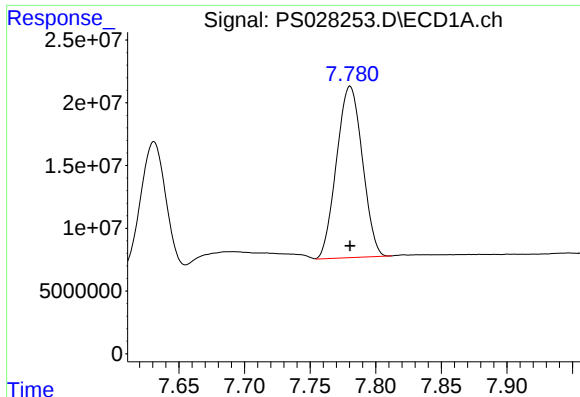

#7 MCPA


R.T.: 7.780 min
Delta R.T.: 0.000 min
Response: 187056081
Conc: 18.07 ug/ml

Instrument :
ECD_S
ClientSampleId :

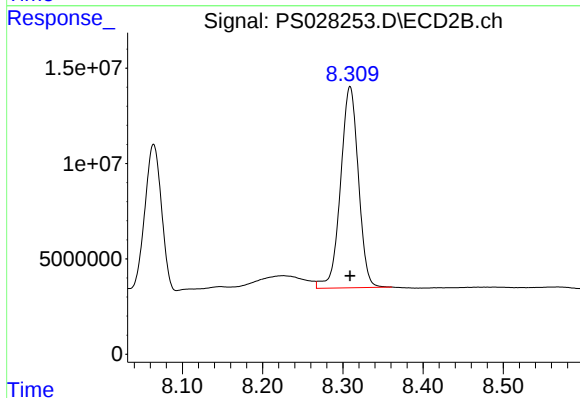


#7 MCPA

R.T.: 8.309 min
Delta R.T.: 0.000 min
Response: 163086934
Conc: 19.51 ug/ml

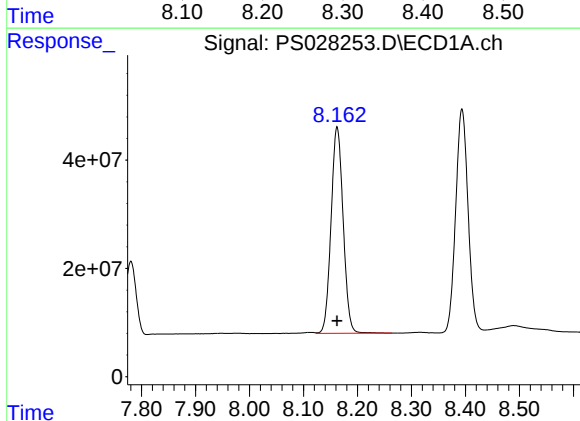


#8 DICHLORPROP

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 591896274
Conc: 206.43 ng/ml

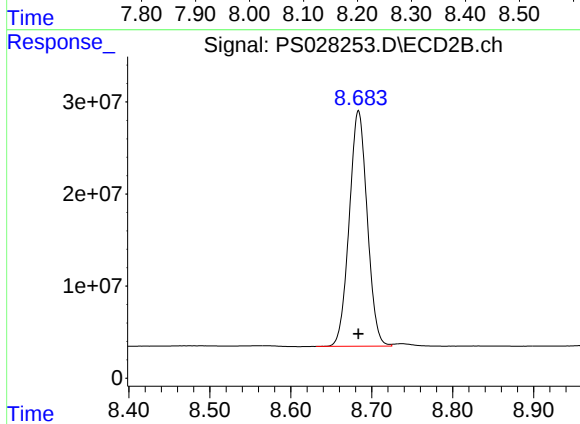

#8 DICHLORPROP


R.T.: 8.684 min
Delta R.T.: 0.000 min
Response: 395301941
Conc: 195.81 ng/ml

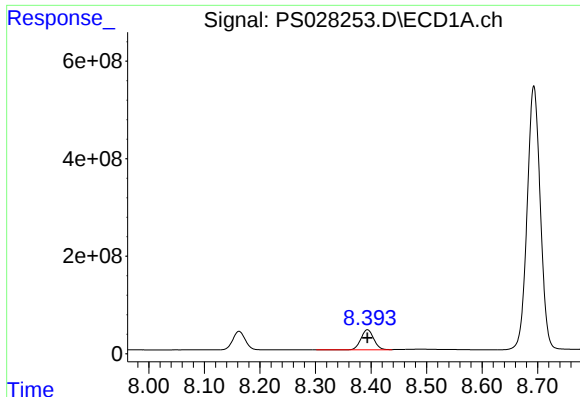

#9 2,4-D


R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 657909754
Conc: 205.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

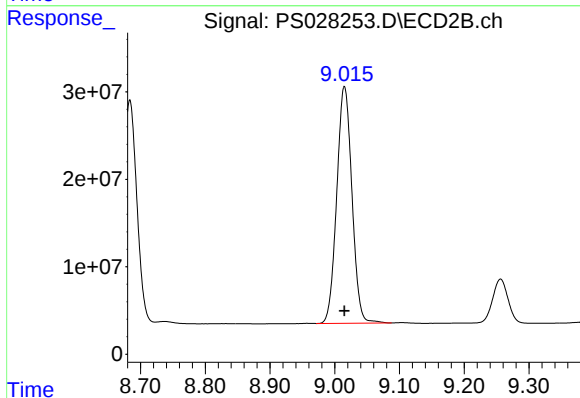


#9 2,4-D

R.T.: 9.015 min
Delta R.T.: 0.000 min
Response: 441456361
Conc: 196.57 ng/ml

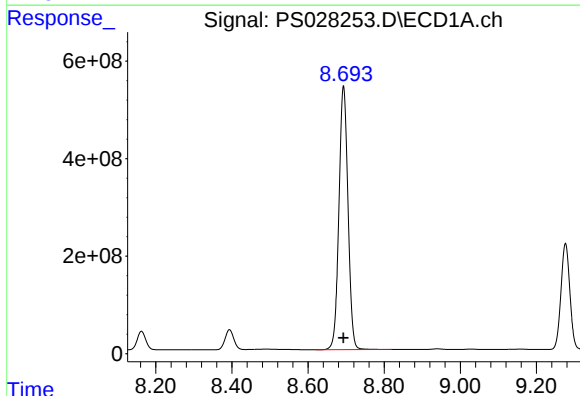


#10 Pentachlorophenol

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 8877976889
Conc: 203.19 ng/ml

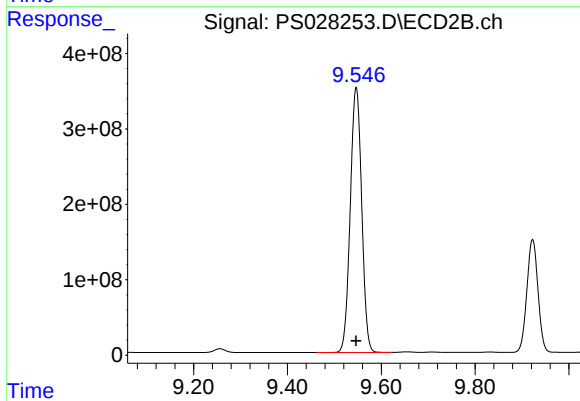

#10 Pentachlorophenol


R.T.: 9.547 min
Delta R.T.: 0.000 min
Response: 5945020071
Conc: 199.51 ng/ml

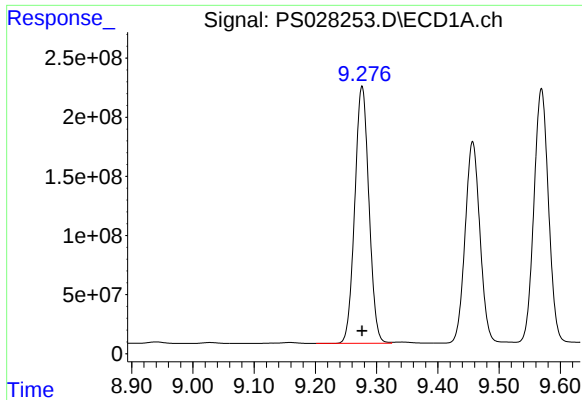

#11 2,4,5-TP (SILVEX)


R.T.: 9.276 min
Delta R.T.: 0.000 min
Response: 3492467343
Conc: 201.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

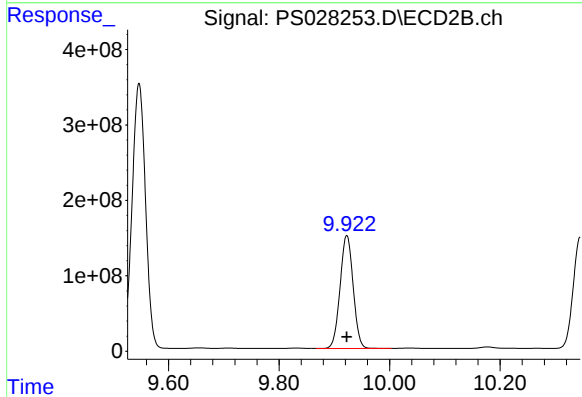


#11 2,4,5-TP (SILVEX)

R.T.: 9.923 min
Delta R.T.: 0.000 min
Response: 2460679717
Conc: 195.55 ng/ml

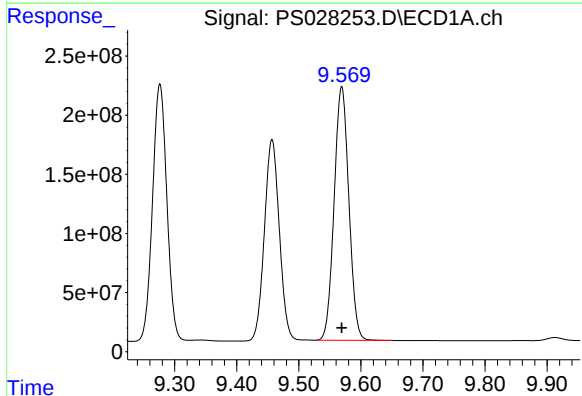


#12 2,4,5-T

R.T.: 9.569 min
Delta R.T.: 0.000 min
Response: 3534947725
Conc: 200.66 ng/ml

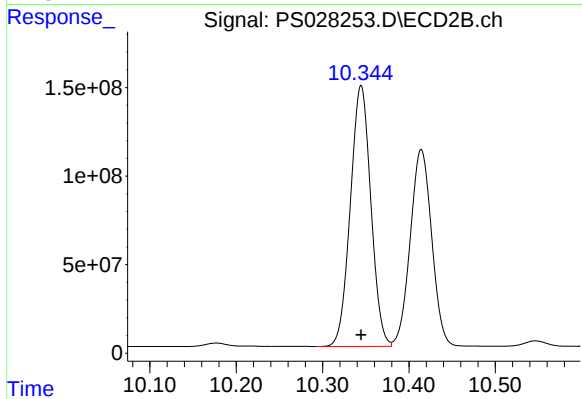

#12 2,4,5-T


R.T.: 10.345 min
Delta R.T.: 0.000 min
Response: 2429791973
Conc: 195.78 ng/ml

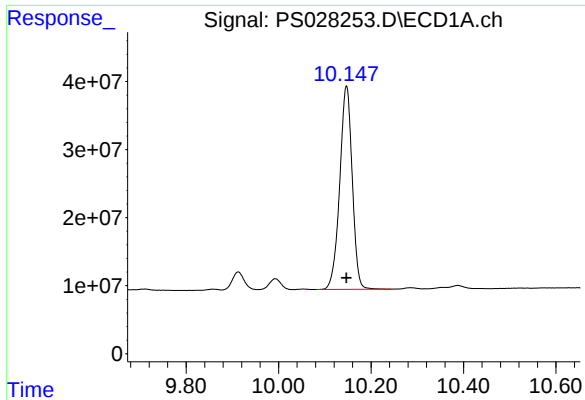

#13 2,4-DB


R.T.: 10.147 min
Delta R.T.: 0.000 min
Response: 561209882
Conc: 197.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

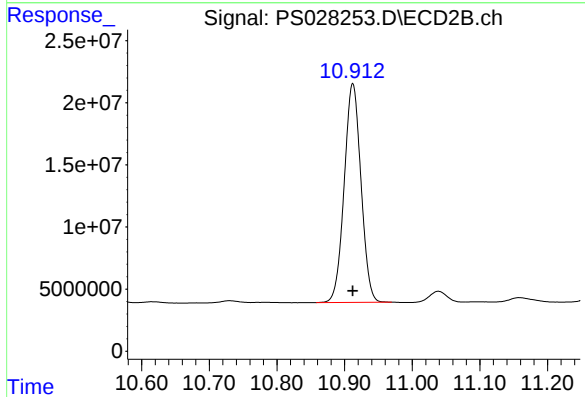


#13 2,4-DB

R.T.: 10.912 min
Delta R.T.: 0.000 min
Response: 302991891
Conc: 191.58 ng/ml

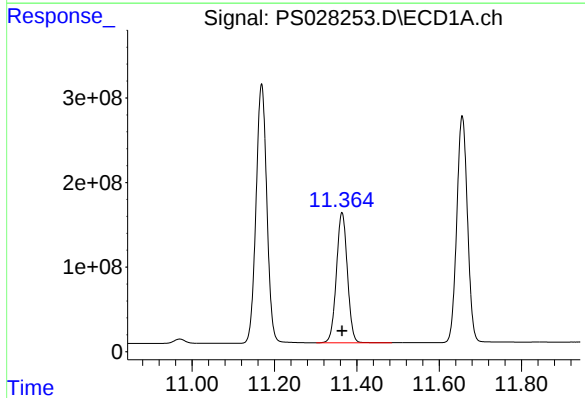


#14 DINOSEB

R.T.: 11.364 min
Delta R.T.: 0.000 min
Response: 2842779862
Conc: 194.79 ng/ml

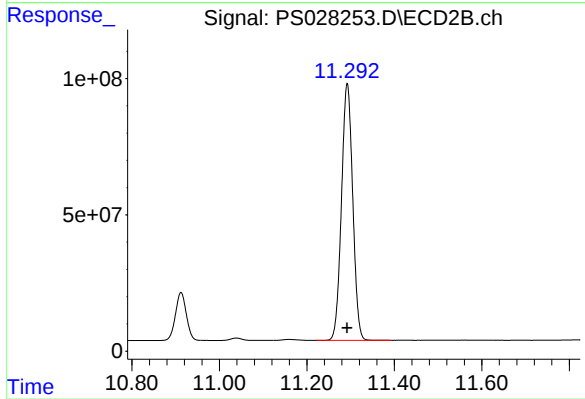

#14 DINOSEB


R.T.: 11.292 min
Delta R.T.: 0.000 min
Response: 1680529004
Conc: 191.52 ng/ml

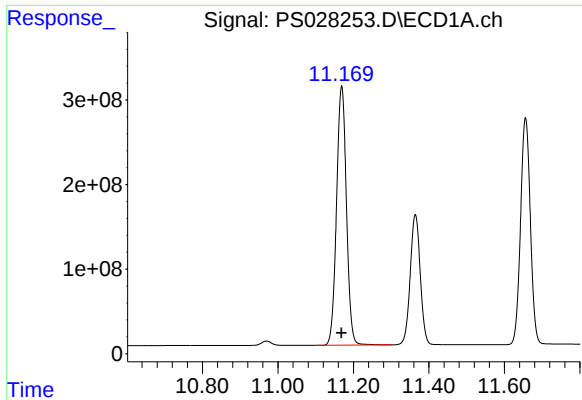

#15 Picloram


R.T.: 11.169 min
Delta R.T.: 0.000 min
Response: 5567638798
Conc: 190.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

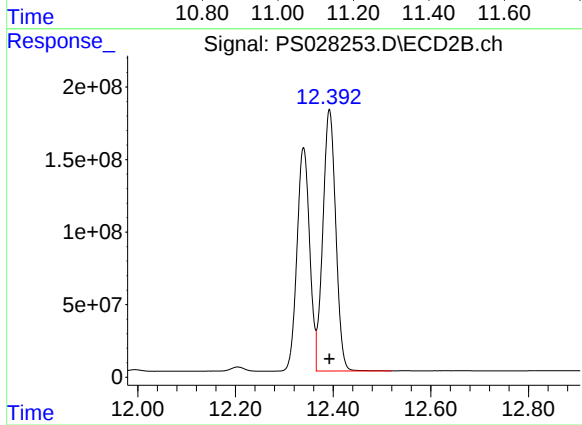


#15 Picloram

R.T.: 12.392 min
Delta R.T.: 0.000 min
Response: 3307364314
Conc: 182.95 ng/ml

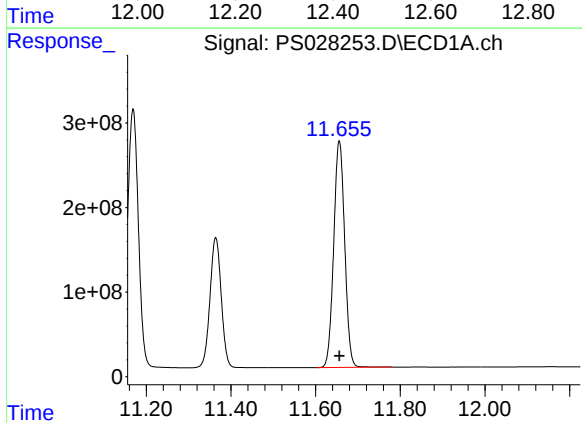

#16 DCPA

R.T.: 11.656 min
Delta R.T.: 0.000 min
Response: 4826032560
Conc: 200.00 ng/ml

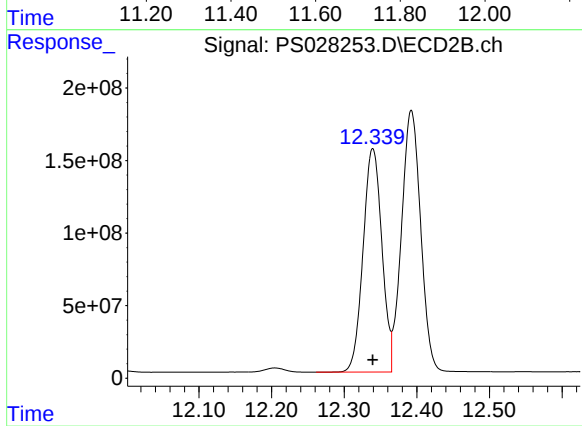

#16 DCPA

R.T.: 12.339 min
Delta R.T.: 0.000 min
Response: 2771776460
Conc: 195.46 ng/ml