

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 12:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 13:28:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.263	7.764	1282.2E6	881.4E6	500.591	506.018
Target Compounds							
1) T	Dalapon	2.640	0.000	753441	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.413	0.000	901724	0	<MDL	N.D. #
3) T	4-Nitroph...	7.055	0.000	6584698	0	3.997	N.D. #
5) T	DICAMBA	0.000	7.959	0	3844282	N.D.	<MDL
6) T	MCP	7.690f	8.058	18343249	1512441	2.419	<MDL #
8) T	DICHLORPROP	8.121f	0.000	1061423	0	<MDL	N.D. #
10) T	Pentachlo...	8.695	0.000	812699	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.945	0	6451491	N.D.	<MDL
12) T	2,4,5-T	0.000	10.339	0	4394998	N.D.	<MDL
13) T	2,4-DB	10.101f	0.000	1696656	0	<MDL	N.D. #
14) T	DINOSEB	11.350	0.000	3406789	0	<MDL	N.D. #
15) T	Picloram	11.167	12.391	60502220	28824710	2.086	1.599
16) T	DCPA	11.642	12.349	7708842	6449381	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 12:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 13:28:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

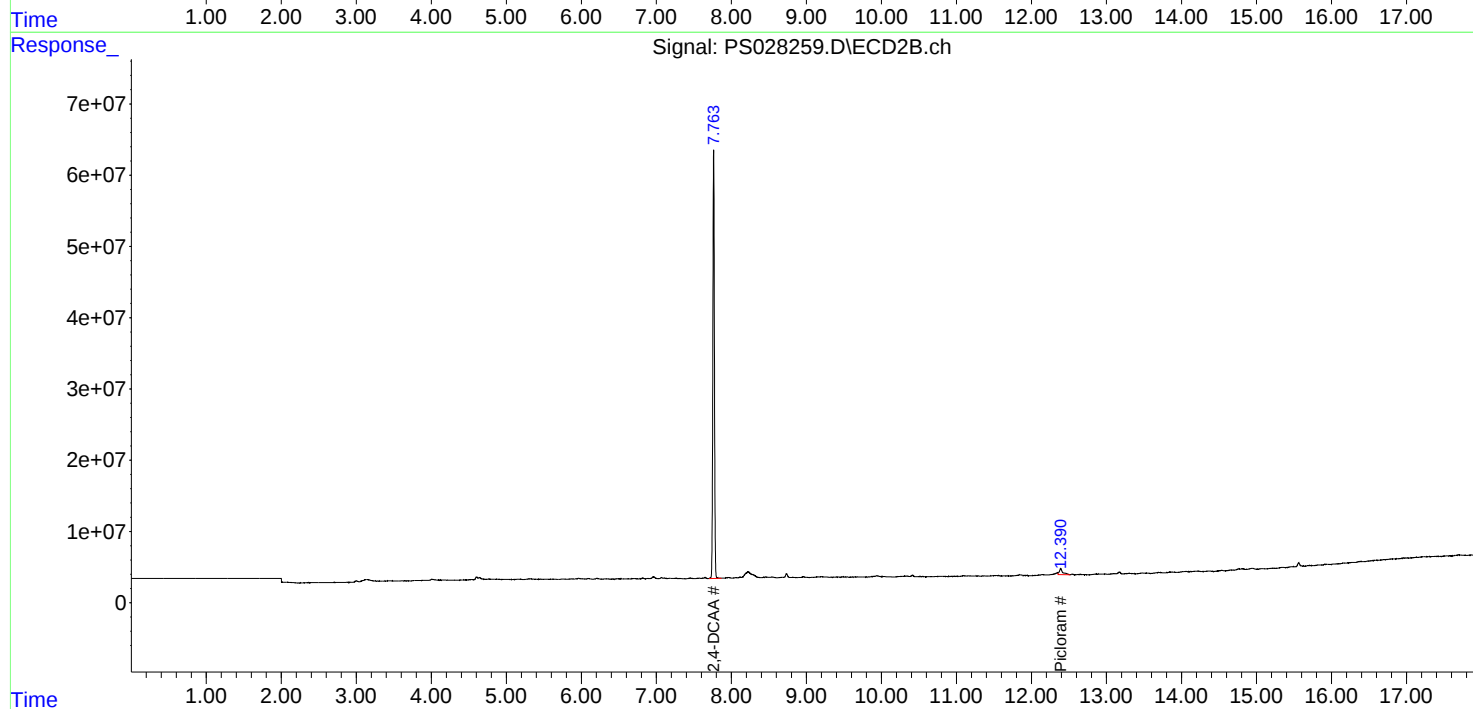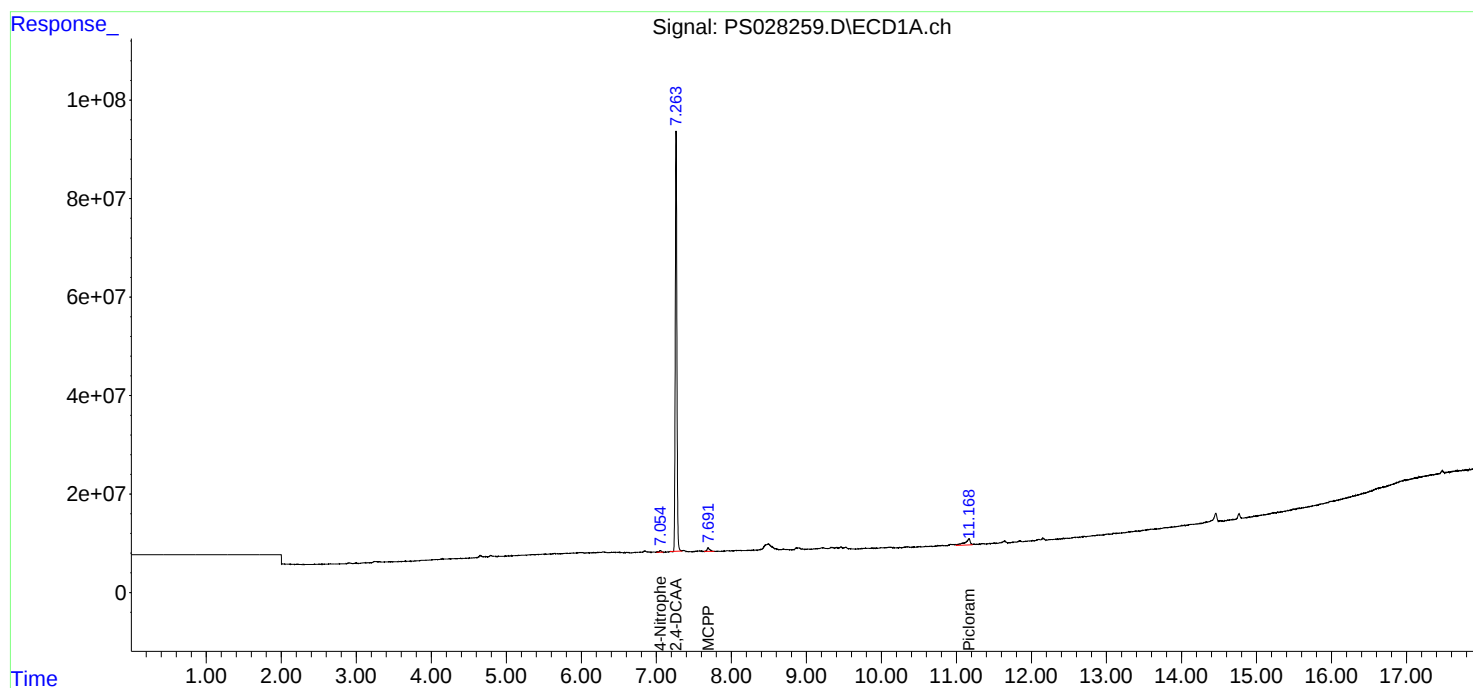


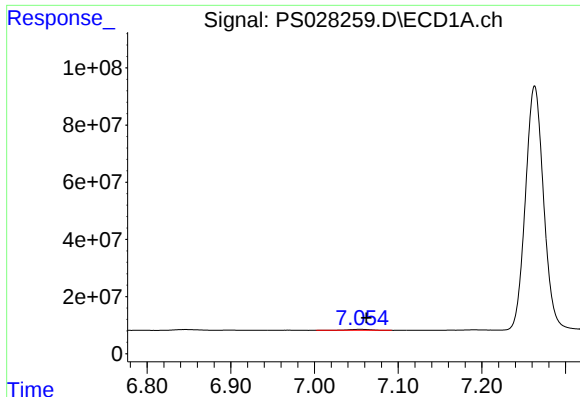

#3 4-Nitrophenol


R.T.: 7.055 min
Delta R.T.: -0.007 min
Response: 6584698
Conc: 4.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

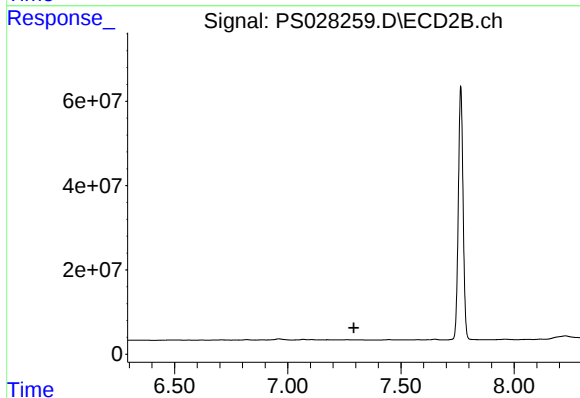


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

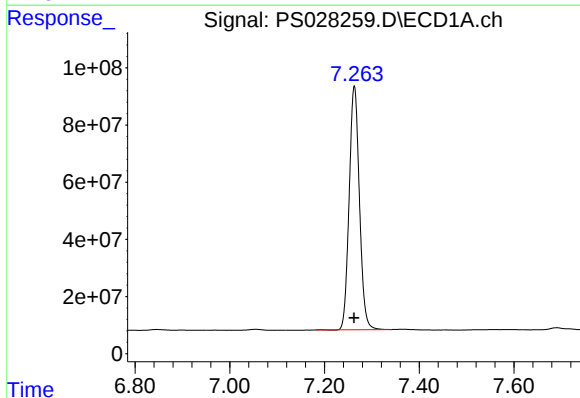


#4 2,4-DCAA

R.T.: 7.263 min
Delta R.T.: 0.000 min
Response: 1282219580
Conc: 500.59 ng/ml

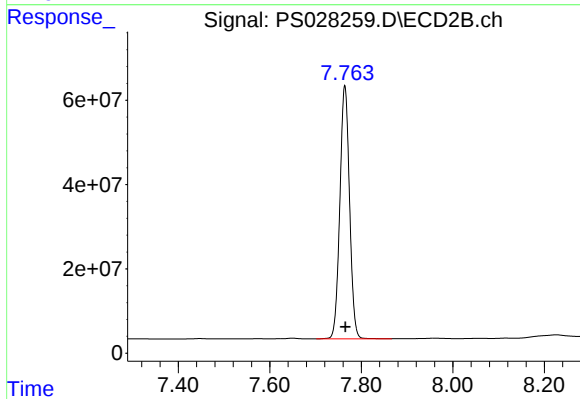

#4 2,4-DCAA


R.T.: 7.764 min
Delta R.T.: -0.001 min
Response: 881371225
Conc: 506.02 ng/ml

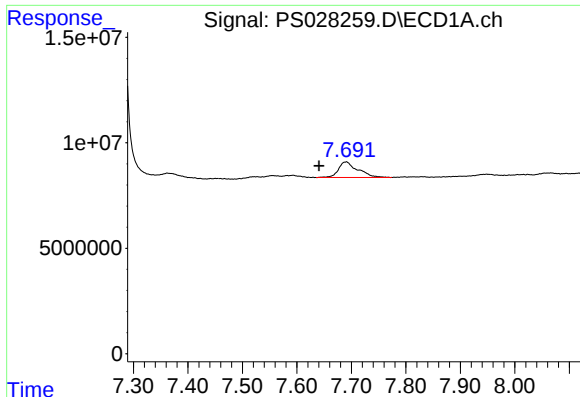

#6 MCP


R.T.: 7.690 min
Delta R.T.: 0.049 min
Response: 18343249
Conc: 2.42 ug/ml

Instrument :
ECD_S
ClientSampleId :

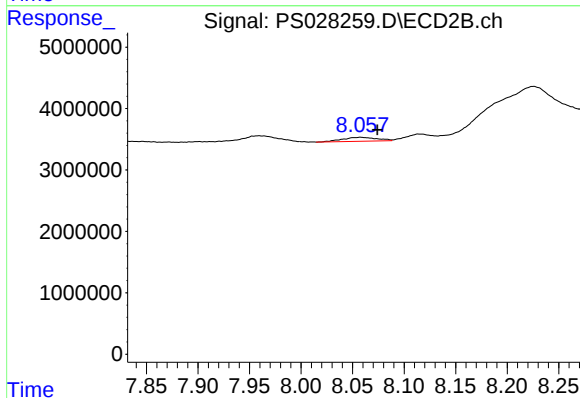


#6 MCP

R.T.: 8.058 min
Delta R.T.: -0.016 min
Response: 1512441
Conc: N.D.

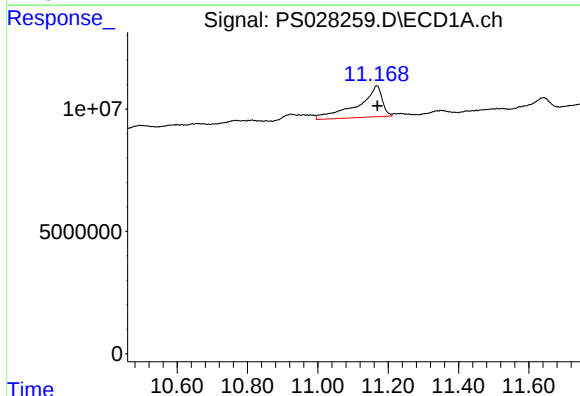

#15 Picloram

R.T.: 11.167 min
Delta R.T.: -0.002 min
Response: 60502220
Conc: 2.09 ng/ml

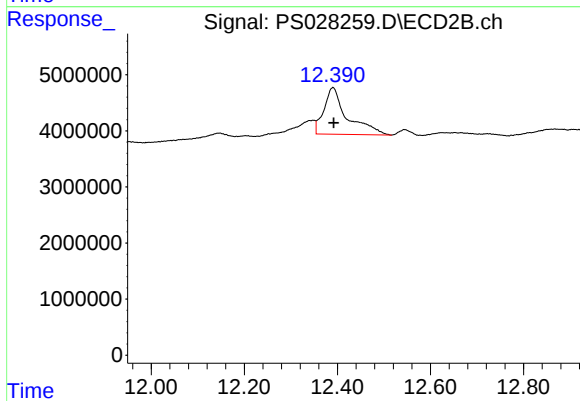

#15 Picloram

R.T.: 12.391 min
Delta R.T.: -0.002 min
Response: 28824710
Conc: 1.60 ng/ml