

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 22:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:54:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.260	7.763	1334.6E6	899.1E6	521.026	516.170
Target Compounds							
1) T	Dalapon	2.673	0.000	2113653	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.402f	0.000	1407942	0	<MDL	N.D. #
3) T	4-Nitroph...	7.047	7.260f	14507380	2282353	8.805	1.992 #
5) T	DICAMBA	0.000	7.956	0	3010866	N.D.	<MDL
6) T	MCP	7.687f	8.058	73702494	2079098	9.720	<MDL #
7) T	MCPA	0.000	8.280f	0	12780723	N.D.	1.533
8) T	DICHLORPROP	8.120f	0.000	2139650	0	<MDL	N.D. #
10) T	Pentachlo...	8.731f	0.000	9242142	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.940	0	13073297	N.D.	1.051
12) T	2,4,5-T	0.000	10.338	0	1542568	N.D.	<MDL
13) T	2,4-DB	10.103f	0.000	1847206	0	<MDL	N.D. #
15) T	Picloram	11.166	12.389	14316810	27060664	<MDL	1.501 #
16) T	DCPA	0.000	12.389f	0	27060664	N.D.	1.931



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 22:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:54:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

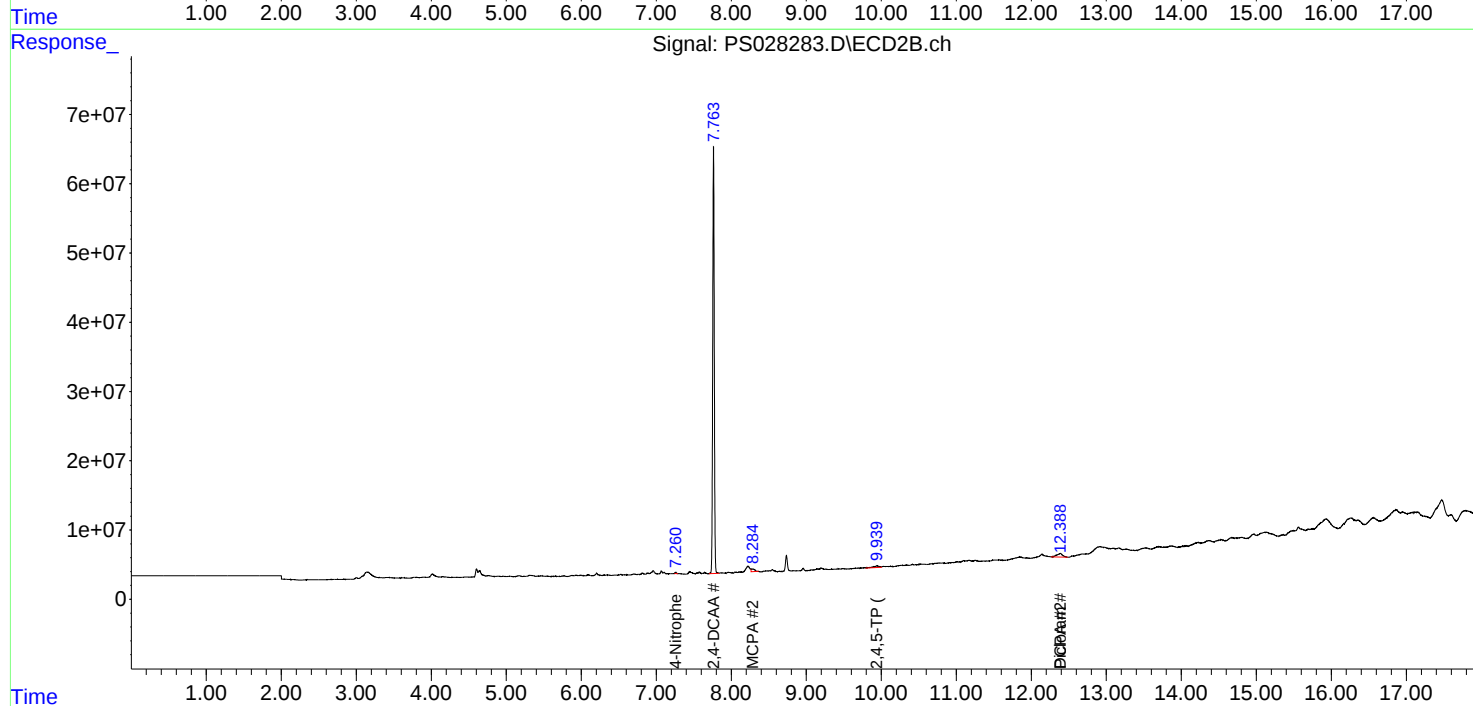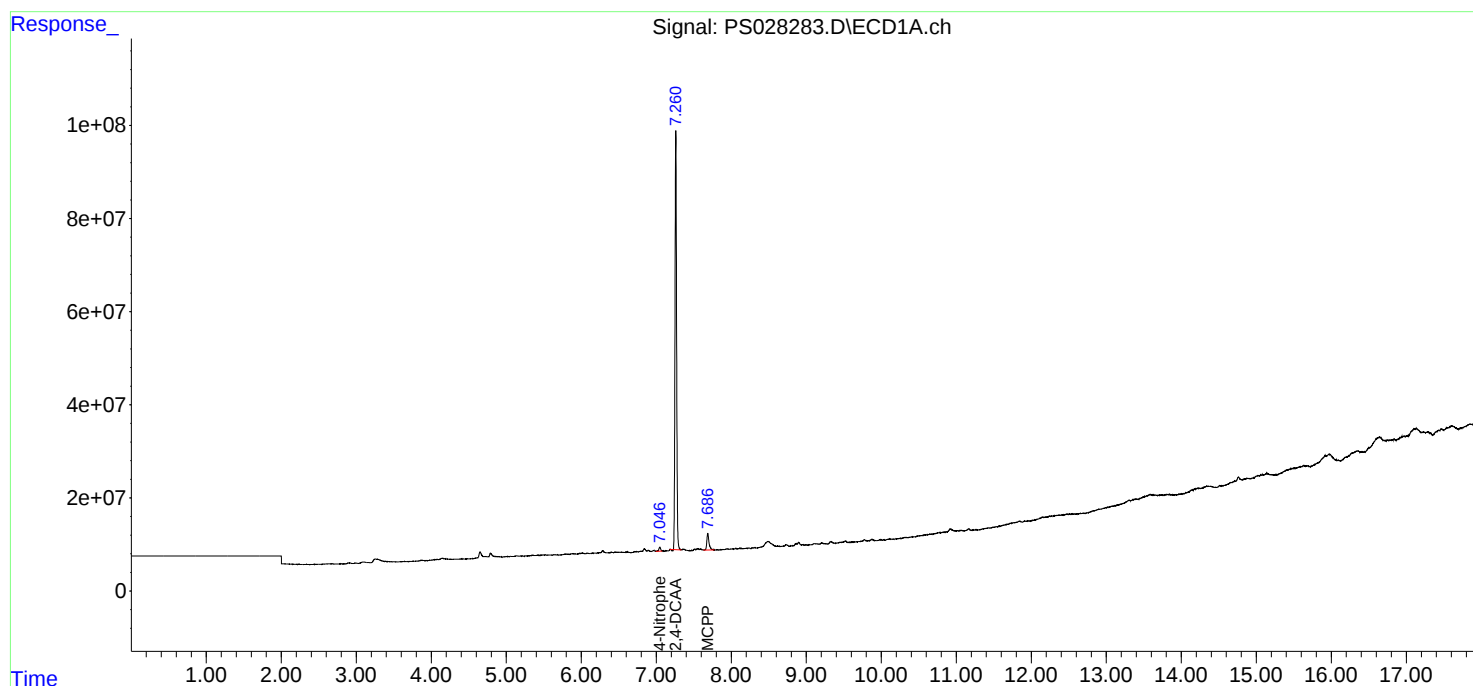


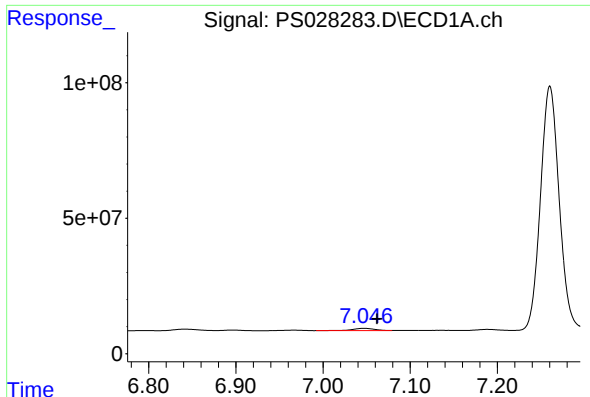

#3 4-Nitrophenol


R.T.: 7.047 min
Delta R.T.: -0.015 min
Response: 14507380
Conc: 8.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

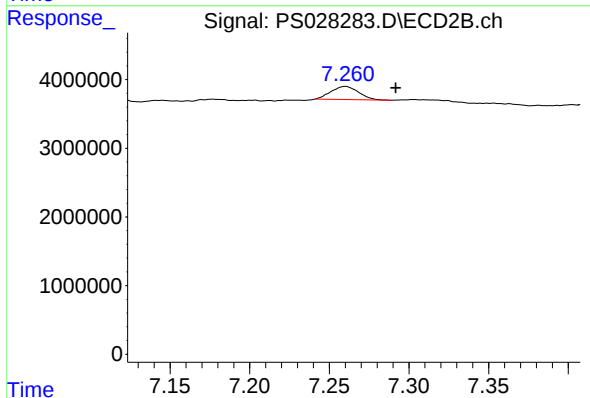


#3 4-Nitrophenol

R.T.: 7.260 min
Delta R.T.: -0.032 min
Response: 2282353
Conc: 1.99 ng/ml

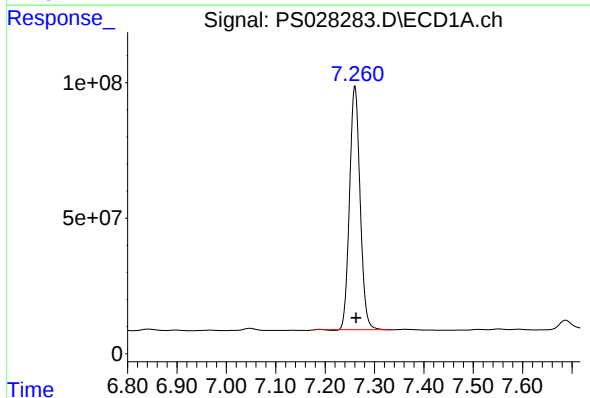


#4 2,4-DCAA

R.T.: 7.260 min
Delta R.T.: -0.002 min
Response: 1334563544
Conc: 521.03 ng/ml

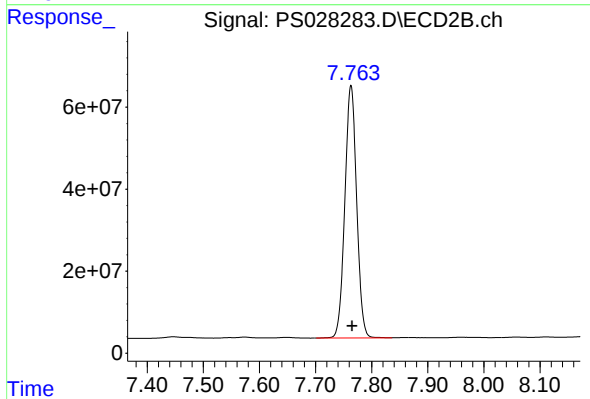

#4 2,4-DCAA


R.T.: 7.763 min
Delta R.T.: -0.002 min
Response: 899054821
Conc: 516.17 ng/ml

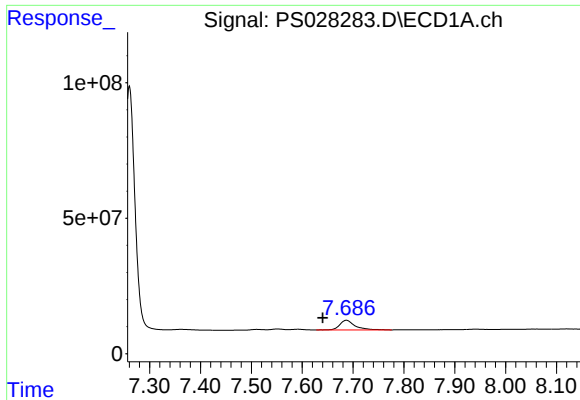

#6 MCPP


R.T.: 7.687 min
Delta R.T.: 0.046 min
Response: 73702494
Conc: 9.72 ug/ml

Instrument :
ECD_S
ClientSampleId :

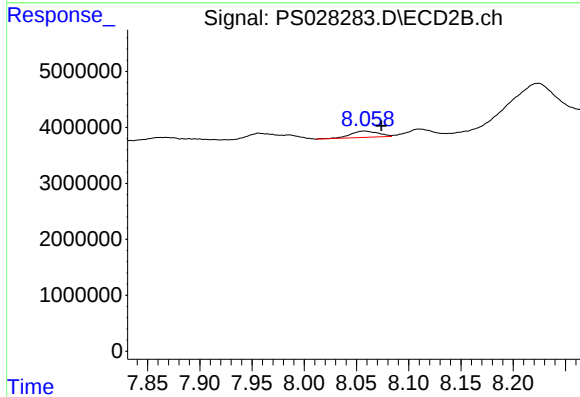


#6 MCPP

R.T.: 8.058 min
Delta R.T.: -0.016 min
Response: 2079098
Conc: N.D.

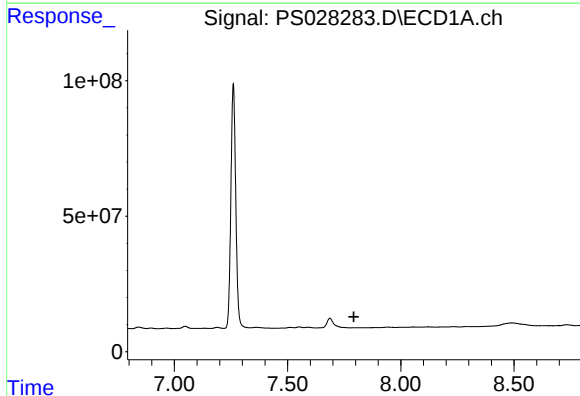


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

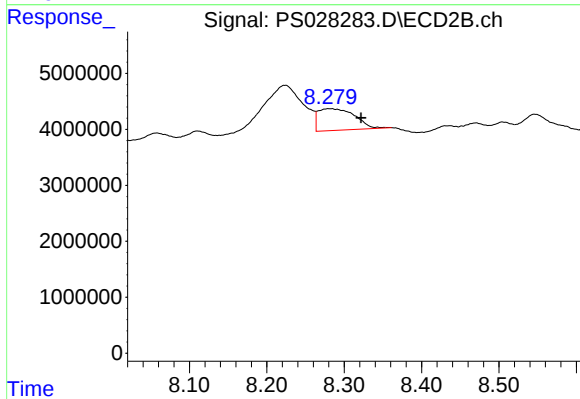

#7 MCPA


R.T.: 8.280 min
Delta R.T.: -0.042 min
Response: 12780723
Conc: 1.53 ug/ml

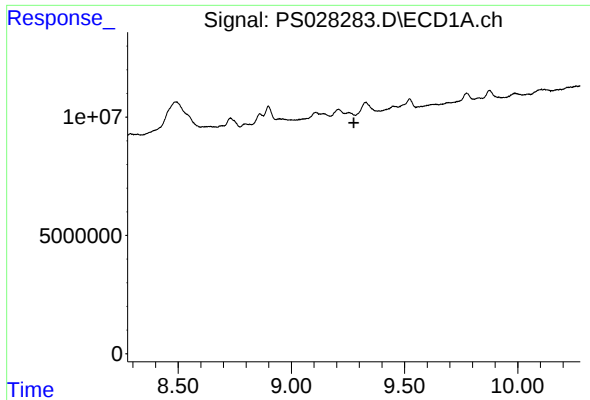

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

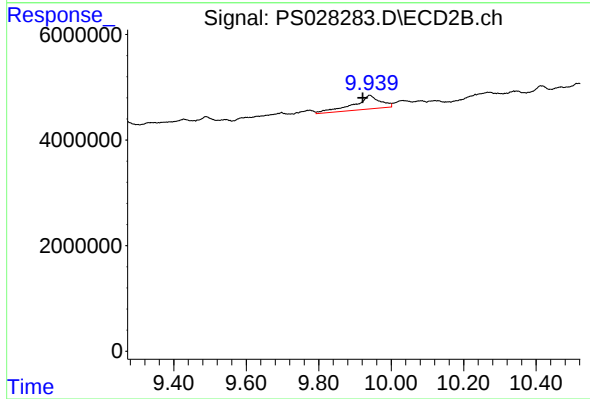


#11 2,4,5-TP (SILVEX)

R.T.: 9.940 min
Delta R.T.: 0.018 min
Response: 13073297
Conc: 1.05 ng/ml

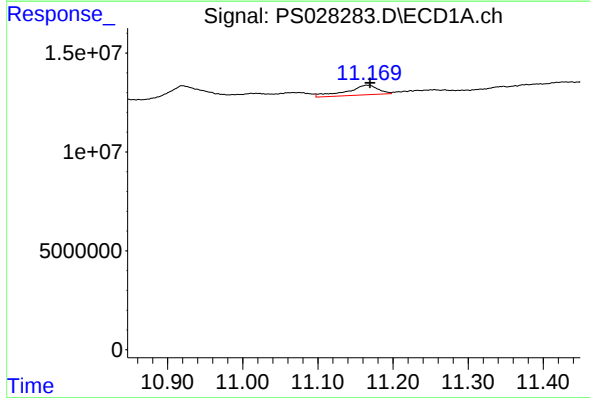


#15 Picloram

R.T.: 11.166 min
Delta R.T.: -0.003 min
Response: 14316810
Conc: N.D.

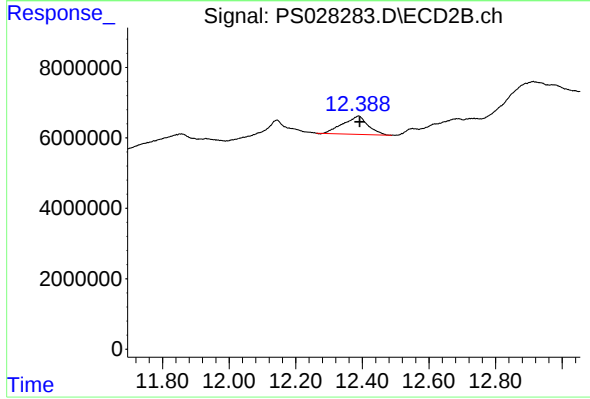

#15 Picloram


R.T.: 12.389 min
Delta R.T.: -0.004 min
Response: 27060664
Conc: 1.50 ng/ml

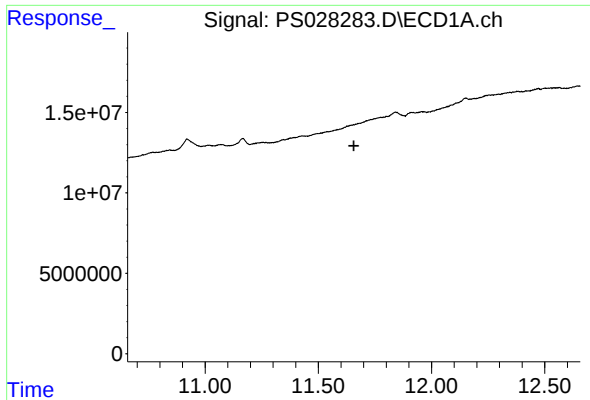

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.657 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

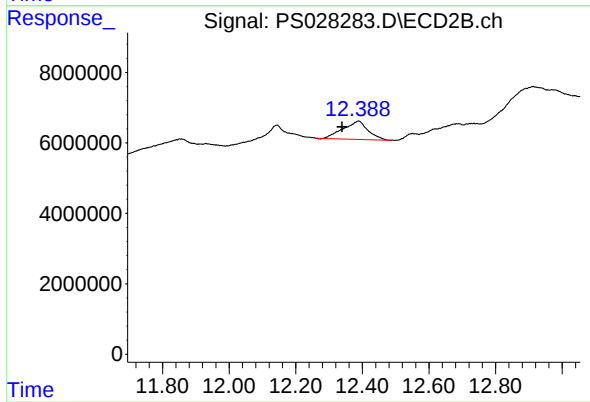

#16 DCPA

R.T.: 12.389 min
Delta R.T.: 0.049 min
Response: 27060664
Conc: 1.93 ng/ml