

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 09:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 10:27:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.257	7.760	1346.1E6	851.9E6	525.516	489.123
Target Compounds							
1) T	Dalapon	2.633	0.000	369480	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.406	0.000	228754	0	<MDL	N.D. #
3) T	4-Nitroph...	7.049	0.000	6034764	0	3.663	N.D. #
5) T	DICAMBA	0.000	7.959	0	2136392	N.D.	<MDL
6) T	MCPD	7.683f	8.112f	19640462	3834909	2.590	<MDL #
7) T	MCPA	0.000	8.283f	0	11872232	N.D.	1.424
8) T	DICHLORPROP	8.116f	8.731f	3946190	9808481	1.400	4.882 #
10) T	Pentachlo...	0.000	9.542	0	1678853	N.D.	<MDL
11) T	2,4,5-TP ...	9.300	9.940	153.3E6	8087345	9.006	<MDL #
13) T	2,4-DB	10.176f	0.000	1435617	0	<MDL	N.D. #
14) T	DINOSEB	11.393f	0.000	14804567	0	1.024	N.D. #
15) T	Picloram	11.168	12.391	15991655	27544817	<MDL	1.528 #
16) T	DCPA	11.641	0.000	3068872	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 09:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 10:27:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

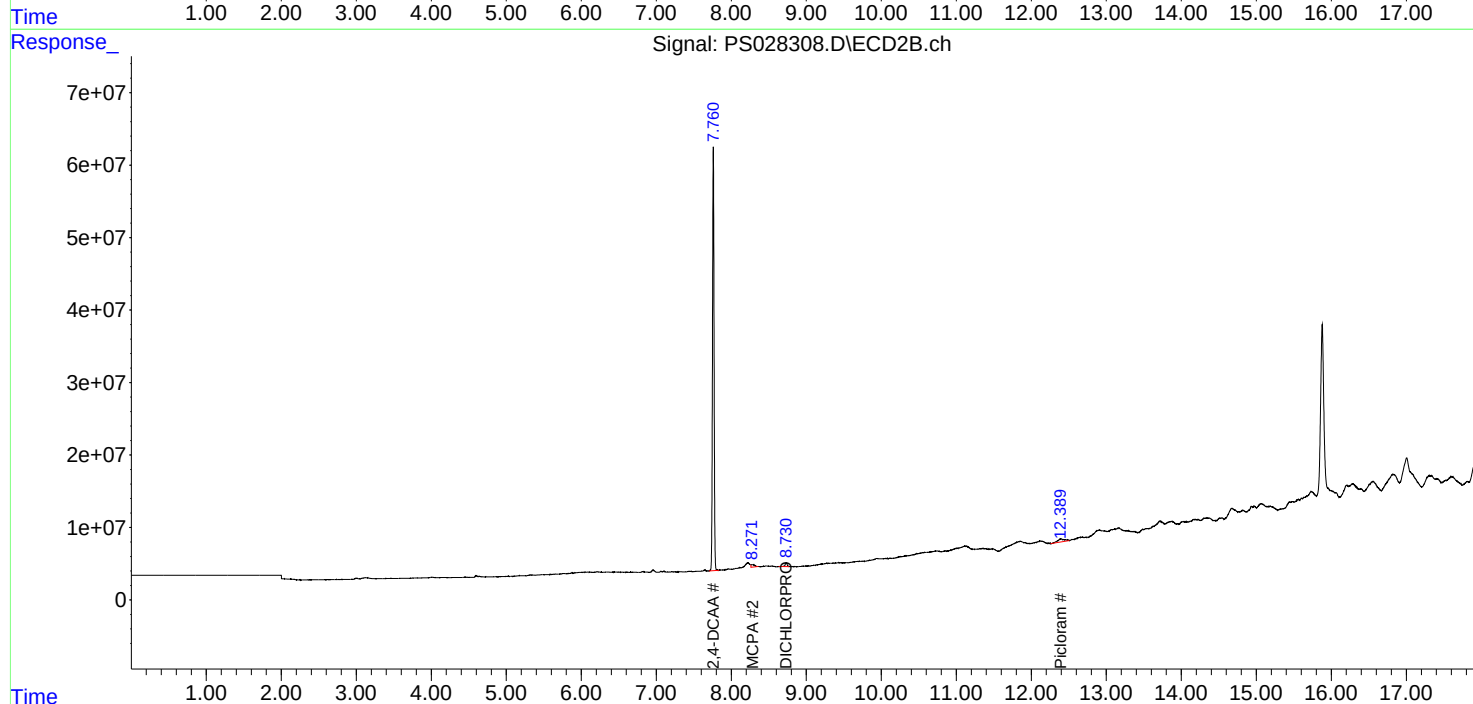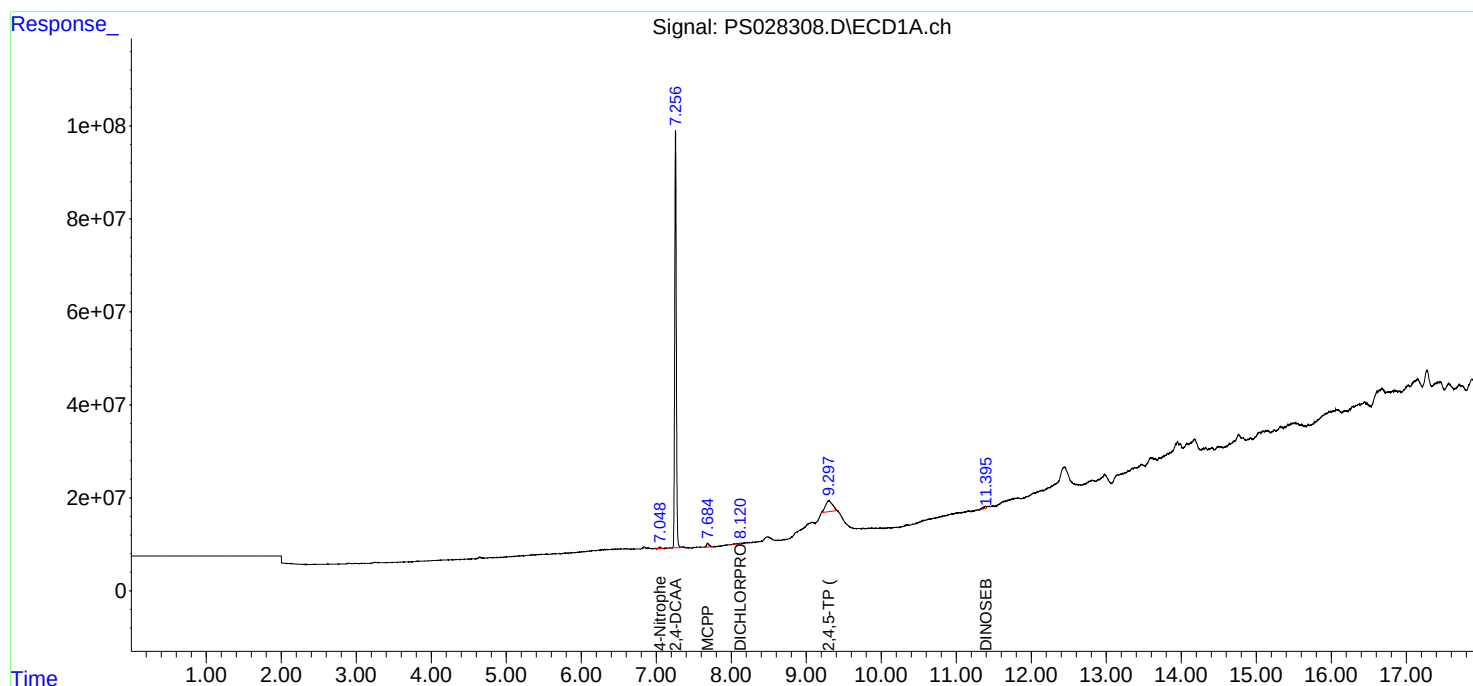


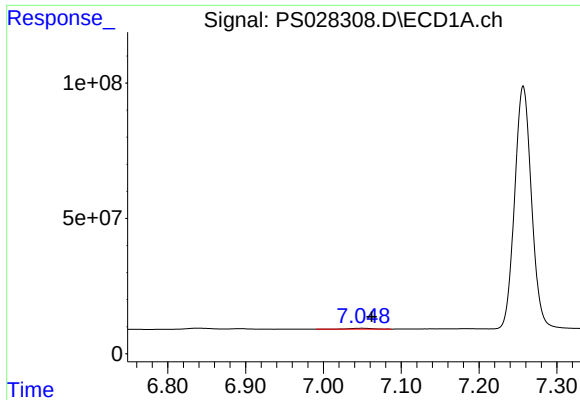

#3 4-Nitrophenol


R.T.: 7.049 min
Delta R.T.: -0.013 min
Response: 6034764
Conc: 3.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

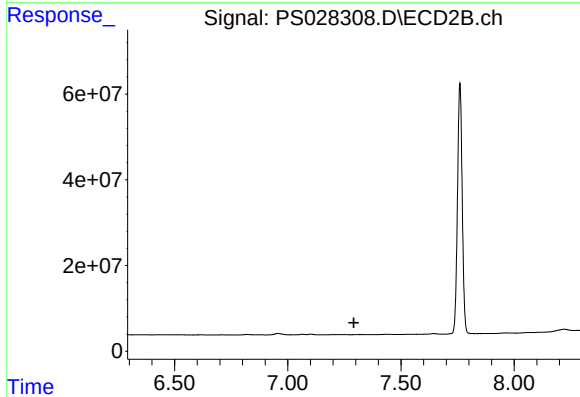


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

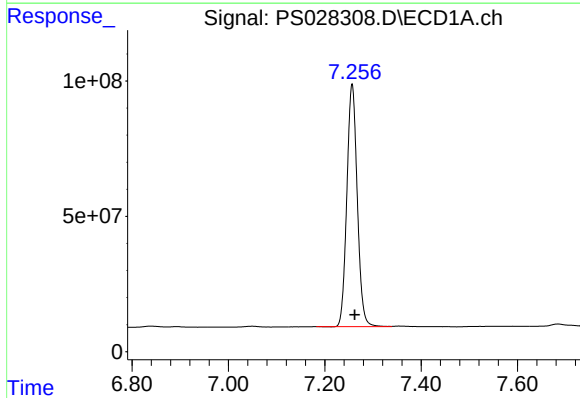


#4 2,4-DCAA

R.T.: 7.257 min
Delta R.T.: -0.006 min
Response: 1346064203
Conc: 525.52 ng/ml

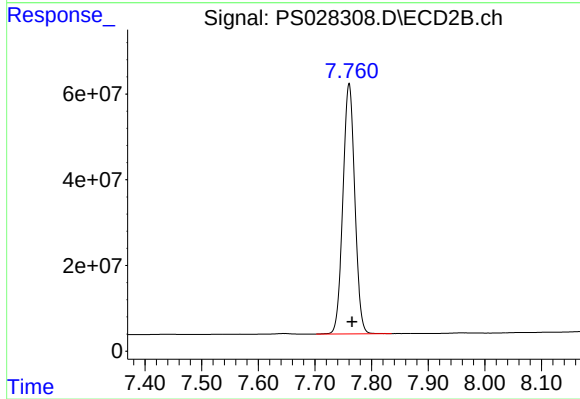

#4 2,4-DCAA


R.T.: 7.760 min
Delta R.T.: -0.005 min
Response: 851944014
Conc: 489.12 ng/ml

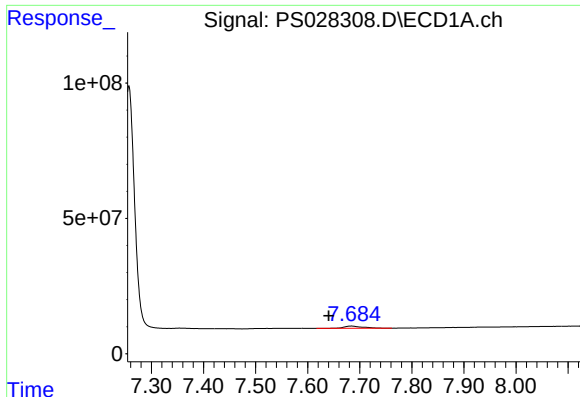

#6 MCPP


R.T.: 7.683 min
Delta R.T.: 0.043 min
Response: 19640462
Conc: 2.59 ug/ml

Instrument :
ECD_S
ClientSampleId :

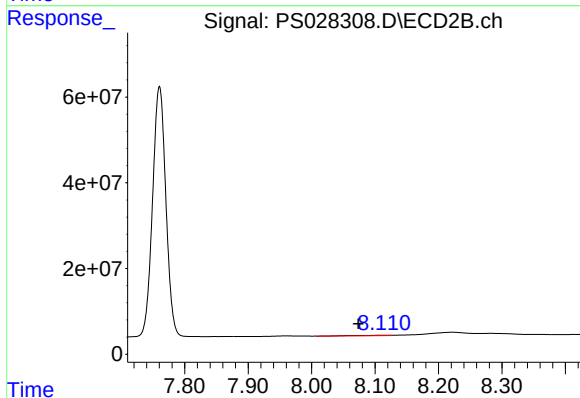


#6 MCPP

R.T.: 8.112 min
Delta R.T.: 0.038 min
Response: 3834909
Conc: N.D.

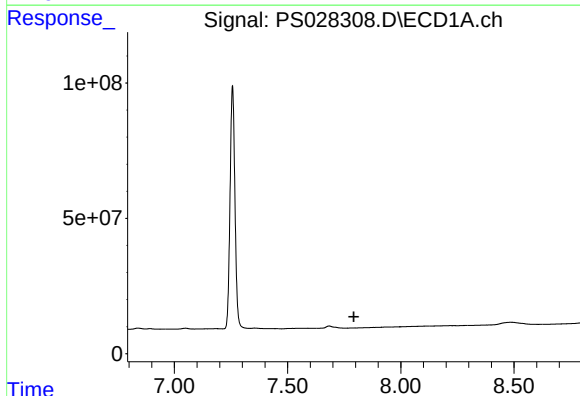


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

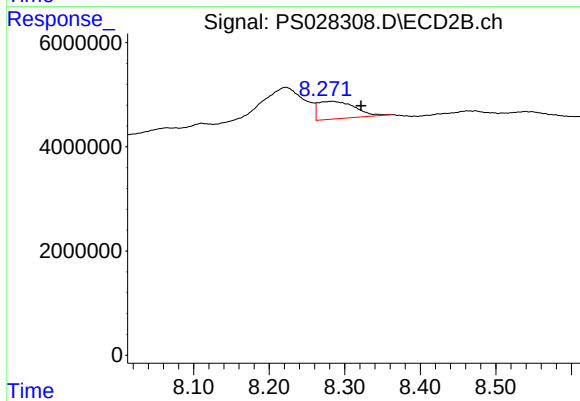

#7 MCPA


R.T.: 8.283 min
Delta R.T.: -0.039 min
Response: 11872232
Conc: 1.42 ug/ml

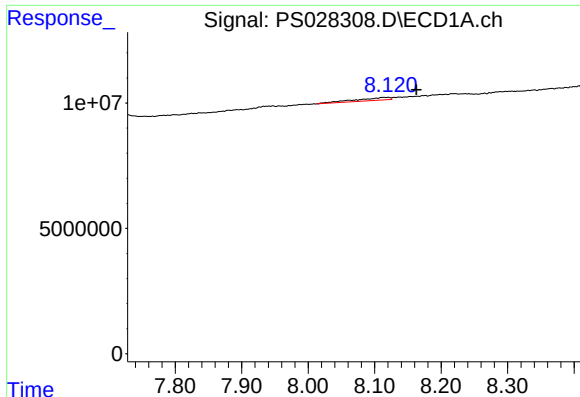

#8 DICHLORPROP


R.T.: 8.116 min
Delta R.T.: -0.047 min
Response: 3946190
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

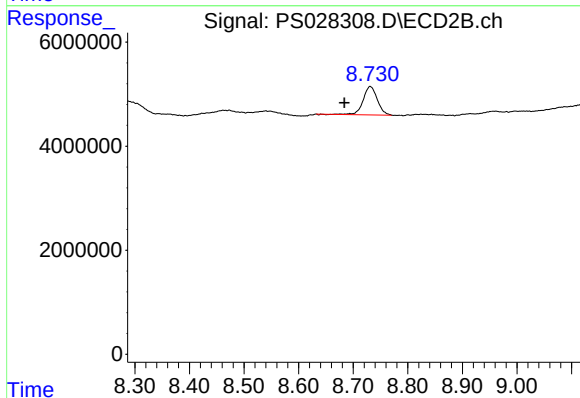


#8 DICHLORPROP

R.T.: 8.731 min
Delta R.T.: 0.047 min
Response: 9808481
Conc: 4.88 ng/ml

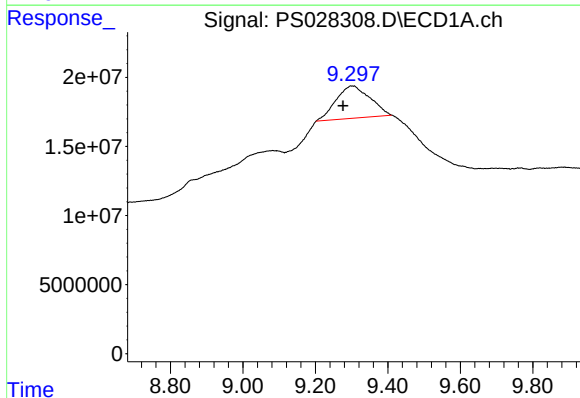


#11 2,4,5-TP (SILVEX)

R.T.: 9.300 min
Delta R.T.: 0.024 min
Response: 153332448
Conc: 9.01 ng/ml

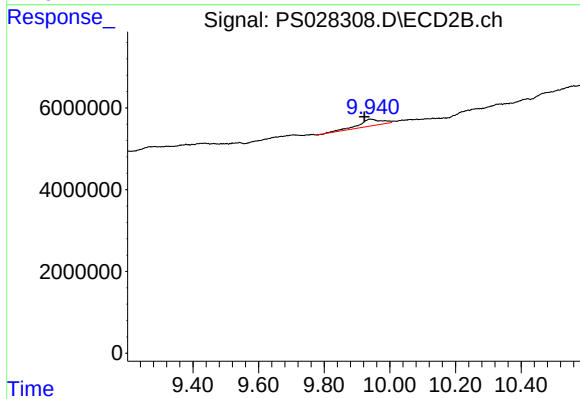

#11 2,4,5-TP (SILVEX)


R.T.: 9.940 min
Delta R.T.: 0.018 min
Response: 8087345
Conc: N.D.

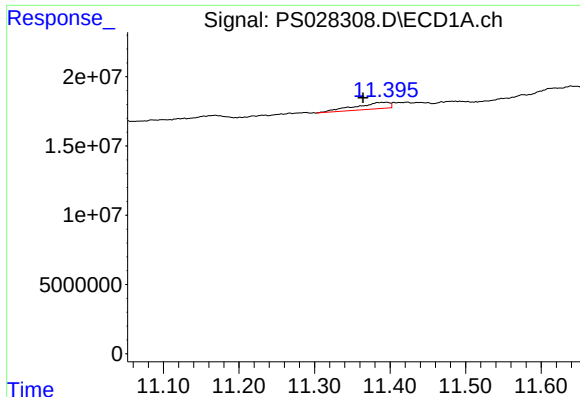

#14 DINOSEB


R.T.: 11.393 min
Delta R.T.: 0.029 min
Response: 14804567
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

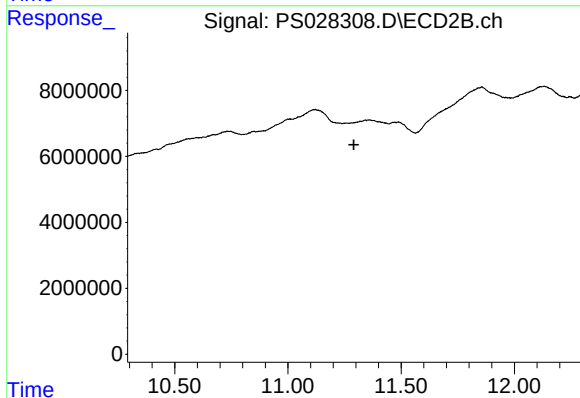


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.291 min
Response: 0
Conc: N.D.

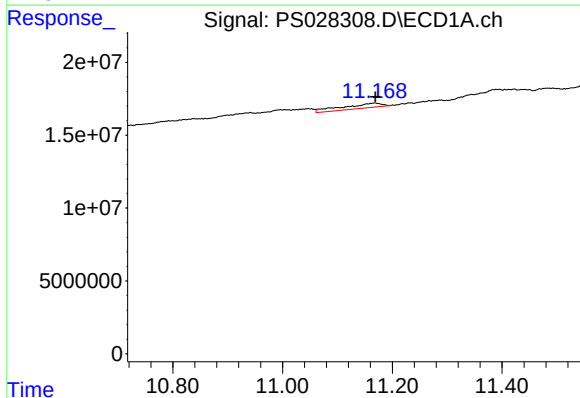

#15 Picloram

R.T.: 11.168 min
Delta R.T.: -0.002 min
Response: 15991655
Conc: N.D.

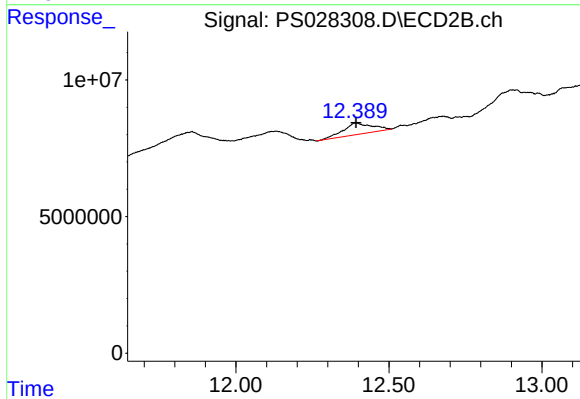

#15 Picloram

R.T.: 12.391 min
Delta R.T.: -0.001 min
Response: 27544817
Conc: 1.53 ng/ml