

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 13:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 03:14:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.255	7.760	1383.8E6	852.4E6	540.240	489.376
Target Compounds							
1) T	Dalapon	2.695f	0.000	2857842	0	<MDL	N.D. #
3) T	4-Nitroph...	7.048	0.000	5927185	0	3.598	N.D. #
6) T	MCP	7.682f	0.000	7336673	0	<MDL	N.D. #
7) T	MCPA	0.000	8.284f	0	12386210	N.D.	1.485
8) T	DICHLORPROP	8.188f	8.732f	366602	5186787	<MDL	2.581 #
10) T	Pentachlo...	8.691	0.000	323795	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.321f	9.945	987965	4882088	<MDL	<MDL #
12) T	2,4,5-T	9.560	10.336	1270553	2781434	<MDL	<MDL #
13) T	2,4-DB	10.162	0.000	388620	0	<MDL	N.D. #
14) T	DINOSEB	11.357	0.000	1412836	0	<MDL	N.D. #
15) T	Picloram	11.159	12.385	39712190	23916770	1.369	1.326
16) T	DCPA	11.638	12.385f	2099884	23916770	<MDL	1.707 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 13:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 03:14:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

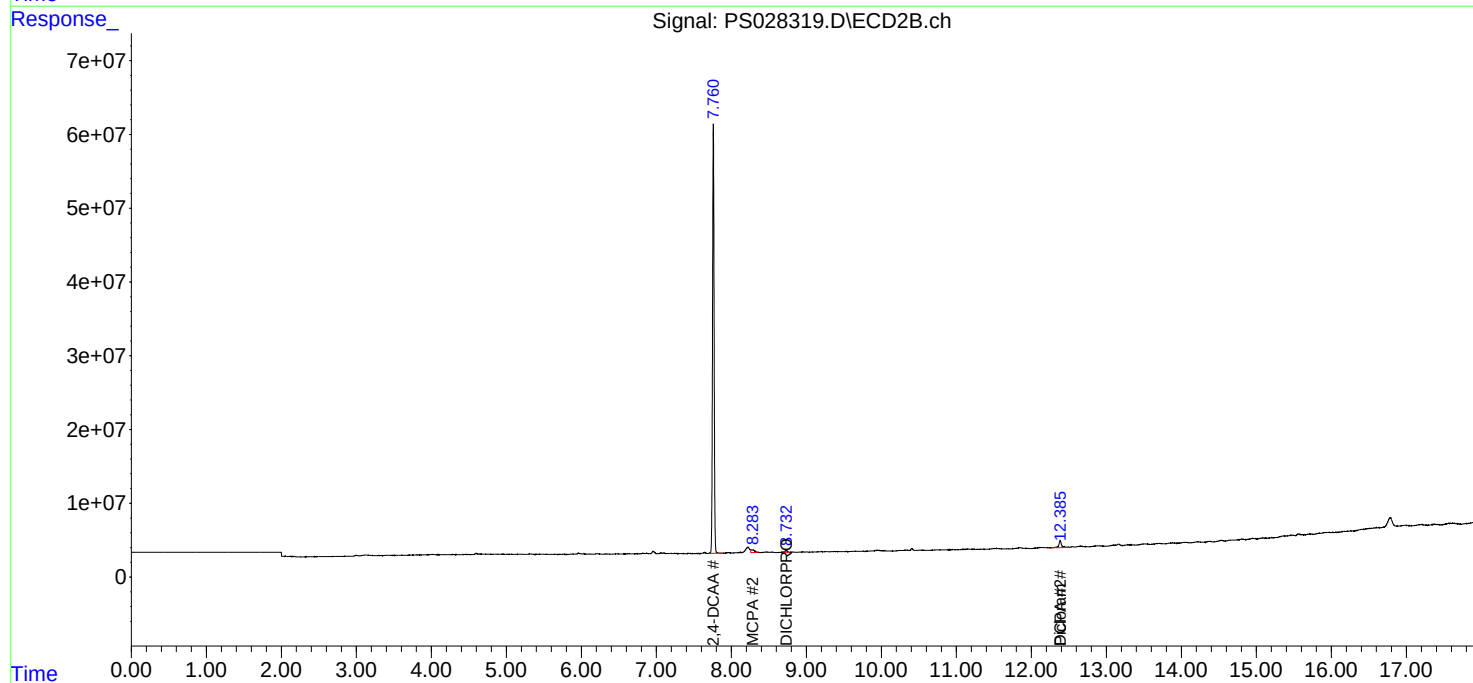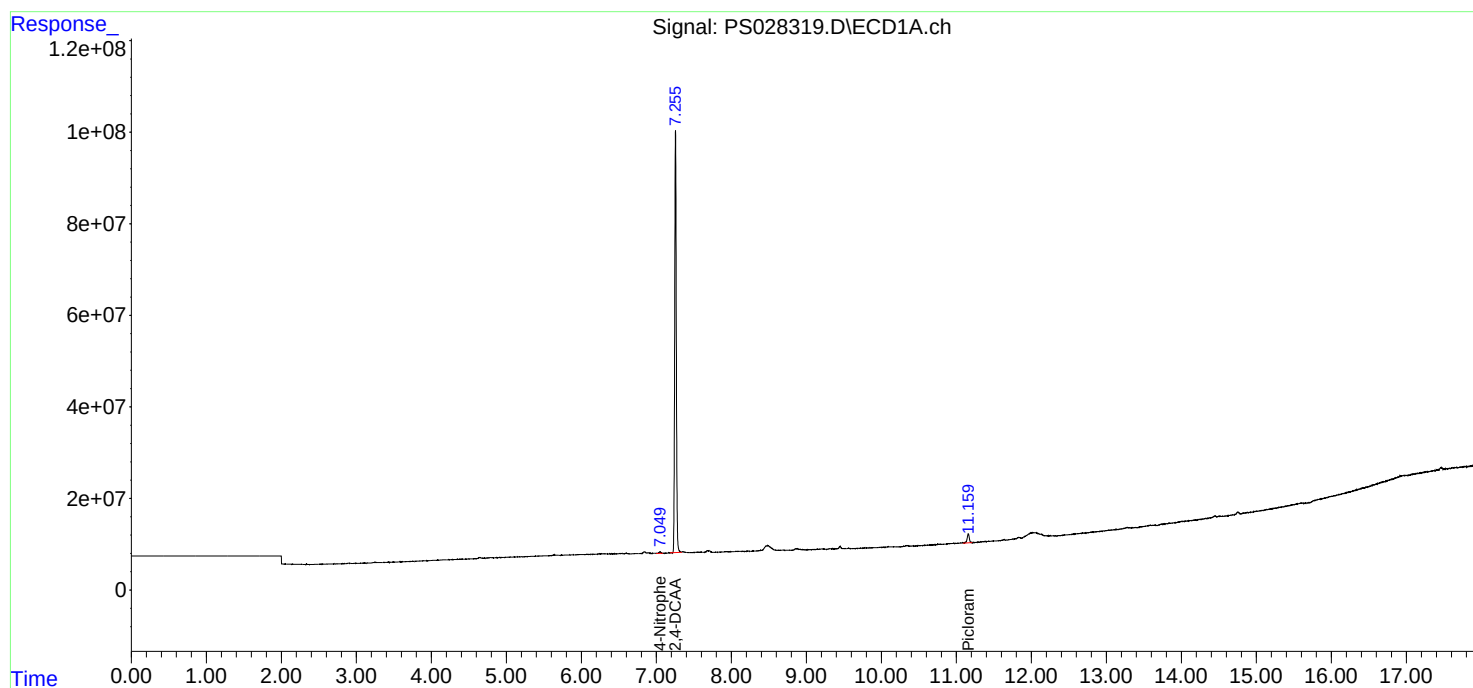


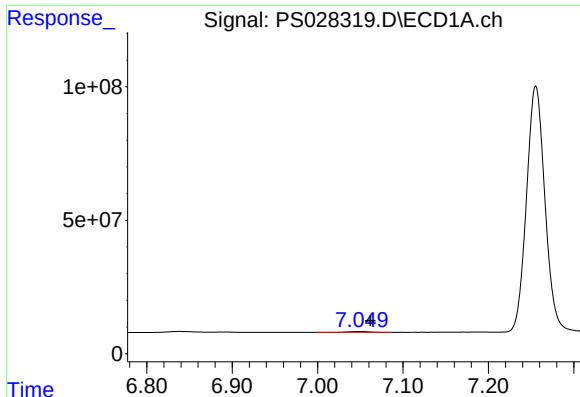

#3 4-Nitrophenol


R.T.: 7.048 min
Delta R.T.: -0.014 min
Response: 5927185
Conc: 3.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

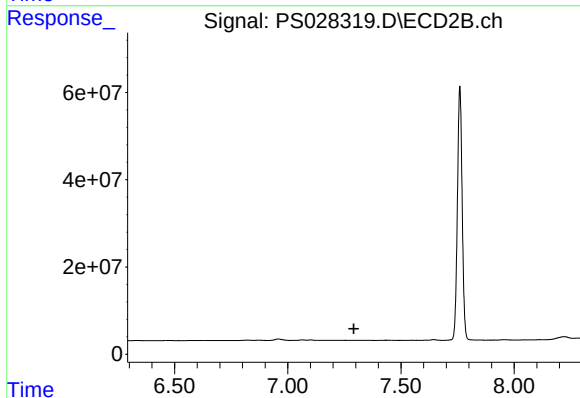


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

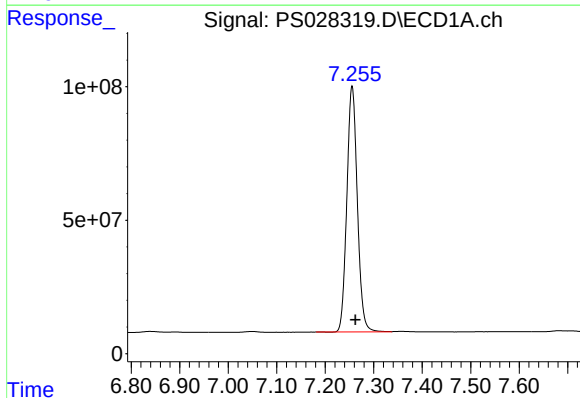


#4 2,4-DCAA

R.T.: 7.255 min
Delta R.T.: -0.007 min
Response: 1383778459
Conc: 540.24 ng/ml

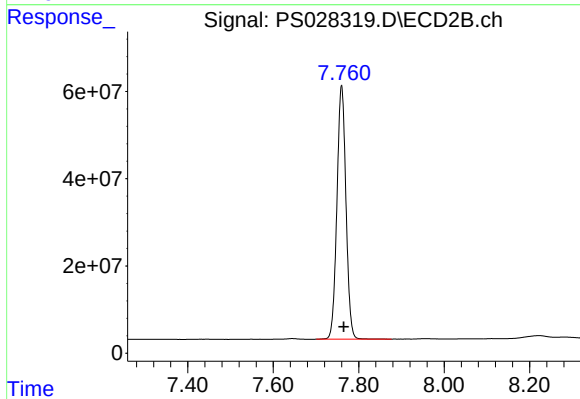

#4 2,4-DCAA


R.T.: 7.760 min
Delta R.T.: -0.005 min
Response: 852386161
Conc: 489.38 ng/ml

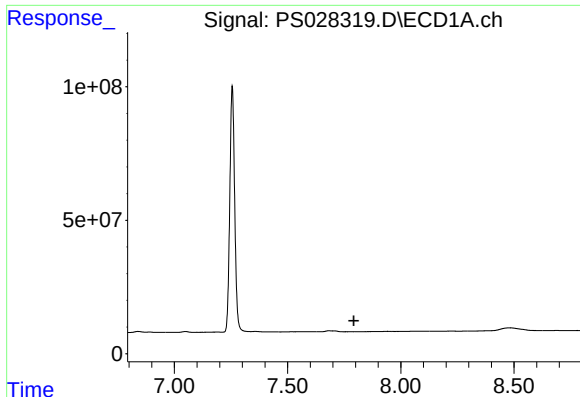

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

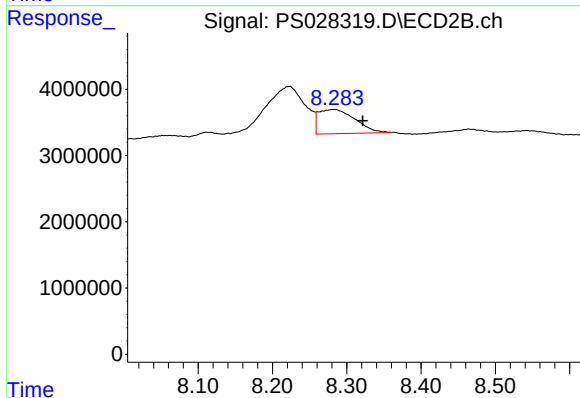


#7 MCPA

R.T.: 8.284 min
Delta R.T.: -0.038 min
Response: 12386210
Conc: 1.49 ug/ml

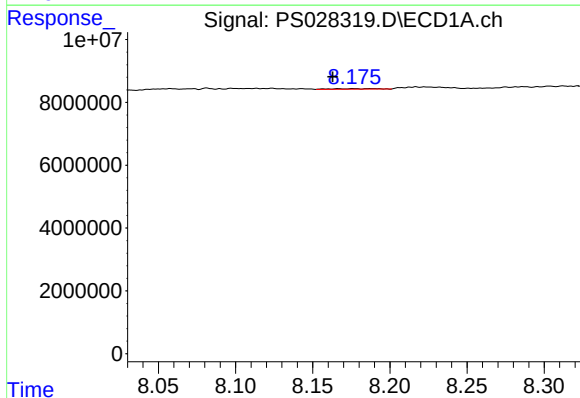


#8 DICHLORPROP

R.T.: 8.188 min
Delta R.T.: 0.025 min
Response: 366602
Conc: N.D.

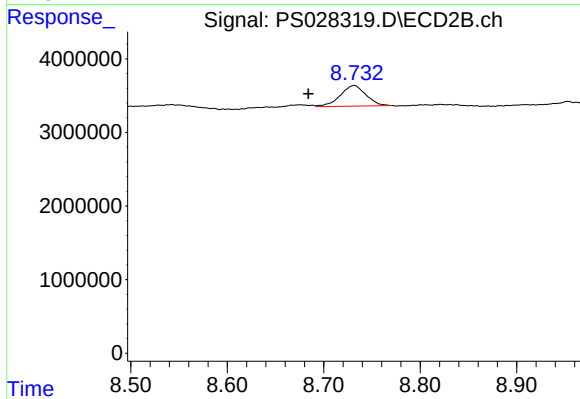

#8 DICHLORPROP


R.T.: 8.732 min
Delta R.T.: 0.048 min
Response: 5186787
Conc: 2.58 ng/ml

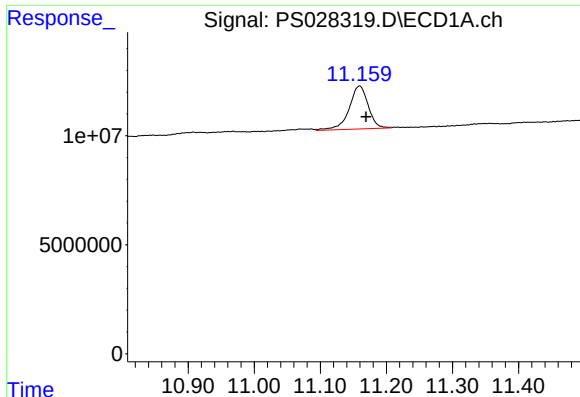

#15 Picloram


R.T.: 11.159 min
Delta R.T.: -0.010 min
Response: 39712190
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

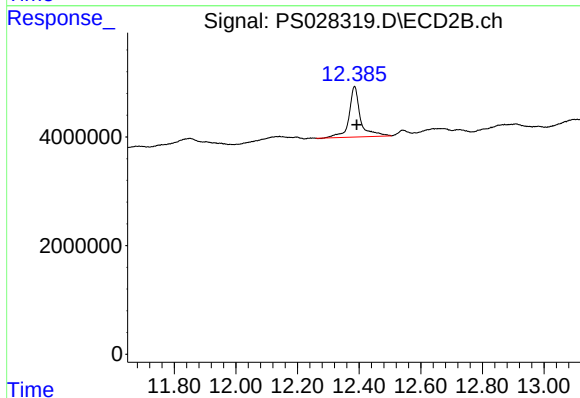


#15 Picloram

R.T.: 12.385 min
Delta R.T.: -0.007 min
Response: 23916770
Conc: 1.33 ng/ml

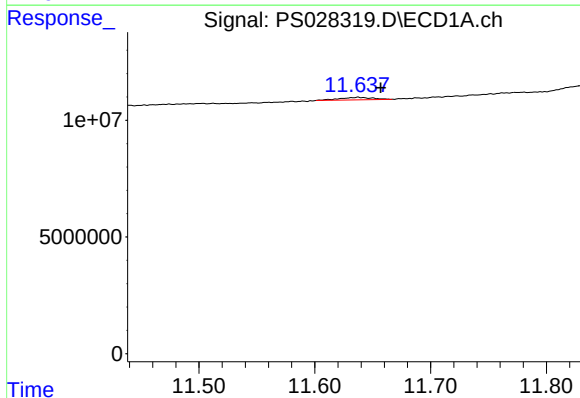

#16 DCPA

R.T.: 11.638 min
Delta R.T.: -0.019 min
Response: 2099884
Conc: N.D.

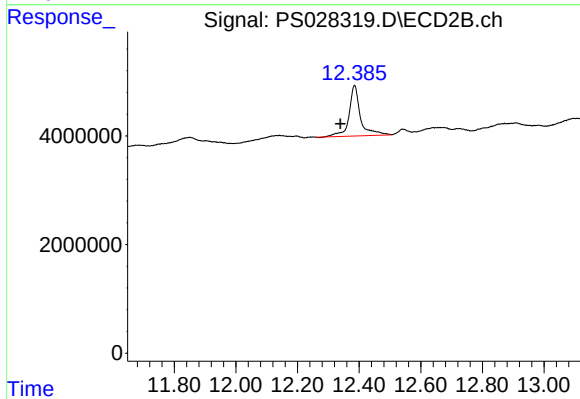

#16 DCPA

R.T.: 12.385 min
Delta R.T.: 0.046 min
Response: 23916770
Conc: 1.71 ng/ml