

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 18:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 03:26:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.254	7.758	1361.3E6	827.1E6	531.472	474.883
Target Compounds							
1) T	Dalapon	2.653	0.000	2830057	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.456f	0.000	2413799	0	<MDL	N.D. #
3) T	4-Nitroph...	7.042	0.000	10790466	0	6.549	N.D. #
5) T	DICAMBA	7.459	7.954	238047	2799023	<MDL	<MDL #
6) T	MCPD	7.681f	8.056	70269128	1470201	9.267	<MDL #
7) T	MCPA	0.000	8.287f	0	11300021	N.D.	1.355
8) T	DICHLORPROP	0.000	8.730f	0	33990071	N.D.	16.917
10) T	Pentachlo...	8.724f	9.544	5984838	3597025	<MDL	<MDL #
11) T	2,4,5-TP ...	9.276	9.938	8072914	29207547	<MDL	2.347 #
12) T	2,4,5-T	9.568	10.337	2566001	12906936	<MDL	1.052 #
13) T	2,4-DB	10.153	0.000	279495	0	<MDL	N.D. #
14) T	DINOSEB	11.382	0.000	6826116	0	<MDL	N.D. #
15) T	Picloram	11.153	12.384	33560274	37270314	1.157	2.067 #
16) T	DCPA	11.637	12.384f	4080365	37270314	<MDL	2.660 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 18:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 03:26:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

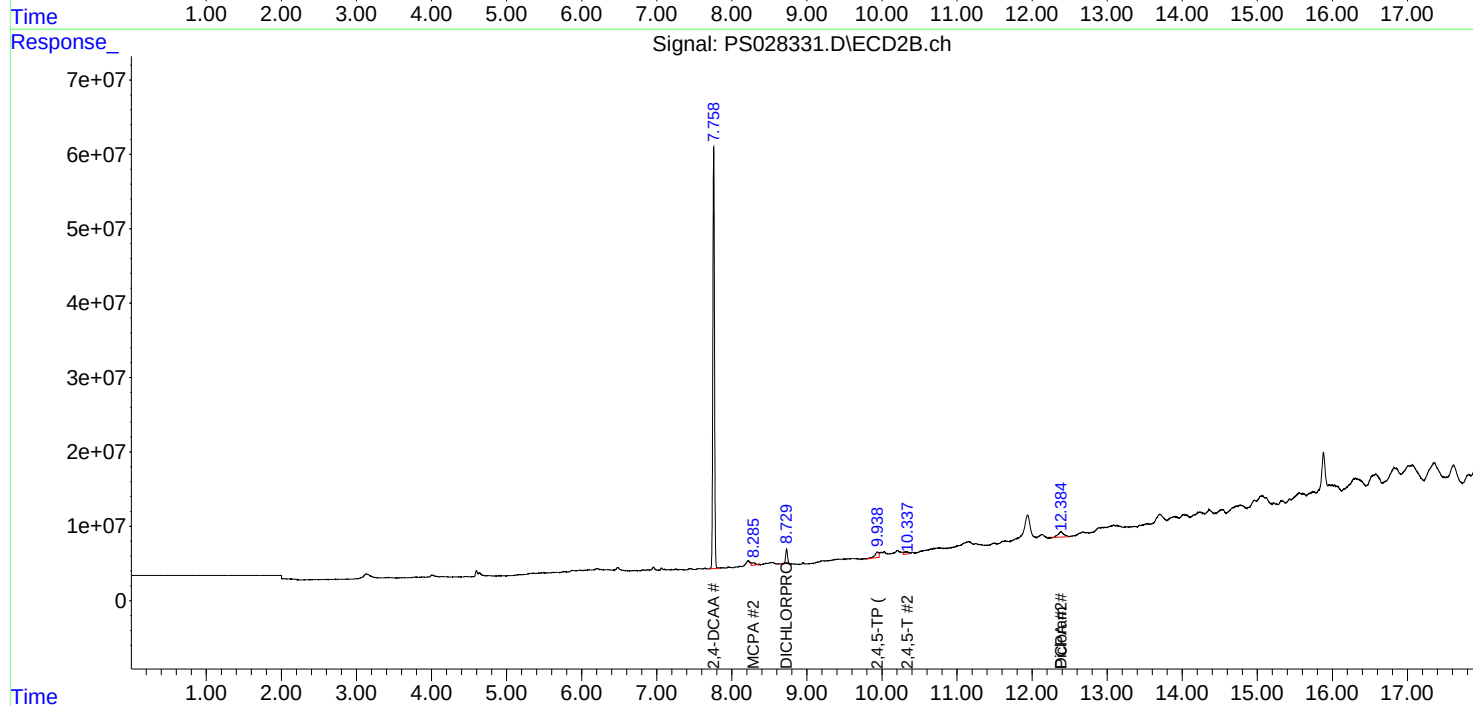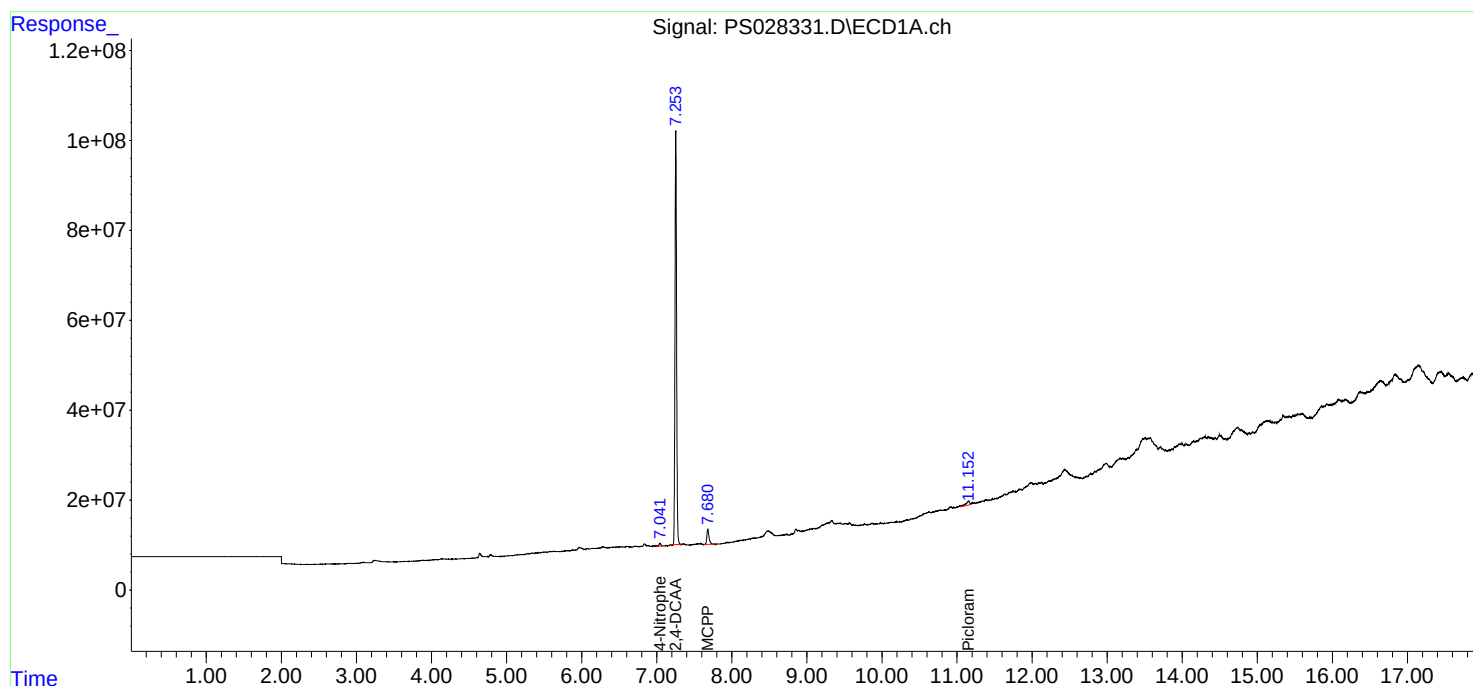


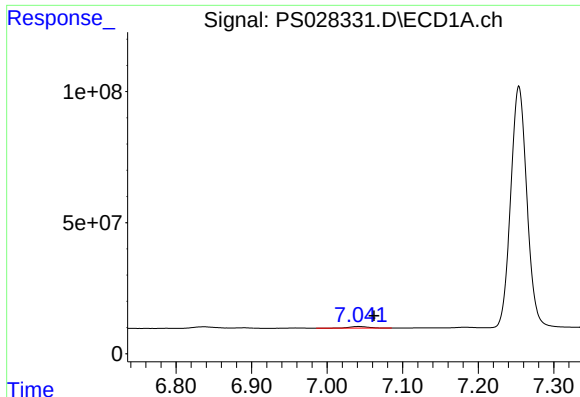

#3 4-Nitrophenol


R.T.: 7.042 min
Delta R.T.: -0.021 min
Response: 10790466
Conc: 6.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

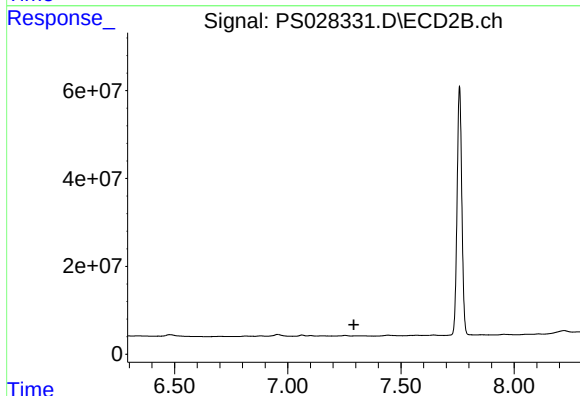


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

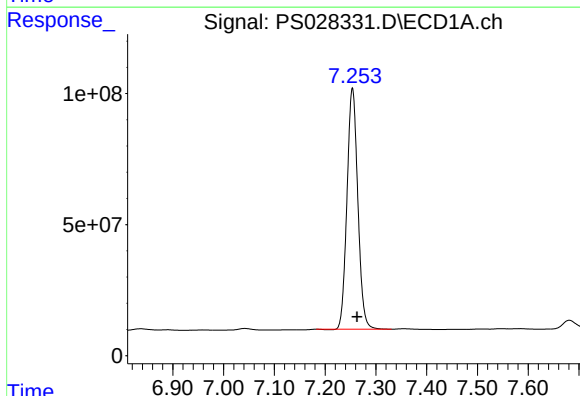


#4 2,4-DCAA

R.T.: 7.254 min
Delta R.T.: -0.009 min
Response: 1361319286
Conc: 531.47 ng/ml

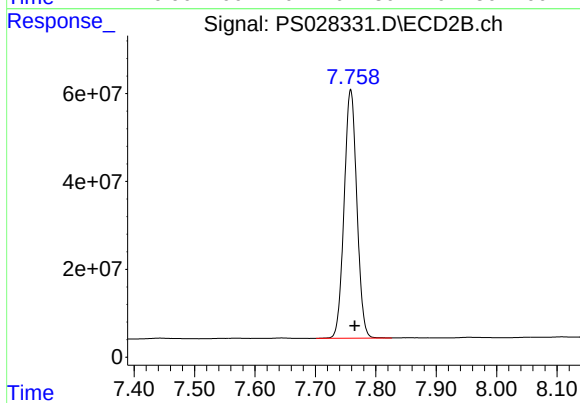

#4 2,4-DCAA


R.T.: 7.758 min
Delta R.T.: -0.007 min
Response: 827141208
Conc: 474.88 ng/ml

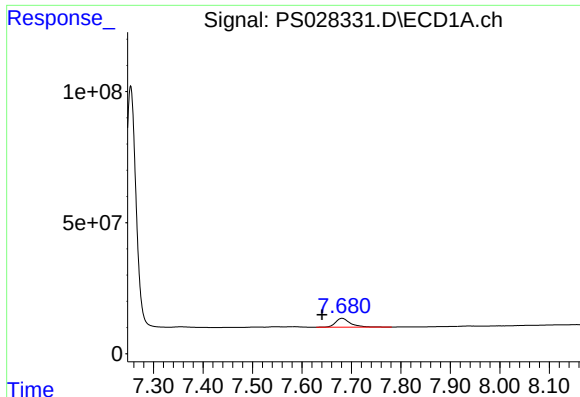

#6 MCPP


R.T.: 7.681 min
Delta R.T.: 0.040 min
Response: 70269128
Conc: 9.27 ug/ml

Instrument :
ECD_S
ClientSampleId :

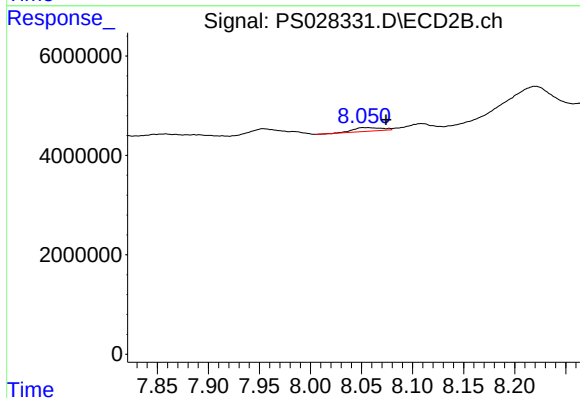


#6 MCPP

R.T.: 8.056 min
Delta R.T.: -0.018 min
Response: 1470201
Conc: N.D.

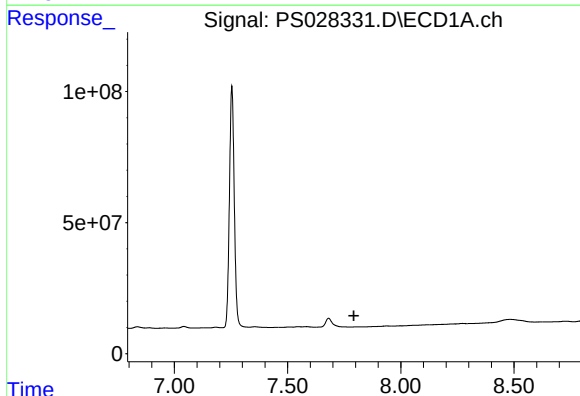


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

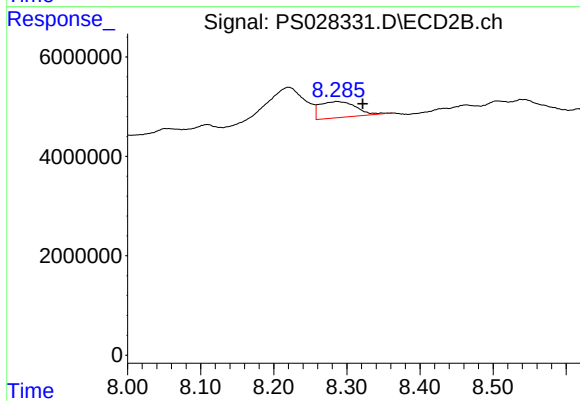

#7 MCPA


R.T.: 8.287 min
Delta R.T.: -0.035 min
Response: 11300021
Conc: 1.36 ug/ml

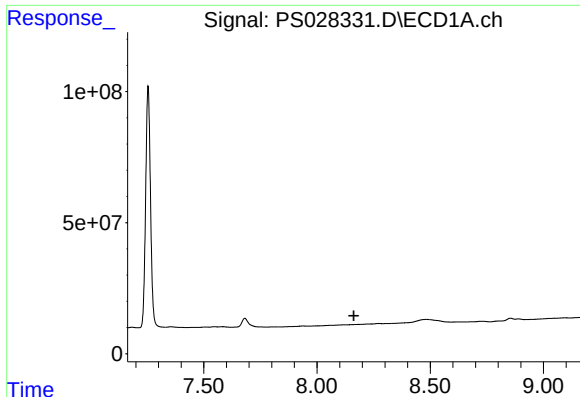

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

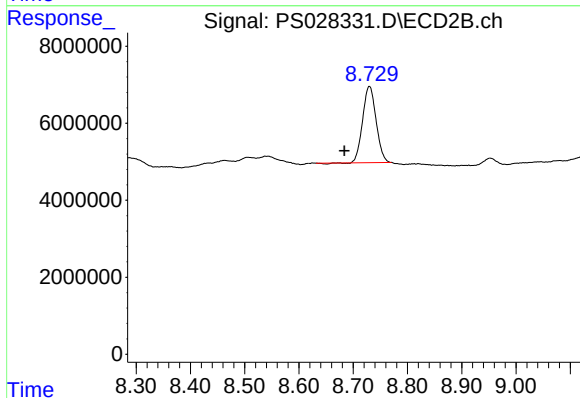


#8 DICHLORPROP

R.T.: 8.730 min
Delta R.T.: 0.046 min
Response: 33990071
Conc: 16.92 ng/ml

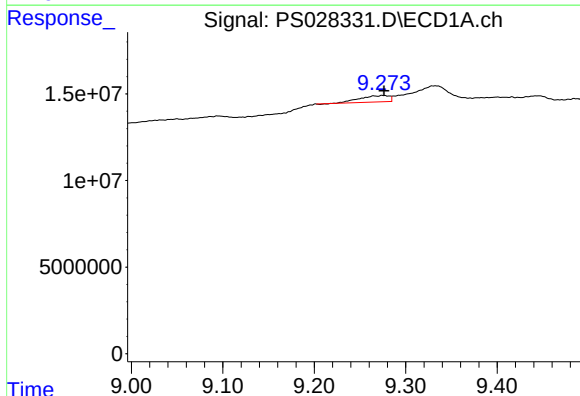


#11 2,4,5-TP (SILVEX)

R.T.: 9.276 min
Delta R.T.: 0.000 min
Response: 8072914
Conc: N.D.

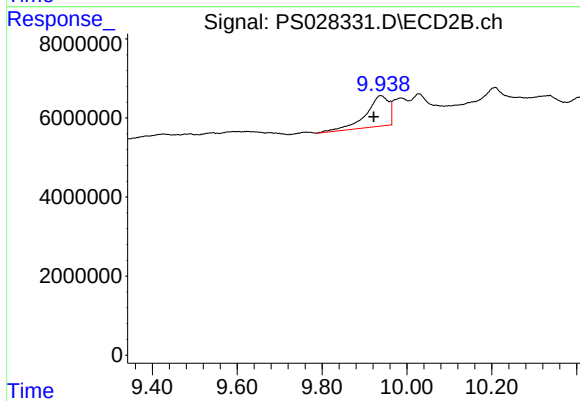

#11 2,4,5-TP (SILVEX)


R.T.: 9.938 min
Delta R.T.: 0.016 min
Response: 29207547
Conc: 2.35 ng/ml

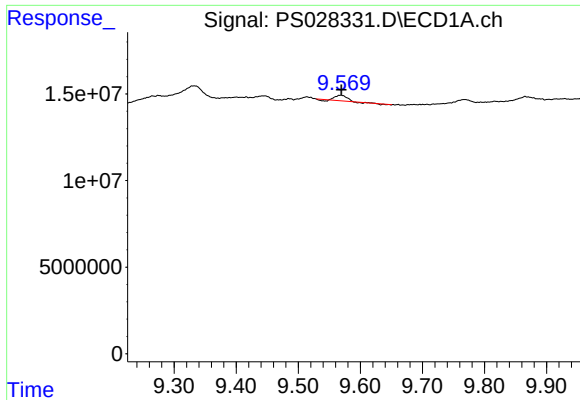

#12 2,4,5-T


R.T.: 9.568 min
Delta R.T.: -0.001 min
Response: 2566001
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

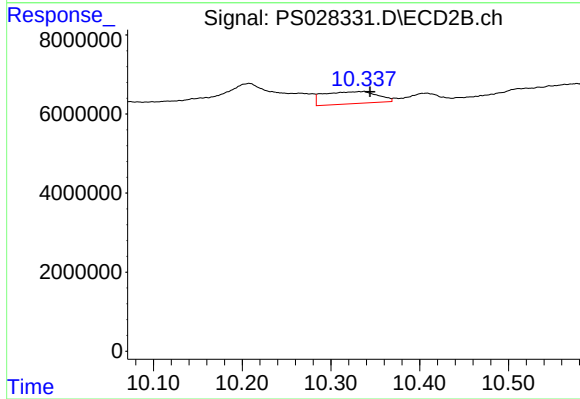


#12 2,4,5-T

R.T.: 10.337 min
Delta R.T.: -0.007 min
Response: 12906936
Conc: 1.05 ng/ml

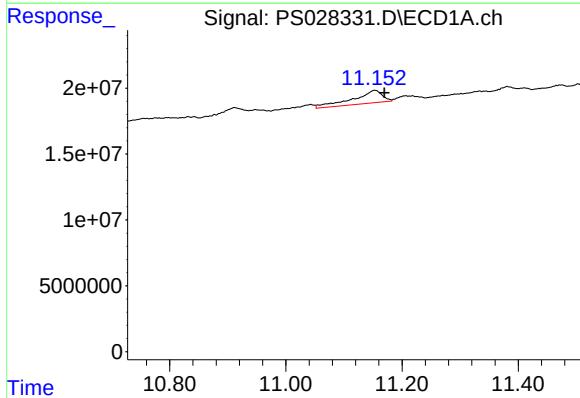


#15 Picloram

R.T.: 11.153 min
Delta R.T.: -0.016 min
Response: 33560274
Conc: 1.16 ng/ml

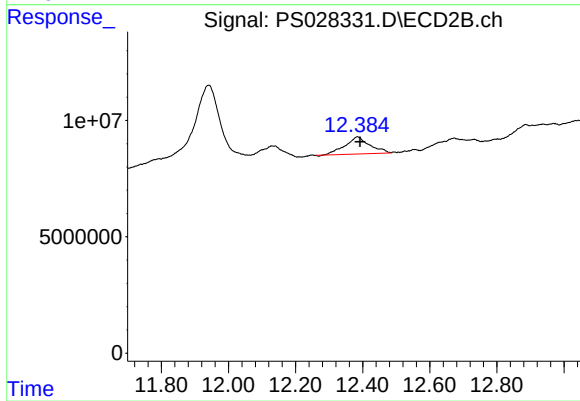

#15 Picloram


R.T.: 12.384 min
Delta R.T.: -0.008 min
Response: 37270314
Conc: 2.07 ng/ml

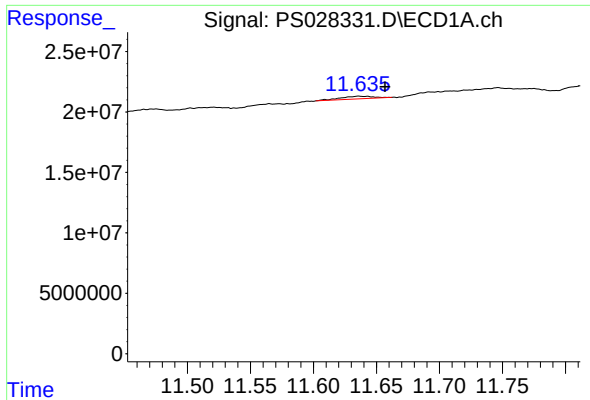

#16 DCPA

R.T.: 11.637 min
Delta R.T.: -0.019 min
Response: 4080365
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

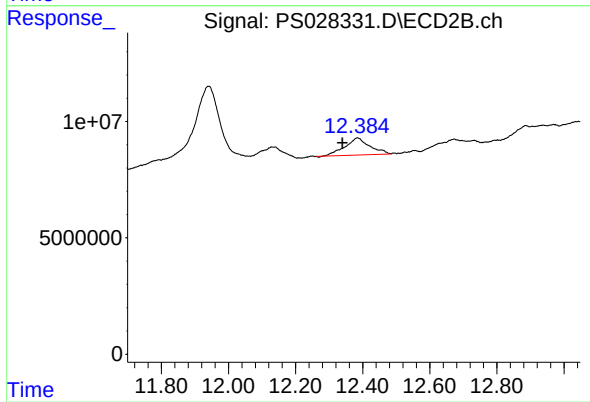

#16 DCPA

R.T.: 12.384 min
Delta R.T.: 0.045 min
Response: 37270314
Conc: 2.66 ng/ml