

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 14:40
 Operator : AR\AJ
 Sample : P4601-29
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CC0Q1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/08/2024
 Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 03:14:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.255	7.760	688.5E6	364.2E6	268.803m	209.074m
Target Compounds						
6) T MCPP	7.622	8.052	56286561	59130123	7.423m	9.739m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 14:40
Operator : AR\AJ
Sample : P4601-29
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CC0Q1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/08/2024
Supervised By : Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 03:14:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

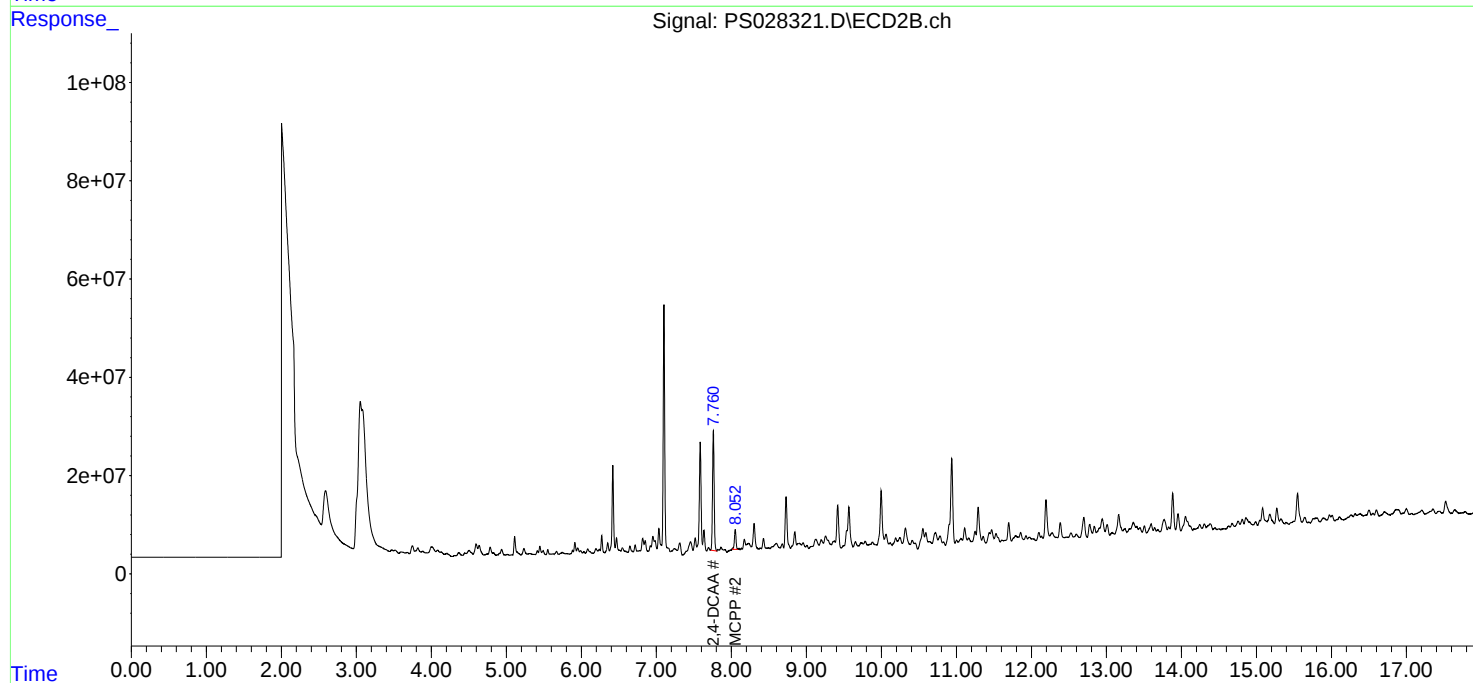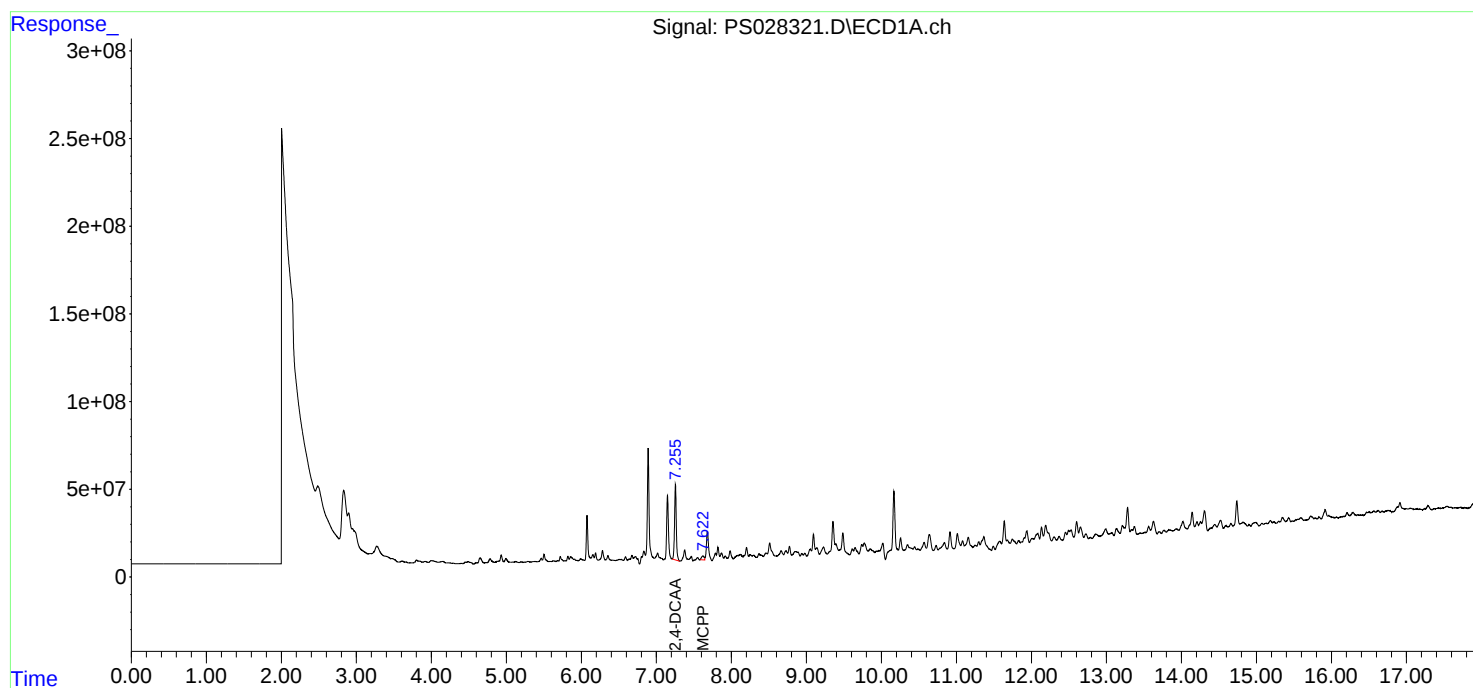

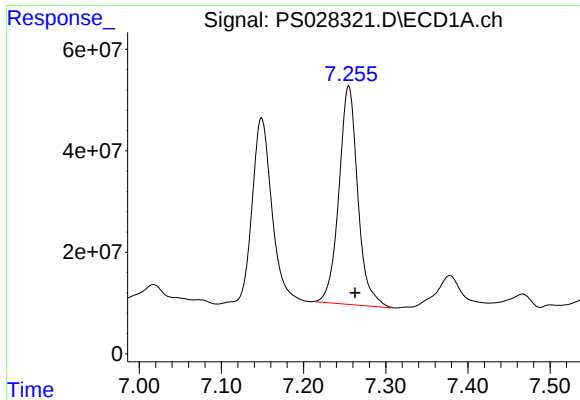


#4 2,4-DCAA

R.T.: 7.255 min
Delta R.T.: -0.008 min
Response: 688515925
Conc: 268.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
CC0Q1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

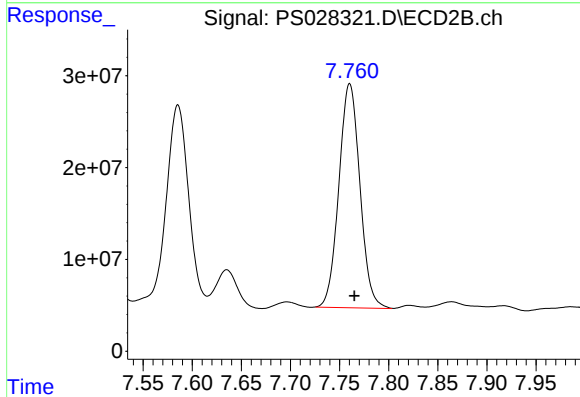


#4 2,4-DCAA

R.T.: 7.760 min
Delta R.T.: -0.005 min
Response: 364160902
Conc: 209.07 ng/ml m

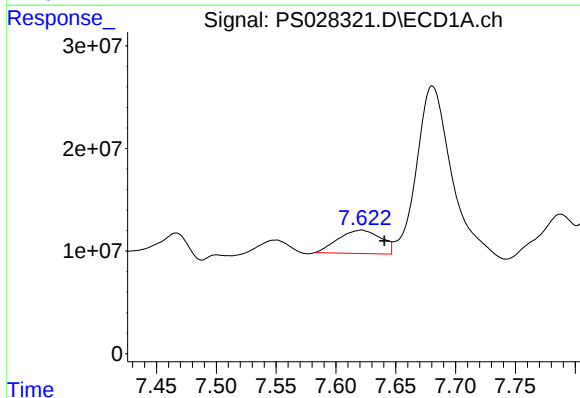

#6 MCP

R.T.: 7.622 min
Delta R.T.: -0.019 min
Response: 56286561
Conc: 7.42 ug/ml m

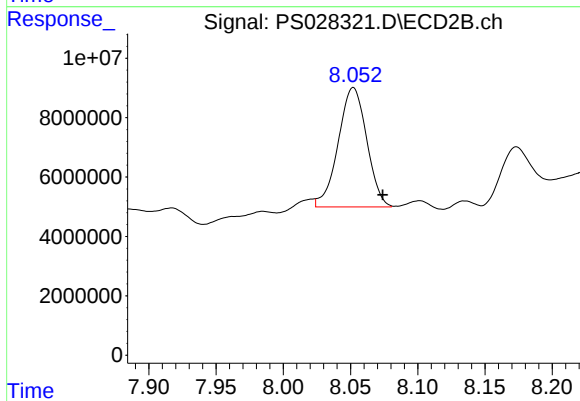

#6 MCP

R.T.: 8.052 min
Delta R.T.: -0.022 min
Response: 59130123
Conc: 9.74 ug/ml m