

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
 Data File : PS028328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 17:29
 Operator : AR\AJ
 Sample : P4601-36
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CC0R7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/08/2024
 Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 03:22:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 11:48:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.254	7.760	1194.3E6	674.1E6	466.278	386.996m
Target Compounds						
6) T MCPP	7.619	8.052	27372444	26479777	3.610m	4.361
7) T MCPA	7.788	8.304	50382479	127.0E6	4.839m	15.234 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110624\
Data File : PS028328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 17:29
Operator : AR\AJ
Sample : P4601-36
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CC0R7


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 03:22:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110624.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 11:48:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

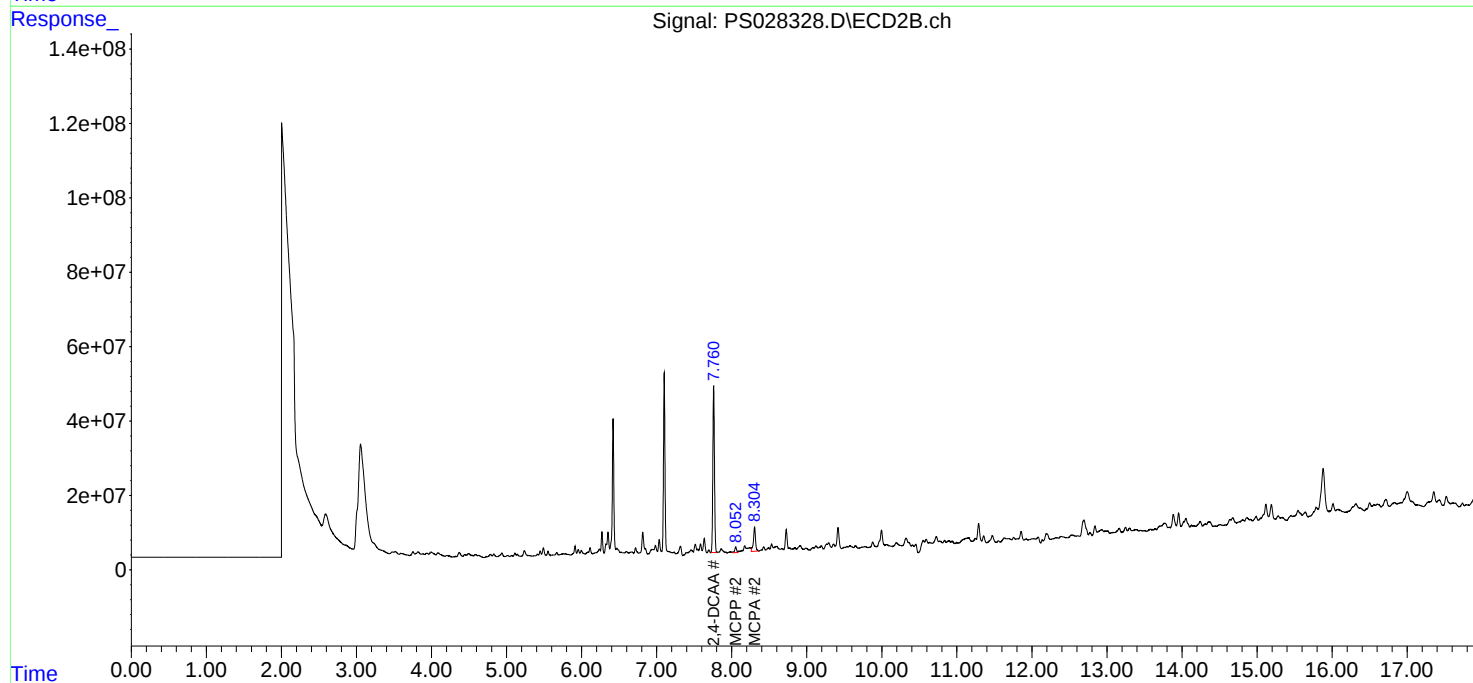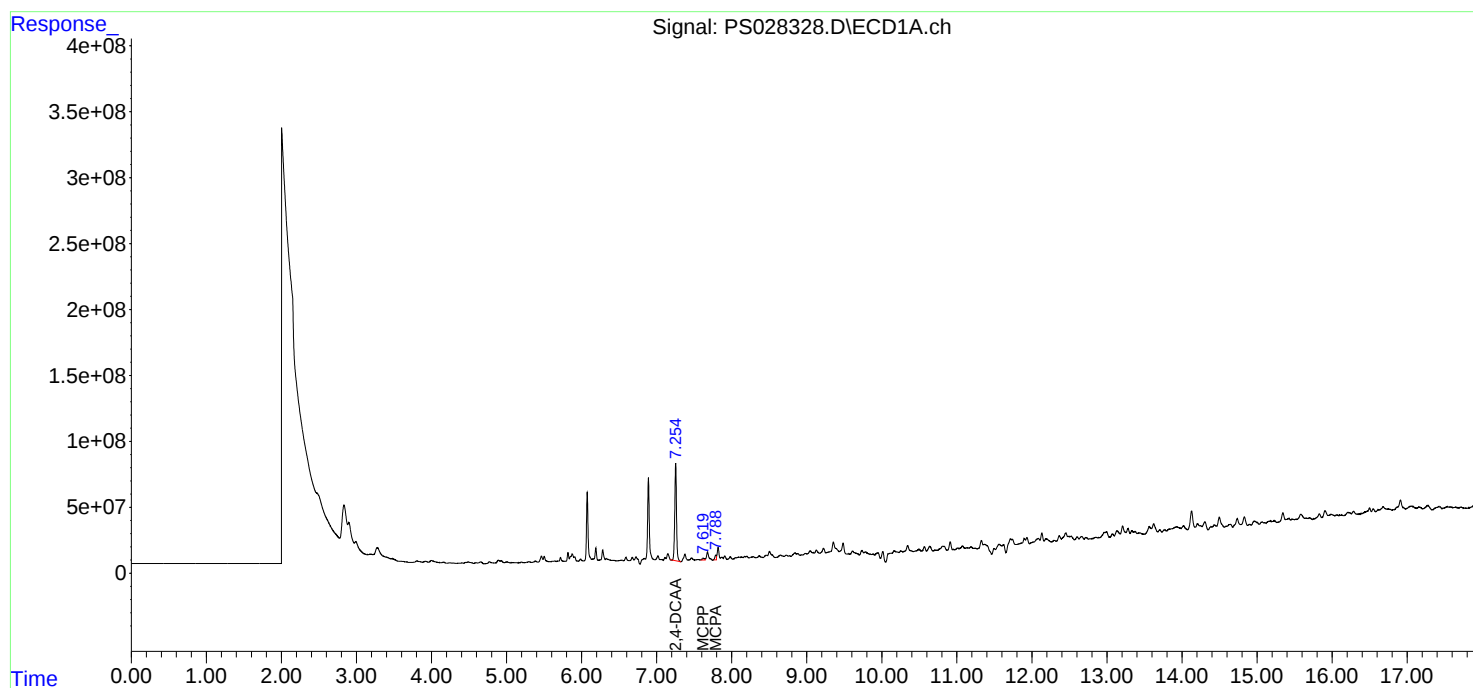

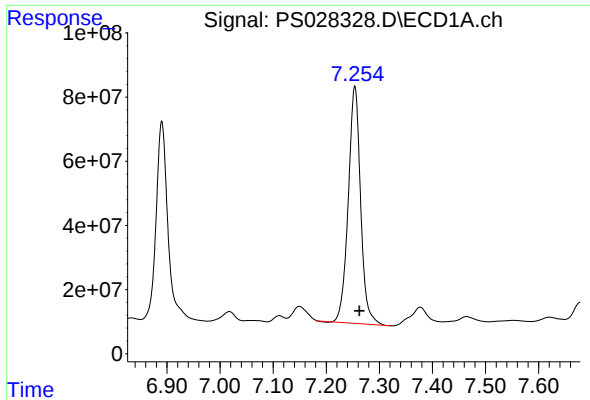


#4 2,4-DCAA

R.T.: 7.254 min
Delta R.T.: -0.009 min
Response: 1194330105
Conc: 466.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
CC0R7


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

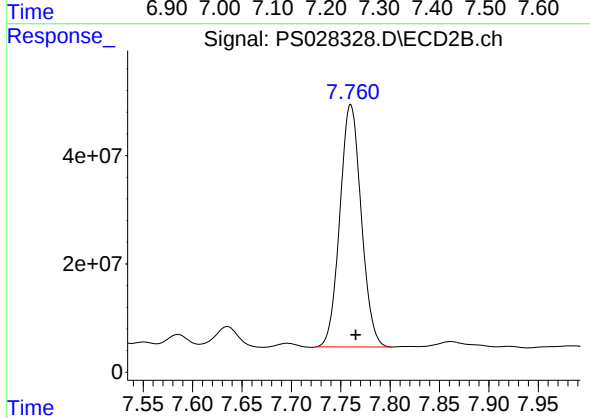


#4 2,4-DCAA

R.T.: 7.760 min
Delta R.T.: -0.006 min
Response: 674061329
Conc: 387.00 ng/ml m

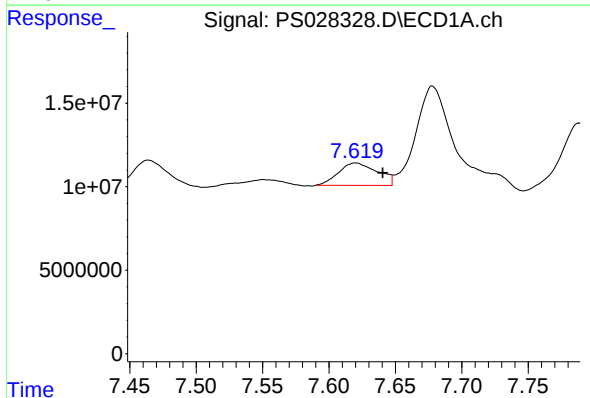


#6 MCPP

R.T.: 7.619 min
Delta R.T.: -0.022 min
Response: 27372444
Conc: 3.61 ug/ml m

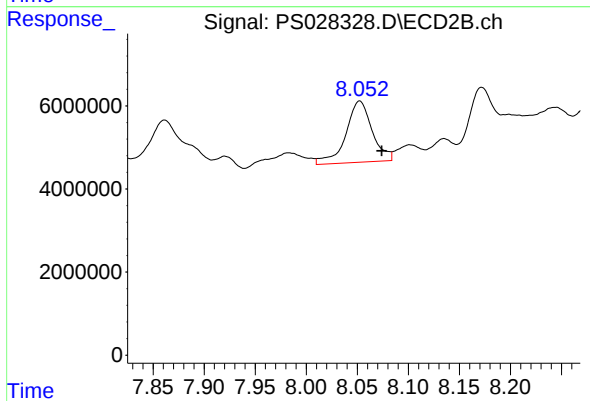

#6 MCPP

R.T.: 8.052 min
Delta R.T.: -0.022 min
Response: 26479777
Conc: 4.36 ug/ml

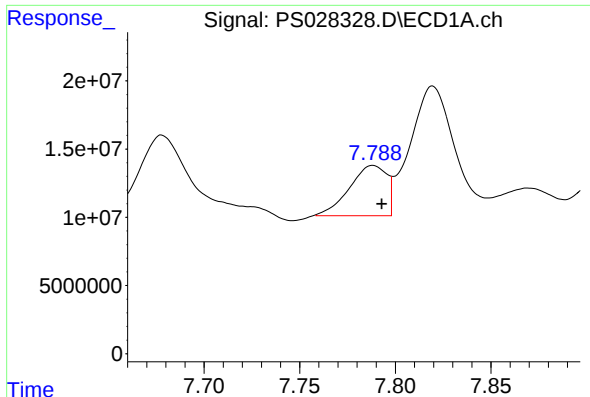


#7 MCPA

R.T.: 7.788 min
Delta R.T.: -0.005 min
Response: 50382479
Conc: 4.84 ug/ml

Instrument :
ECD_S
ClientSampleId :
CC0R7

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

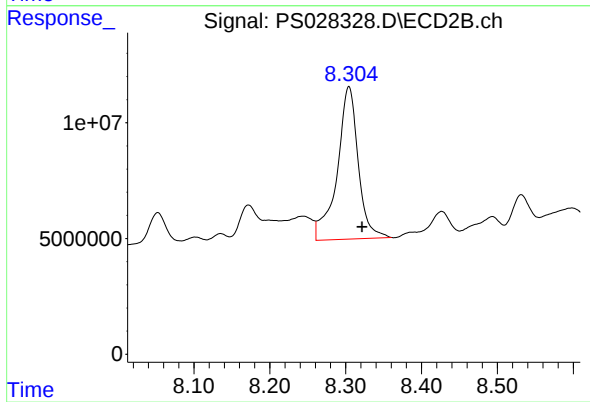

#7 MCPA

R.T.: 8.304 min
Delta R.T.: -0.017 min
Response: 127033962
Conc: 15.23 ug/ml