

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
 Data File : PS032277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 10:11
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:05:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.289	0.000	2590840	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.438	0.000	17074732	0	2.641	N.D. #
3) T	4-Nitroph...	7.122	7.135f	7094	498119	<MDL	<MDL #
5) T	DICAMBA	7.471	7.813	1625761	2309875	<MDL	<MDL #
6) T	MCP	0.000	7.908	0	13561990	N.D.	1.020
7) T	MCPA	7.782	8.113f	4113423	959834	<MDL	<MDL #
8) T	DICHLORPROP	8.183	0.000	1328787	0	<MDL	N.D. #
9) T	2,4-D	0.000	8.851	0	3367778	N.D.	<MDL
10) T	Pentachlo...	8.701	9.362	3573145	5204645	<MDL	<MDL #
11) T	2,4,5-TP ...	9.286	9.767	4006605	2393193	<MDL	<MDL #
12) T	2,4,5-T	9.616f	10.138f	11149063	2793371	<MDL	<MDL #
14) T	DINOSEB	11.343	11.111	21837912	4194856	1.050	<MDL #
15) T	Picloram	11.172	0.000	15109598	0	<MDL	N.D. #
16) T	DCPA	11.646	12.169f	9691393	25602471	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
Data File : PS032277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 10:11
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:05:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

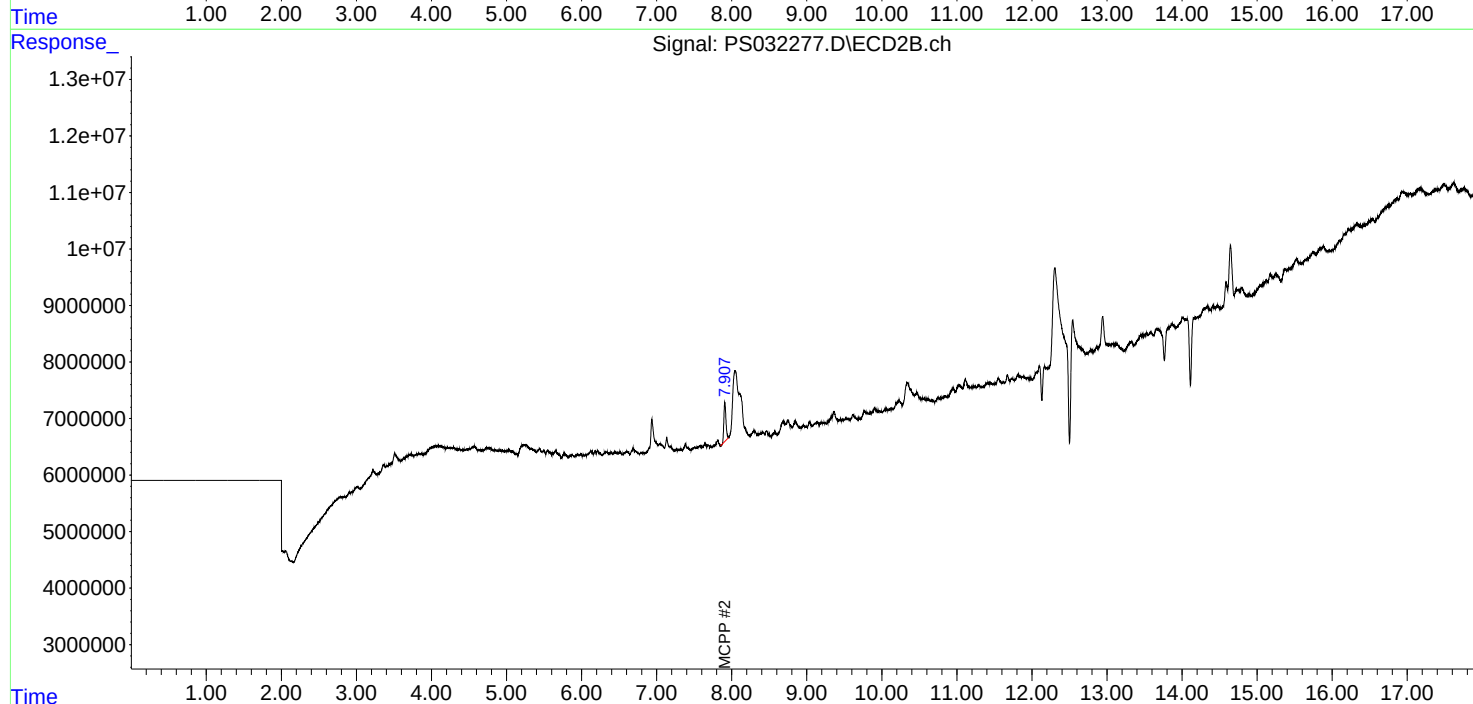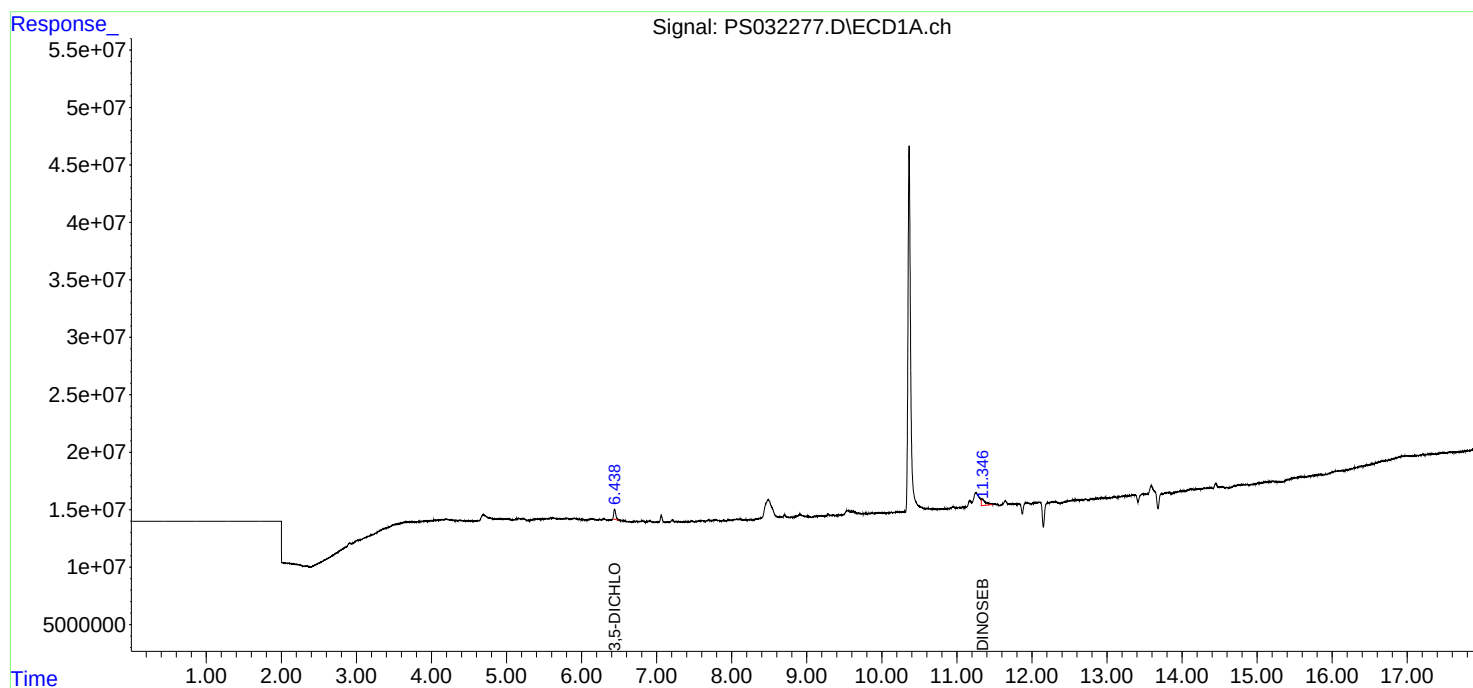


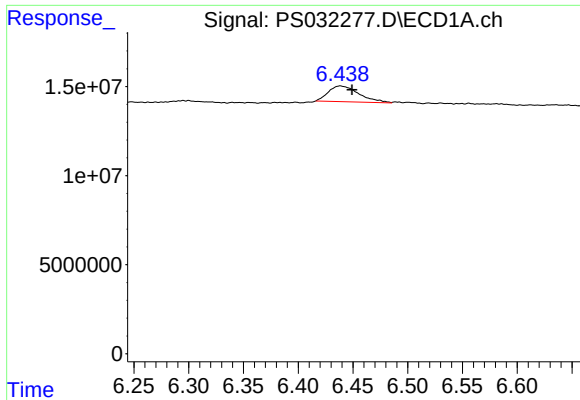

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.438 min
Delta R.T.: -0.011 min
Response: 17074732
Conc: 2.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

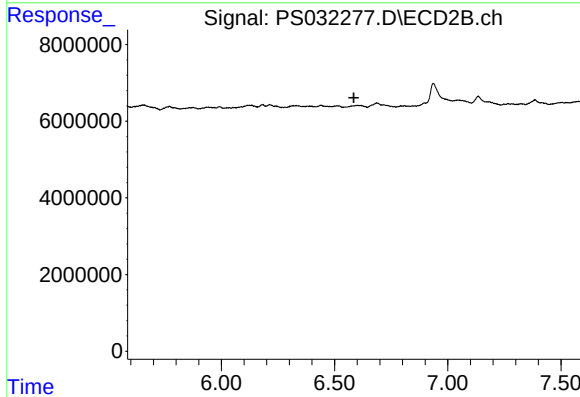


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

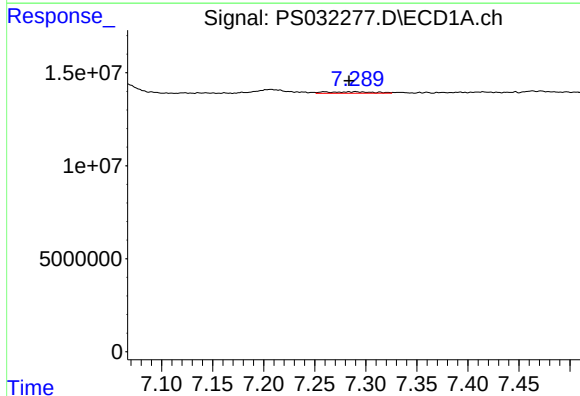


#4 2,4-DCAA

R.T.: 7.289 min
Delta R.T.: 0.006 min
Response: 2590840
Conc: N.D.

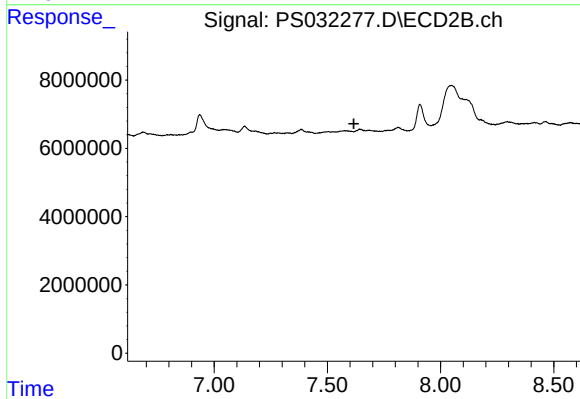

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.617 min
Response: 0
Conc: N.D.

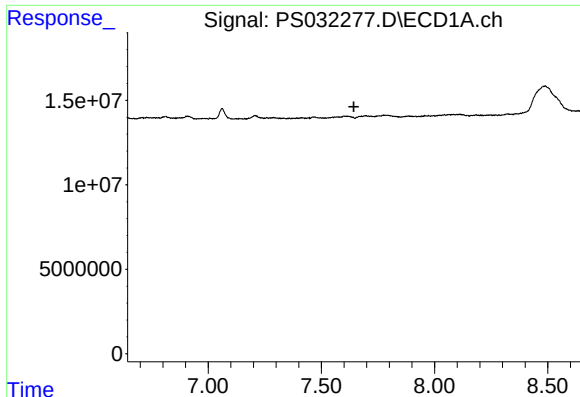

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

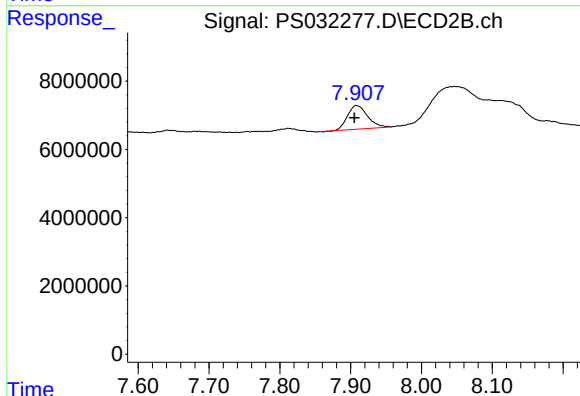


#6 MCP

R.T.: 7.908 min
Delta R.T.: 0.003 min
Response: 13561990
Conc: 1.02 ug/ml

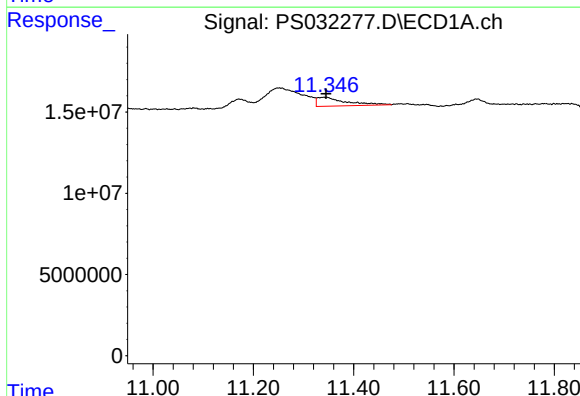

#14 DINOSEB

R.T.: 11.343 min
Delta R.T.: -0.002 min
Response: 21837912
Conc: 1.05 ng/ml

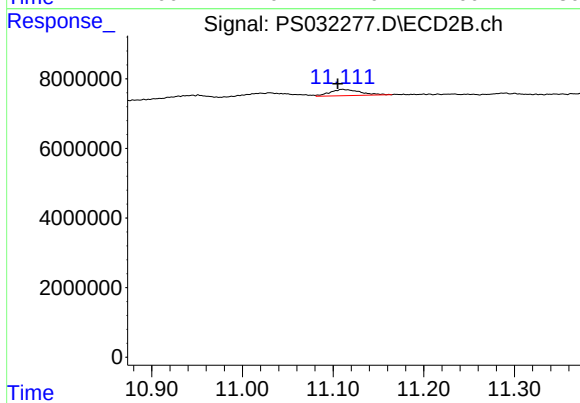

#14 DINOSEB

R.T.: 11.111 min
Delta R.T.: 0.006 min
Response: 4194856
Conc: N.D.