

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
 Data File : PS032278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 10:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:05:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.282	7.617	1865.5E6	1936.1E6	411.687	531.104 #
Target Compounds							
2) T	3,5-DICHL...	6.437	0.000	2966755	0	<MDL	N.D. #
6) T	MCP	7.671f	0.000	369964	0	<MDL	N.D. #
7) T	MCPA	7.786	0.000	521763	0	<MDL	N.D. #
8) T	DICHLORPROP	8.175	0.000	225426	0	<MDL	N.D. #
10) T	Pentachlo...	8.712	9.367	5566783	5893556	<MDL	<MDL #
11) T	2,4,5-TP ...	9.282	9.769	5943135	1141738	<MDL	<MDL #
12) T	2,4,5-T	9.582	10.138f	876604	1769891	<MDL	<MDL #
13) T	2,4-DB	10.154	0.000	463112	0	<MDL	N.D. #
14) T	DINOSEB	11.343	11.118	11339634	1813847	<MDL	<MDL #
15) T	Picloram	11.178	0.000	3609832	0	<MDL	N.D. #
16) T	DCPA	11.645	12.163	4654925	3898058	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
Data File : PS032278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 10:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:05:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

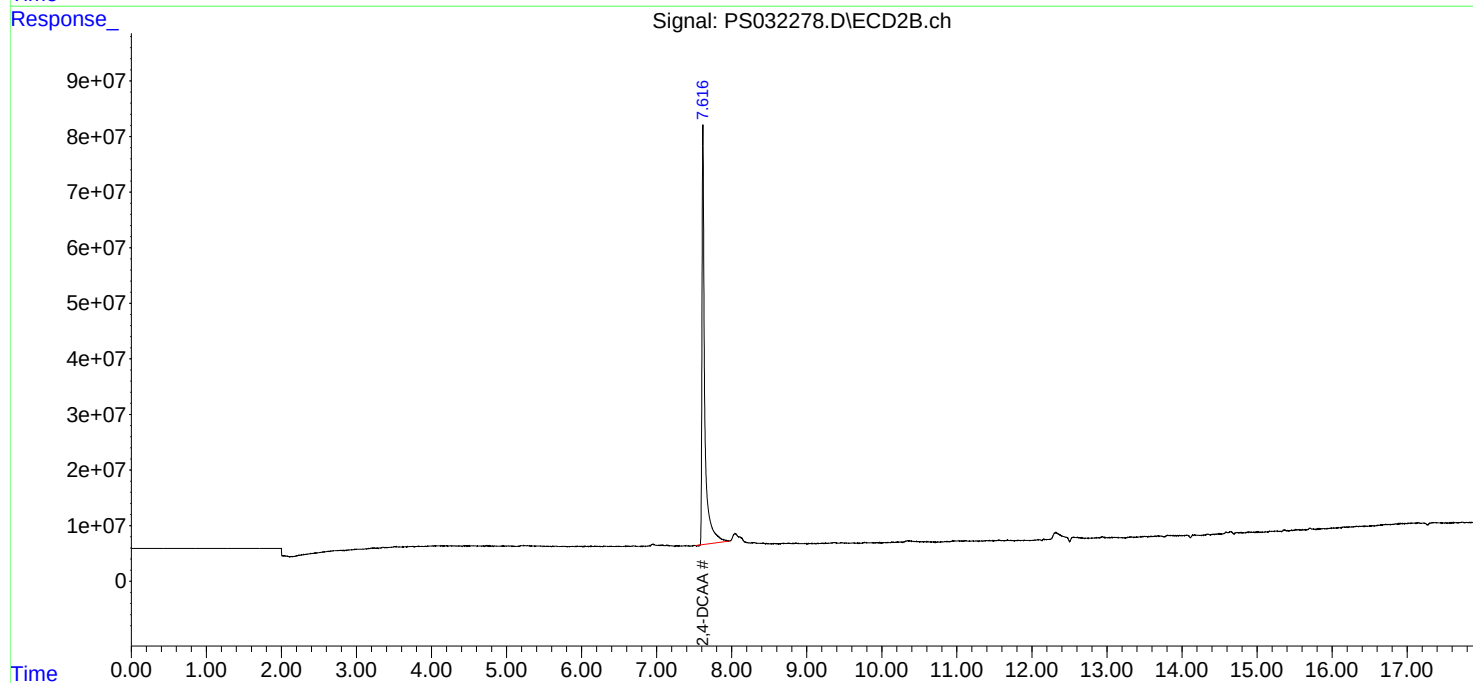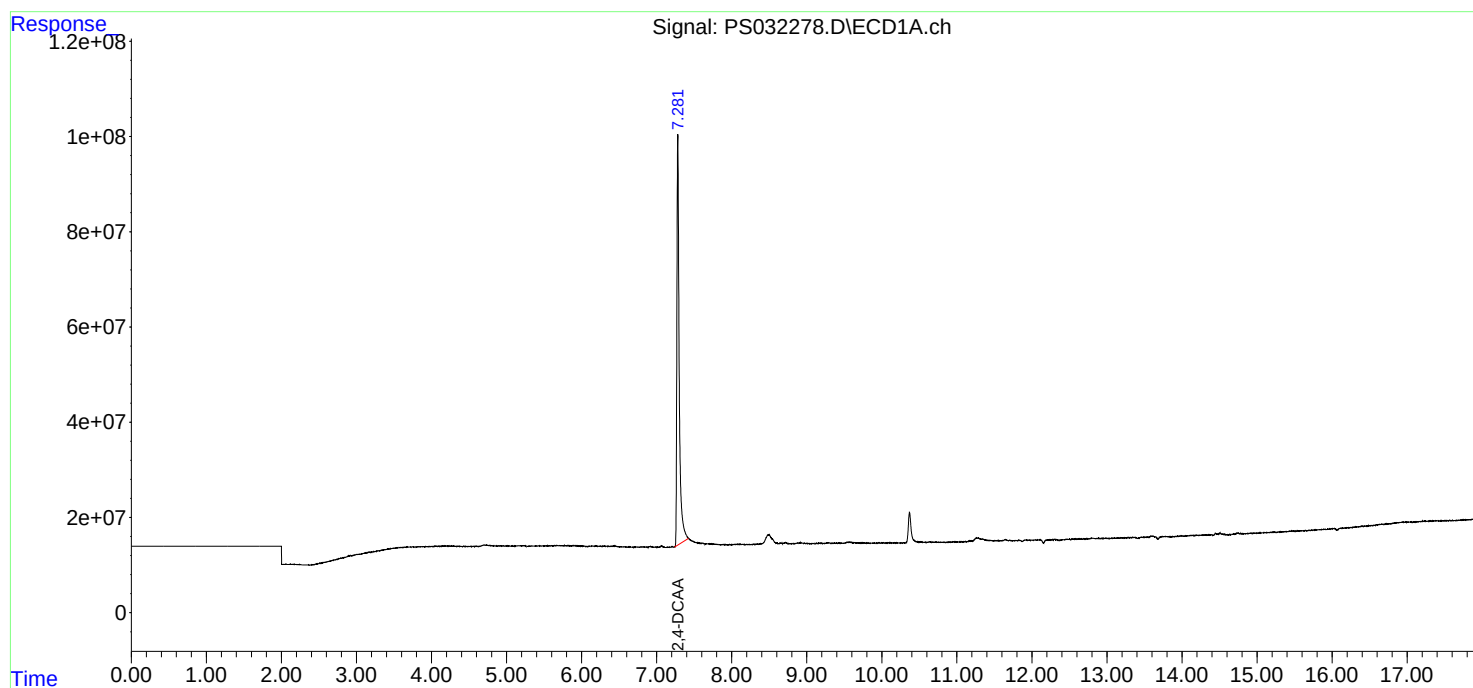


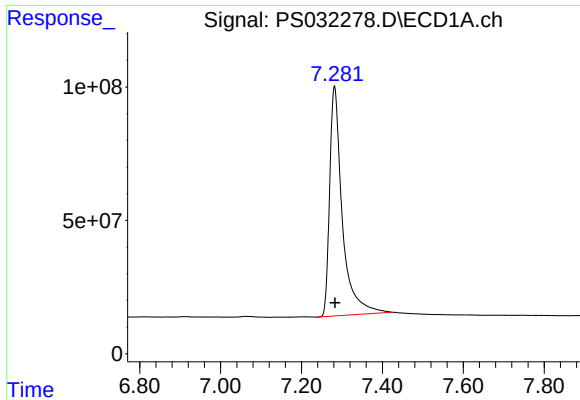

#4 2,4-DCAA

R.T.: 7.282 min
Delta R.T.: -0.002 min
Response: 1865465253
Conc: 411.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

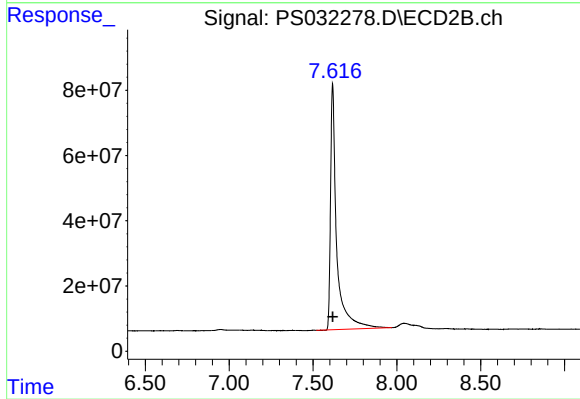

#4 2,4-DCAA

R.T.: 7.617 min
Delta R.T.: 0.000 min
Response: 1936138177
Conc: 531.10 ng/ml