

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
 Data File : PS032287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 14:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:06:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.618	1762.3E6	1896.6E6	388.910	520.255 #
Target Compounds							
2) T	3,5-DICHL...	6.443	0.000	9544421	0	1.476	N.D. #
6) T	MCP	0.000	7.900	0	14931228	N.D.	1.123
7) T	MCPA	7.803	0.000	2239586	0	<MDL	N.D. #
8) T	DICHLORPROP	8.169	0.000	495274	0	<MDL	N.D. #
10) T	Pentachlo...	8.709	9.368	5119758	1753600	<MDL	<MDL #
11) T	2,4,5-TP ...	9.278	0.000	4331963	0	<MDL	N.D. #
12) T	2,4,5-T	9.576	10.141f	2006522	1631475	<MDL	<MDL #
13) T	2,4-DB	10.179	0.000	502780	0	<MDL	N.D. #
14) T	DINOSEB	11.340	0.000	2116690	0	<MDL	N.D. #
15) T	Picloram	11.164	12.178f	243018	5188201	<MDL	<MDL #
16) T	DCPA	11.642	12.178f	451534	5188201	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
Data File : PS032287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 14:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:06:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

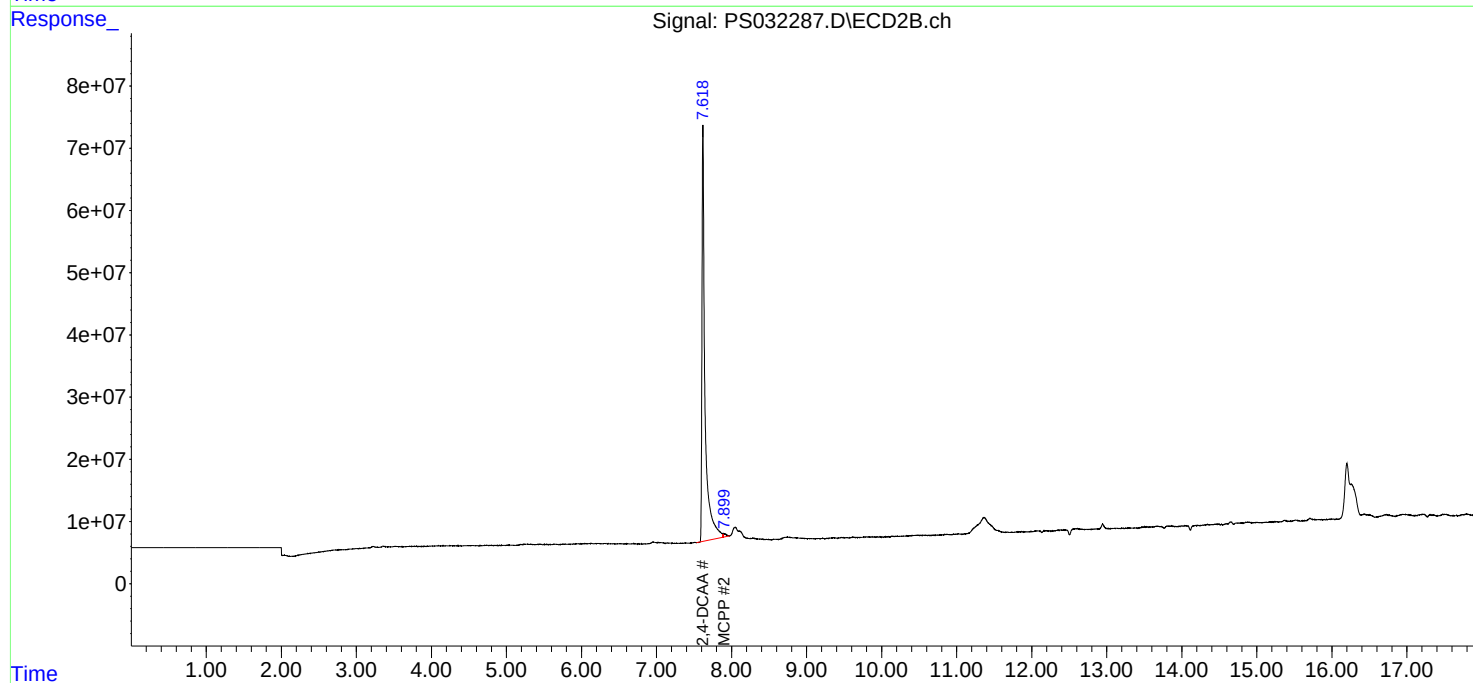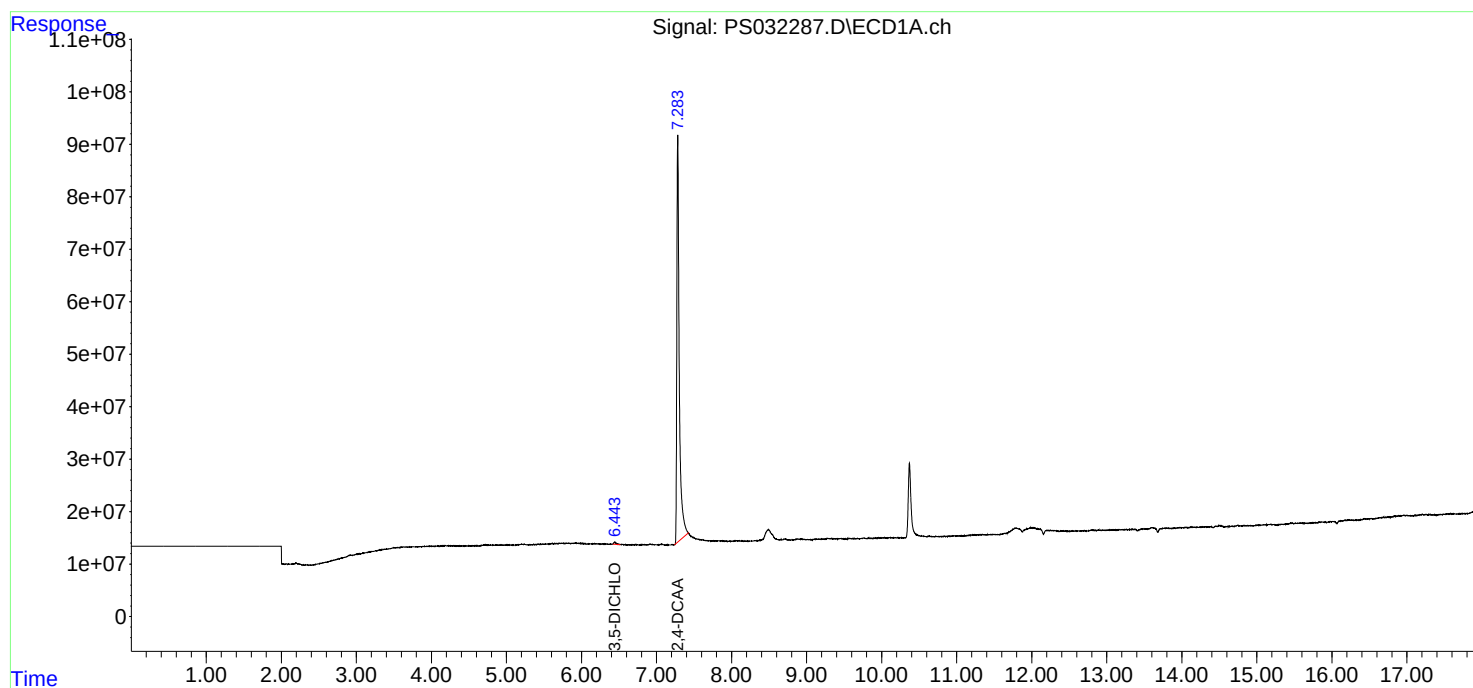


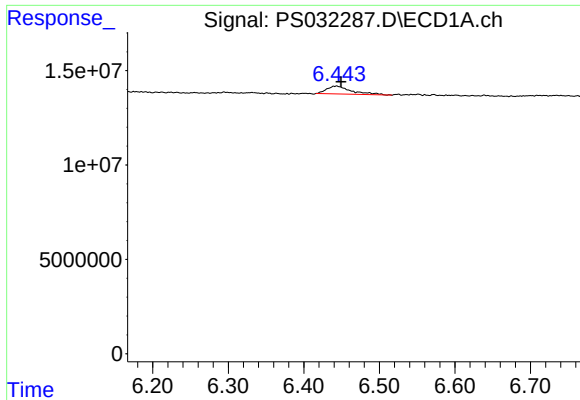

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.443 min
Delta R.T.: -0.007 min
Response: 9544421
Conc: 1.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

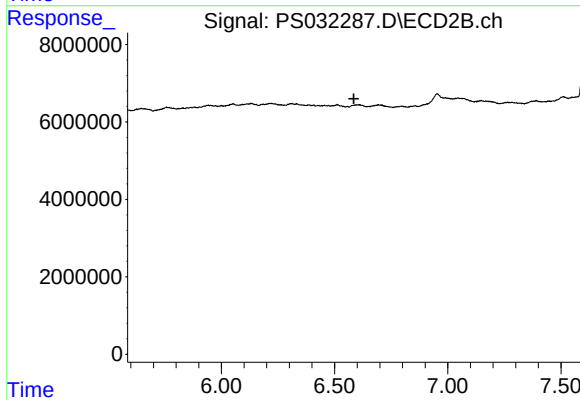


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

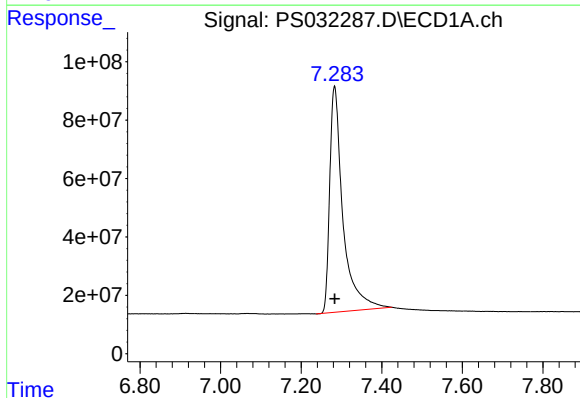


#4 2,4-DCAA

R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1762257577
Conc: 388.91 ng/ml

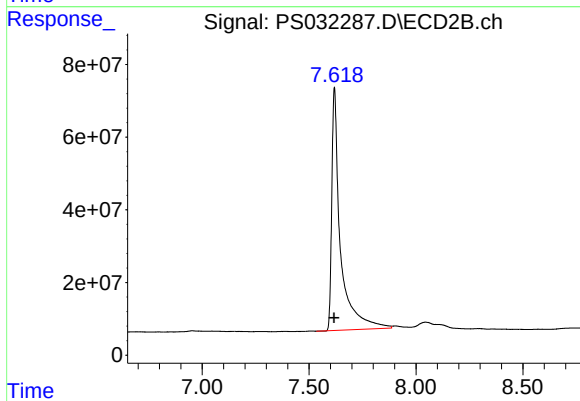

#4 2,4-DCAA


R.T.: 7.618 min
Delta R.T.: 0.001 min
Response: 1896588059
Conc: 520.26 ng/ml

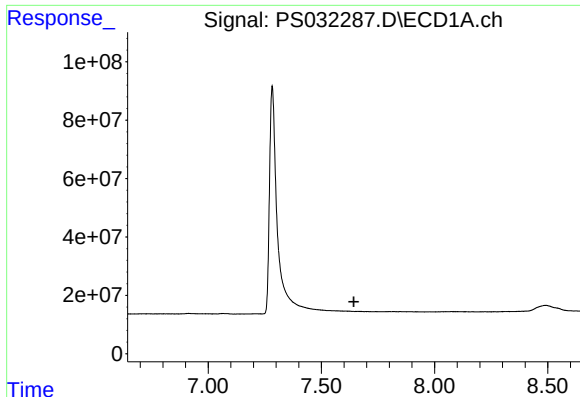

#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

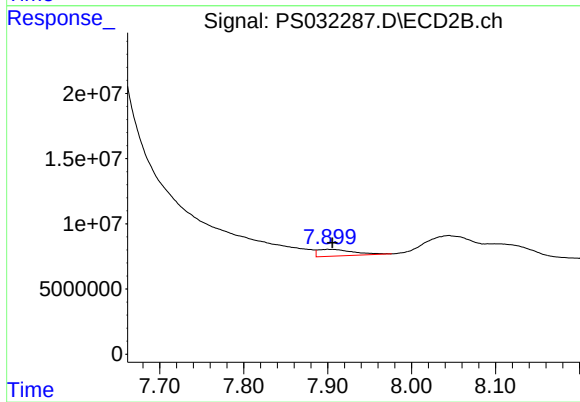

#6 MCPP

R.T.: 7.900 min
Delta R.T.: -0.005 min
Response: 14931228
Conc: 1.12 ug/ml