

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
 Data File : PS032298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 19:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:08:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.283	7.619	1753.1E6	1873.2E6	386.887	513.850	#
Target Compounds								
2) T	3,5-DICHL...	6.442	0.000	31353612	0	4.849	N.D.	#
3) T	4-Nitroph...	7.076f	0.000	1379716	0	1.028	N.D.	#
6) T	MCP	7.602f	7.910	-35172	24101919	N.D.	1.812	
7) T	MCPA	7.806	0.000	746738	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.189	0.000	863715	0	<MDL	N.D.	#
9) T	2,4-D	8.455f	0.000	36068956	0	7.994	N.D.	#
10) T	Pentachlo...	8.718	9.366	3821721	2754698	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.280	9.776f	2537529	1452254	<MDL	<MDL	#
12) T	2,4,5-T	9.570	10.177	2386982	2078556	<MDL	<MDL	#
13) T	2,4-DB	10.174	0.000	1604088	0	<MDL	N.D.	#
14) T	DINOSEB	11.348	0.000	7857688	0	<MDL	N.D.	#
15) T	Picloram	11.195	0.000	6808110	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
Data File : PS032298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 19:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:08:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

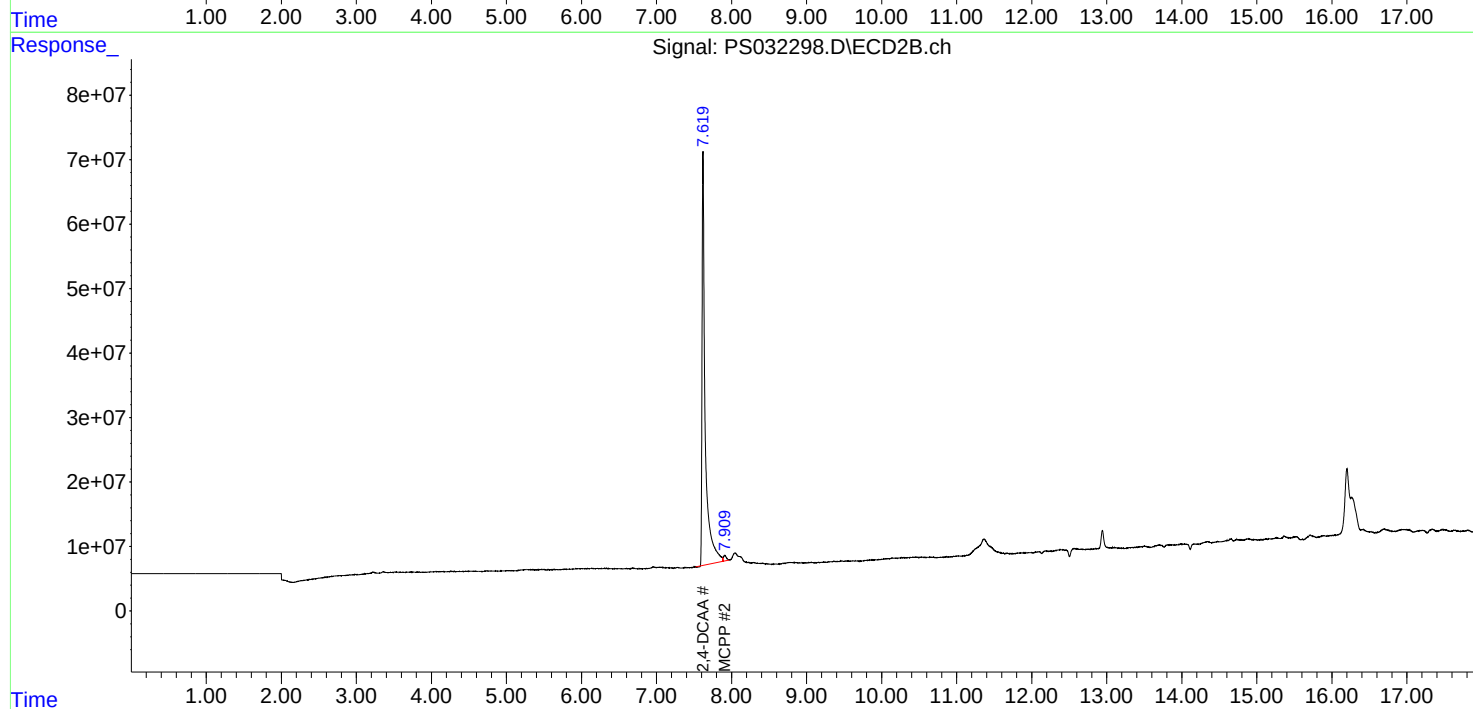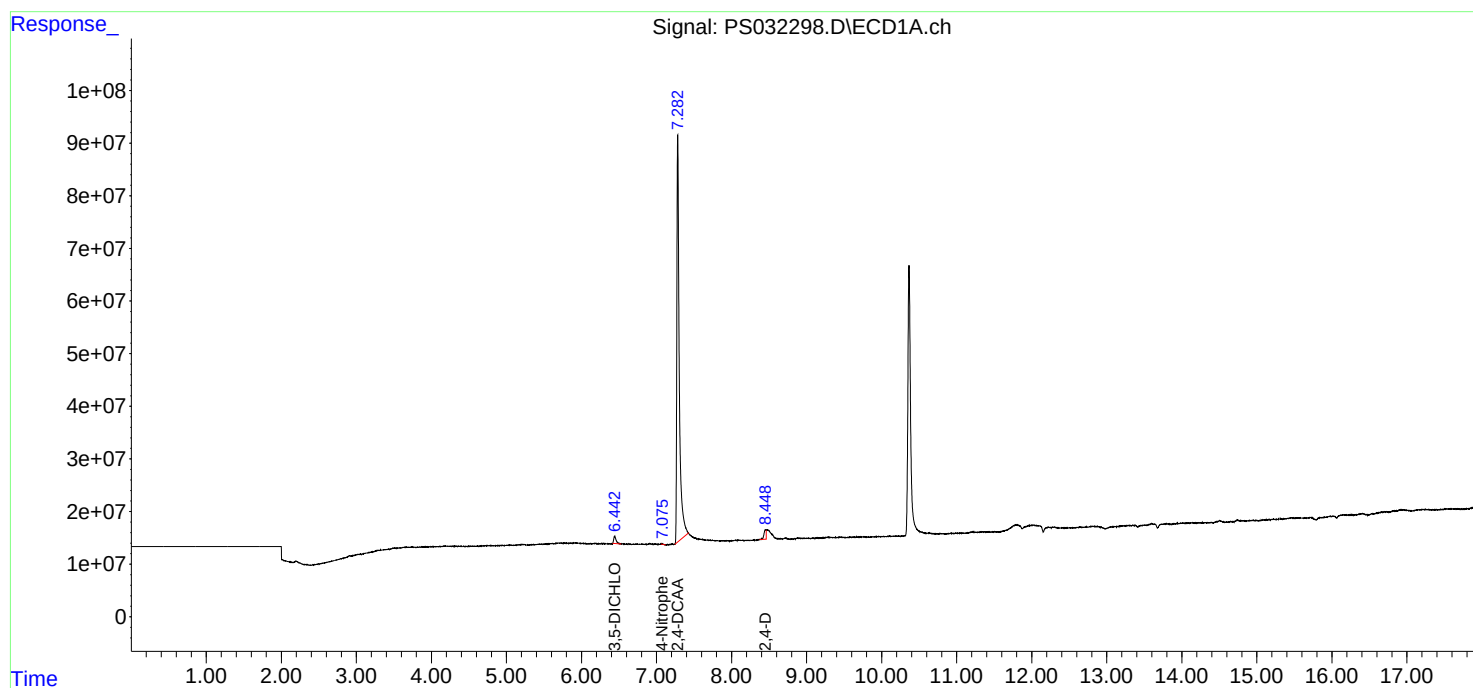


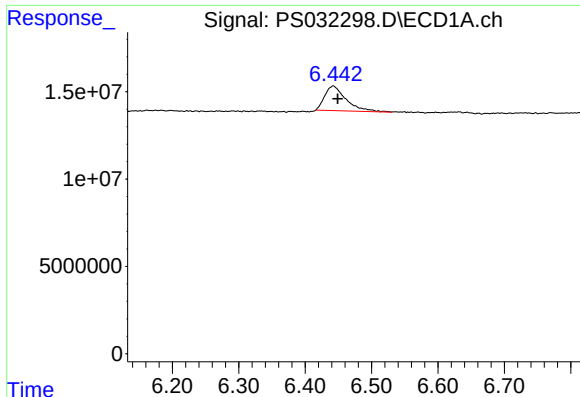

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.442 min
Delta R.T.: -0.007 min
Response: 31353612
Conc: 4.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

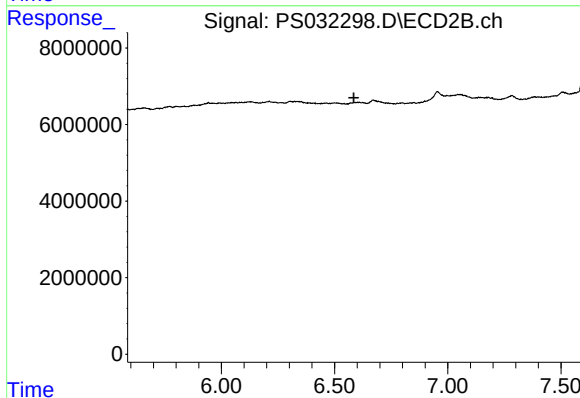


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

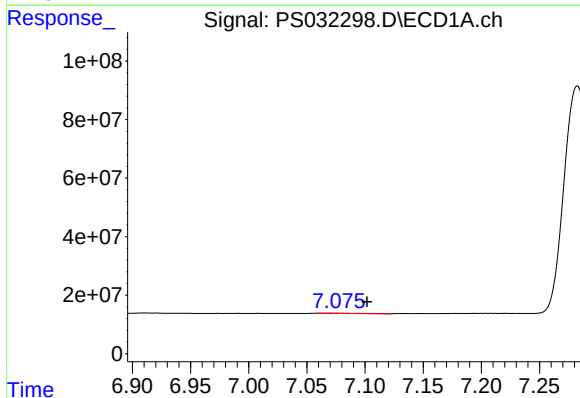


#3 4-Nitrophenol

R.T.: 7.076 min
Delta R.T.: -0.026 min
Response: 1379716
Conc: 1.03 ng/ml

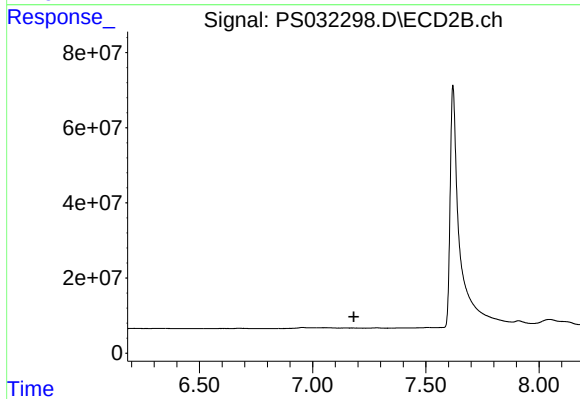

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

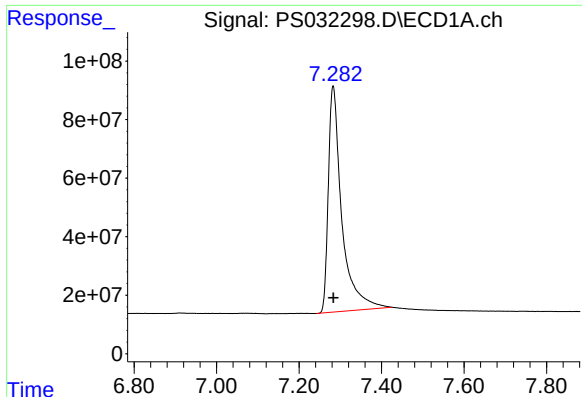

#4 2,4-DCAA


R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1753092544
Conc: 386.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

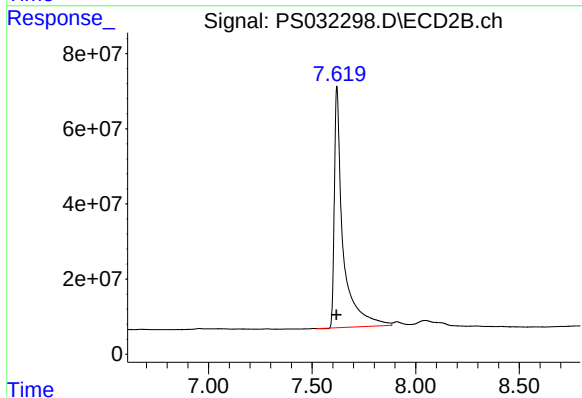


#4 2,4-DCAA

R.T.: 7.619 min
Delta R.T.: 0.002 min
Response: 1873237503
Conc: 513.85 ng/ml

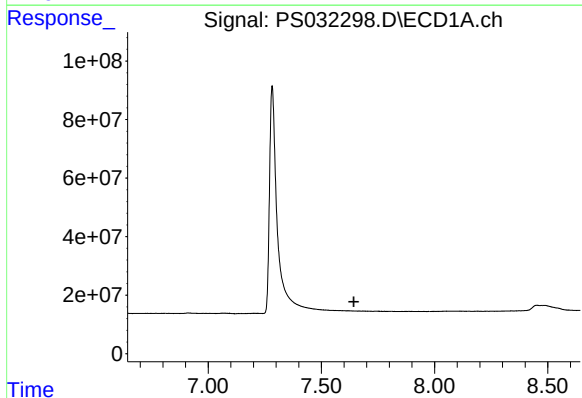


#6 MCP

R.T.: 7.602 min
Delta R.T.: -0.042 min
Response: -35172
Conc: N.D.

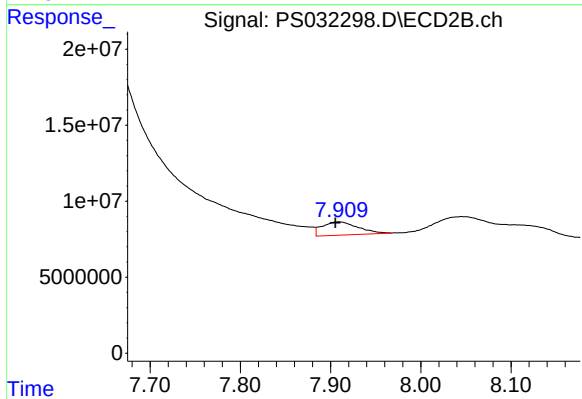

#6 MCP


R.T.: 7.910 min
Delta R.T.: 0.004 min
Response: 24101919
Conc: 1.81 ug/ml

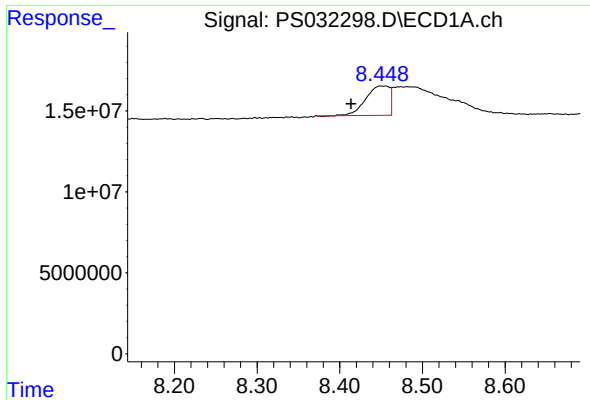

#9 2,4-D

R.T.: 8.455 min
Delta R.T.: 0.042 min
Response: 36068956
Conc: 7.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

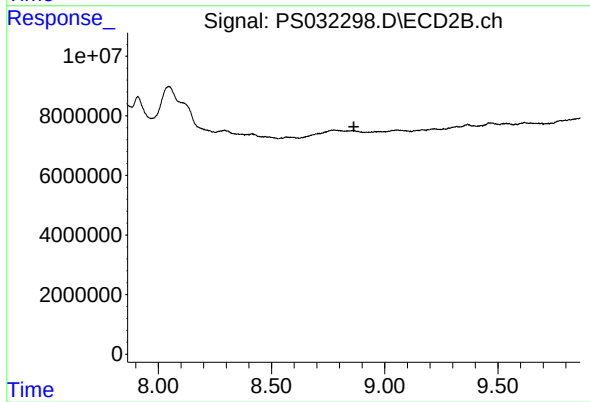

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.864 min
Response: 0
Conc: N.D.