

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
 Data File : PS032303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 21:49
 Operator : AR\AJ
 Sample : Q3530-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:09:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.279	7.613	1705.8E6	1926.5E6	376.454	528.458 #
Target Compounds							
1) T	Dalapon	2.636	2.615	2697.8E6	5196.7E6	375.798	747.293 #
2) T	3,5-DICHL...	6.452	6.591	268.8E6	215.0E6	41.573	35.774
3) T	4-Nitroph...	7.130f	7.227f	71629179	87595646	53.357	38.590 #
5) T	DICAMBA	7.465	7.807	787.4E6	836.6E6	41.734	48.438
6) T	MCPD	7.636	7.899	-1086719	32081072	N.D.	2.412
7) T	MCPA	7.787	8.144	33755131	33634841	2.514	2.063
8) T	DICHLORPROP	8.175	8.524	283.6E6	257.1E6	63.743	53.919
9) T	2,4-D	8.427	8.881	223.3E6	327.3E6	49.494	62.391 #
10) T	Pentachlo...	8.700	9.357	3298.2E6	3454.7E6	52.570	58.851
11) T	2,4,5-TP ...	9.279	9.742	1288.1E6	2037.8E6	49.521	75.884 #
12) T	2,4,5-T	9.583	10.186	1336.7E6	1264.8E6	56.076	53.325
13) T	2,4-DB	10.172	10.755	644.2E6	232.7E6	244.460	61.703 #
14) T	DINOSEB	11.343	11.106	833.3E6	653.4E6	40.049	36.943
15) T	Picloram	11.151f	12.256f	86483339	1480.8E6	4.074	39.825 #
16) T	DCPA	11.639	12.139	1323.6E6	1960.6E6	39.449	61.538 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
Data File : PS032303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 21:49
Operator : AR\AJ
Sample : Q3530-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:09:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

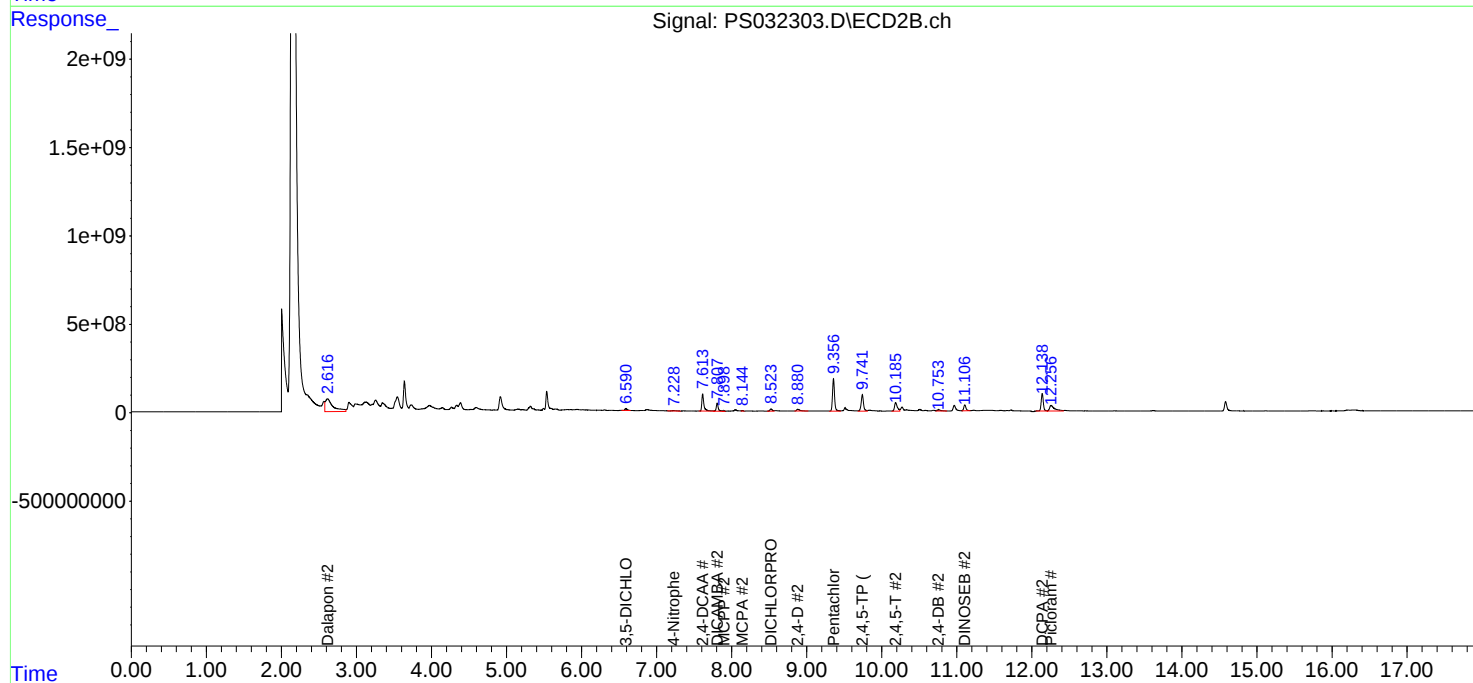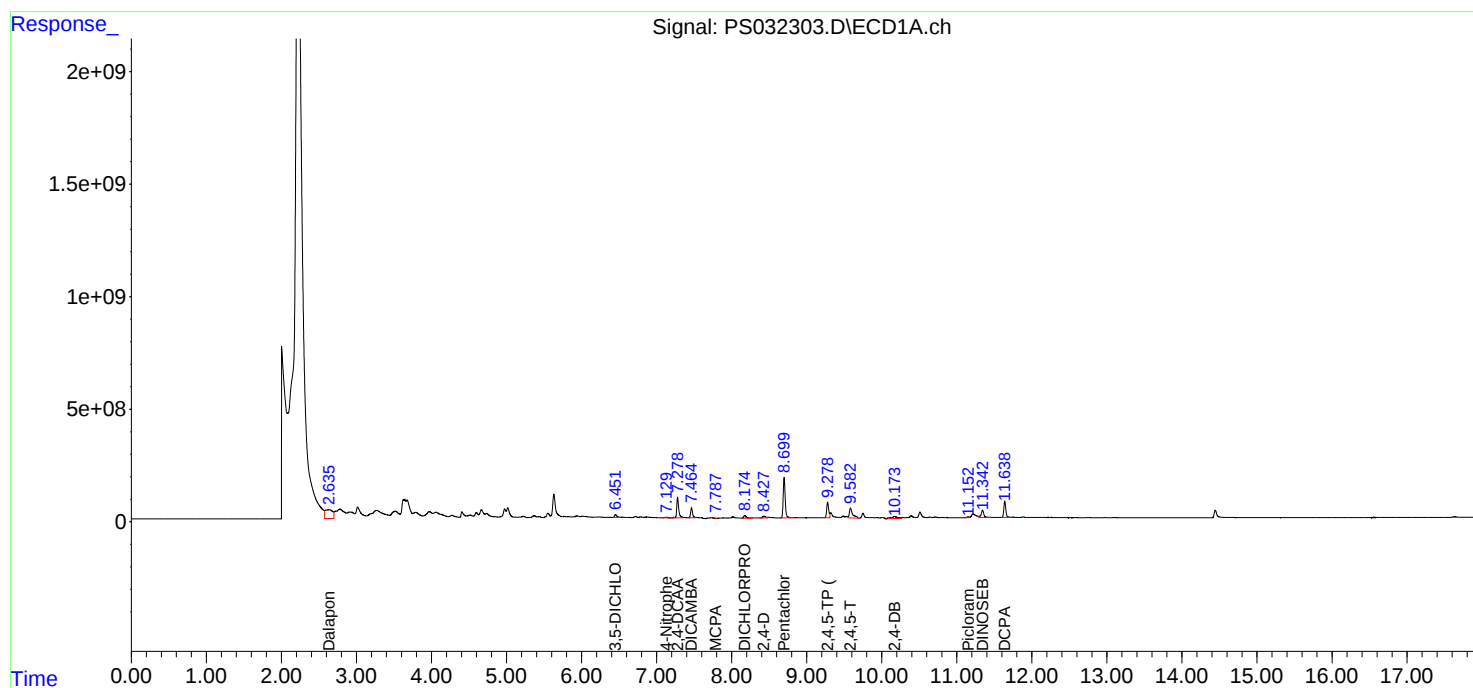


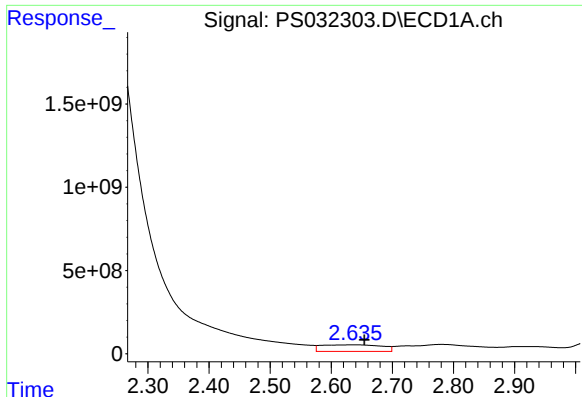

#1 Dalapon


R.T.: 2.636 min
Delta R.T.: -0.018 min
Response: 2697766951
Conc: 375.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

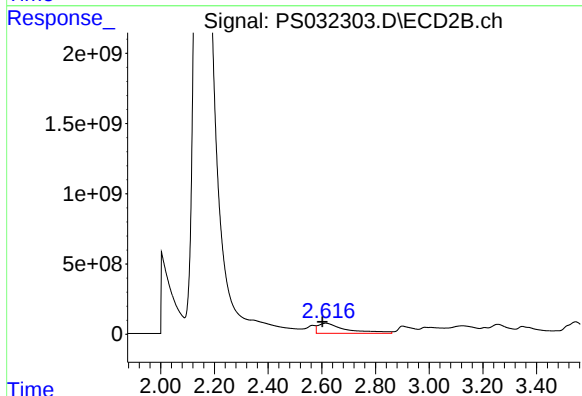


#1 Dalapon

R.T.: 2.615 min
Delta R.T.: 0.012 min
Response: 5196675927
Conc: 747.29 ng/ml

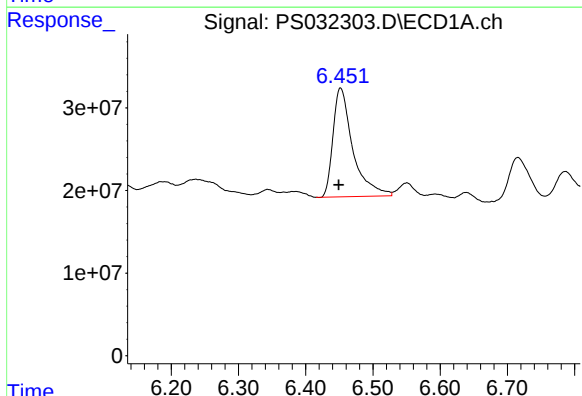


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.452 min
Delta R.T.: 0.003 min
Response: 268819380
Conc: 41.57 ng/ml

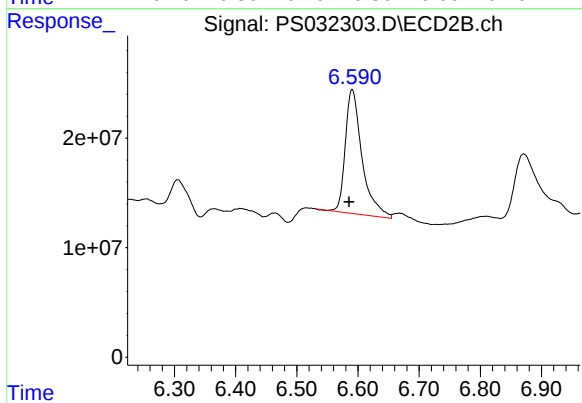

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.591 min
Delta R.T.: 0.005 min
Response: 214963365
Conc: 35.77 ng/ml

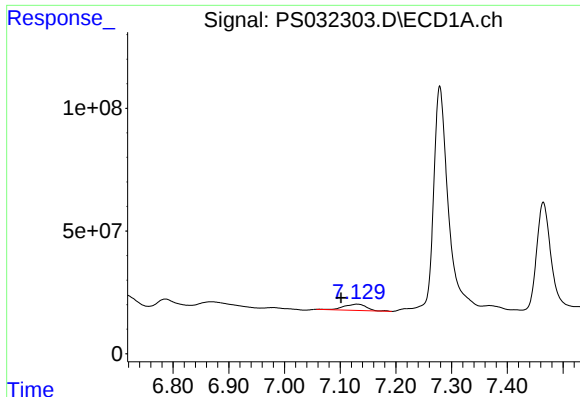

#3 4-Nitrophenol


R.T.: 7.130 min
Delta R.T.: 0.029 min
Response: 71629179
Conc: 53.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

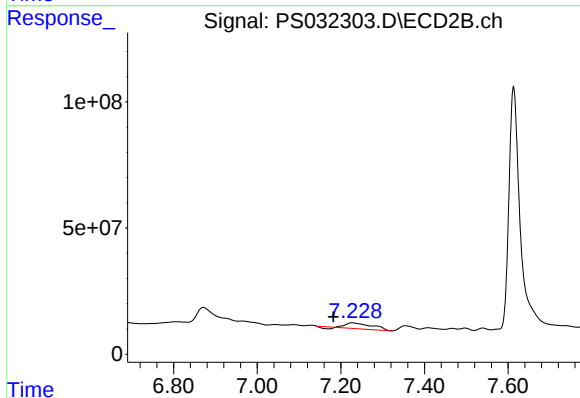


#3 4-Nitrophenol

R.T.: 7.227 min
Delta R.T.: 0.045 min
Response: 87595646
Conc: 38.59 ng/ml

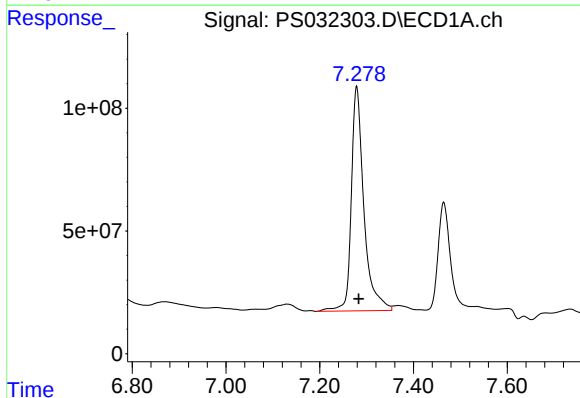


#4 2,4-DCAA

R.T.: 7.279 min
Delta R.T.: -0.005 min
Response: 1705817294
Conc: 376.45 ng/ml

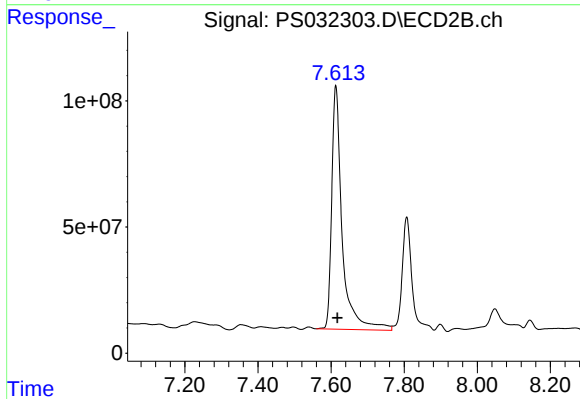

#4 2,4-DCAA


R.T.: 7.613 min
Delta R.T.: -0.004 min
Response: 1926490544
Conc: 528.46 ng/ml

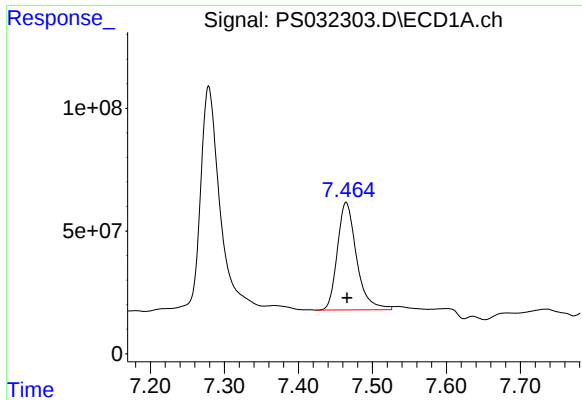

#5 DICAMBA


R.T.: 7.465 min
Delta R.T.: -0.001 min
Response: 787358351
Conc: 41.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

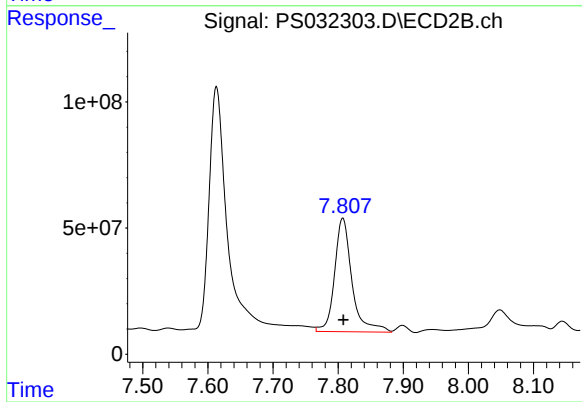


#5 DICAMBA

R.T.: 7.807 min
Delta R.T.: 0.000 min
Response: 836647572
Conc: 48.44 ng/ml

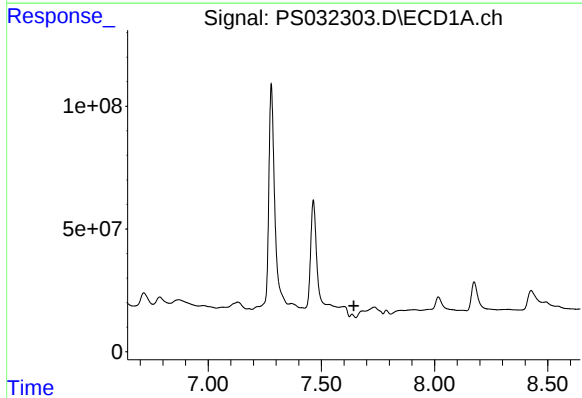


#6 MCP

R.T.: 7.636 min
Delta R.T.: -0.008 min
Response: -1086719
Conc: N.D.

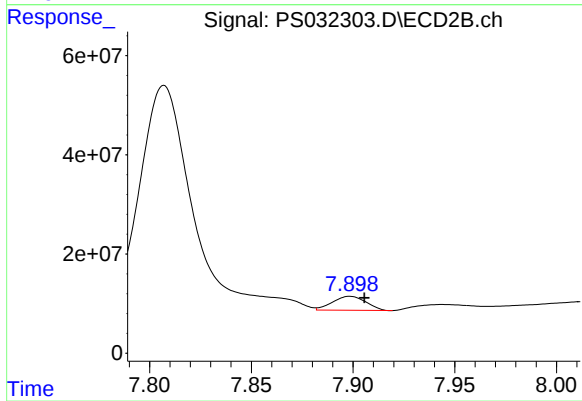

#6 MCP


R.T.: 7.899 min
Delta R.T.: -0.007 min
Response: 32081072
Conc: 2.41 ug/ml

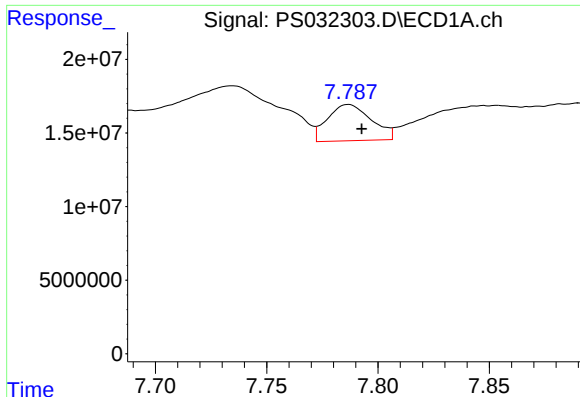

#7 MCPA


R.T.: 7.787 min
Delta R.T.: -0.006 min
Response: 33755131
Conc: 2.51 ug/ml

Instrument :
ECD_S
ClientSampleId :

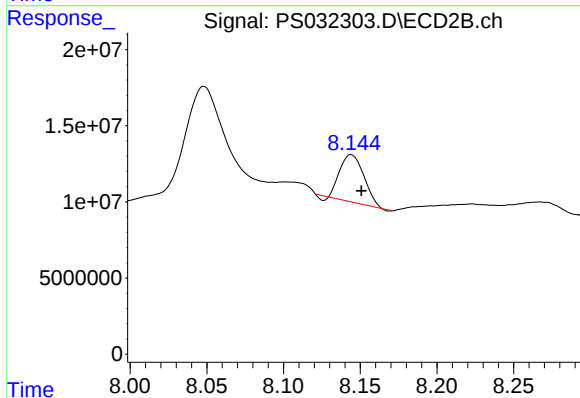


#7 MCPA

R.T.: 8.144 min
Delta R.T.: -0.007 min
Response: 33634841
Conc: 2.06 ug/ml

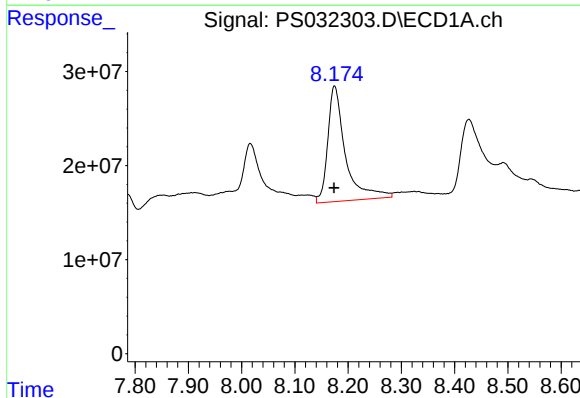


#8 DICHLORPROP

R.T.: 8.175 min
Delta R.T.: 0.000 min
Response: 283575896
Conc: 63.74 ng/ml

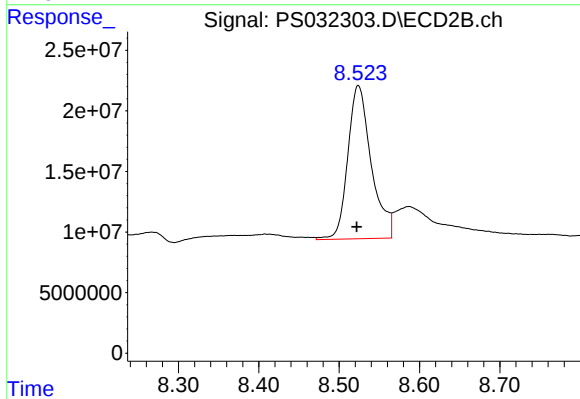

#8 DICHLORPROP


R.T.: 8.524 min
Delta R.T.: 0.002 min
Response: 257148342
Conc: 53.92 ng/ml

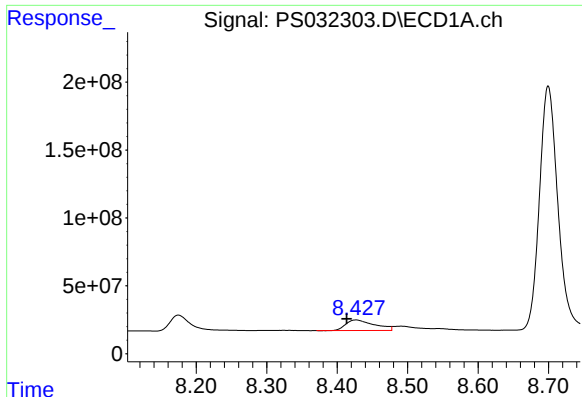

#9 2,4-D


R.T.: 8.427 min
Delta R.T.: 0.013 min
Response: 223306027
Conc: 49.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

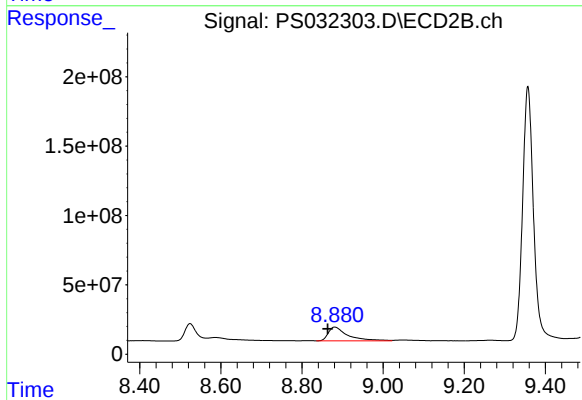


#9 2,4-D

R.T.: 8.881 min
Delta R.T.: 0.017 min
Response: 327283788
Conc: 62.39 ng/ml

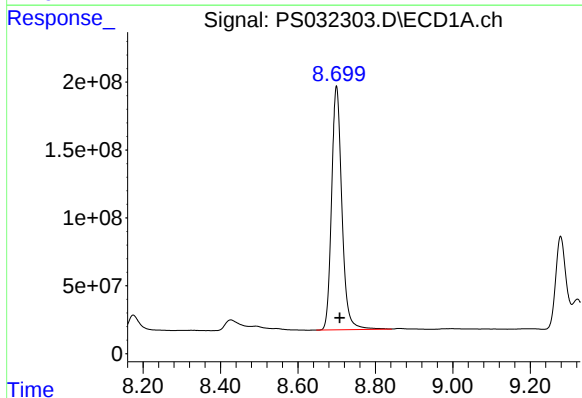


#10 Pentachlorophenol

R.T.: 8.700 min
Delta R.T.: -0.008 min
Response: 3298205333
Conc: 52.57 ng/ml

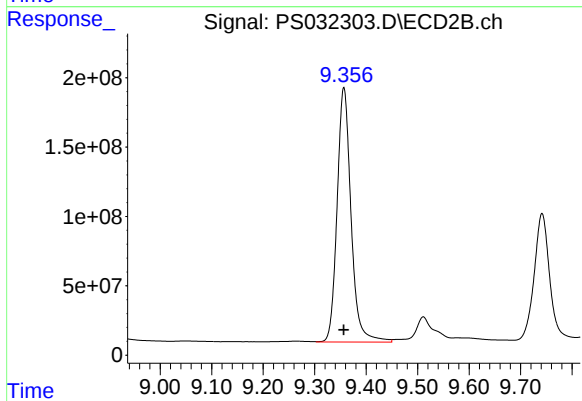

#10 Pentachlorophenol


R.T.: 9.357 min
Delta R.T.: 0.000 min
Response: 3454688412
Conc: 58.85 ng/ml

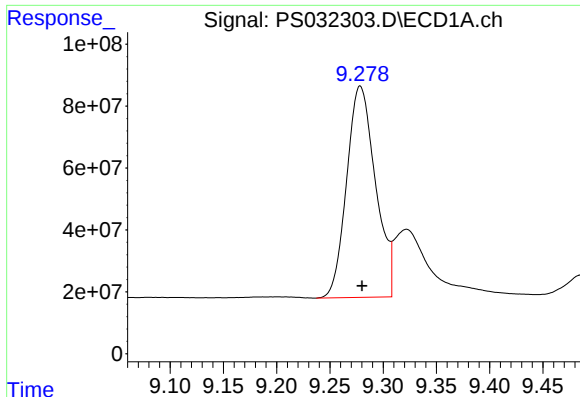

#11 2,4,5-TP (SILVEX)


R.T.: 9.279 min
Delta R.T.: -0.002 min
Response: 1288125676
Conc: 49.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

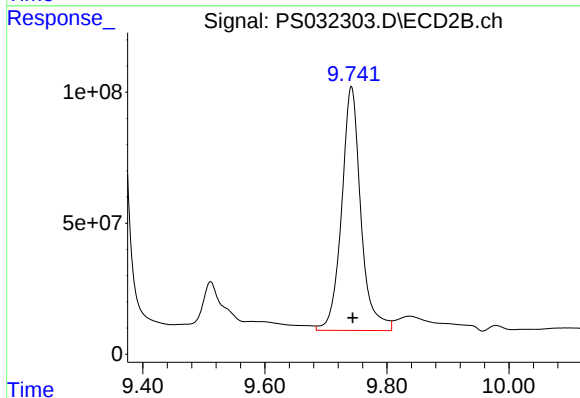


#11 2,4,5-TP (SILVEX)

R.T.: 9.742 min
Delta R.T.: -0.002 min
Response: 2037791247
Conc: 75.88 ng/ml

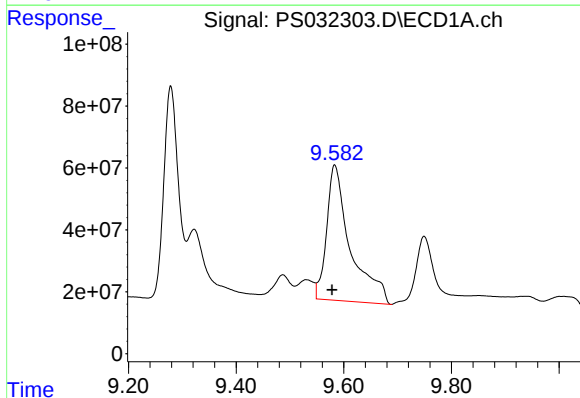


#12 2,4,5-T

R.T.: 9.583 min
Delta R.T.: 0.005 min
Response: 1336744918
Conc: 56.08 ng/ml

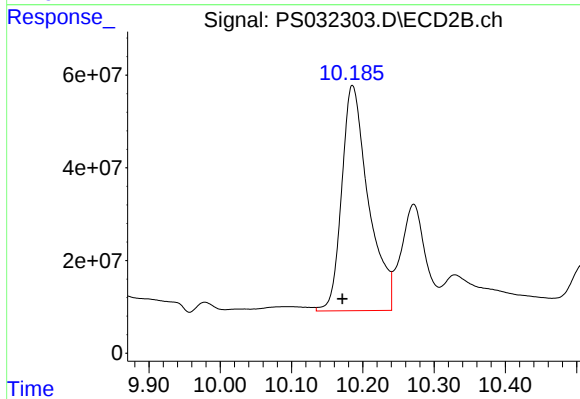

#12 2,4,5-T


R.T.: 10.186 min
Delta R.T.: 0.014 min
Response: 1264755435
Conc: 53.32 ng/ml

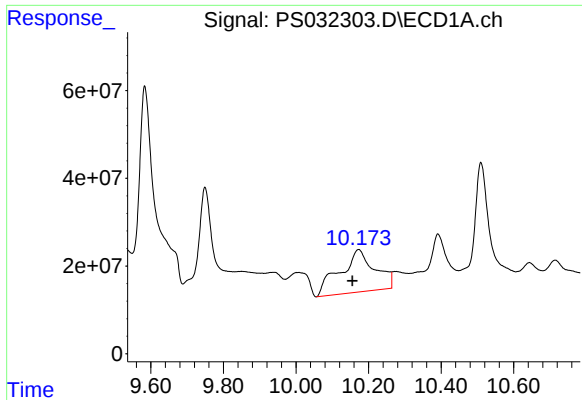

#13 2,4-DB


R.T.: 10.172 min
Delta R.T.: 0.017 min
Response: 644180216
Conc: 244.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

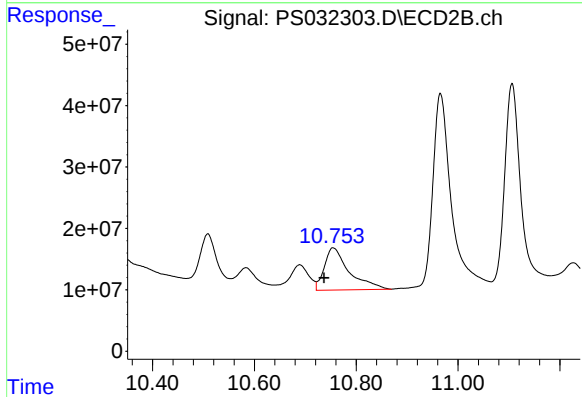


#13 2,4-DB

R.T.: 10.755 min
Delta R.T.: 0.018 min
Response: 232701695
Conc: 61.70 ng/ml

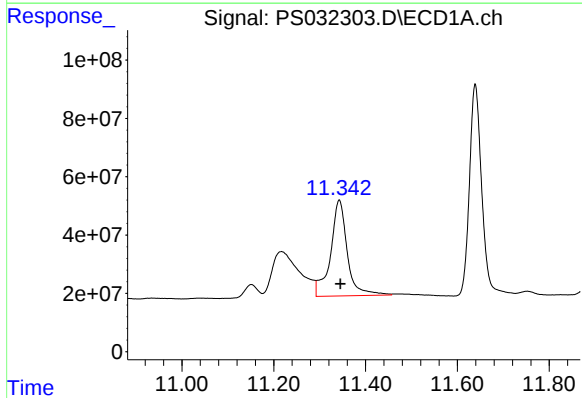


#14 DINOSEB

R.T.: 11.343 min
Delta R.T.: -0.003 min
Response: 833316682
Conc: 40.05 ng/ml

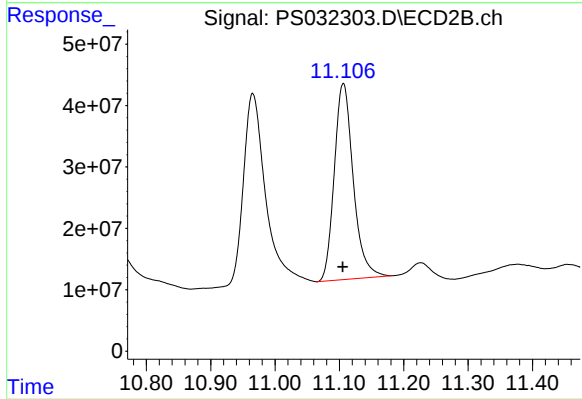

#14 DINOSEB


R.T.: 11.106 min
Delta R.T.: 0.000 min
Response: 653423477
Conc: 36.94 ng/ml

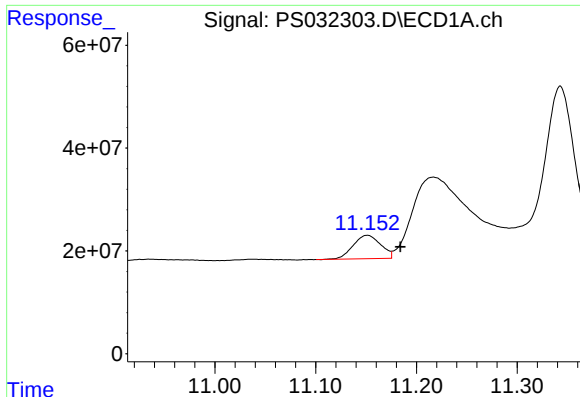

#15 Picloram


R.T.: 11.151 min
Delta R.T.: -0.033 min
Response: 86483339
Conc: 4.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

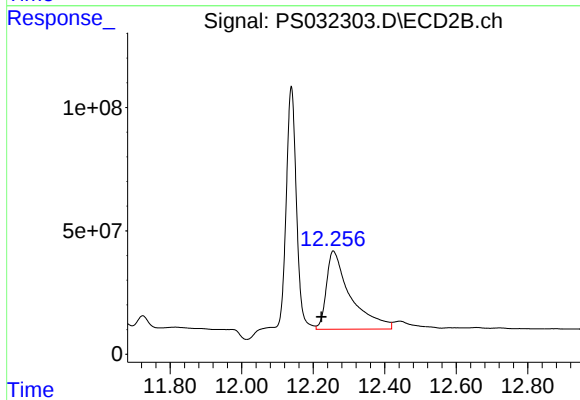


#15 Picloram

R.T.: 12.256 min
Delta R.T.: 0.033 min
Response: 1480760482
Conc: 39.82 ng/ml

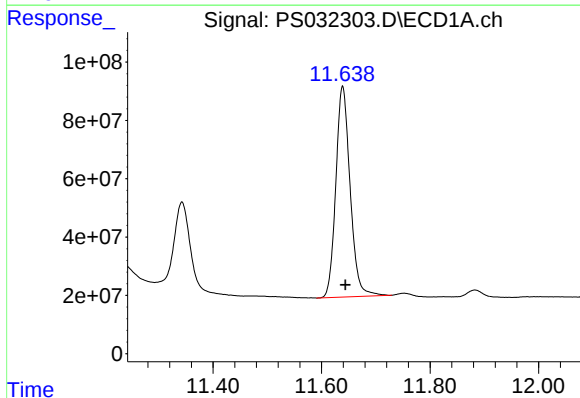

#16 DCPA

R.T.: 11.639 min
Delta R.T.: -0.005 min
Response: 1323594500
Conc: 39.45 ng/ml

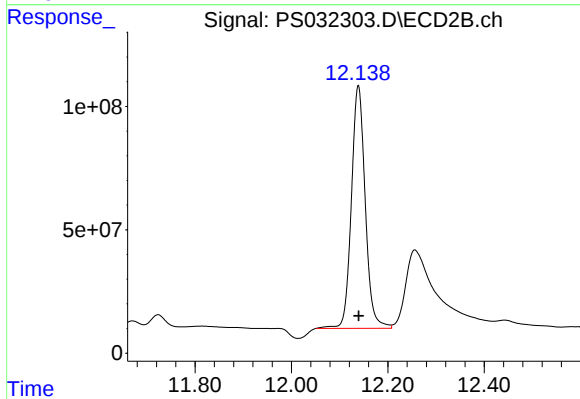

#16 DCPA

R.T.: 12.139 min
Delta R.T.: 0.000 min
Response: 1960642813
Conc: 61.54 ng/ml