

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
 Data File : PS032306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2025 23:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:10:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.620	1719.8E6	1885.8E6	379.538	517.297 #
Target Compounds							
2) T	3,5-DICHL...	6.443	0.000	33106077	0	5.120	N.D. #
6) T	MCPP	7.678f	7.907	-1939017	27111189	N.D.	2.038
7) T	MCPA	7.819f	8.102f	10964149	3648124	<MDL	<MDL #
8) T	DICHLORPROP	8.163	0.000	433449	0	<MDL	N.D. #
9) T	2,4-D	8.451f	0.000	116.1E6	0	25.740	N.D. #
10) T	Pentachlo...	8.708	9.364	10745790	10849304	<MDL	<MDL #
11) T	2,4,5-TP ...	9.296	9.769f	10489184	7615686	<MDL	<MDL #
12) T	2,4,5-T	9.591	10.191	4319808	3072331	<MDL	<MDL #
13) T	2,4-DB	10.106f	0.000	2018677	0	<MDL	N.D. #
14) T	DINOSEB	11.343	11.114	8289411	3602223	<MDL	<MDL #
15) T	Picloram	11.223f	0.000	6302183	0	<MDL	N.D. #
16) T	DCPA	11.645	12.157	6070265	33446007	<MDL	1.050 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110625\
Data File : PS032306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2025 23:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:10:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

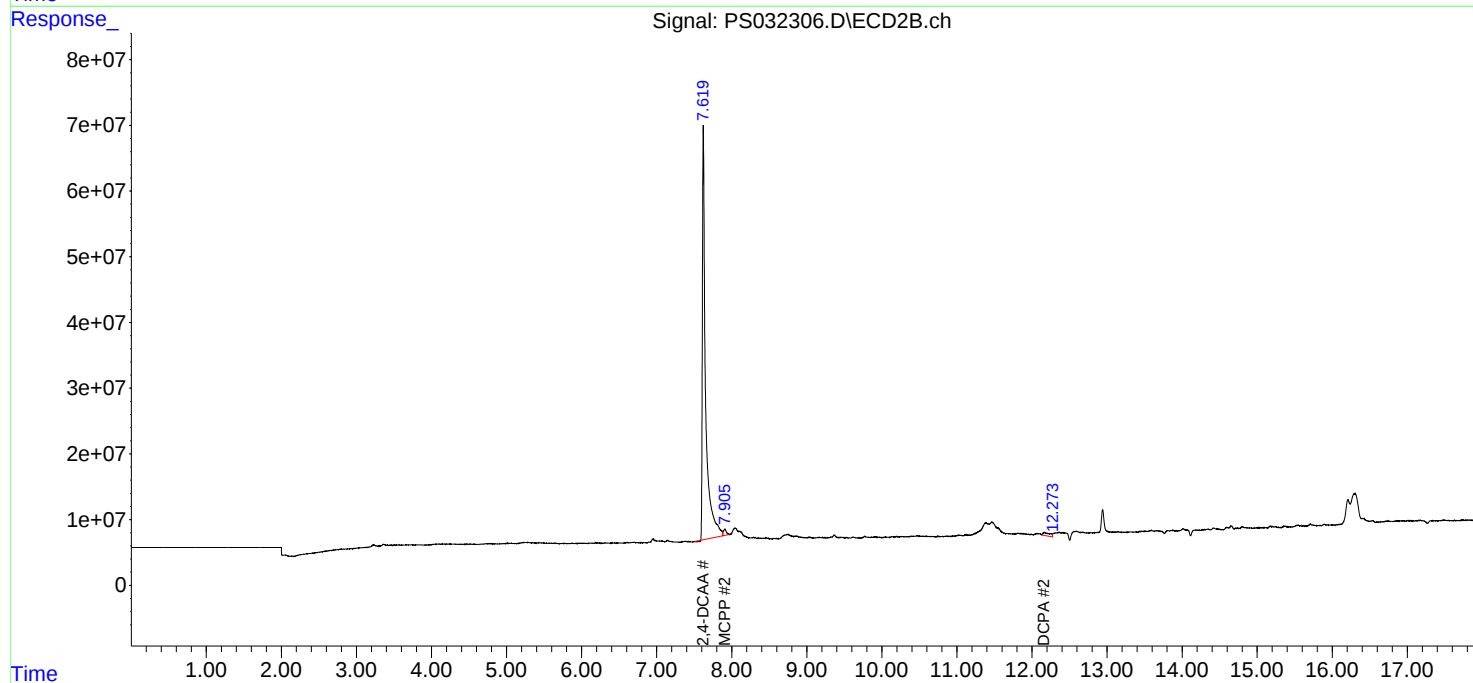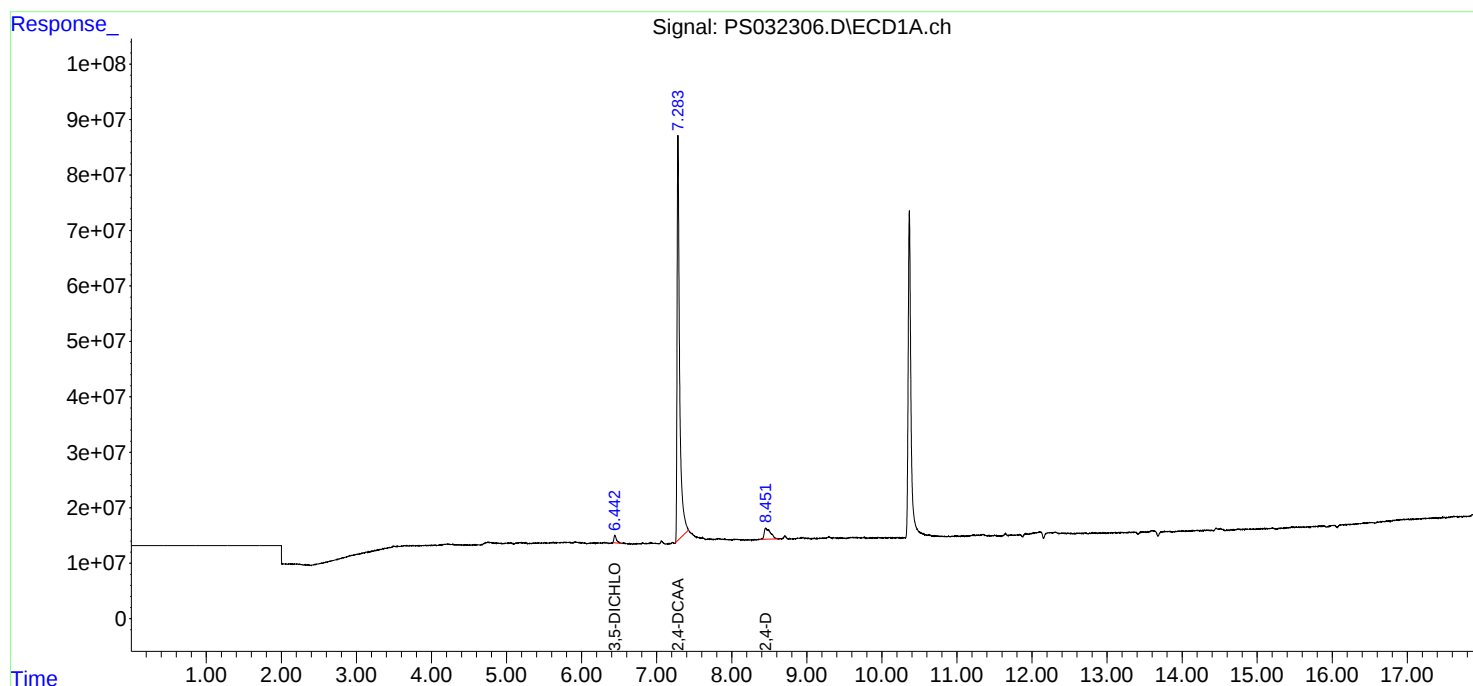


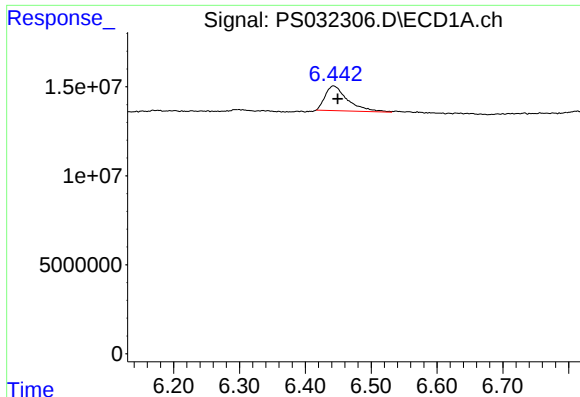

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.443 min
Delta R.T.: -0.007 min
Response: 33106077
Conc: 5.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

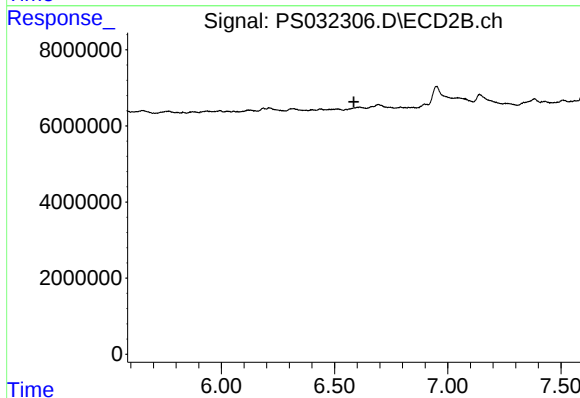


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

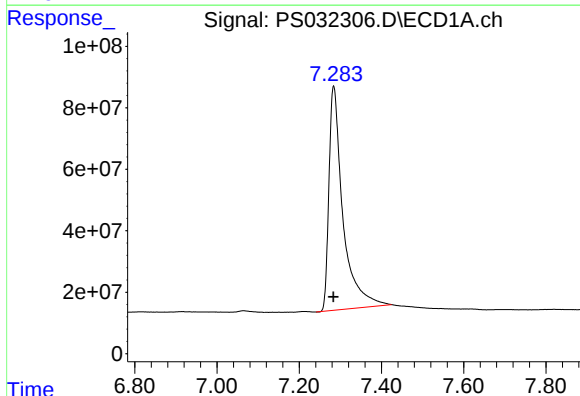


#4 2,4-DCAA

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1719791779
Conc: 379.54 ng/ml

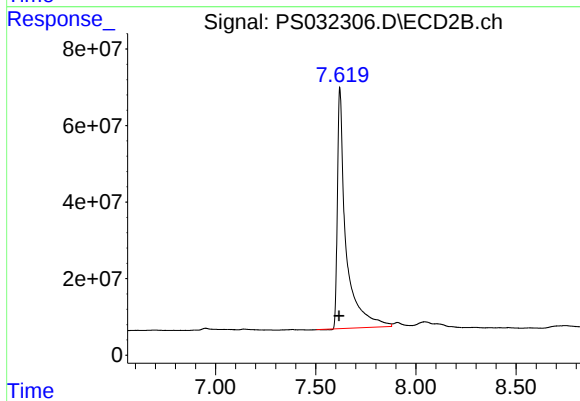

#4 2,4-DCAA


R.T.: 7.620 min
Delta R.T.: 0.003 min
Response: 1885804025
Conc: 517.30 ng/ml

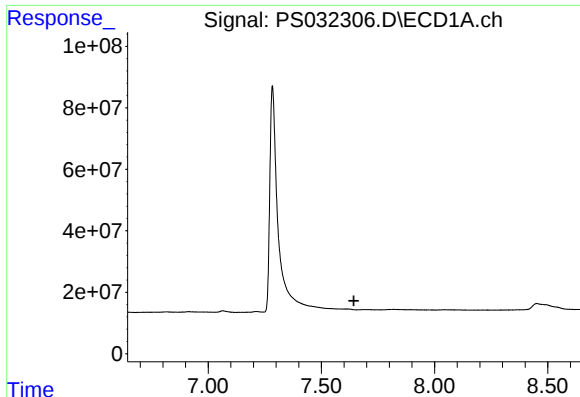

#6 MCP


R.T.: 7.678 min
Delta R.T.: 0.034 min
Response: -1939017
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

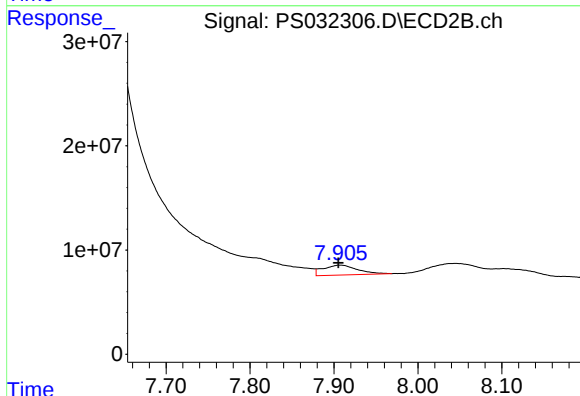


#6 MCP

R.T.: 7.907 min
Delta R.T.: 0.002 min
Response: 27111189
Conc: 2.04 ug/ml

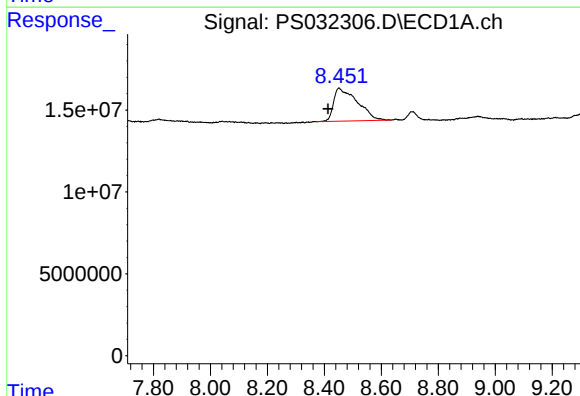


#9 2,4-D

R.T.: 8.451 min
Delta R.T.: 0.038 min
Response: 116134716
Conc: 25.74 ng/ml

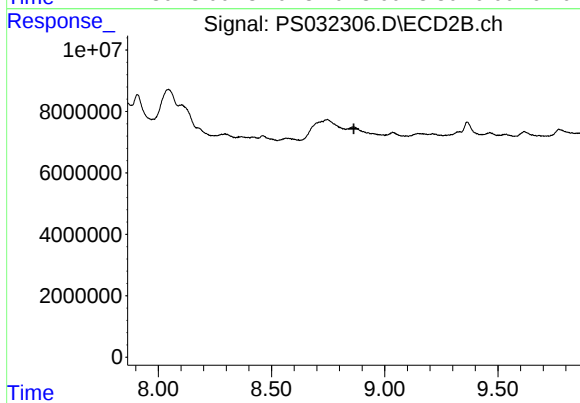

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.864 min
Response: 0
Conc: N.D.

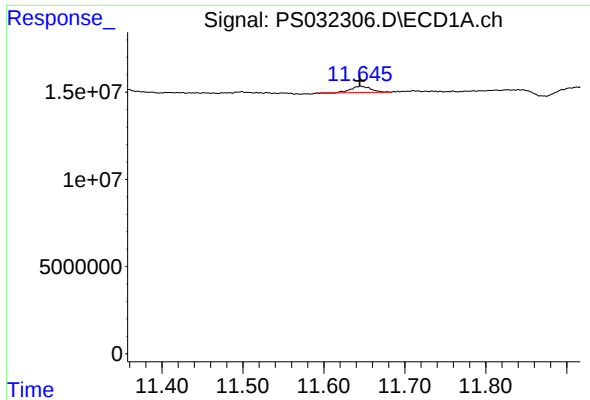

#16 DCPA

R.T.: 11.645 min
Delta R.T.: 0.001 min
Response: 6070265
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

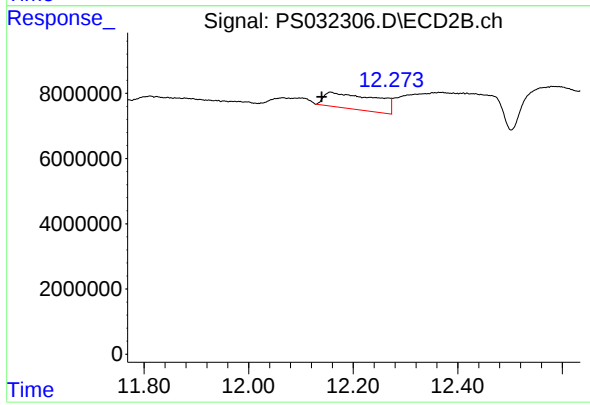

#16 DCPA

R.T.: 12.157 min
Delta R.T.: 0.017 min
Response: 33446007
Conc: 1.05 ng/ml