

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
 Data File : PS002362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 10:27
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 12:51:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.332	0	13669	N.D.	0.030 #
3) T	4-Nitroph...	11.037	0.000	1104737	0	6.622	N.D. #
5) T	DICAMBA	0.000	11.148	0	159594	N.D.	0.128 #
12) T	2,4,5-T	0.000	14.525	0	6227424	N.D.	4.159 #
15) T	Picloram	16.939	16.782	12650451	497788	5.304	0.220 #
16) T	DCPA	0.000	16.834	0	17174923	N.D.	7.253 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
Data File : PS002362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 10:27
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 12:51:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

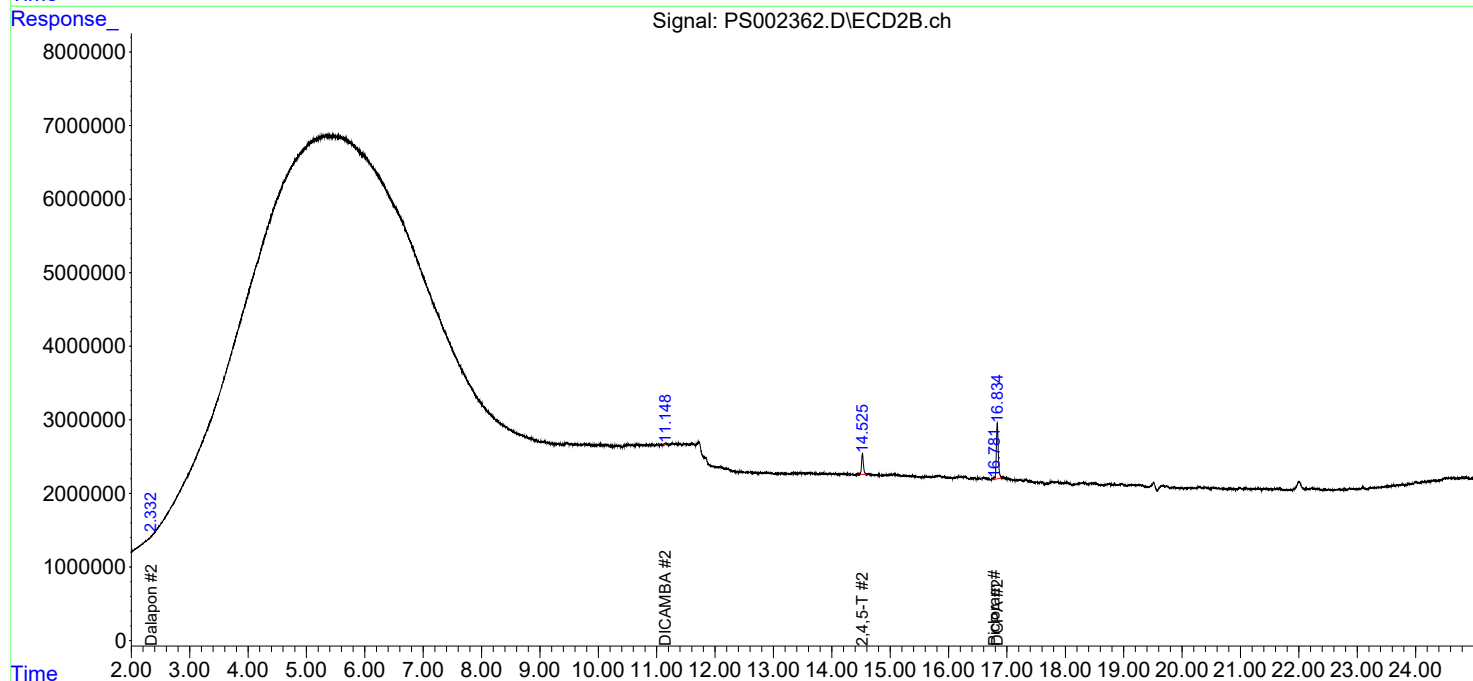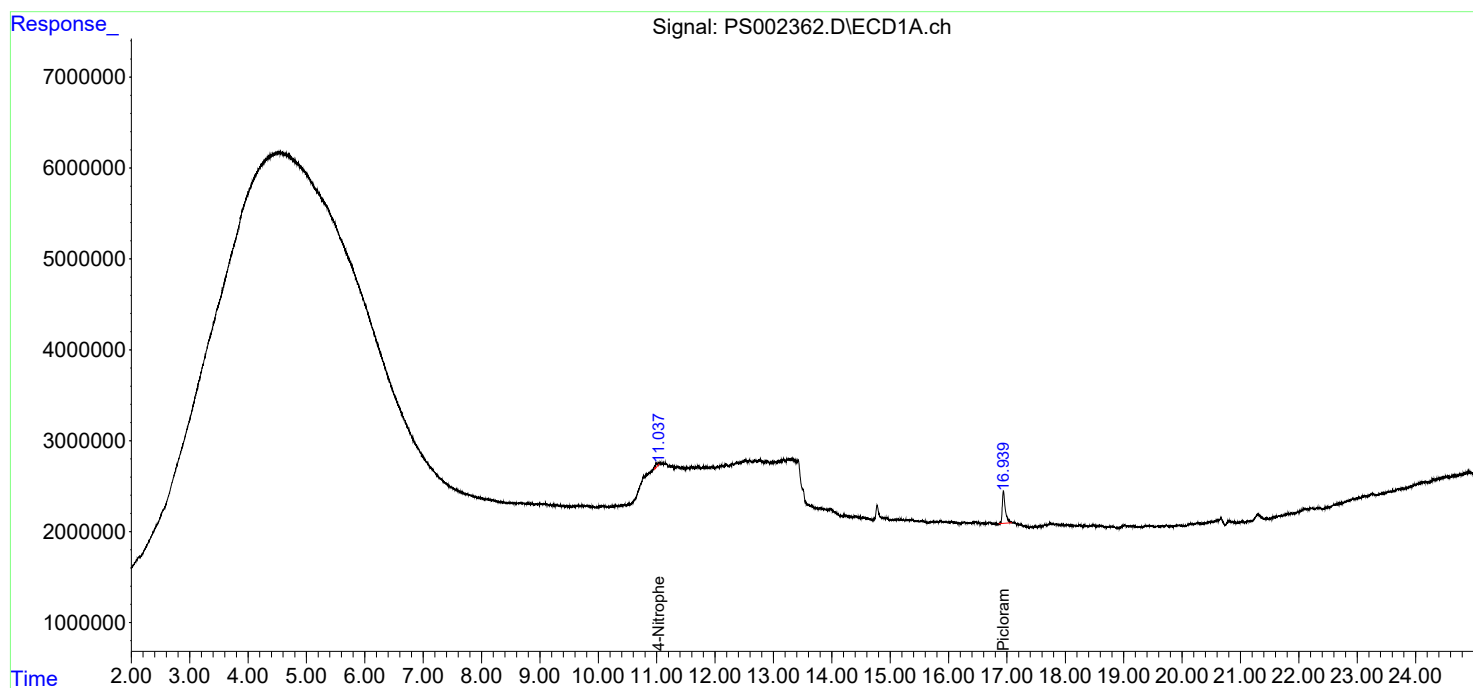


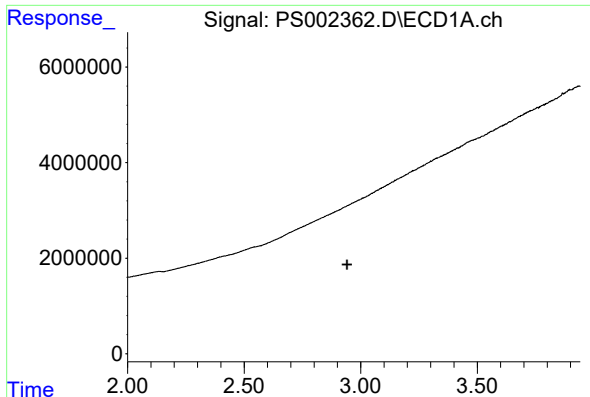

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

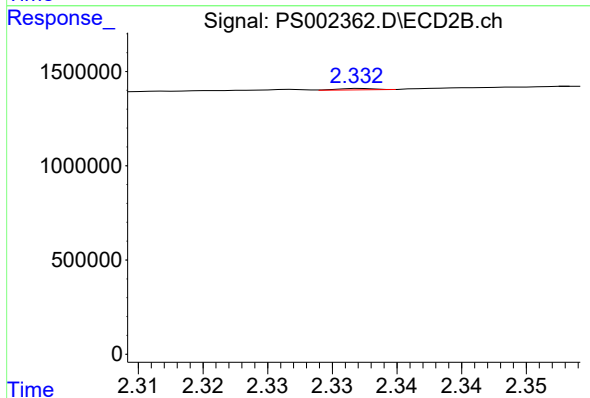


#1 Dalapon

R.T.: 2.332 min
Delta R.T.: -0.041 min
Response: 13669
Conc: 0.03 ng/ml

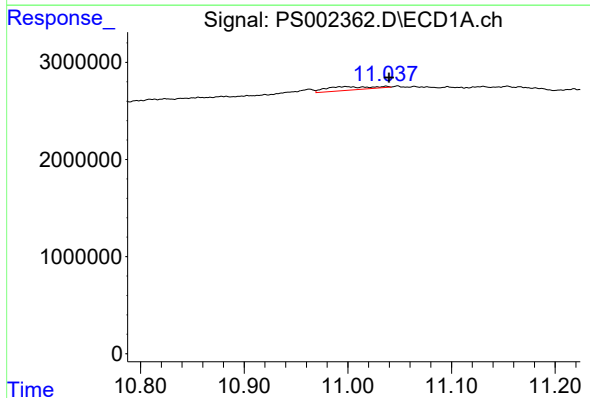


#3 4-Nitrophenol

R.T.: 11.037 min
Delta R.T.: -0.003 min
Response: 1104737
Conc: 6.62 ng/ml

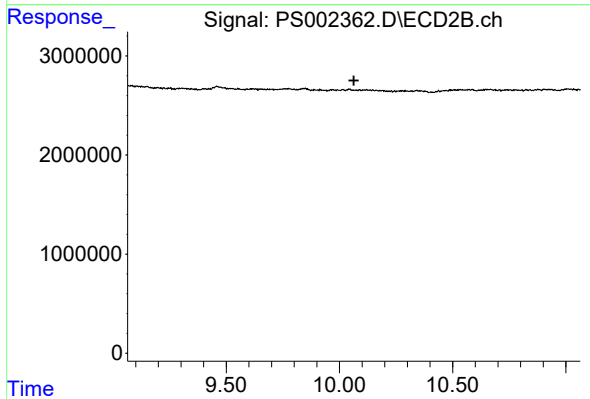

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

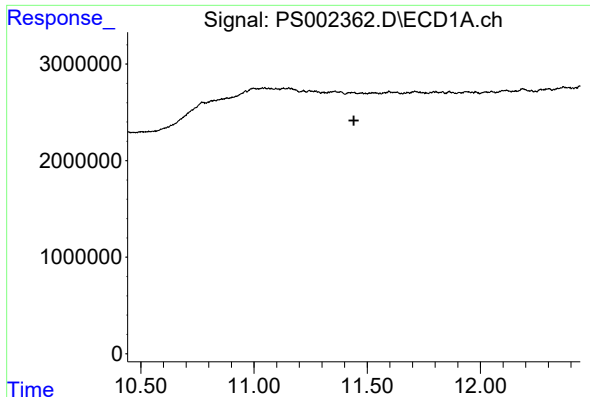

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

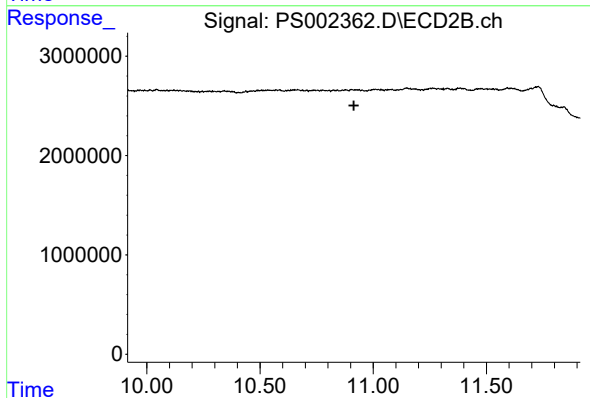


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 10.914 min
Response: 0
Conc: N.D.

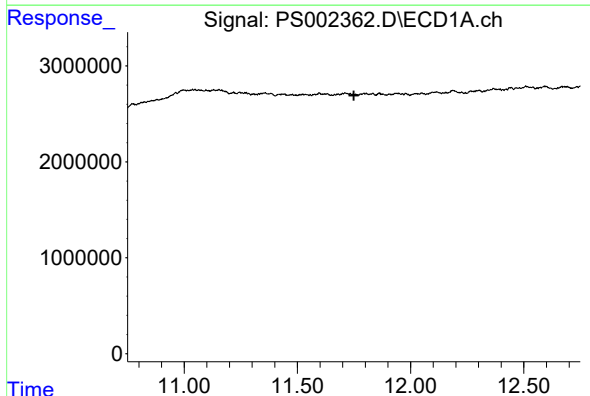


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.750 min
Response: 0
Conc: N.D.

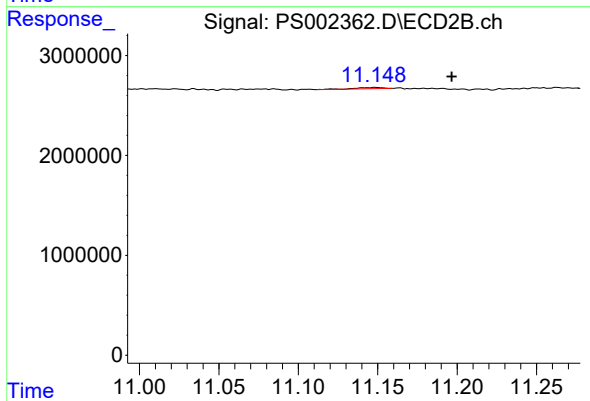

#5 DICAMBA


R.T.: 11.148 min
Delta R.T.: -0.048 min
Response: 159594
Conc: 0.13 ng/ml

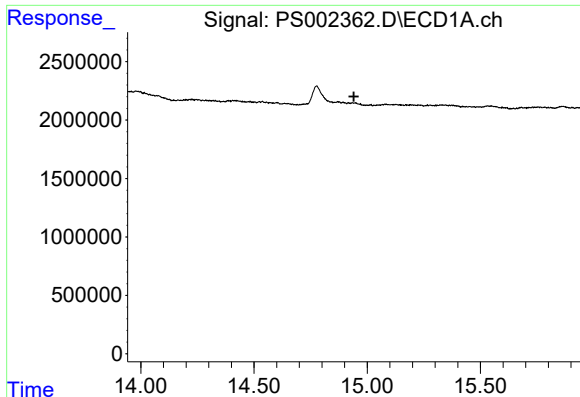

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

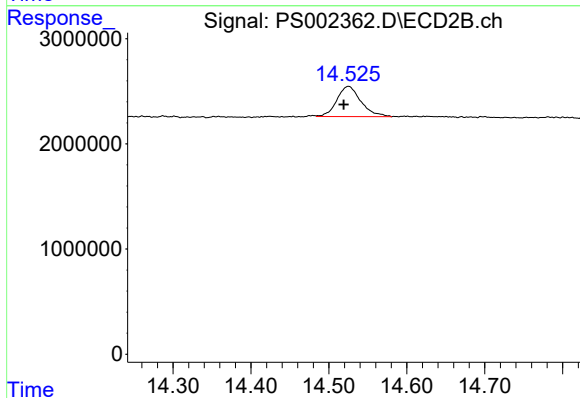


#12 2,4,5-T

R.T.: 14.525 min
Delta R.T.: 0.006 min
Response: 6227424
Conc: 4.16 ng/ml

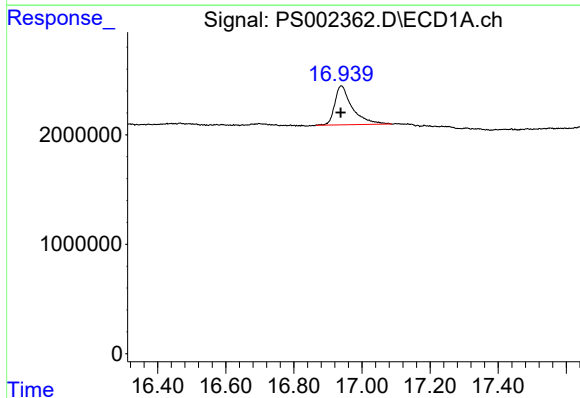


#15 Picloram

R.T.: 16.939 min
Delta R.T.: 0.002 min
Response: 12650451
Conc: 5.30 ng/ml

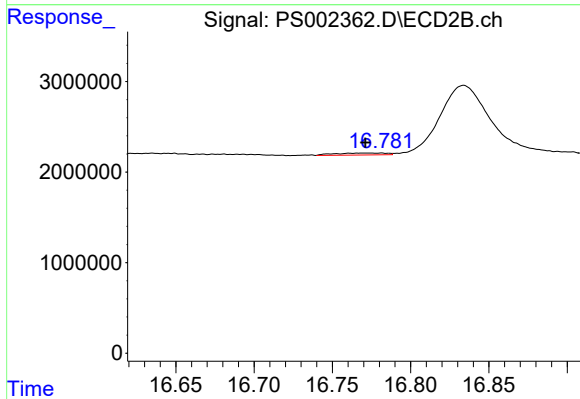

#15 Picloram


R.T.: 16.782 min
Delta R.T.: 0.010 min
Response: 497788
Conc: 0.22 ng/ml

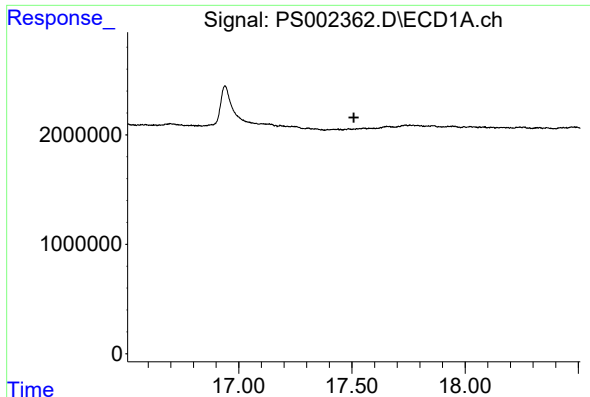

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

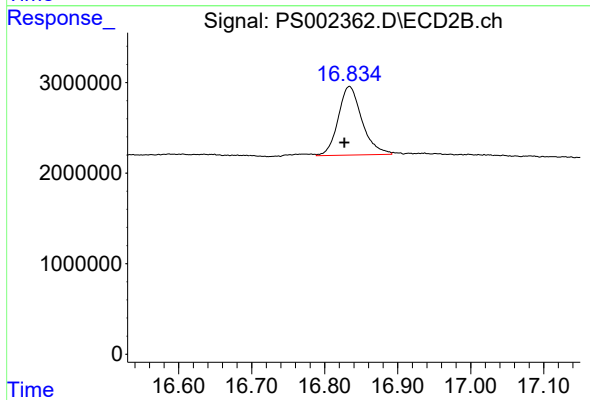

#16 DCPA

R.T.: 16.834 min
Delta R.T.: 0.007 min
Response: 17174923
Conc: 7.25 ng/ml