

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
 Data File : PS002363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 10:58
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 12:51:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.409	10.900	149.5E6	147.9E6	474.984	411.816
Target Compounds							
7) T	MCPA	0.000	11.797	0	3156219	N.D.	2.332 #
12) T	2,4,5-T	0.000	14.520	0	2746976	N.D.	1.834 #
15) T	Picloram	16.936	16.826	5317493	9848019	2.229	4.353 #
16) T	DCPA	0.000	16.826	0	9848019	N.D.	4.159 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
Data File : PS002363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 10:58
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 12:51:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

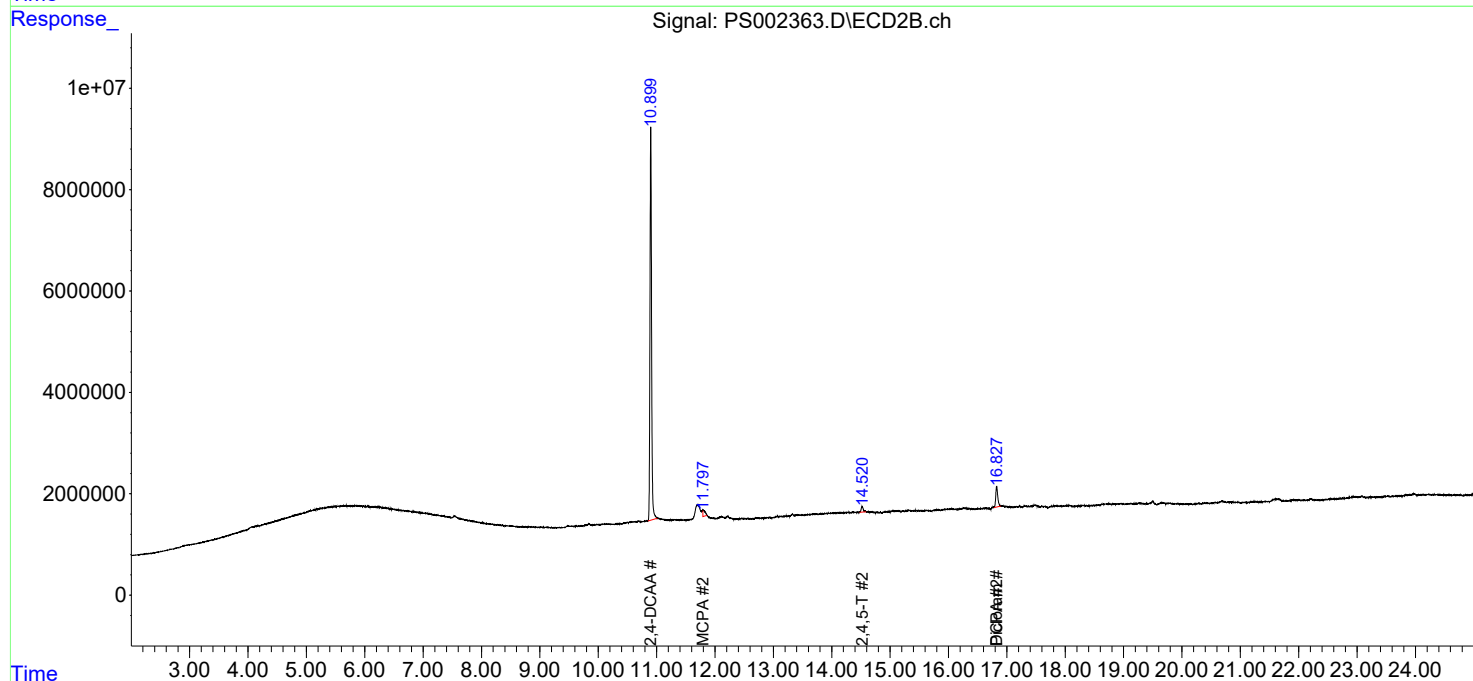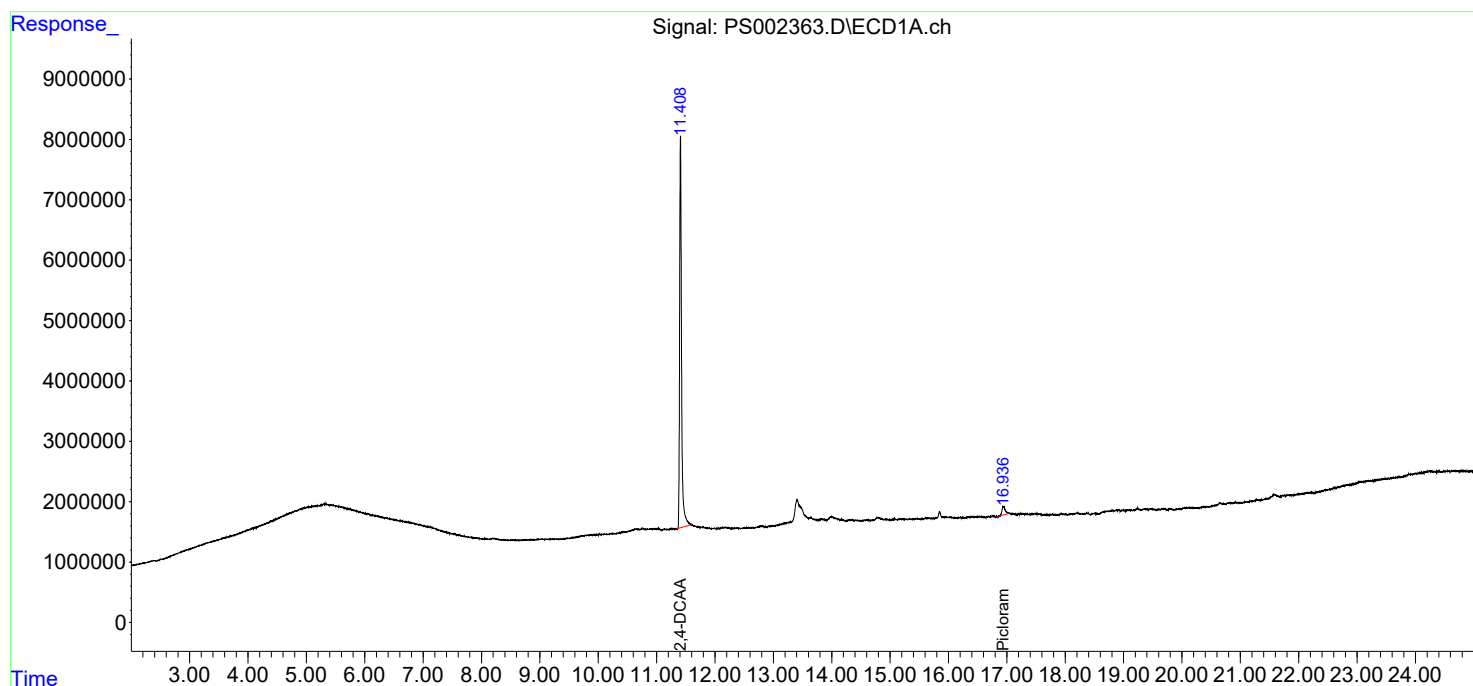


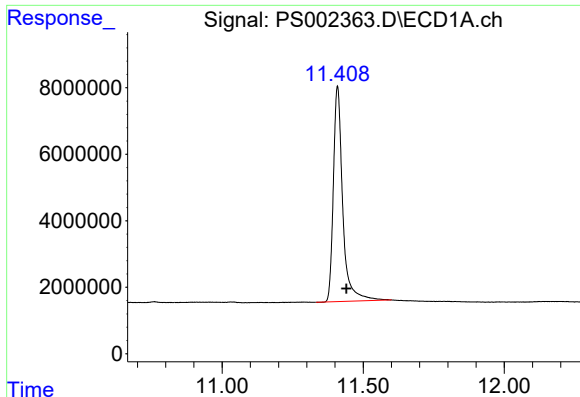

#4 2,4-DCAA


R.T.: 11.409 min
Delta R.T.: -0.032 min
Response: 149470707
Conc: 474.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

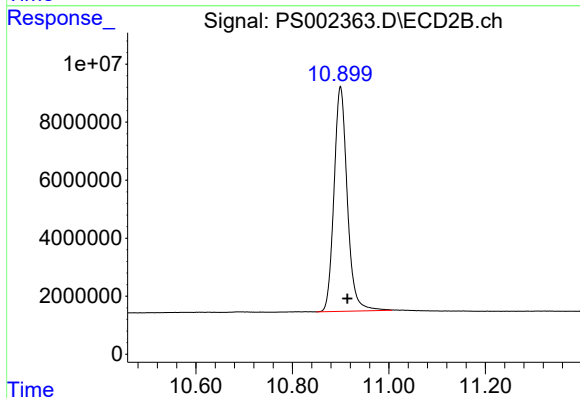


#4 2,4-DCAA

R.T.: 10.900 min
Delta R.T.: -0.015 min
Response: 147882416
Conc: 411.82 ng/ml

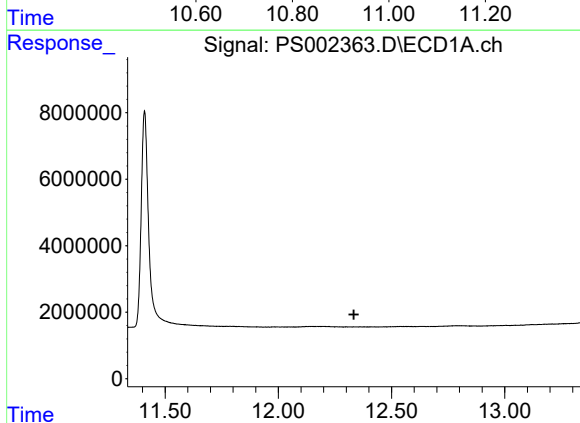


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

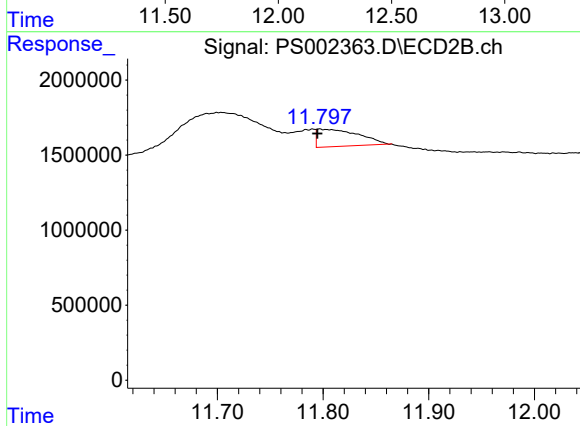

#7 MCPA


R.T.: 11.797 min
Delta R.T.: 0.002 min
Response: 3156219
Conc: 2.33 ug/ml

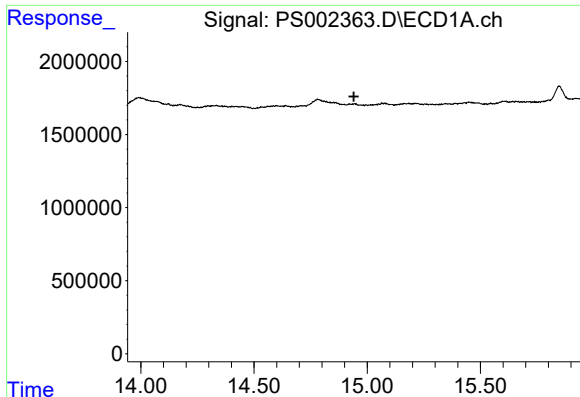

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

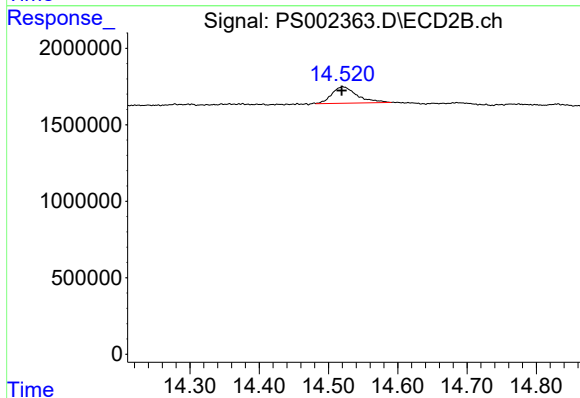


#12 2,4,5-T

R.T.: 14.520 min
Delta R.T.: 0.001 min
Response: 2746976
Conc: 1.83 ng/ml

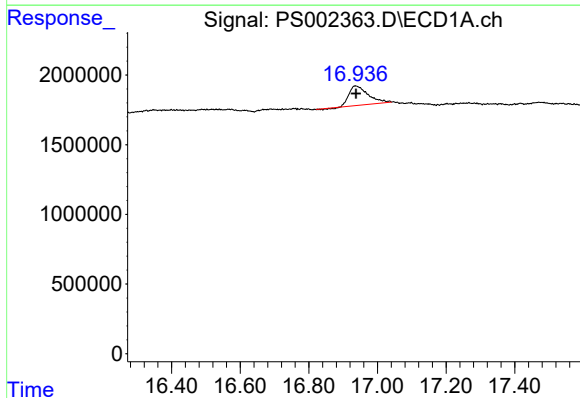


#15 Picloram

R.T.: 16.936 min
Delta R.T.: -0.002 min
Response: 5317493
Conc: 2.23 ng/ml

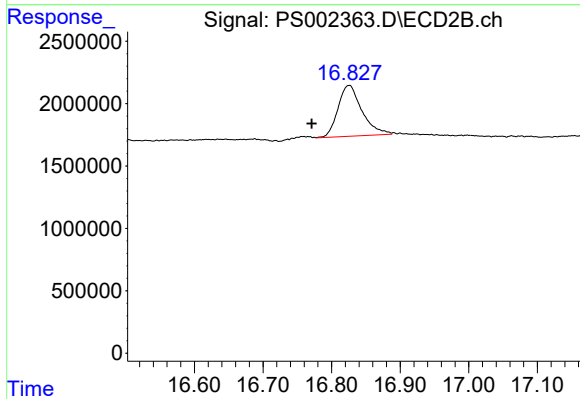

#15 Picloram


R.T.: 16.826 min
Delta R.T.: 0.055 min
Response: 9848019
Conc: 4.35 ng/ml

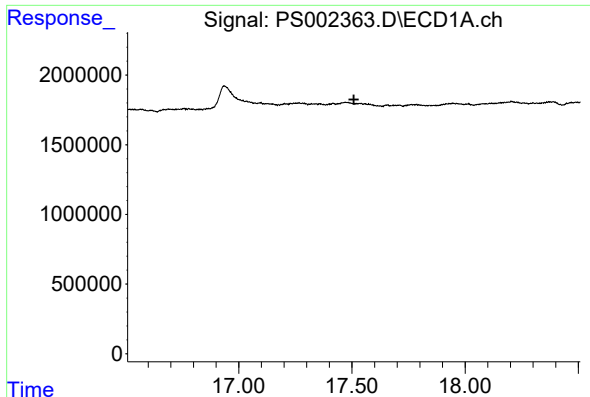

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

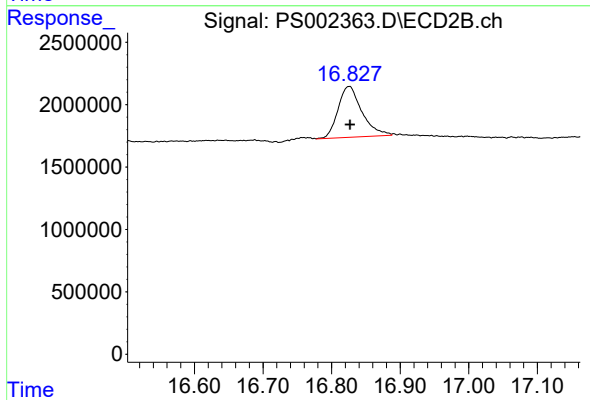

#16 DCPA

R.T.: 16.826 min
Delta R.T.: 0.000 min
Response: 9848019
Conc: 4.16 ng/ml