

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
 Data File : PS002366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 12:53
 Operator : EI\SJ
 Sample : J5816-12RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 13:21:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.467	10.959	83360496	72468292	264.901	201.806
Target Compounds							
1) T	Dalapon	2.944	2.401	8138873	11230802	17.745	24.874 #
2) T	3,5-DICHL...	0.000	9.054	0	10519586	N.D.	23.717 #
5) T	DICAMBA	0.000	11.199	0	23713860	N.D.	18.976 #
6) T	MCP	12.052	0.000	1845042	0	1.868	N.D. #
7) T	MCPA	0.000	11.754	0	11650646	N.D.	8.608 #
8) T	DICHLORPROP	0.000	12.260	0	19505749	N.D.	60.740 #
9) T	2,4-D	0.000	12.790	0	293778	N.D.	0.690 #
11) T	2,4,5-TP ...	0.000	13.965	0	162916	N.D.	0.089 #
12) T	2,4,5-T	0.000	14.570	0	5892772	N.D.	3.935 #
15) T	Picloram	16.969	16.719	24900229	199662	10.439	0.088 #
16) T	DCPA	0.000	16.876	0	27525578	N.D.	11.625 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
Data File : PS002366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 12:53
Operator : EI\SJ
Sample : J5816-12RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 13:21:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

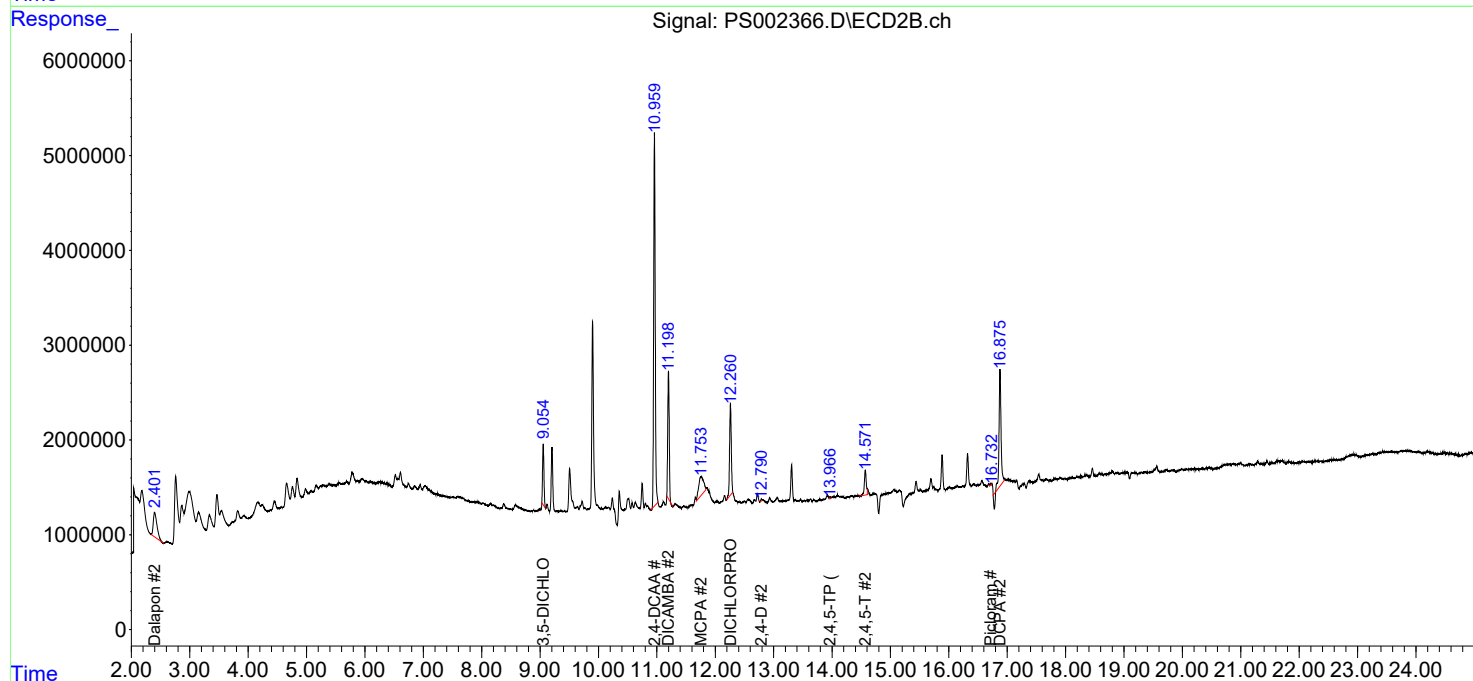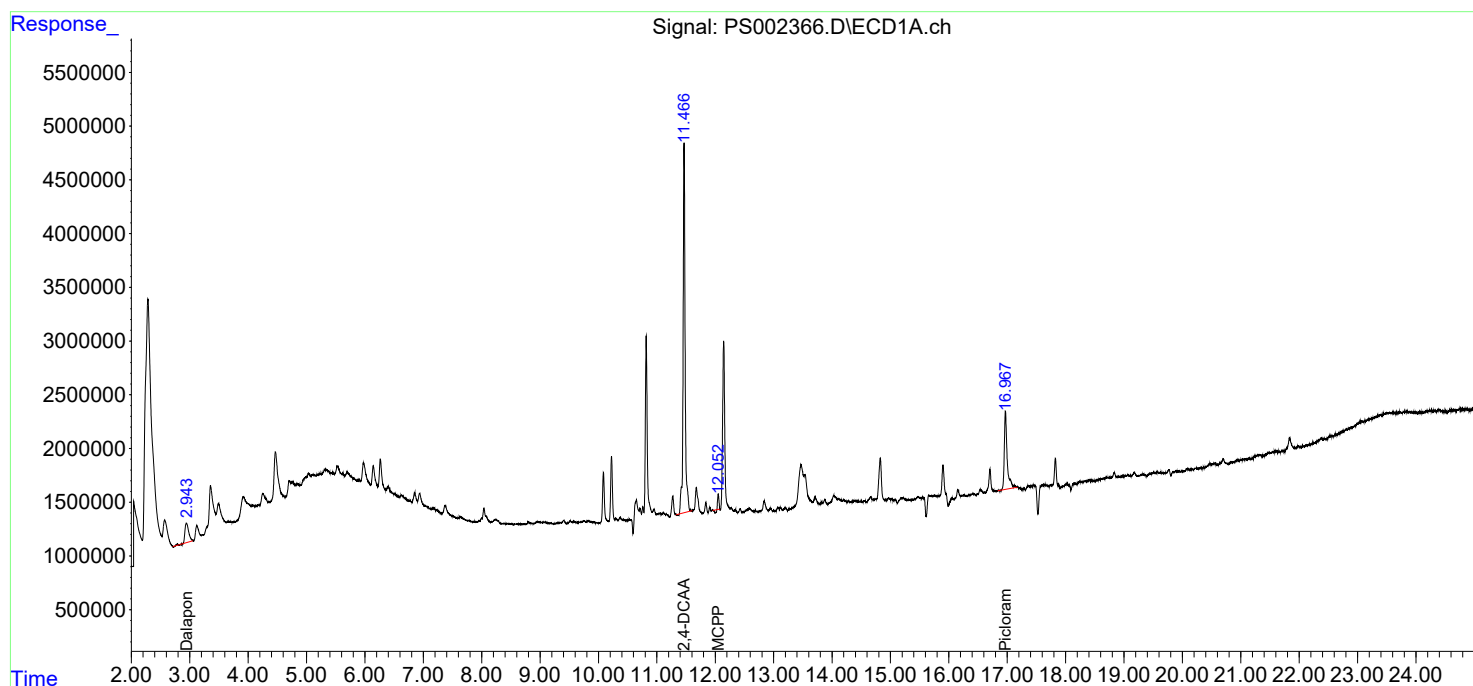


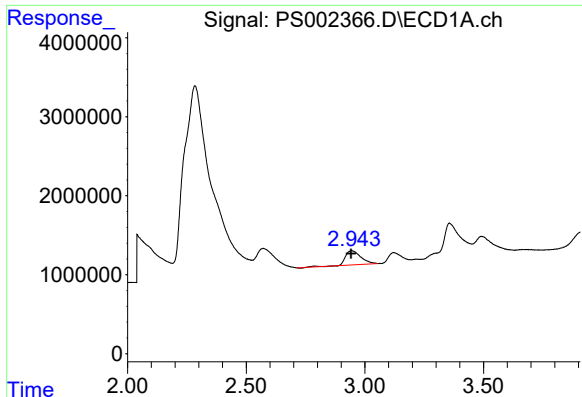

#1 Dalapon


R.T.: 2.944 min
Delta R.T.: 0.002 min
Response: 8138873
Conc: 17.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

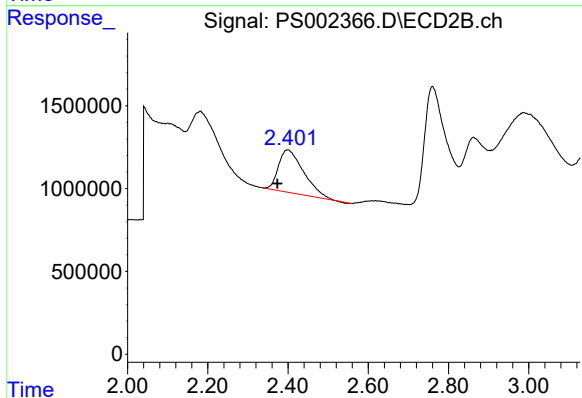


#1 Dalapon

R.T.: 2.401 min
Delta R.T.: 0.028 min
Response: 11230802
Conc: 24.87 ng/ml

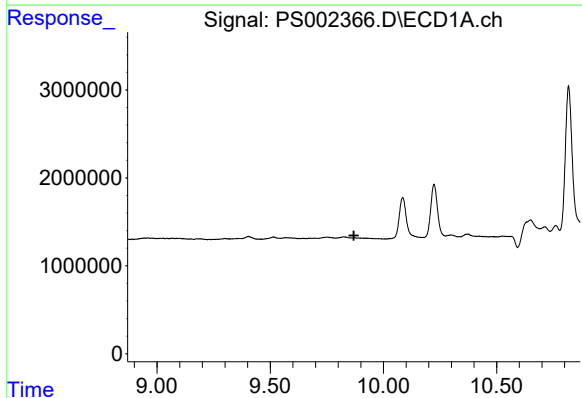


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

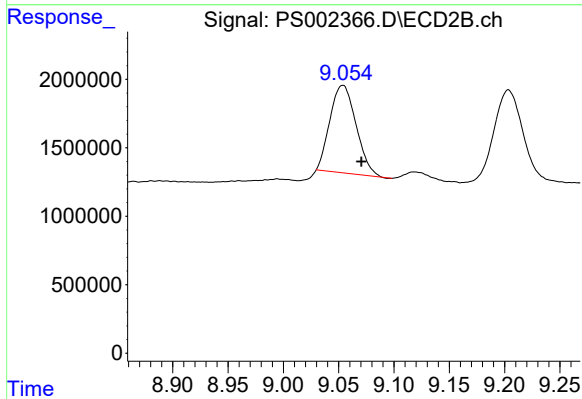

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.054 min
Delta R.T.: -0.016 min
Response: 10519586
Conc: 23.72 ng/ml

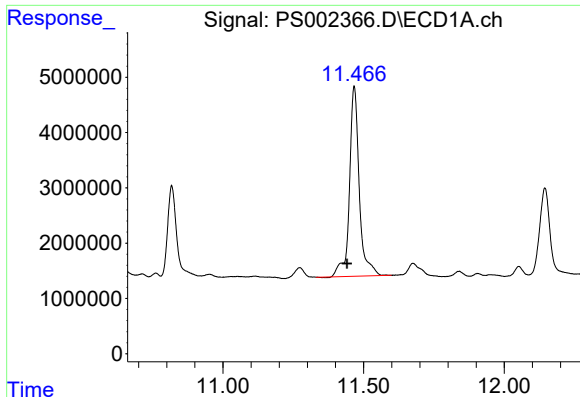

#4 2,4-DCAA


R.T.: 11.467 min
Delta R.T.: 0.026 min
Response: 83360496
Conc: 264.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

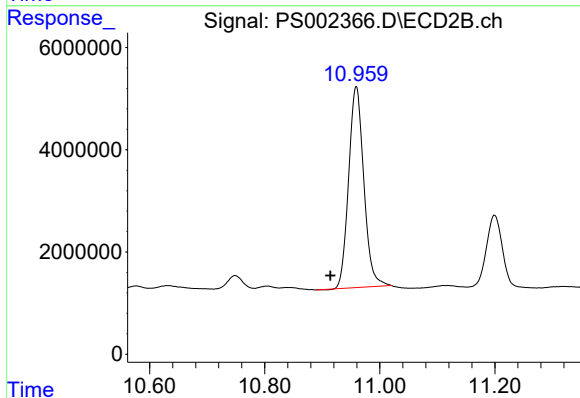


#4 2,4-DCAA

R.T.: 10.959 min
Delta R.T.: 0.045 min
Response: 72468292
Conc: 201.81 ng/ml

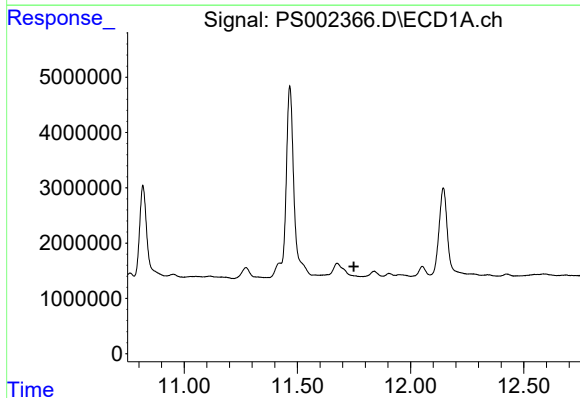


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.750 min
Response: 0
Conc: N.D.

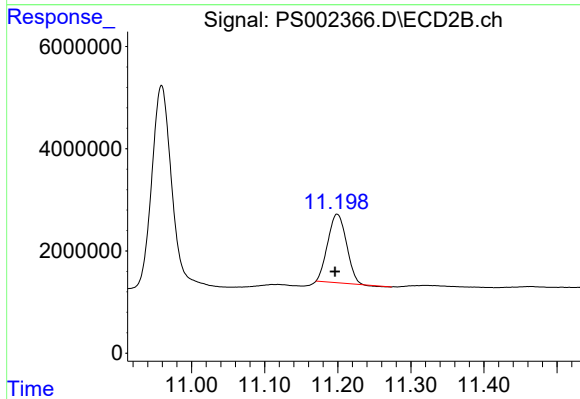

#5 DICAMBA


R.T.: 11.199 min
Delta R.T.: 0.003 min
Response: 23713860
Conc: 18.98 ng/ml

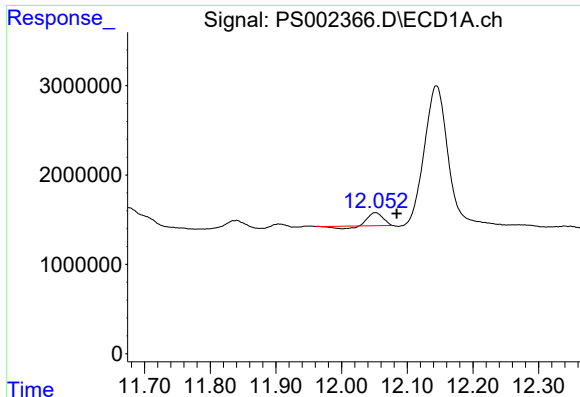

#6 MCPP


R.T.: 12.052 min
Delta R.T.: -0.032 min
Response: 1845042
Conc: 1.87 ug/ml

Instrument :
ECD_S
ClientSampleId :

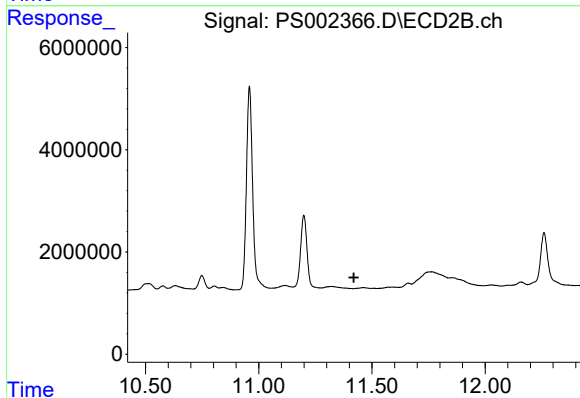


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

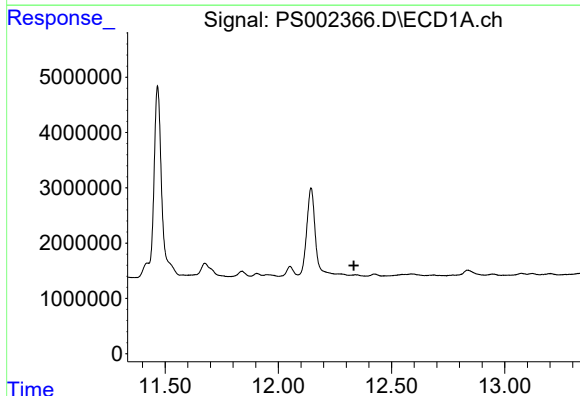


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

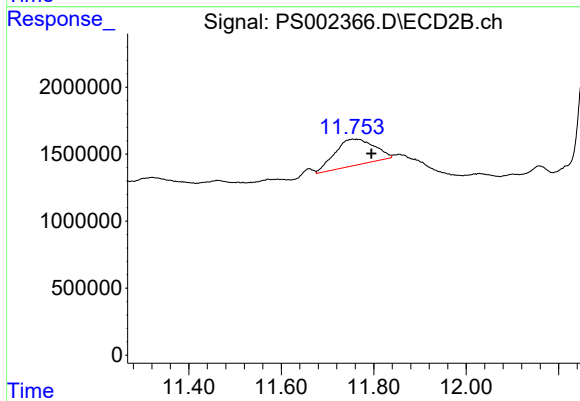

#7 MCPA


R.T.: 11.754 min
Delta R.T.: -0.041 min
Response: 11650646
Conc: 8.61 ug/ml

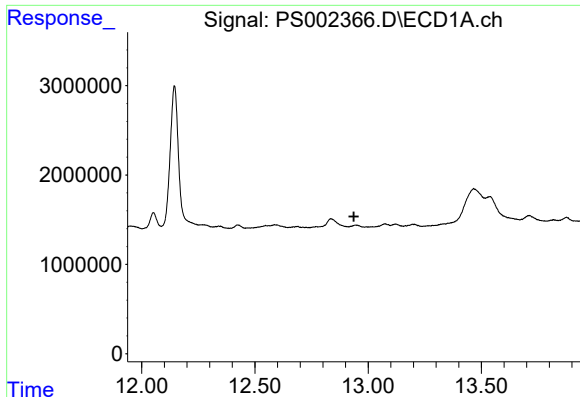

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

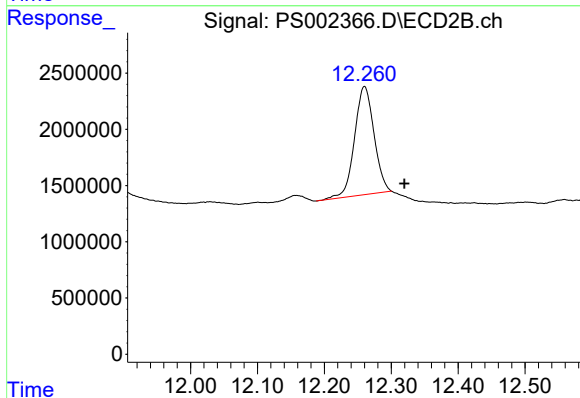


#8 DICHLORPROP

R.T.: 12.260 min
Delta R.T.: -0.059 min
Response: 19505749
Conc: 60.74 ng/ml

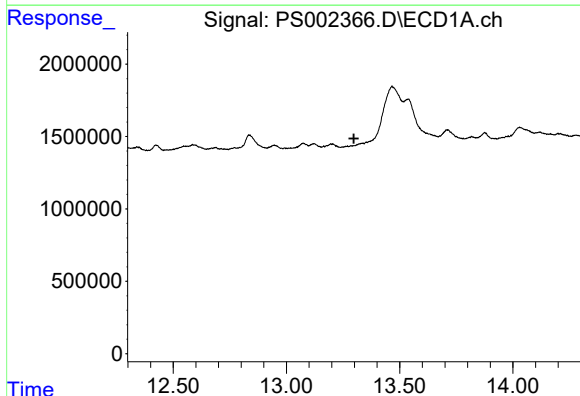


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

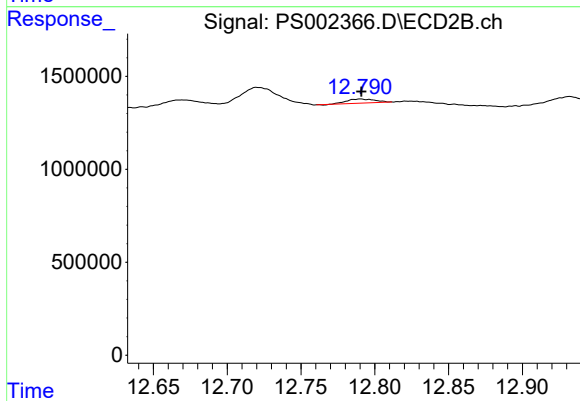

#9 2,4-D


R.T.: 12.790 min
Delta R.T.: 0.000 min
Response: 293778
Conc: 0.69 ng/ml

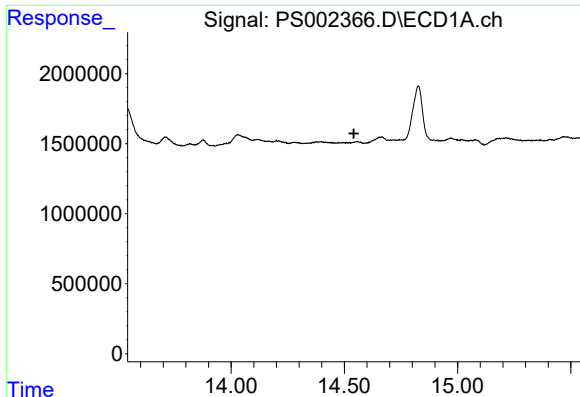

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

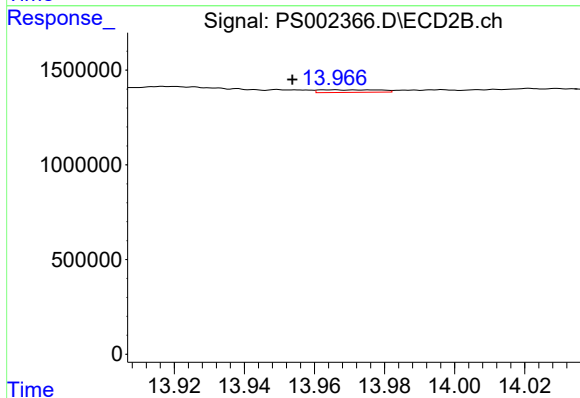


#11 2,4,5-TP (SILVEX)

R.T.: 13.965 min
Delta R.T.: 0.012 min
Response: 162916
Conc: 0.09 ng/ml

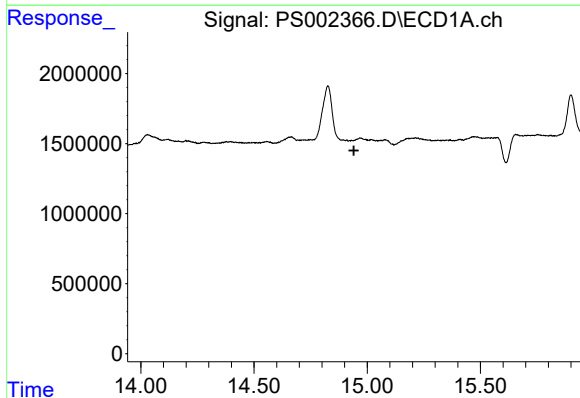


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

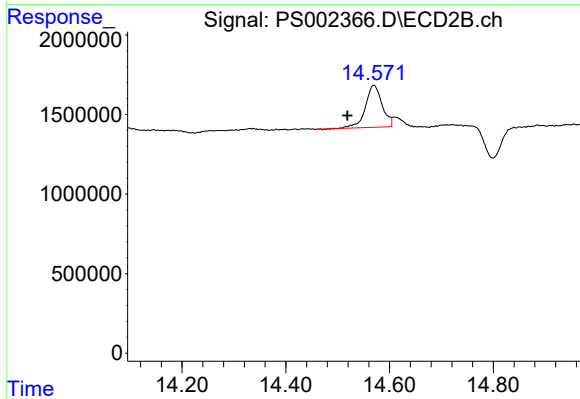

#12 2,4,5-T


R.T.: 14.570 min
Delta R.T.: 0.051 min
Response: 5892772
Conc: 3.94 ng/ml

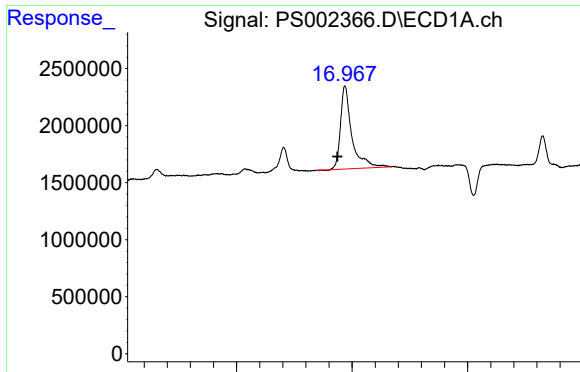

#15 Picloram


R.T.: 16.969 min
Delta R.T.: 0.032 min
Response: 24900229
Conc: 10.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

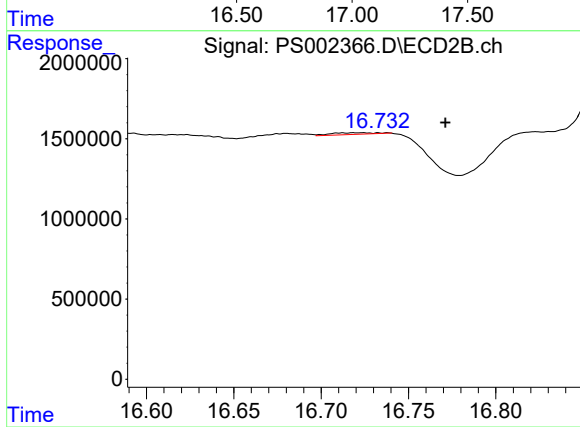


#15 Picloram

R.T.: 16.719 min
Delta R.T.: -0.052 min
Response: 199662
Conc: 0.09 ng/ml

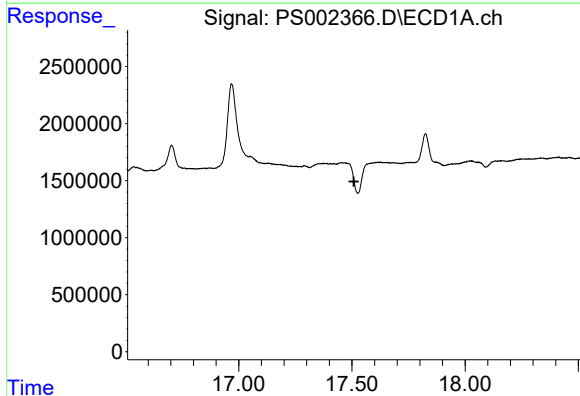

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

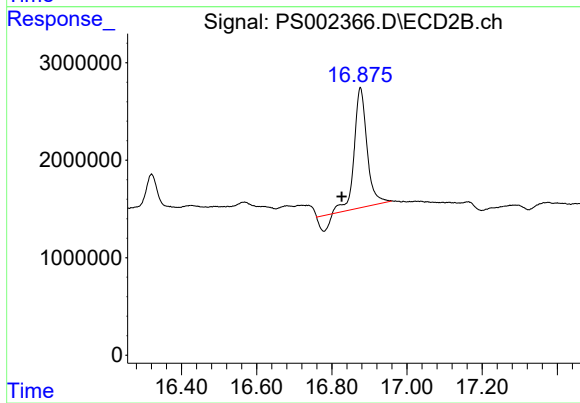

#16 DCPA

R.T.: 16.876 min
Delta R.T.: 0.049 min
Response: 27525578
Conc: 11.62 ng/ml