

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
 Data File : PS002368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 17:03
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 10:35:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.423	10.915	211.1E6	282.0E6	670.894	785.316
Target Compounds							
1) T	Dalapon	2.947	2.388	313.0E6	306.7E6	682.305	679.171
2) T	3,5-DICHL...	0.000	9.070	0	322.5E6	N.D.	727.074 #
3) T	4-Nitroph...	11.016	10.061	119.2E6	121.3E6	714.394	680.246
5) T	DICAMBA	11.732	11.197	977.3E6	824.7E6	735.889	659.955
6) T	MCPD	0.000	11.428	0	66765468	N.D.	77.604 #
7) T	MCPA	0.000	11.804	0	106.3E6	N.D.	78.563 #
8) T	DICHLORPROP	12.919	12.321	251.8E6	128.8E6	722.898	401.224 #
9) T	2,4-D	13.276	12.792	53670715	299.0E6	133.380	702.066 #
10) T	Pentachlo...	13.655	13.337	3575.3E6	3662.7E6	743.204	779.716
11) T	2,4,5-TP ...	0.000	13.955	0	1514.6E6	N.D.	827.828 #
12) T	2,4,5-T	14.920	14.520	1263.1E6	1088.6E6	704.771	726.967
13) T	2,4-DB	15.666	15.170	-60507129	161.2E6	N.D.	727.706
14) T	DINOSEB	17.145	15.597	988.4E6	1032.3E6	721.449	815.501
15) T	Picloram	16.912	16.775	1408.3E6	1866.8E6	590.403	825.218 #
16) T	DCPA	0.000	16.828	0	1504.1E6	N.D.	635.228 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110718\
Data File : PS002368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 17:03
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 10:35:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

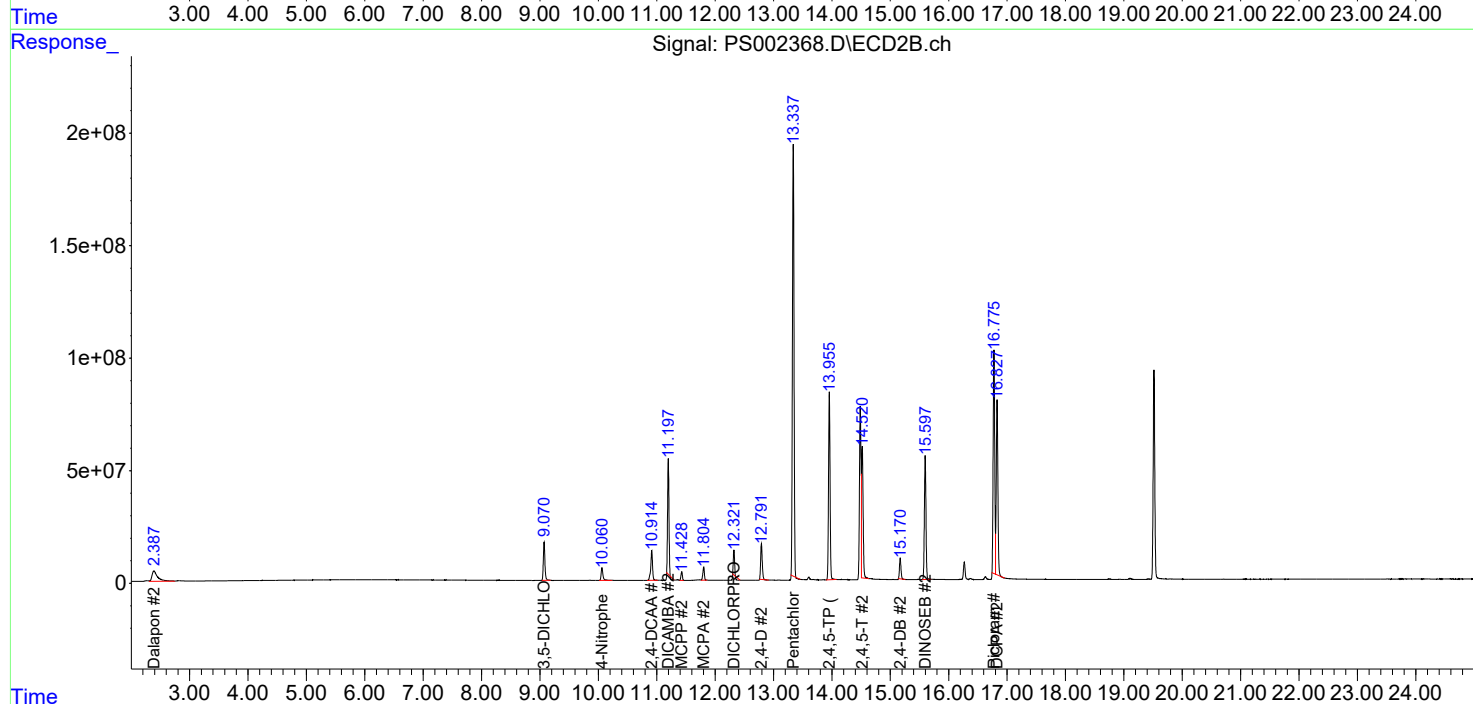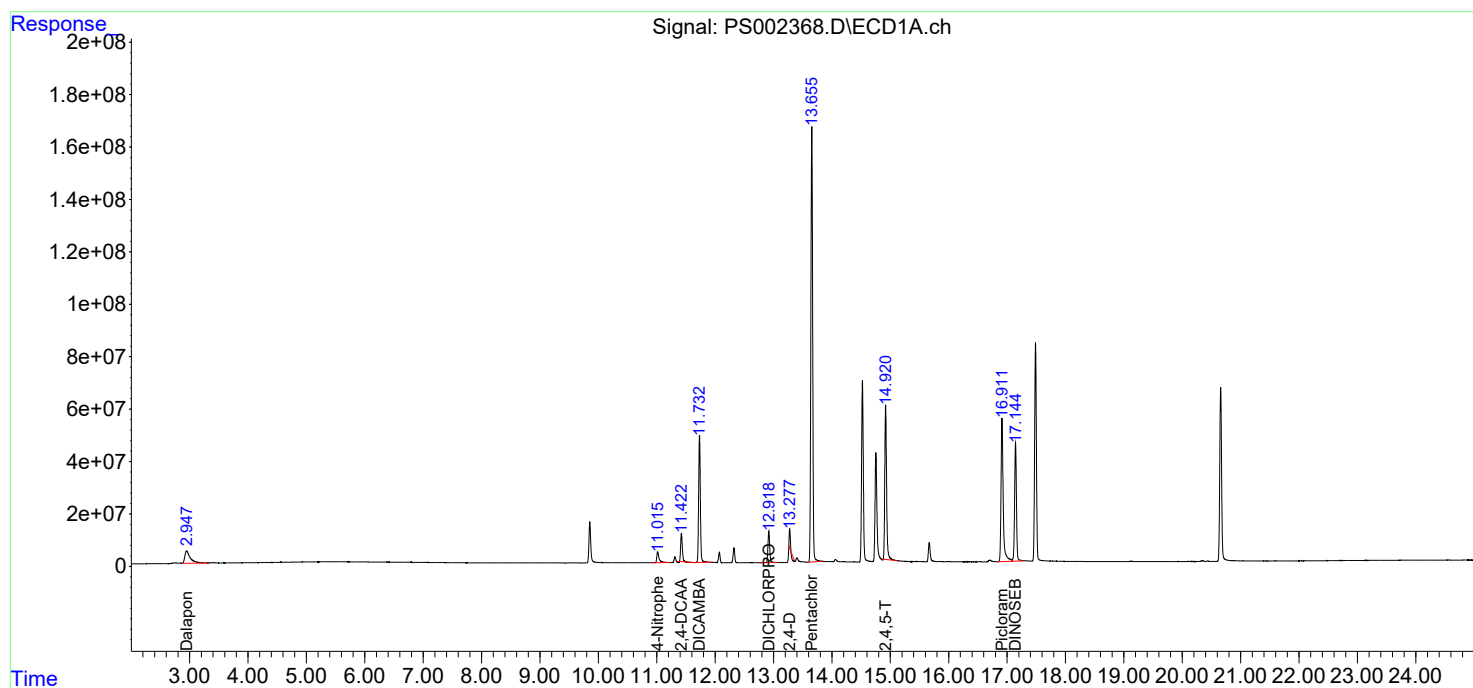


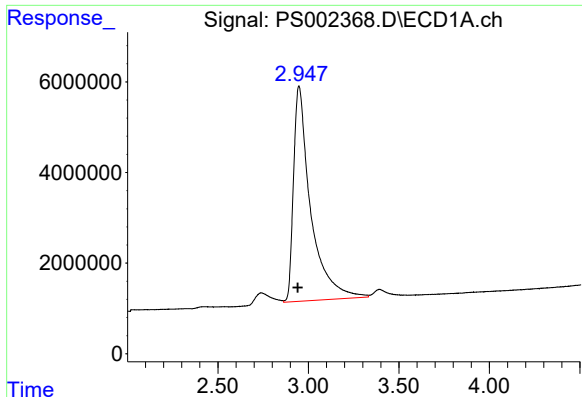

#1 Dalapon


R.T.: 2.947 min
Delta R.T.: 0.005 min
Response: 312950650
Conc: 682.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

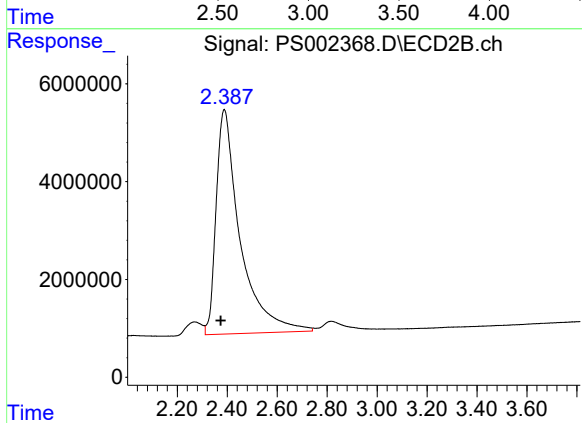


#1 Dalapon

R.T.: 2.388 min
Delta R.T.: 0.014 min
Response: 306650296
Conc: 679.17 ng/ml

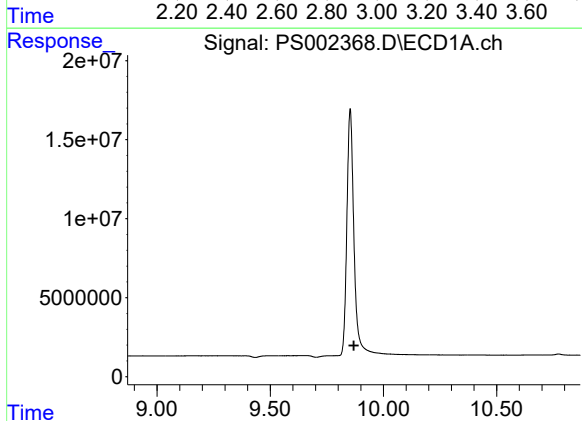


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

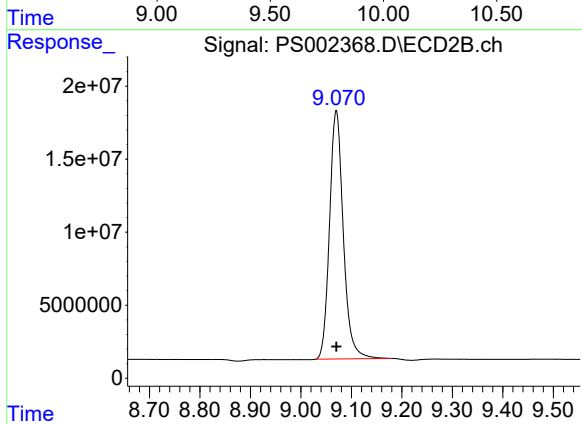

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.070 min
Delta R.T.: 0.000 min
Response: 322497300
Conc: 727.07 ng/ml

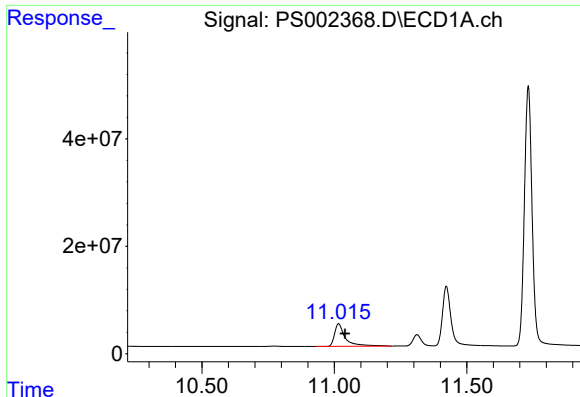

#3 4-Nitrophenol


R.T.: 11.016 min
Delta R.T.: -0.024 min
Response: 119181648
Conc: 714.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

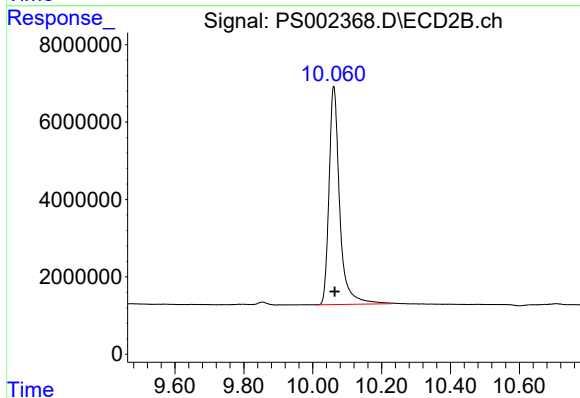


#3 4-Nitrophenol

R.T.: 10.061 min
Delta R.T.: -0.003 min
Response: 121295110
Conc: 680.25 ng/ml

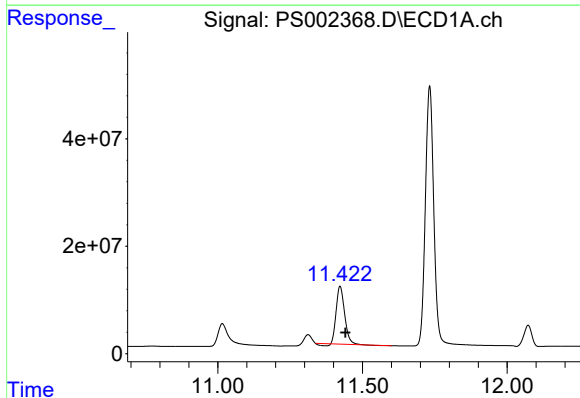


#4 2,4-DCAA

R.T.: 11.423 min
Delta R.T.: -0.019 min
Response: 211120879
Conc: 670.89 ng/ml

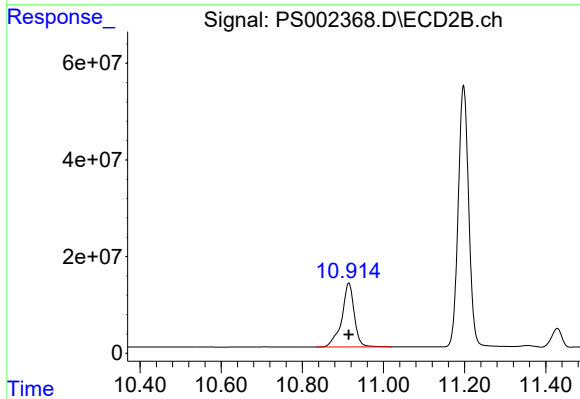

#4 2,4-DCAA


R.T.: 10.915 min
Delta R.T.: 0.000 min
Response: 282005254
Conc: 785.32 ng/ml

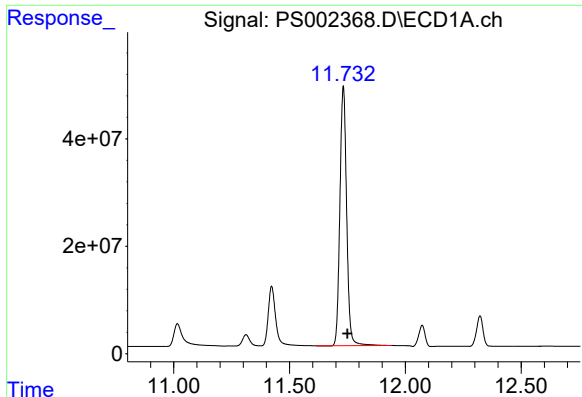

#5 DICAMBA


R.T.: 11.732 min
Delta R.T.: -0.017 min
Response: 977274106
Conc: 735.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

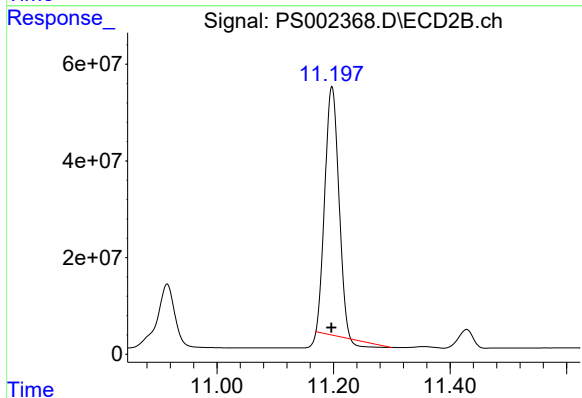


#5 DICAMBA

R.T.: 11.197 min
Delta R.T.: 0.000 min
Response: 824745526
Conc: 659.96 ng/ml

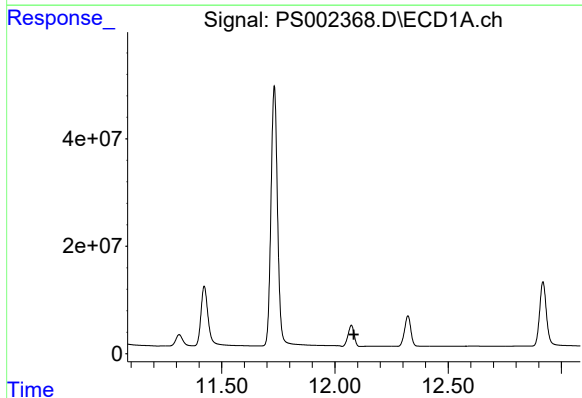


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

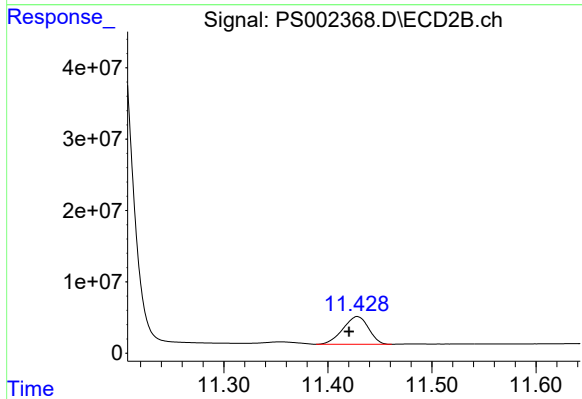

#6 MCP


R.T.: 11.428 min
Delta R.T.: 0.008 min
Response: 66765468
Conc: 77.60 ug/ml

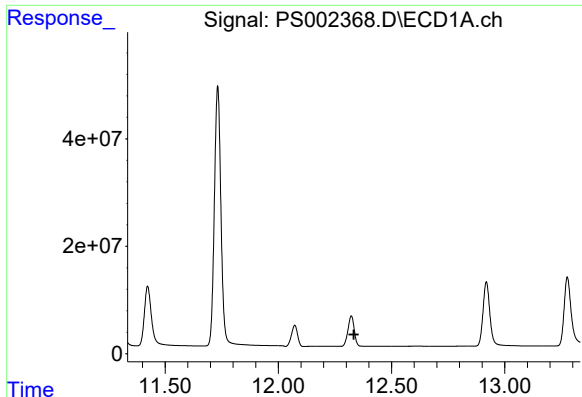

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

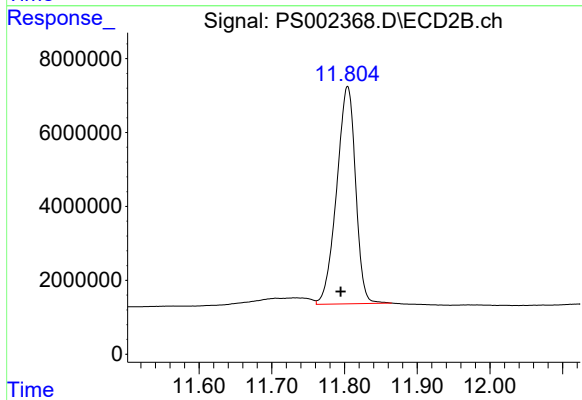


#7 MCPA

R.T.: 11.804 min
Delta R.T.: 0.009 min
Response: 106327783
Conc: 78.56 ug/ml

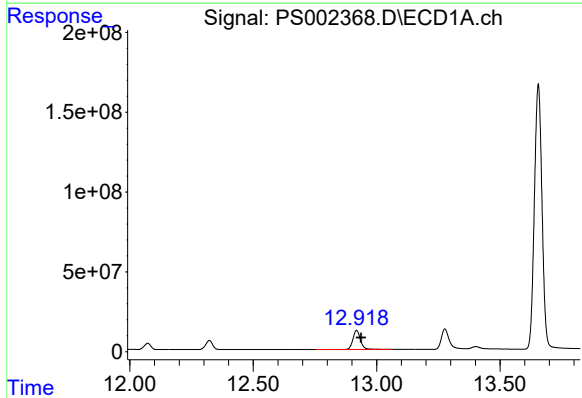


#8 DICHLORPROP

R.T.: 12.919 min
Delta R.T.: -0.019 min
Response: 251751085
Conc: 722.90 ng/ml

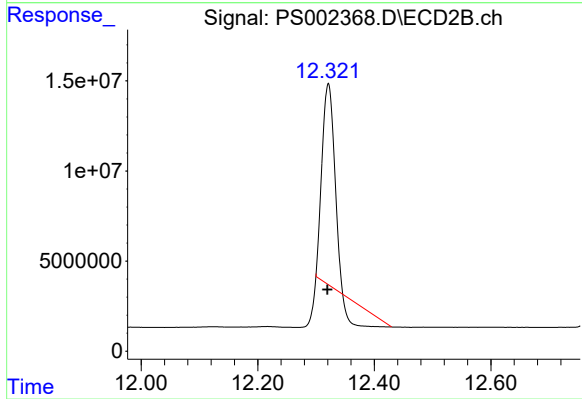

#8 DICHLORPROP


R.T.: 12.321 min
Delta R.T.: 0.002 min
Response: 128846724
Conc: 401.22 ng/ml

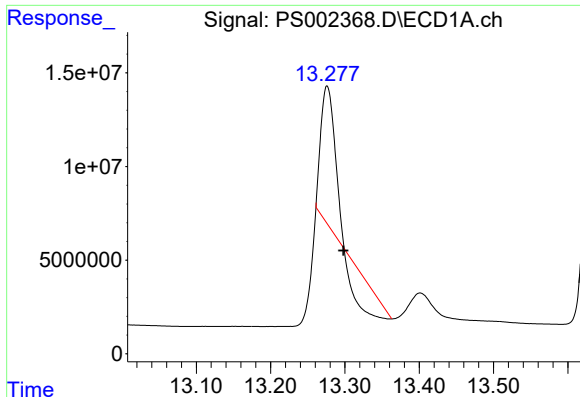

#9 2,4-D


R.T.: 13.276 min
Delta R.T.: -0.022 min
Response: 53670715
Conc: 133.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

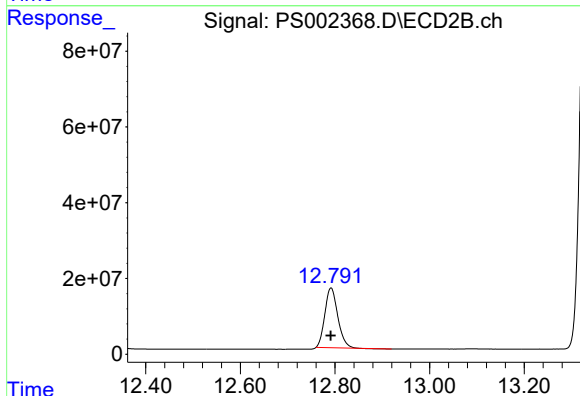


#9 2,4-D

R.T.: 12.792 min
Delta R.T.: 0.000 min
Response: 299004746
Conc: 702.07 ng/ml

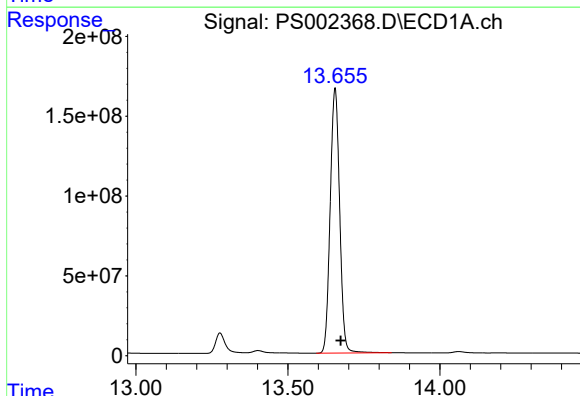


#10 Pentachlorophenol

R.T.: 13.655 min
Delta R.T.: -0.019 min
Response: 3575312810
Conc: 743.20 ng/ml

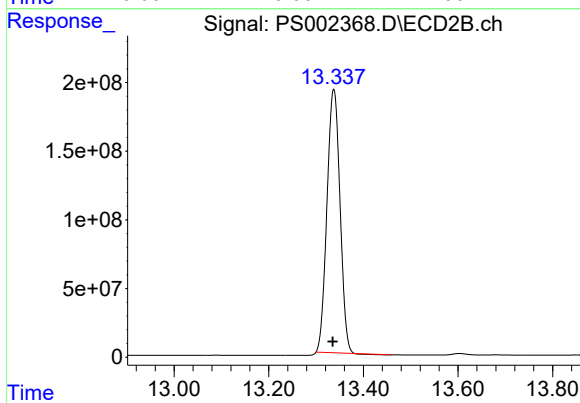

#10 Pentachlorophenol


R.T.: 13.337 min
Delta R.T.: 0.002 min
Response: 3662670261
Conc: 779.72 ng/ml

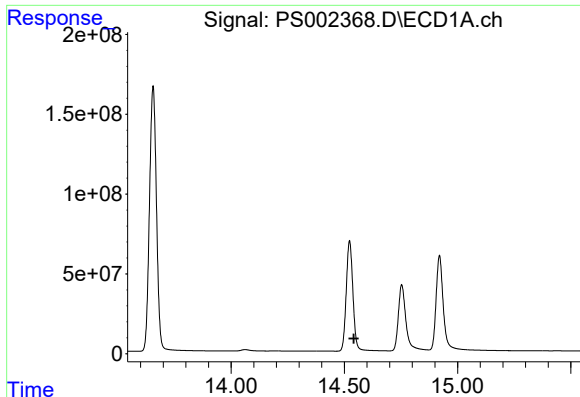

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

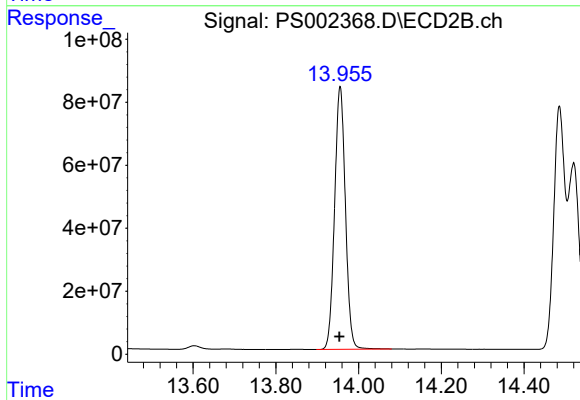


#11 2,4,5-TP (SILVEX)

R.T.: 13.955 min
Delta R.T.: 0.002 min
Response: 1514564414
Conc: 827.83 ng/ml

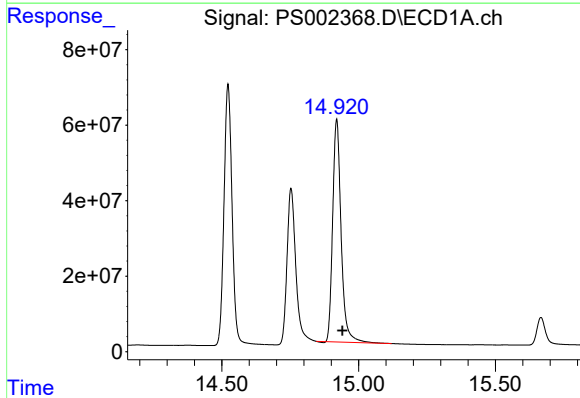


#12 2,4,5-T

R.T.: 14.920 min
Delta R.T.: -0.021 min
Response: 1263132020
Conc: 704.77 ng/ml

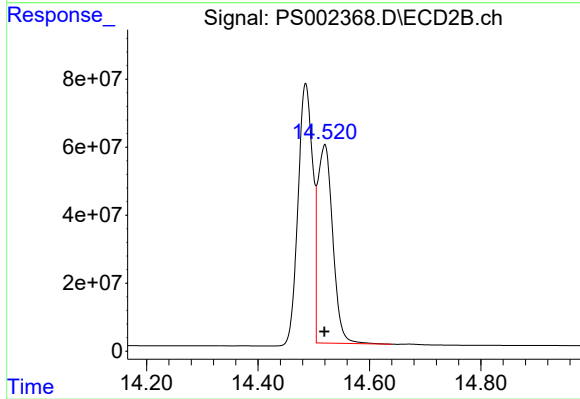

#12 2,4,5-T


R.T.: 14.520 min
Delta R.T.: 0.000 min
Response: 1088617390
Conc: 726.97 ng/ml

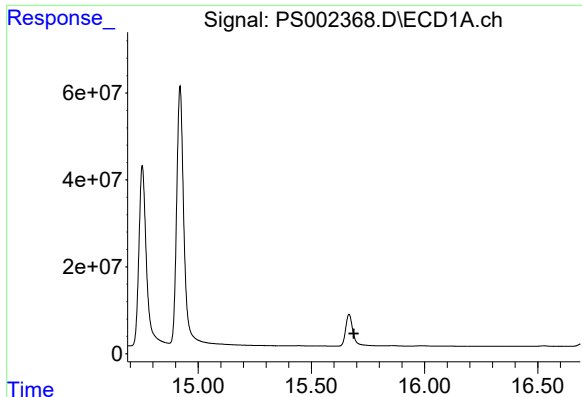

#13 2,4-DB


R.T.: 15.666 min
Delta R.T.: -0.022 min
Response: -60507129
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

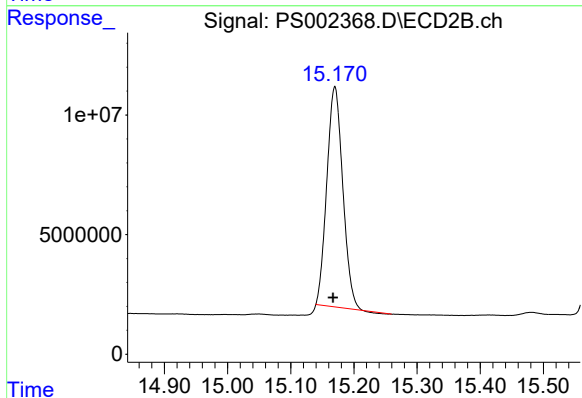


#13 2,4-DB

R.T.: 15.170 min
Delta R.T.: 0.003 min
Response: 161229391
Conc: 727.71 ng/ml

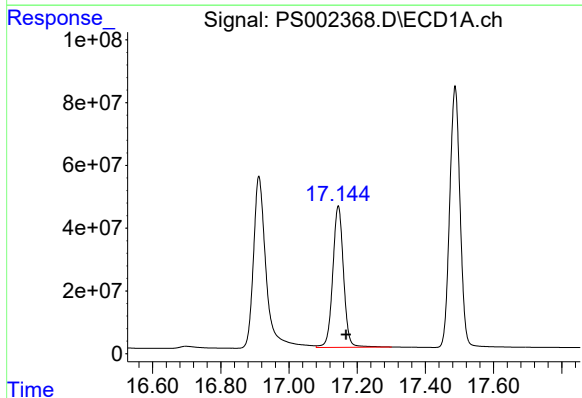


#14 DINOSEB

R.T.: 17.145 min
Delta R.T.: -0.023 min
Response: 988420763
Conc: 721.45 ng/ml

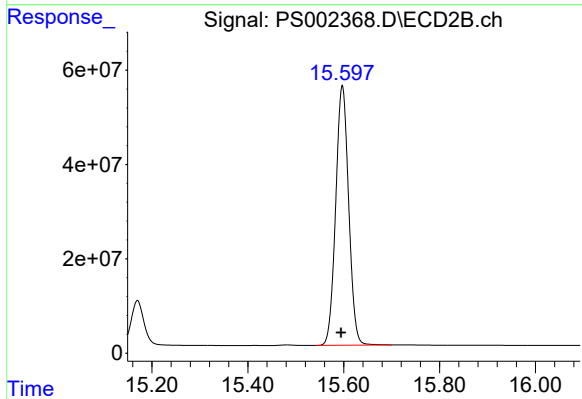

#14 DINOSEB


R.T.: 15.597 min
Delta R.T.: 0.003 min
Response: 1032317090
Conc: 815.50 ng/ml

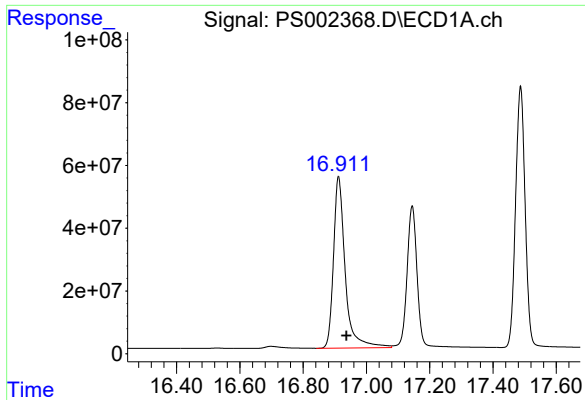

#15 Picloram


R.T.: 16.912 min
Delta R.T.: -0.026 min
Response: 1408283701
Conc: 590.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

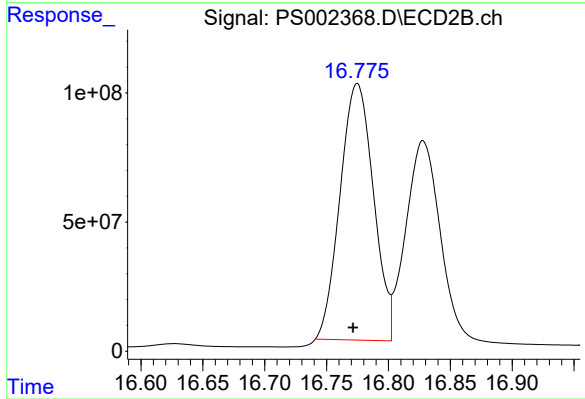


#15 Picloram

R.T.: 16.775 min
Delta R.T.: 0.004 min
Response: 1866825337
Conc: 825.22 ng/ml

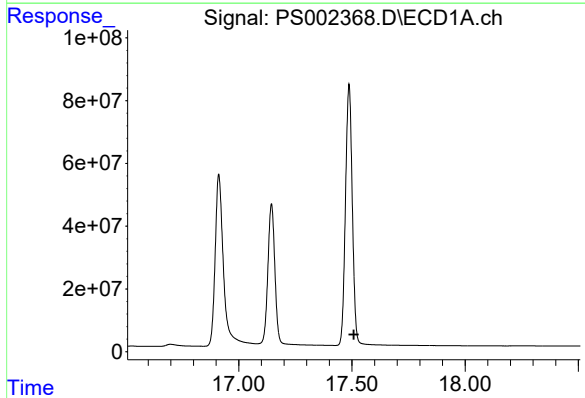

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

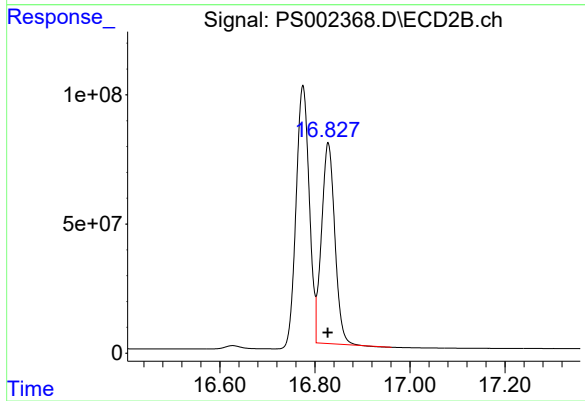

#16 DCPA

R.T.: 16.828 min
Delta R.T.: 0.001 min
Response: 1504133168
Conc: 635.23 ng/ml